


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022025\
Data File : VY021246.D
Acq On : 20 Feb 2025 13:21
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Title : SW846 8260
Last Update : Mon Feb 03 13:08:38 2025

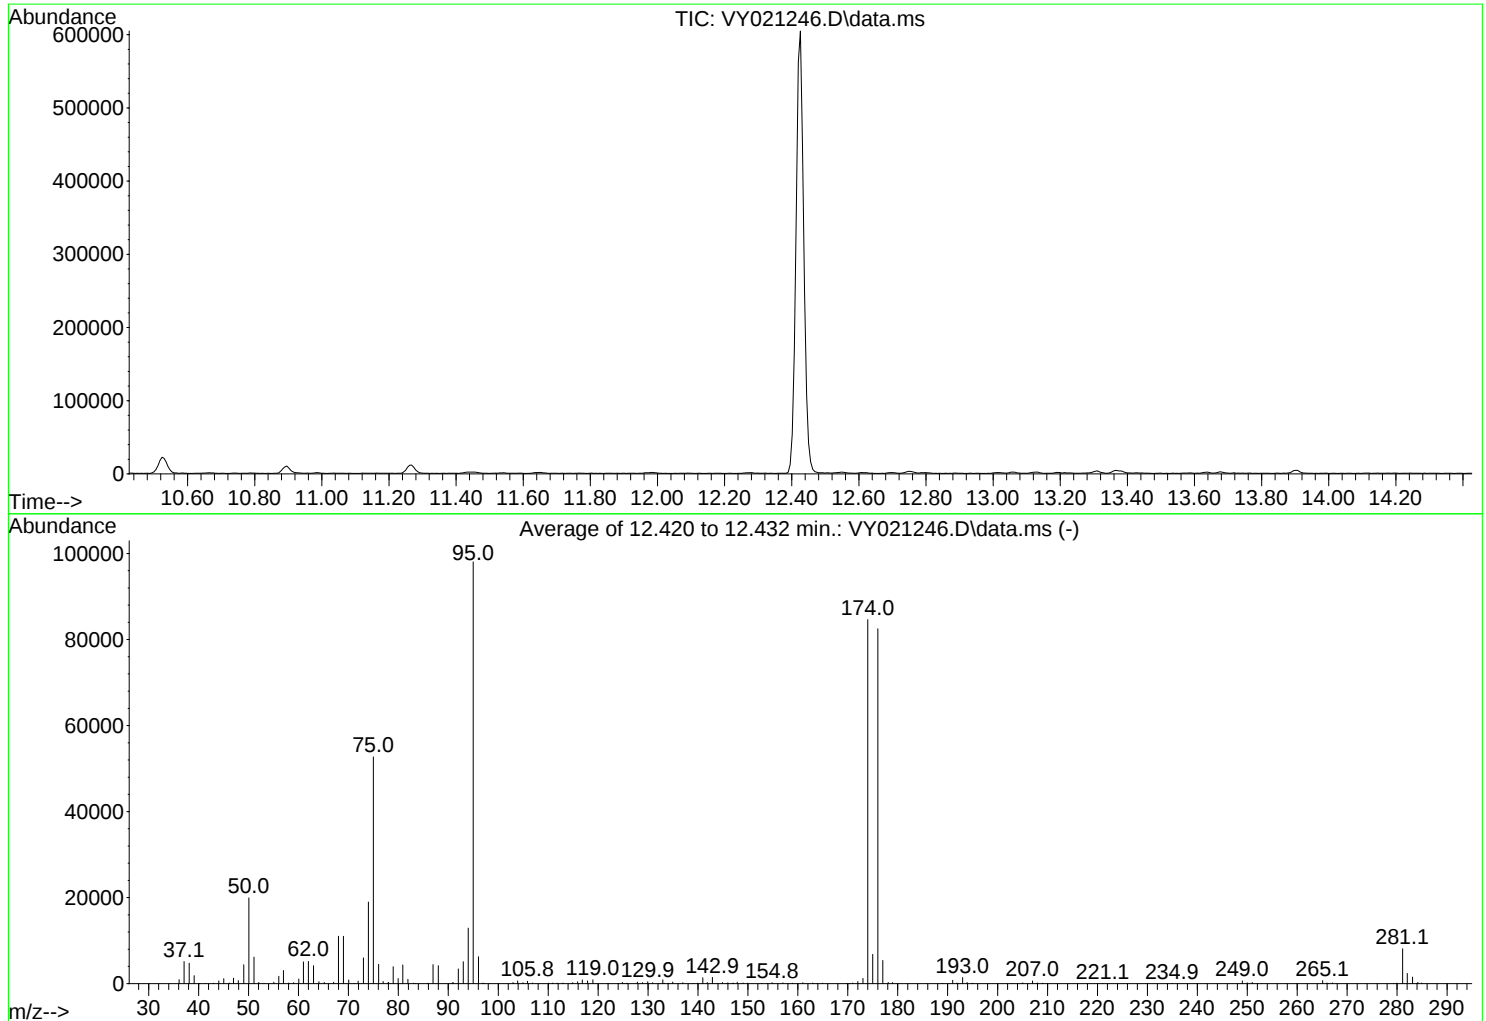

AutoFind: Scans 1755, 1756, 1757; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	19953	PASS
75	95	30	60	53.7	52709	PASS
95	95	100	100	100.0	98064	PASS
96	95	5	9	6.4	6251	PASS
173	174	0.00	2	1.5	1228	PASS
174	95	50	100	86.3	84616	PASS
175	174	5	9	8.0	6807	PASS
176	174	95	101	97.5	82499	PASS
177	176	5	9	6.6	5412	PASS