

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022125\
 Data File : VY021294.D
 Acq On : 21 Feb 2025 18:31
 Operator : SY/MD
 Sample : Q1382-15
 Misc : 5.83g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-PCS-TC-08-021725

Quant Time: Feb 21 23:10:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 03 13:08:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	161604	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	318713	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	297417	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.353	152	119366	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	92947	56.135	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.280%
35) Dibromofluoromethane	7.640	113	101408	49.648	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.300%
50) Toluene-d8	10.109	98	393214	50.567	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.140%
62) 4-Bromofluorobenzene	12.408	95	122440	48.197	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	96.400%
Target Compounds						
16) Acetone	3.879	43	13125	50.830	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022125\
Data File : VY021294.D
Acq On : 21 Feb 2025 18:31
Operator : SY/MD
Sample : Q1382-15
Misc : 5.83g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-08-021725

Quant Time: Feb 21 23:10:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020325S.M
Quant Title : SW846 8260
QLast Update : Mon Feb 03 13:08:38 2025
Response via : Initial Calibration




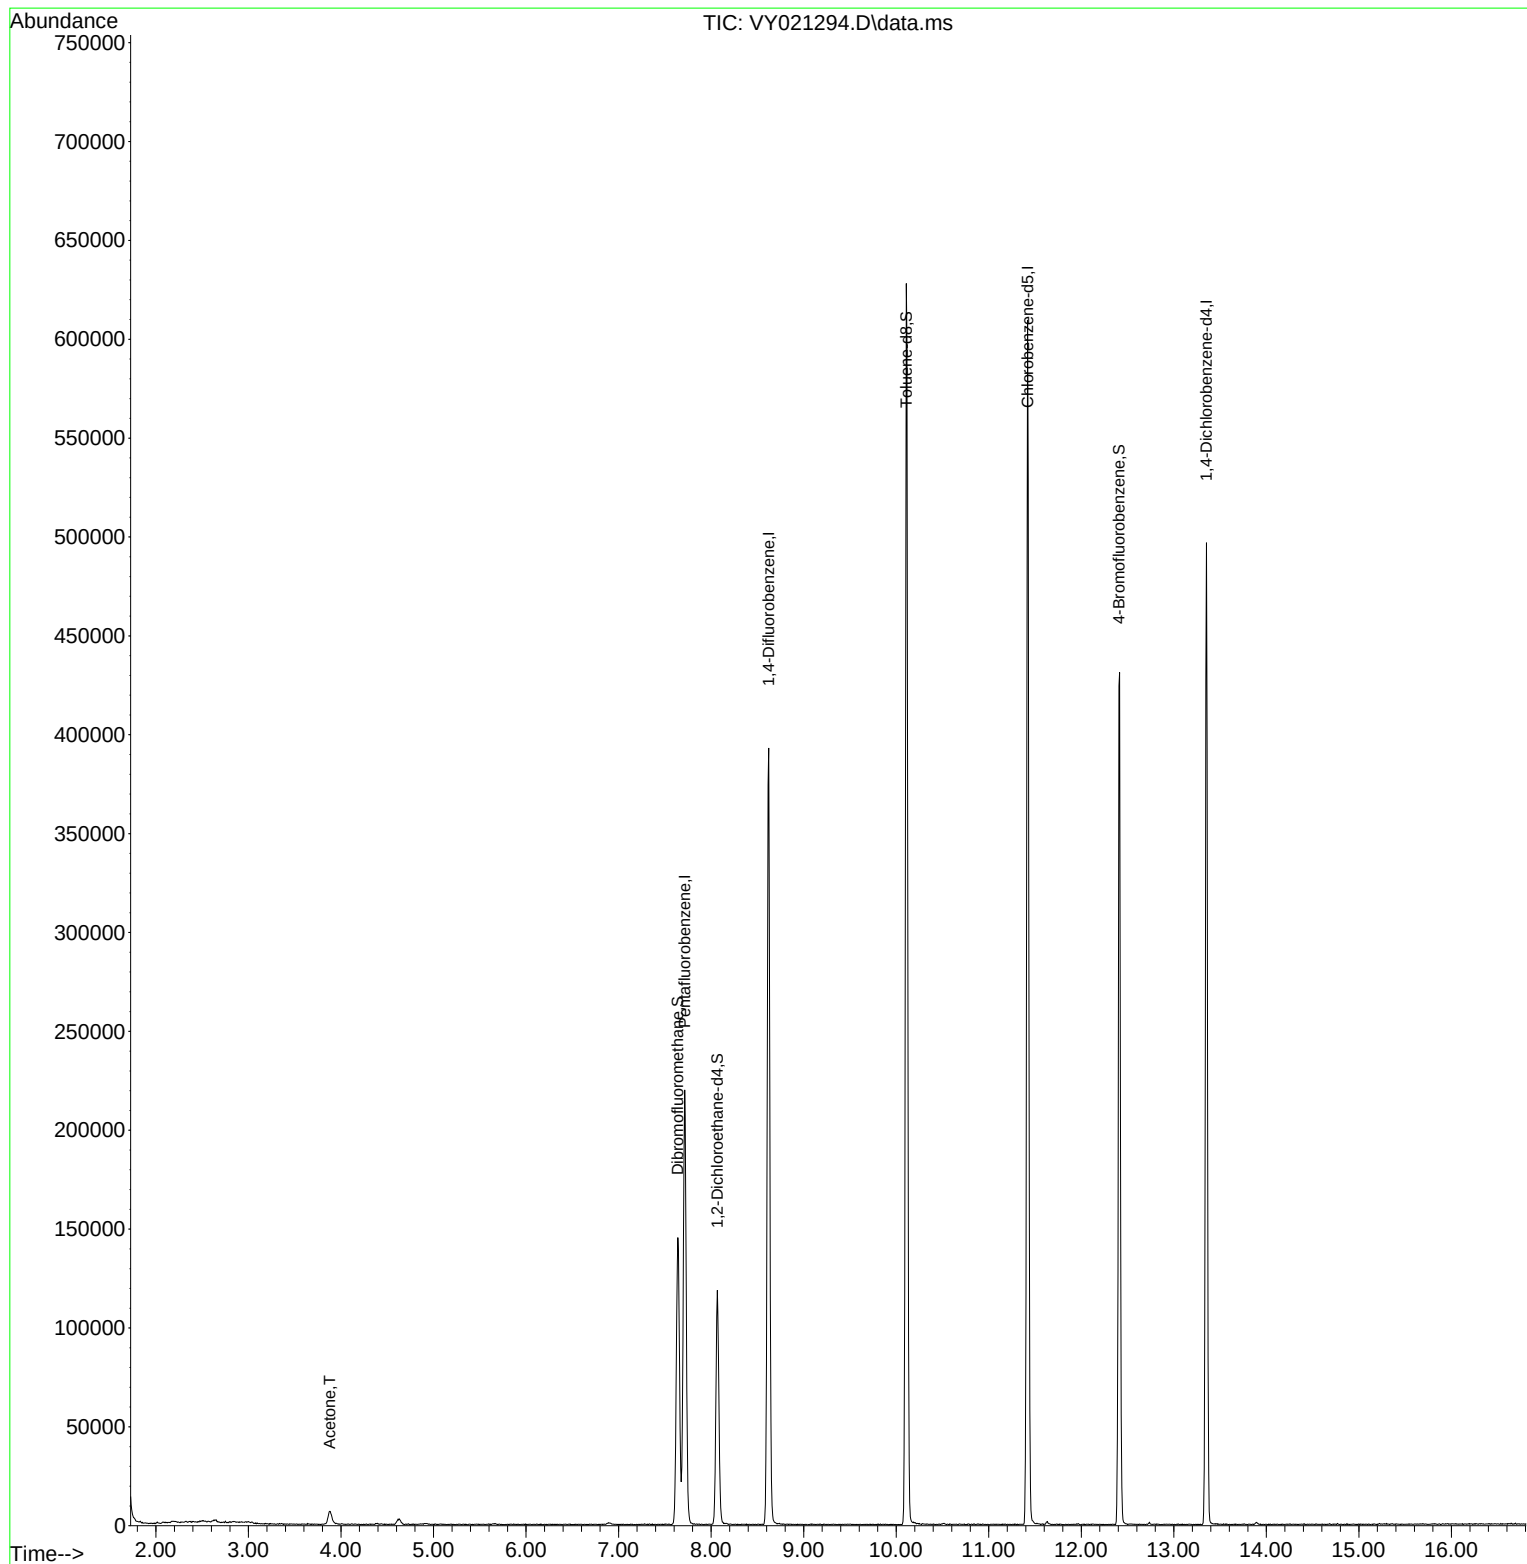


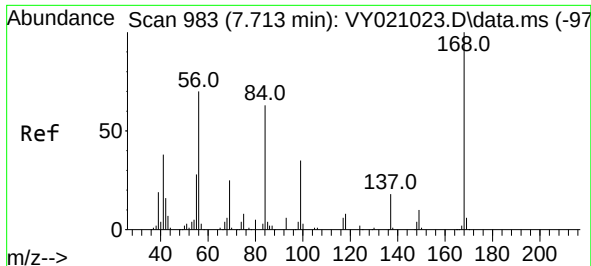

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 99
Delta R.T. 0.000 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-08-021725


Tgt Ion:168 Resp: 161604
Ion Ratio Lower Upper
168 100
99 58.4 44.2 66.4

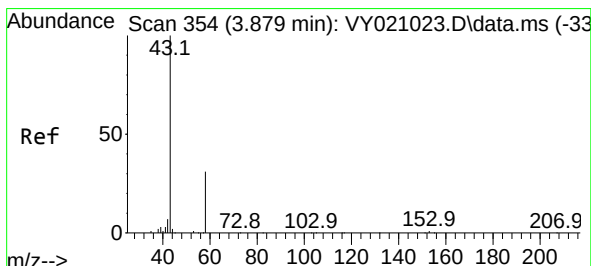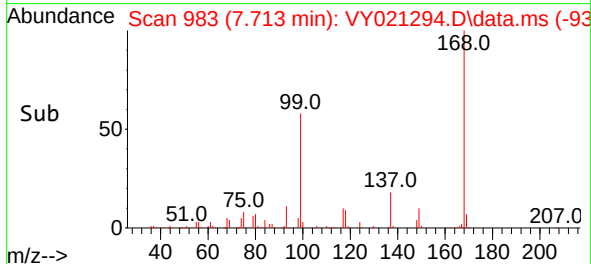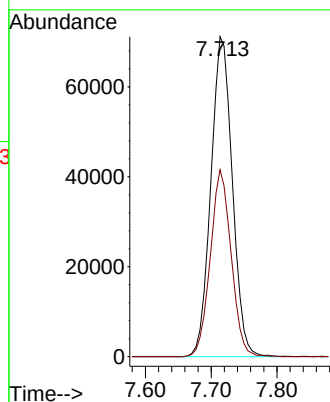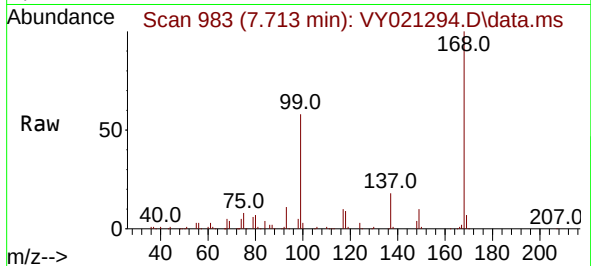

#16
Acetone
Concen: 50.830 ug/l
RT: 3.879 min Scan# 354
Delta R.T. -0.000 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31

Tgt Ion: 43 Resp: 13125
Ion Ratio Lower Upper
43 100
58 32.1 26.6 39.8

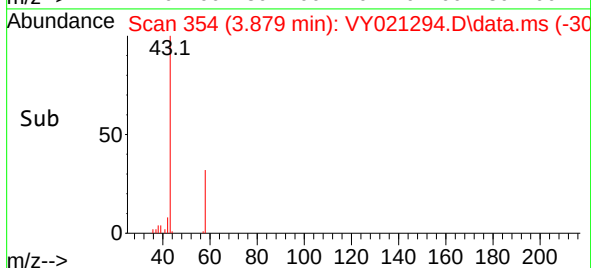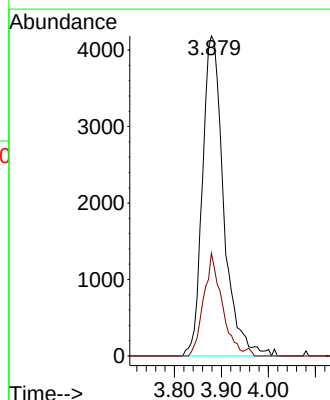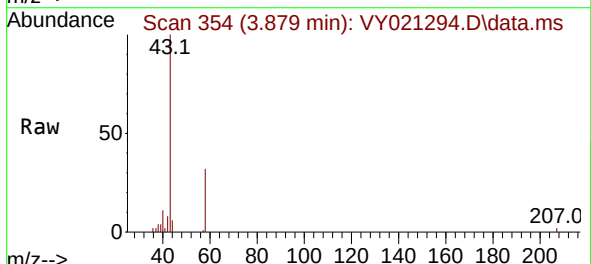

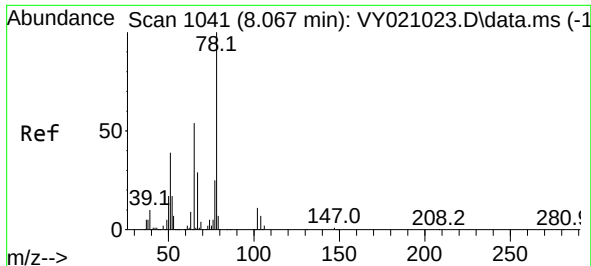

#33

1,2-Dichloroethane-d4

Concen: 56.135 ug/l

RT: 8.067 min Scan# 1104

Delta R.T. -0.000 min

Lab File: VY021294.D

Acq: 21 Feb 2025 18:31

Instrument :

MSVOA_Y

ClientSampleId :





OU4-PCS-TC-08-021725

Tgt Ion: 65 Resp: 92947

Ion Ratio Lower Upper

65 100

67 52.0 0.0 109.0

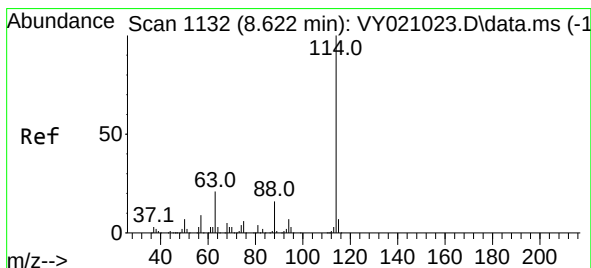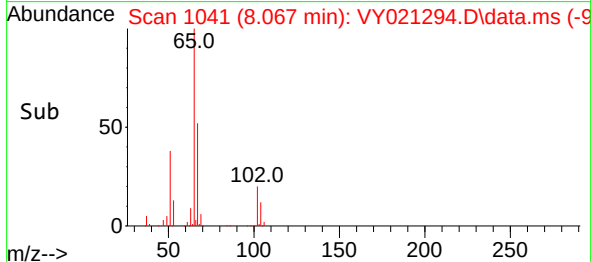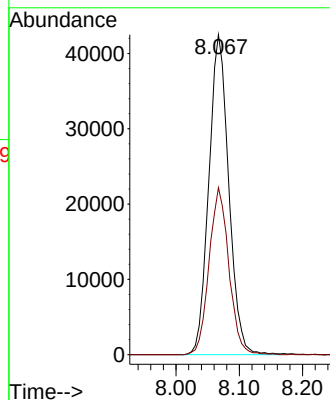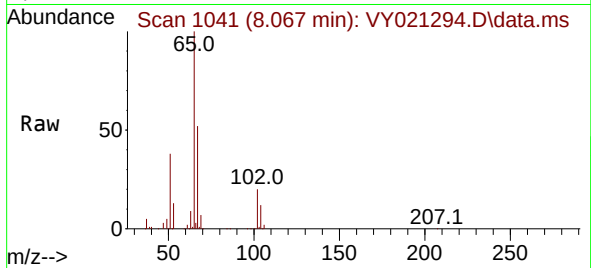

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.622 min Scan# 1132

Delta R.T. -0.000 min

Lab File: VY021294.D

Acq: 21 Feb 2025 18:31




Tgt Ion: 114 Resp: 318713


Ion Ratio Lower Upper

114 100

63 20.5 0.0 37.4

88 15.3 0.0 29.0


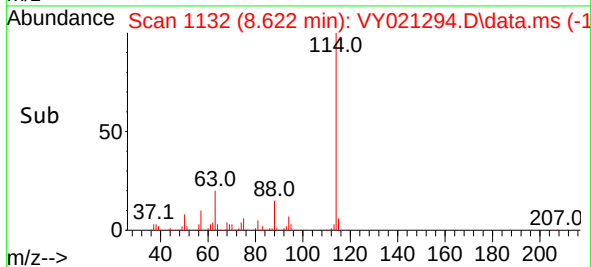
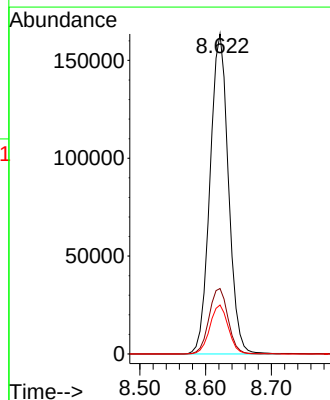
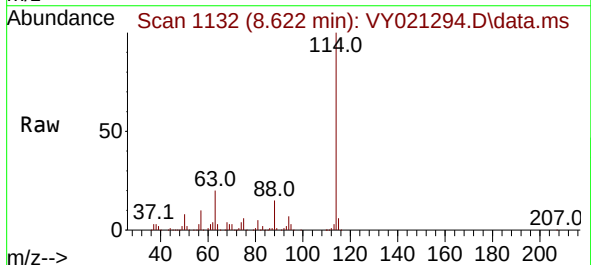


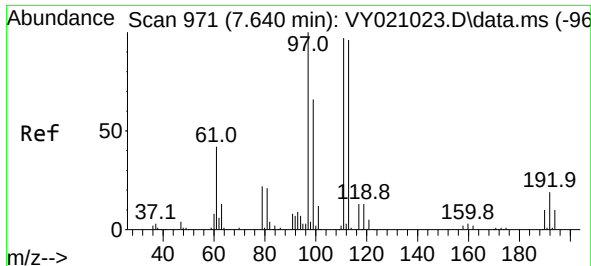

#35
Dibromofluoromethane
Concen: 49.648 ug/l
RT: 7.640 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-08-021725


Tgt Ion:113 Resp: 101408
Ion Ratio Lower Upper
113 100
111 102.7 83.8 125.6
192 19.6 14.5 21.7

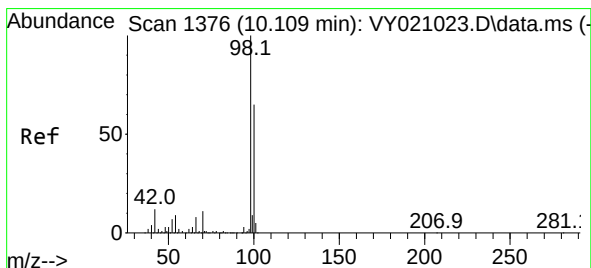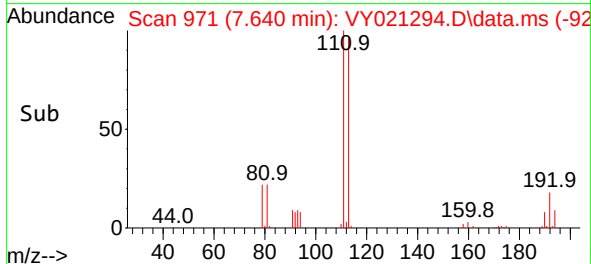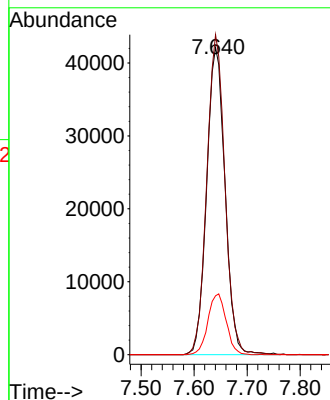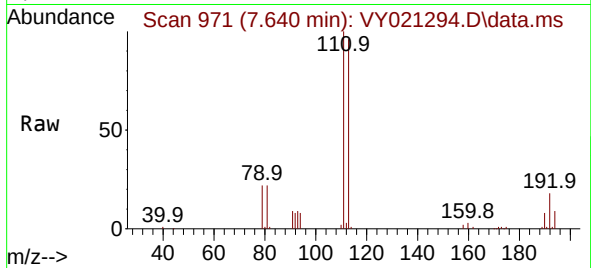

#50
Toluene-d8
Concen: 50.567 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31

Tgt Ion: 98 Resp: 393214
Ion Ratio Lower Upper
98 100
100 64.3 52.3 78.5


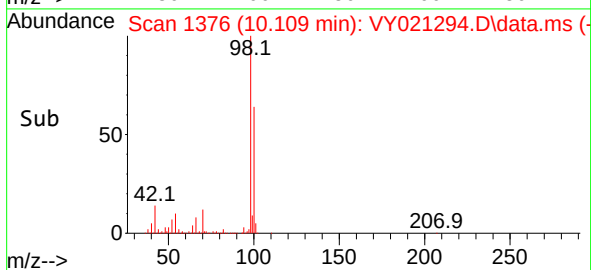
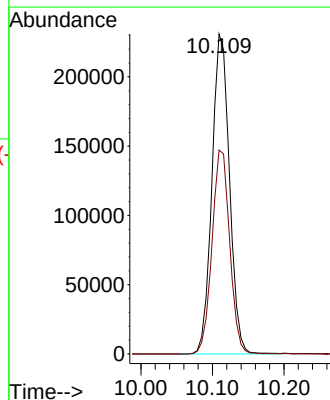
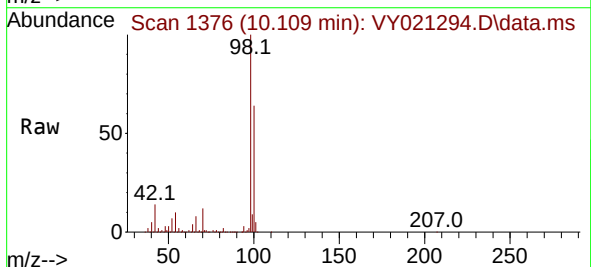


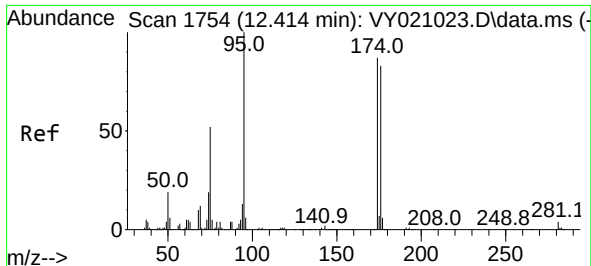

#62
4-Bromofluorobenzene
Concen: 48.197 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.006 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31




Instrument :
MSVOA_Y
ClientSampleId :
OU4-PCS-TC-08-021725


Tgt Ion:	95	Resp:	122440
Ion Ratio	Lower	Upper	
95	100		
174	86.2	0.0	160.0
176	82.6	0.0	151.8

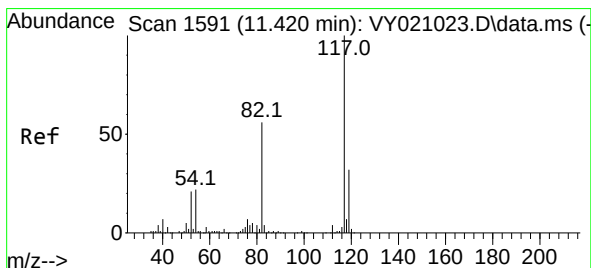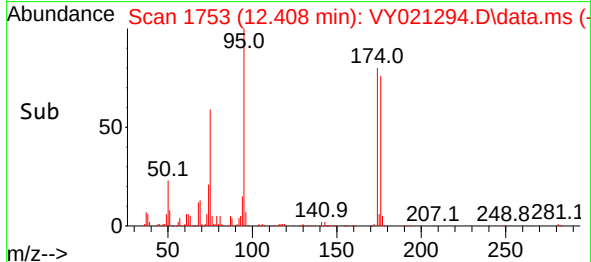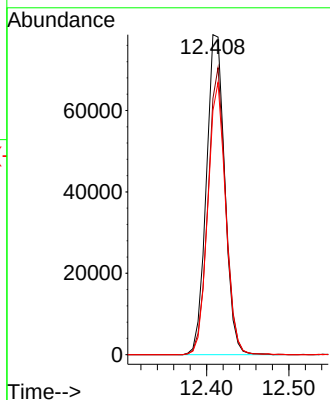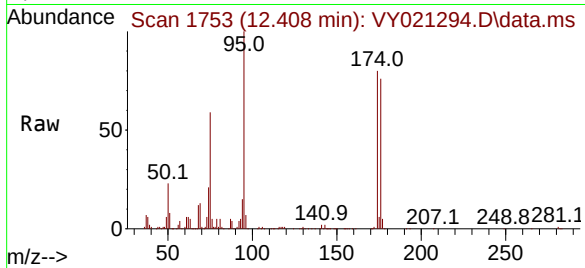

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 1591
Delta R.T. -0.000 min
Lab File: VY021294.D
Acq: 21 Feb 2025 18:31

Tgt Ion:	117	Resp:	297417
Ion Ratio	Lower	Upper	
117	100		
82	56.9	43.8	65.8
119	32.4	26.5	39.7

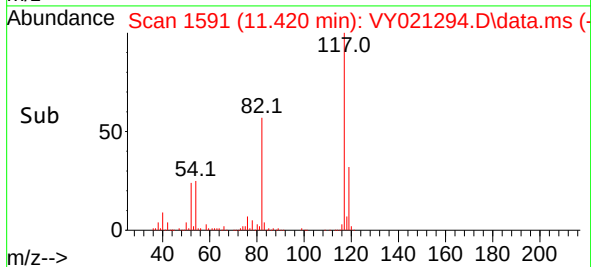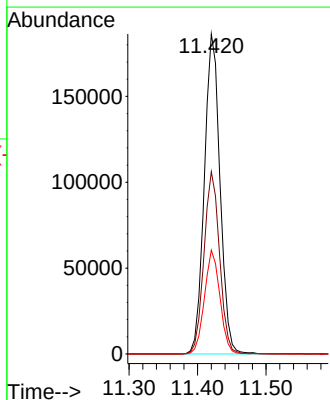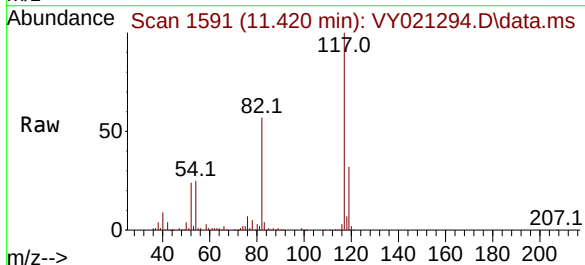

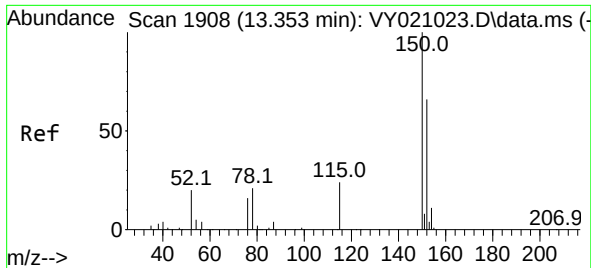

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.353 min Scan# 1908

Delta R.T. -0.000 min

Lab File: VY021294.D


Acq: 21 Feb 2025 18:31

Instrument :

MSVOA_Y

ClientSampleId :

OU4-PCS-TC-08-021725

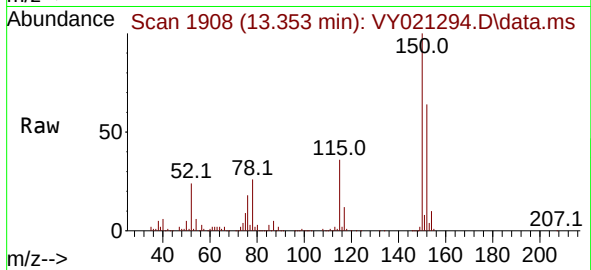

Tgt Ion:152 Resp: 119366

Ion Ratio Lower Upper

152 100

115 57.1 30.0 90.0

150 154.7 0.0 344.6

