
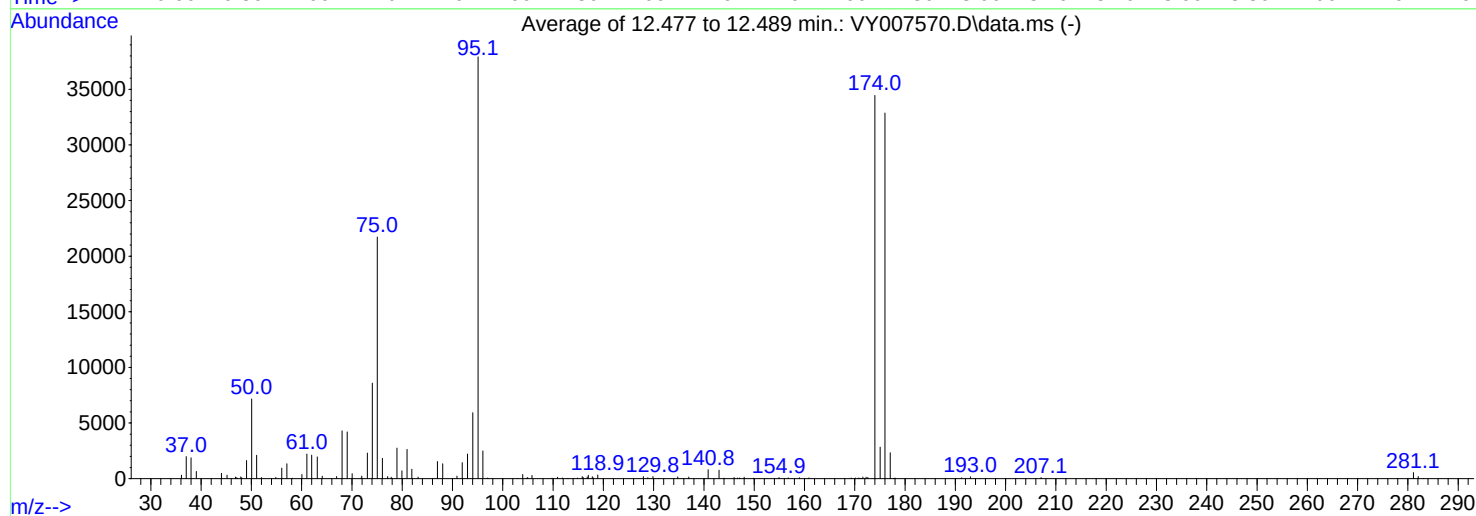


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022222\
Data File : VY007570.D
Acq On : 22 Feb 2022 08:42
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022122S.M
Title : SW846 8260
Last Update : Mon Feb 21 15:25:36 2022

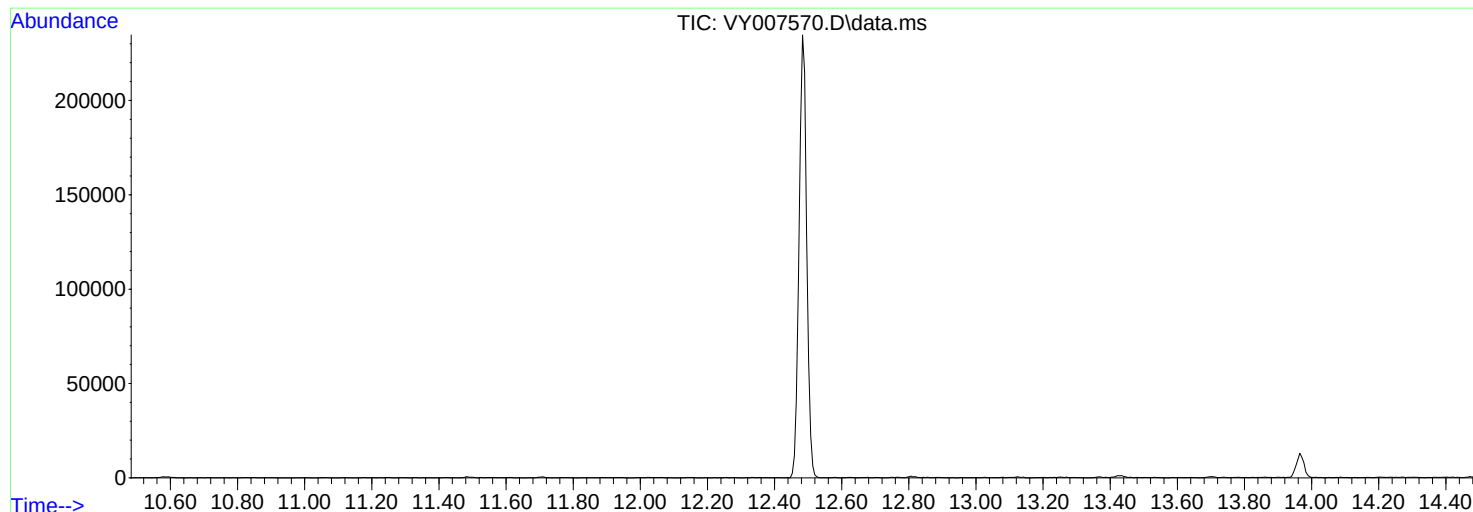

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	7162	PASS
75	95	30	60	57.3	21715	PASS
95	95	100	100	100.0	37920	PASS
96	95	5	9	6.6	2485	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.9	34453	PASS
175	174	5	9	8.2	2836	PASS
176	174	95	101	95.4	32864	PASS
177	176	5	9	7.1	2331	PASS