


Chloromethane

Response Ratio

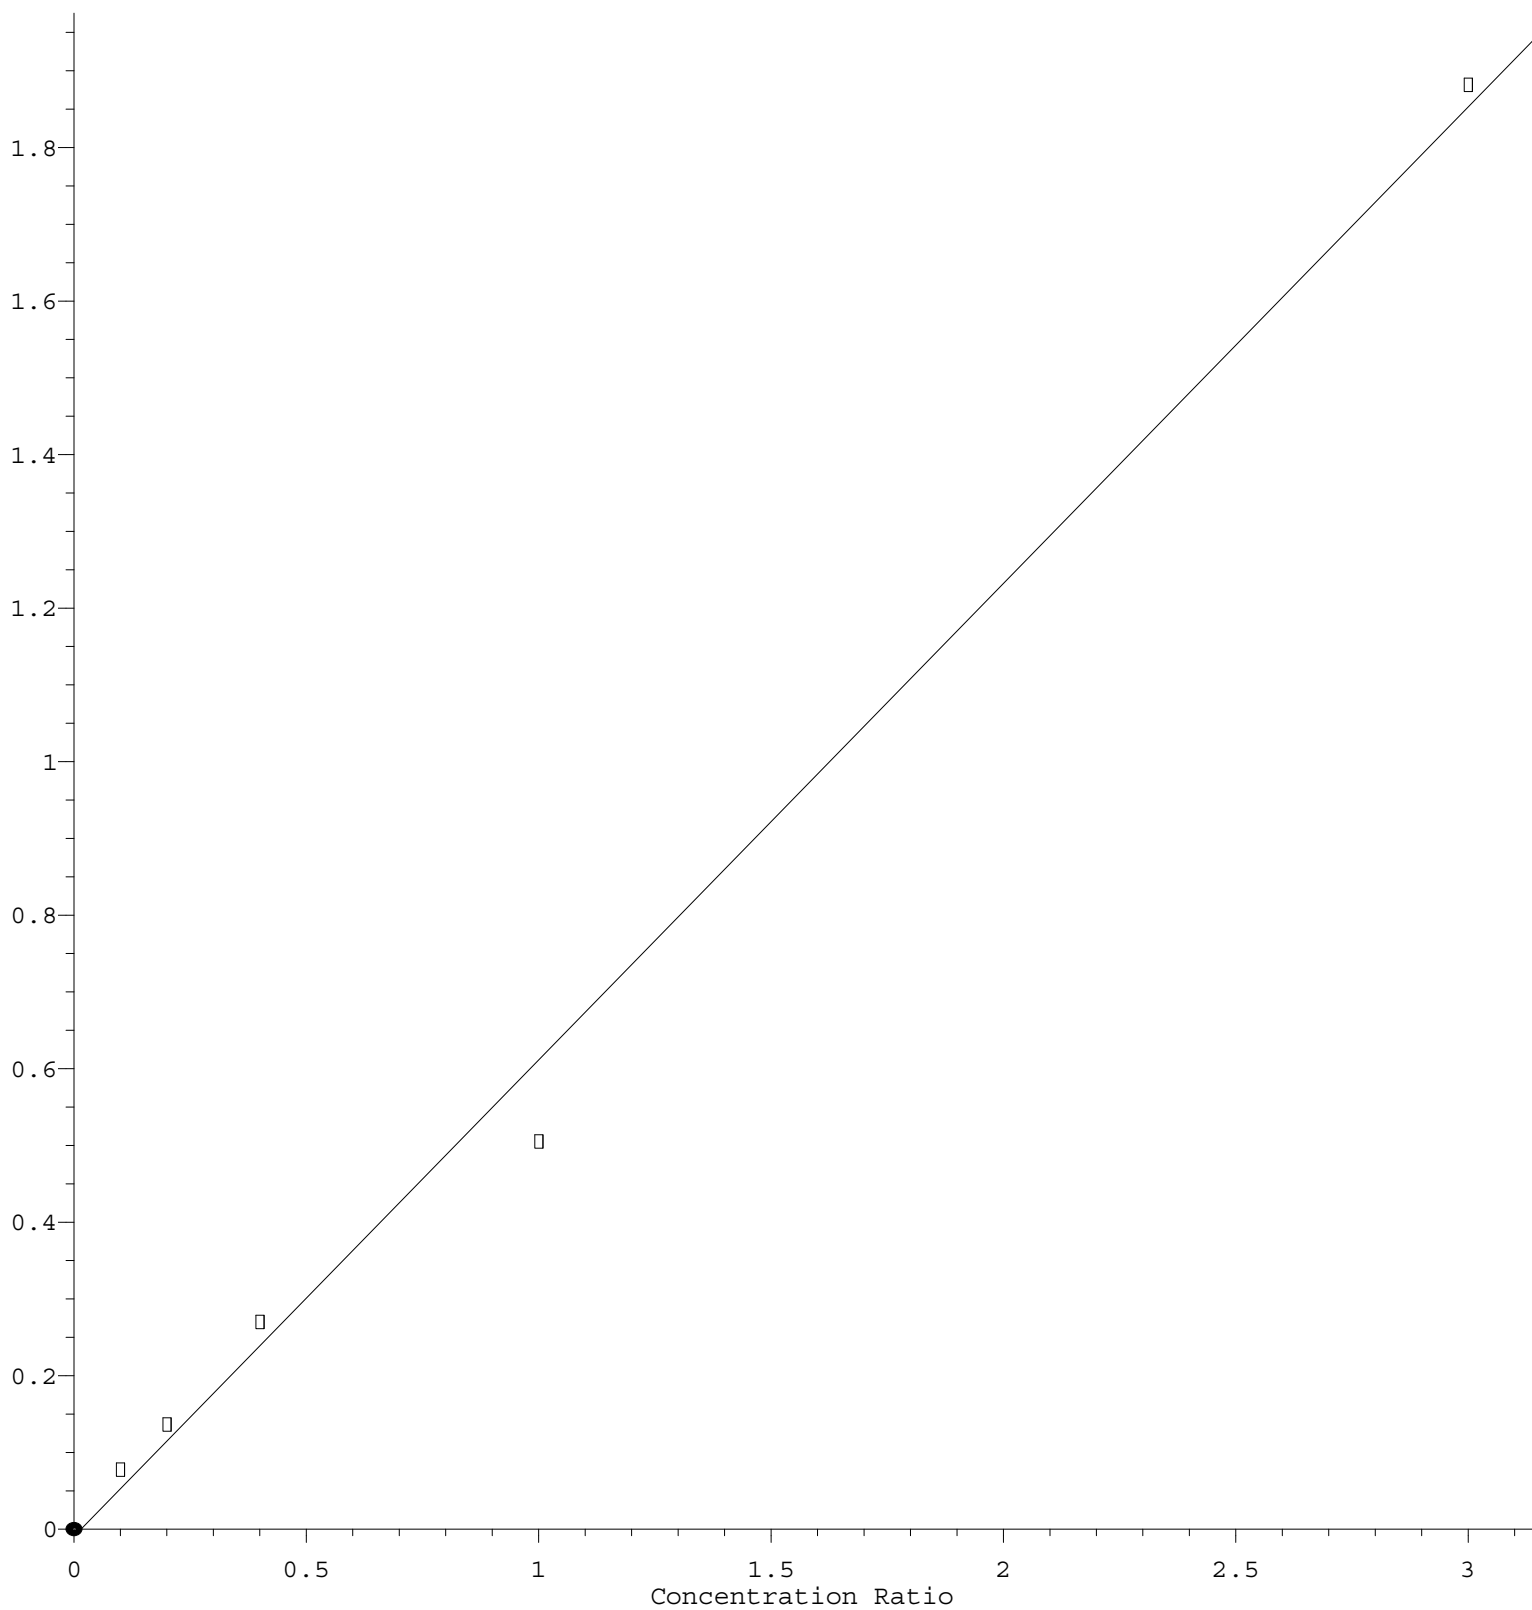

$$\text{Response} = 6.206\text{e-}001 * \text{Amt} - 9.360\text{e-}003$$


Coef of Det (r^2) = 0.993685 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M

Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Tetrachloroethene

Response Ratio

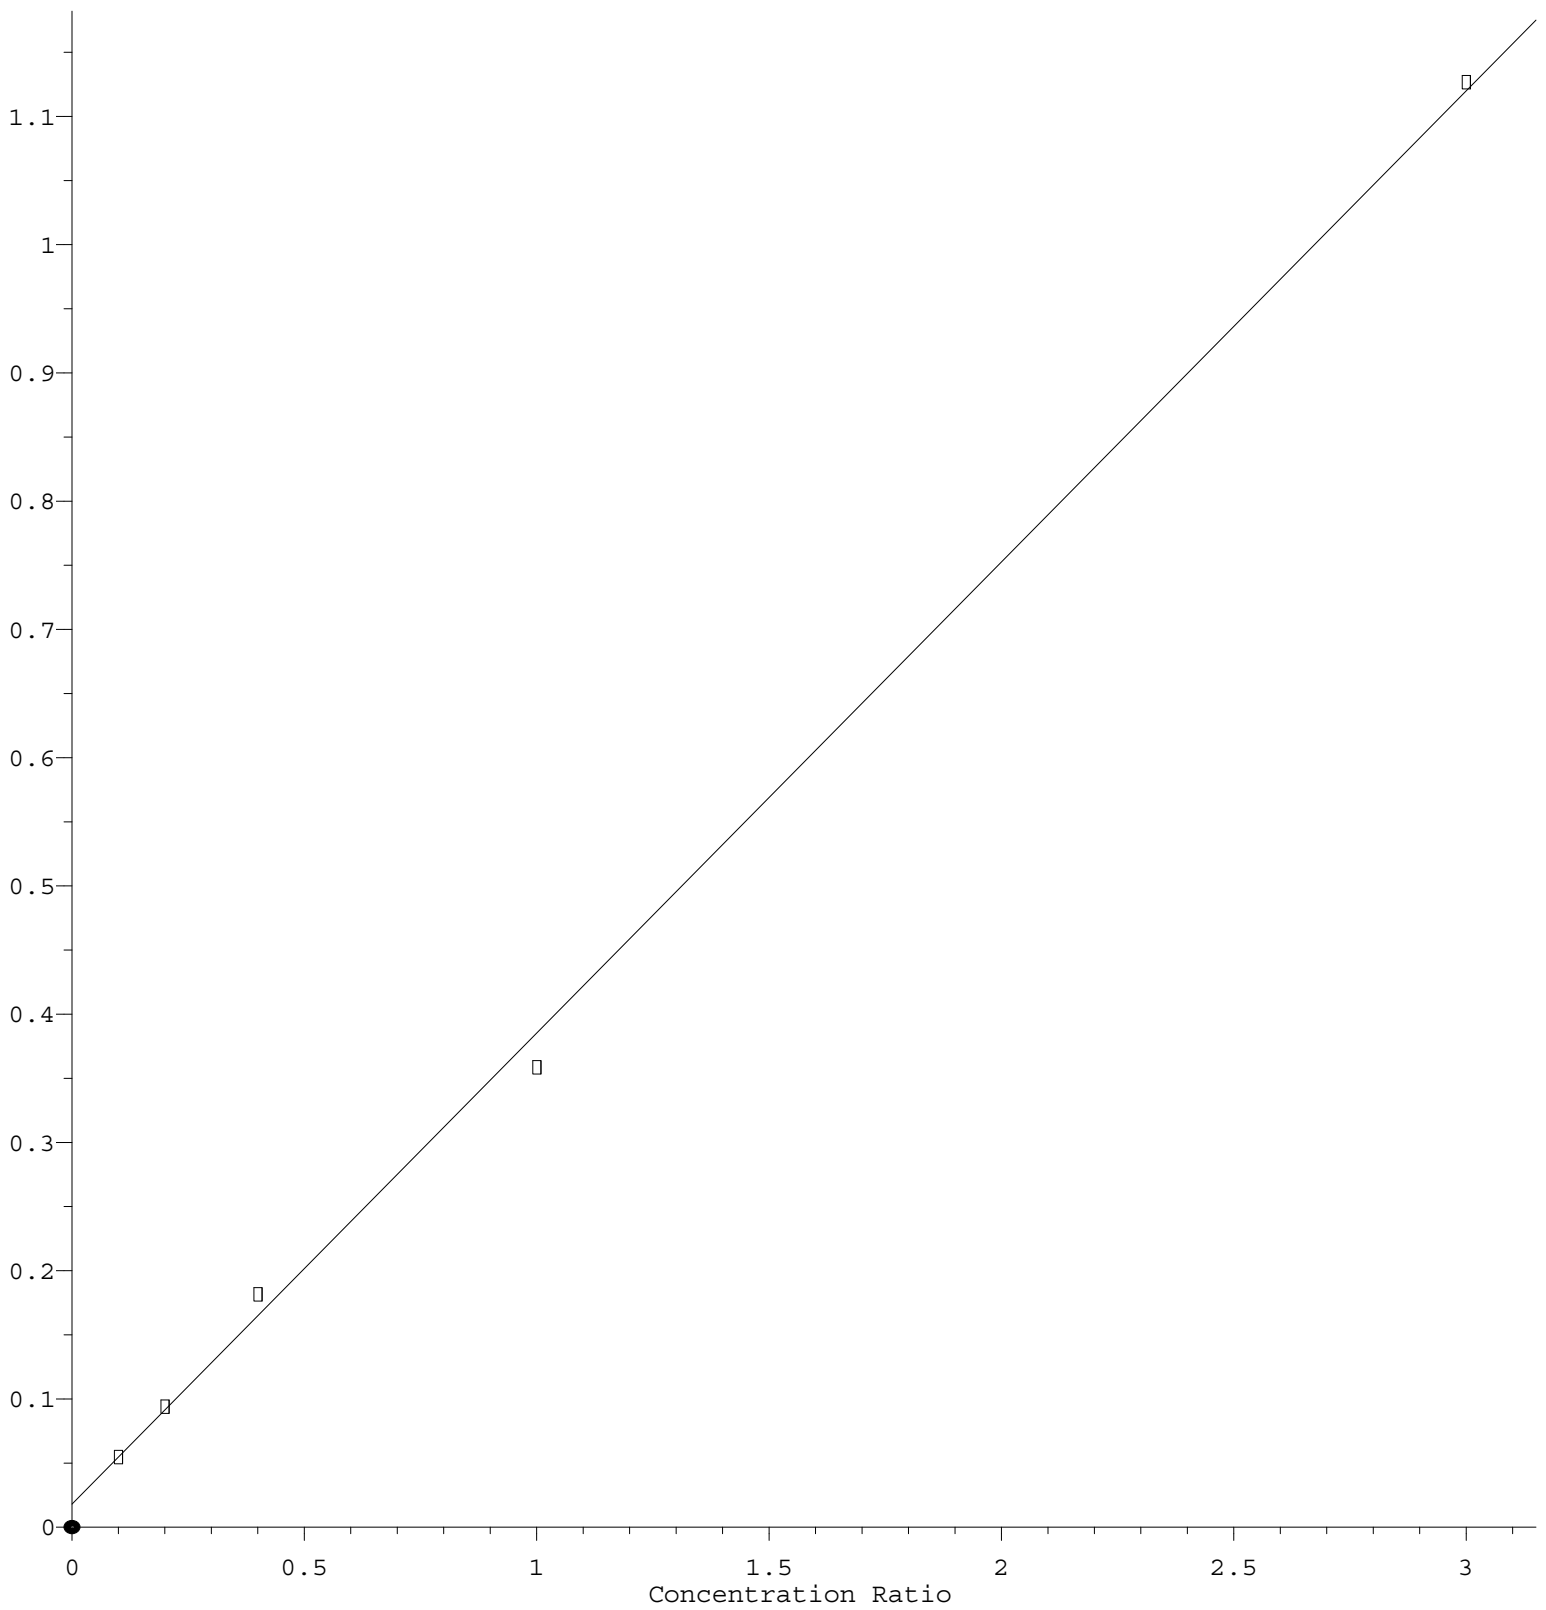

$$\text{Response} = 3.676\text{e-}001 * \text{Amt} + 1.756\text{e-}002$$


Coef of Det (r^2) = 0.998670 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M

Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Toluene-d8


Response Ratio

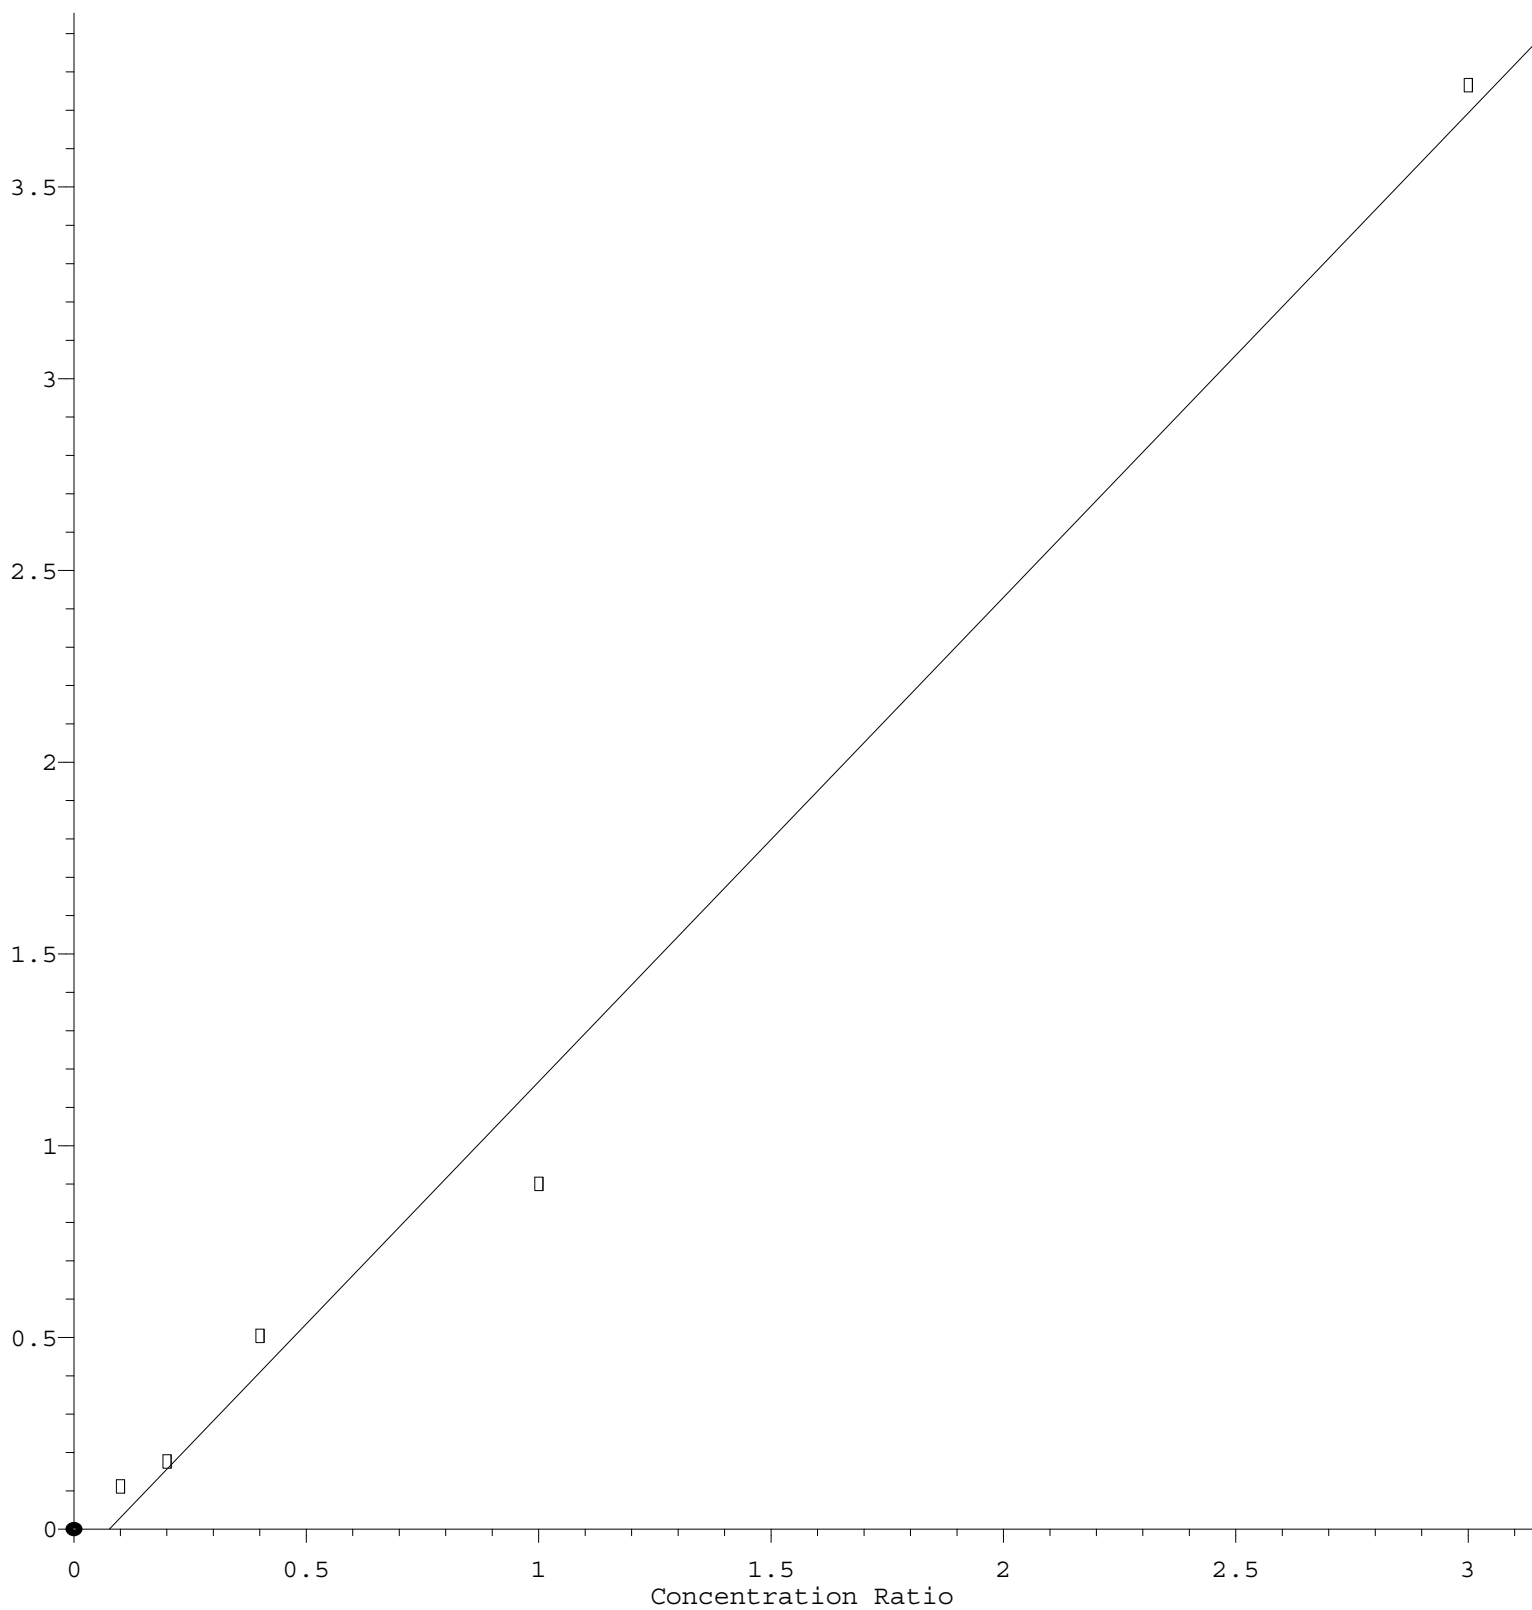

Response = 1.263e+000 * Amt - 9.557e-002
Coef of Det (r^2) = 0.990113 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M
Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Methylcyclohexane

Response Ratio

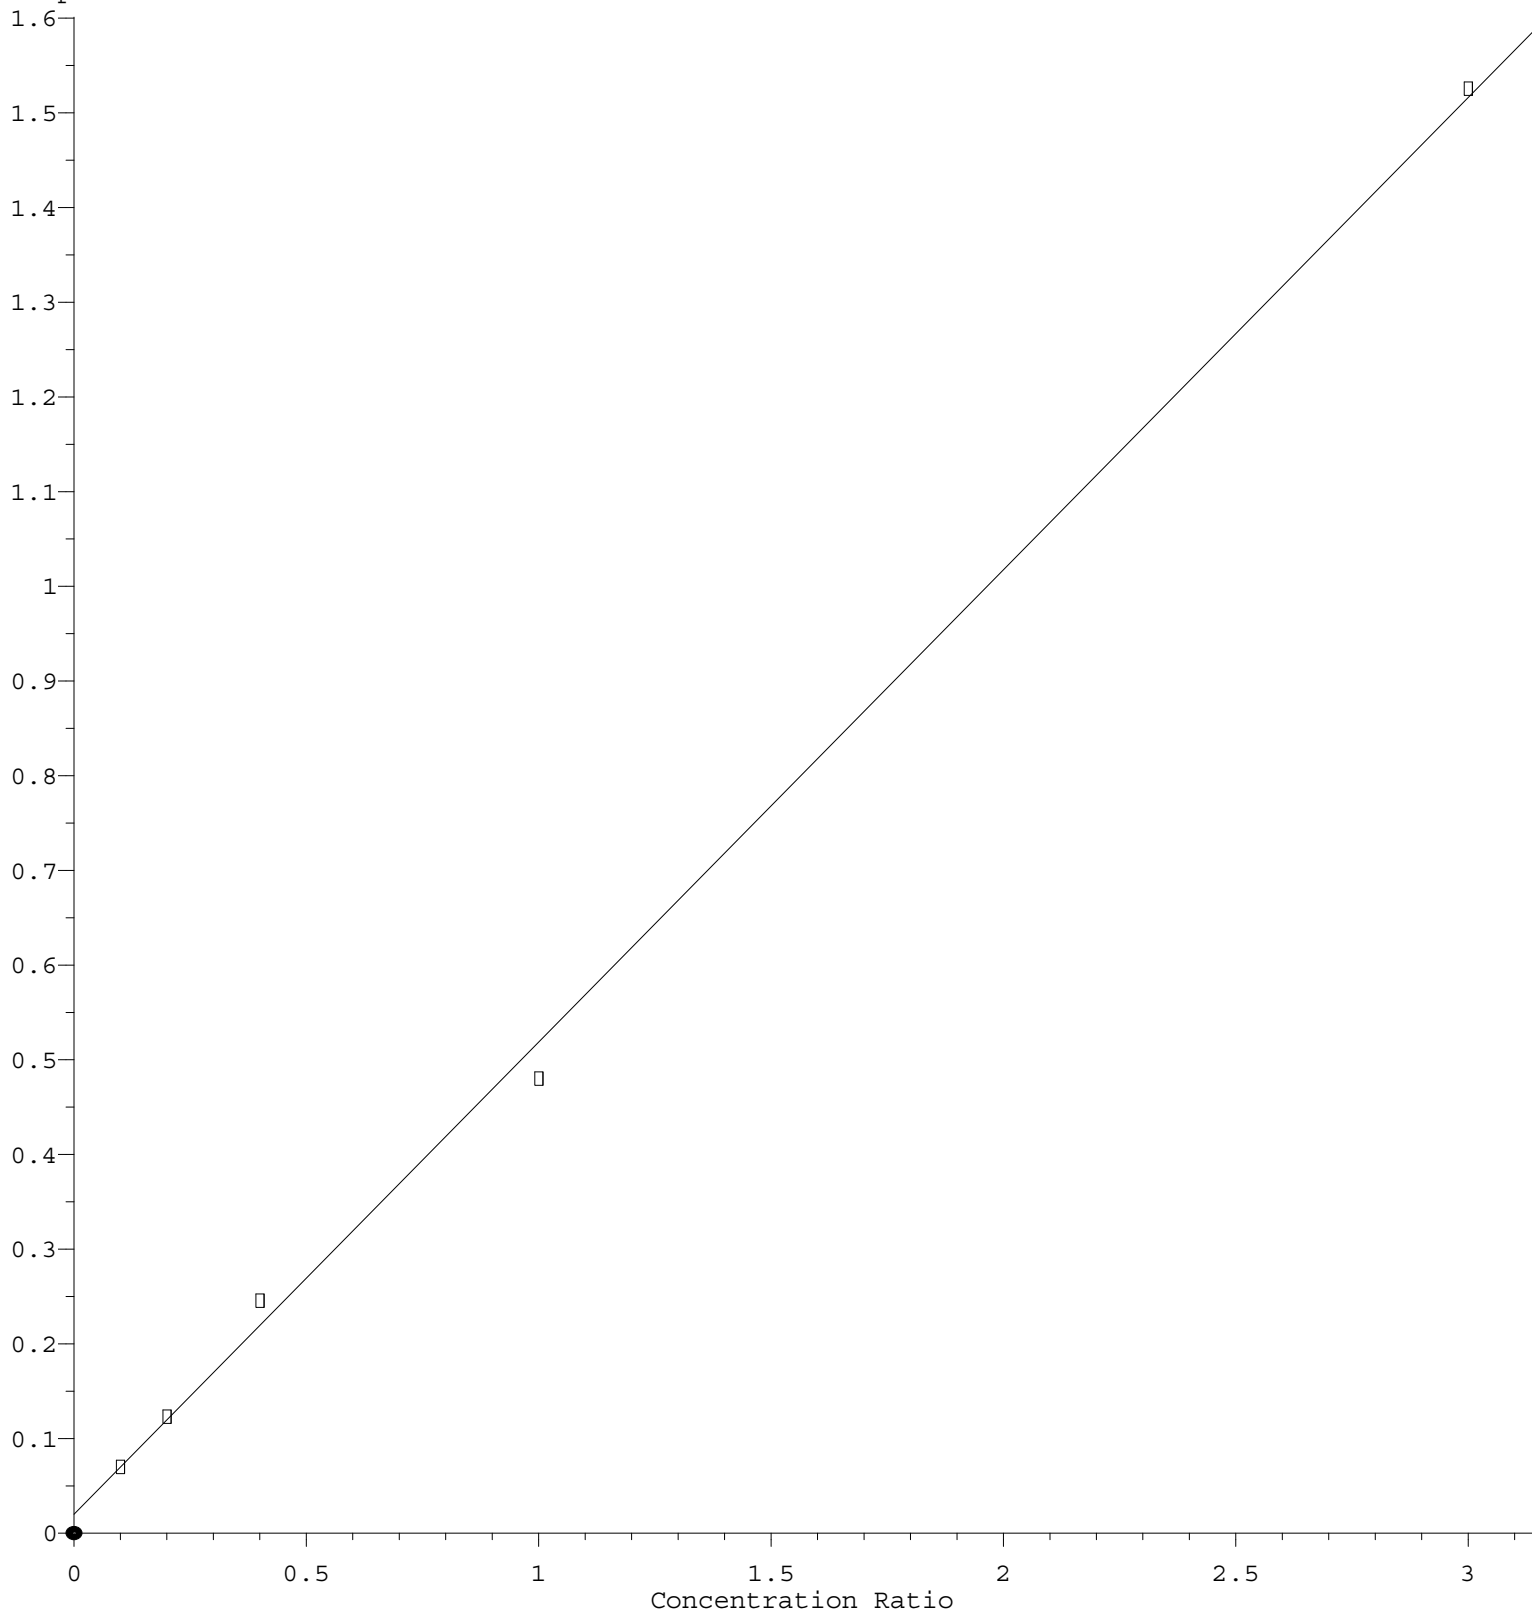

$$\text{Response} = 4.988\text{e-}001 * \text{Amt} + 1.997\text{e-}002$$


Coef of Det (r^2) = 0.998423 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M

Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Cyclohexane


Response Ratio

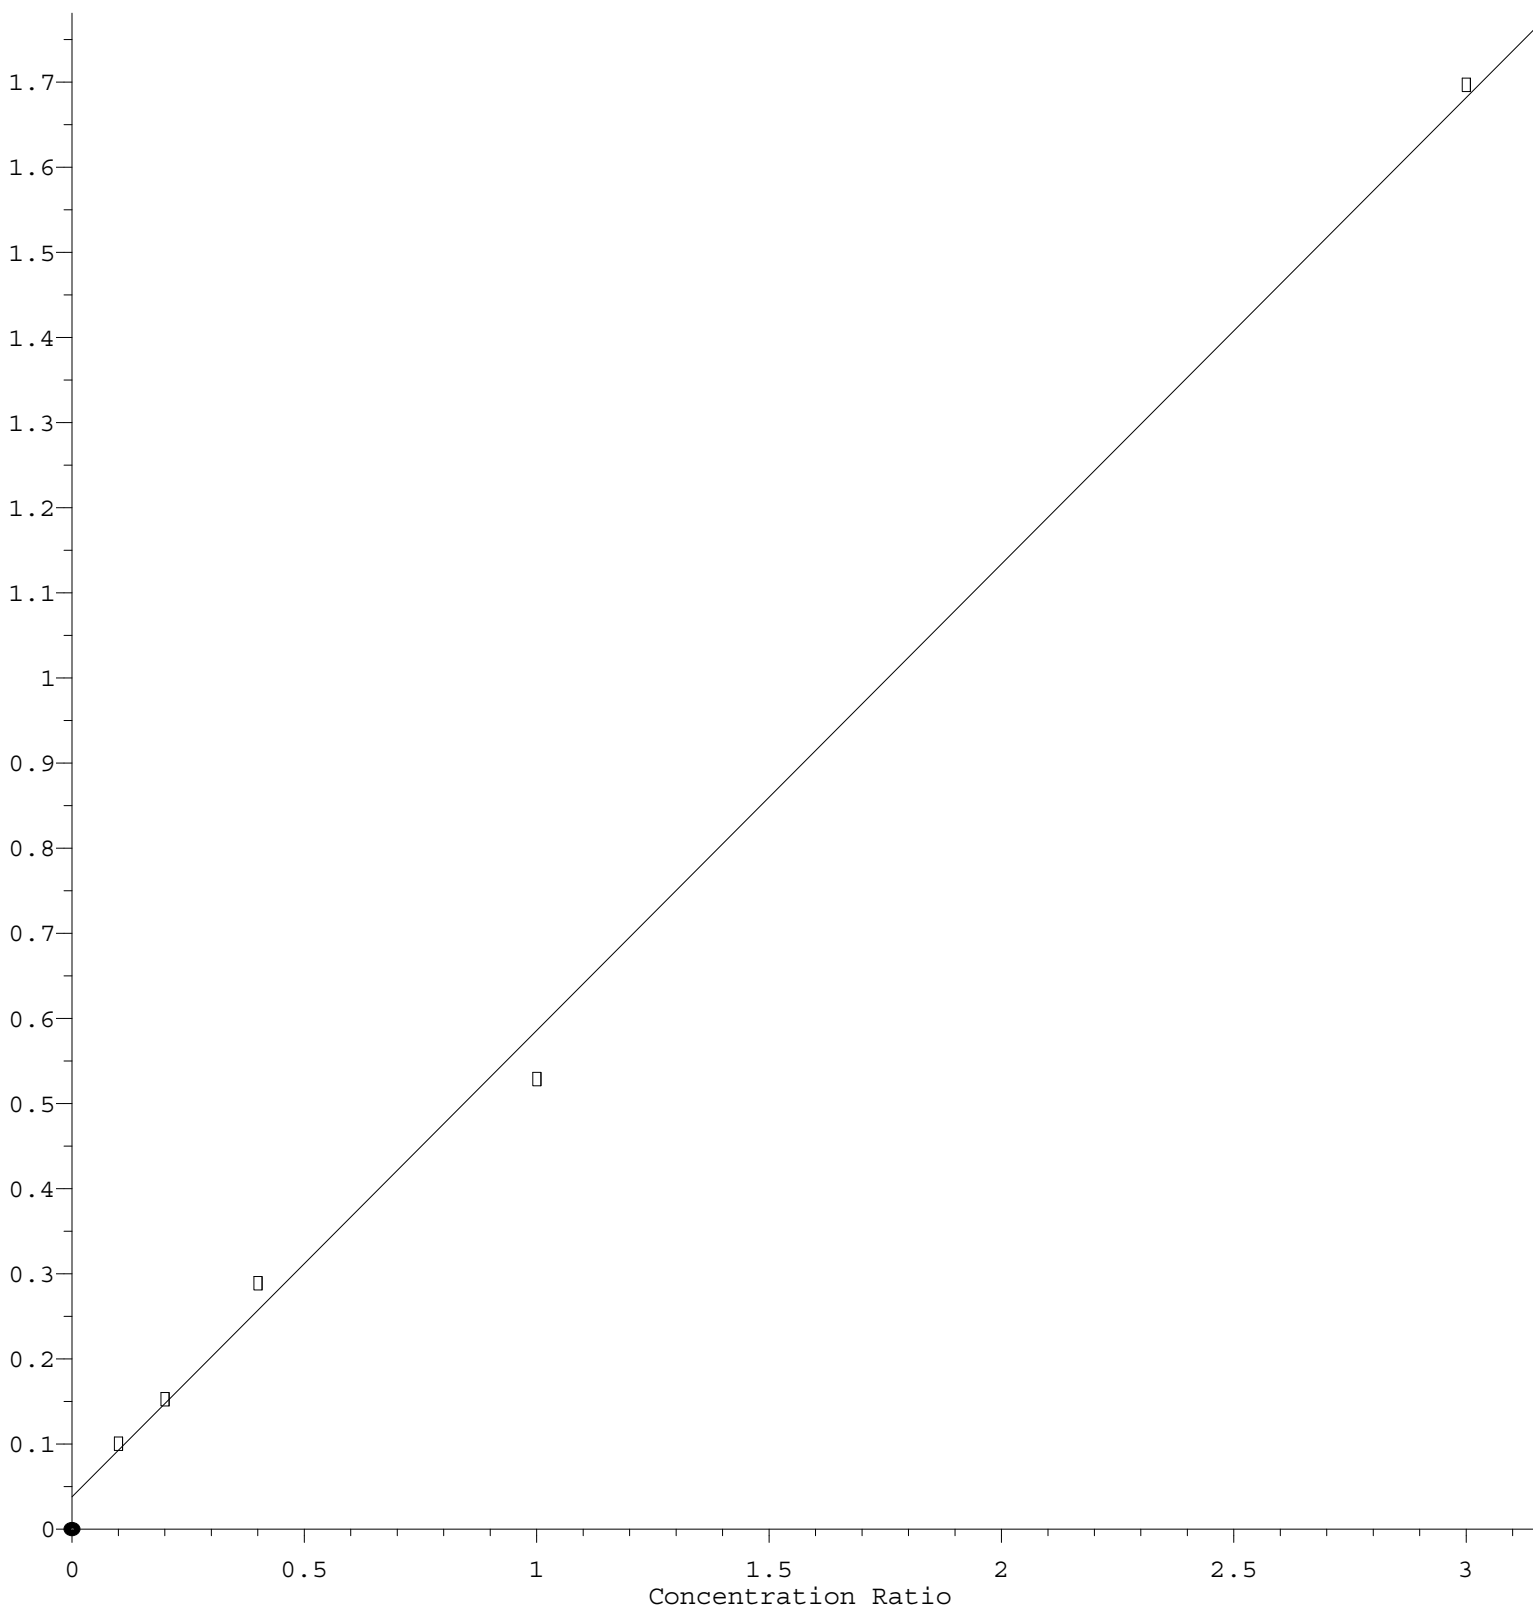

$\text{Response} = 5.479\text{e-}001 * \text{Amt} + 3.845\text{e-}002$
 Coef of Det (r^2) = 0.997365 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M
 Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Methylene Chloride

Response Ratio

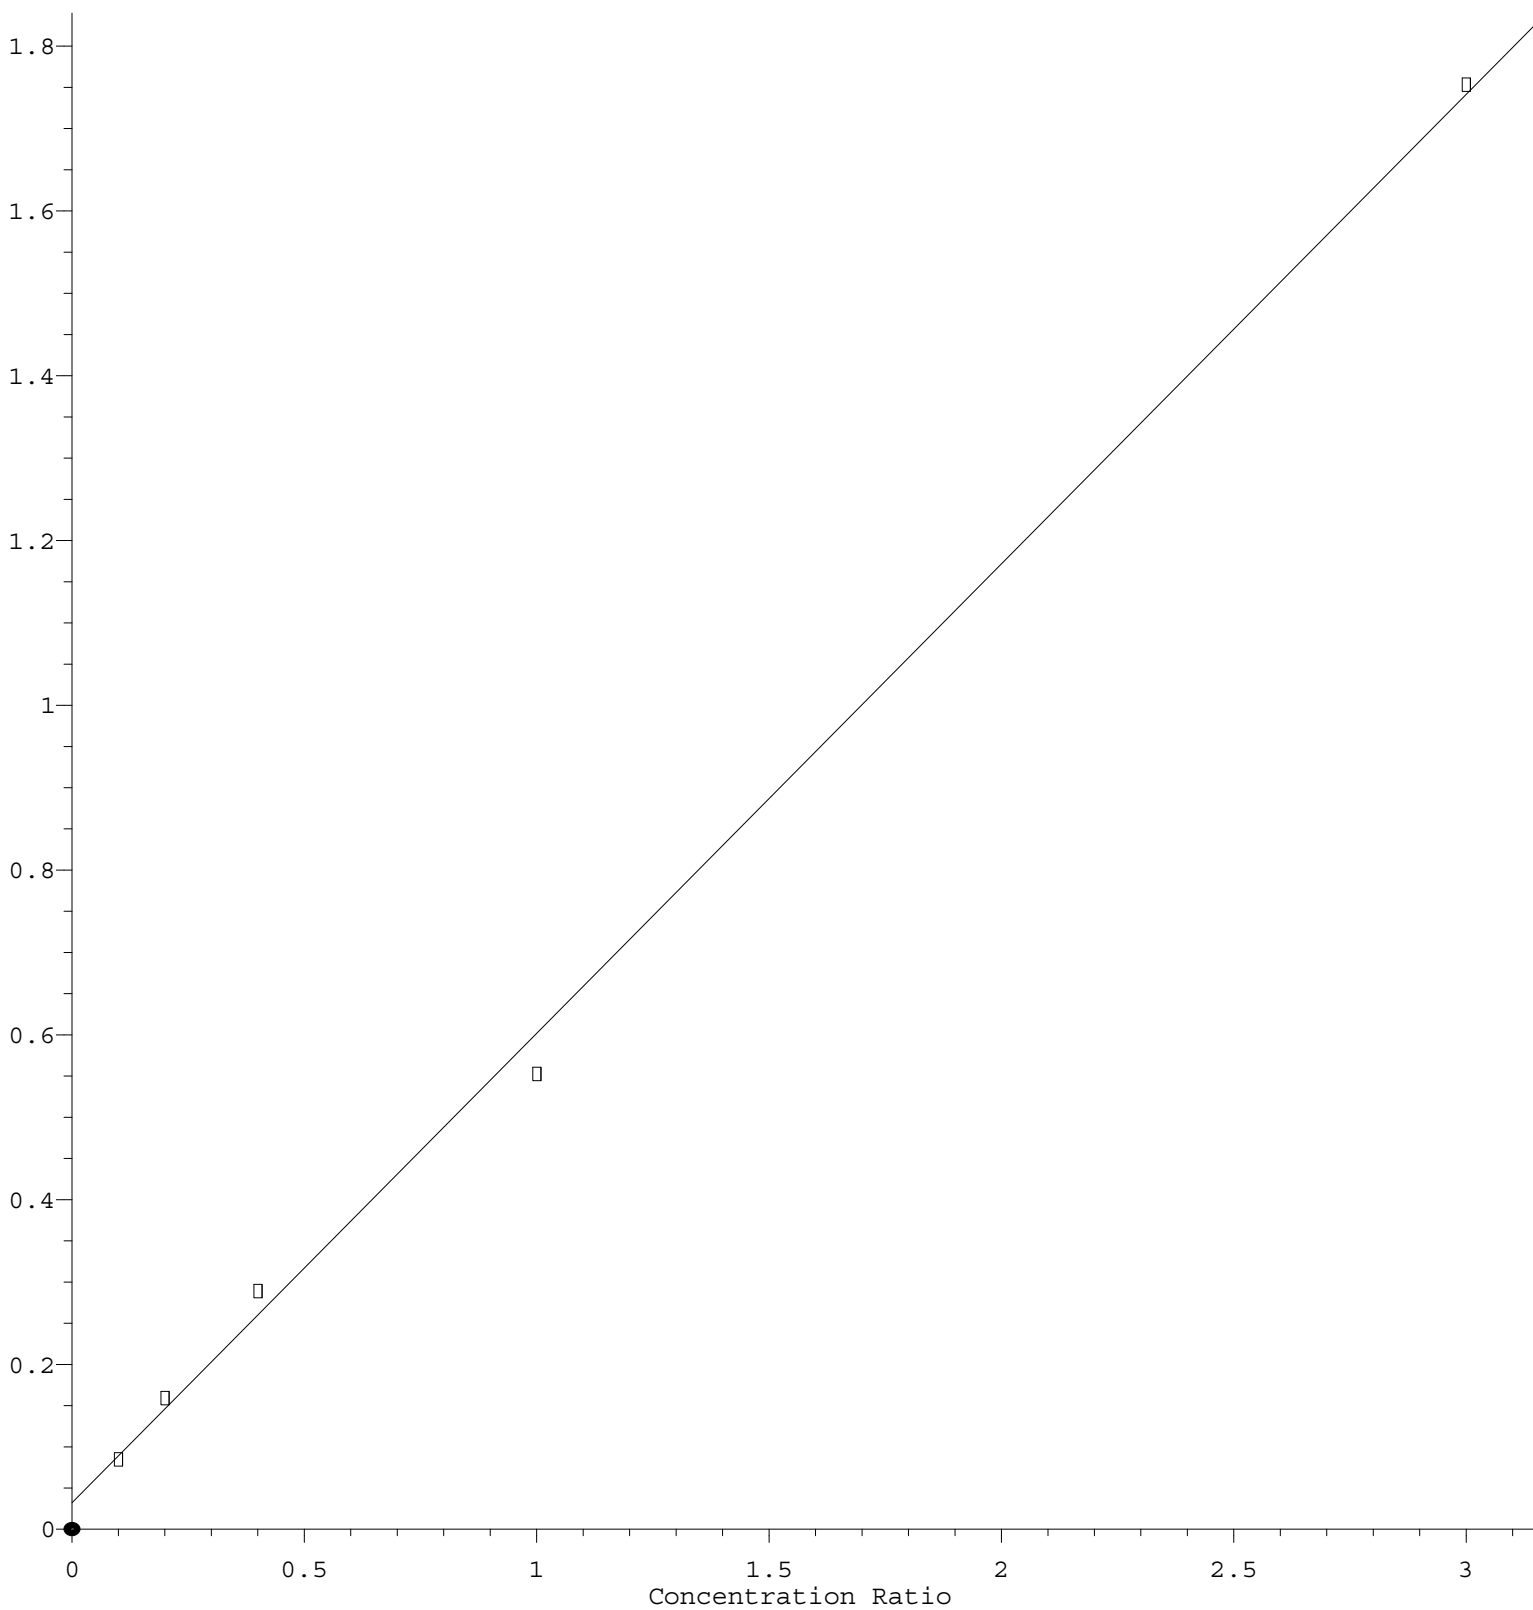


$$\text{Response} = 5.697\text{e-}001 * \text{Amt} + 3.218\text{e-}002$$

Coef of Det (r^2) = 0.998082 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M

Calibration Table Last Updated: Thu Feb 24 07:13:58 2022


Methyl Acetate

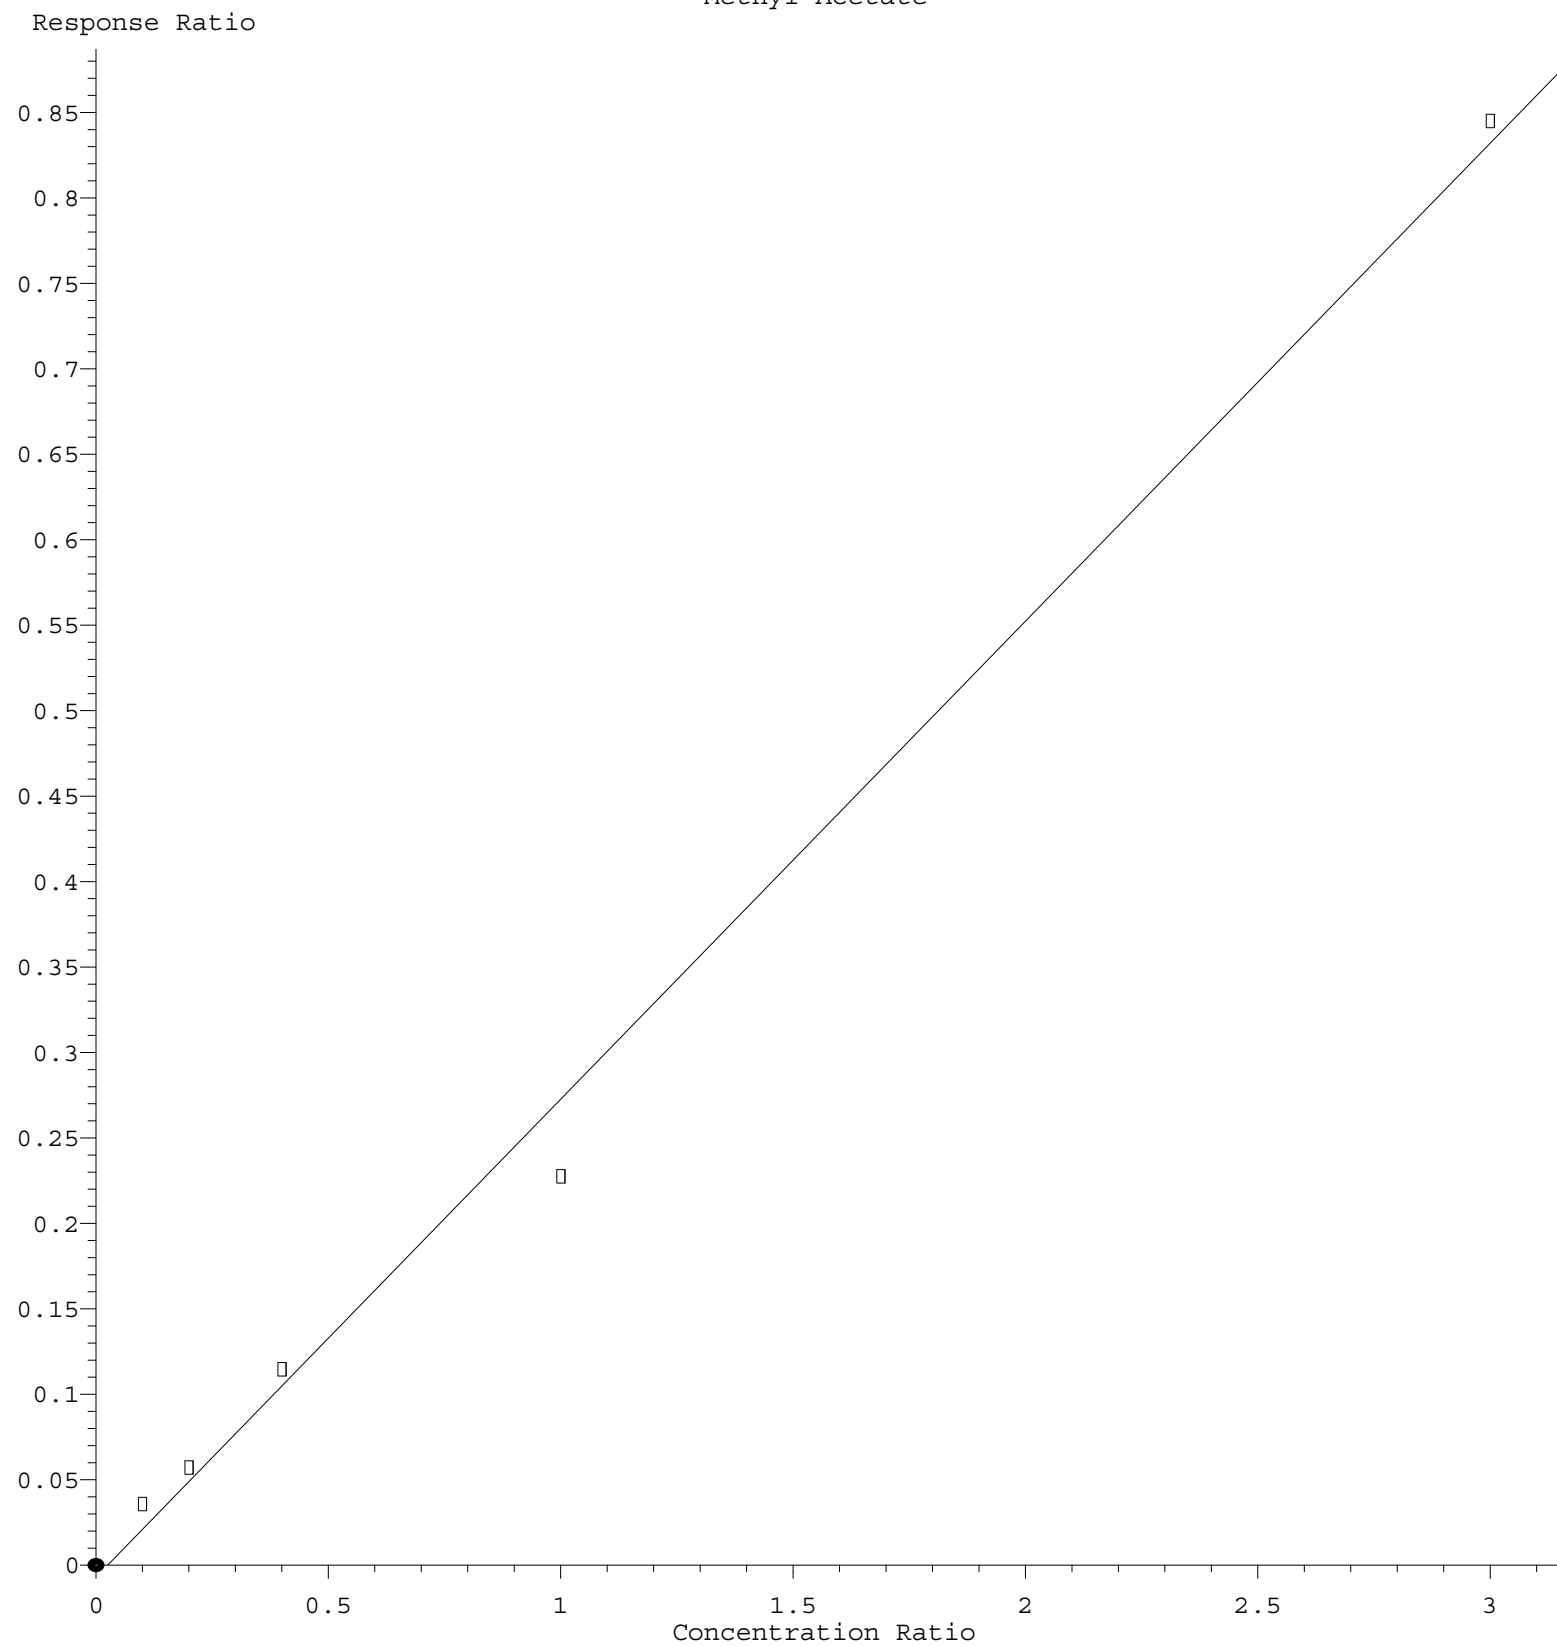

Response = 2.797e-001 * Amt - 6.951e-003
Coef of Det (r^2) = 0.994321 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M
Calibration Table Last Updated: Thu Feb 24 07:13:58 2022

Bromomethane

Response Ratio

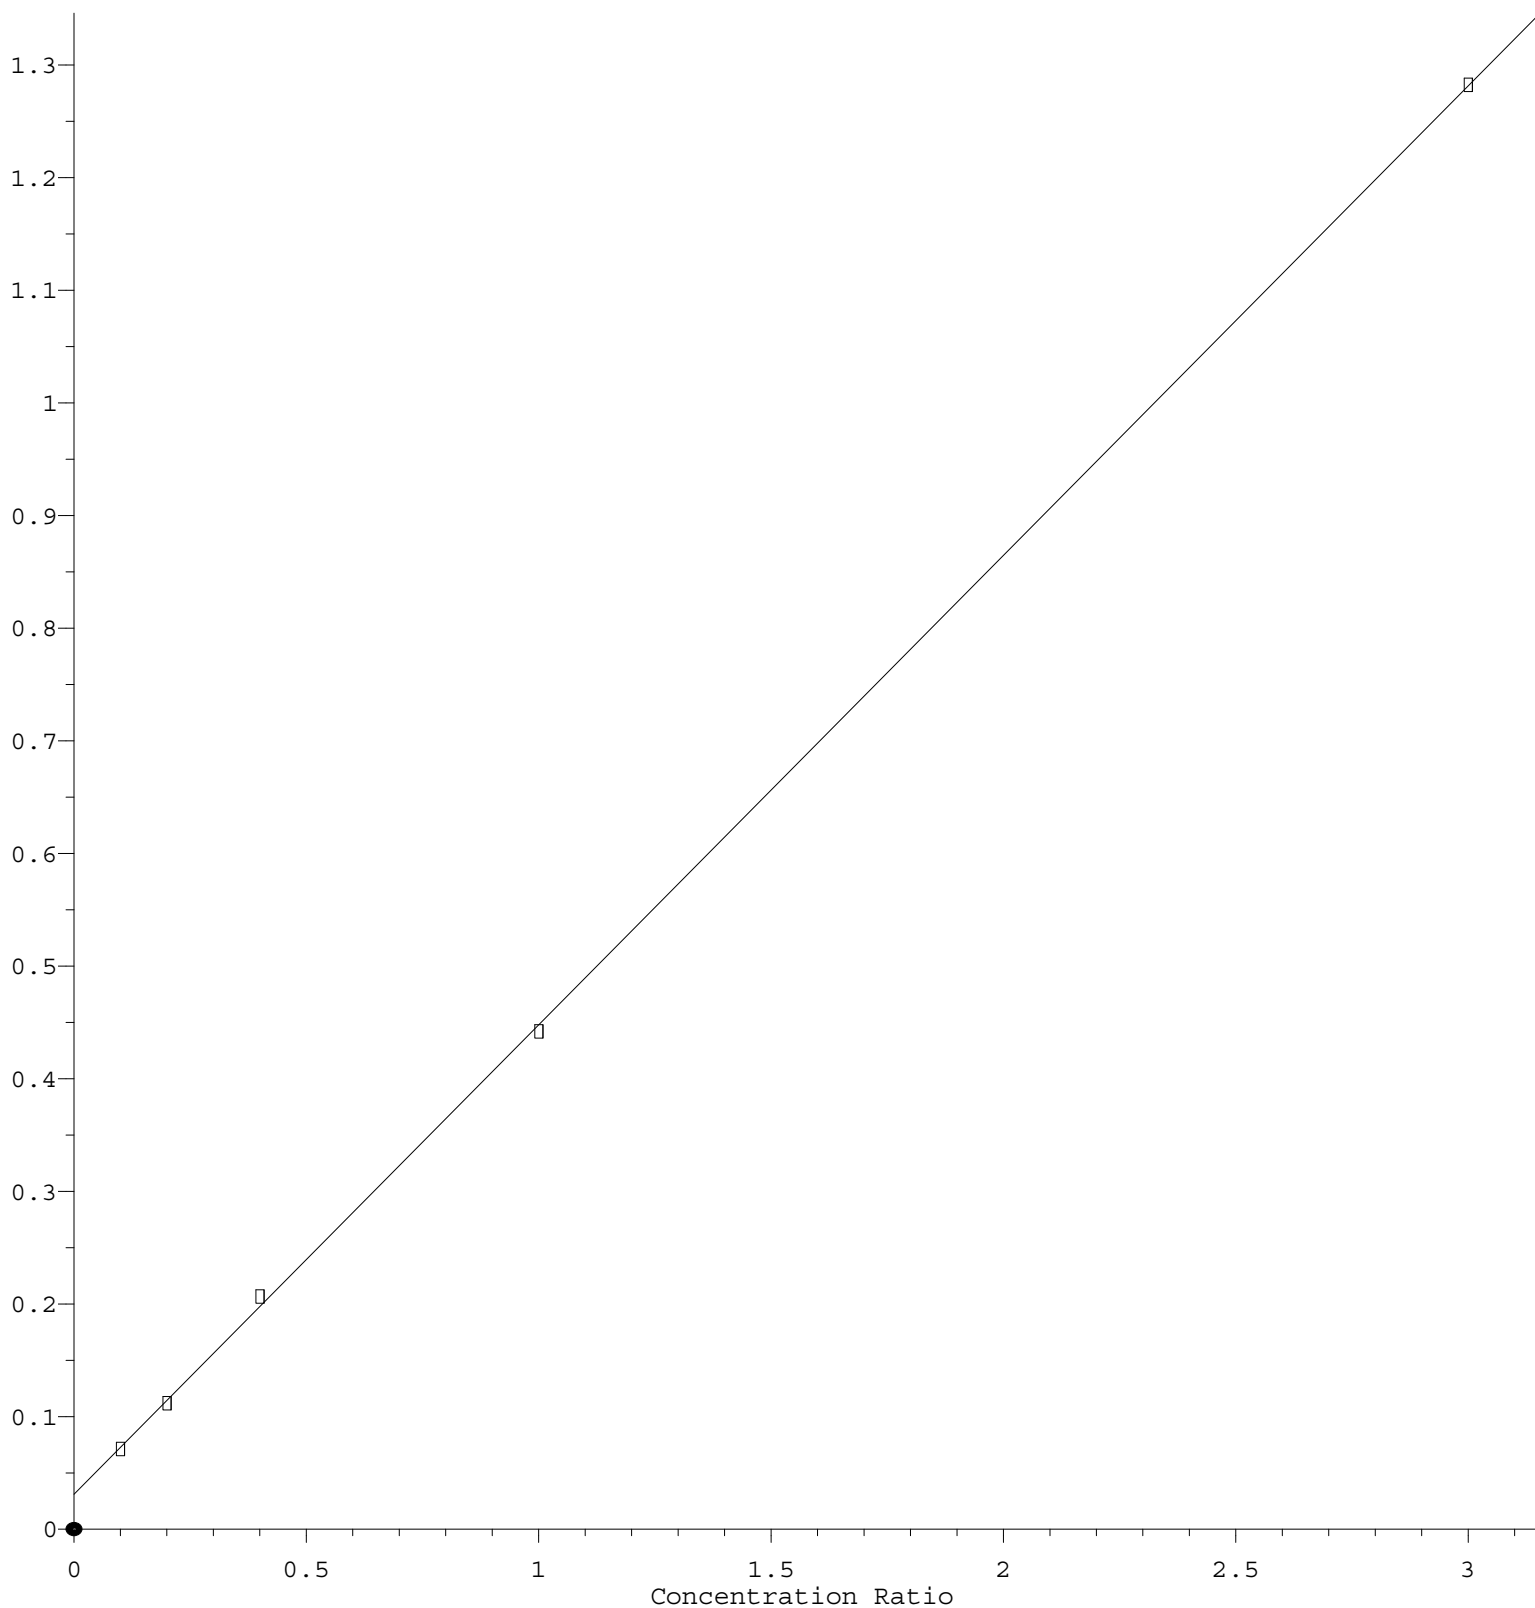

$$\text{Response} = 4.168\text{e-}001 * \text{Amt} + 3.098\text{e-}002$$

Coef of Det (r^2) = 0.999878 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022322S.M

Calibration Table Last Updated: Thu Feb 24 07:13:58 2022