
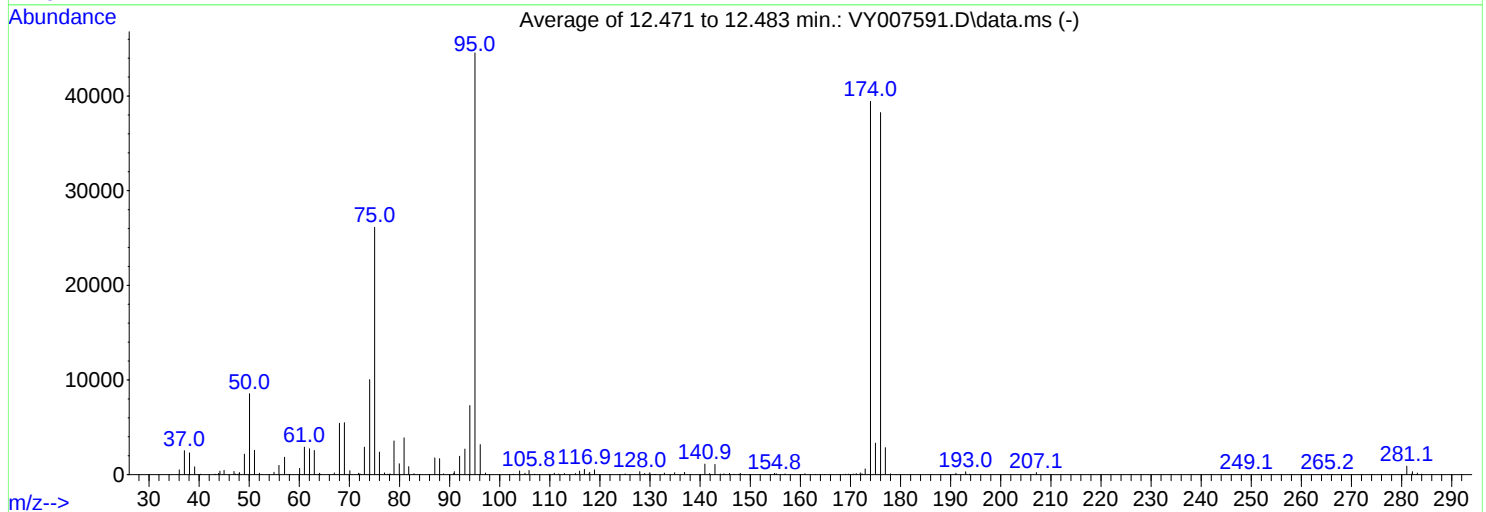


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022322\
 Data File : VY007591.D
 Acq On : 23 Feb 2022 09:54
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022322S.M
 Title : SW846 8260
 Last Update : Thu Feb 24 07:13:58 2022

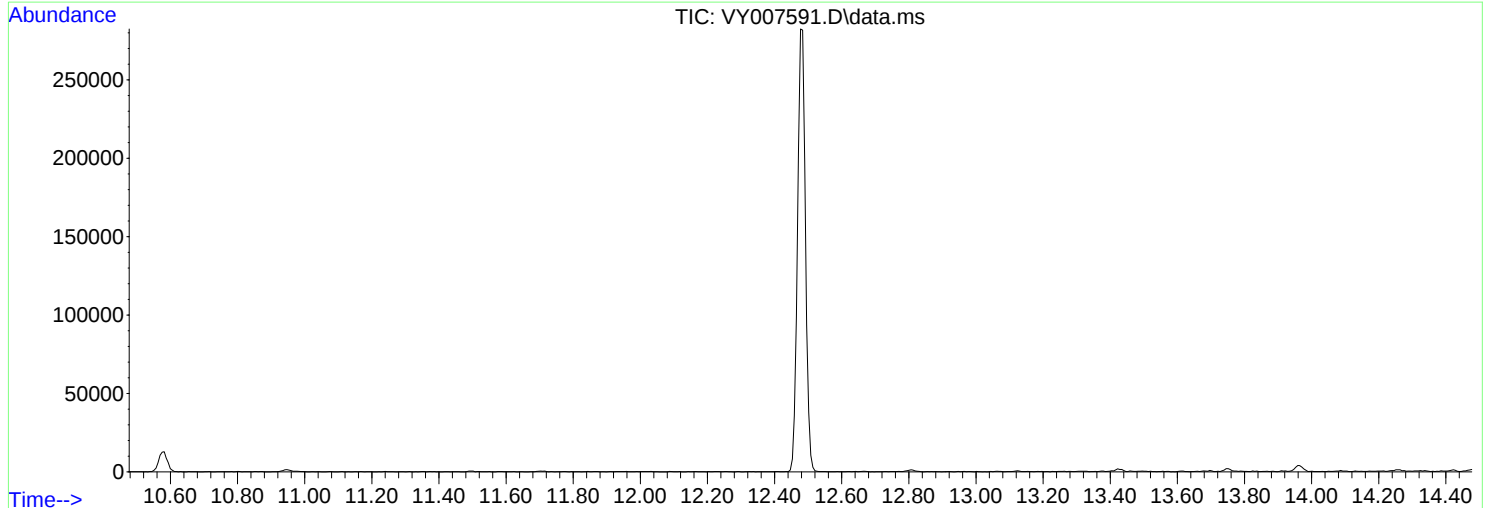

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	8561	PASS
75	95	30	60	58.6	26128	PASS
95	95	100	100	100.0	44560	PASS
96	95	5	9	7.1	3177	PASS
173	174	0.00	2	1.6	614	PASS
174	95	50	100	88.5	39443	PASS
175	174	5	9	8.5	3334	PASS
176	174	95	101	97.0	38251	PASS
177	176	5	9	7.5	2863	PASS