
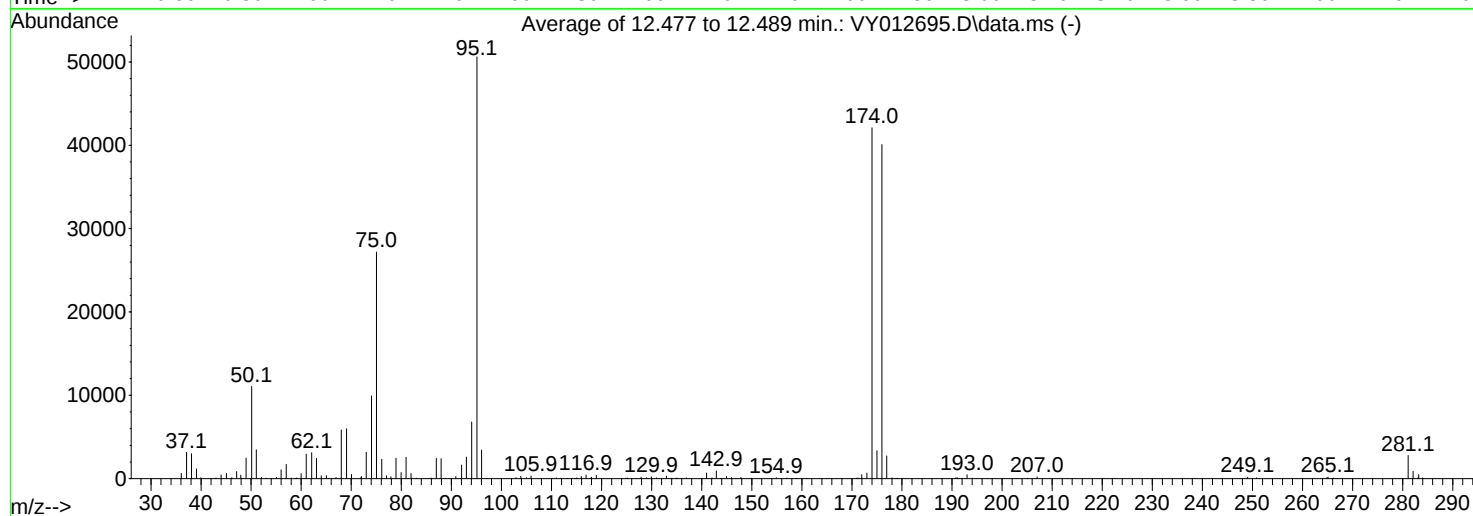


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022323\
Data File : VY012695.D
Acq On : 23 Feb 2023 09:03
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
Title : SW846 8260
Last Update : Wed Feb 22 01:21:05 2023

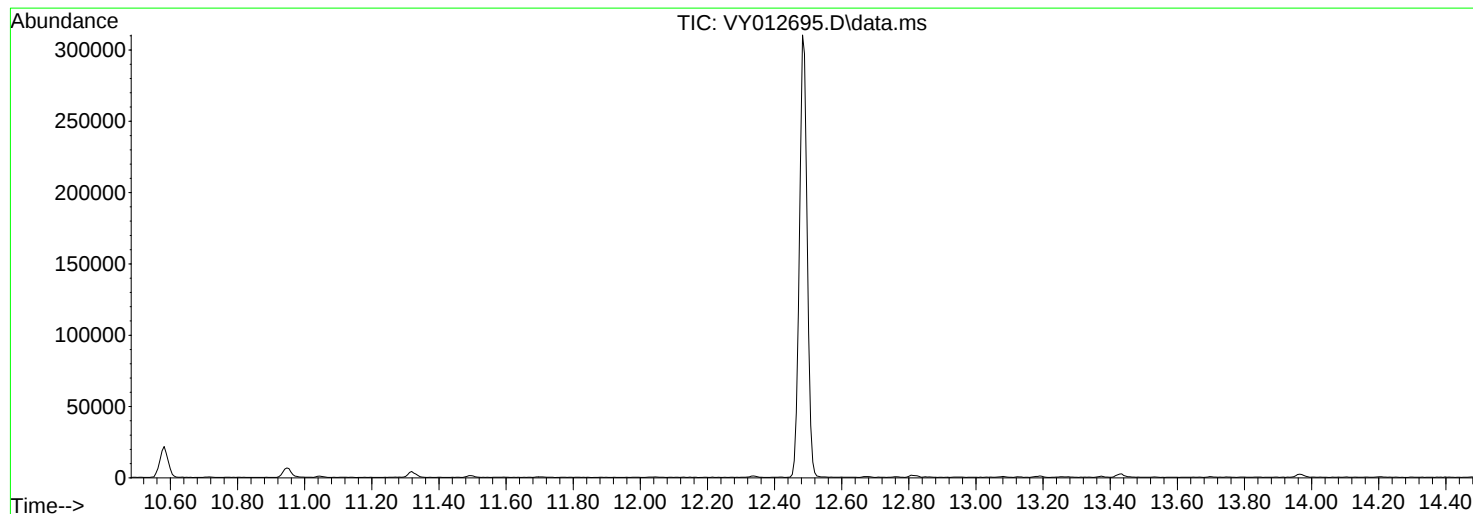

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	11057	PASS
75	95	30	60	53.7	27184	PASS
95	95	100	100	100.0	50613	PASS
96	95	5	9	6.8	3430	PASS
173	174	0.00	2	1.6	673	PASS
174	95	50	100	83.2	42109	PASS
175	174	5	9	8.0	3363	PASS
176	174	95	101	95.2	40080	PASS
177	176	5	9	6.8	2736	PASS