

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022423\
 Data File : VY012719.D
 Acq On : 24 Feb 2023 13:24
 Operator : KP/MD
 Sample : 01665-01RE
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-231RE

Quant Time: Feb 25 00:48:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 22 01:21:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	42895	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	70566	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	63810	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	24007	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	24112	47.595	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	95.180%
35) Dibromofluoromethane	7.716	113	24250	50.878	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.760%
50) Toluene-d8	10.179	98	85222	47.726	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	95.460%
62) 4-Bromofluorobenzene	12.483	95	22439	39.269	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	78.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022423\
Data File : VY012719.D
Acq On : 24 Feb 2023 13:24
Operator : KP/MD
Sample : 01665-01RE
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-231RE

Quant Time: Feb 25 00:48:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 22 01:21:05 2023
Response via : Initial Calibration




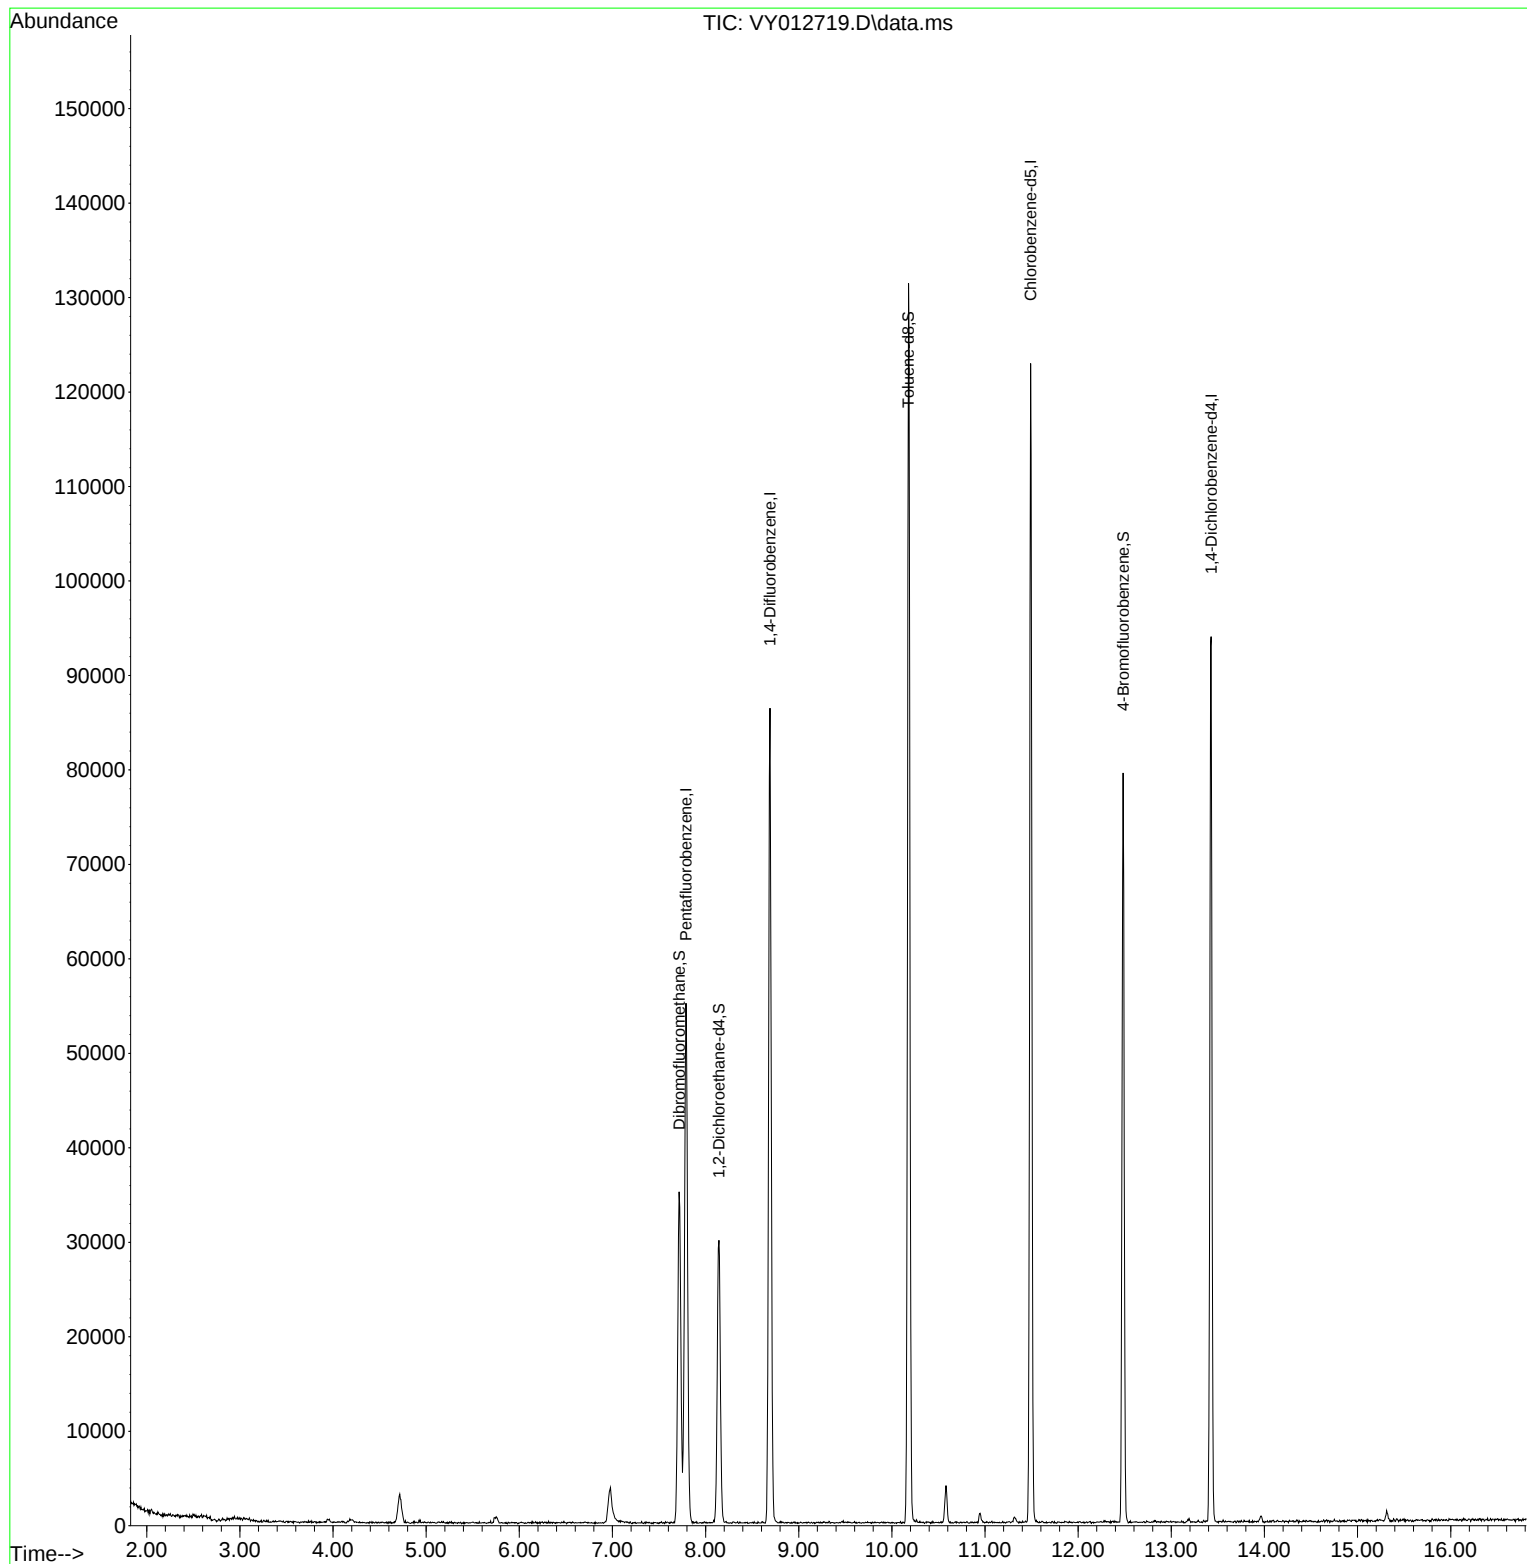


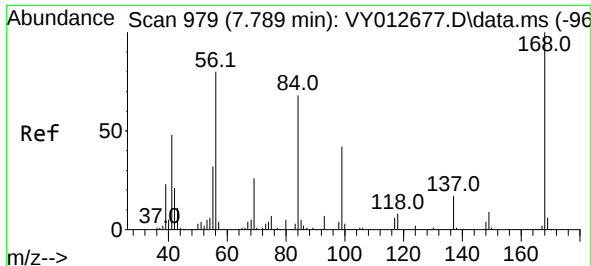

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-231RE


Tgt Ion:168 Resp: 42895
Ion Ratio Lower Upper
168 100
99 50.3 45.4 68.2

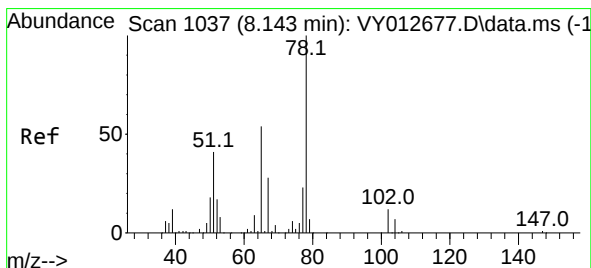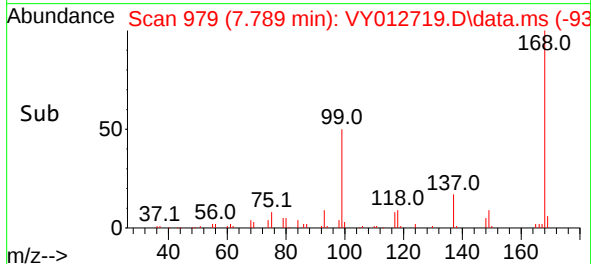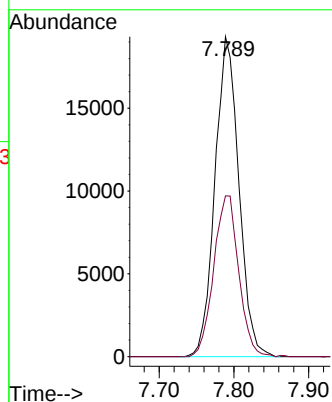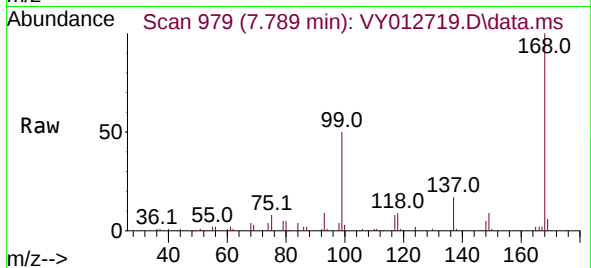

#33
1,2-Dichloroethane-d4
Concen: 47.595 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24

Tgt Ion: 65 Resp: 24112
Ion Ratio Lower Upper
65 100
67 52.3 0.0 104.6

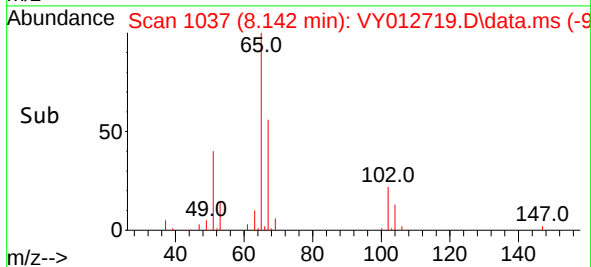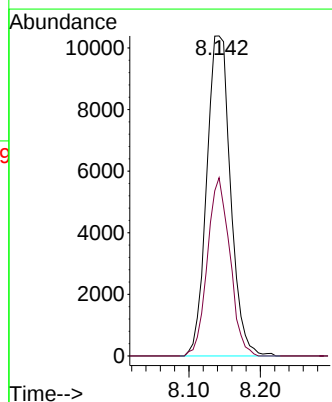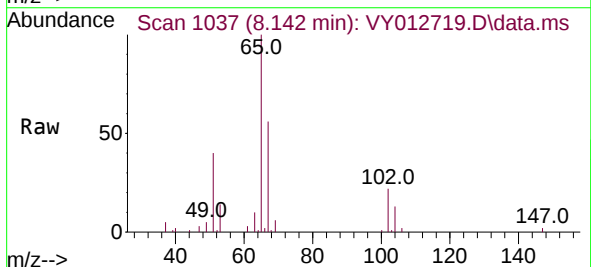

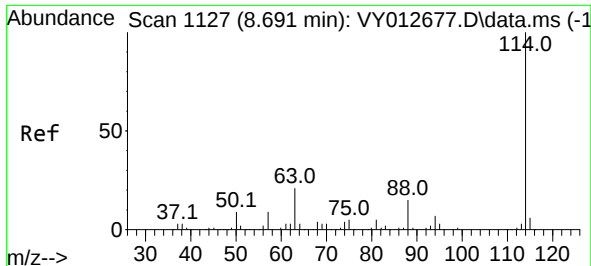

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY012719.D

Acq: 24 Feb 2023 13:24

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-231RE





Tgt Ion:114 Resp: 70566

Ion Ratio Lower Upper

114 100

63 19.6 0.0 42.8

88 14.7 0.0 29.6

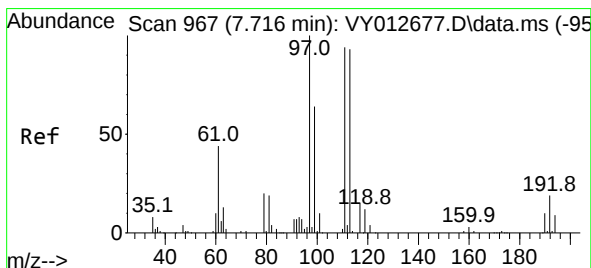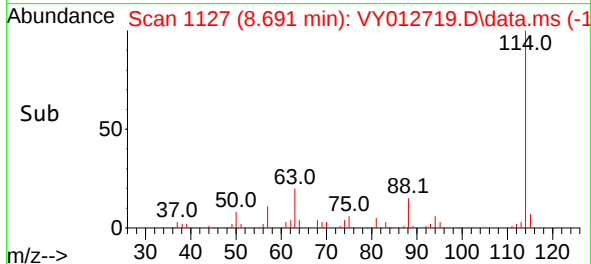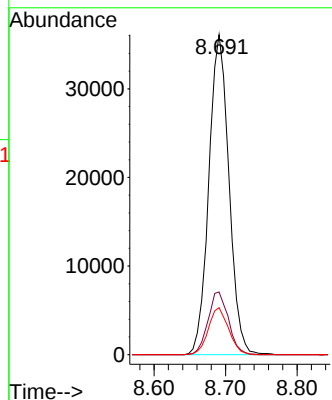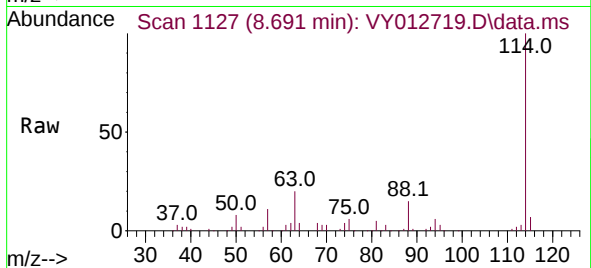

#35

Dibromofluoromethane

Concen: 50.878 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012719.D

Acq: 24 Feb 2023 13:24




Tgt Ion:113 Resp: 24250


Ion Ratio Lower Upper

113 100

111 102.3 82.0 123.0

192 20.8 16.2 24.2


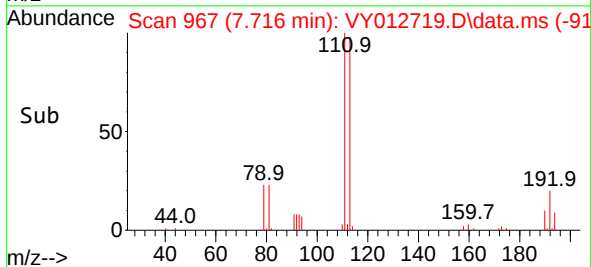
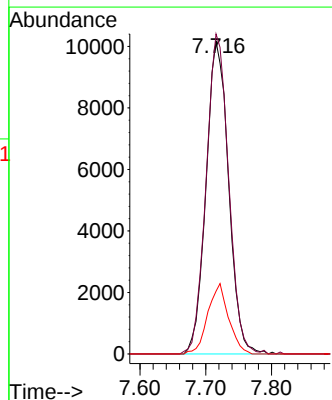
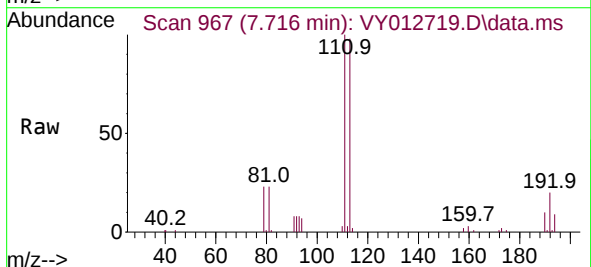


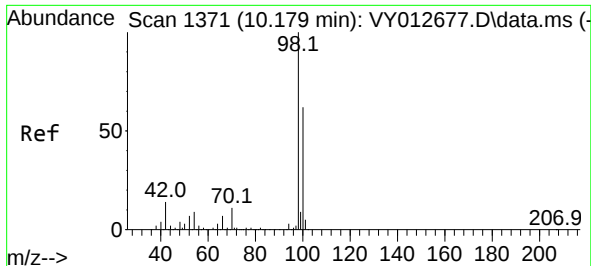

#50
Toluene-d8
Concen: 47.726 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.001 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-231RE


Tgt Ion: 98 Resp: 85222
Ion Ratio Lower Upper
98 100
100 63.5 51.2 76.8

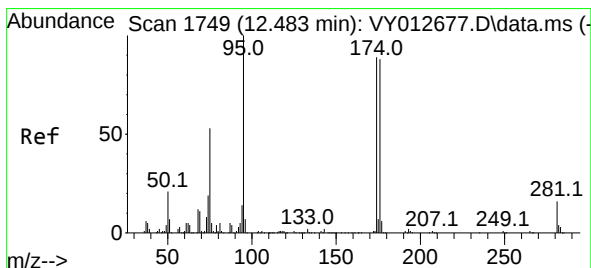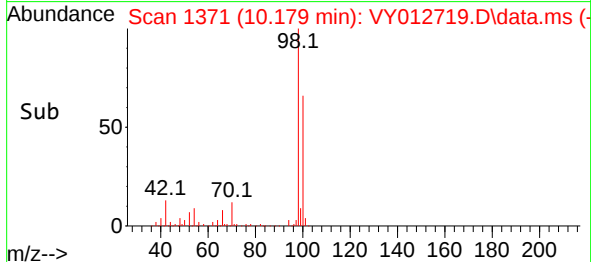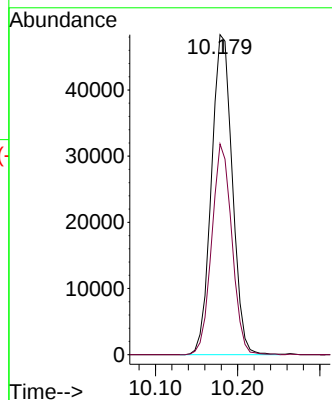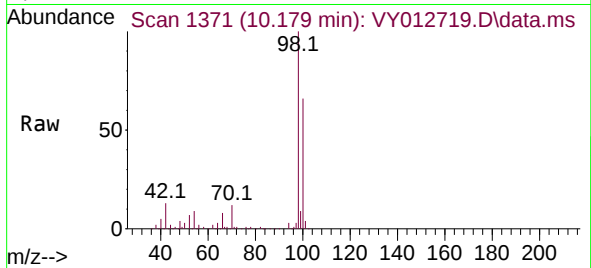

#62
4-Bromofluorobenzene
Concen: 39.269 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24

Tgt Ion: 95 Resp: 22439
Ion Ratio Lower Upper
95 100
174 91.0 0.0 172.8
176 87.2 0.0 169.4


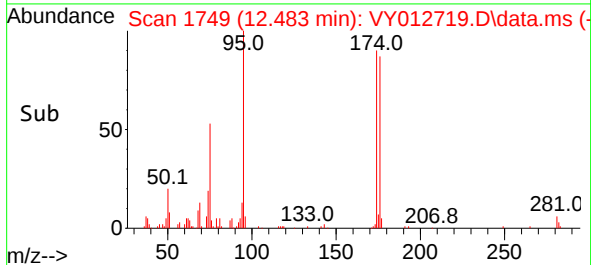
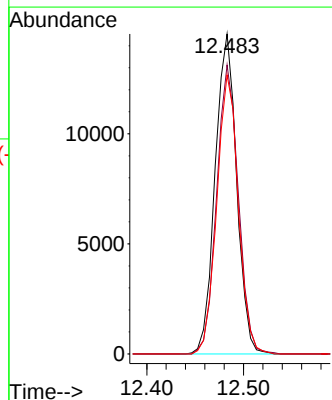
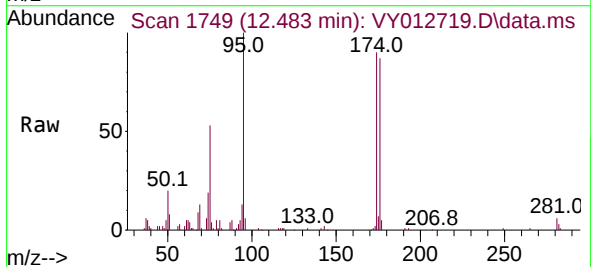


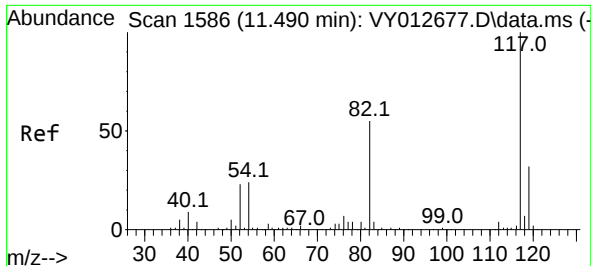

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-231RE

Tgt Ion:117 Resp: 63810
Ion Ratio Lower Upper
117 100
82 55.7 44.1 66.1
119 34.0 25.5 38.3

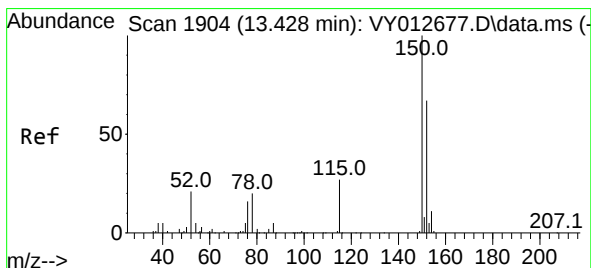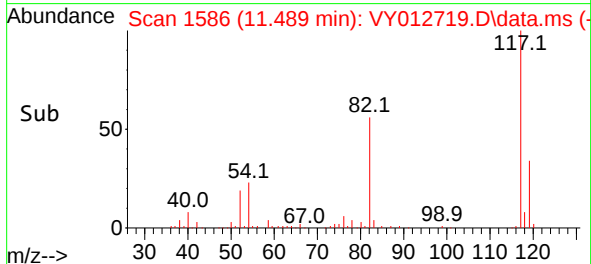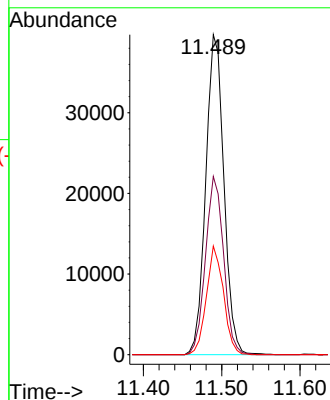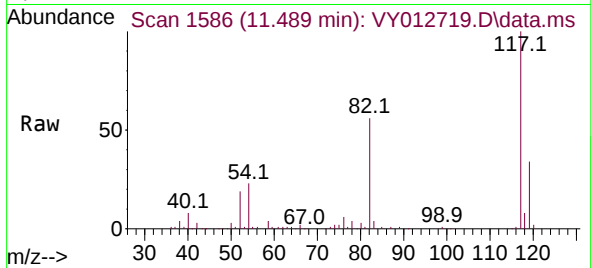

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012719.D
Acq: 24 Feb 2023 13:24

Tgt Ion:152 Resp: 24007
Ion Ratio Lower Upper
152 100
115 57.4 28.7 86.3
150 160.1 0.0 347.6

