
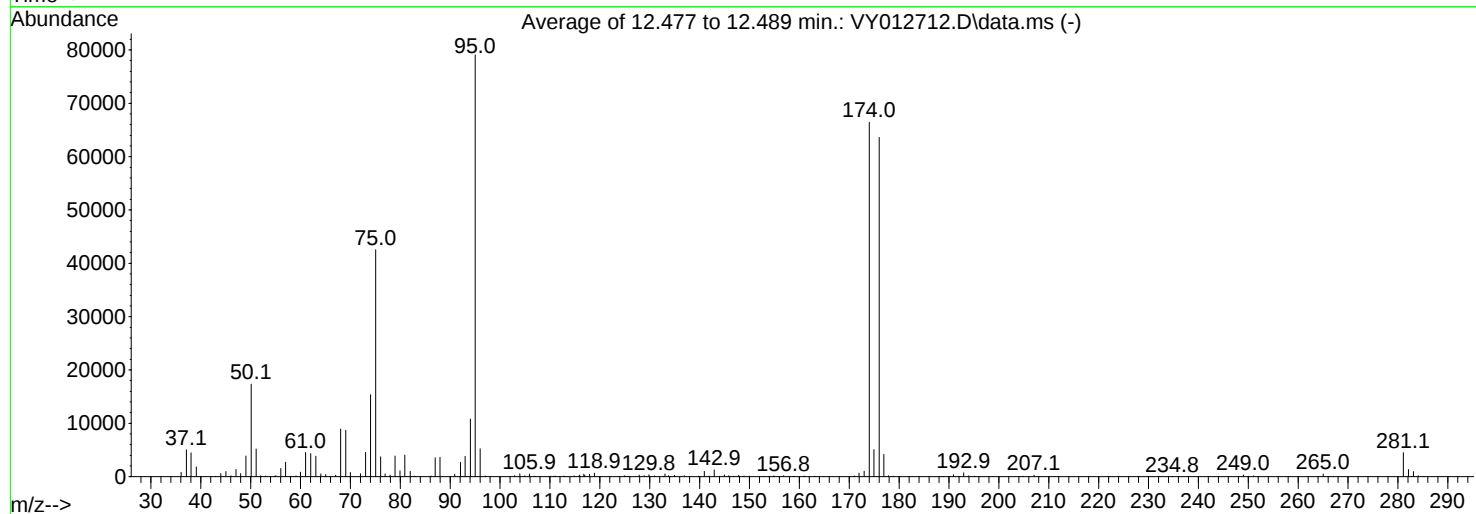


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022423\
Data File : VY012712.D
Acq On : 24 Feb 2023 08:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022123S.M
Title : SW846 8260
Last Update : Wed Feb 22 01:21:05 2023

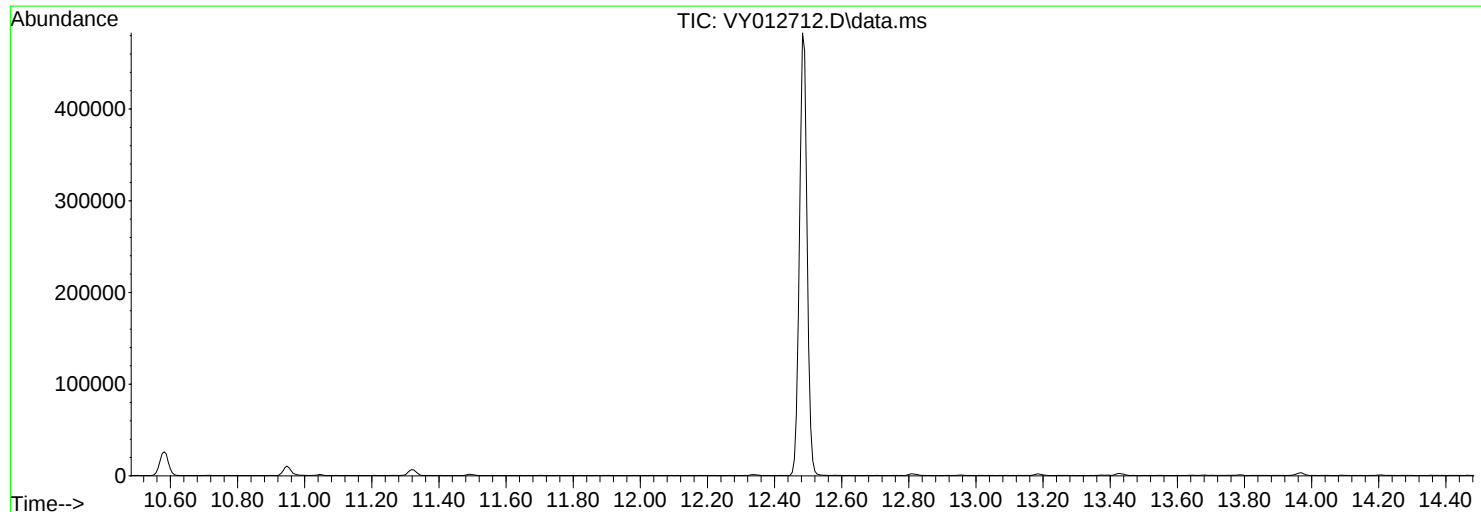

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	17333	PASS
75	95	30	60	53.8	42536	PASS
95	95	100	100	100.0	79085	PASS
96	95	5	9	6.6	5222	PASS
173	174	0.00	2	1.6	1033	PASS
174	95	50	100	84.0	66445	PASS
175	174	5	9	7.6	5064	PASS
176	174	95	101	95.7	63595	PASS
177	176	5	9	6.6	4186	PASS