

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022525\  
Data File : VY021318.D  
Acq On : 25 Feb 2025 17:54  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y022525S.M

Title : SW846 8260

Signal : TIC: VY021318.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 6.884       | 838           | 847         | 858          | rBV2     | 9452           | 29497         | 1.84%           | 0.361%        |
| 2         | 7.634       | 960           | 970         | 976          | rBV      | 213676         | 516145        | 32.20%          | 6.310%        |
| 3         | 7.707       | 976           | 982         | 996          | rVB      | 326721         | 746878        | 46.60%          | 9.131%        |
| 4         | 8.061       | 1028          | 1040        | 1053         | rBV      | 183002         | 414826        | 25.88%          | 5.071%        |
| 5         | 8.616       | 1122          | 1131        | 1149         | rBV      | 583862         | 1148447       | 71.65%          | 14.040%       |
| 6         | 10.109      | 1366          | 1376        | 1390         | rBV      | 918605         | 1602826       | 100.00%         | 19.595%       |
| 7         | 10.512      | 1435          | 1442        | 1449         | rVB2     | 16021          | 30274         | 1.89%           | 0.370%        |
| 8         | 10.877      | 1496          | 1502        | 1512         | rBV2     | 9693           | 17452         | 1.09%           | 0.213%        |
| 9         | 11.414      | 1582          | 1590        | 1603         | rBV      | 902026         | 1458232       | 90.98%          | 17.828%       |
| 10        | 12.408      | 1746          | 1753        | 1766         | rBV      | 695326         | 1072700       | 66.93%          | 13.114%       |
| 11        | 13.346      | 1901          | 1907        | 1917         | rVB      | 750726         | 1142339       | 71.27%          | 13.966%       |


Sum of corrected areas: 8179616

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022525\  
Data File : VY021318.D  
Acq On : 25 Feb 2025 17:54  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y022525S.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

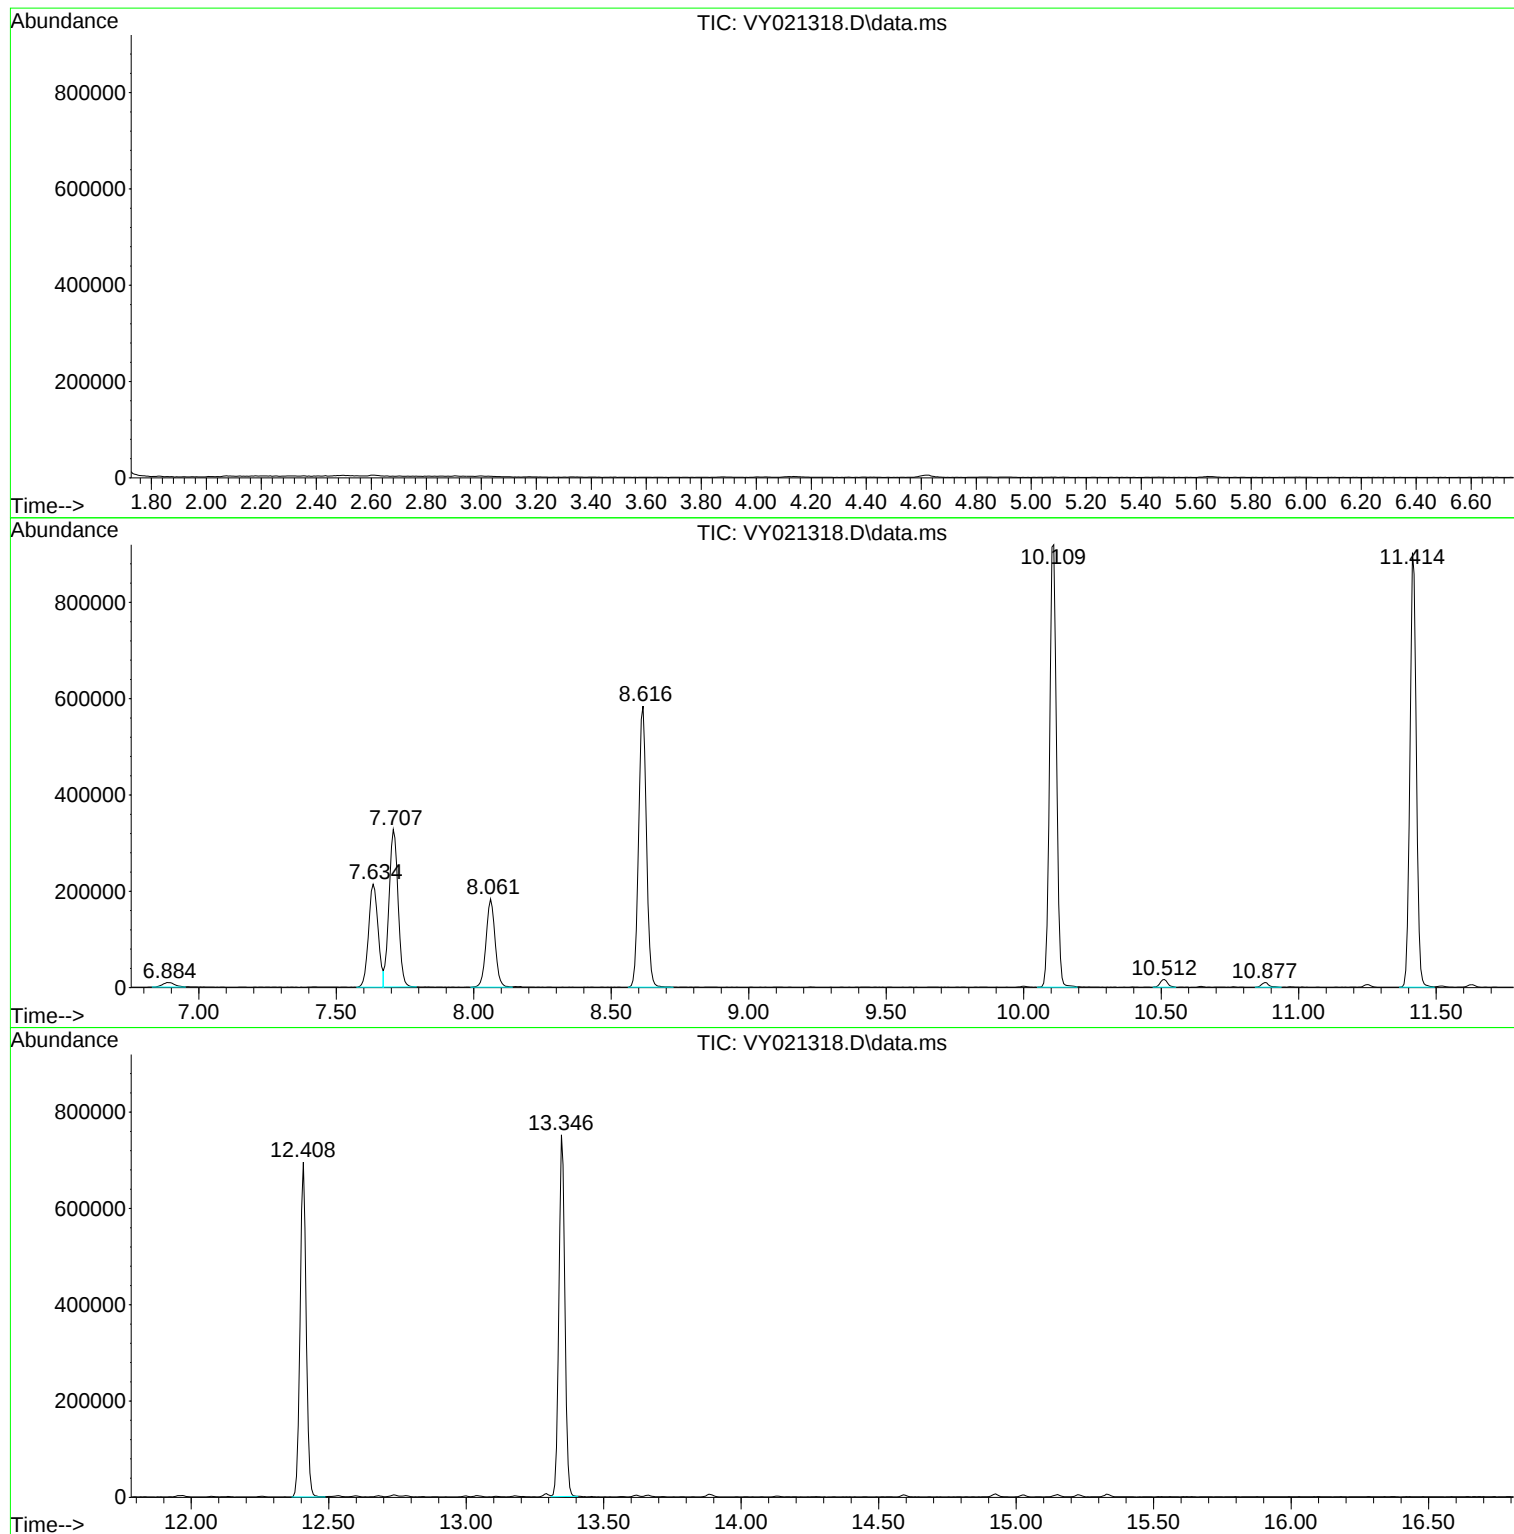

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022525\  
Data File : VY021318.D  
Acq On : 25 Feb 2025 17:54  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y022525S.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY022525\  
Data File : VY021318.D  
Acq On : 25 Feb 2025 17:54  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y022525S.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |