


Dichlorodifluoromethane

Response Ratio

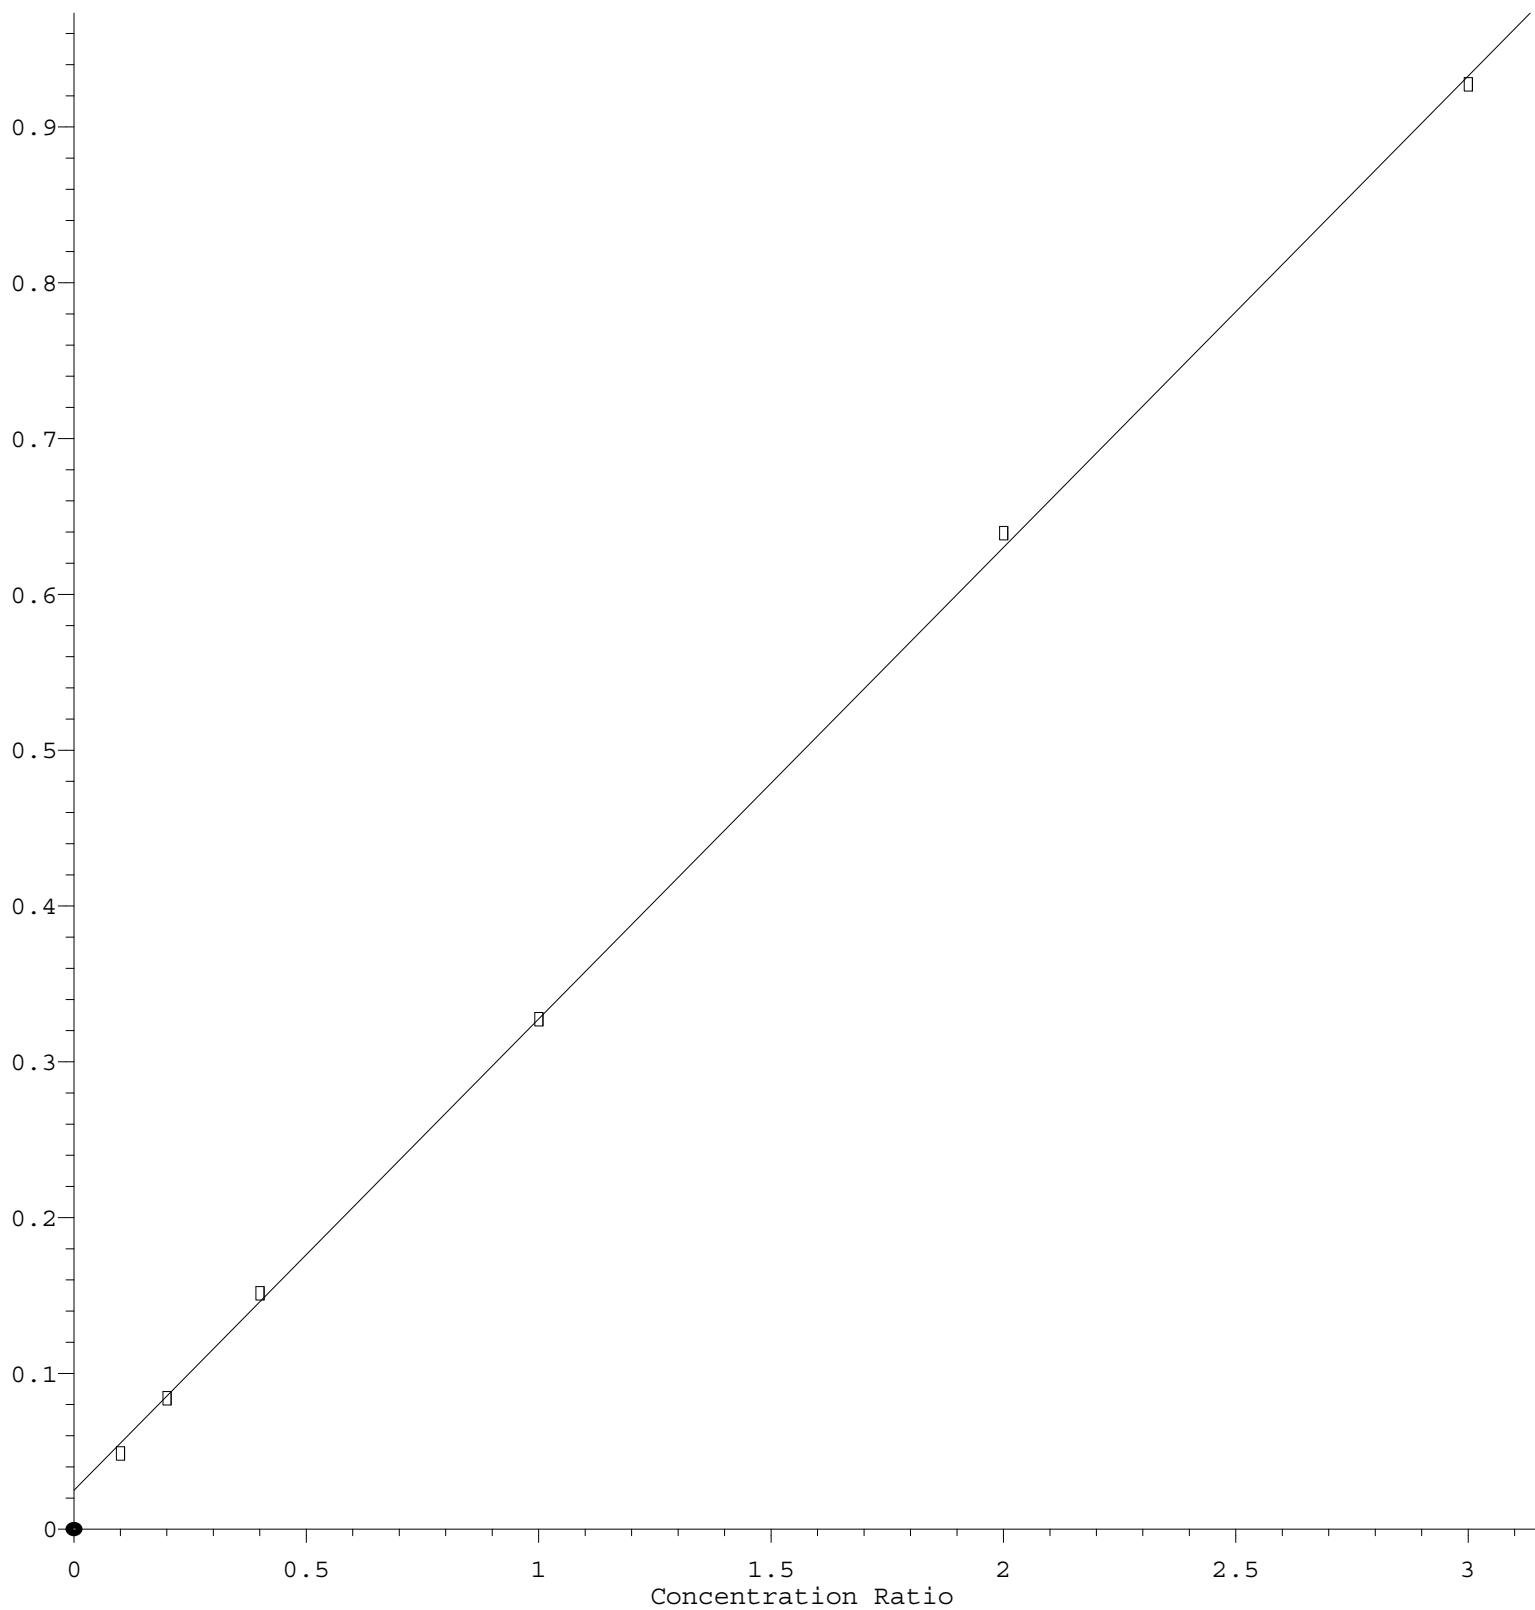

$$\text{Response} = 3.029\text{e-}001 * \text{Amt} + 2.472\text{e-}002$$


Coef of Det (r^2) = 0.999696 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M

Calibration Table Last Updated: Tue Mar 01 09:08:03 2022

Cyclohexane

Response Ratio

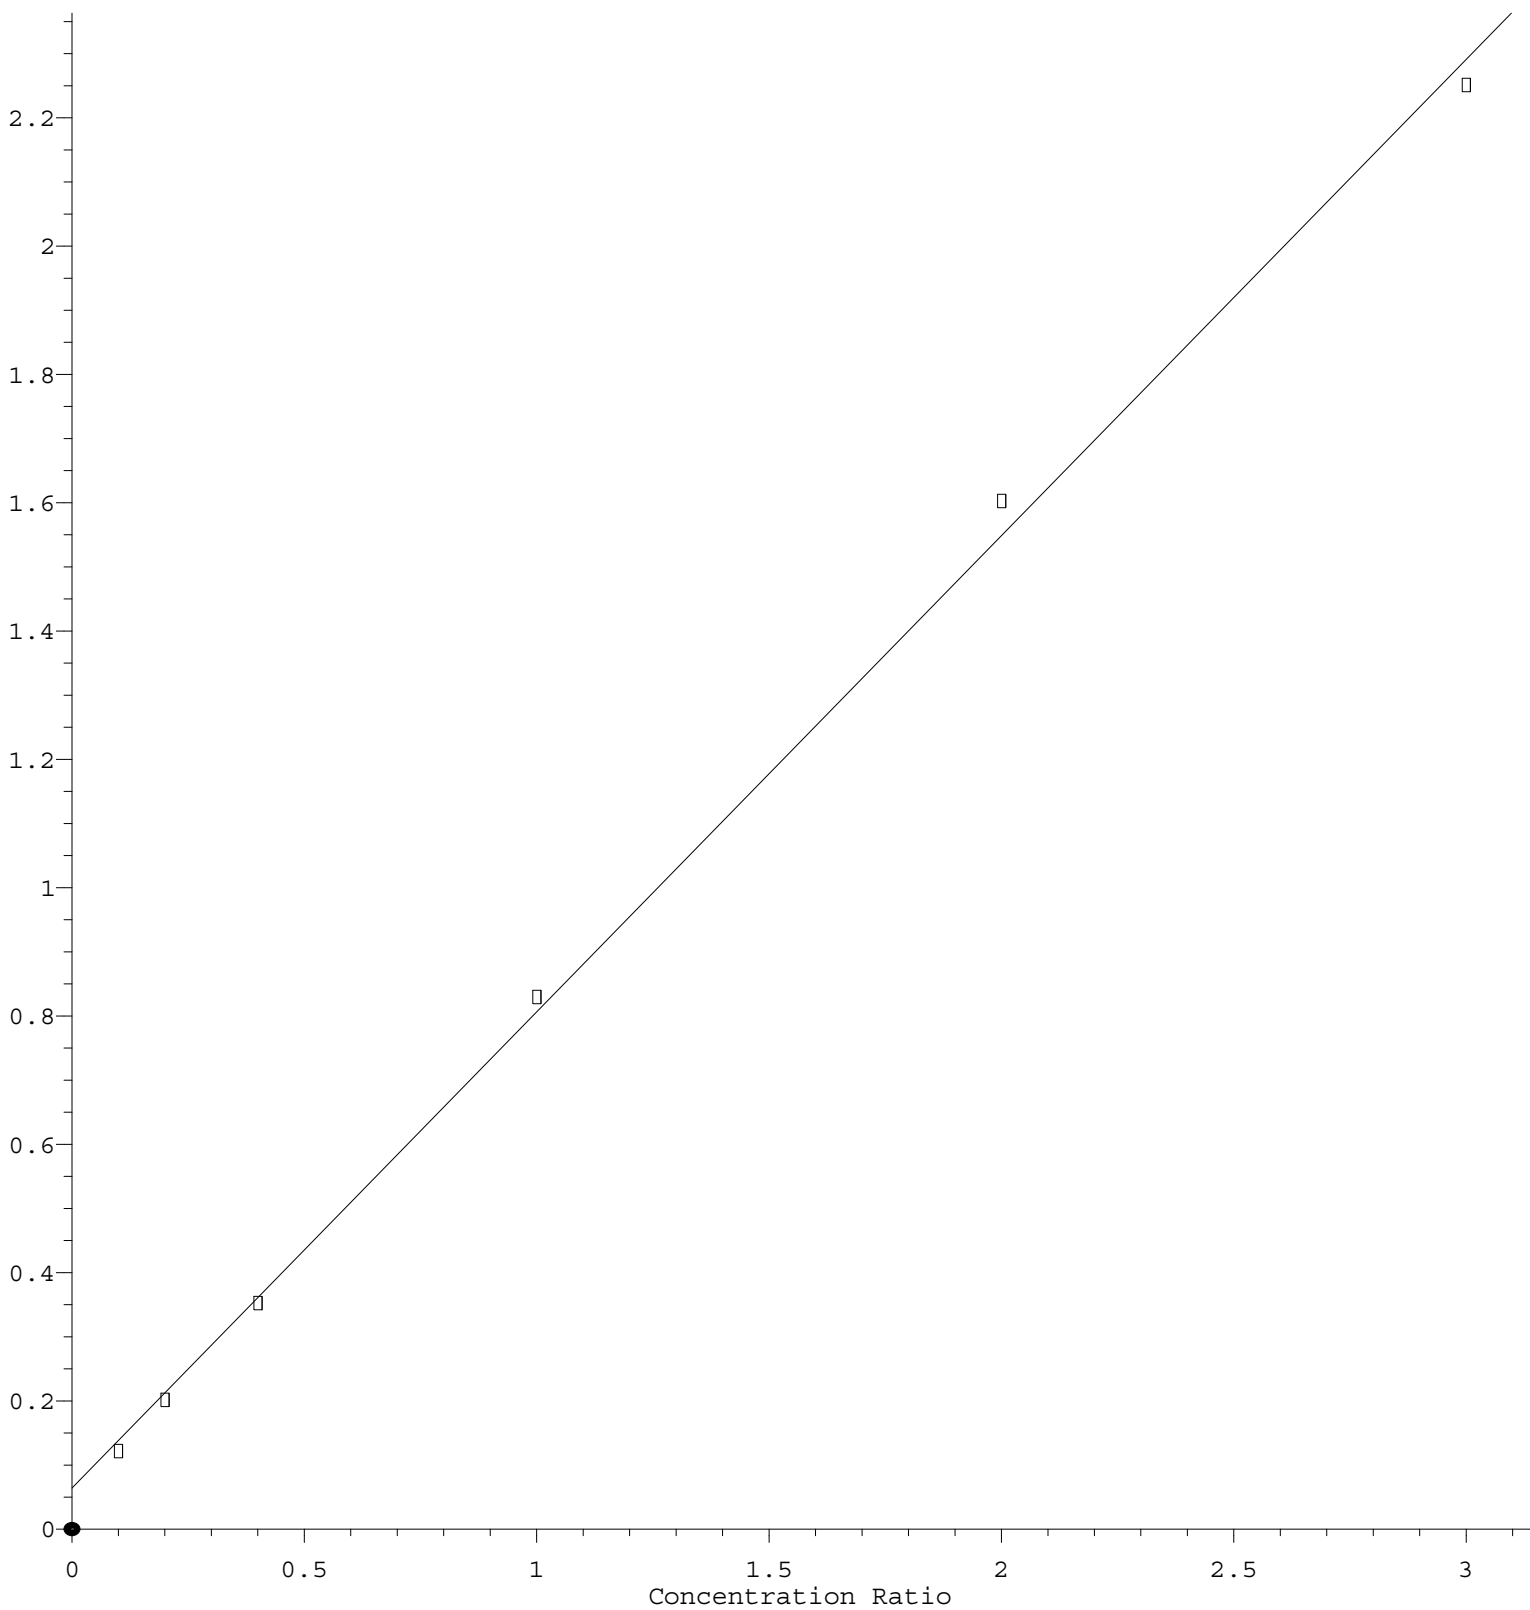

$$\text{Response} = 7.427\text{e-}001 * \text{Amt} + 6.381\text{e-}002$$


Coef of Det (r^2) = 0.998519 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M

Calibration Table Last Updated: Tue Mar 01 09:08:03 2022


Methylene Chloride

Response Ratio

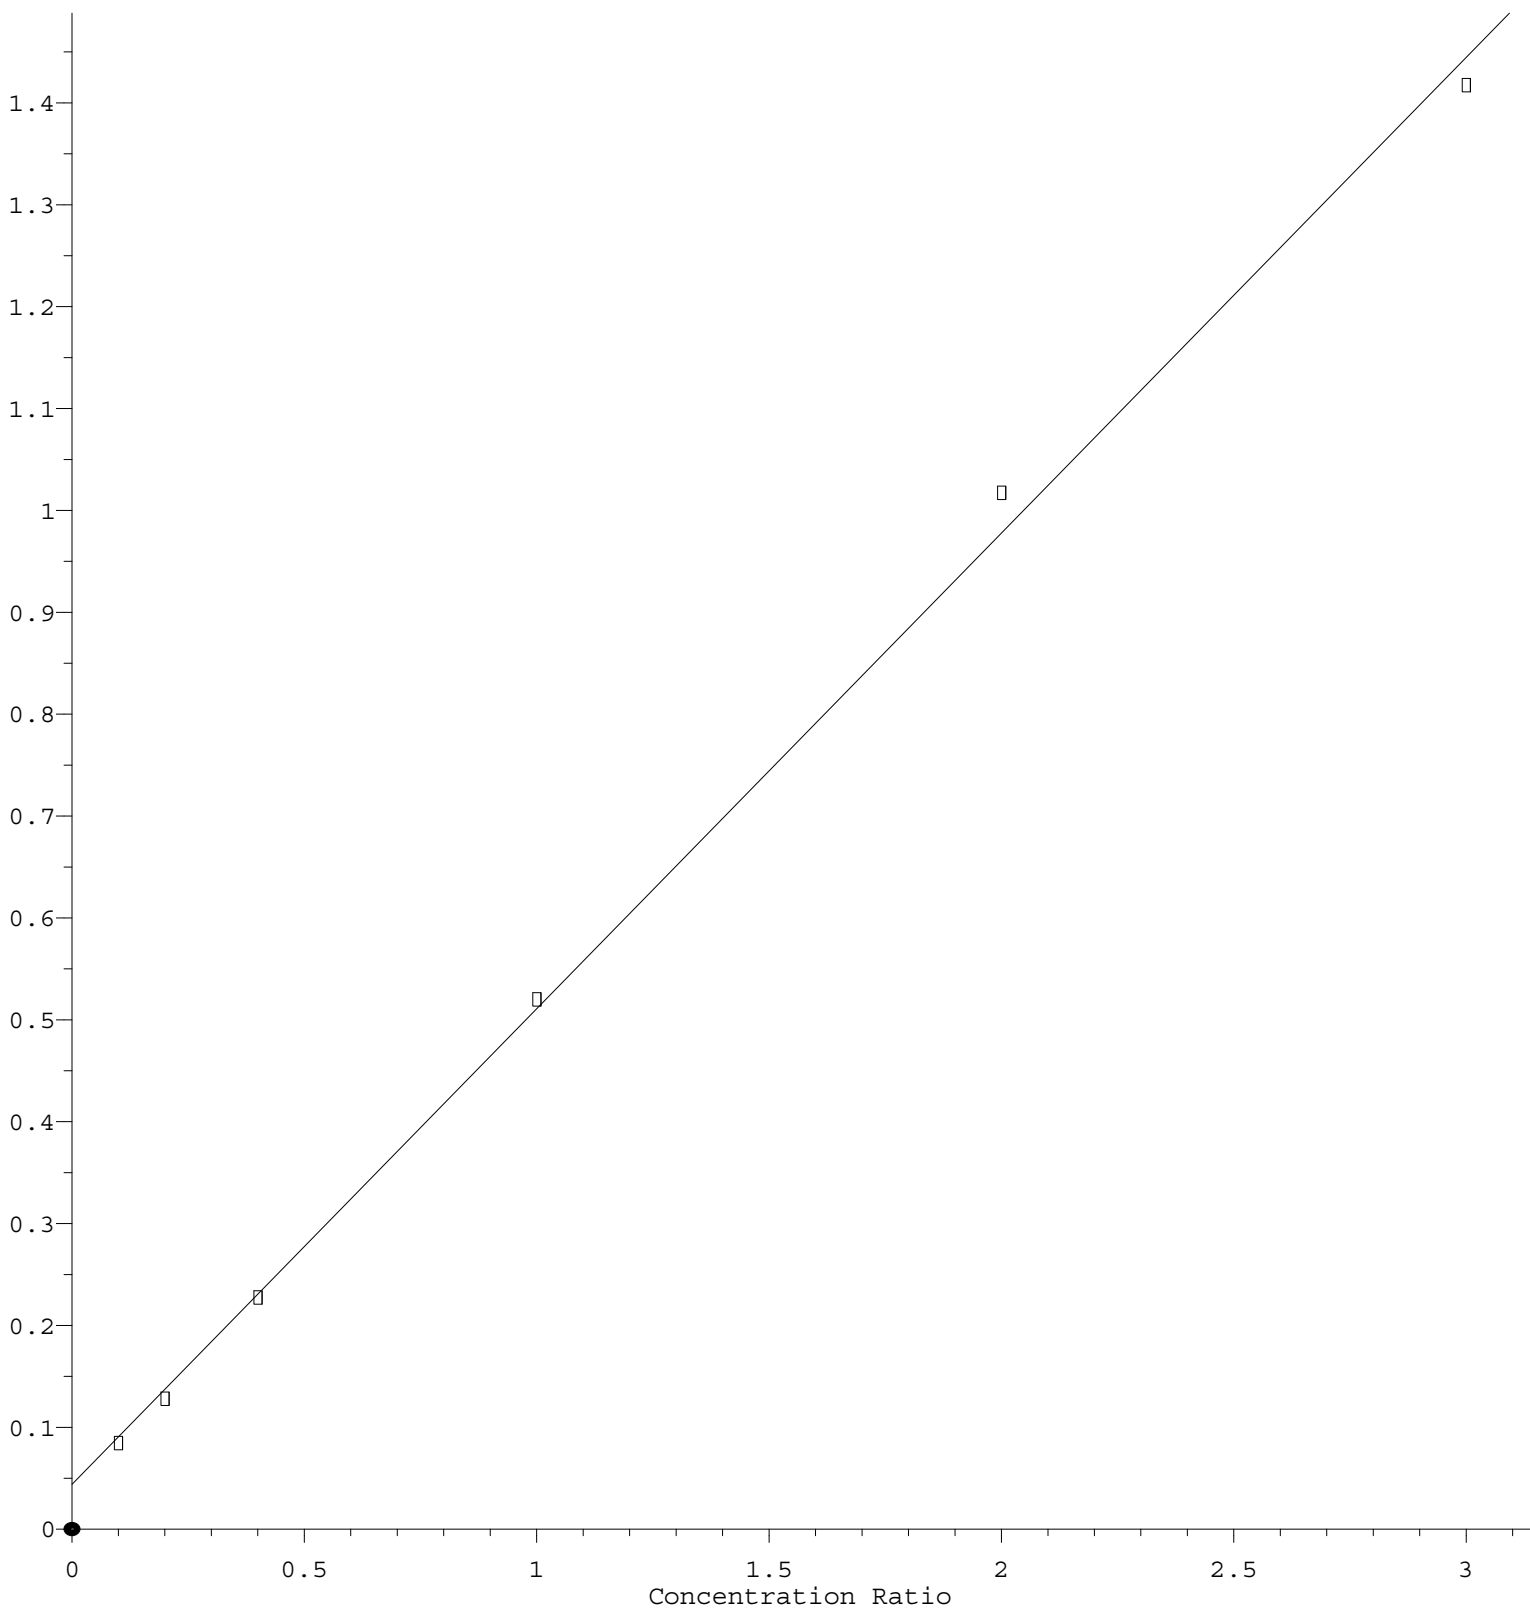

Response = 4.668e-001 * Amt + 4.444e-002
Coef of Det (r^2) = 0.998282 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M
Calibration Table Last Updated: Tue Mar 01 09:08:03 2022


Methyl Acetate

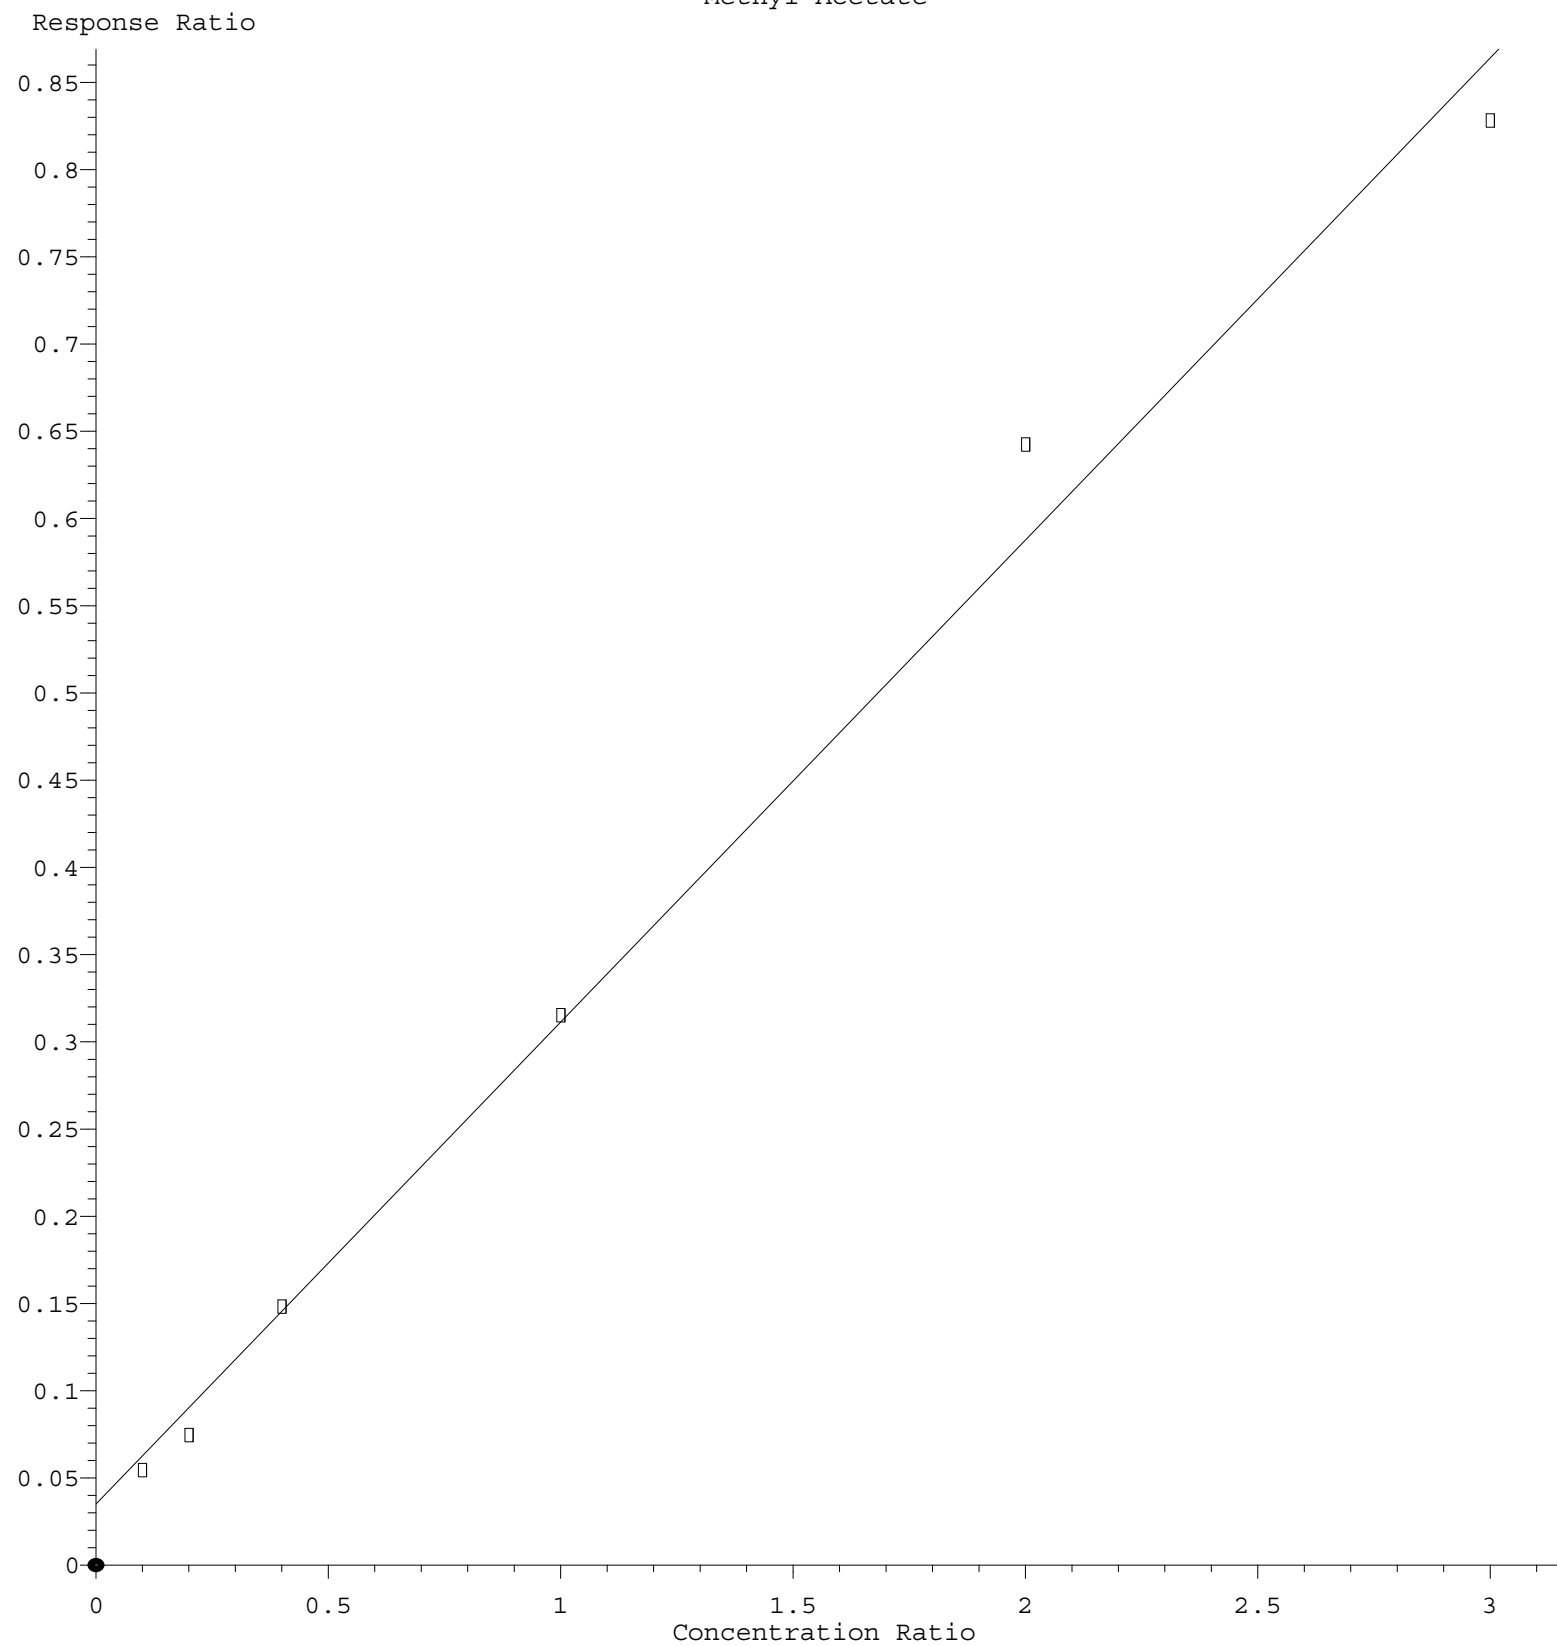

$\text{Response} = 2.765\text{e-}001 * \text{Amt} + 3.509\text{e-}002$
 Coef of Det (r^2) = 0.991093 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M
 Calibration Table Last Updated: Tue Mar 01 09:08:03 2022

Carbon Disulfide

Response Ratio

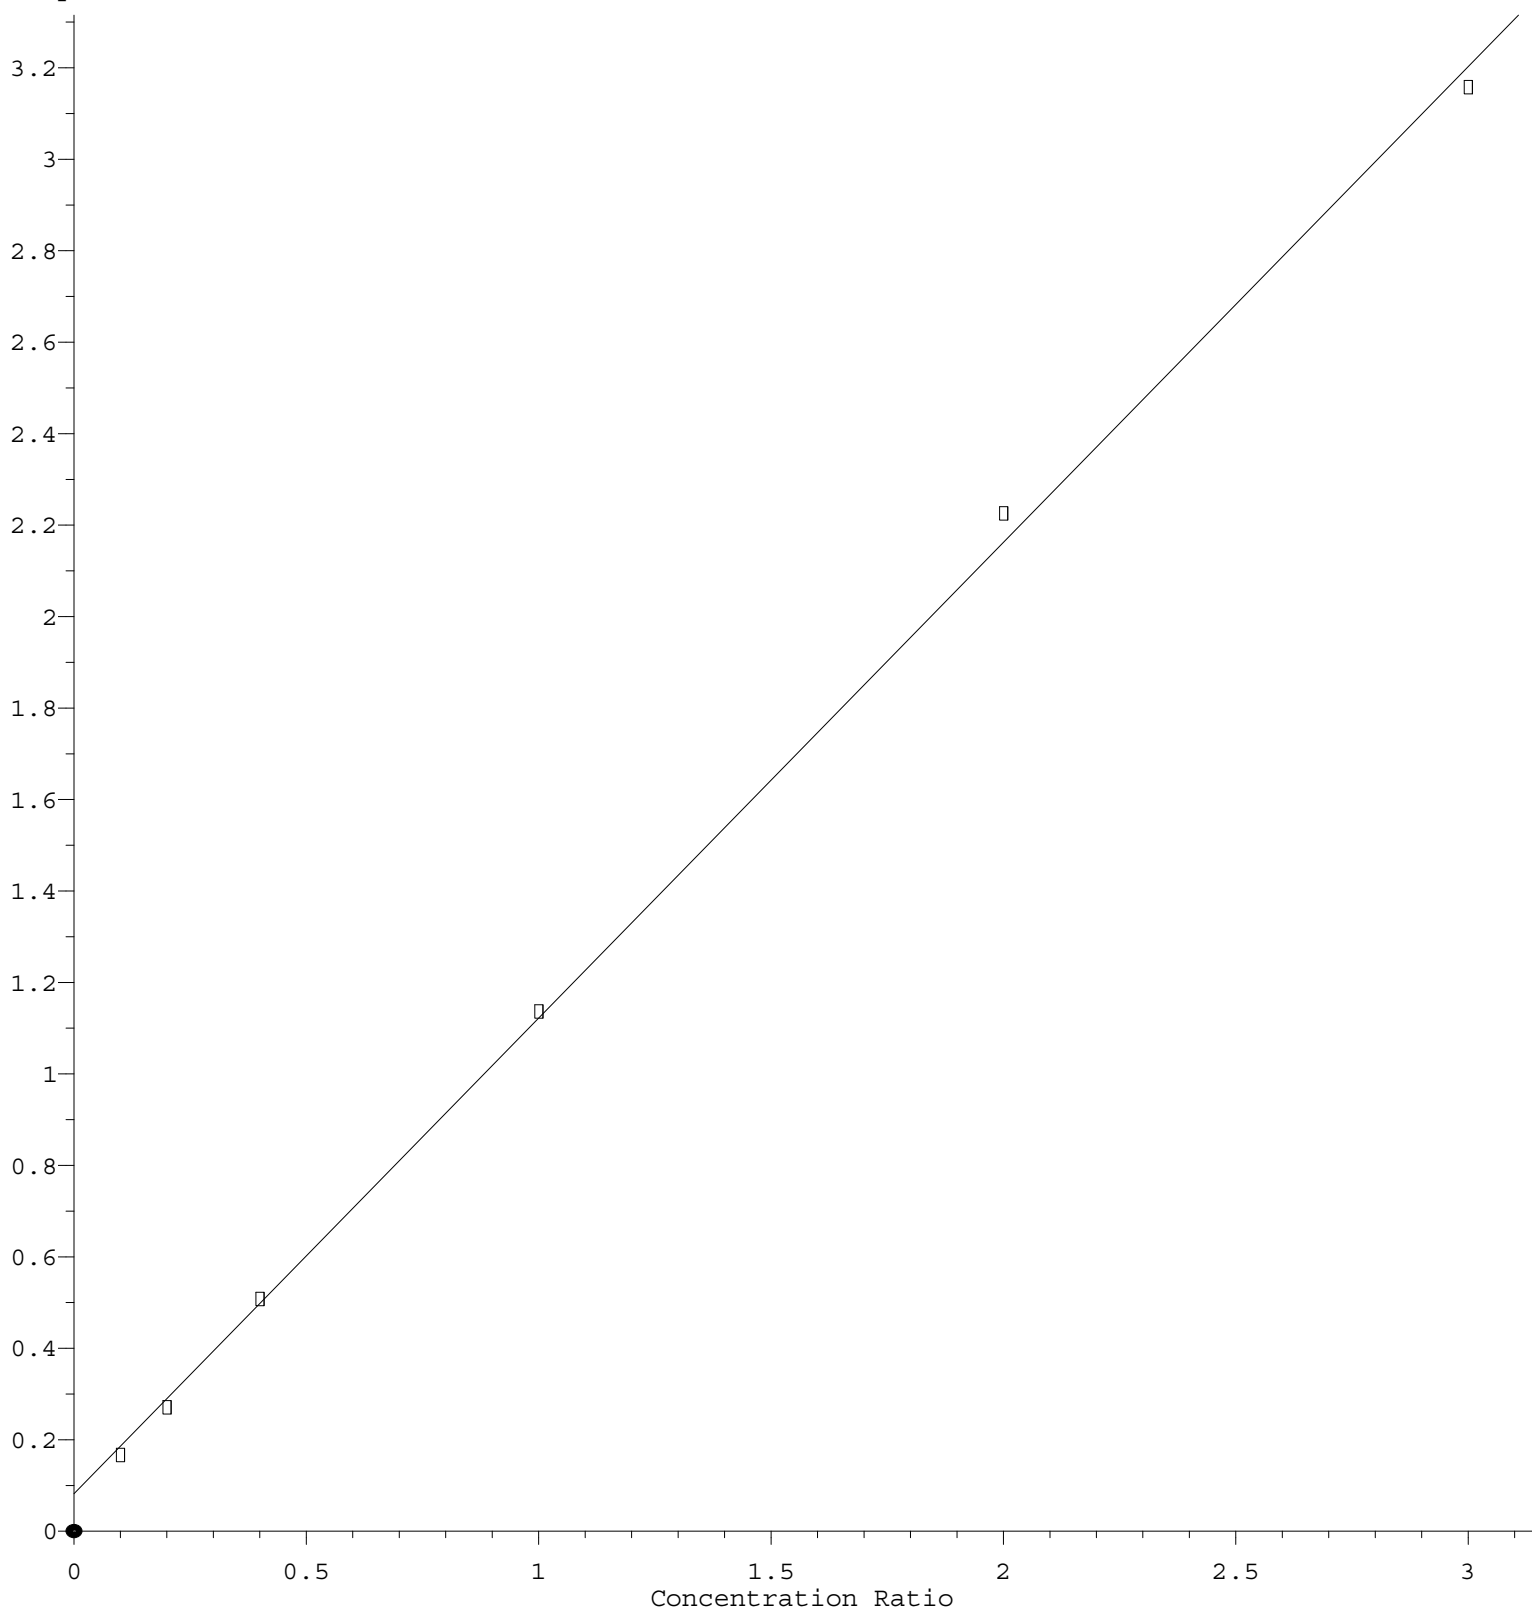


$$\text{Response} = 1.040\text{e}+000 * \text{Amt} + 8.248\text{e}-002$$

Coef of Det (r^2) = 0.999036 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M

Calibration Table Last Updated: Tue Mar 01 09:08:03 2022


Acrolein

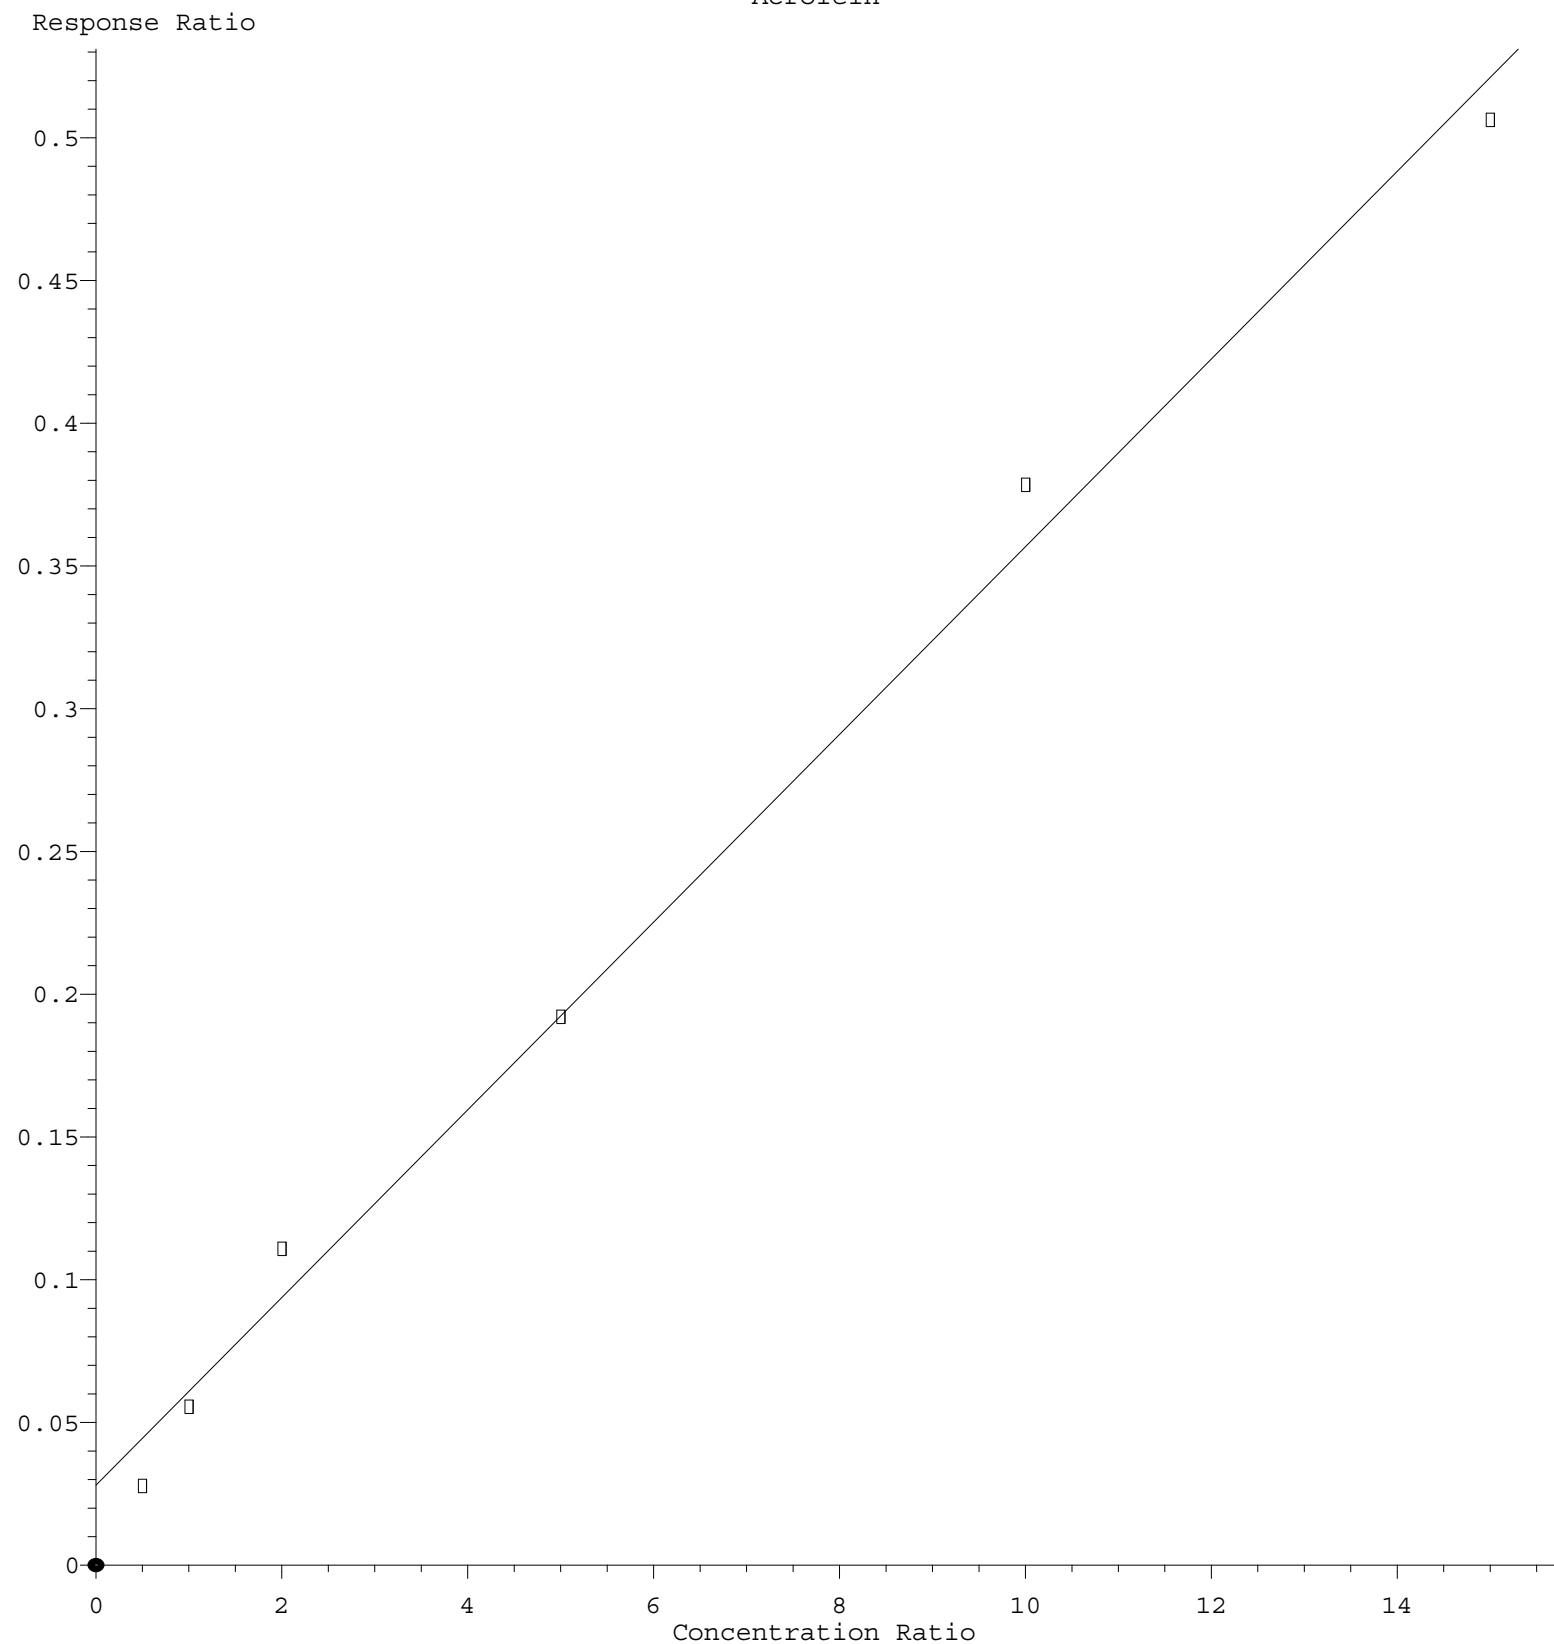

Response = 3.290e-002 * Amt + 2.810e-002
 Coef of Det (r^2) = 0.992964 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M
 Calibration Table Last Updated: Tue Mar 01 09:08:03 2022

Chloromethane

Response Ratio

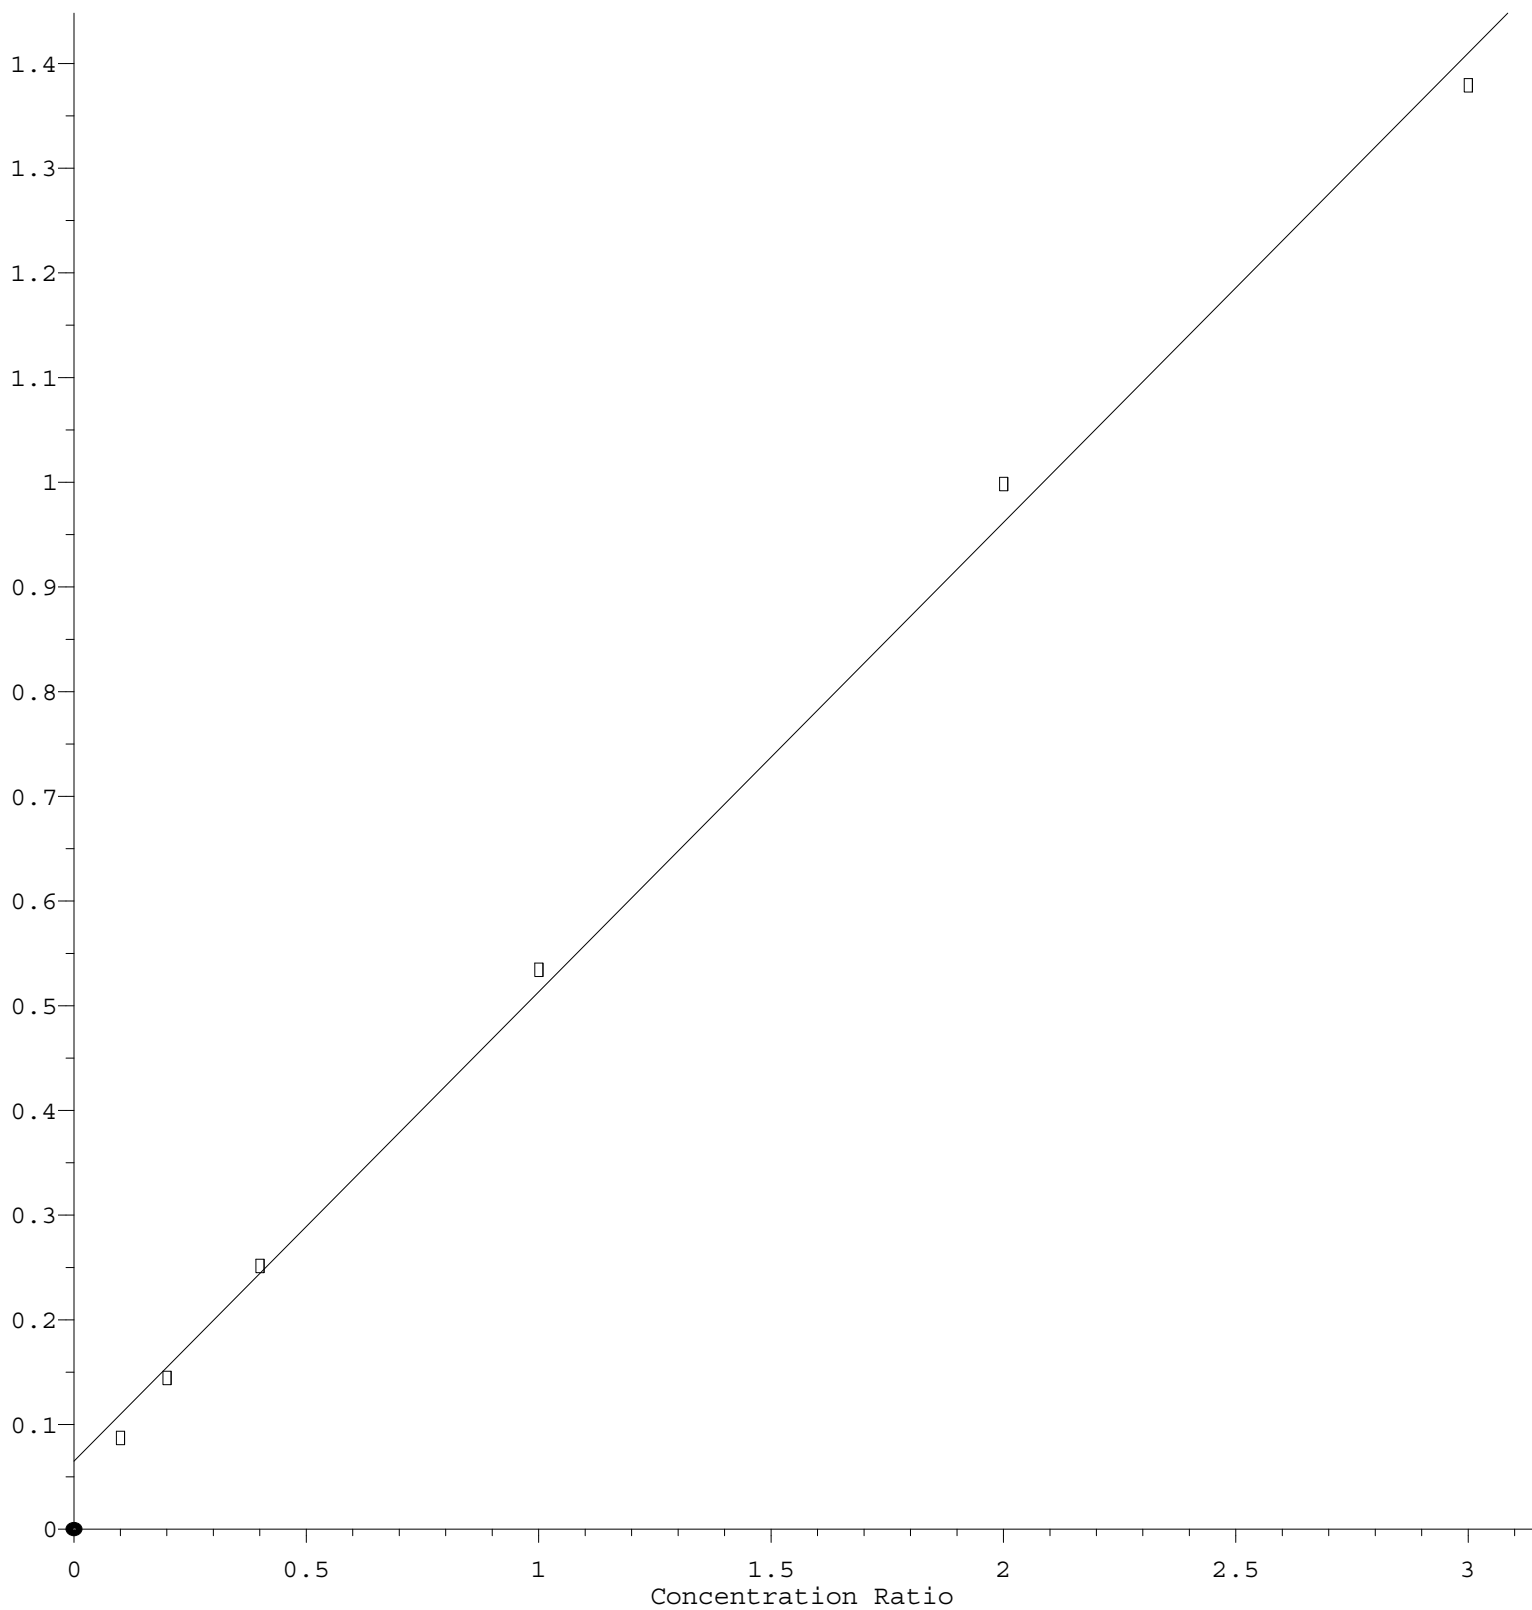

$$\text{Response} = 4.482\text{e-}001 * \text{Amt} + 6.529\text{e-}002$$

Coef of Det (r^2) = 0.997494 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y022822S.M

Calibration Table Last Updated: Tue Mar 01 09:08:03 2022