

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022825\
 Data File : VY021379.D
 Acq On : 28 Feb 2025 12:56
 Operator : SY/MD
 Sample : Q1421-07RE
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P001-CLAY-CF01-02RE

Quant Time: Mar 03 00:25:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 26 02:09:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	106394	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	179401	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	142440	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	40324	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	66950	55.471	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.940%
35) Dibromofluoromethane	7.628	113	63826	54.266	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.540%
50) Toluene-d8	10.103	98	210035	46.207	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	92.420%
62) 4-Bromofluorobenzene	12.407	95	48798	31.899	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	63.800%
Target Compounds						
16) Acetone	3.872	43	3847	16.616	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022825\
Data File : VY021379.D
Acq On : 28 Feb 2025 12:56
Operator : SY/MD
Sample : Q1421-07RE
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P001-CLAY-CF01-02RE

Quant Time: Mar 03 00:25:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 26 02:09:13 2025
Response via : Initial Calibration




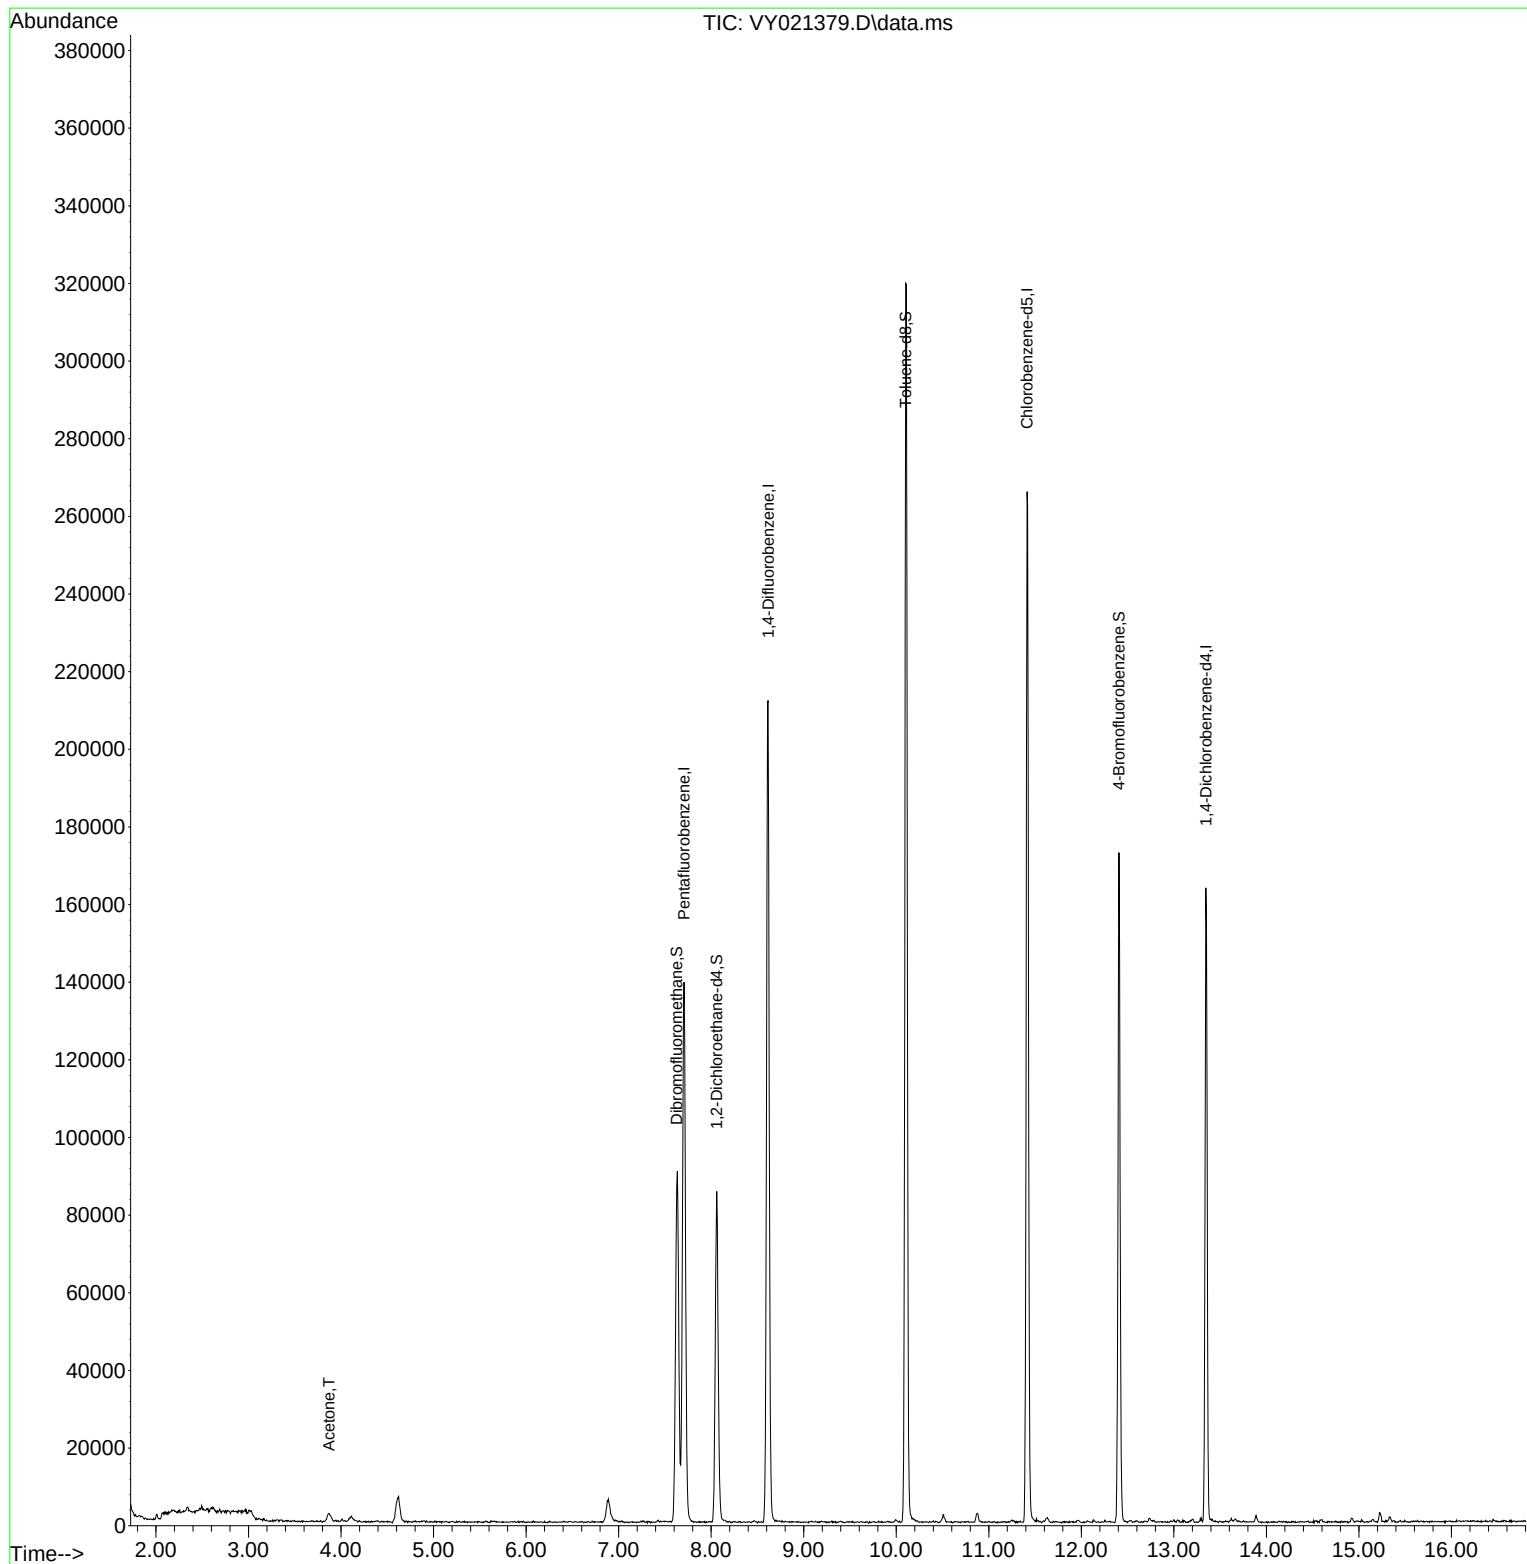


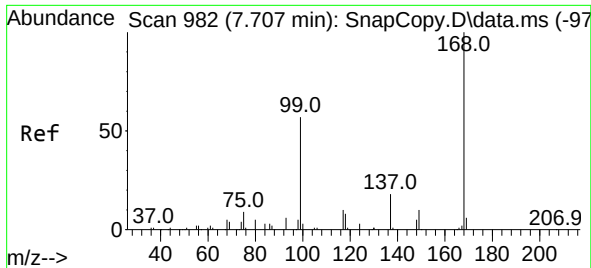

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56




Instrument :
MSVOA_Y
ClientSampleId :
P001-CLAY-CF01-02RE


Tgt Ion:168 Resp: 106394
Ion Ratio Lower Upper
168 100
99 54.8 47.1 70.7

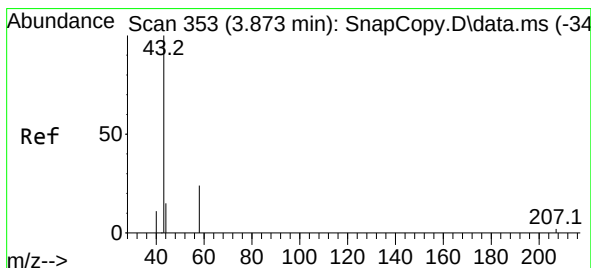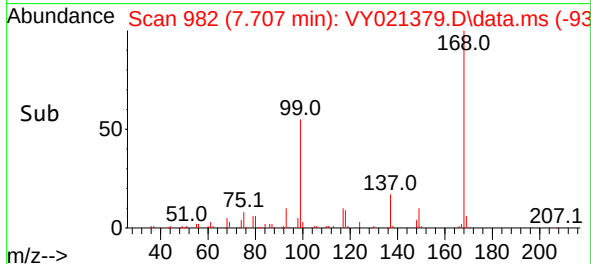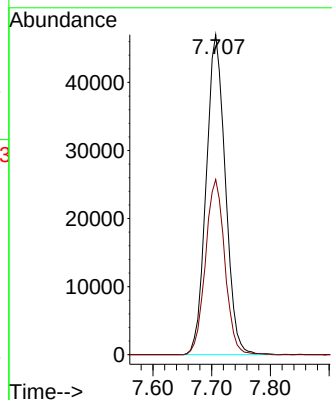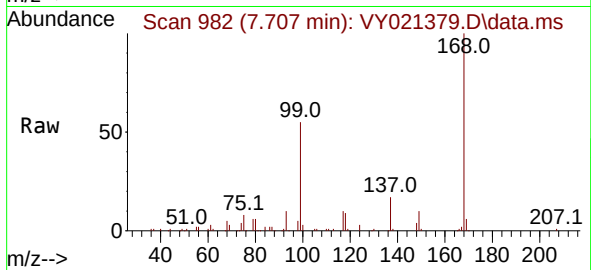

#16
Acetone
Concen: 16.616 ug/l
RT: 3.872 min Scan# 353
Delta R.T. 0.006 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56

Tgt Ion: 43 Resp: 3847
Ion Ratio Lower Upper
43 100
58 28.6 23.5 35.3

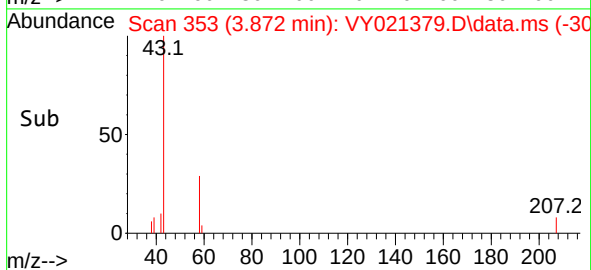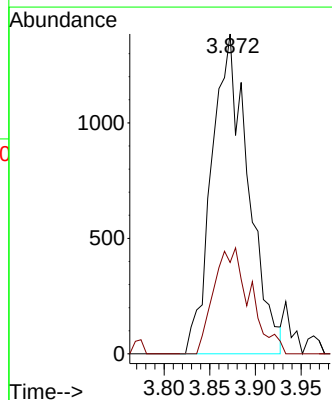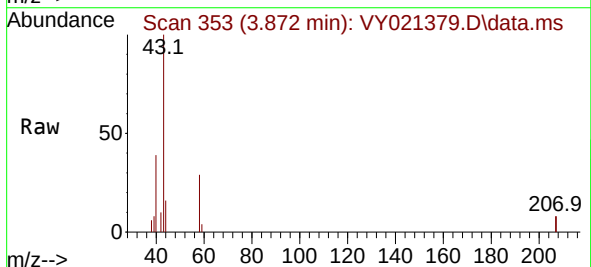

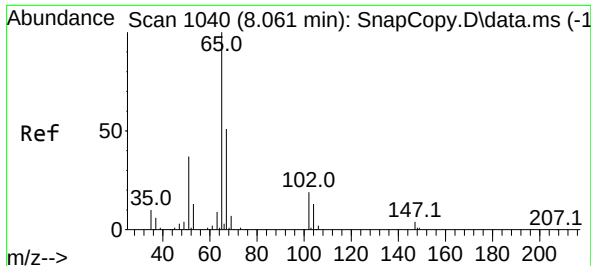

#33

1,2-Dichloroethane-d4

Concen: 55.471 ug/l

RT: 8.060 min Scan# 110

Delta R.T. -0.000 min

Lab File: VY021379.D

Acq: 28 Feb 2025 12:56

Instrument :

MSVOA_Y

ClientSampleId :





P001-CLAY-CF01-02RE

Tgt Ion: 65 Resp: 66950

Ion Ratio Lower Upper

65 100

67 51.0 0.0 103.6

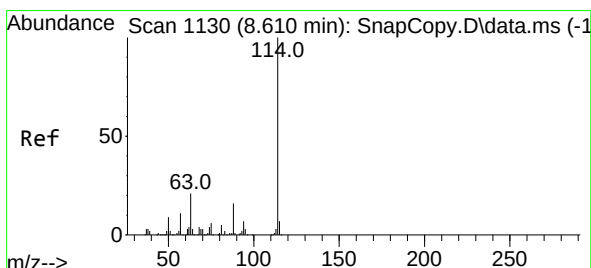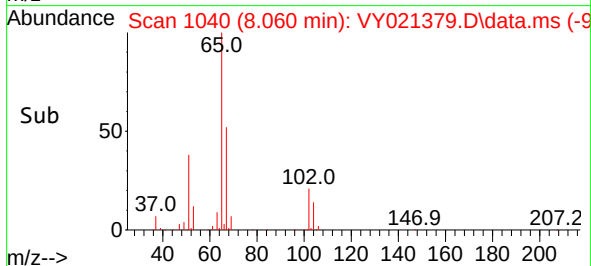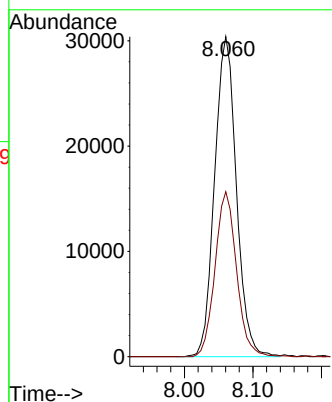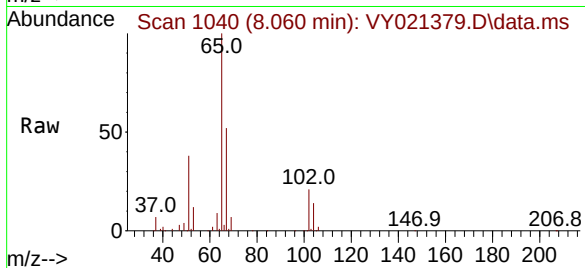

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY021379.D

Acq: 28 Feb 2025 12:56




Tgt Ion:114 Resp: 179401


Ion Ratio Lower Upper

114 100

63 19.8 0.0 42.2

88 14.3 0.0 29.8


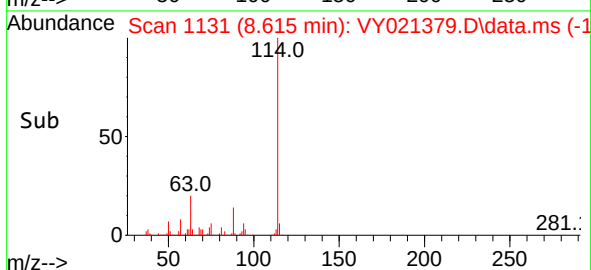
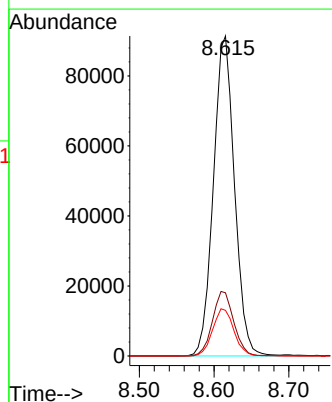
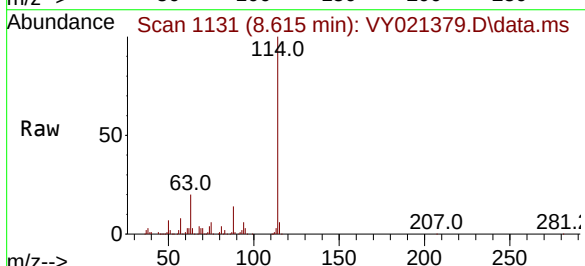


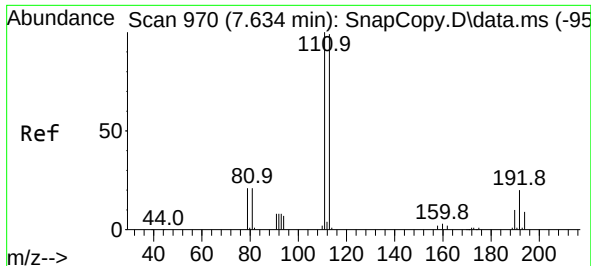

#35
Dibromofluoromethane
Concen: 54.266 ug/l
RT: 7.628 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56




Instrument :
MSVOA_Y
ClientSampleId :
P001-CLAY-CF01-02RE


Tgt Ion:113 Resp: 63826
Ion Ratio Lower Upper
113 100
111 102.6 81.0 121.6
192 20.7 15.8 23.8

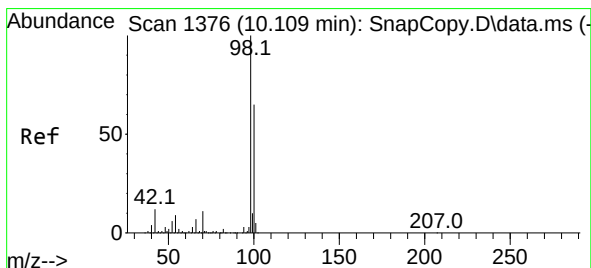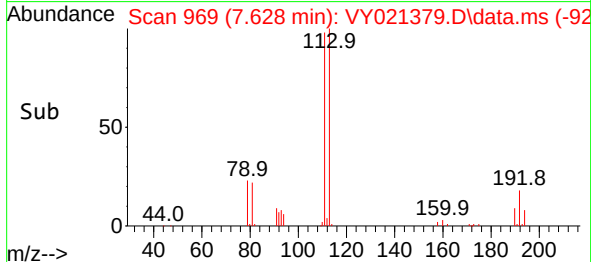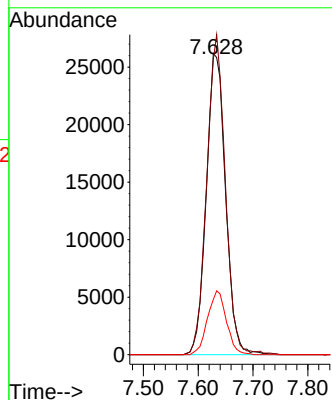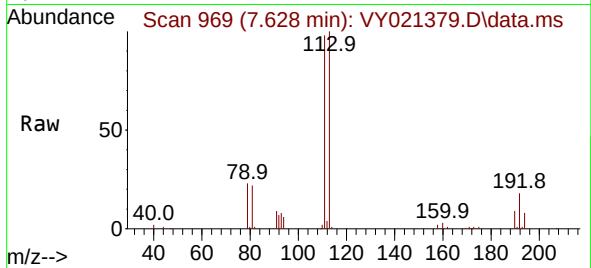

#50
Toluene-d8
Concen: 46.207 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. -0.000 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56

Tgt Ion: 98 Resp: 210035
Ion Ratio Lower Upper
98 100
100 64.2 52.4 78.6


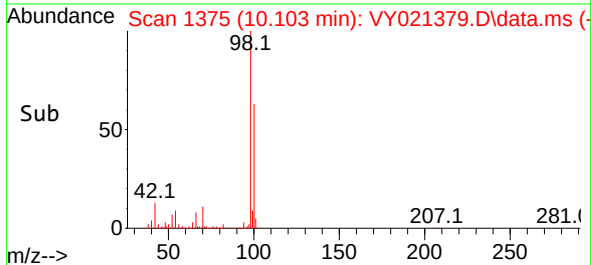
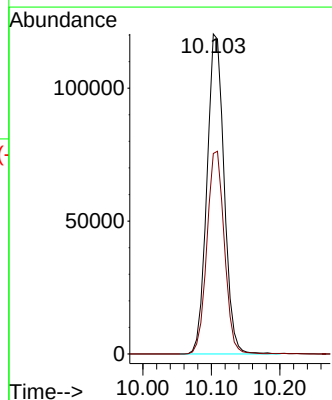
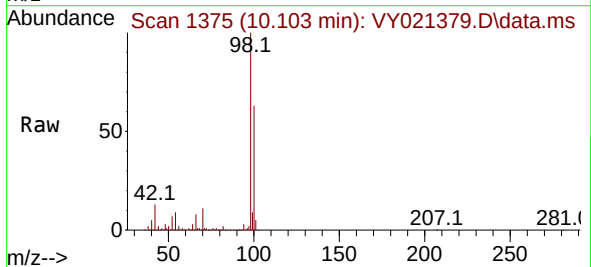


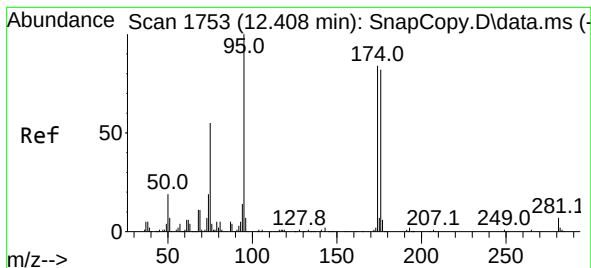

#62
4-Bromofluorobenzene
Concen: 31.899 ug/l
RT: 12.407 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56




Instrument :
MSVOA_Y
ClientSampleId :
P001-CLAY-CF01-02RE


Tgt Ion:	95	Resp:	48798
Ion Ratio	Lower	Upper	
95	100		
174	89.7	0.0	168.0
176	86.1	0.0	162.6

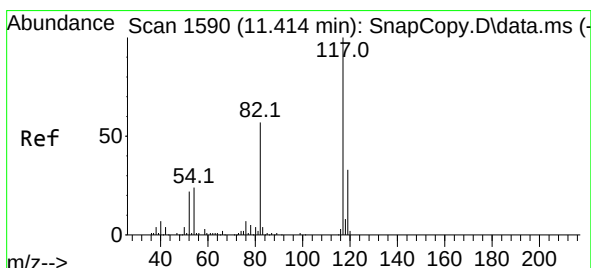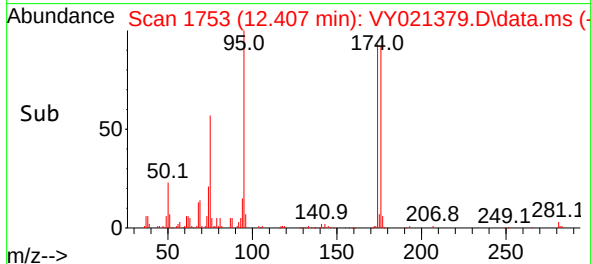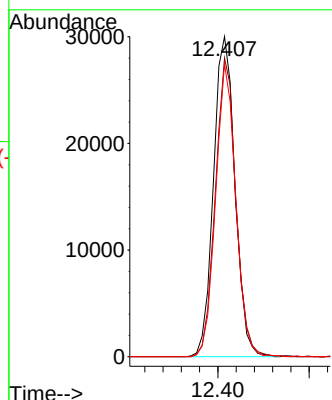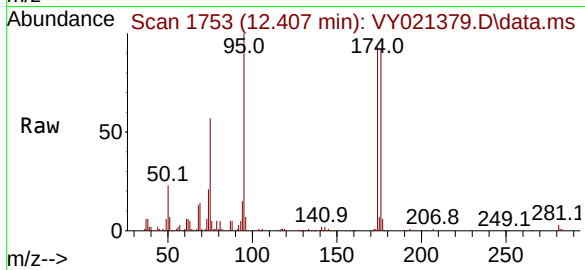

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.000 min
Lab File: VY021379.D
Acq: 28 Feb 2025 12:56


Tgt Ion:	117	Resp:	142440
Ion Ratio	Lower	Upper	
117	100		
82	55.8	46.2	69.4
119	30.5	24.9	37.3

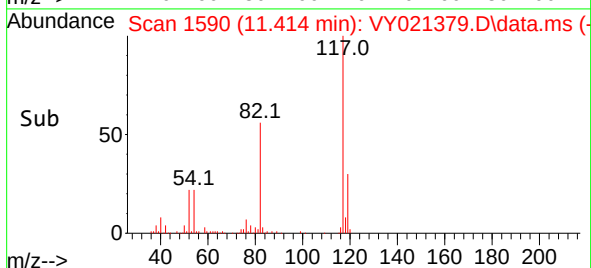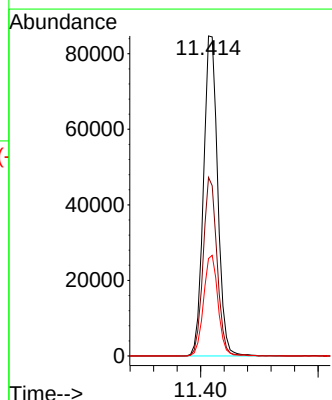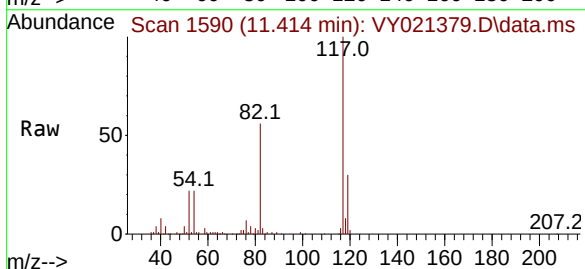

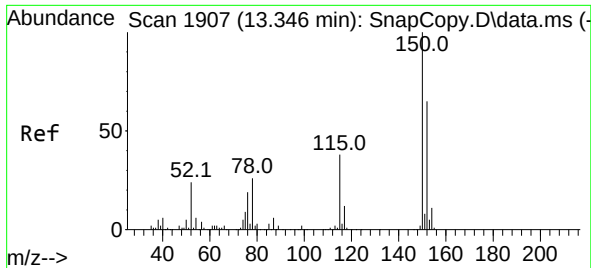

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY021379.D
 Acq: 28 Feb 2025 12:56

Instrument :
 MSVOA_Y
 ClientSampleId :
 P001-CLAY-CF01-02RE

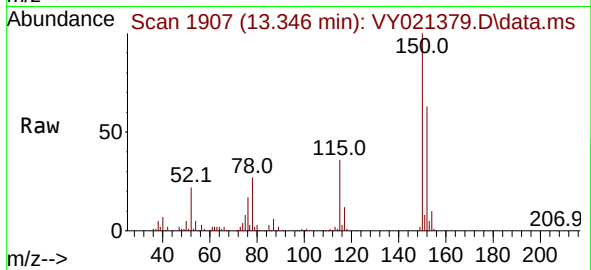

Tgt Ion:	152	Resp:	40324
Ion Ratio	Lower	Upper	
152	100		
115	58.3	29.3	88.0
150	158.3	0.0	347.4

