

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022825\
 Data File : VY021389.D
 Acq On : 28 Feb 2025 18:38
 Operator : SY/MD
 Sample : Q1463-01
 Misc : 6.60g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 T1

Quant Time: Feb 28 22:23:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 26 02:09:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	116223	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	210275	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	179550	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	66737	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	76620	58.114	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	116.220%
35) Dibromofluoromethane	7.634	113	75185	54.538	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.080%
50) Toluene-d8	10.109	98	195728	36.737	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	73.480%
62) 4-Bromofluorobenzene	12.407	95	72623	40.502	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022825\
Data File : VY021389.D
Acq On : 28 Feb 2025 18:38
Operator : SY/MD
Sample : Q1463-01
Misc : 6.60g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
T1

Quant Time: Feb 28 22:23:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 26 02:09:13 2025
Response via : Initial Calibration




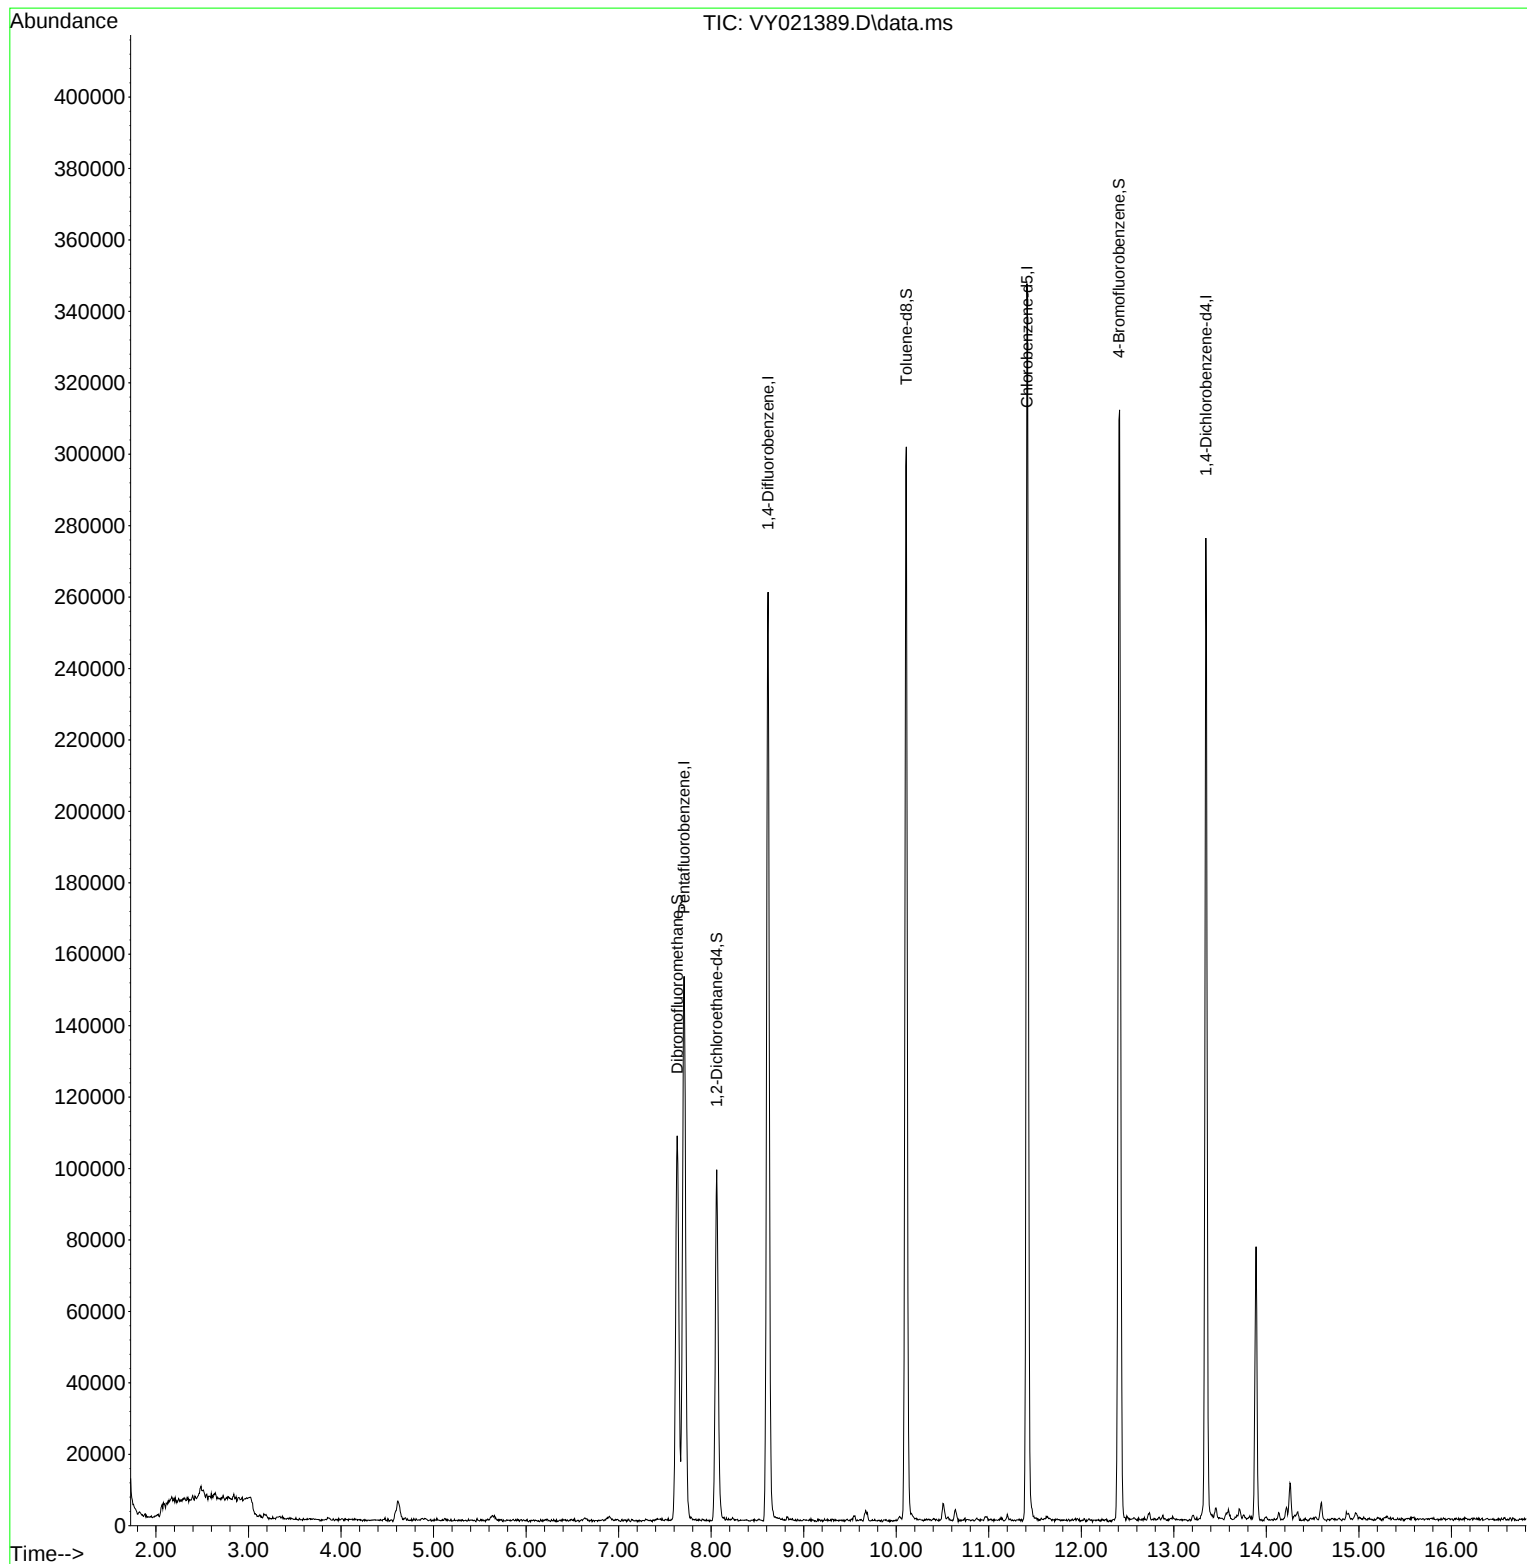


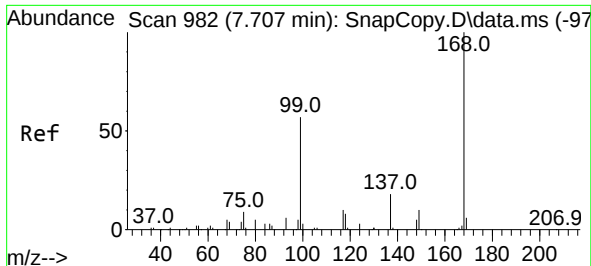

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38




Instrument :
MSVOA_Y
ClientSampleId :
T1


Tgt Ion:168 Resp: 116223
Ion Ratio Lower Upper
168 100
99 56.7 47.1 70.7

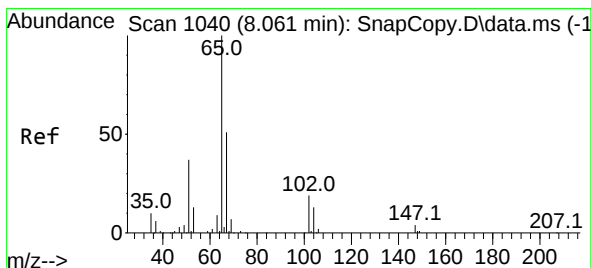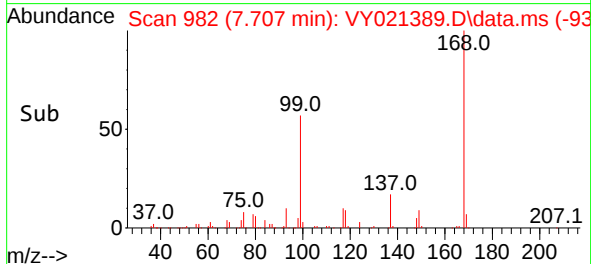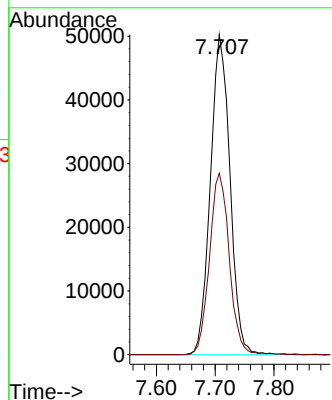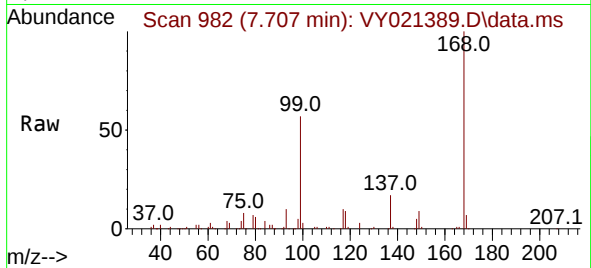

#33
1,2-Dichloroethane-d4
Concen: 58.114 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38

Tgt Ion: 65 Resp: 76620
Ion Ratio Lower Upper
65 100
67 50.8 0.0 103.6


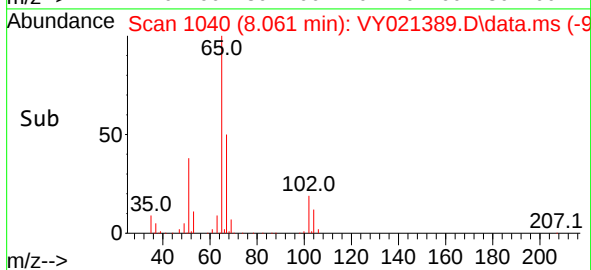
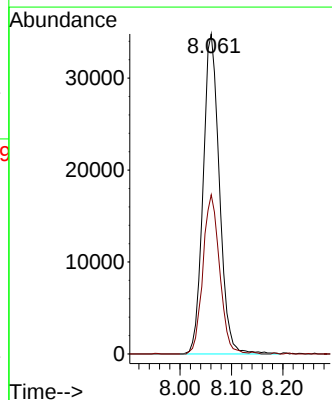
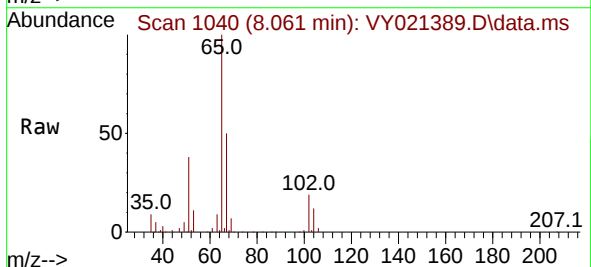


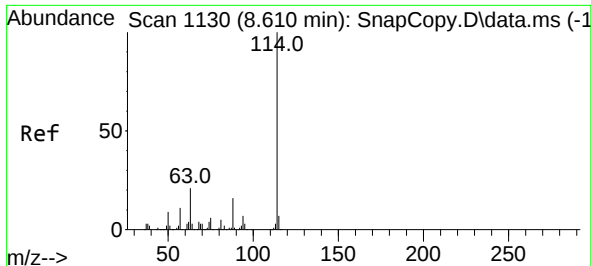

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38




Instrument :
MSVOA_Y
ClientSampleId :
T1


Tgt Ion:114 Resp: 210275
Ion Ratio Lower Upper
114 100
63 21.2 0.0 42.2
88 15.0 0.0 29.8

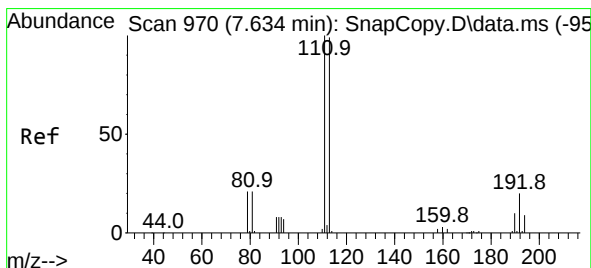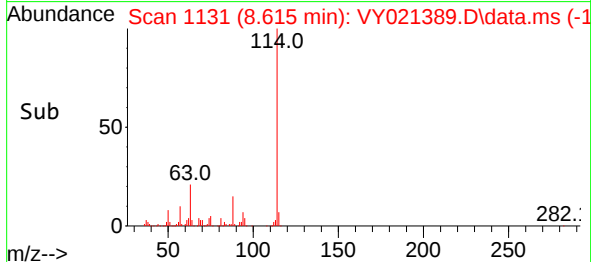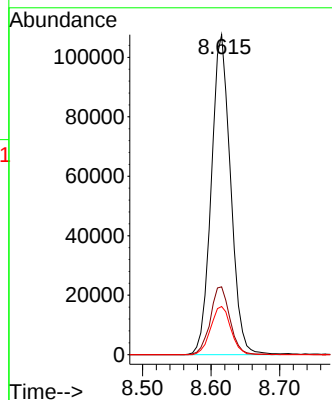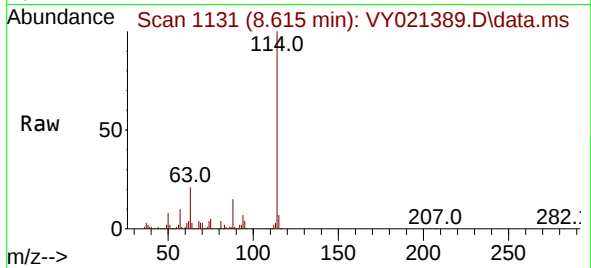

#35
Dibromofluoromethane
Concen: 54.538 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38

Tgt Ion:113 Resp: 75185
Ion Ratio Lower Upper
113 100
111 105.1 81.0 121.6
192 19.2 15.8 23.8


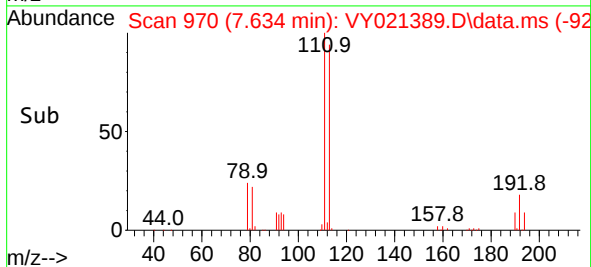
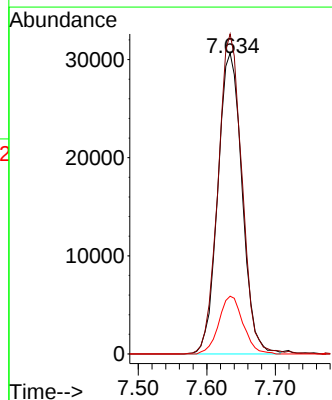
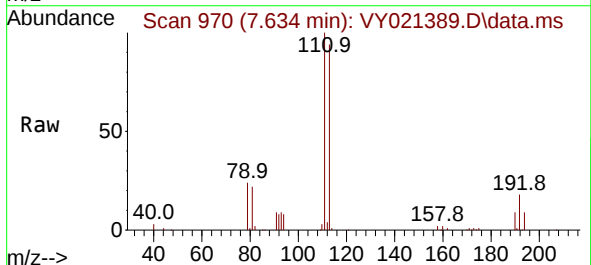


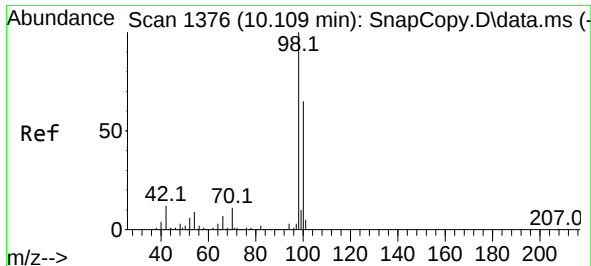

#50
Toluene-d8
Concen: 36.737 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38




Instrument :
MSVOA_Y
ClientSampleId :
T1


Tgt Ion: 98 Resp: 195728
Ion Ratio Lower Upper
98 100
100 63.9 52.4 78.6

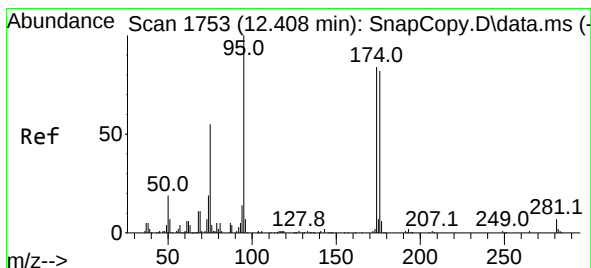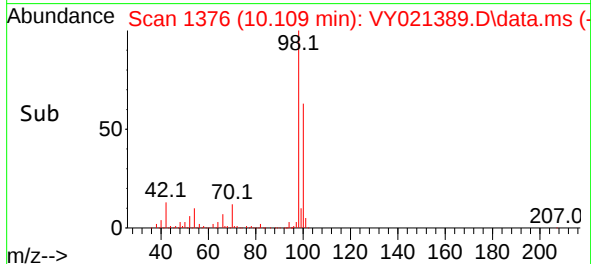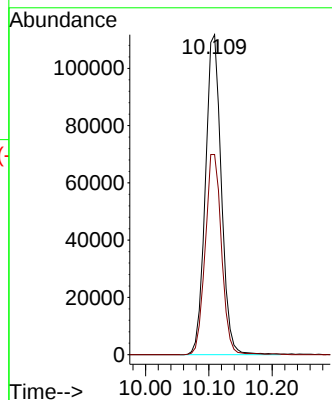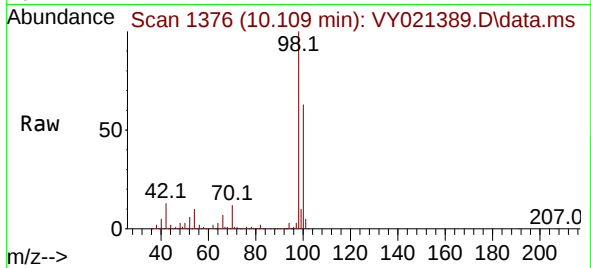

#62
4-Bromofluorobenzene
Concen: 40.502 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY021389.D
Acq: 28 Feb 2025 18:38

Tgt Ion: 95 Resp: 72623
Ion Ratio Lower Upper
95 100
174 82.0 0.0 168.0
176 80.1 0.0 162.6

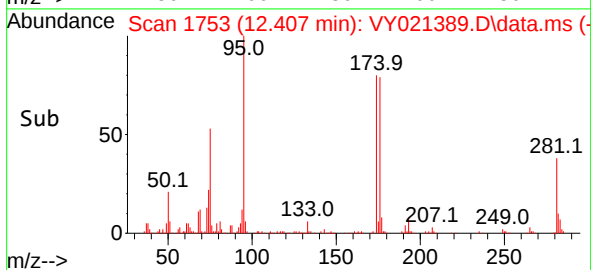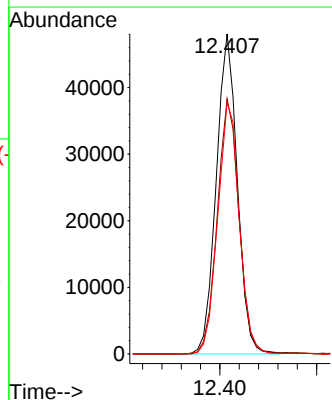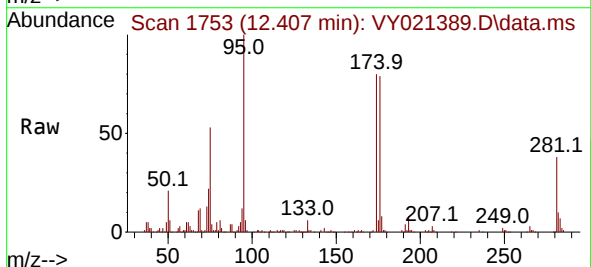

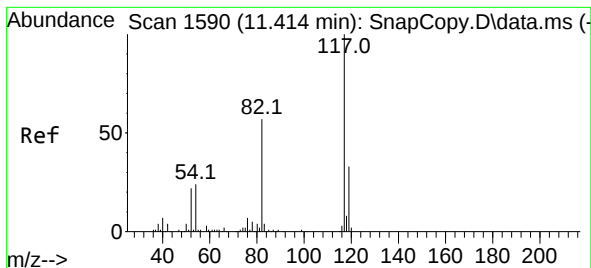

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY021389.D

Acq: 28 Feb 2025 18:38

Instrument :

MSVOA_Y

ClientSampleId :

T1





Tgt Ion:117 Resp: 179550

Ion Ratio Lower Upper

117 100

82 58.1 46.2 69.4

119 32.0 24.9 37.3

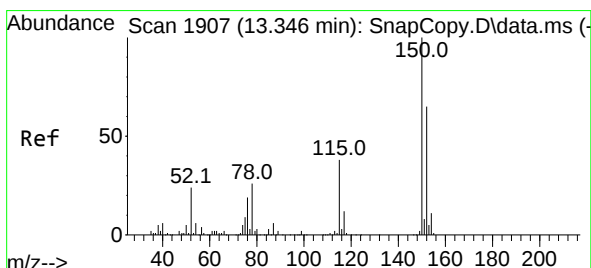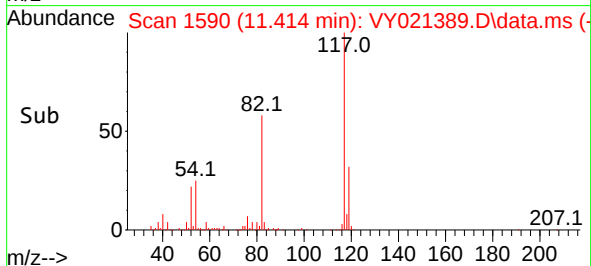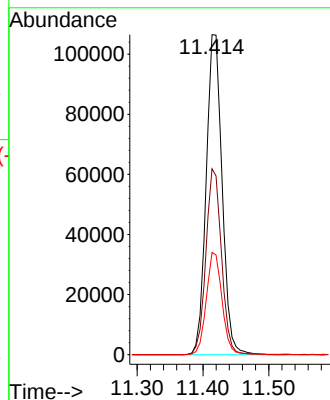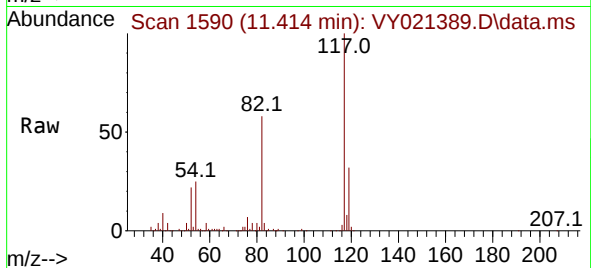

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY021389.D

Acq: 28 Feb 2025 18:38

Tgt Ion:152 Resp: 66737

Ion Ratio Lower Upper

152 100

115 59.8 29.3 88.0

150 158.4 0.0 347.4

