
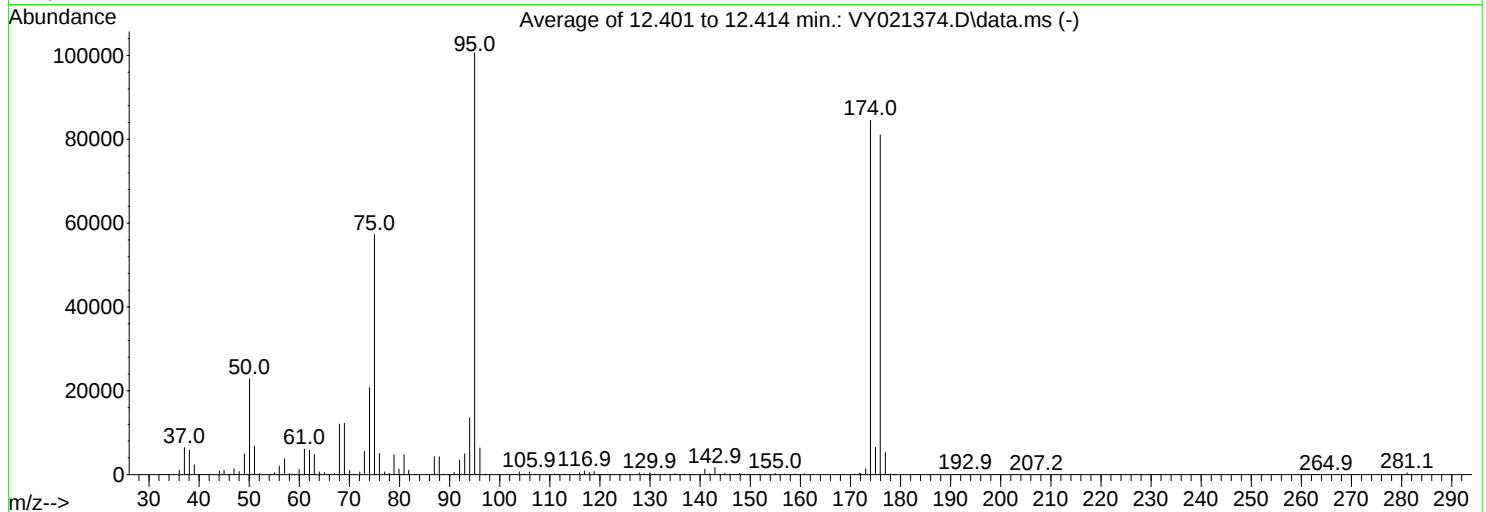


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY022825\
Data File : VY021374.D
Acq On : 28 Feb 2025 09:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022525S.M
Title : SW846 8260
Last Update : Wed Feb 26 02:09:13 2025

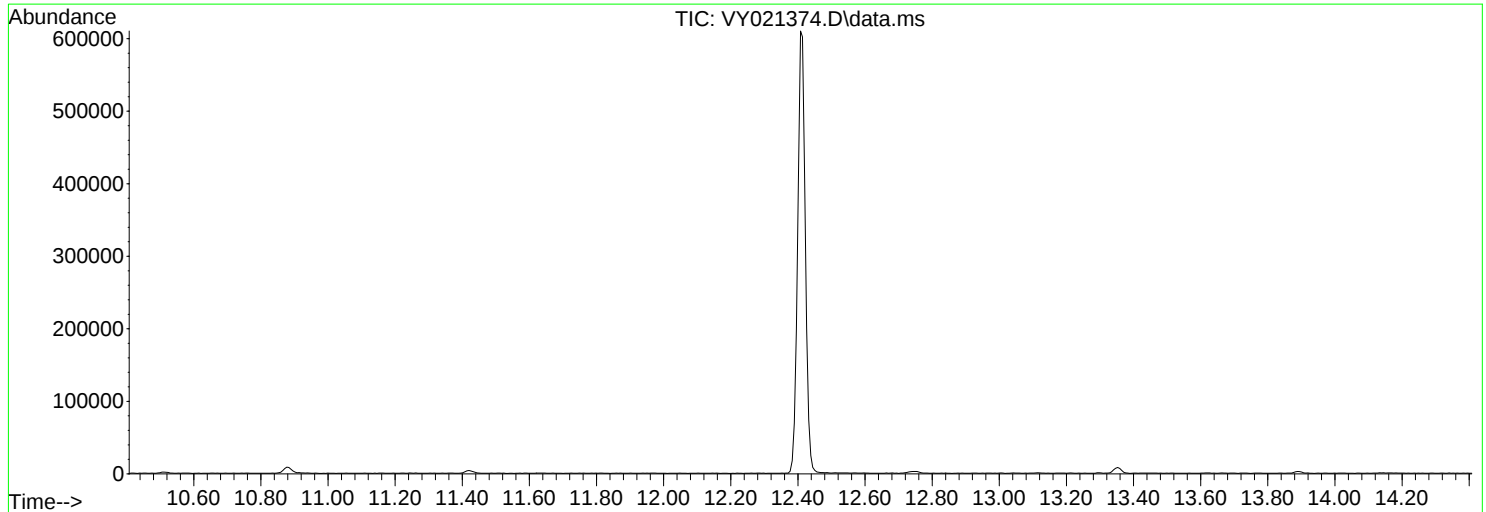

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	22835	PASS
75	95	30	60	56.9	57275	PASS
95	95	100	100	100.0	100624	PASS
96	95	5	9	6.3	6358	PASS
173	174	0.00	2	1.6	1366	PASS
174	95	50	100	84.0	84512	PASS
175	174	5	9	7.7	6516	PASS
176	174	95	101	95.9	81021	PASS
177	176	5	9	6.5	5274	PASS