
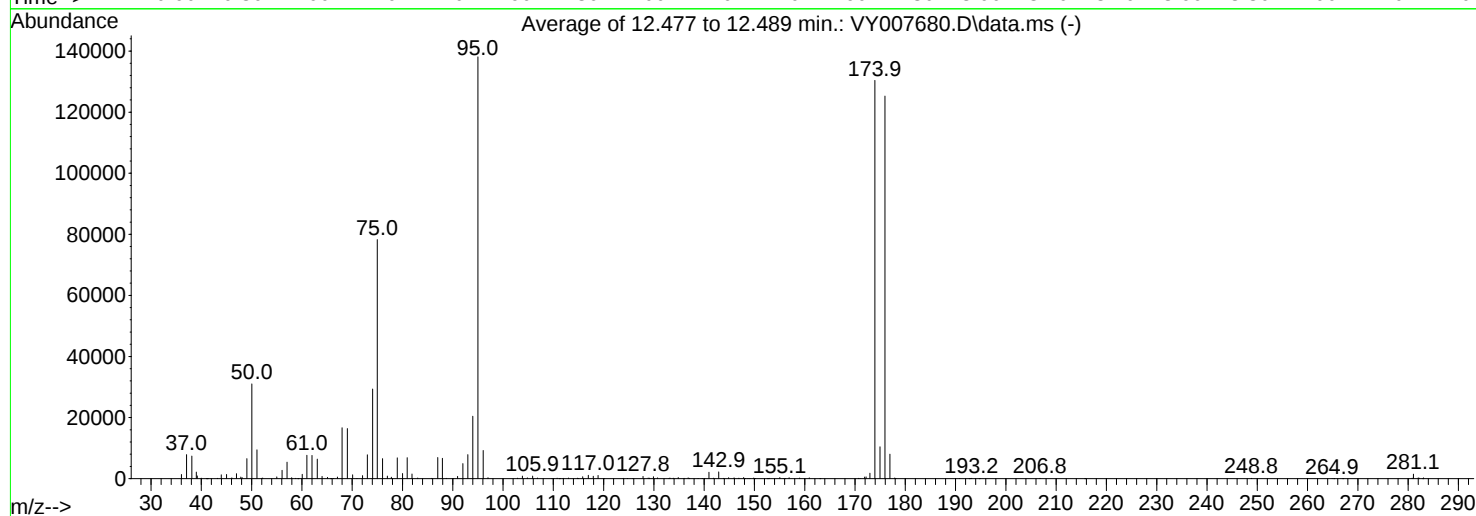


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030222\
 Data File : VY007680.D
 Acq On : 02 Mar 2022 08:51
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
 Title : SW846 8260
 Last Update : Tue Mar 01 09:08:03 2022

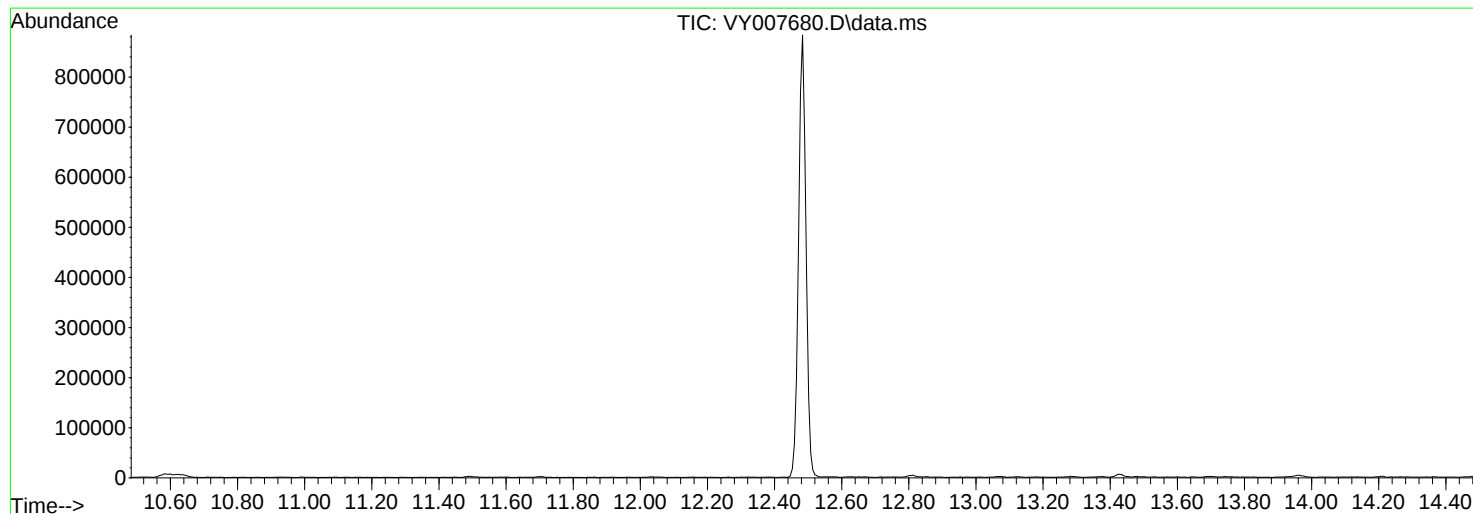

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	31005	PASS
75	95	30	60	56.7	78299	PASS
95	95	100	100	100.0	138115	PASS
96	95	5	9	6.7	9253	PASS
173	174	0.00	2	1.4	1784	PASS
174	95	50	100	94.4	130376	PASS
175	174	5	9	8.0	10433	PASS
176	174	95	101	96.1	125275	PASS
177	176	5	9	6.4	7996	PASS