

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030322\
 Data File : VY007709.D
 Acq On : 03 Mar 2022 17:05
 Operator : SY/MD
 Sample : N1759-07
 Misc : 6.76g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 LINE-2-3

Quant Time: Mar 04 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 01 09:08:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	239274	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	437994	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	440332	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	199326	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	159324	63.603	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.200%
35) Dibromofluoromethane	7.716	113	150140	53.617	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.240%
50) Toluene-d8	10.179	98	553893	53.735	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.480%
62) 4-Bromofluorobenzene	12.483	95	190205	57.245	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	114.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030322\
Data File : VY007709.D
Acq On : 03 Mar 2022 17:05
Operator : SY/MD
Sample : N1759-07
Misc : 6.76g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
LINE-2-3

Quant Time: Mar 04 00:42:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 01 09:08:03 2022
Response via : Initial Calibration




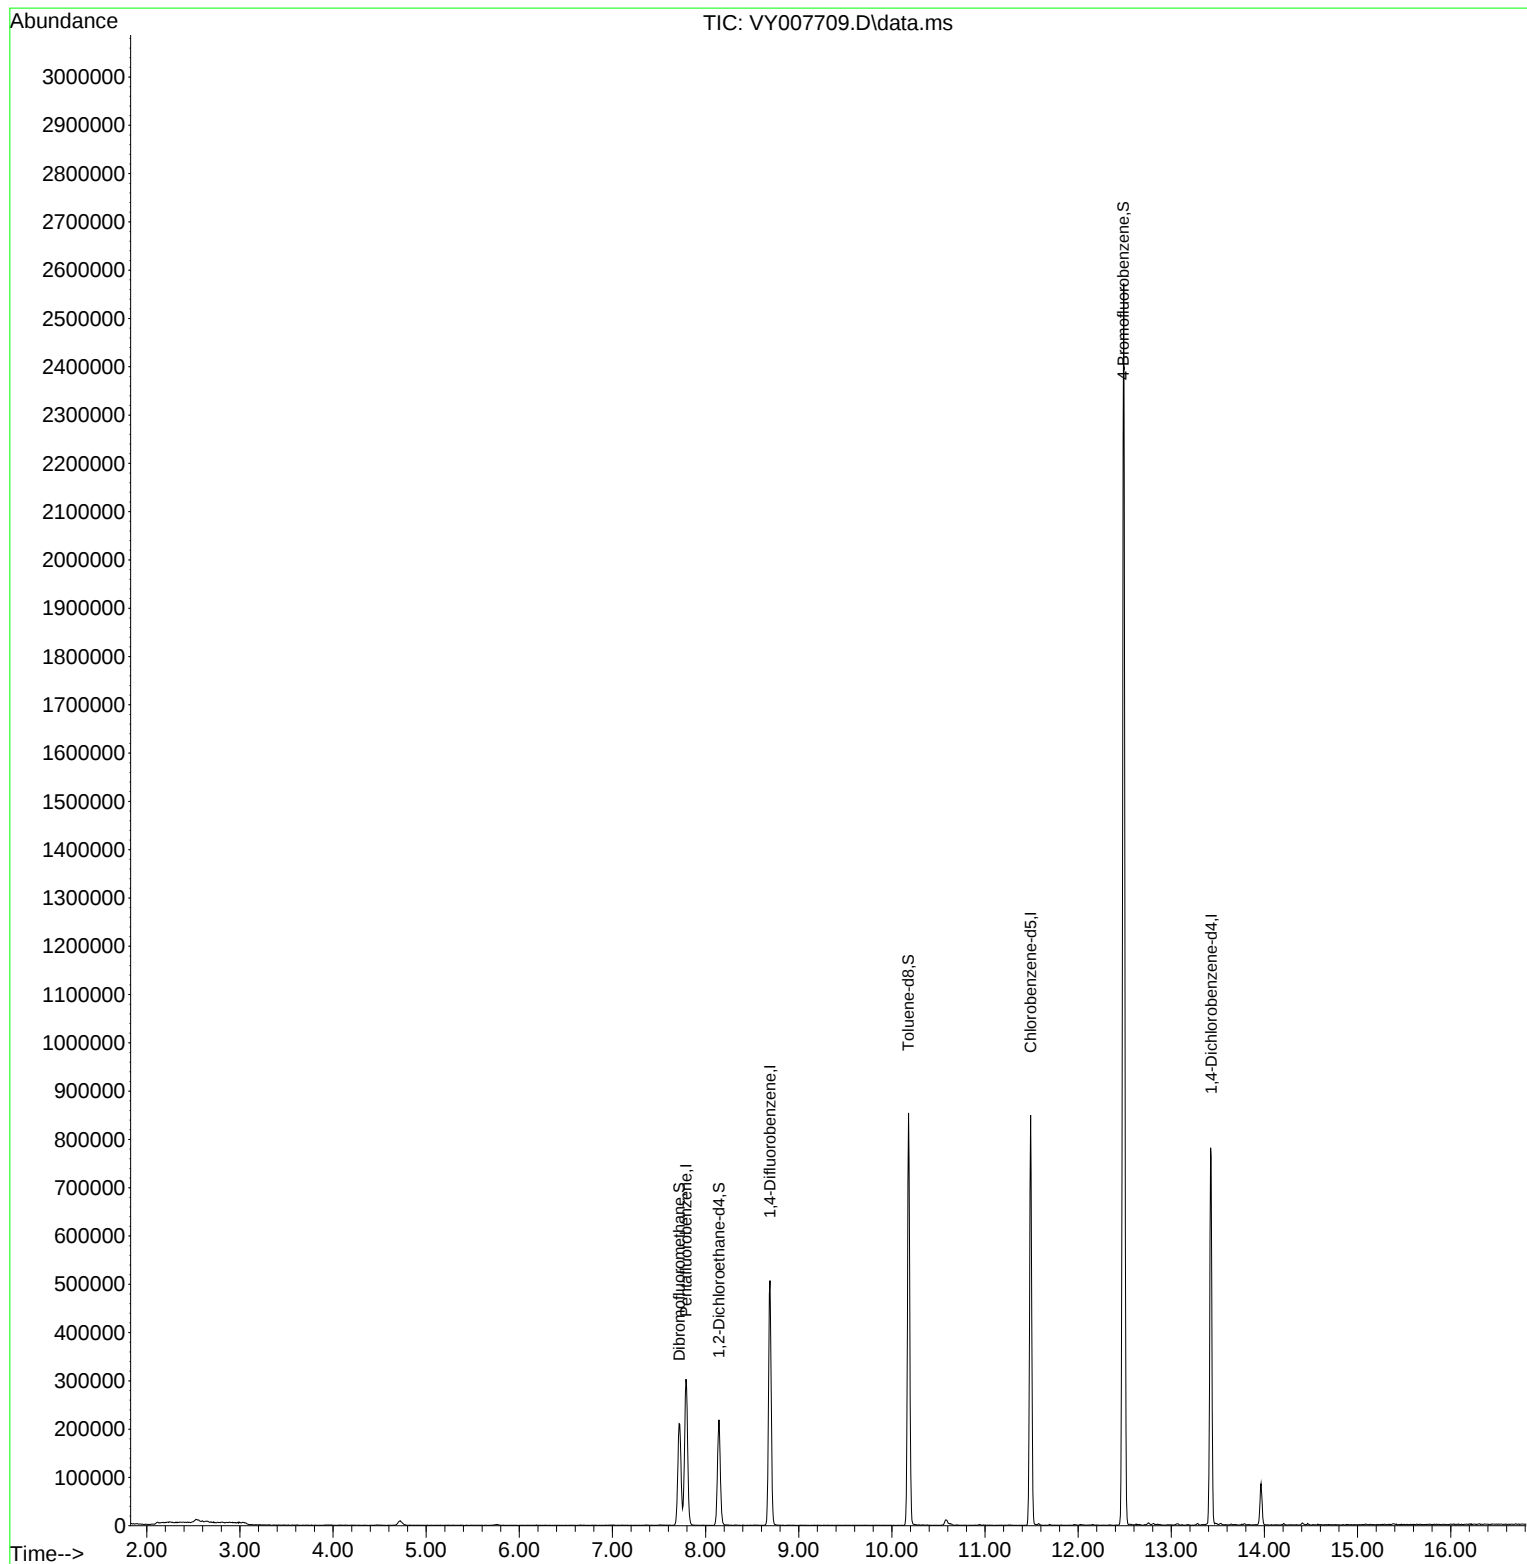


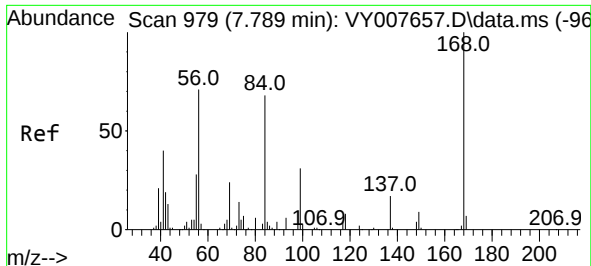

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05




Instrument :
MSVOA_Y
ClientSampleId :
LINE-2-3


Tgt Ion:168 Resp: 239274
Ion Ratio Lower Upper
168 100
99 51.7 46.9 70.3

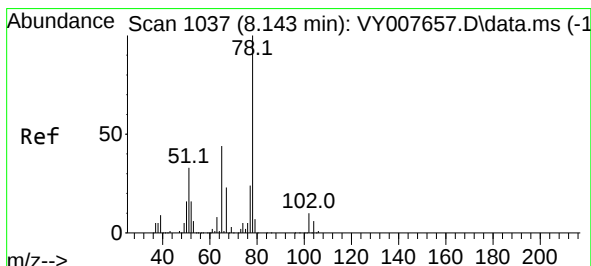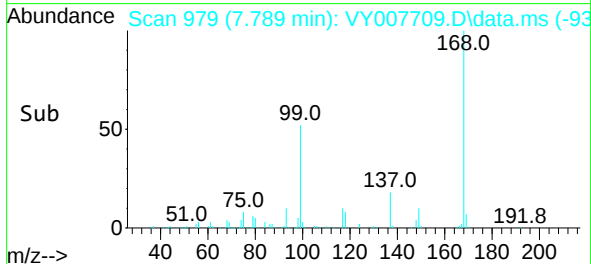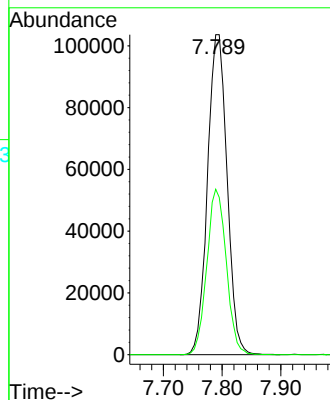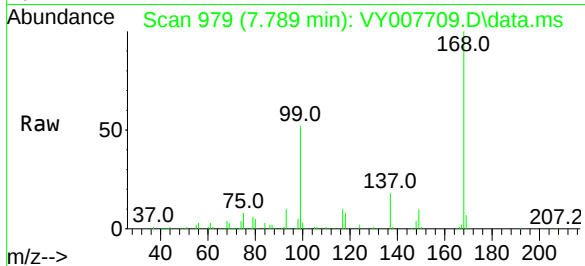

#33
1,2-Dichloroethane-d4
Concen: 63.603 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05

Tgt Ion: 65 Resp: 159324
Ion Ratio Lower Upper
65 100
67 53.1 0.0 99.4

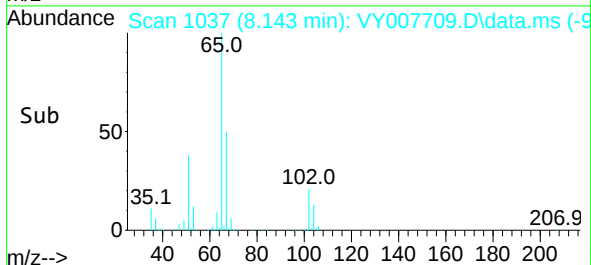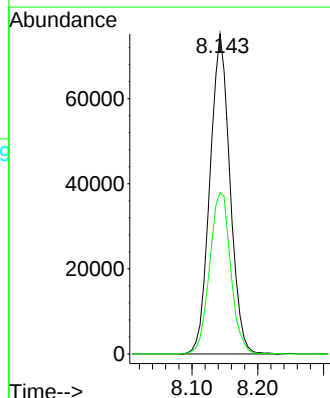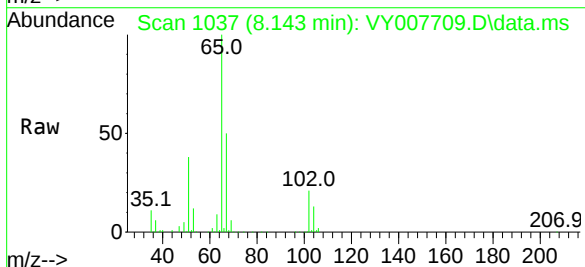

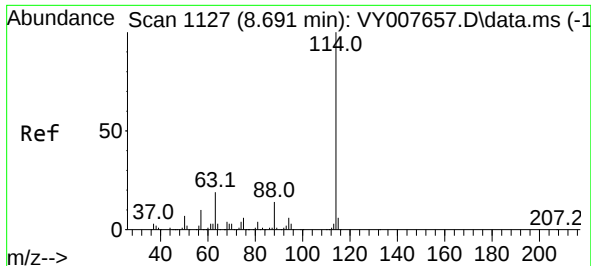

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY007709.D

Acq: 03 Mar 2022 17:05

Instrument :

MSVOA_Y

ClientSampleId :

LINE-2-3





Tgt Ion:114 Resp: 437994

Ion Ratio Lower Upper

114 100

63 19.0 0.0 43.2

88 13.6 0.0 31.8

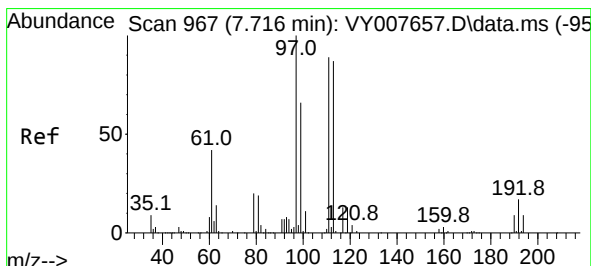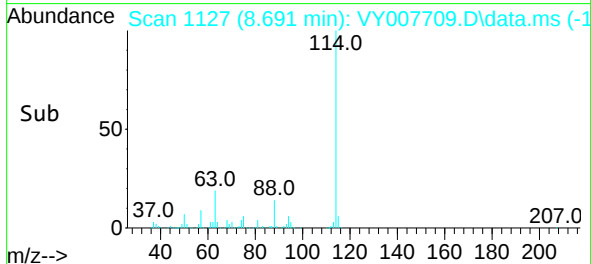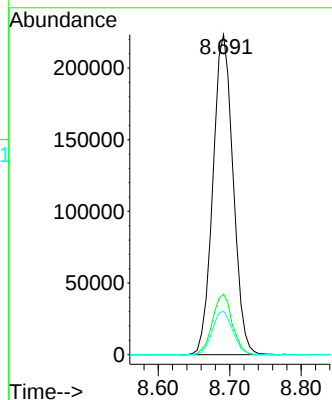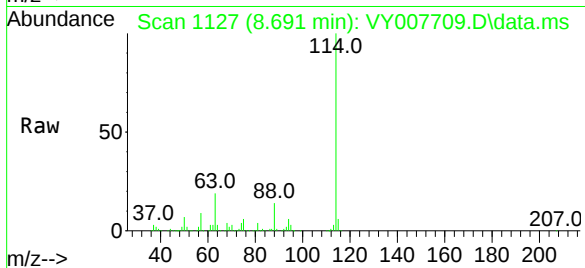

#35

Dibromofluoromethane

Concen: 53.617 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY007709.D

Acq: 03 Mar 2022 17:05




Tgt Ion:113 Resp: 150140


Ion Ratio Lower Upper

113 100

111 101.2 82.6 124.0

192 19.2 17.6 26.4


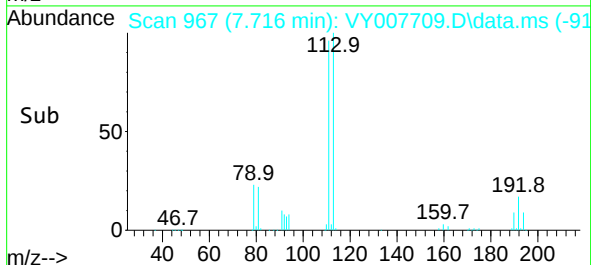
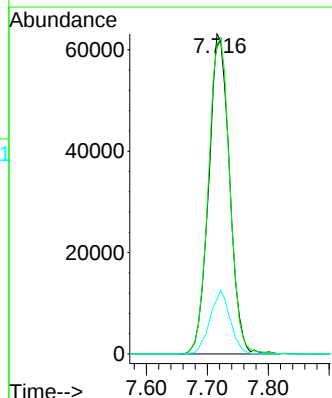
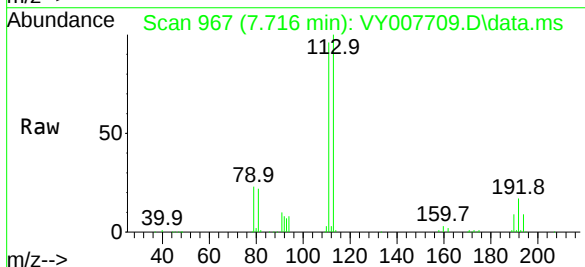


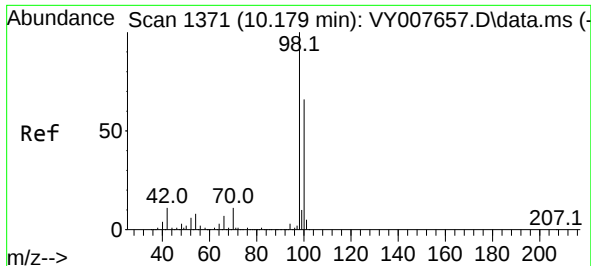

#50
Toluene-d8
Concen: 53.735 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05




Instrument :
MSVOA_Y
ClientSampleId :
LINE-2-3


Tgt Ion: 98 Resp: 553893
Ion Ratio Lower Upper
98 100
100 63.4 50.2 75.2

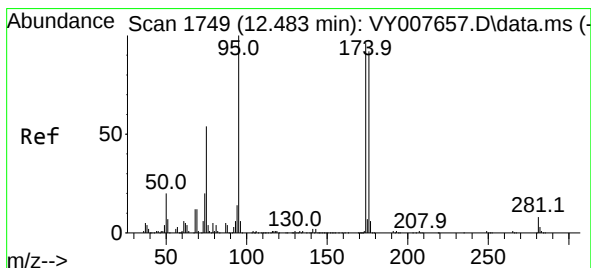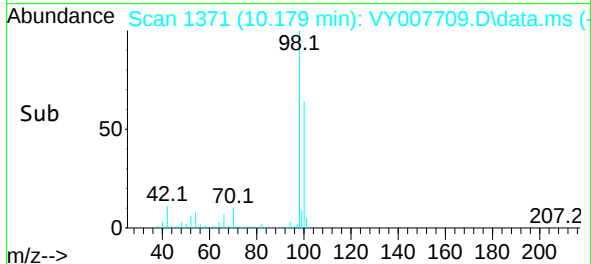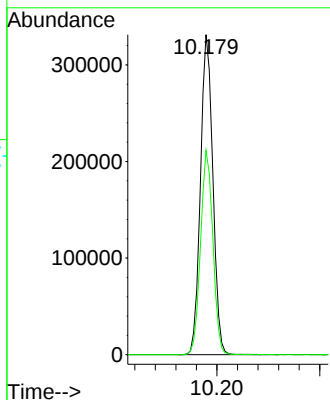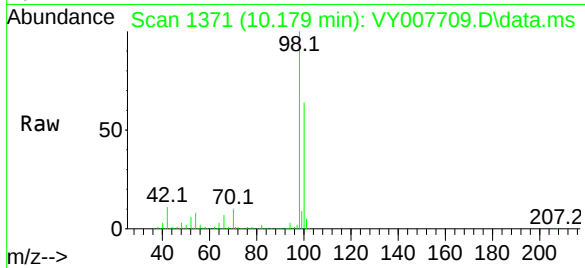

#62
4-Bromofluorobenzene
Concen: 57.245 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05

Tgt Ion: 95 Resp: 190205
Ion Ratio Lower Upper
95 100
174 95.3 0.0 177.0
176 93.6 0.0 175.8


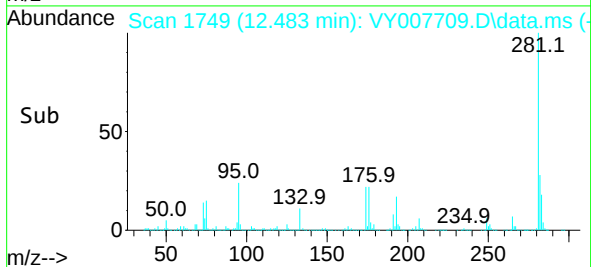
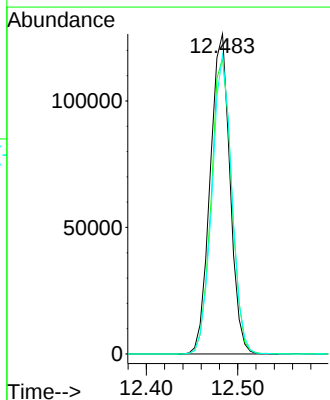
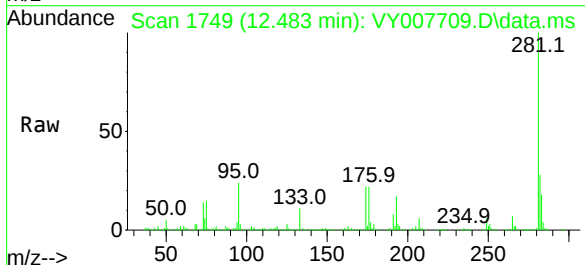


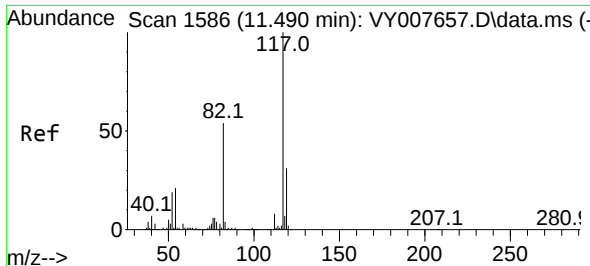

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05

Instrument :
MSVOA_Y
ClientSampleId :
LINE-2-3

Tgt Ion:117 Resp: 440332
Ion Ratio Lower Upper
117 100
82 53.1 43.0 64.4
119 32.3 25.4 38.0

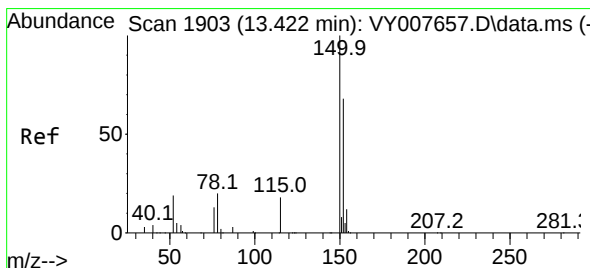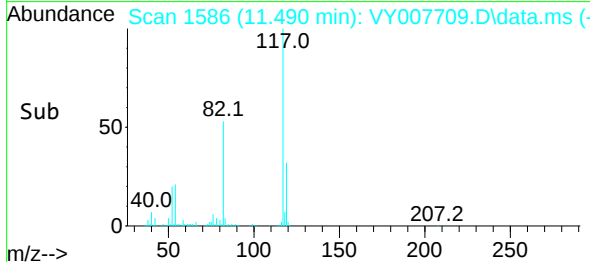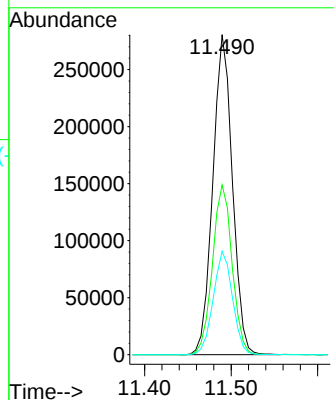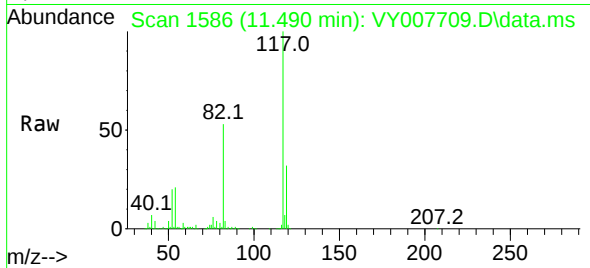

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY007709.D
Acq: 03 Mar 2022 17:05

Tgt Ion:152 Resp: 199326
Ion Ratio Lower Upper
152 100
115 55.1 28.2 84.7
150 156.5 0.0 347.6

