
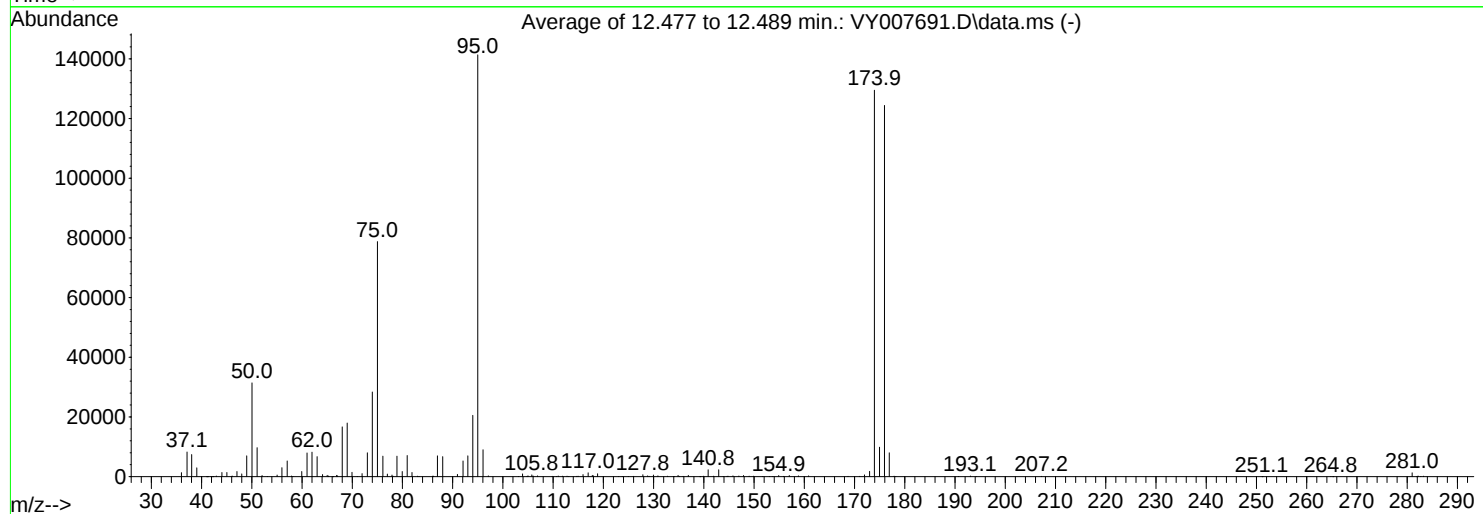


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030322\
Data File : VY007691.D
Acq On : 03 Mar 2022 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
Title : SW846 8260
Last Update : Tue Mar 01 09:08:03 2022

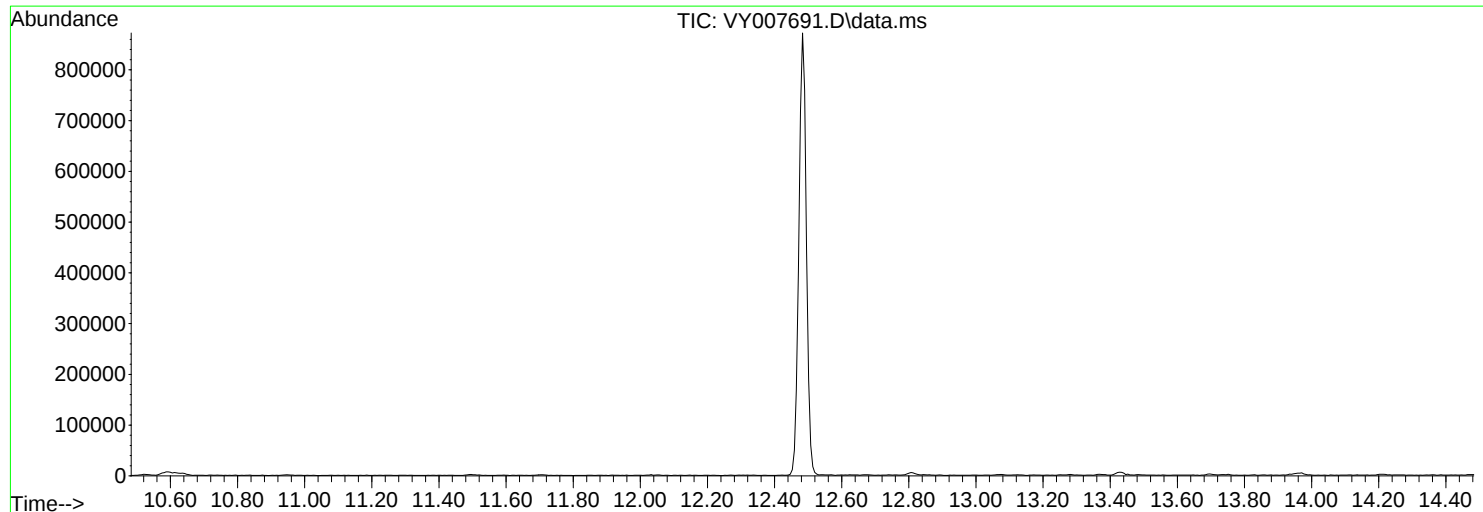

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	31395	PASS
75	95	30	60	55.7	78789	PASS
95	95	100	100	100.0	141333	PASS
96	95	5	9	6.4	9034	PASS
173	174	0.00	2	1.4	1768	PASS
174	95	50	100	91.6	129464	PASS
175	174	5	9	7.6	9854	PASS
176	174	95	101	96.1	124392	PASS
177	176	5	9	6.4	7996	PASS