


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030322\
 Data File : VY007717.D
 Acq On : 03 Mar 2022 20:34
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
 Title : SW846 8260
 Last Update : Tue Mar 01 09:08:03 2022

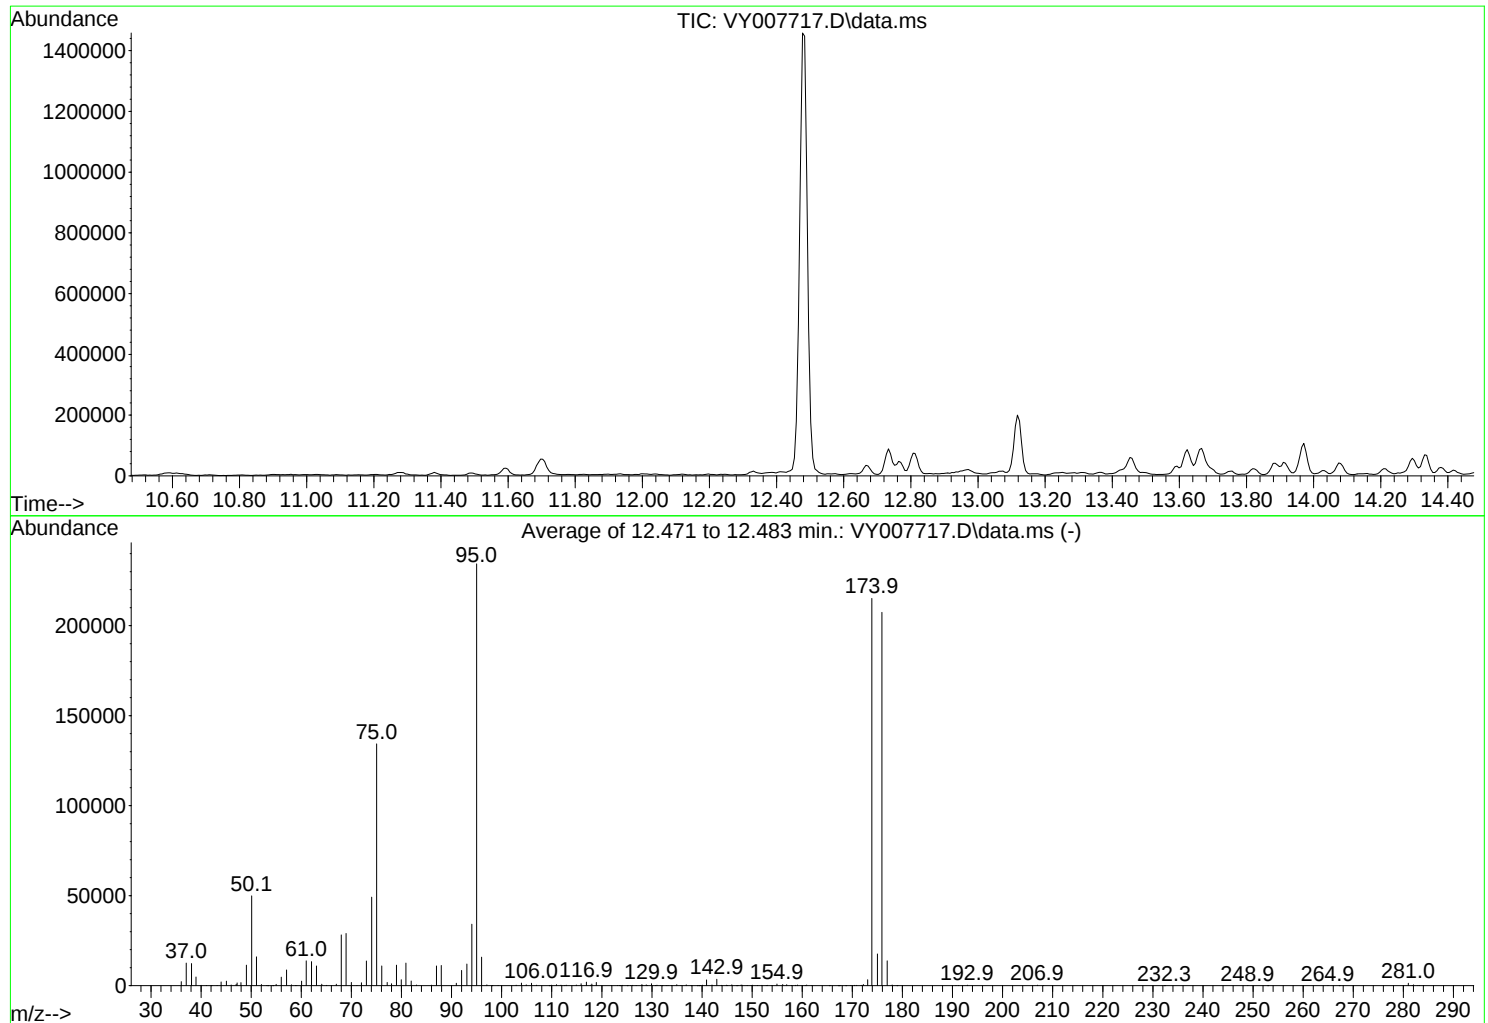

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1736

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	49888	PASS
75	95	30	60	57.3	134309	PASS
95	95	100	100	100.0	234368	PASS
96	95	5	9	6.8	15850	PASS
173	174	0.00	2	1.5	3327	PASS
174	95	50	100	91.8	215168	PASS
175	174	5	9	8.2	17584	PASS
176	174	95	101	96.4	207381	PASS
177	176	5	9	6.7	13813	PASS