



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030422\
Data File : VY007737.D
Acq On : 04 Mar 2022 10:47
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
Title : SW846 8260
Last Update : Tue Mar 01 09:08:03 2022

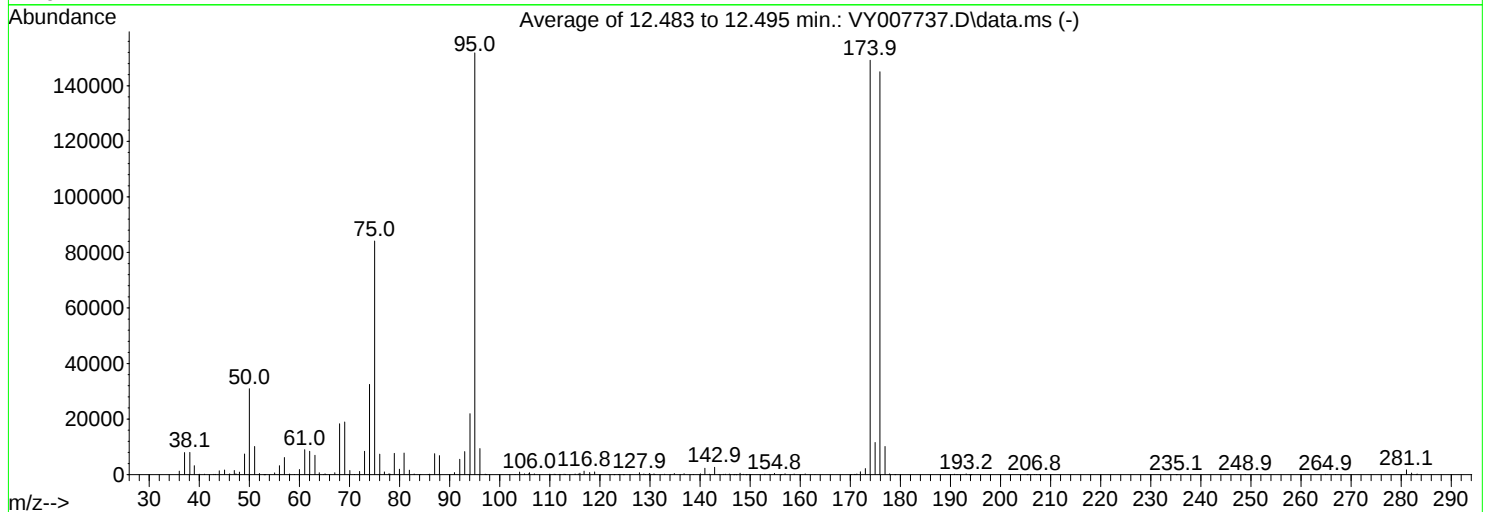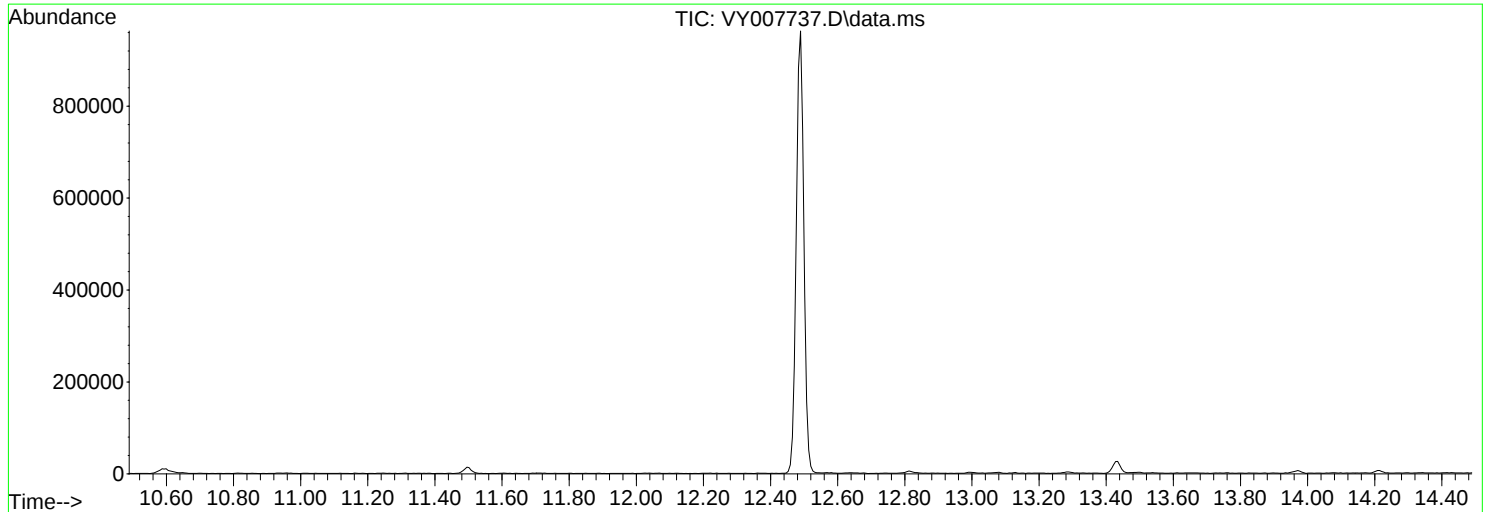

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	30965	PASS
75	95	30	60	55.4	84125	PASS
95	95	100	100	100.0	151848	PASS
96	95	5	9	6.2	9420	PASS
173	174	0.00	2	1.5	2183	PASS
174	95	50	100	98.2	149184	PASS
175	174	5	9	7.7	11556	PASS
176	174	95	101	97.2	145067	PASS
177	176	5	9	7.0	10141	PASS