

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030525\
 Data File : VY021407.D
 Acq On : 05 Mar 2025 12:02
 Operator : SY/MD
 Sample : VY0305SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0305SBL01

Quant Time: Mar 06 02:54:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 05 12:42:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	222723	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	373589	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	318454	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	140807	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	135276	57.465	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.940%
35) Dibromofluoromethane	7.634	113	123966	50.482	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.960%
50) Toluene-d8	10.109	98	448479	48.234	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.460%
62) 4-Bromofluorobenzene	12.408	95	138502	43.792	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	87.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030525\
Data File : VY021407.D
Acq On : 05 Mar 2025 12:02
Operator : SY/MD
Sample : VY0305SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0305SBL01

Quant Time: Mar 06 02:54:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 05 12:42:45 2025
Response via : Initial Calibration




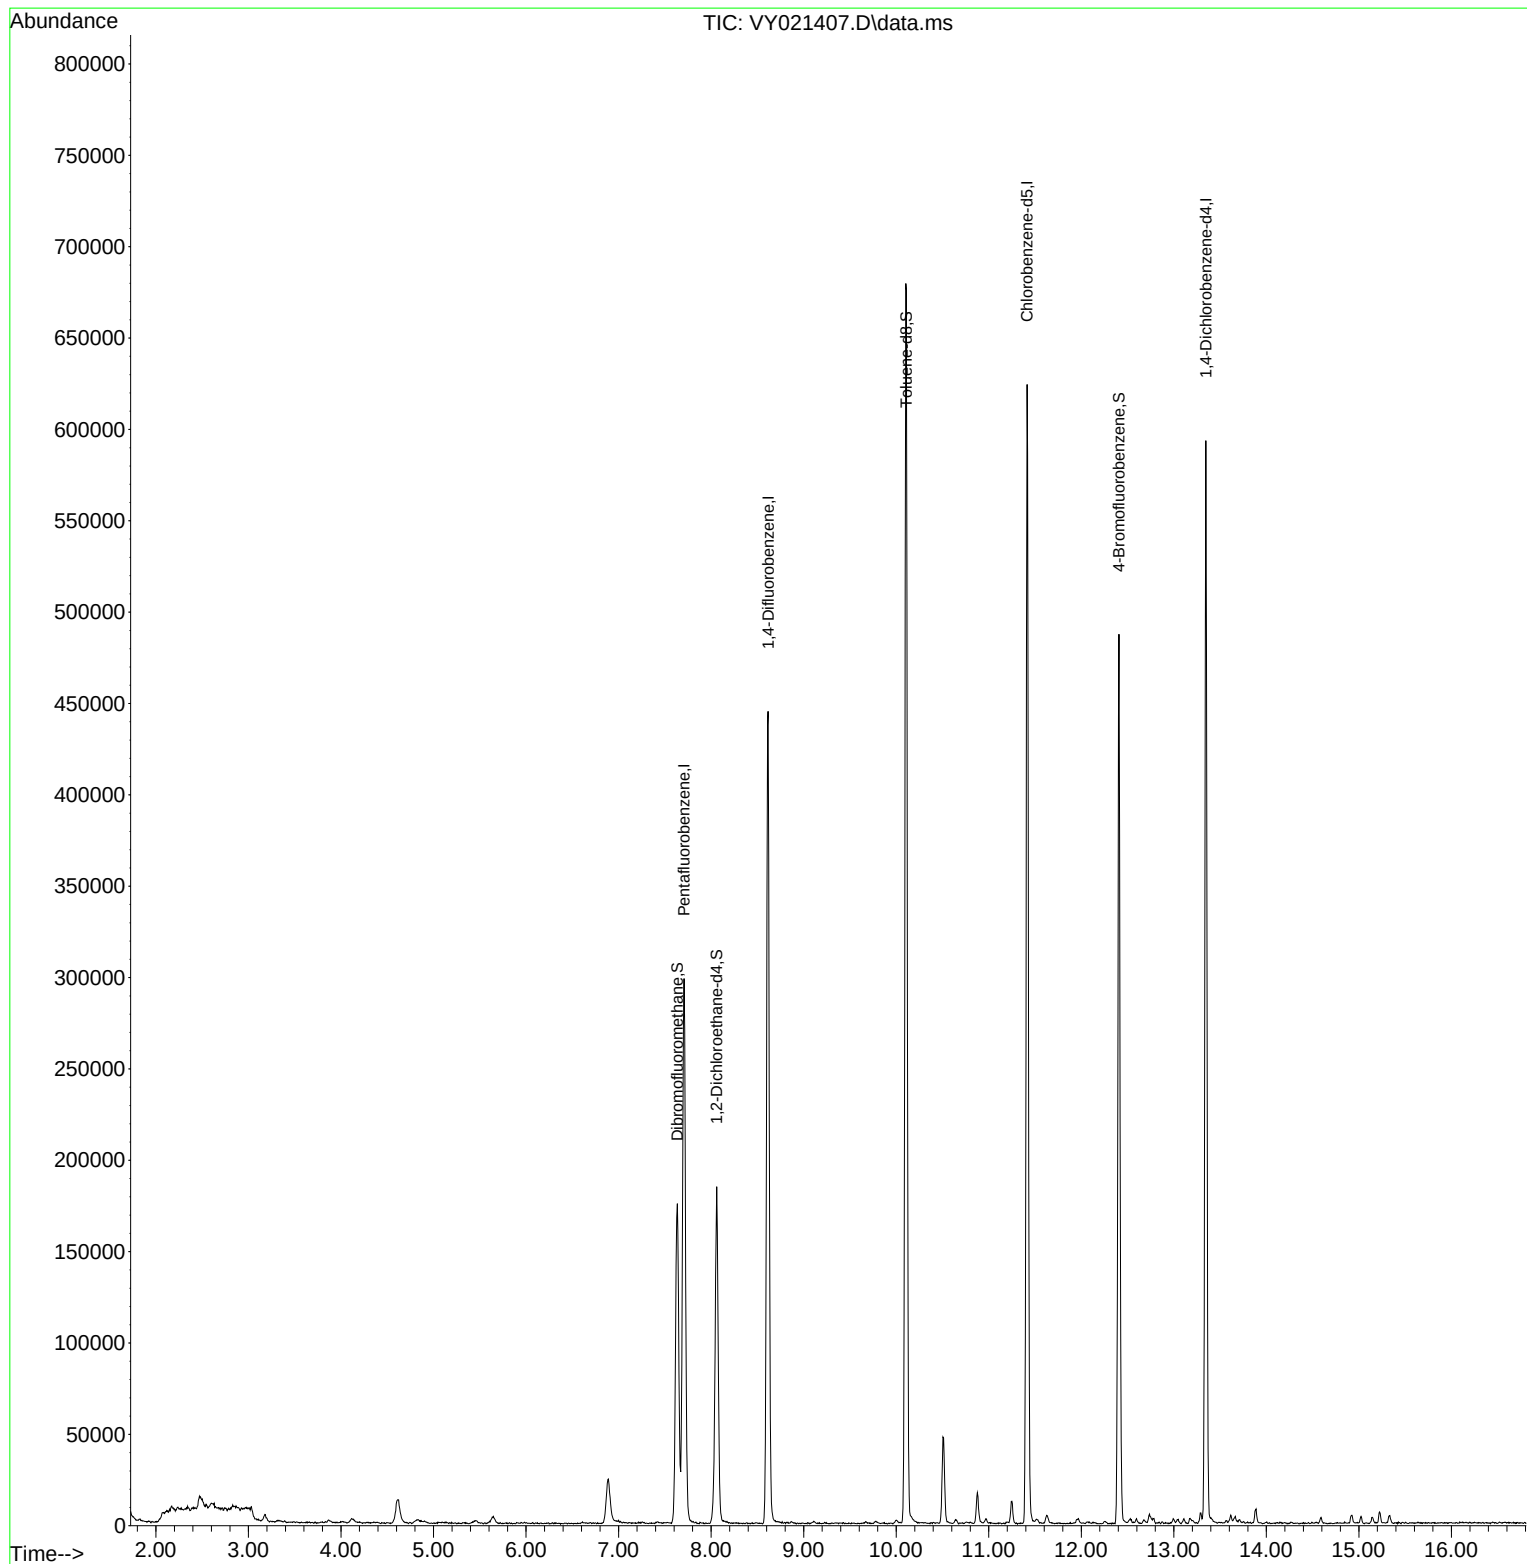


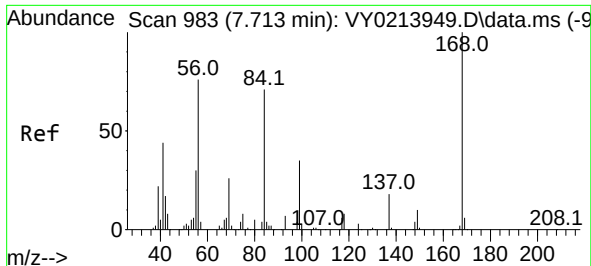

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02




Instrument :
MSVOA_Y
ClientSampleId :
VY0305SBL01


Tgt Ion:168 Resp: 222723
Ion Ratio Lower Upper
168 100
99 55.9 46.0 69.0

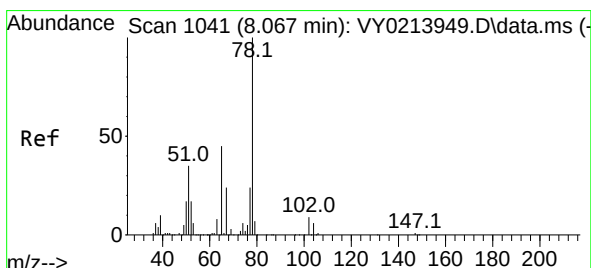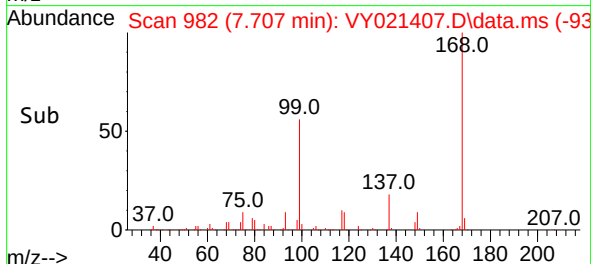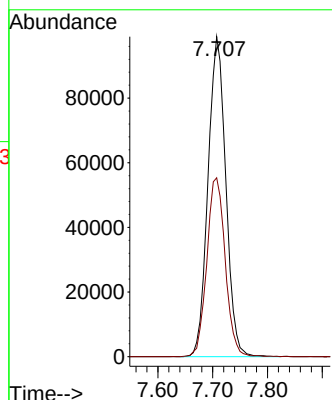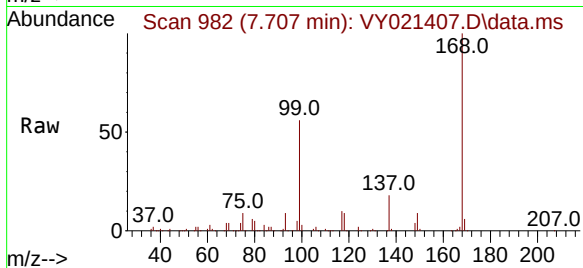

#33
1,2-Dichloroethane-d4
Concen: 57.465 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02

Tgt Ion: 65 Resp: 135276
Ion Ratio Lower Upper
65 100
67 52.9 0.0 102.8


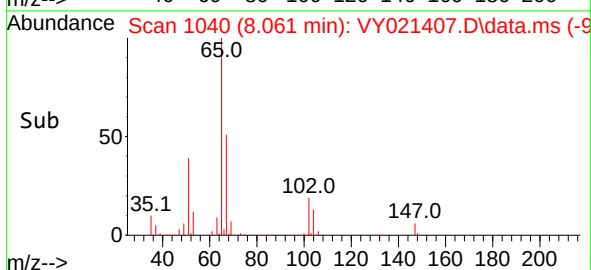
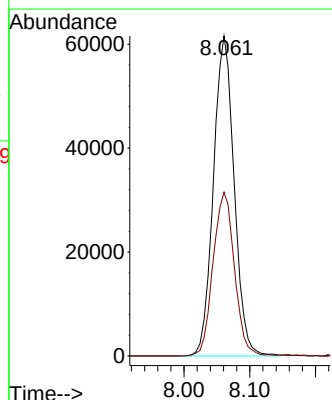
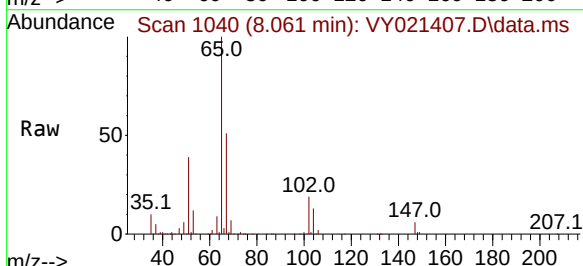


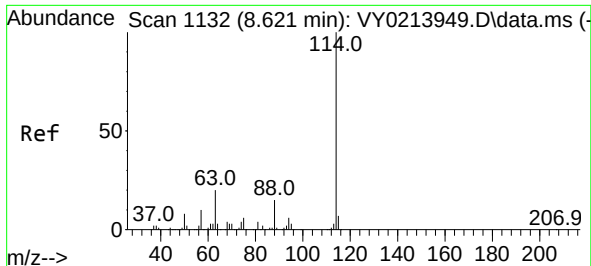

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1132
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02




Instrument :
MSVOA_Y
ClientSampleId :
VY0305SBL01


Tgt Ion:114 Resp: 373589
Ion Ratio Lower Upper
114 100
63 20.8 0.0 40.8
88 15.5 0.0 30.8

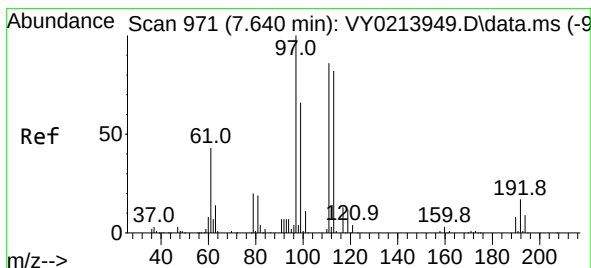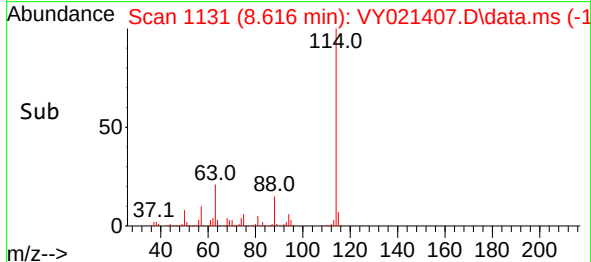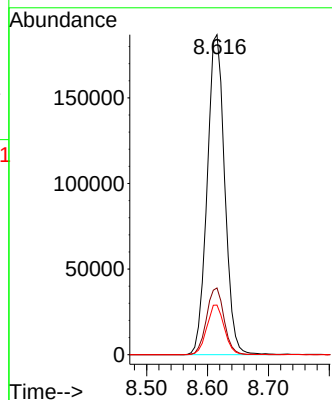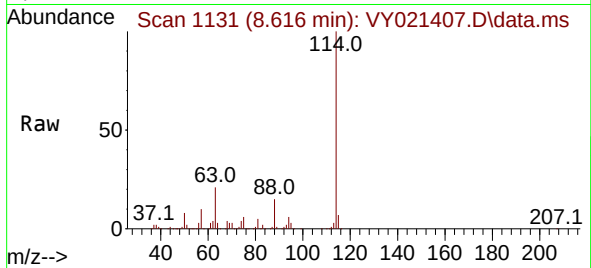

#35
Dibromofluoromethane
Concen: 50.482 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02

Tgt Ion:113 Resp: 123966
Ion Ratio Lower Upper
113 100
111 104.7 82.0 123.0
192 19.3 15.9 23.9


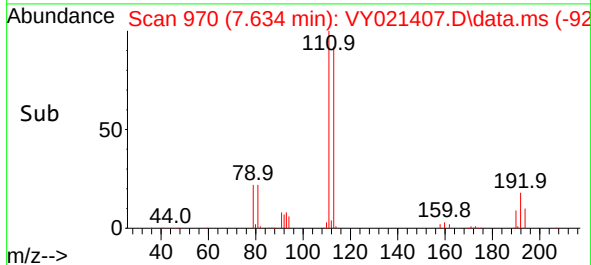
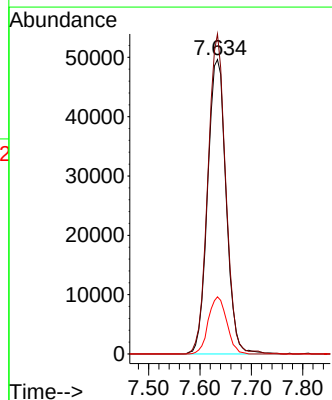
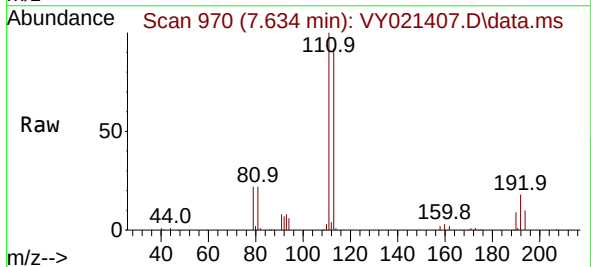


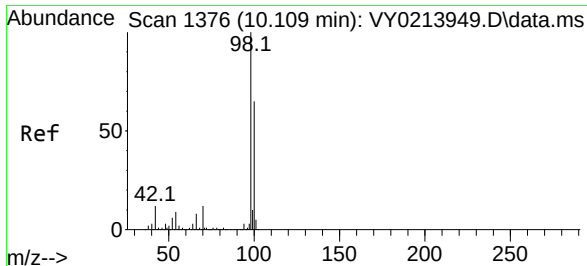

#50
Toluene-d8
Concen: 48.234 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02




Instrument :
MSVOA_Y
ClientSampleId :
VY0305SBL01


Tgt Ion: 98 Resp: 448479
Ion Ratio Lower Upper
98 100
100 64.5 52.1 78.1

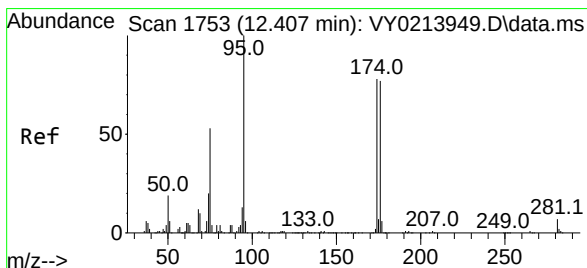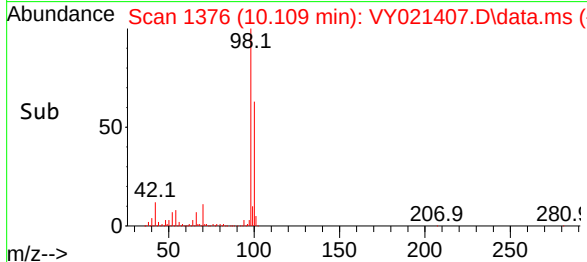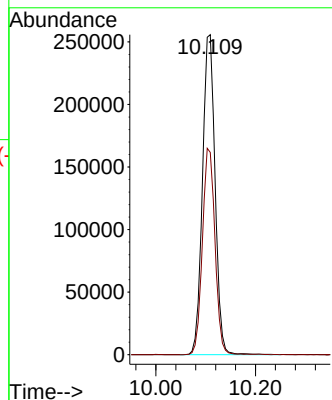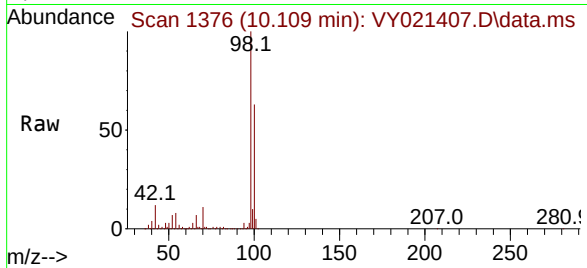

#62
4-Bromofluorobenzene
Concen: 43.792 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02

Tgt Ion: 95 Resp: 138502
Ion Ratio Lower Upper
95 100
174 82.2 0.0 165.0
176 79.2 0.0 160.0


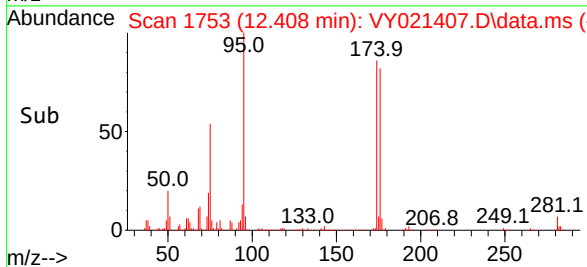
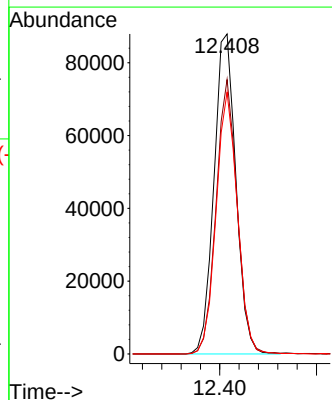
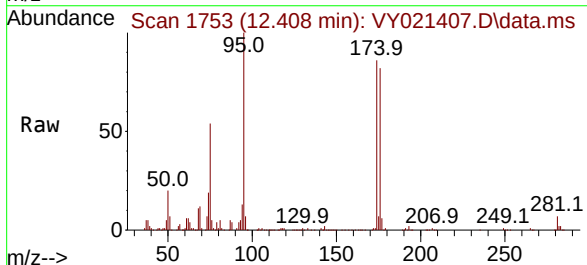


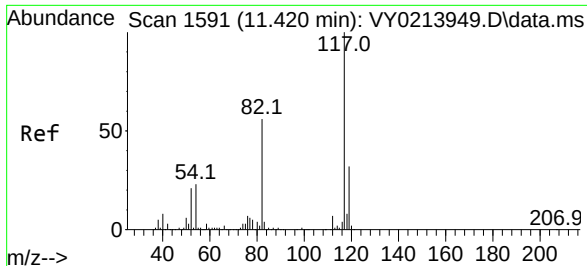

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02

Instrument :
MSVOA_Y
ClientSampleId :
VY0305SBL01

Tgt Ion:117 Resp: 318454
Ion Ratio Lower Upper
117 100
82 56.9 44.6 67.0
119 31.3 25.4 38.0

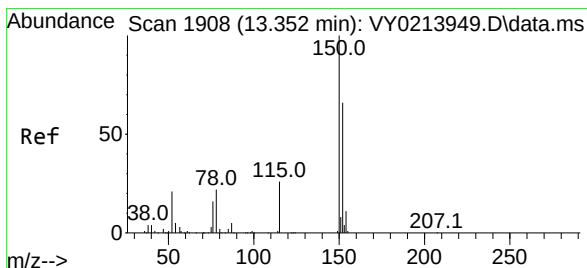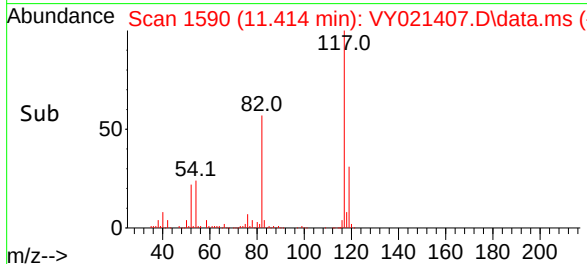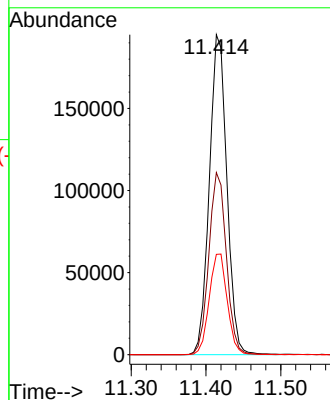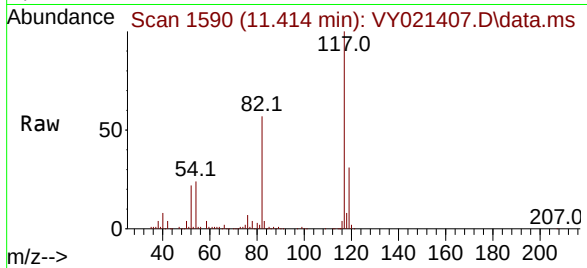

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.006 min
Lab File: VY021407.D
Acq: 05 Mar 2025 12:02

Tgt Ion:152 Resp: 140807
Ion Ratio Lower Upper
152 100
115 59.0 29.0 87.0
150 158.7 0.0 347.2

