
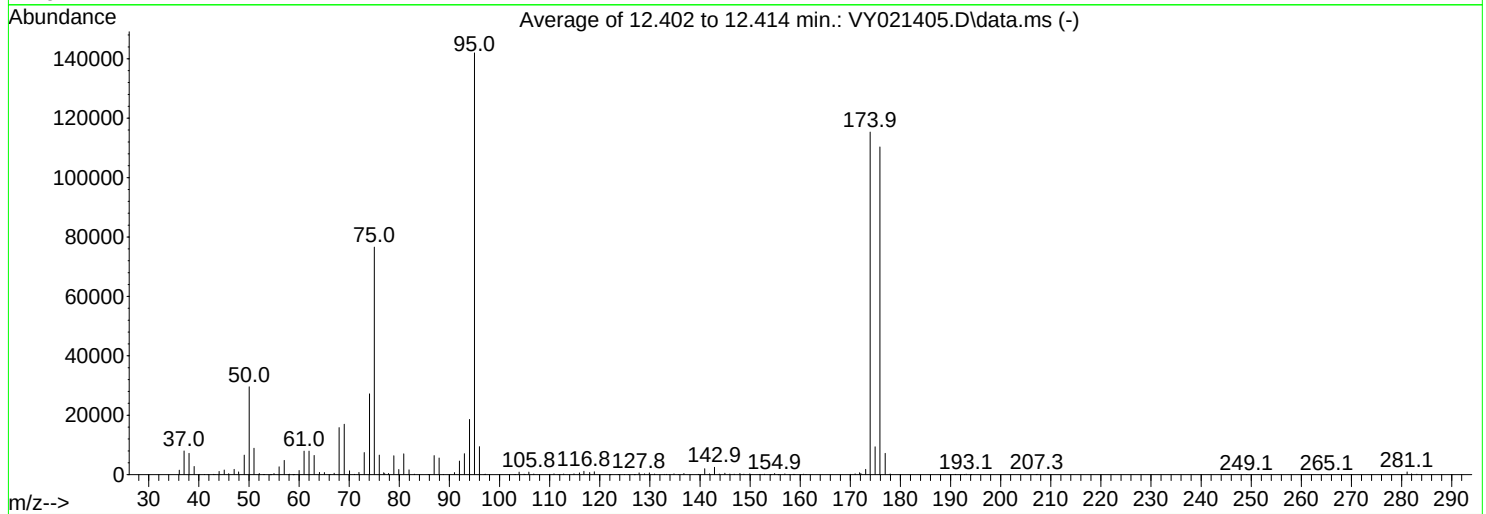


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030525\
Data File : VY021405.D
Acq On : 05 Mar 2025 09:41
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Title : SW846 8260
Last Update : Wed Mar 05 12:42:45 2025

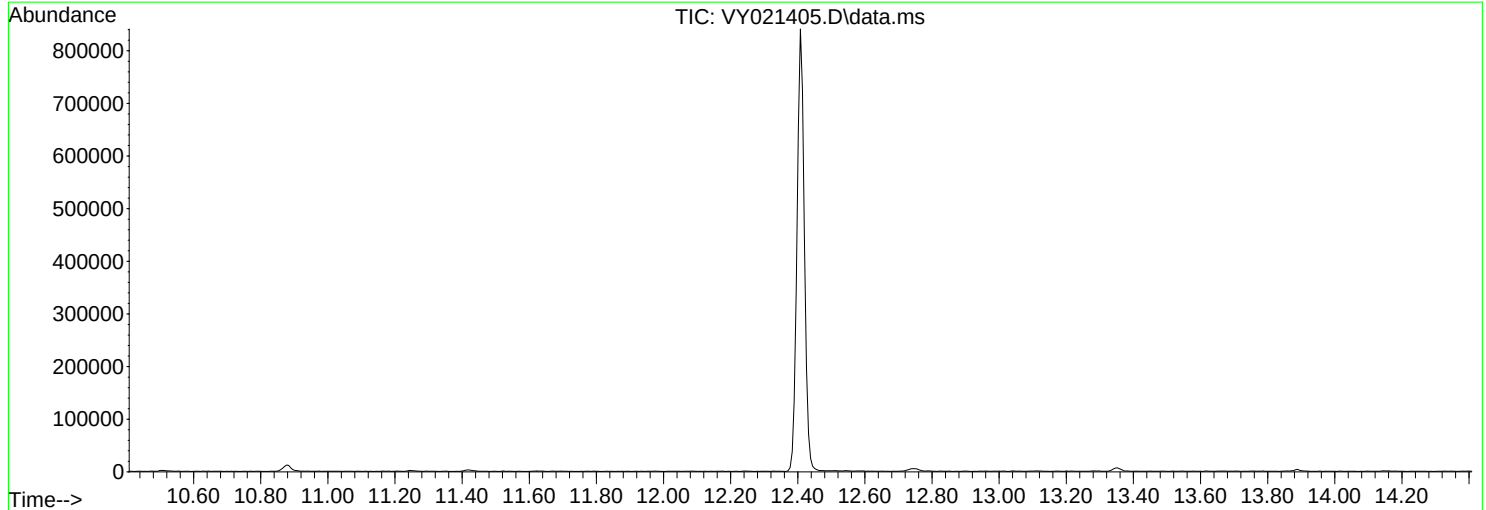

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	29576	PASS
75	95	30	60	53.9	76600	PASS
95	95	100	100	100.0	141997	PASS
96	95	5	9	6.7	9451	PASS
173	174	0.00	2	1.5	1767	PASS
174	95	50	100	81.2	115336	PASS
175	174	5	9	8.1	9391	PASS
176	174	95	101	95.7	110341	PASS
177	176	5	9	6.5	7156	PASS