

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030822\
 Data File : VY007773.D
 Acq On : 08 Mar 2022 12:34
 Operator : SY/MD
 Sample : VY0308SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0308SBL01

Quant Time: Mar 09 00:25:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 01 09:08:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	276313	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	449598	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	406964	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	187508	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	156302	54.032	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	108.060%
35) Dibromofluoromethane	7.716	113	151309	52.640	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.280%
50) Toluene-d8	10.179	98	541856	51.211	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.420%
62) 4-Bromofluorobenzene	12.483	95	159648	46.808	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	93.620%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030822\
Data File : VY007773.D
Acq On : 08 Mar 2022 12:34
Operator : SY/MD
Sample : VY0308SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0308SBL01

Quant Time: Mar 09 00:25:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022822S.M
Quant Title : SW846 8260
QLast Update : Tue Mar 01 09:08:03 2022
Response via : Initial Calibration




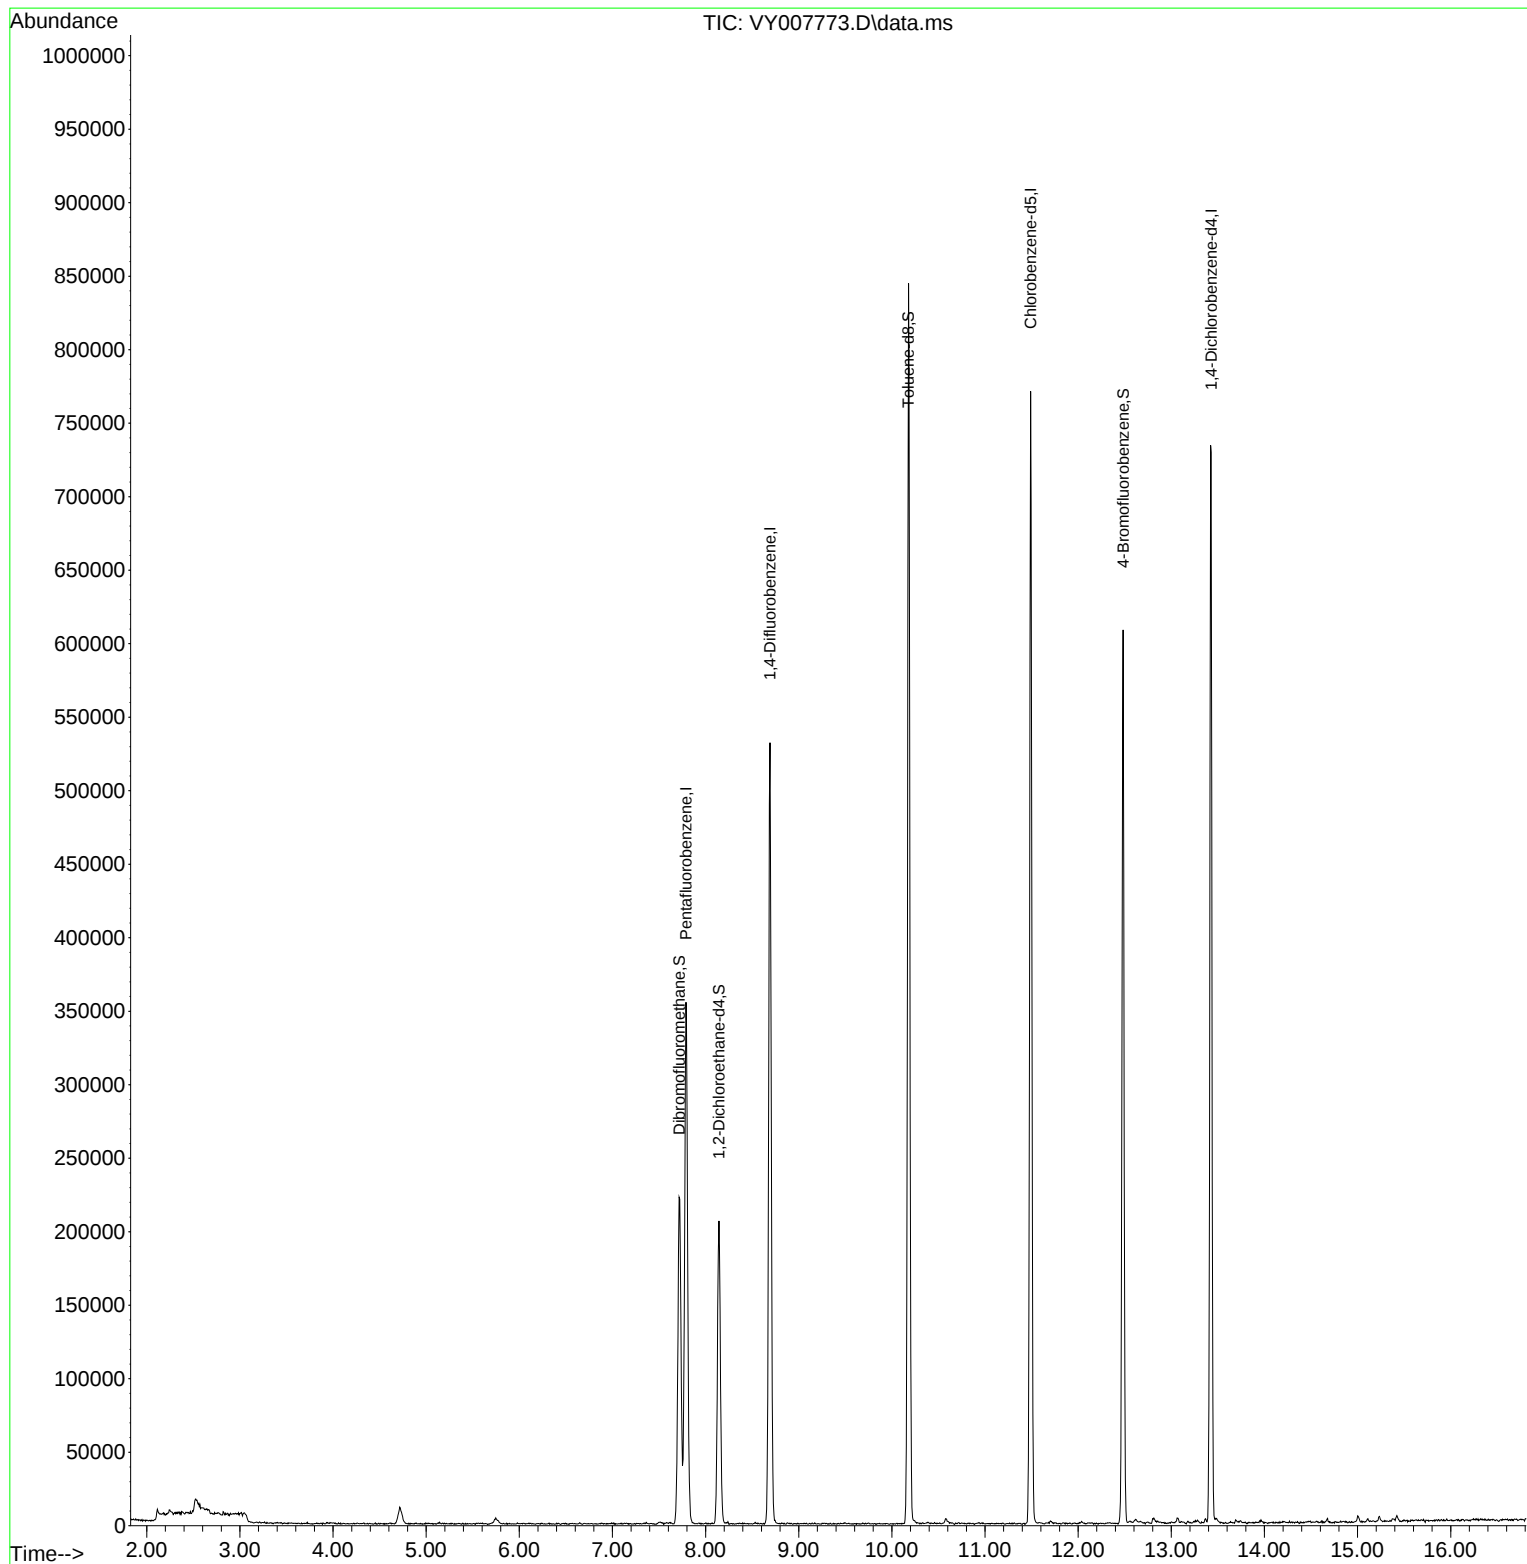


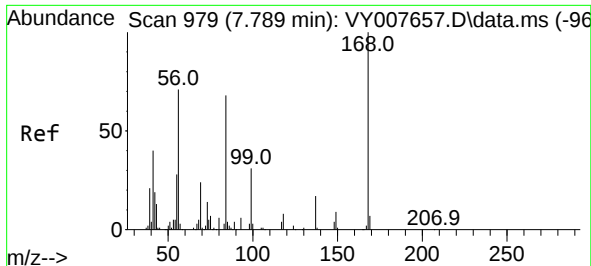

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34




Instrument :
MSVOA_Y
ClientSampleId :
VY0308SBL01


Tgt Ion:168 Resp: 276313
Ion Ratio Lower Upper
168 100
99 49.9 46.9 70.3

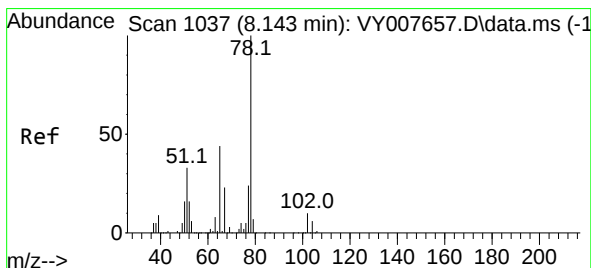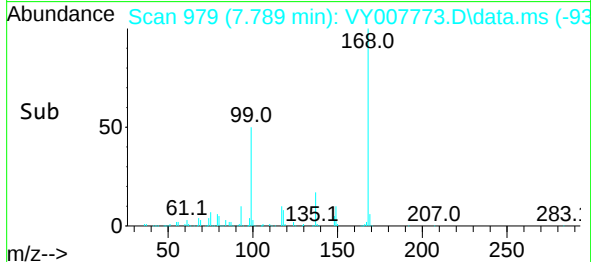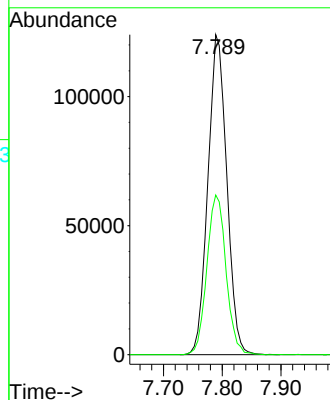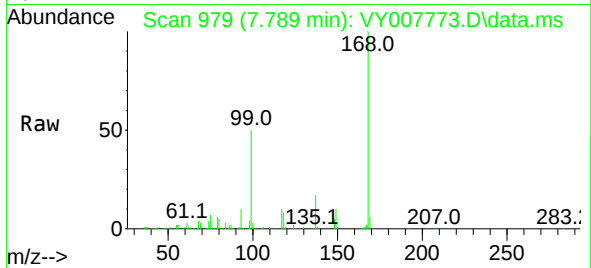

#33
1,2-Dichloroethane-d4
Concen: 54.032 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34

Tgt Ion: 65 Resp: 156302
Ion Ratio Lower Upper
65 100
67 51.5 0.0 99.4


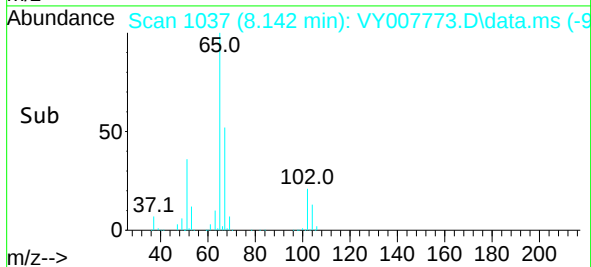
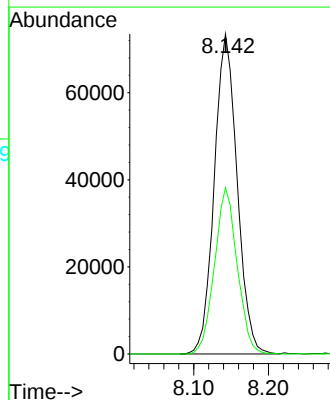
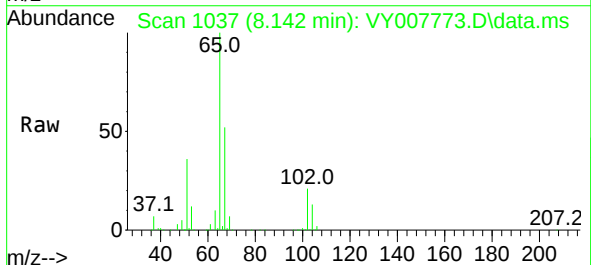


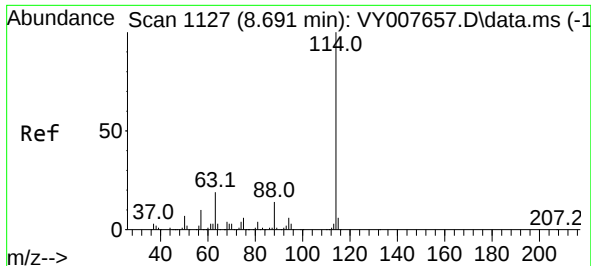

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34




Instrument :
MSVOA_Y
ClientSampleId :
VY0308SBL01


Tgt Ion:114 Resp: 449598
Ion Ratio Lower Upper
114 100
63 19.2 0.0 43.2
88 14.7 0.0 31.8

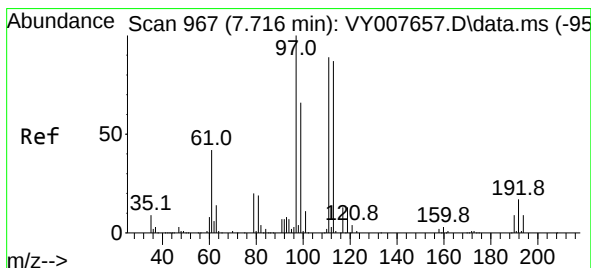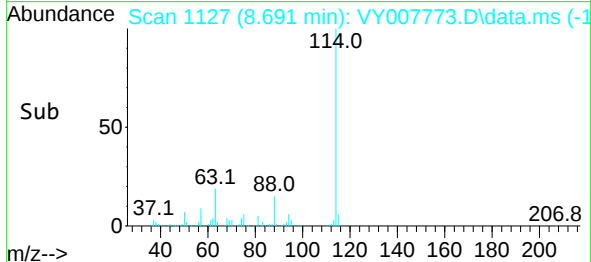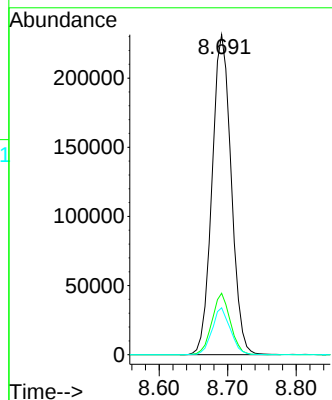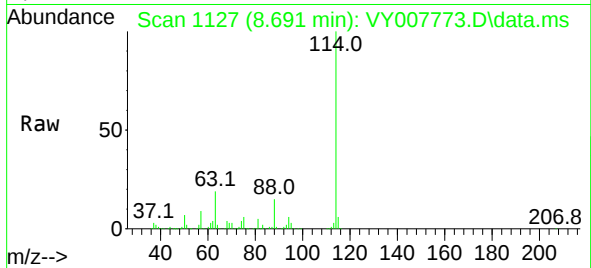

#35
Dibromofluoromethane
Concen: 52.640 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34

Tgt Ion:113 Resp: 151309
Ion Ratio Lower Upper
113 100
111 102.1 82.6 124.0
192 20.7 17.6 26.4


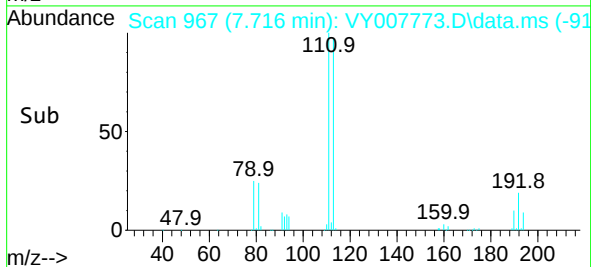
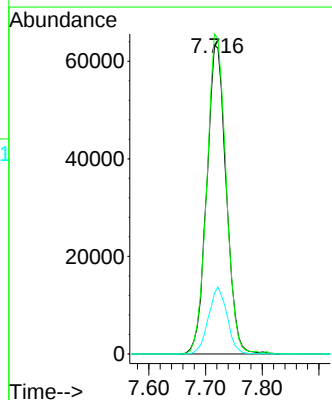
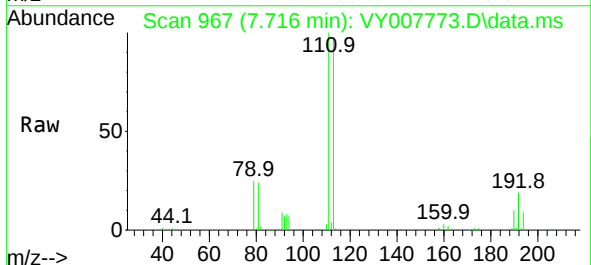


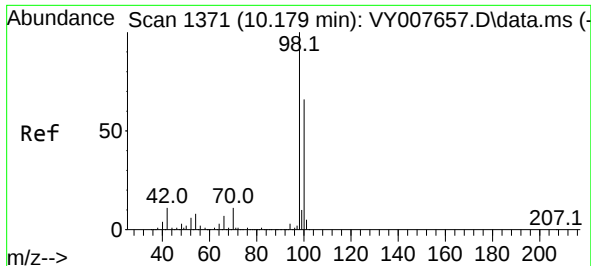

#50
Toluene-d8
Concen: 51.211 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34




Instrument :
MSVOA_Y
ClientSampleId :
VY0308SBL01


Tgt Ion: 98 Resp: 541856
Ion Ratio Lower Upper
98 100
100 63.4 50.2 75.2

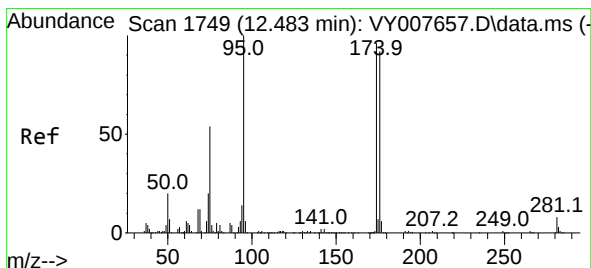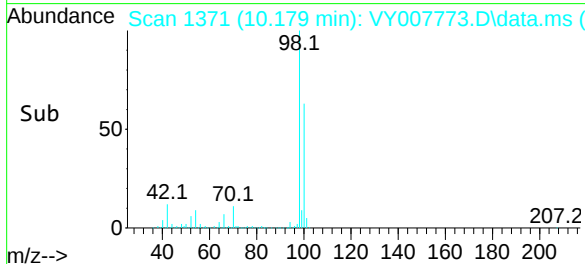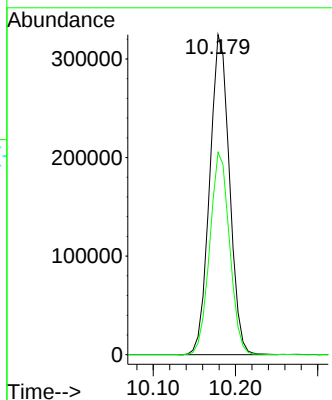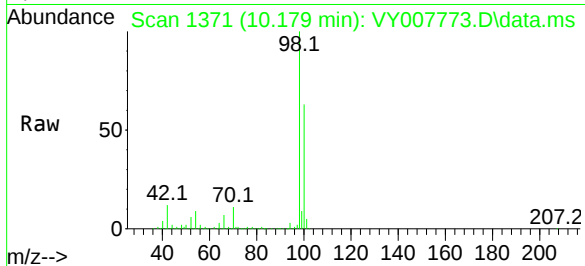

#62
4-Bromofluorobenzene
Concen: 46.808 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34

Tgt Ion: 95 Resp: 159648
Ion Ratio Lower Upper
95 100
174 96.7 0.0 177.0
176 94.3 0.0 175.8

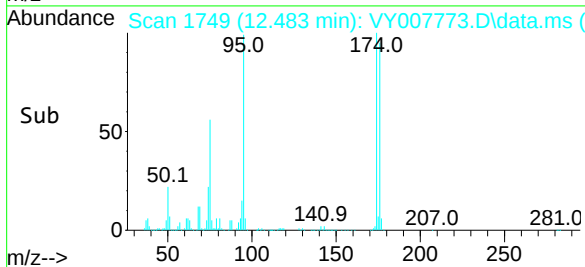
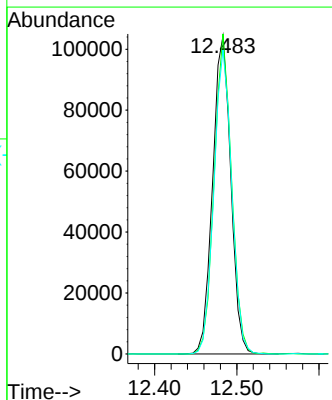
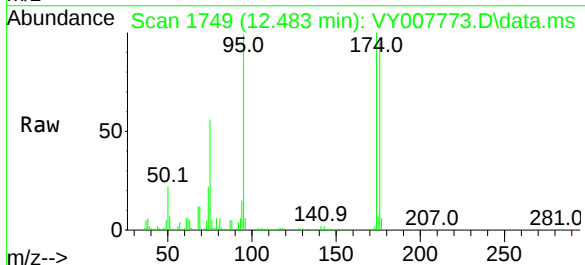


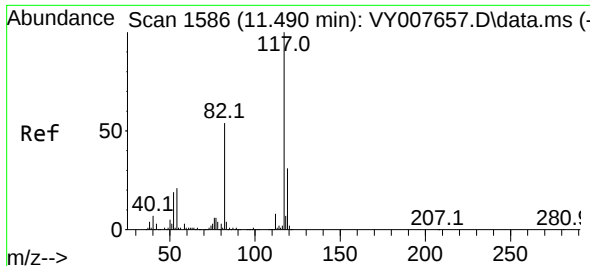

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34

Instrument :
MSVOA_Y
ClientSampleId :
VY0308SBL01

Tgt Ion:117 Resp: 406964
Ion Ratio Lower Upper
117 100
82 52.1 43.0 64.4
119 30.9 25.4 38.0

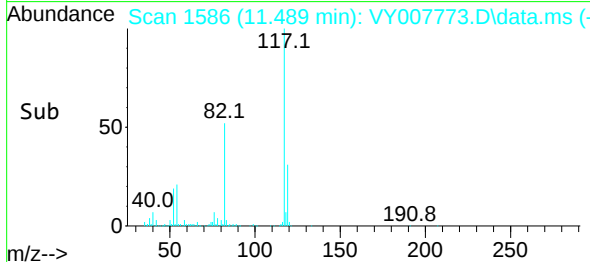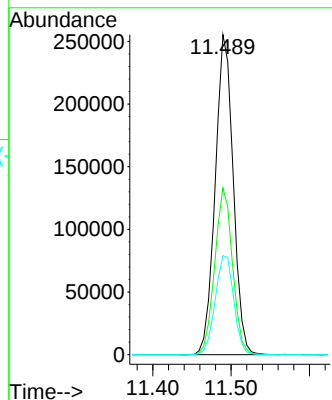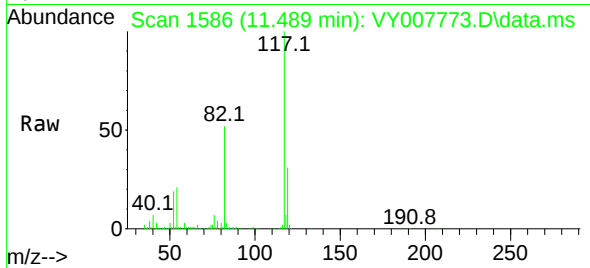

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY007773.D
Acq: 08 Mar 2022 12:34

Tgt Ion:152 Resp: 187508
Ion Ratio Lower Upper
152 100
115 54.0 28.2 84.7
150 157.7 0.0 347.6

