
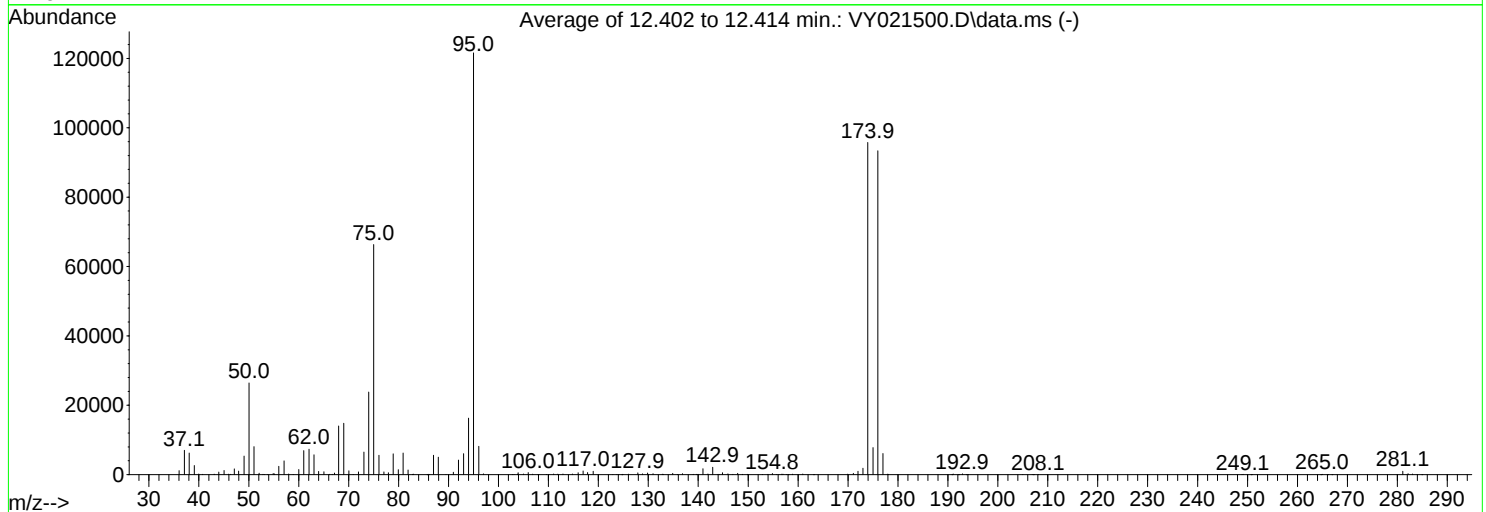


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY031225\  
Data File : VY021500.D  
Acq On : 12 Mar 2025 09:05  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y030425S.M  
Title : SW846 8260  
Last Update : Wed Mar 05 12:42:45 2025

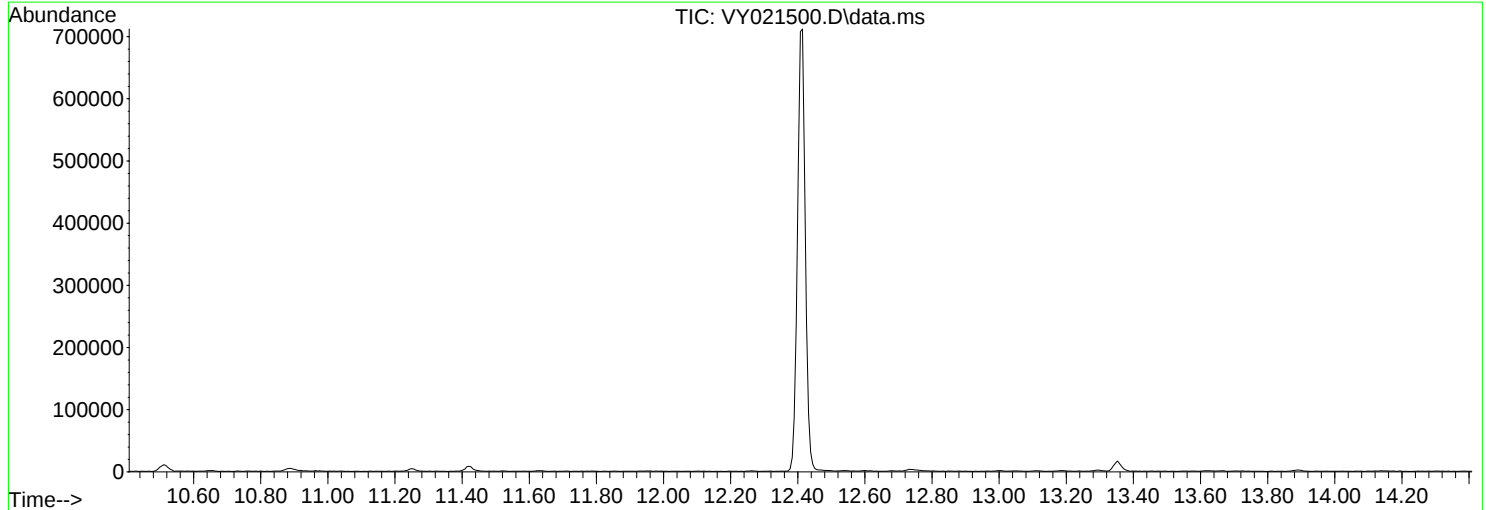

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.7  | 26421  | PASS      |
| 75     | 95      | 30     | 60     | 54.6  | 66355  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 121605 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 8165   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.9   | 1854   | PASS      |
| 174    | 95      | 50     | 100    | 78.7  | 95747  | PASS      |
| 175    | 174     | 5      | 9      | 8.1   | 7799   | PASS      |
| 176    | 174     | 95     | 101    | 97.5  | 93355  | PASS      |
| 177    | 176     | 5      | 9      | 6.5   | 6111   | PASS      |