

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031425\
 Data File : VY021534.D
 Acq On : 14 Mar 2025 12:39
 Operator : SY/MD
 Sample : Q1553-01
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RT2321RE

Quant Time: Mar 15 02:01:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 05 12:42:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	33341	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	49875	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	34521	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	6334	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	16832	47.765	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	95.520%
35) Dibromofluoromethane	7.628	113	17630	53.777	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.560%
50) Toluene-d8	10.103	98	54897	44.226	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	88.460%
62) 4-Bromofluorobenzene	12.401	95	9867	23.368	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	46.740%
Target Compounds						
					Qvalue	
3) Chloromethane	2.068	50	1085	2.515	ug/l #	79
5) Bromomethane	2.611	94	1185	3.478	ug/l #	59
10) Methyl Iodide	4.025	142	1277	3.344	ug/l #	57
11) Tert butyl alcohol	4.842	59	723	9.915	ug/l #	72
13) Acrolein	3.793	56	20	1.116	ug/l #	10
16) Acetone	3.872	43	567	7.377	ug/l #	47
20) Methylene Chloride	4.598	84	544	1.348	ug/l #	57
25) 2-Butanone	6.902	43	228	2.144	ug/l #	48
29) Tetrahydrofuran	7.262	42	91	1.386	ug/l #	33
31) Cyclohexane	7.701	56	965	1.462	ug/l #	42
38) Carbon Tetrachloride	7.707	117	3733	6.325	ug/l #	18
51) 4-Methyl-2-Pentanone	9.999	43	313	1.378	ug/l #	63
59) 2-Hexanone	10.774	43	253	1.684	ug/l	71
74) N-amyl acetate	12.072	43	190	1.753	ug/l #	65
76) 1,2,3-Trichloropropane	12.408	75	5799	90.855	ug/l #	100
77) Bromobenzene	12.523	156	133	1.139	ug/l	95
78) n-propylbenzene	12.597	91	630	1.040	ug/l #	71
80) 1,3,5-Trimethylbenzene	12.737	105	416	1.026	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.408	75	5799	206.543	ug/l #	9
82) 4-Chlorotoluene	12.779	91	475	1.324	ug/l #	41
84) 1,2,4-Trimethylbenzene	13.042	105	609	1.513	ug/l	91
87) 1,3-Dichlorobenzene	13.291	146	336	1.446	ug/l	88
88) 1,4-Dichlorobenzene	13.365	146	424	1.866	ug/l	84
89) n-Butylbenzene	13.615	91	540	1.319	ug/l	92
91) 1,2-Dichlorobenzene	13.663	146	422	2.119	ug/l #	64
92) 1,2-Dibromo-3-Chloropr...	14.279	75	22	1.668	ug/l #	56
93) 1,2,4-Trichlorobenzene	14.925	180	426	3.916	ug/l	87
94) Hexachlorobutadiene	15.029	225	197	2.889	ug/l #	55
95) Naphthalene	15.151	128	831	6.248	ug/l #	92
96) 1,2,3-Trichlorobenzene	15.334	180	490	5.356	ug/l #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031425\
Data File : VY021534.D
Acq On : 14 Mar 2025 12:39
Operator : SY/MD
Sample : Q1553-01
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE

Quant Time: Mar 15 02:01:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 05 12:42:45 2025
Response via : Initial Calibration

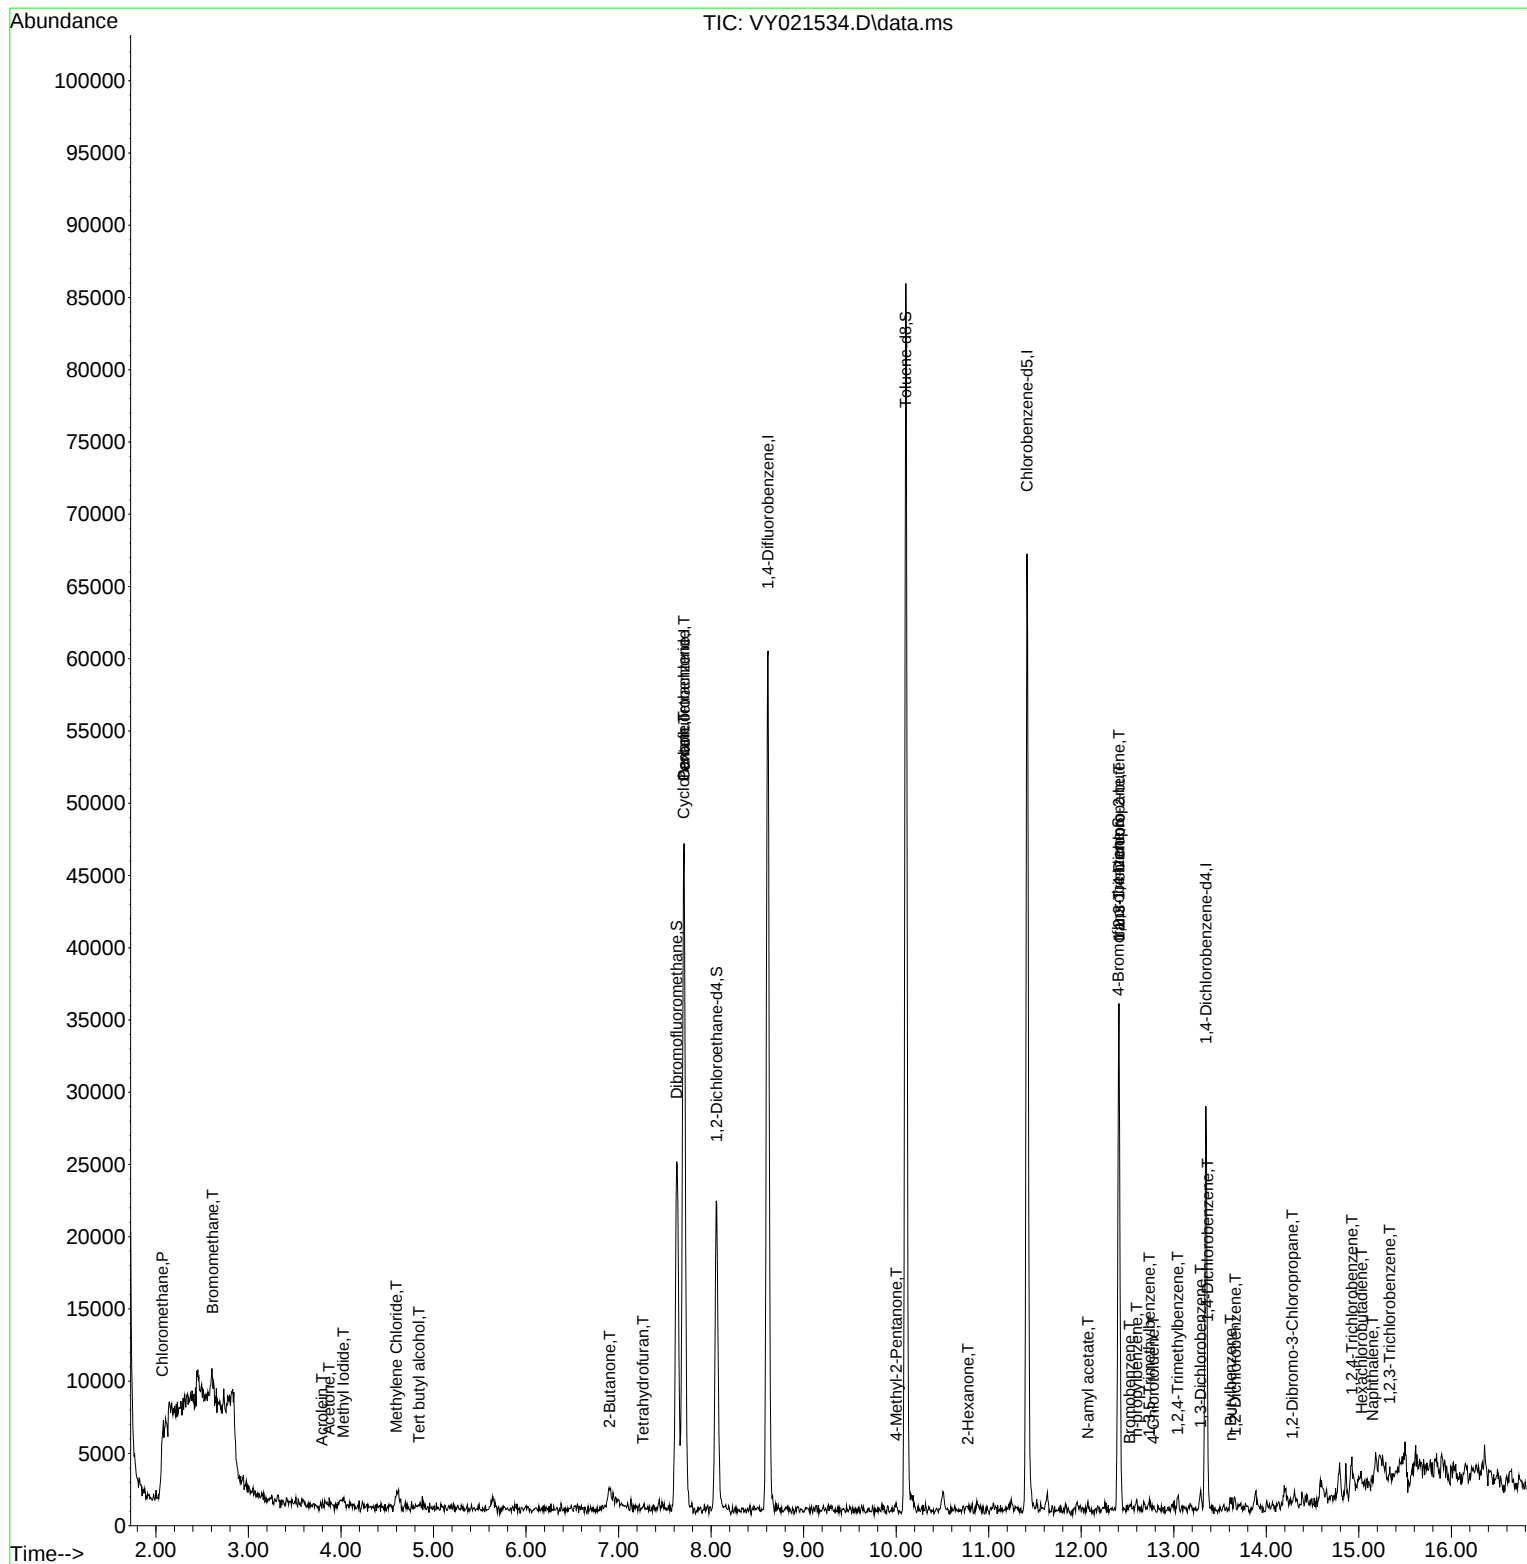

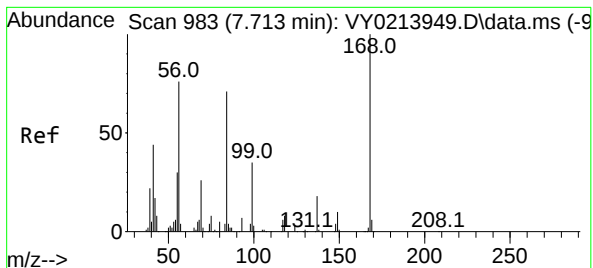

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.707 min Scan# 9

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :





RT2321RE

Tgt Ion:168 Resp: 33341

Ion Ratio Lower Upper

168 100

99 65.1 46.0 69.0

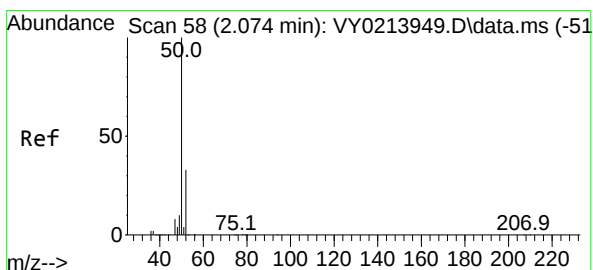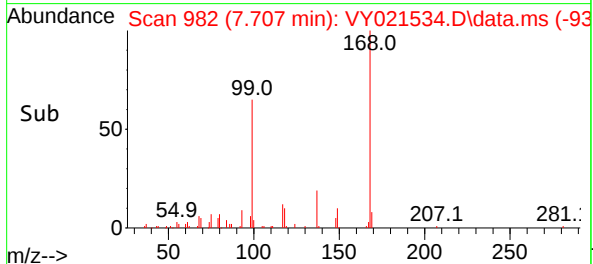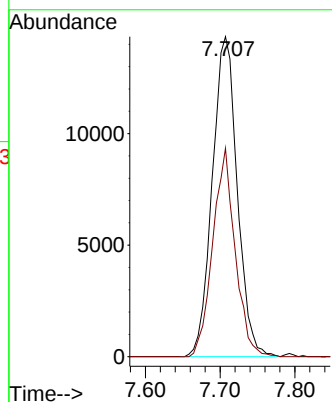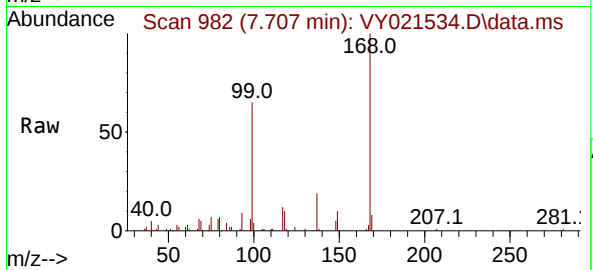

#3

Chloromethane

Concen: 2.515 ug/l

RT: 2.068 min Scan# 57

Delta R.T. -0.006 min

Lab File: VY021534.D




Acq: 14 Mar 2025 12:39


Tgt Ion: 50 Resp: 1085

Ion Ratio Lower Upper

50 100

52 20.9 26.2 39.2#


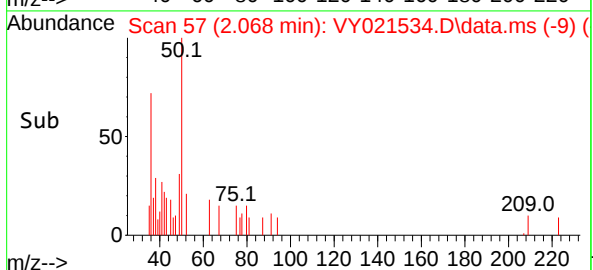

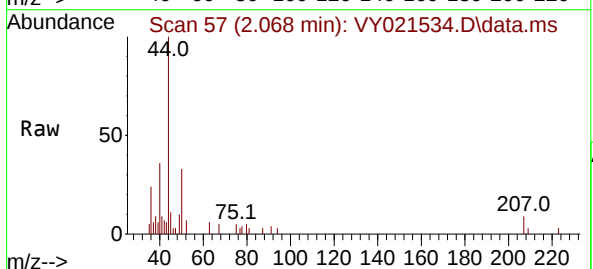


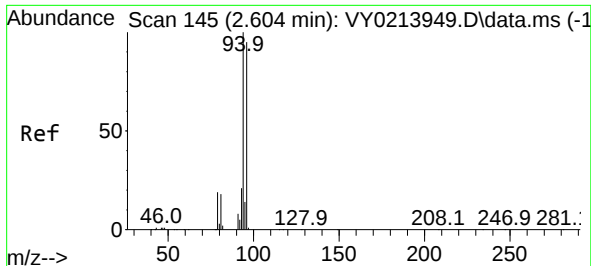

#5
Bromomethane
Concen: 3.478 ug/l
RT: 2.611 min Scan# 145
Delta R.T. 0.006 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 94 Resp: 1185
Ion Ratio Lower Upper
94 100
96 55.5 76.3 114.5#

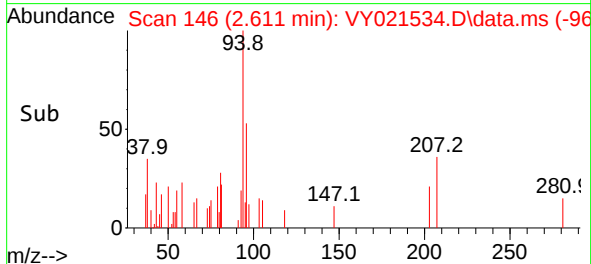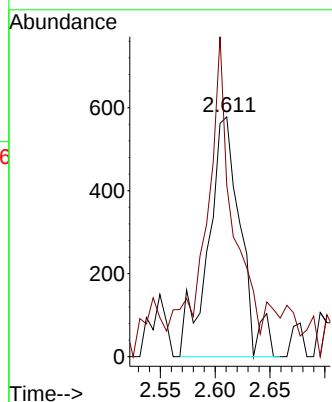

#10
Methyl Iodide
Concen: 3.344 ug/l
RT: 4.025 min Scan# 378
Delta R.T. 0.012 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 142 Resp: 1277
Ion Ratio Lower Upper
142 100
127 16.8 39.1 58.7#
141 2.0 11.8 17.6#


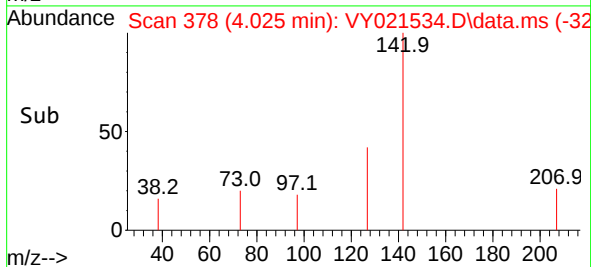

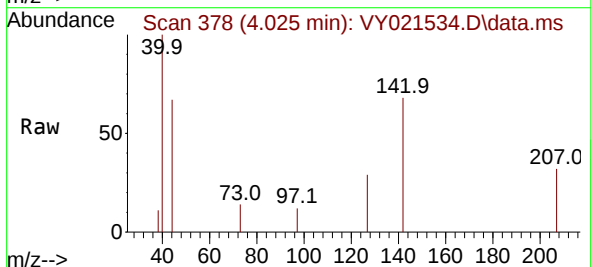


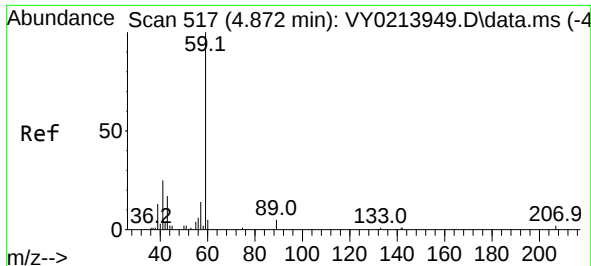

#11
Tert butyl alcohol
Concen: 9.915 ug/l
RT: 4.842 min Scan# 517
Delta R.T. -0.030 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 59 Resp: 723
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

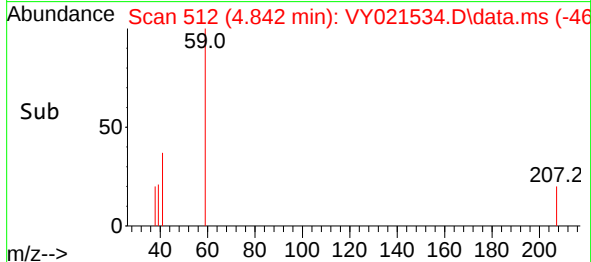

#13
Acrolein
Concen: 1.116 ug/l
RT: 3.793 min Scan# 340
Delta R.T. 0.128 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 56 Resp: 20
Ion Ratio Lower Upper
56 100
55 0.0 63.4 95.2#


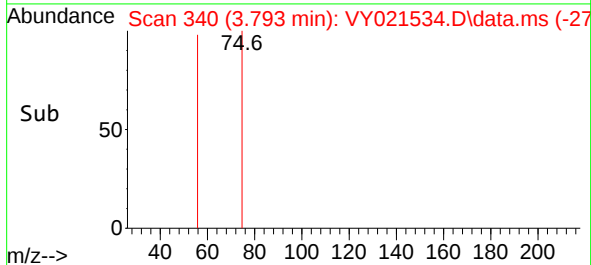

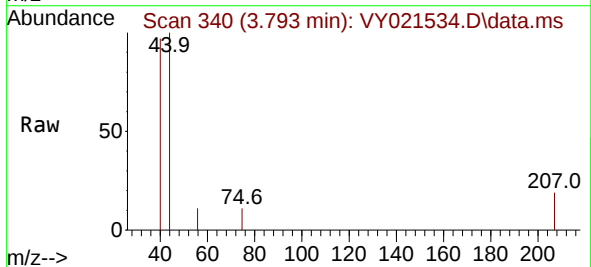


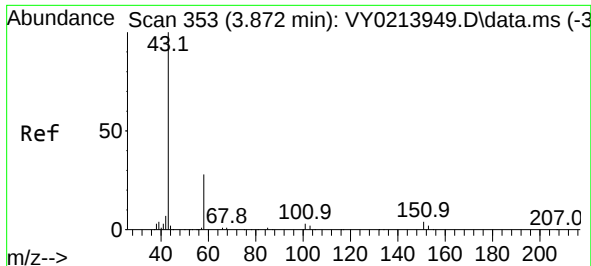

#16
Acetone
Concen: 7.377 ug/l
RT: 3.872 min Scan# 31
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 43 Resp: 567
Ion Ratio Lower Upper
43 100
58 0.0 22.1 33.1#

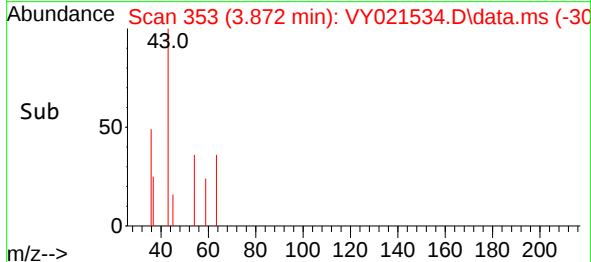

#20
Methylene Chloride
Concen: 1.348 ug/l
RT: 4.598 min Scan# 472
Delta R.T. -0.024 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 84 Resp: 544
Ion Ratio Lower Upper
84 100
49 65.6 102.0 153.0#
51 29.8 33.0 49.6#
86 34.2 50.5 75.7#


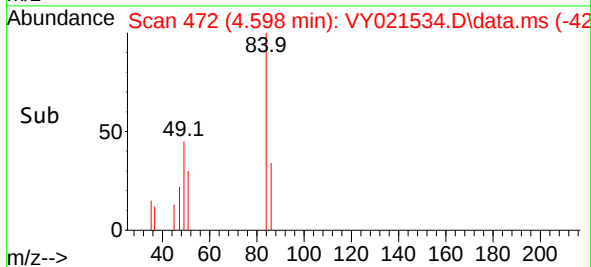

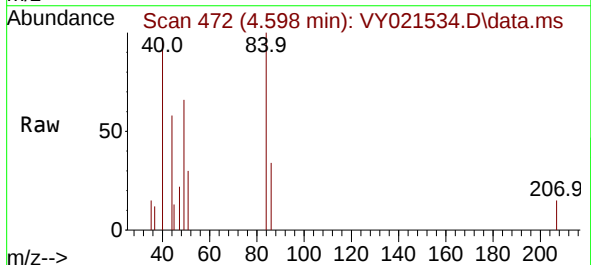


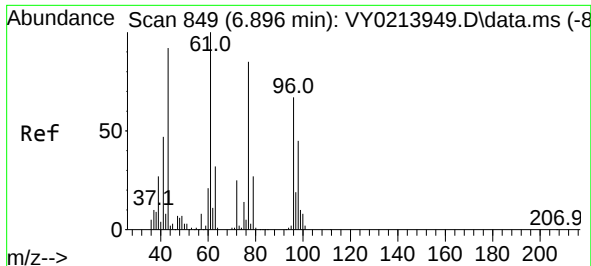

#25
2-Butanone
Concen: 2.144 ug/l
RT: 6.902 min Scan# 849
Delta R.T. 0.006 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 43 Resp: 228
Ion Ratio Lower Upper
43 100
72 0.0 21.4 32.0#

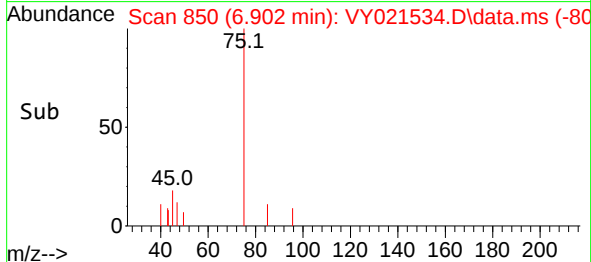

#29
Tetrahydrofuran
Concen: 1.386 ug/l
RT: 7.262 min Scan# 909
Delta R.T. -0.006 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 42 Resp: 91
Ion Ratio Lower Upper
42 100
72 0.0 34.8 52.2#
71 0.0 32.6 48.8#

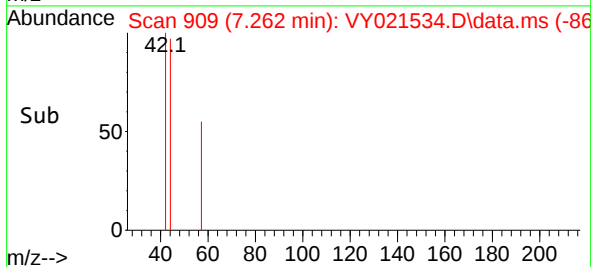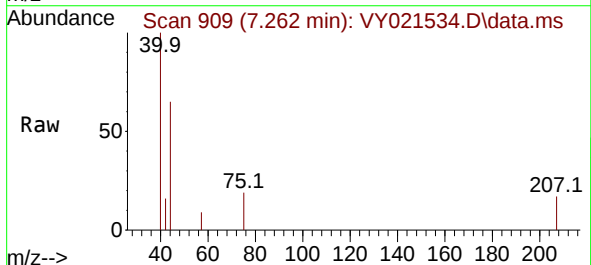



#31

Cyclohexane

Concen: 1.462 ug/l

RT: 7.701 min Scan# 91

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :

RT2321RE





Tgt Ion: 56 Resp: 965

Ion Ratio Lower Upper

56 100

69 142.5 27.0 40.4#

84 81.9 71.1 106.7

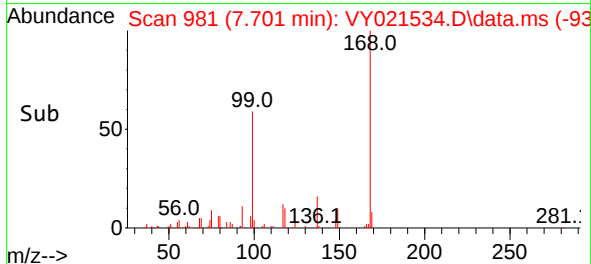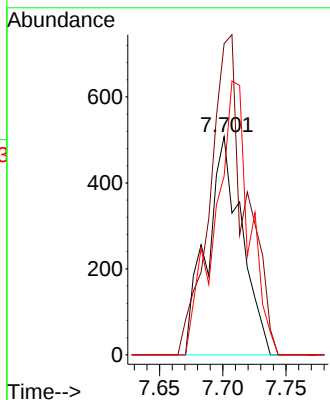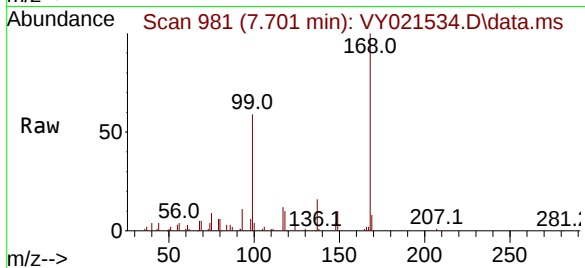

#33

1,2-Dichloroethane-d4

Concen: 47.765 ug/l

RT: 8.061 min Scan# 1040

Delta R.T. -0.006 min

Lab File: VY021534.D




Acq: 14 Mar 2025 12:39


Tgt Ion: 65 Resp: 16832

Ion Ratio Lower Upper

65 100

67 54.2 0.0 102.8

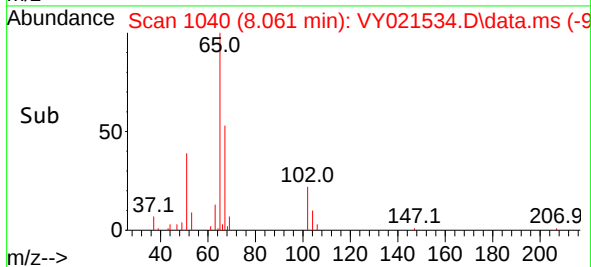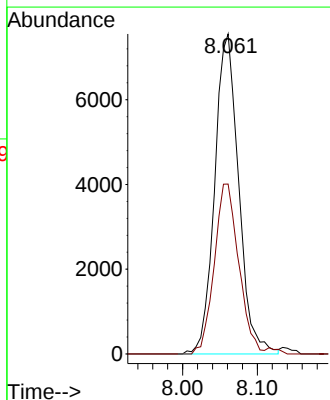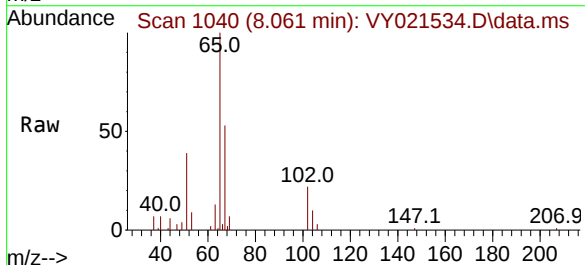

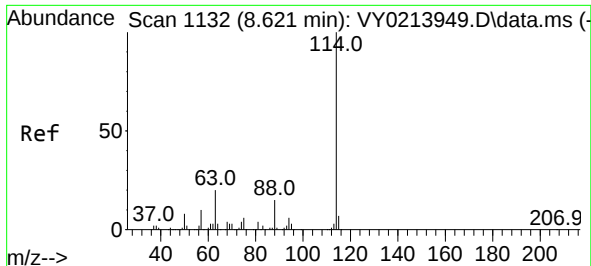

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1132

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :

RT2321RE





Tgt Ion:114 Resp: 49875

Ion Ratio Lower Upper

114 100

63 20.9 0.0 40.8

88 16.7 0.0 30.8

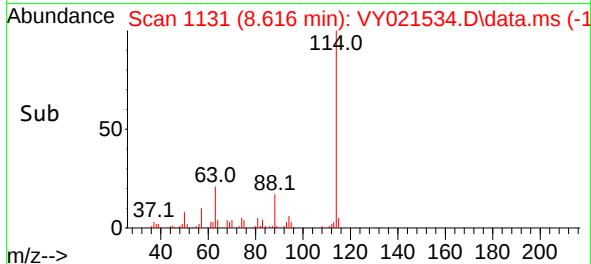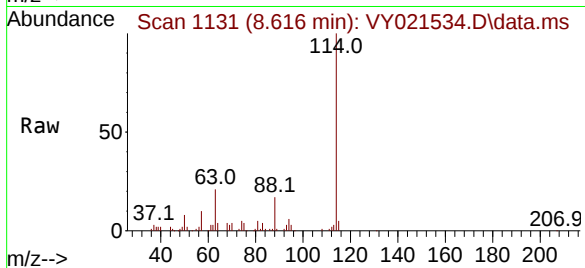

#35

Dibromofluoromethane

Concen: 53.777 ug/l

RT: 7.628 min Scan# 969

Delta R.T. -0.012 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39




Tgt Ion:113 Resp: 17630


Ion Ratio Lower Upper

113 100

111 103.8 82.0 123.0

192 19.1 15.9 23.9

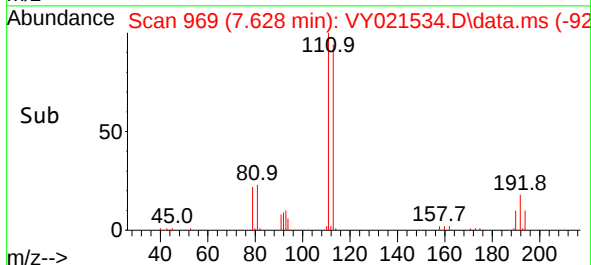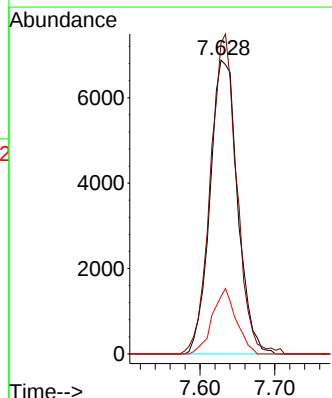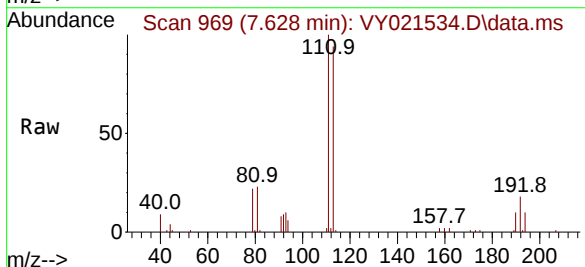



#38

Carbon Tetrachloride

Concen: 6.325 ug/l

RT: 7.707 min Scan# 91

Delta R.T. -0.116 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :

RT2321RE





Tgt Ion:117 Resp: 3733

Ion Ratio Lower Upper

117 100

119 7.2 75.8 113.8#

121 0.0 23.9 35.9#

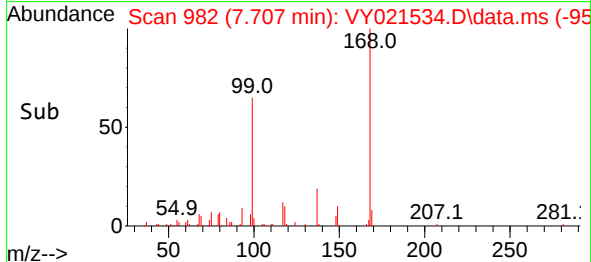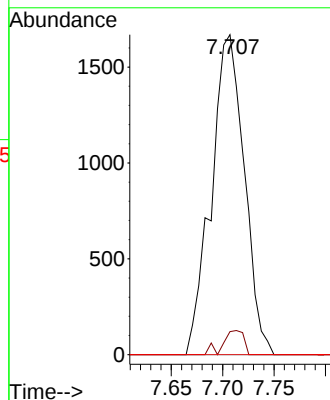

#50

Toluene-d8

Concen: 44.226 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.006 min

Lab File: VY021534.D




Acq: 14 Mar 2025 12:39


Tgt Ion: 98 Resp: 54897

Ion Ratio Lower Upper

98 100

100 63.9 52.1 78.1


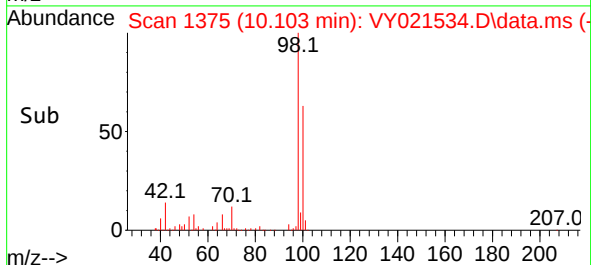
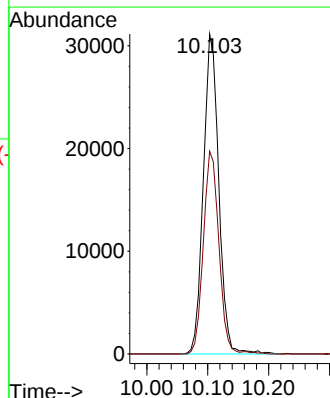
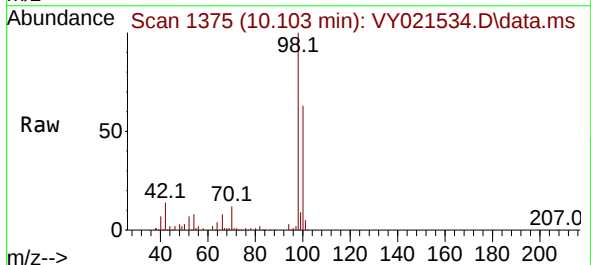




#51
4-Methyl-2-Pentanone
Concen: 1.378 ug/l
RT: 9.999 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 43 Resp: 313
Ion Ratio Lower Upper
43 100
58 16.9 31.4 47.2#

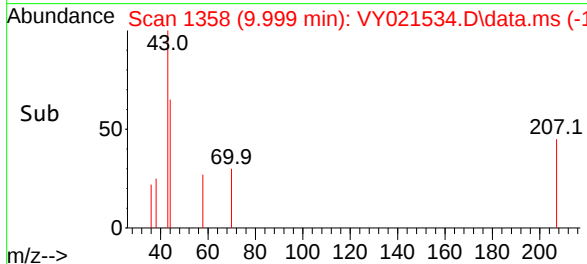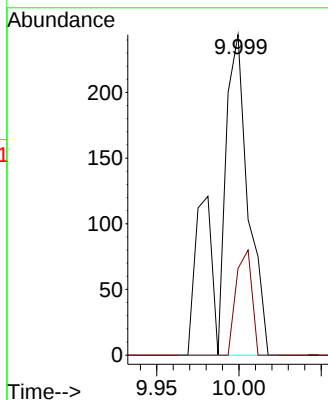

#59
2-Hexanone
Concen: 1.684 ug/l
RT: 10.774 min Scan# 1485
Delta R.T. 0.012 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 43 Resp: 253
Ion Ratio Lower Upper
43 100
58 33.6 27.3 81.8

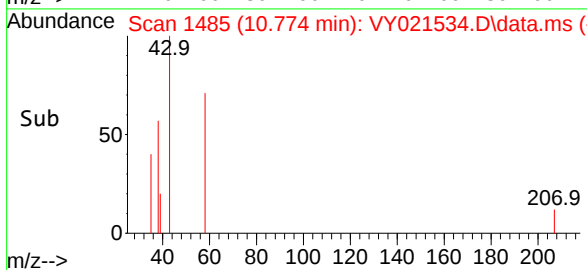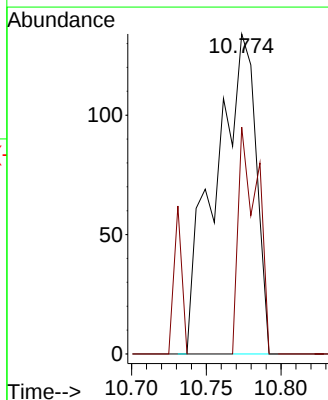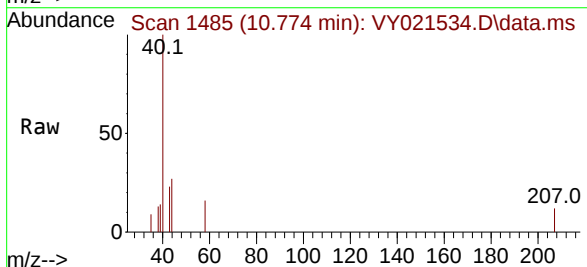

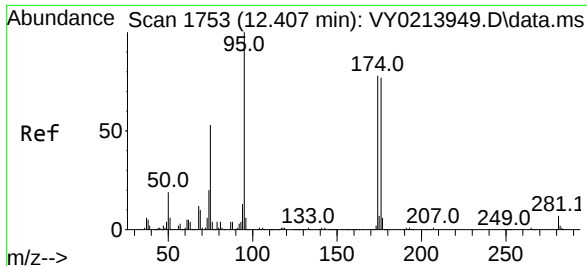

#62

4-Bromofluorobenzene

Concen: 23.368 ug/l

RT: 12.401 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :

RT2321RE





Tgt Ion: 95 Resp: 9867

Ion Ratio Lower Upper

95 100

174 82.3 0.0 165.0

176 82.0 0.0 160.0

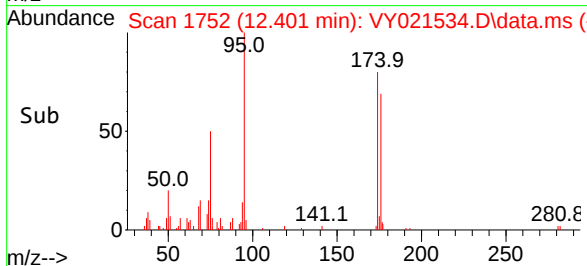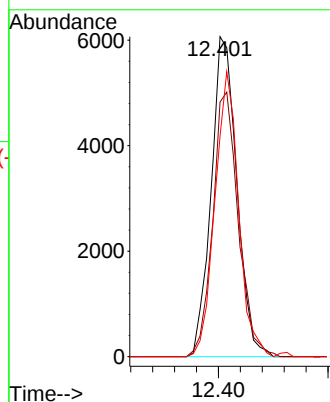

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39




Tgt Ion: 117 Resp: 34521


Ion Ratio Lower Upper

117 100

82 53.8 44.6 67.0

119 29.1 25.4 38.0


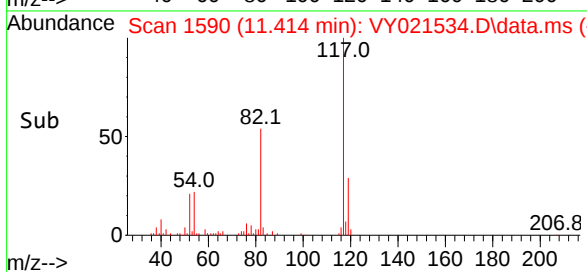
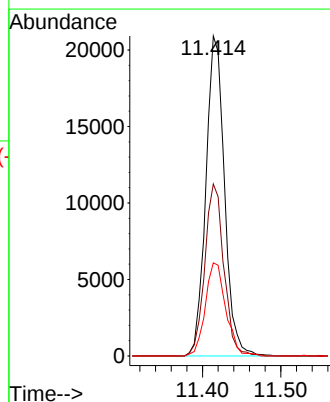
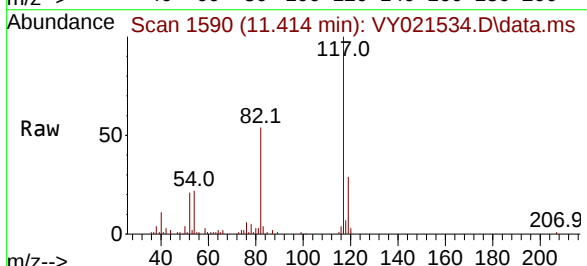


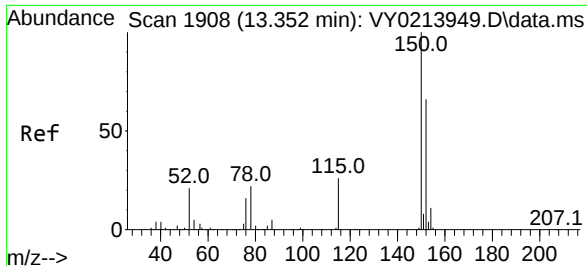

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1908
Delta R.T. -0.006 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion:152 Resp: 6334
Ion Ratio Lower Upper
152 100
115 65.6 29.0 87.0
150 170.2 0.0 347.2

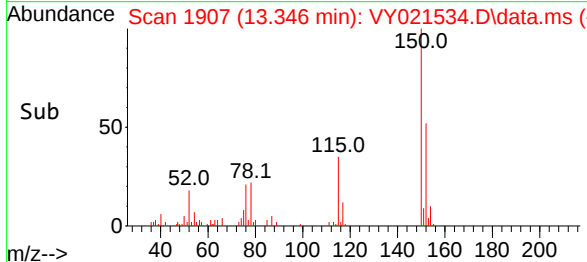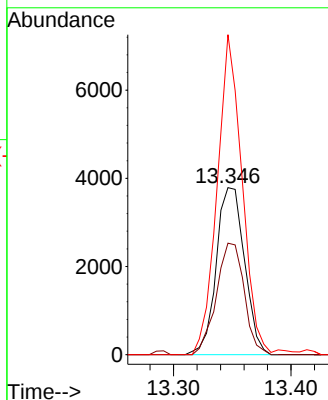

#74
N-ethyl acetate
Concen: 1.753 ug/l
RT: 12.072 min Scan# 1698
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 43 Resp: 190
Ion Ratio Lower Upper
43 100
70 0.0 34.6 51.8#
55 28.9 21.1 31.7
61 28.4 19.4 29.0


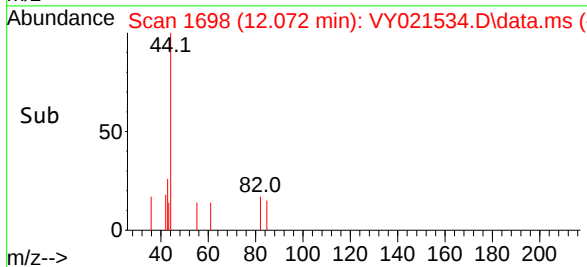
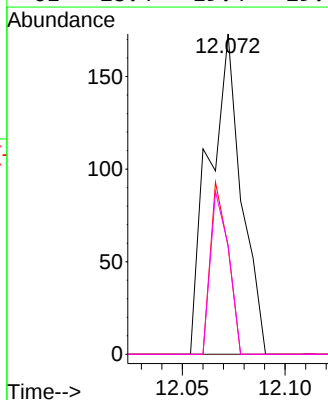
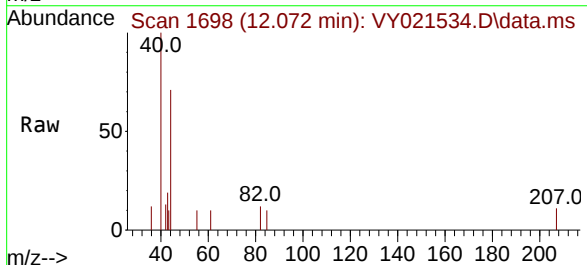


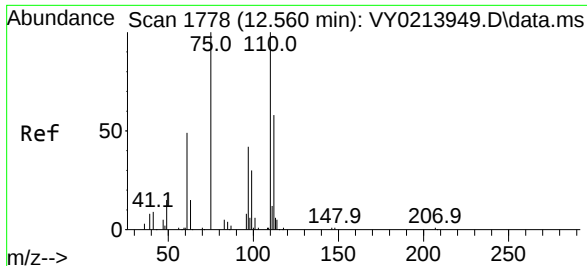

#76
1,2,3-Trichloropropane
Concen: 90.855 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.152 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 75 Resp: 5799
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

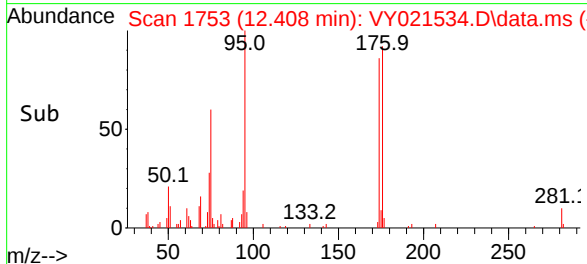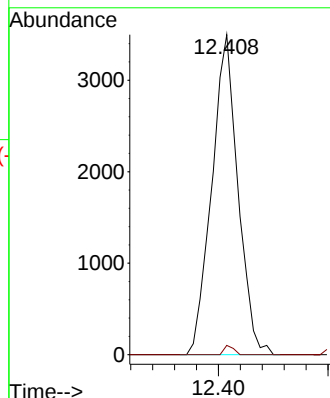

#77
Bromobenzene
Concen: 1.139 ug/l
RT: 12.523 min Scan# 1772
Delta R.T. -0.012 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 156 Resp: 133
Ion Ratio Lower Upper
156 100
77 182.7 93.6 280.8
158 88.7 48.3 144.8


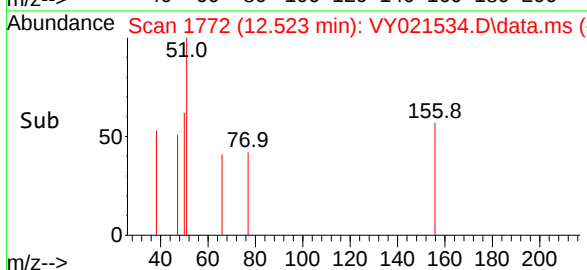
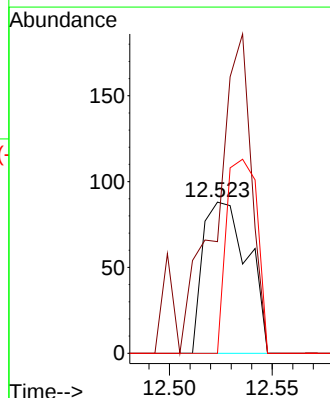
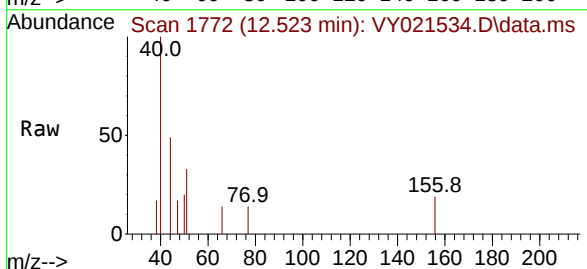


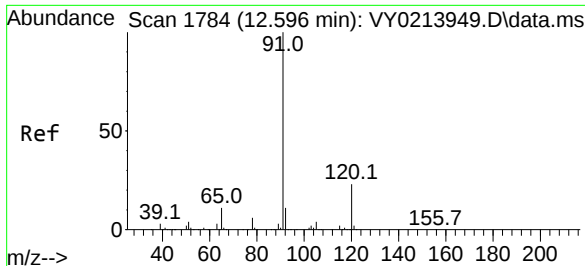

#78
n-propylbenzene
Concen: 1.040 ug/l
RT: 12.597 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 91 Resp: 630
Ion Ratio Lower Upper
91 100
120 8.7 11.3 33.8#

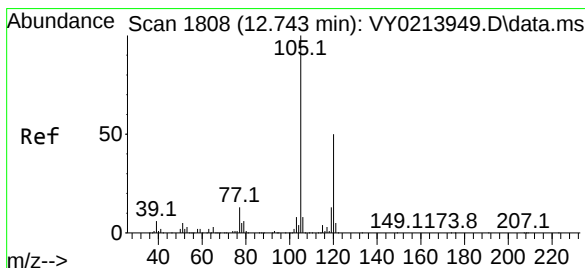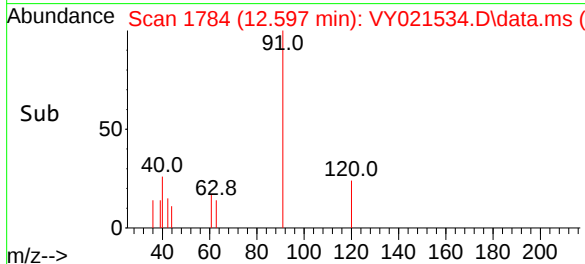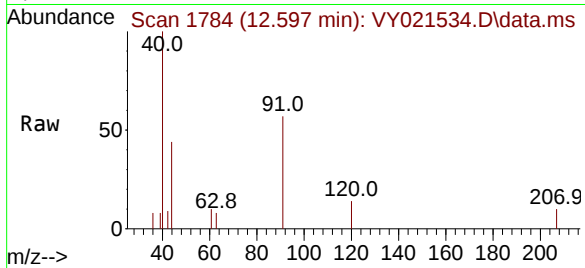

#80
1,3,5-Trimethylbenzene
Concen: 1.026 ug/l
RT: 12.737 min Scan# 1807
Delta R.T. -0.006 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 105 Resp: 416
Ion Ratio Lower Upper
105 100
120 54.1 24.6 73.6


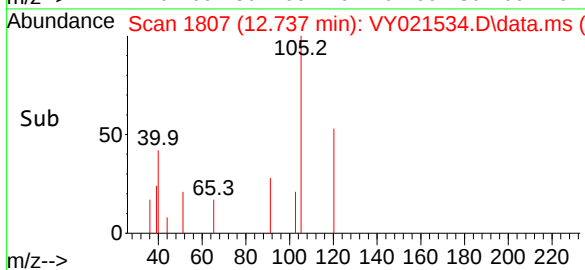

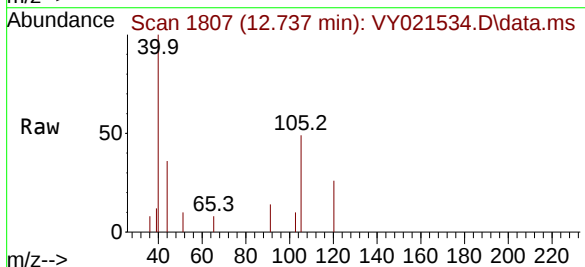


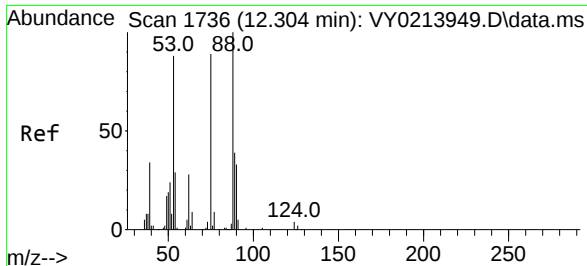

#81
trans-1,4-Dichloro-2-butene
Concen: 206.543 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.104 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39




Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE


Tgt Ion: 75 Resp: 5799
Ion Ratio Lower Upper
75 100
53 0.0 81.0 121.4#
89 0.0 36.9 55.3#

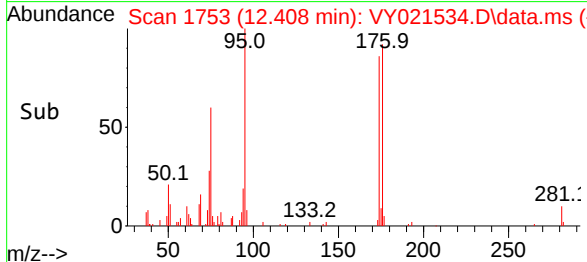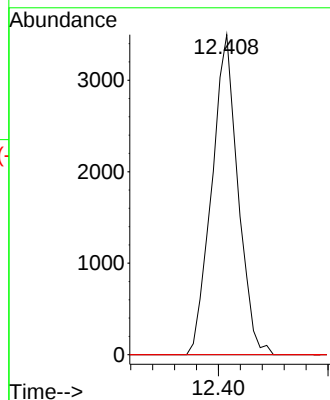

#82
4-Chlorotoluene
Concen: 1.324 ug/l
RT: 12.779 min Scan# 1814
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion: 91 Resp: 475
Ion Ratio Lower Upper
91 100
126 0.0 17.0 51.0#

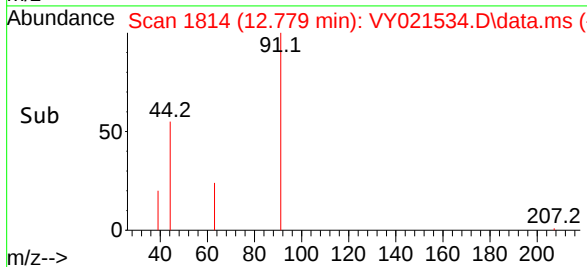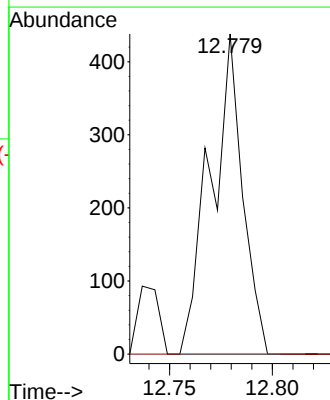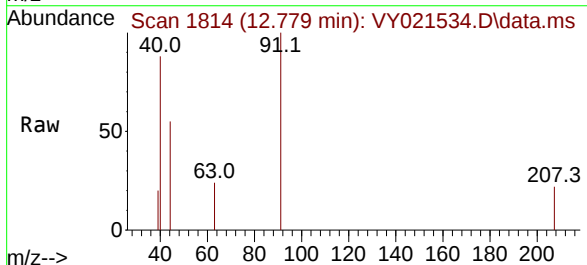

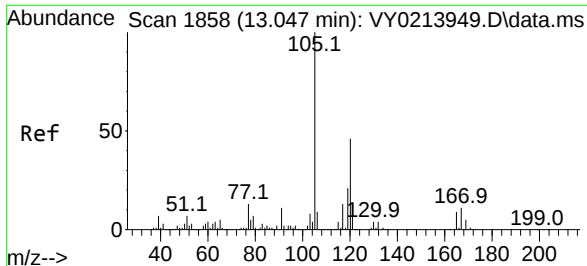

#84

1,2,4-Trimethylbenzene

Concen: 1.513 ug/l

RT: 13.042 min Scan# 1857

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Instrument :

MSVOA_Y

ClientSampleId :





RT2321RE

Tgt Ion:105 Resp: 609

Ion Ratio Lower Upper

105 100

120 51.2 22.7 68.1

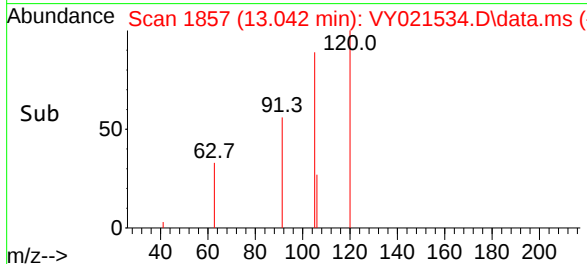

#87

1,3-Dichlorobenzene

Concen: 1.446 ug/l

RT: 13.291 min Scan# 1898

Delta R.T. 0.000 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39




Tgt Ion:146 Resp: 336


Ion Ratio Lower Upper

146 100

111 39.9 20.0 60.0

148 78.3 31.8 95.3

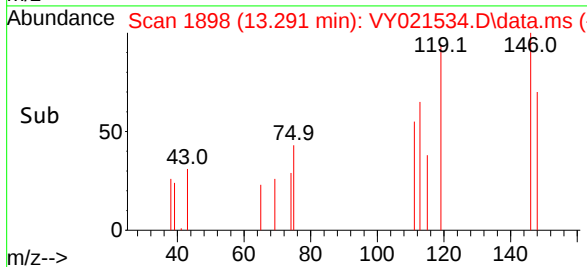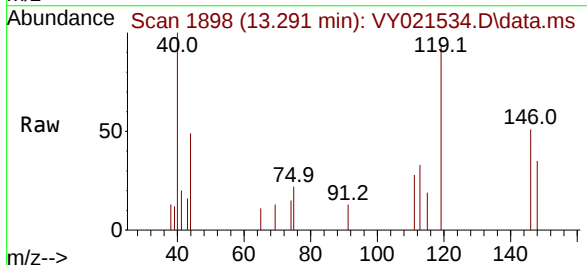

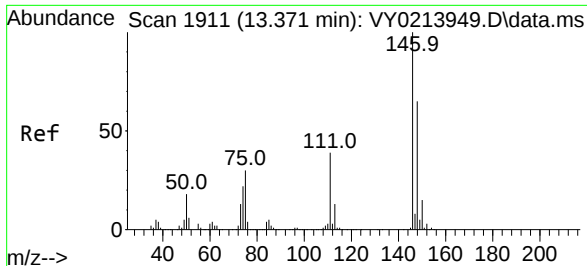

#88

1,4-Dichlorobenzene

Concen: 1.866 ug/l

RT: 13.365 min Scan# 1911

Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39





Instrument :

MSVOA_Y

ClientSampleId :

RT2321RE

Tgt Ion:	146	Resp:	424
Ion	Ratio	Lower	Upper
146	100		
111	34.2	19.6	58.8
148	80.4	32.3	96.8

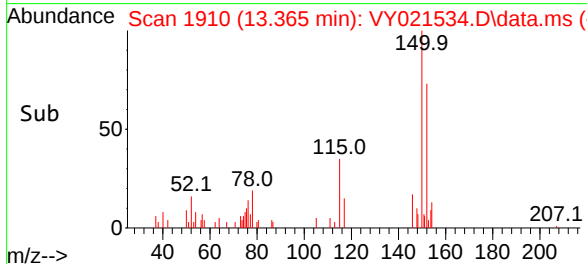

#89

n-Butylbenzene

Concen: 1.319 ug/l




RT: 13.615 min Scan# 1951


Delta R.T. -0.006 min

Lab File: VY021534.D

Acq: 14 Mar 2025 12:39

Tgt Ion:	91	Resp:	540
Ion	Ratio	Lower	Upper
91	100		
92	48.9	26.1	78.3
134	32.6	12.6	37.8


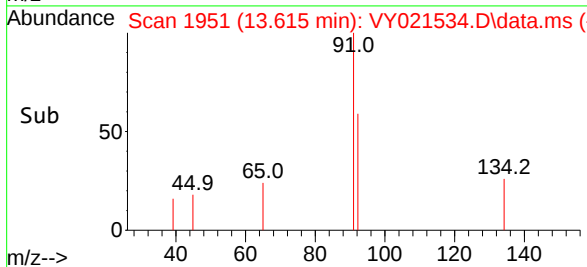

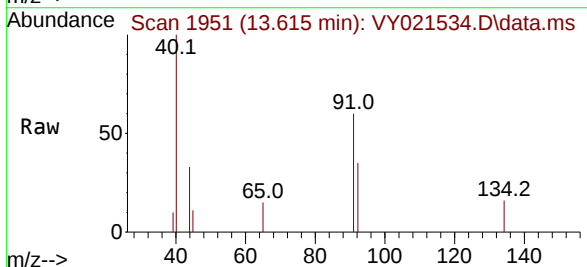




#91
 1,2-Dichlorobenzene
 Concen: 2.119 ug/l
 RT: 13.663 min Scan# 1959
 Delta R.T. 0.000 min
 Lab File: VY021534.D
 Acq: 14 Mar 2025 12:39




Instrument :
 MSVOA_Y
 ClientSampleId :
 RT2321RE


Tgt Ion:146 Resp: 422
 Ion Ratio Lower Upper
 146 100
 111 30.3 20.7 62.1
 148 27.0 32.1 96.5#

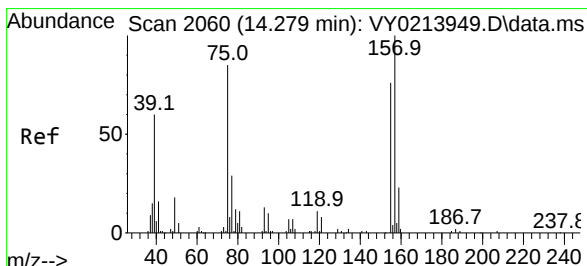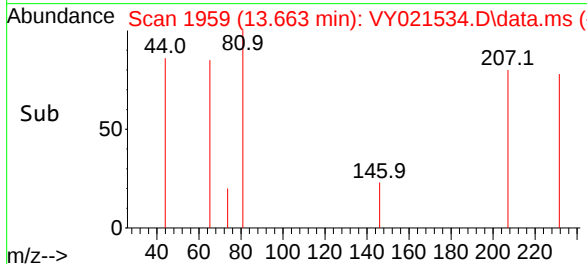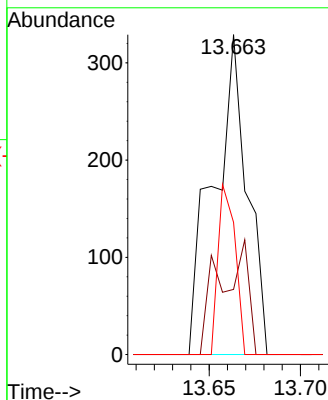

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.668 ug/l
 RT: 14.279 min Scan# 2060
 Delta R.T. 0.000 min
 Lab File: VY021534.D
 Acq: 14 Mar 2025 12:39

Tgt Ion: 75 Resp: 22
 Ion Ratio Lower Upper
 75 100
 155 0.0 43.5 130.5#
 157 104.5 54.4 163.2


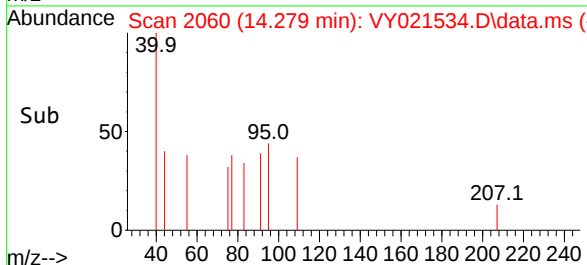
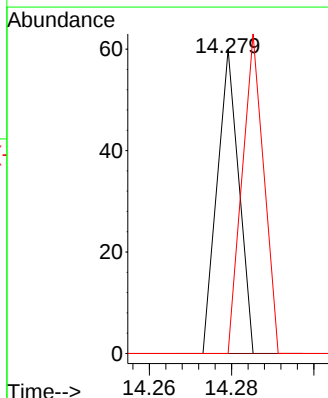
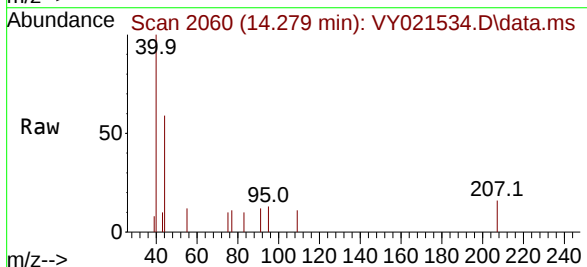




#93
 1,2,4-Trichlorobenzene
 Concen: 3.916 ug/l
 RT: 14.925 min Scan# 2166
 Delta R.T. 0.000 min
 Lab File: VY021534.D
 Acq: 14 Mar 2025 12:39




Instrument :
 MSVOA_Y
 ClientSampleId :
 RT2321RE


Tgt Ion:	180	Resp:	426
Ion	Ratio	Lower	Upper
180	100		
182	85.2	46.7	140.0
145	16.2	15.6	46.8

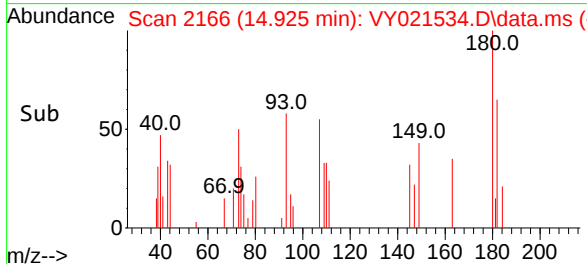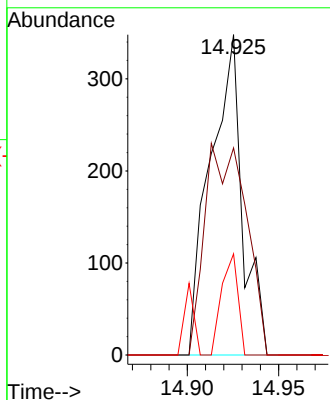

#94
 Hexachlorobutadiene
 Concen: 2.889 ug/l
 RT: 15.029 min Scan# 2183
 Delta R.T. 0.000 min
 Lab File: VY021534.D
 Acq: 14 Mar 2025 12:39

Tgt Ion:	225	Resp:	197
Ion	Ratio	Lower	Upper
225	100		
223	0.0	31.4	94.2#
227	56.9	31.8	95.4


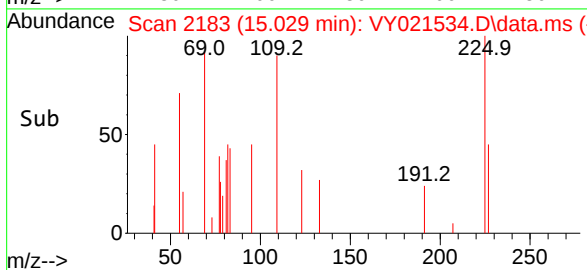
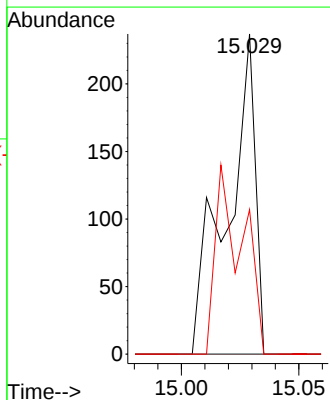
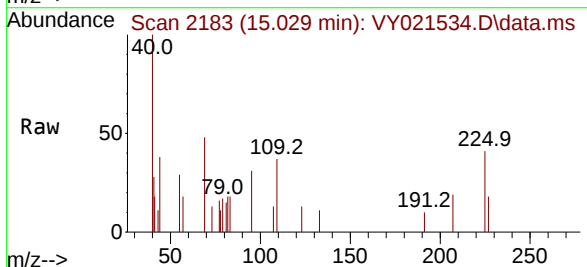


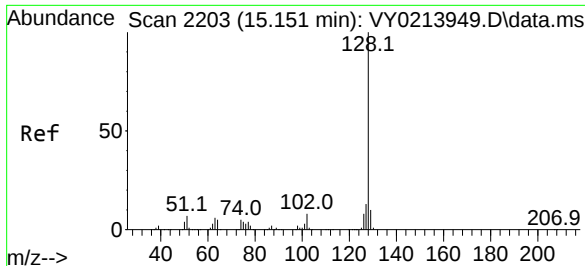

#95
Naphthalene
Concen: 6.248 ug/l
RT: 15.151 min Scan# 2111
Delta R.T. -0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Instrument :
MSVOA_Y
ClientSampleId :
RT2321RE

Tgt Ion:128 Resp: 831
Ion Ratio Lower Upper
128 100
127 10.0 10.6 15.8#
129 7.8 8.6 13.0#

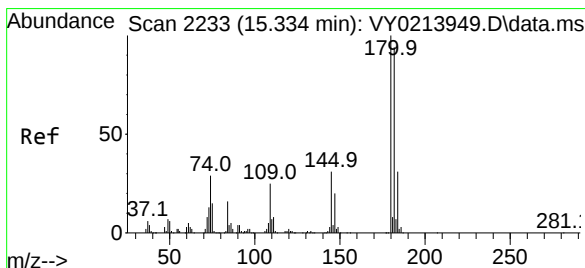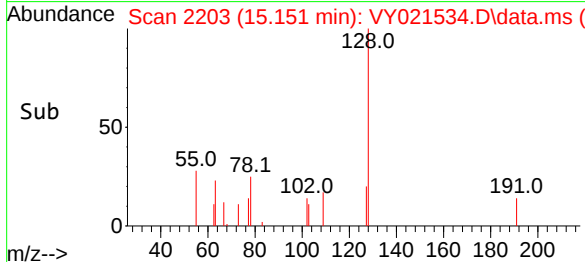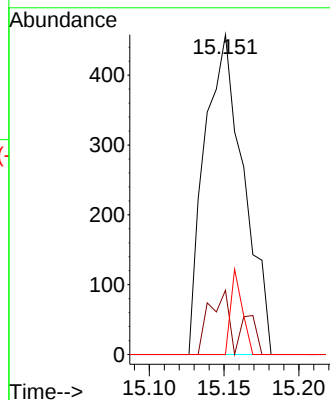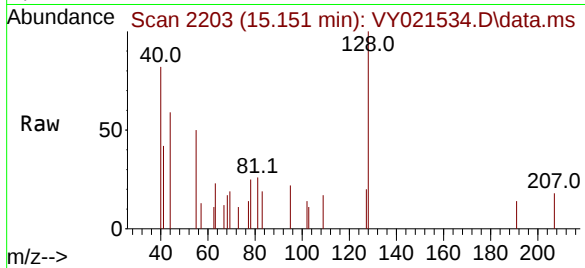

#96
1,2,3-Trichlorobenzene
Concen: 5.356 ug/l
RT: 15.334 min Scan# 2233
Delta R.T. 0.000 min
Lab File: VY021534.D
Acq: 14 Mar 2025 12:39

Tgt Ion:180 Resp: 490
Ion Ratio Lower Upper
180 100
182 67.6 47.2 141.6
145 49.8 16.4 49.1#

