

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
 Data File : VY007903.D
 Acq On : 18 Mar 2022 15:34
 Operator : SY/MD
 Sample : N1948-01
 Misc : 5.54g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 COMP-4

Quant Time: Mar 19 01:36:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 13:55:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	286301	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	520339	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	477951	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	207662	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	174486	53.452	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.900%
35) Dibromofluoromethane	7.716	113	162570	44.487	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	88.980%
50) Toluene-d8	10.179	98	622018	57.224	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	114.440%
62) 4-Bromofluorobenzene	12.483	95	220825	42.105	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	84.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
Data File : VY007903.D
Acq On : 18 Mar 2022 15:34
Operator : SY/MD
Sample : N1948-01
Misc : 5.54g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
COMP-4

Quant Time: Mar 19 01:36:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 13:55:34 2022
Response via : Initial Calibration




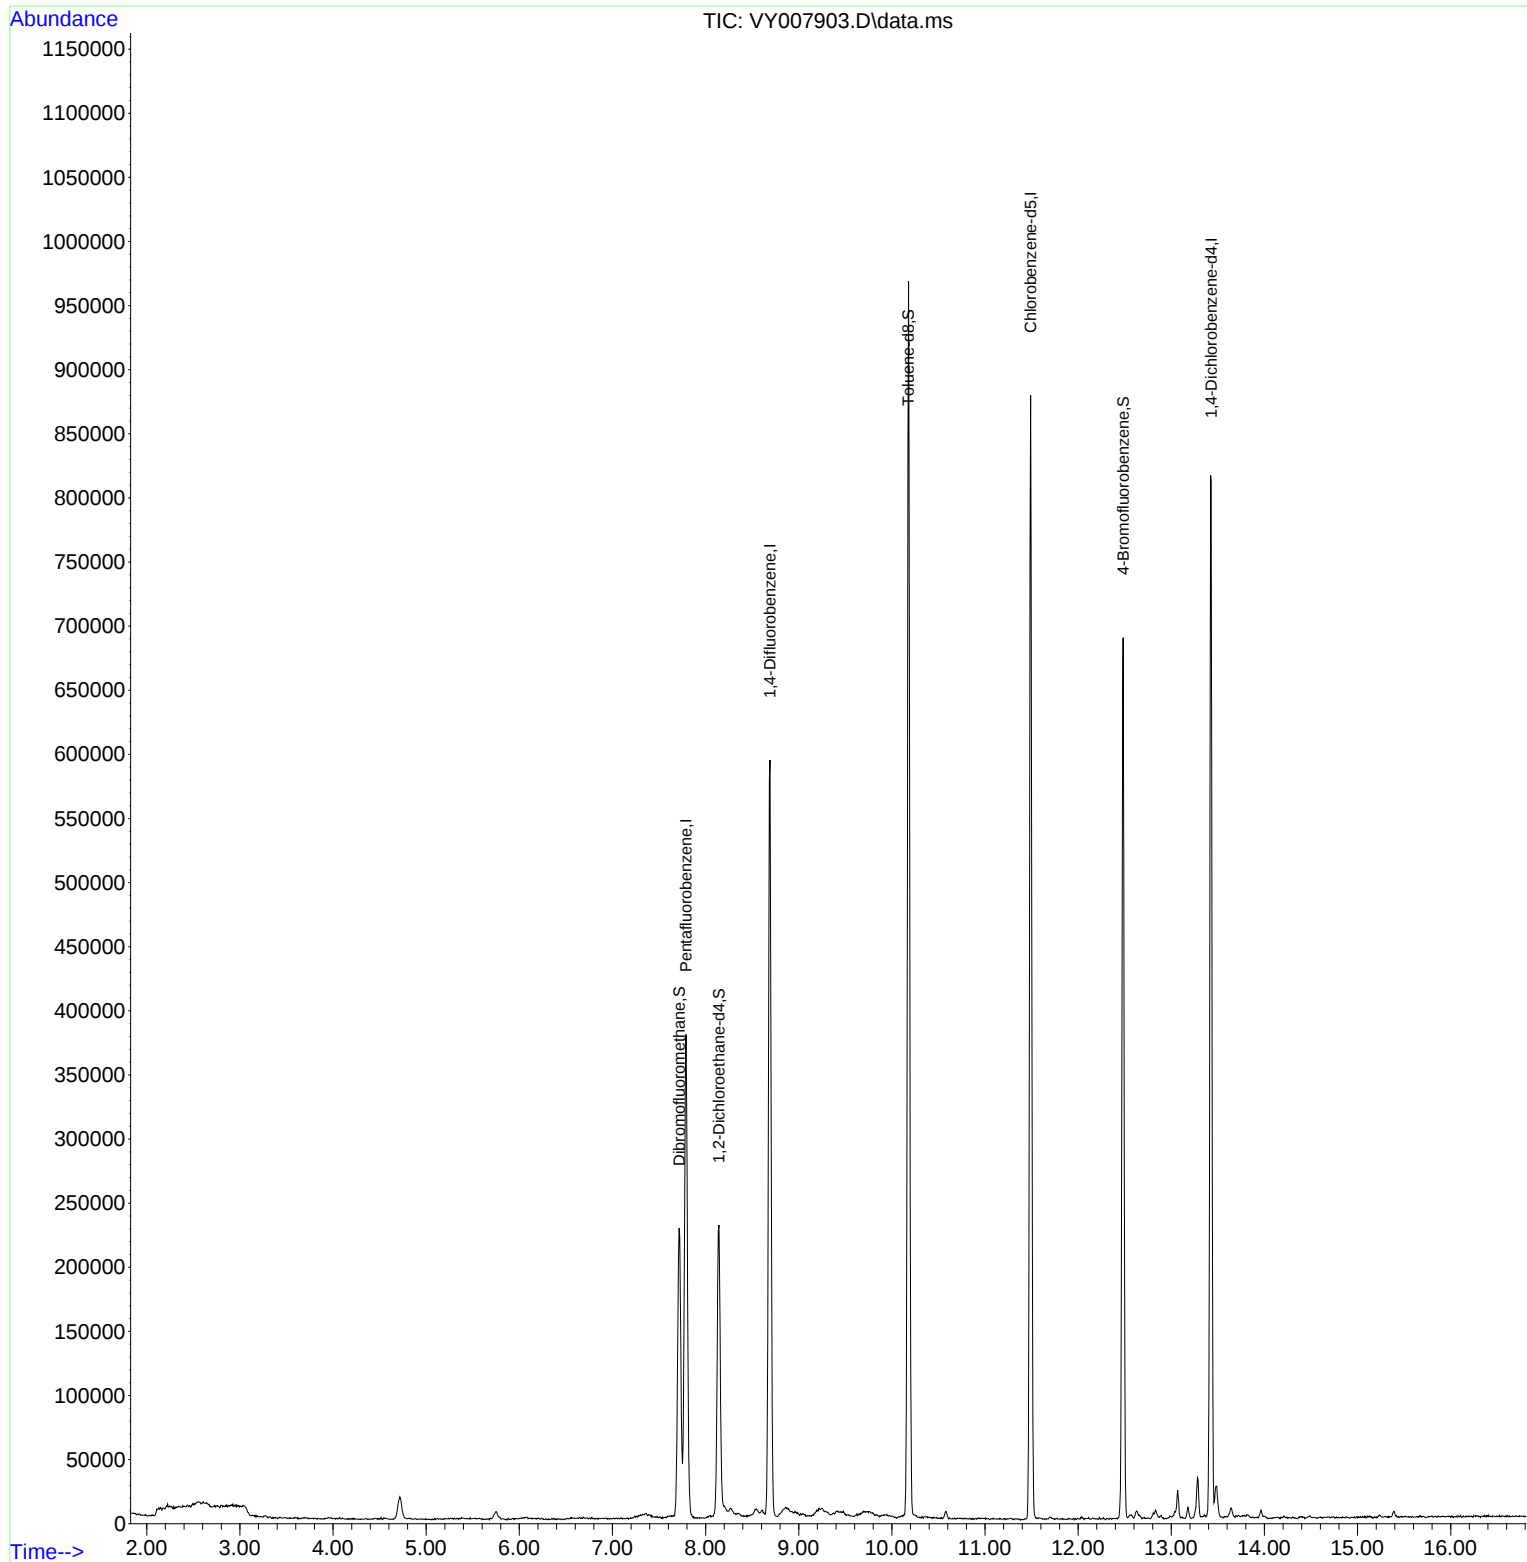


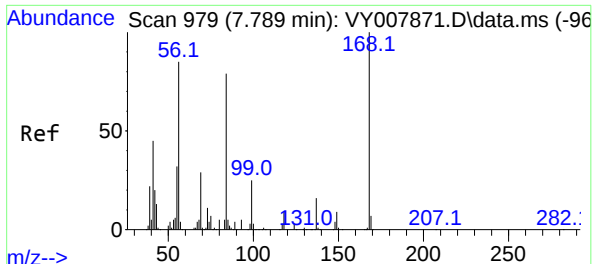

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34




Instrument :
MSVOA_Y
ClientSampleId :
COMP-4


Tgt Ion:168 Resp: 286301
Ion Ratio Lower Upper
168 100
99 60.5 46.9 70.3

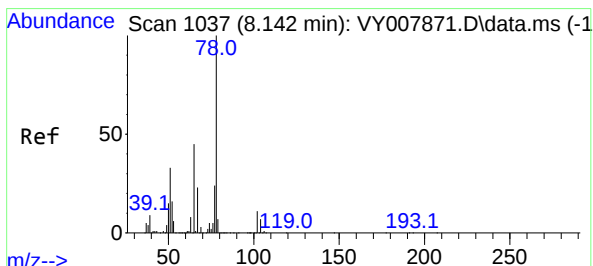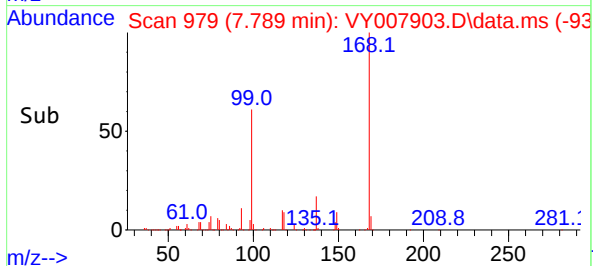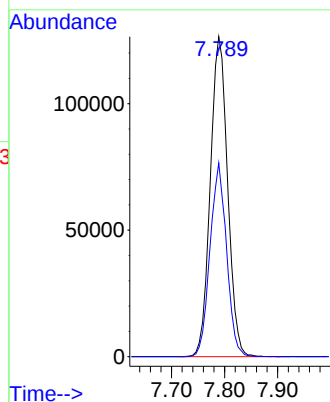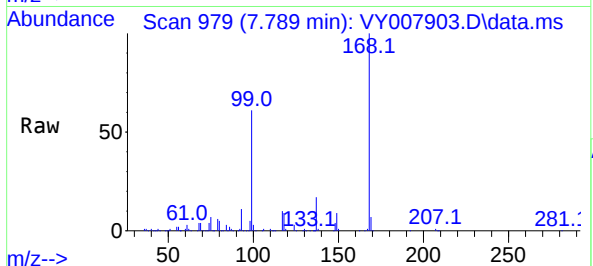

#33
1,2-Dichloroethane-d4
Concen: 53.452 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34

Tgt Ion: 65 Resp: 174486
Ion Ratio Lower Upper
65 100
67 54.2 0.0 99.4


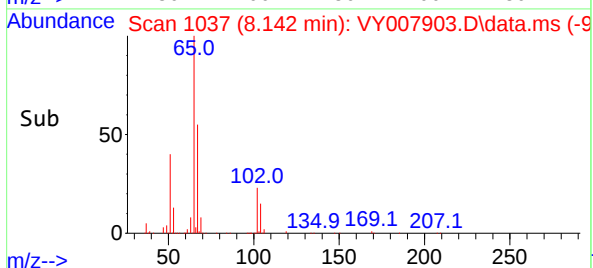
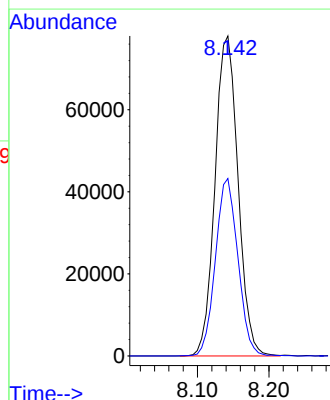
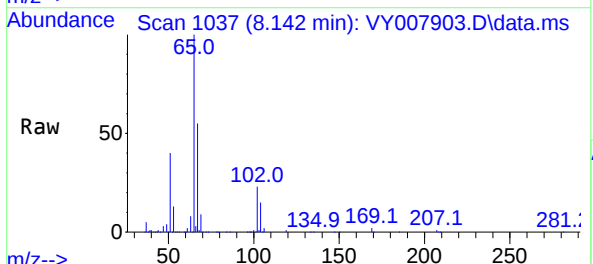


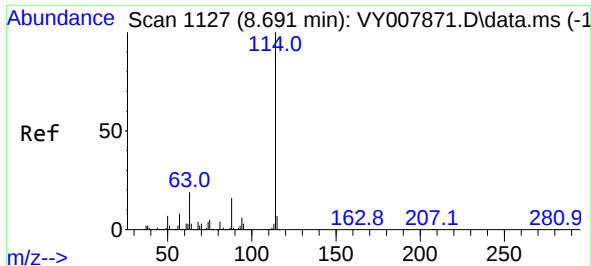

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34




Instrument :
MSVOA_Y
ClientSampleId :
COMP-4


Tgt Ion:114 Resp: 520339
Ion Ratio Lower Upper
114 100
63 18.8 0.0 43.2
88 14.7 0.0 31.8

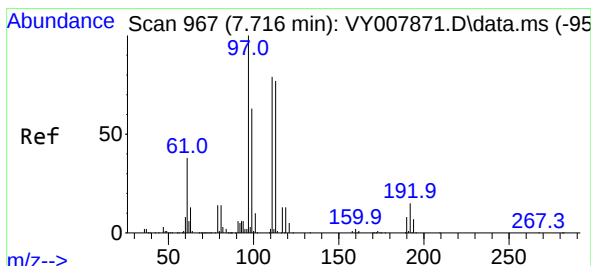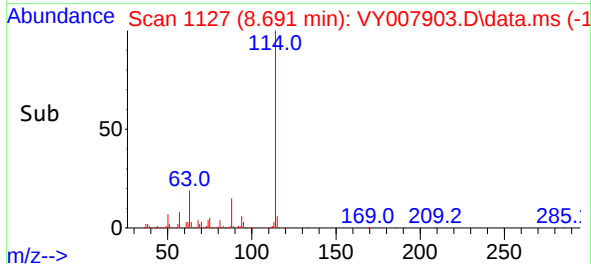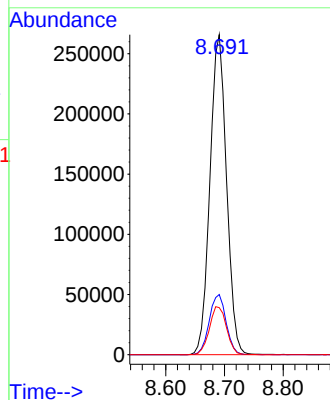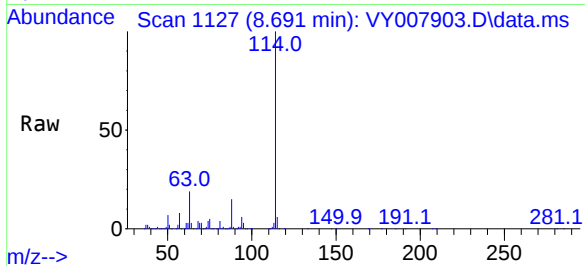

#35
Dibromofluoromethane
Concen: 44.487 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34

Tgt Ion:113 Resp: 162570
Ion Ratio Lower Upper
113 100
111 103.1 82.6 124.0
192 17.7 17.6 26.4


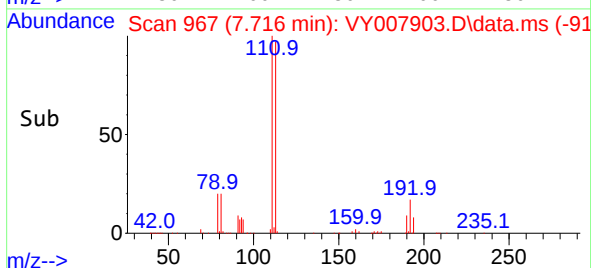
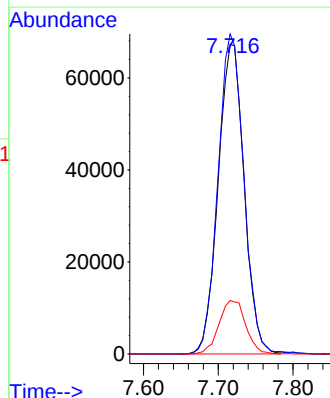
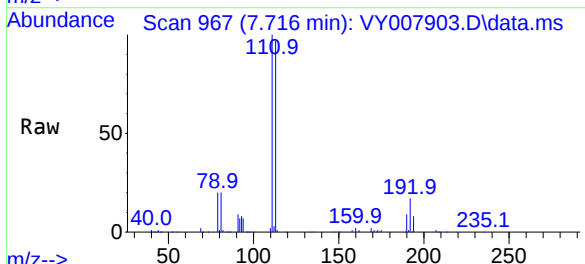


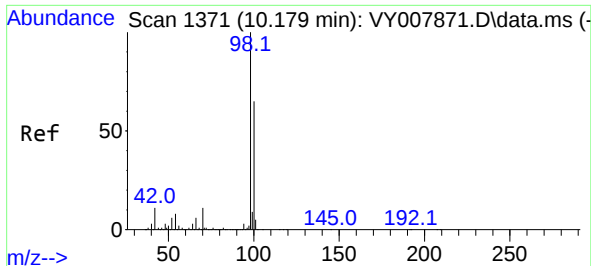

#50
Toluene-d8
Concen: 57.224 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34




Instrument :
MSVOA_Y
ClientSampleId :
COMP-4


Tgt Ion: 98 Resp: 622018
Ion Ratio Lower Upper
98 100
100 65.8 50.2 75.2

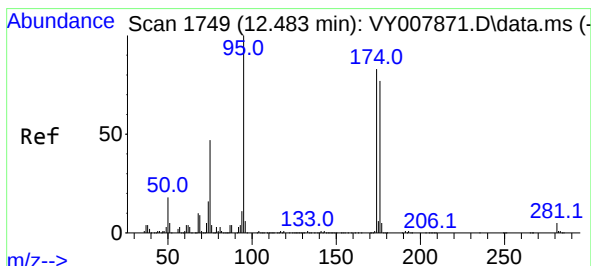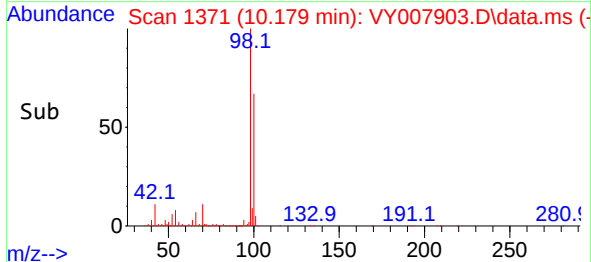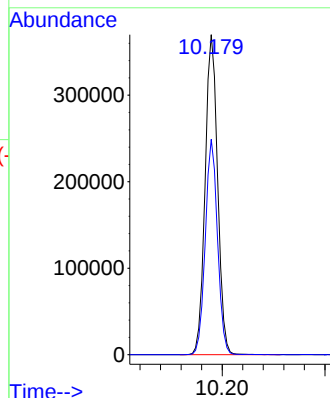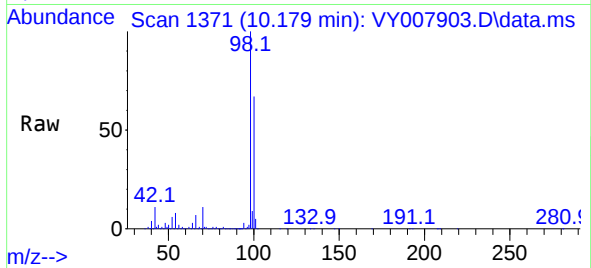

#62
4-Bromofluorobenzene
Concen: 42.105 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34

Tgt Ion: 95 Resp: 220825
Ion Ratio Lower Upper
95 100
174 75.6 0.0 177.0
176 72.4 0.0 175.8


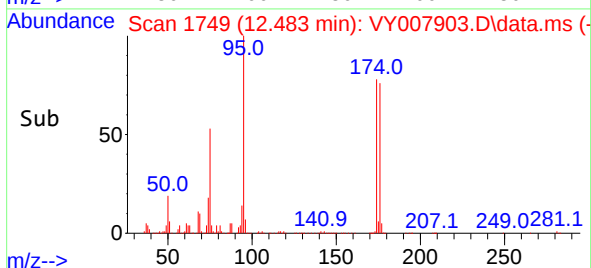
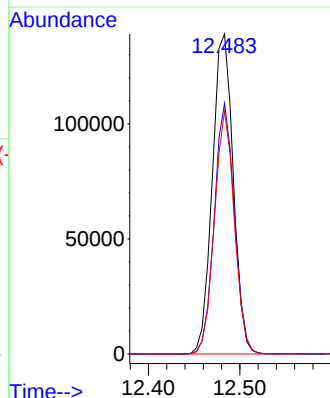
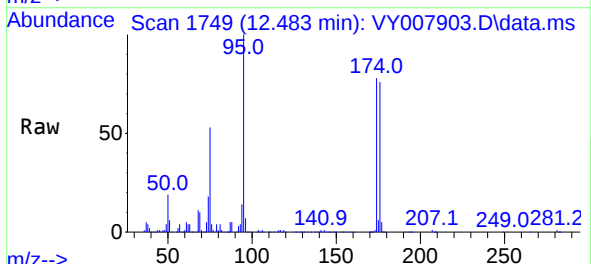


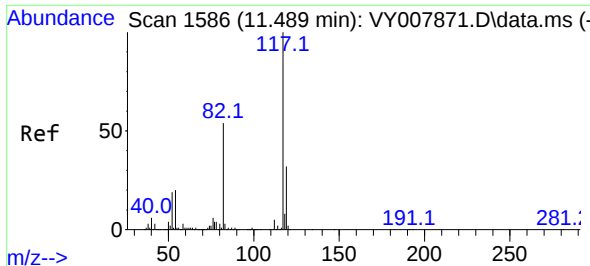

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34

Instrument :
MSVOA_Y
ClientSampleId :
COMP-4

Tgt Ion:117 Resp: 477951
Ion Ratio Lower Upper
117 100
82 54.4 43.0 64.4
119 31.8 25.4 38.0

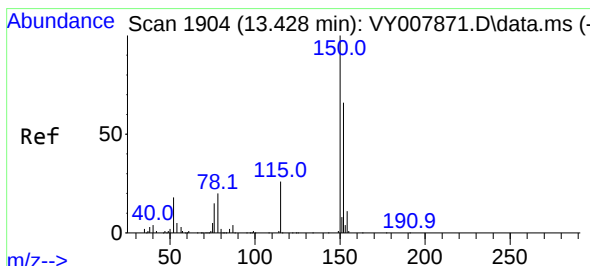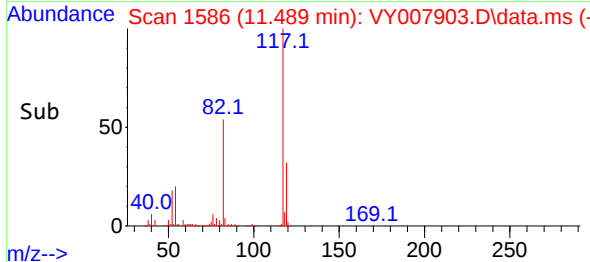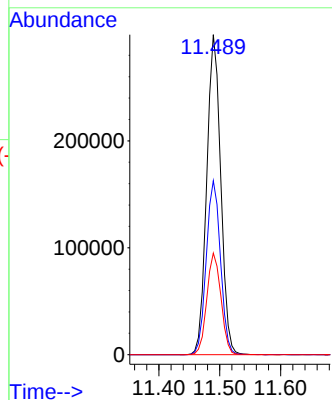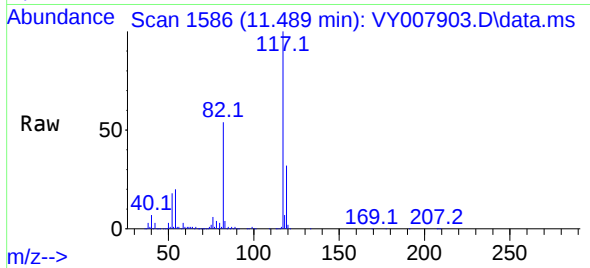

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY007903.D
Acq: 18 Mar 2022 15:34

Tgt Ion:152 Resp: 207662
Ion Ratio Lower Upper
152 100
115 61.3 28.2 84.7
150 158.7 0.0 347.6

