

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
 Data File : VY007932.D
 Acq On : 19 Mar 2022 04:23
 Operator : SY/MD
 Sample : N1958-12
 Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 C-12-11-12

Quant Time: Mar 21 03:20:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 13:55:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	245594	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	458001	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	424260	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	184353	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	160952	57.478	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.960%
35) Dibromofluoromethane	7.716	113	144236	44.842	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	89.680%
50) Toluene-d8	10.179	98	566765	59.465	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	118.920%
62) 4-Bromofluorobenzene	12.483	95	200460	43.424	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.840%
Target Compounds						
16) Acetone	3.942	43	27743	37.346	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
Data File : VY007932.D
Acq On : 19 Mar 2022 04:23
Operator : SY/MD
Sample : N1958-12
Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
C-12-11-12

Quant Time: Mar 21 03:20:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 13:55:34 2022
Response via : Initial Calibration




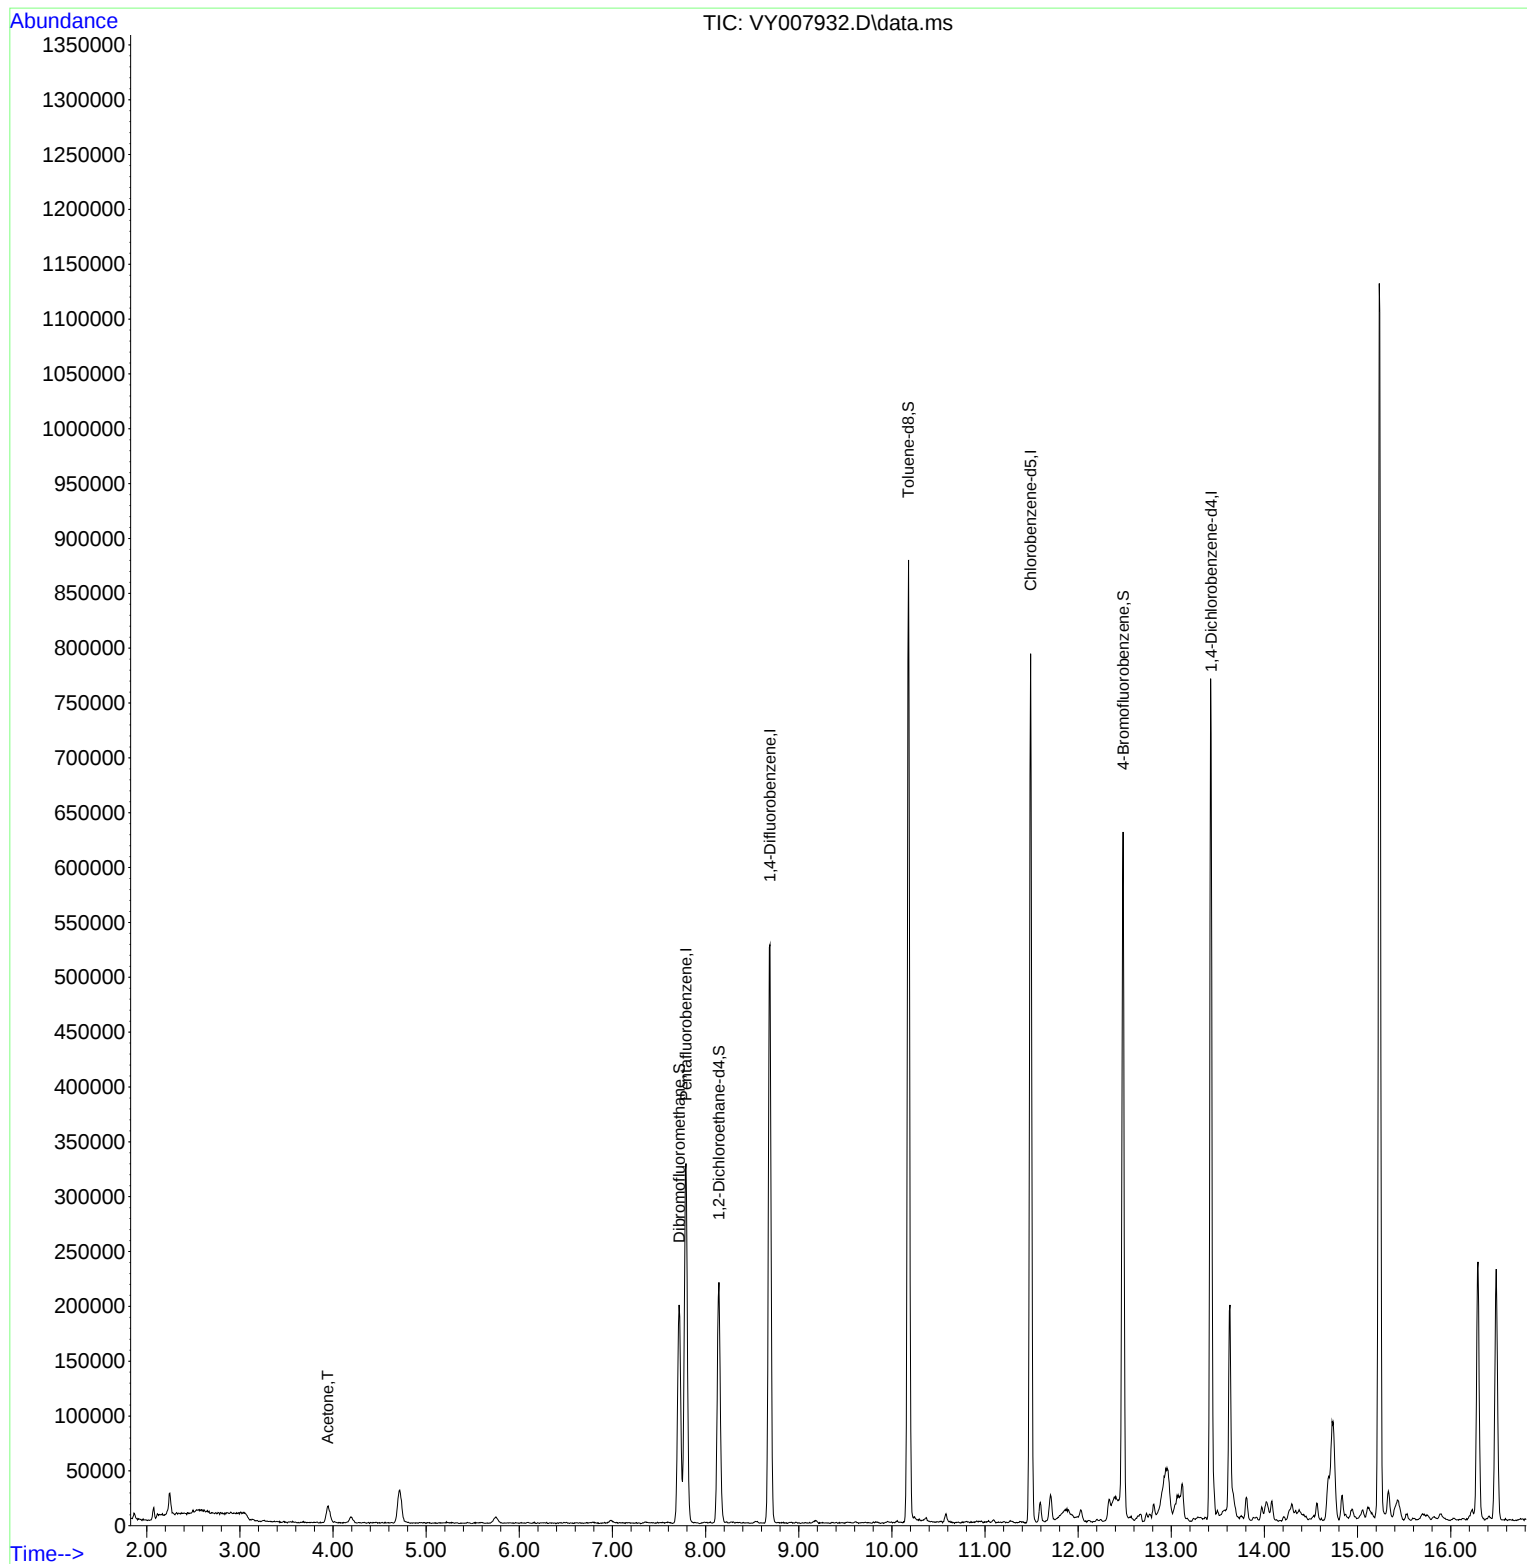


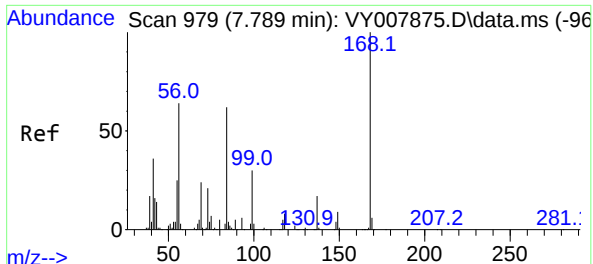

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23




Instrument :
MSVOA_Y
ClientSampleId :
C-12-11-12


Tgt Ion:168 Resp: 245594
Ion Ratio Lower Upper
168 100
99 60.1 46.9 70.3

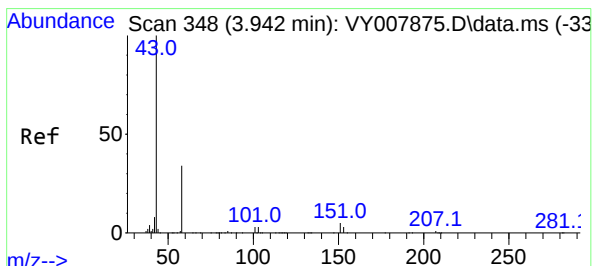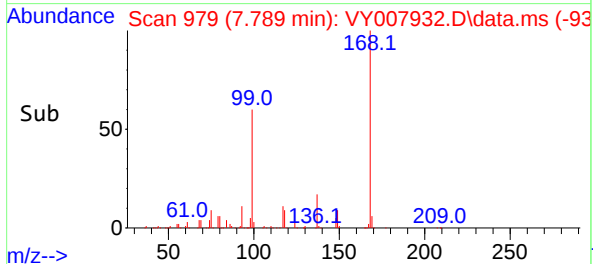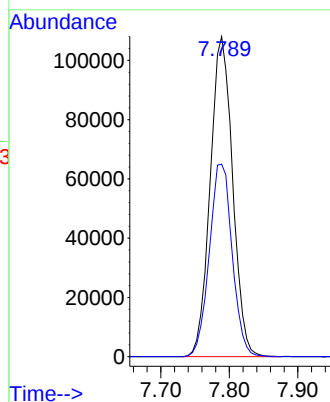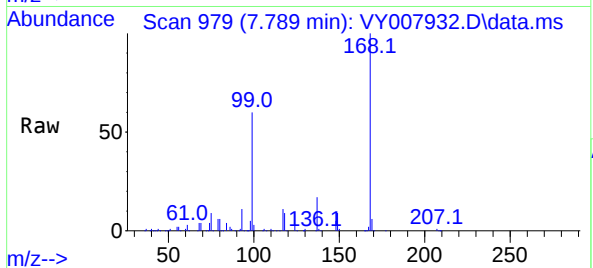

#16
Acetone
Concen: 37.346 ug/l
RT: 3.942 min Scan# 348
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23

Tgt Ion: 43 Resp: 27743
Ion Ratio Lower Upper
43 100
58 29.3 22.0 33.0


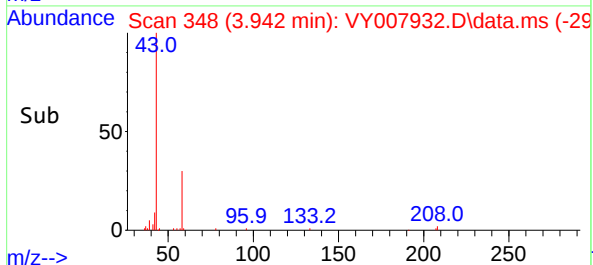
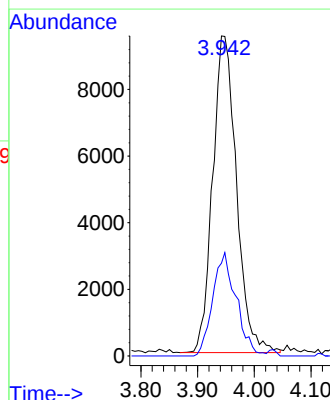
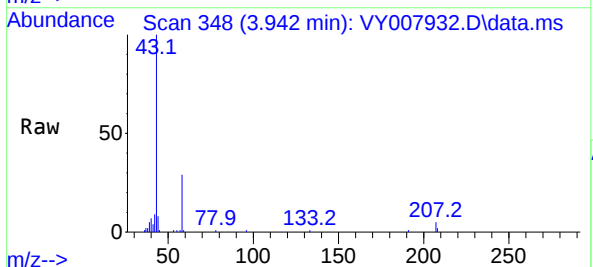


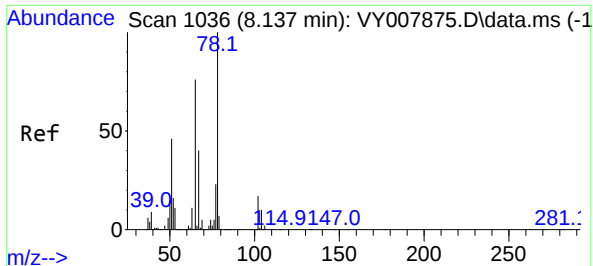

#33
1,2-Dichloroethane-d4
Concen: 57.478 ug/l
RT: 8.142 min Scan# 1036
Delta R.T. 0.006 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23




Instrument :
MSVOA_Y
ClientSampleId :
C-12-11-12


Tgt Ion: 65 Resp: 160952
Ion Ratio Lower Upper
65 100
67 53.5 0.0 99.4

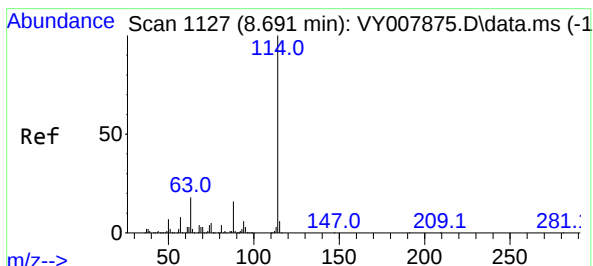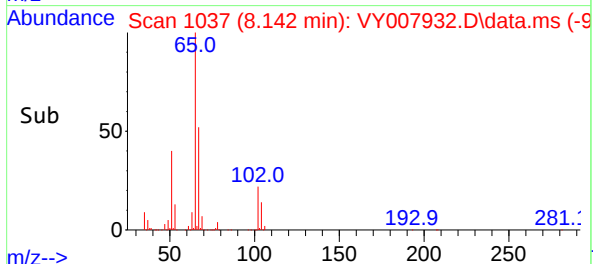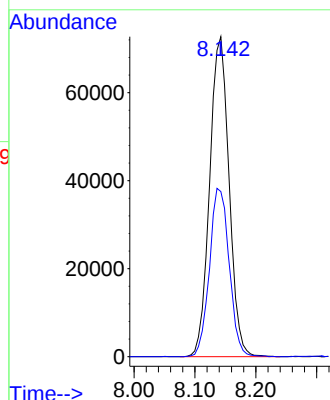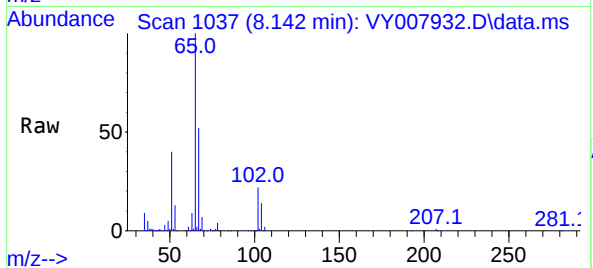

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23

Tgt Ion:114 Resp: 458001
Ion Ratio Lower Upper
114 100
63 19.5 0.0 43.2
88 16.0 0.0 31.8


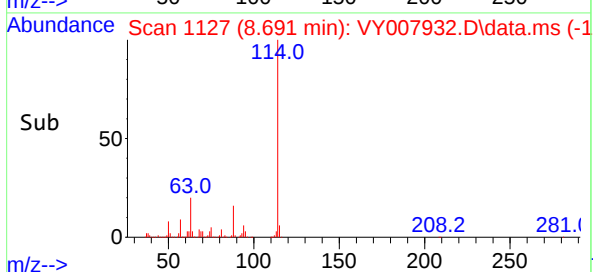
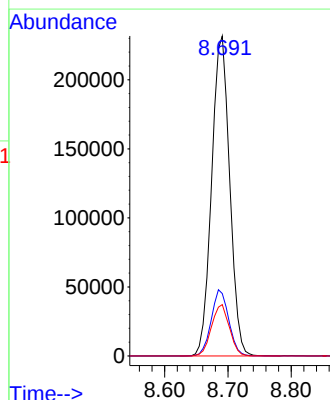
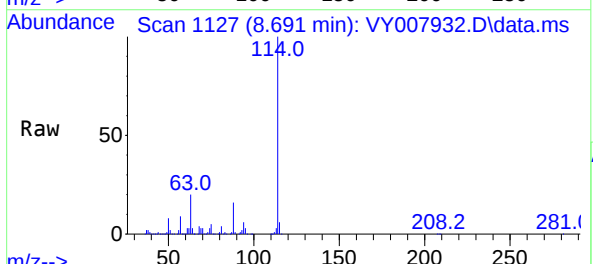


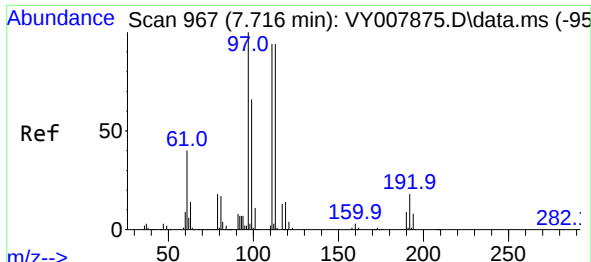

#35
Dibromofluoromethane
Concen: 44.842 ug/l
RT: 7.716 min Scan# 90
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23




Instrument :
MSVOA_Y
ClientSampleId :
C-12-11-12


Tgt Ion:113 Resp: 144236
Ion Ratio Lower Upper
113 100
111 104.3 82.6 124.0
192 16.9 17.6 26.4#

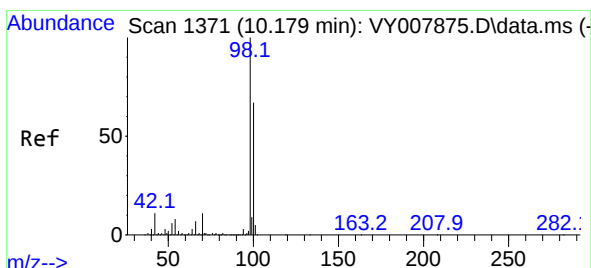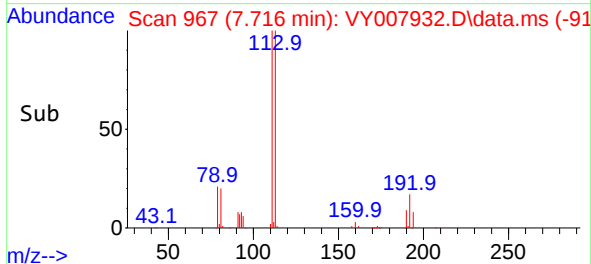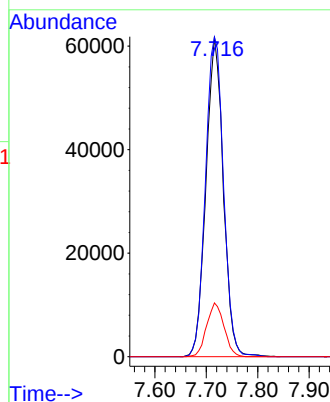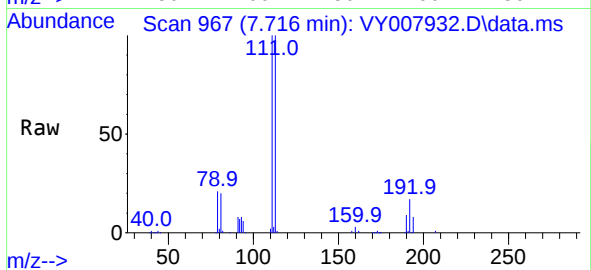

#50
Toluene-d8
Concen: 59.465 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23

Tgt Ion: 98 Resp: 566765
Ion Ratio Lower Upper
98 100
100 65.5 50.2 75.2


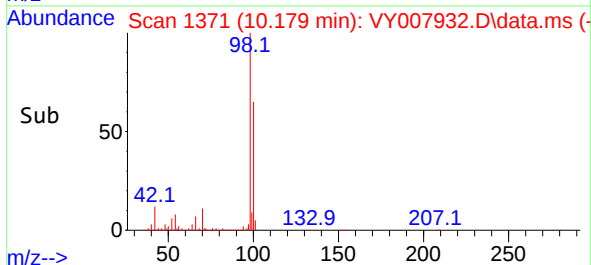
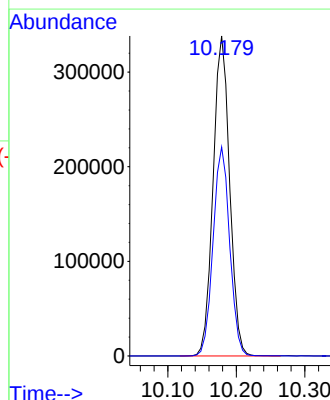
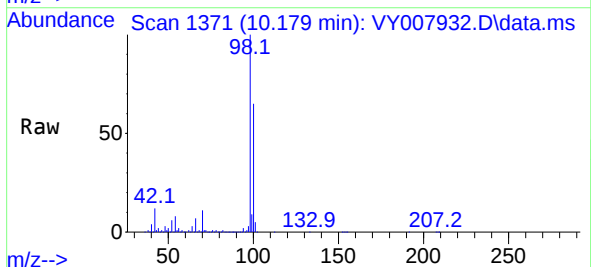


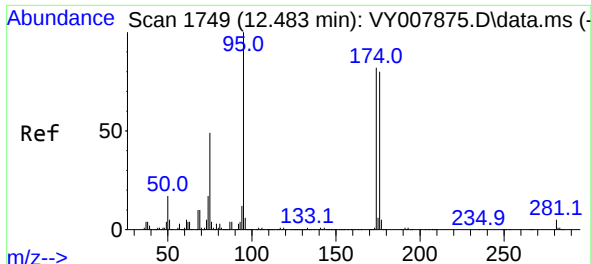

#62
4-Bromofluorobenzene
Concen: 43.424 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23




Instrument :
MSVOA_Y
ClientSampleId :
C-12-11-12


Tgt Ion: 95 Resp: 200460
Ion Ratio Lower Upper
95 100
174 72.4 0.0 177.0
176 69.7 0.0 175.8

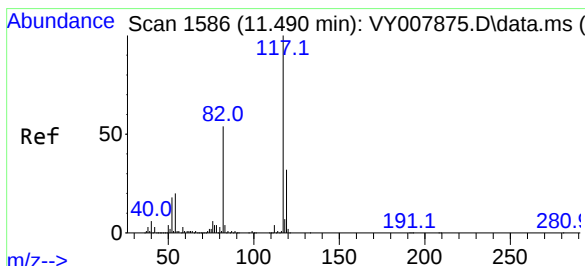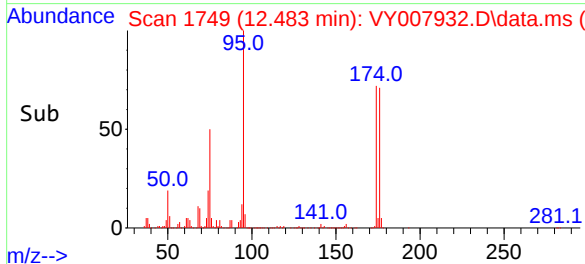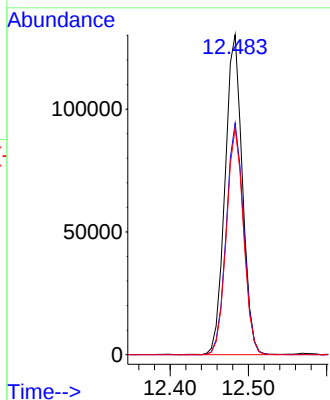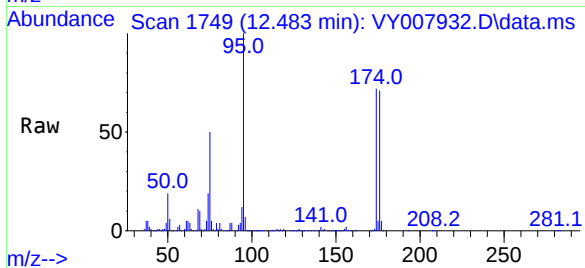

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY007932.D
Acq: 19 Mar 2022 04:23

Tgt Ion: 117 Resp: 424260
Ion Ratio Lower Upper
117 100
82 55.9 43.0 64.4
119 32.4 25.4 38.0

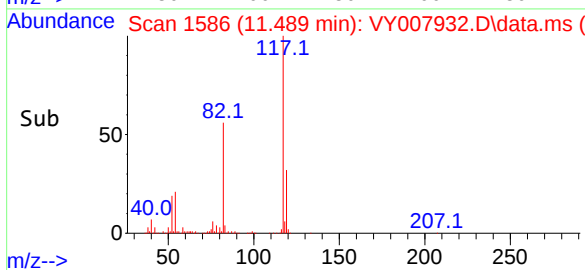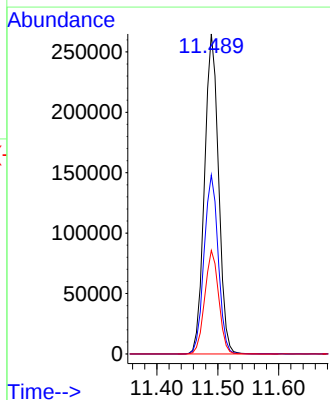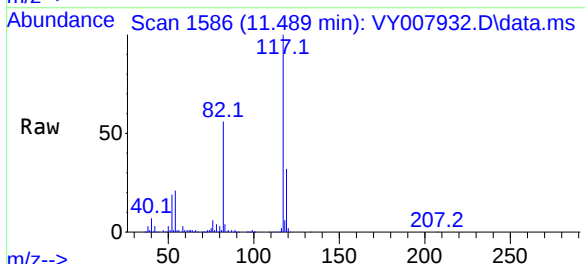

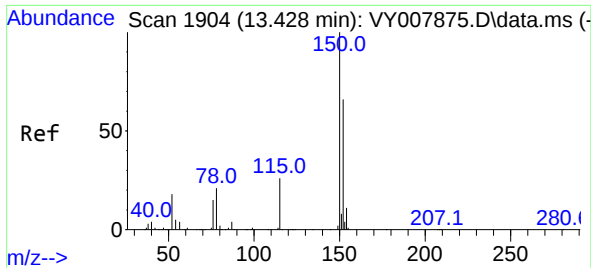

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY007932.D
 Acq: 19 Mar 2022 04:23

Instrument :
 MSVOA_Y
 ClientSampleId :
 C-12-11-12

Tgt Ion:152 Resp: 184353

Ion	Ratio	Lower	Upper
152	100		
115	62.9	28.2	84.7
150	159.7	0.0	347.6

