
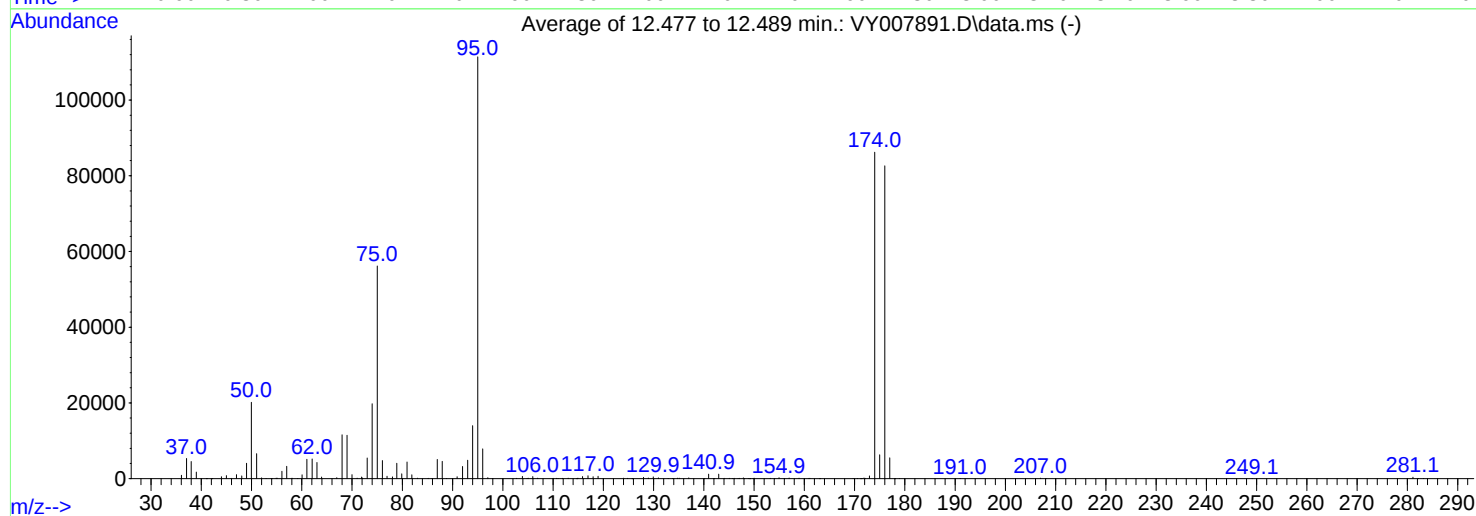


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
 Data File : VY007891.D
 Acq On : 18 Mar 2022 09:19
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Title : SW846 8260
 Last Update : Thu Mar 17 13:55:34 2022

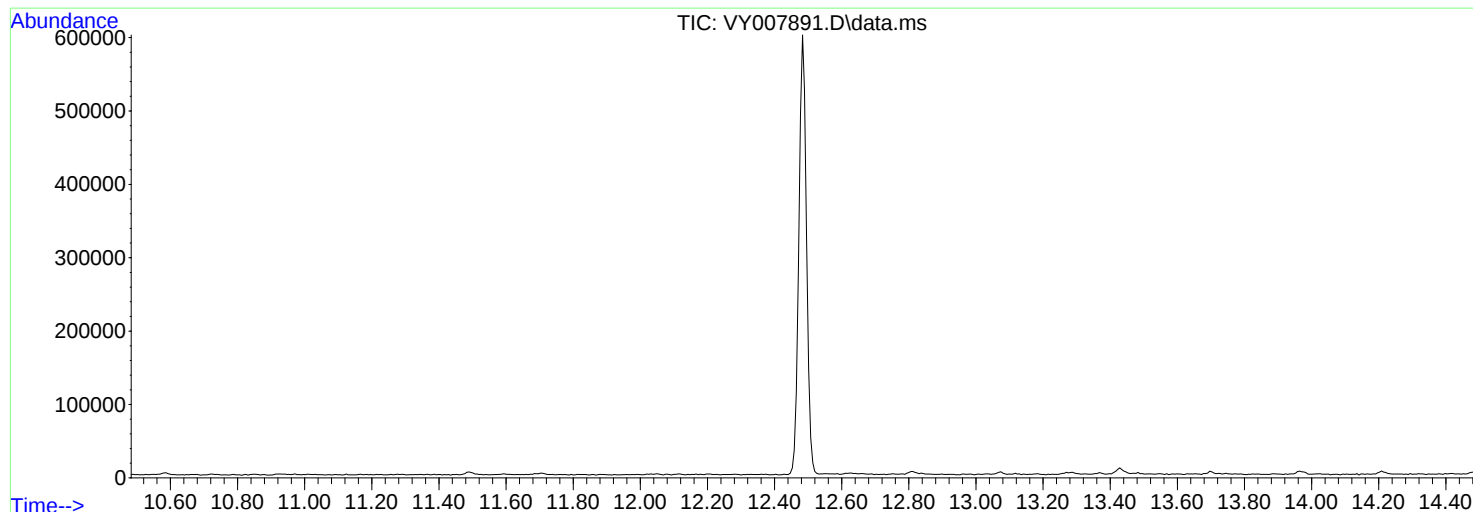

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	20178	PASS
75	95	30	60	50.4	56163	PASS
95	95	100	100	100.0	111413	PASS
96	95	5	9	7.1	7875	PASS
173	174	0.00	2	0.9	743	PASS
174	95	50	100	77.4	86229	PASS
175	174	5	9	7.3	6282	PASS
176	174	95	101	95.8	82608	PASS
177	176	5	9	6.7	5496	PASS