


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031822\
 Data File : VY007917.D
 Acq On : 18 Mar 2022 21:23
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Title : SW846 8260
 Last Update : Thu Mar 17 13:55:34 2022

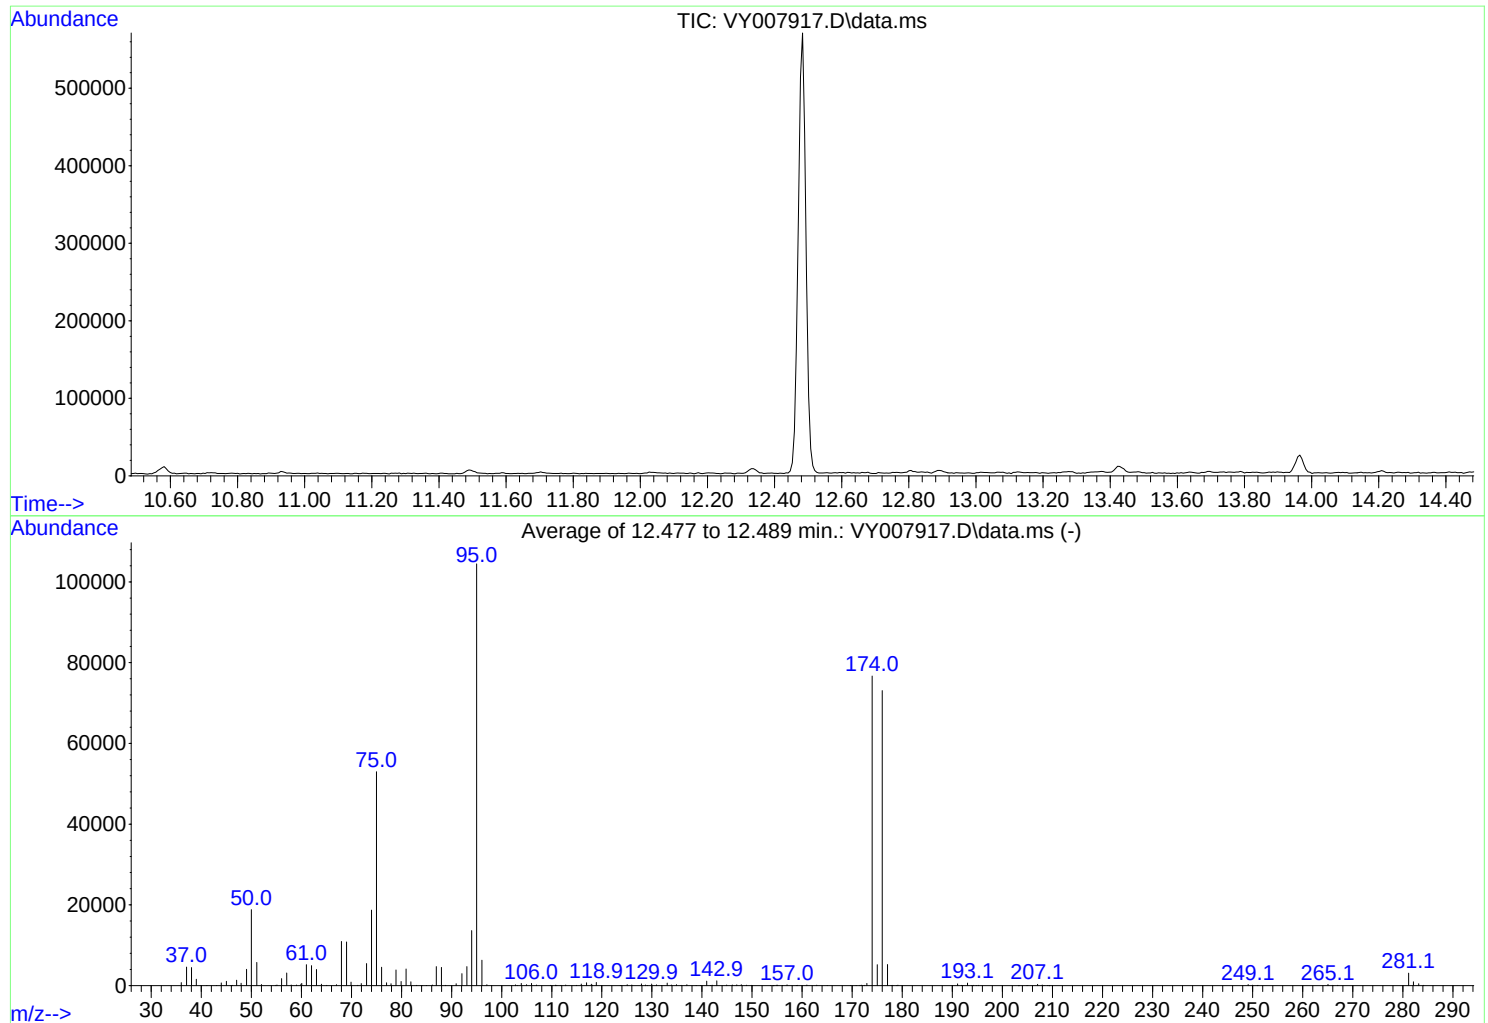

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1736

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	18827	PASS
75	95	30	60	50.7	52992	PASS
95	95	100	100	100.0	104469	PASS
96	95	5	9	6.0	6319	PASS
173	174	0.00	2	0.7	540	PASS
174	95	50	100	73.4	76699	PASS
175	174	5	9	6.8	5214	PASS
176	174	95	101	95.3	73096	PASS
177	176	5	9	7.2	5244	PASS