

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031824\
 Data File : VY017691.D
 Acq On : 18 Mar 2024 16:13
 Operator : SY/MD
 Sample : P1764-01
 Misc : 5.23g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 GRAB-1

Quant Time: Mar 19 04:10:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 24 04:41:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	114573	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	213963	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	190022	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	68273	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	62862	57.892	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.780%
35) Dibromofluoromethane	7.722	113	71498	47.954	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.900%
50) Toluene-d8	10.185	98	247439	47.466	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.940%
62) 4-Bromofluorobenzene	12.489	95	64482	39.359	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	78.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031824\
Data File : VY017691.D
Acq On : 18 Mar 2024 16:13
Operator : SY/MD
Sample : P1764-01
Misc : 5.23g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
GRAB-1

Quant Time: Mar 19 04:10:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 24 04:41:20 2024
Response via : Initial Calibration




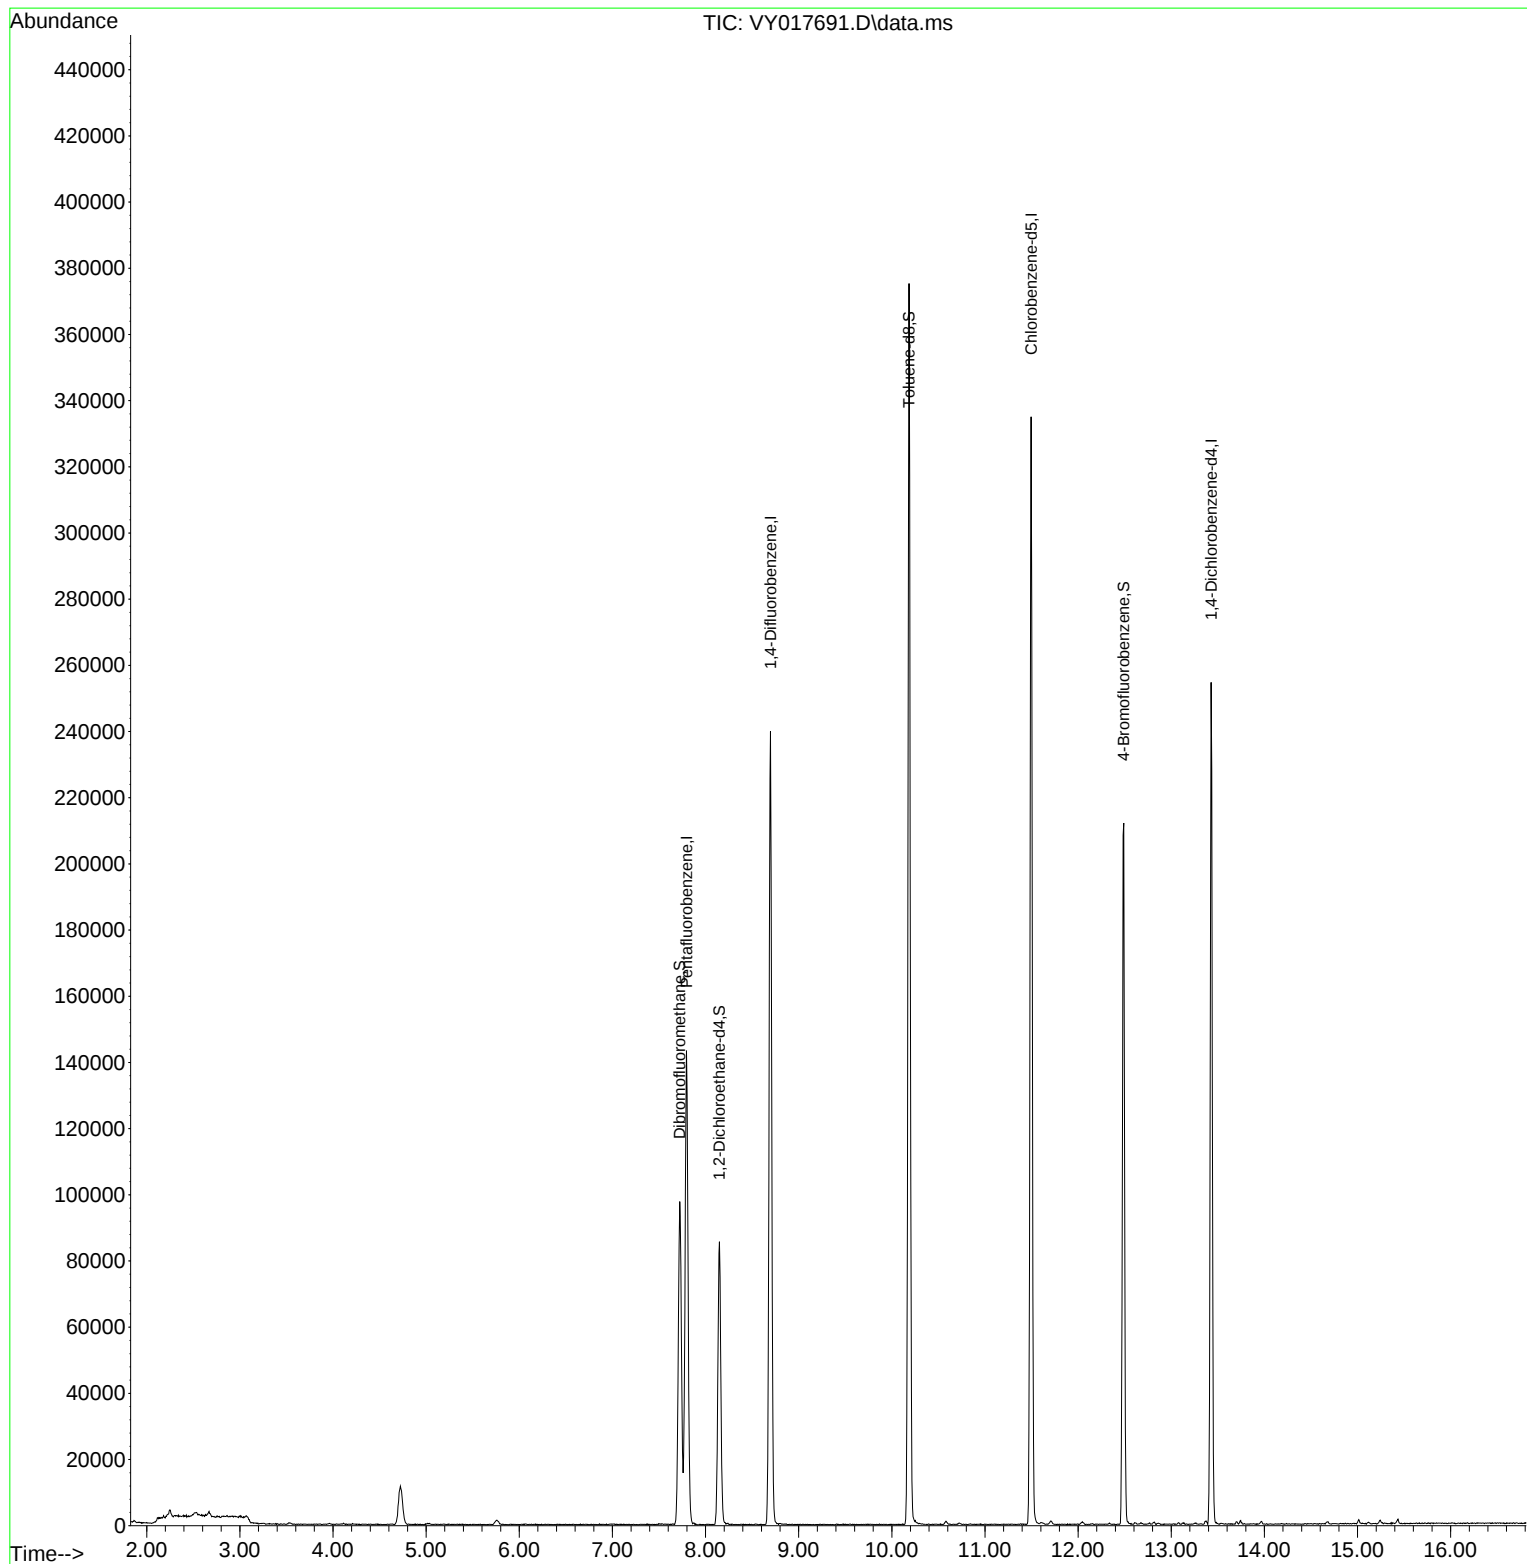


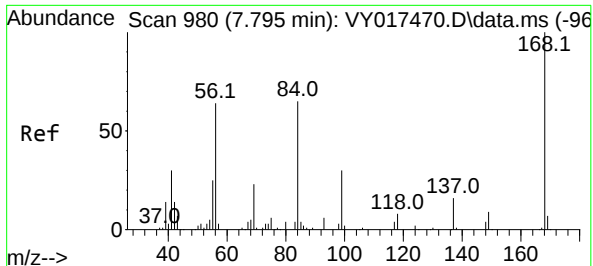

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13




Instrument :
MSVOA_Y
ClientSampleId :
GRAB-1


Tgt Ion:168 Resp: 114573
Ion Ratio Lower Upper
168 100
99 51.1 39.1 58.7

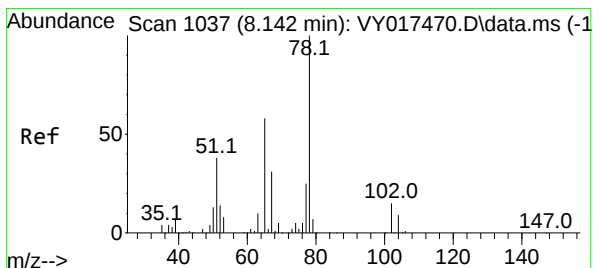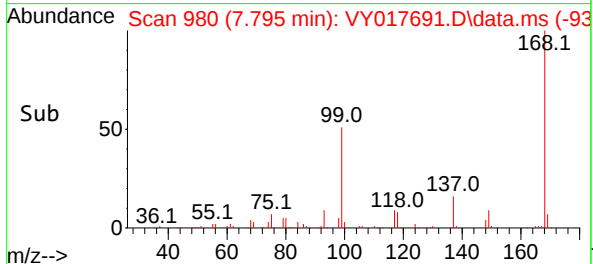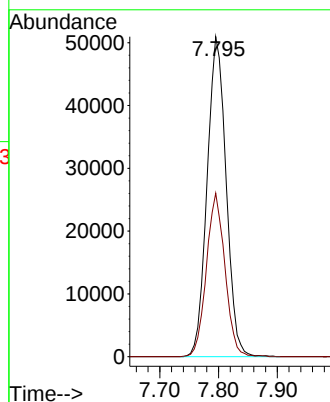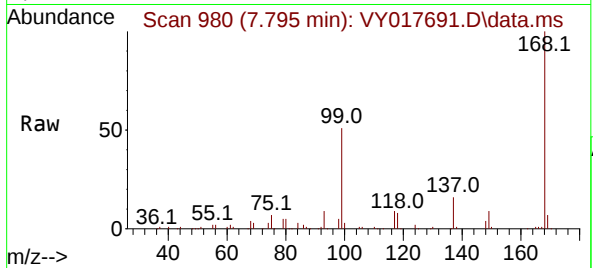

#33
1,2-Dichloroethane-d4
Concen: 57.892 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13

Tgt Ion: 65 Resp: 62862
Ion Ratio Lower Upper
65 100
67 55.2 0.0 109.6

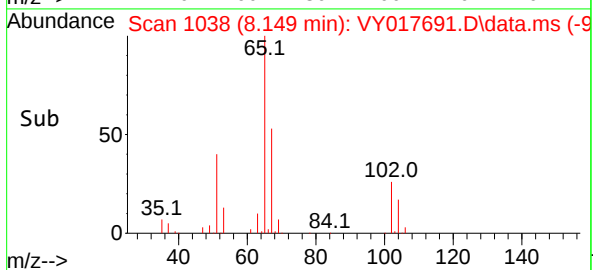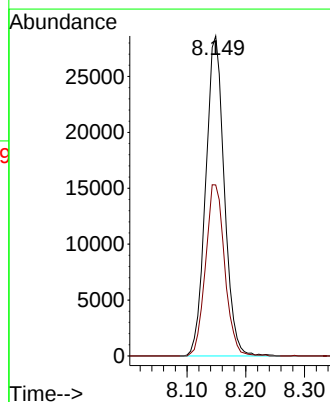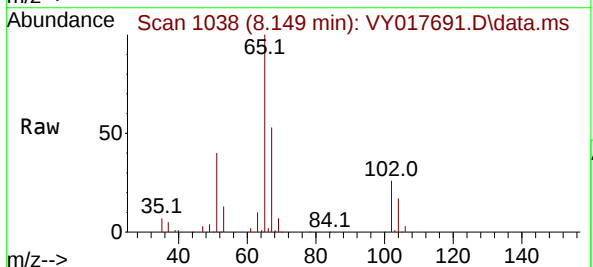

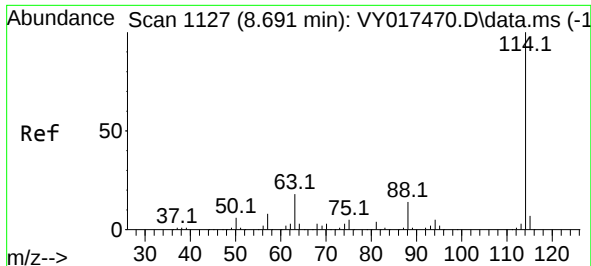

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY017691.D

Acq: 18 Mar 2024 16:13

Instrument :

MSVOA_Y

ClientSampleId :

GRAB-1





Tgt Ion:114 Resp: 213963

Ion Ratio Lower Upper

114 100

63 17.0 0.0 35.0

88 13.3 0.0 27.2

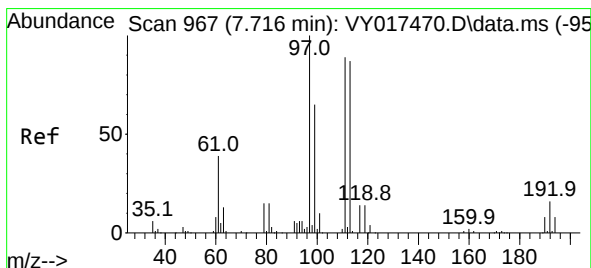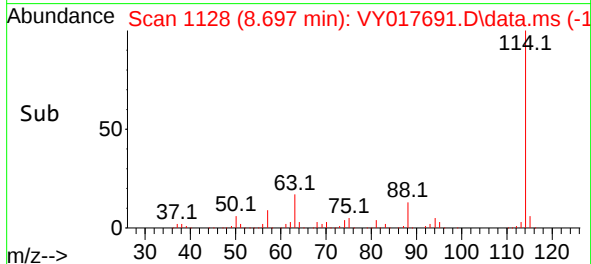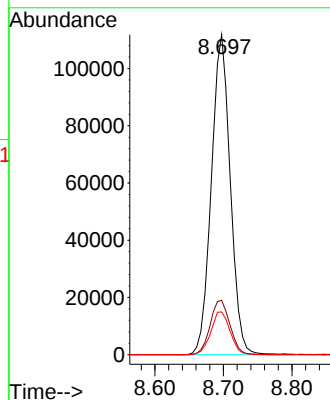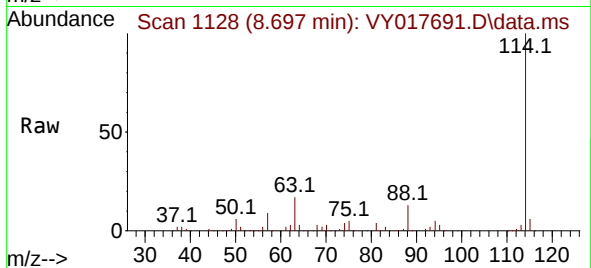

#35

Dibromofluoromethane

Concen: 47.954 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY017691.D

Acq: 18 Mar 2024 16:13




Tgt Ion:113 Resp: 71498


Ion Ratio Lower Upper

113 100

111 102.4 82.2 123.4

192 19.5 15.9 23.9


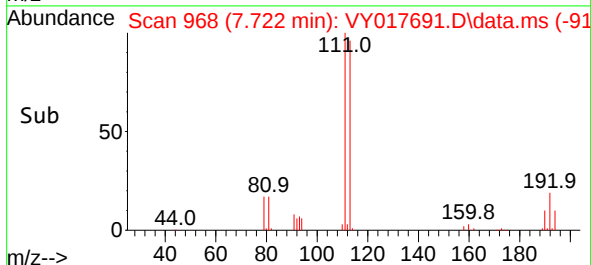
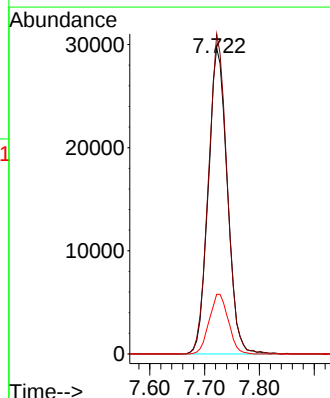
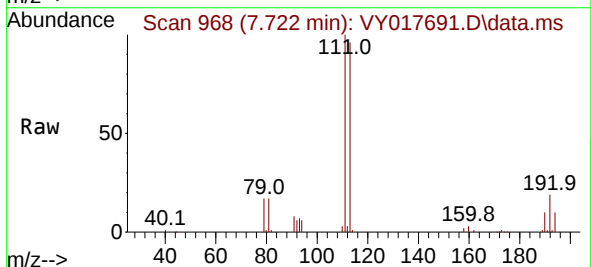


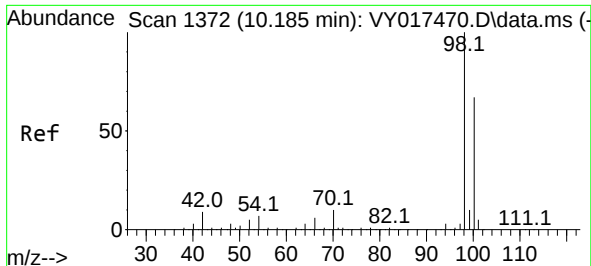

#50
Toluene-d8
Concen: 47.466 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13




Instrument :
MSVOA_Y
ClientSampleId :
GRAB-1


Tgt Ion: 98 Resp: 247439
Ion Ratio Lower Upper
98 100
100 64.5 52.0 78.0

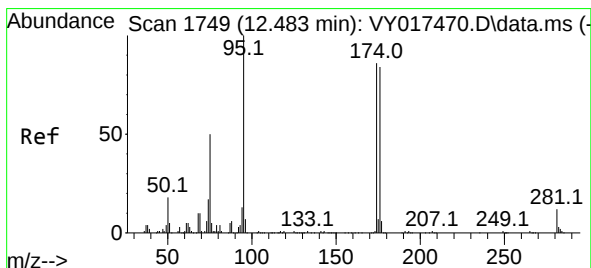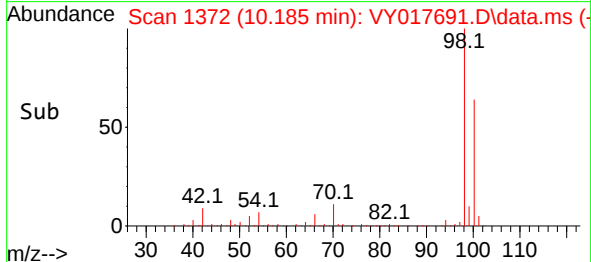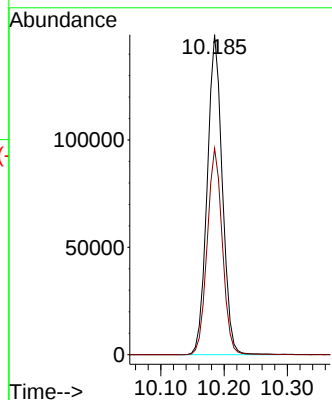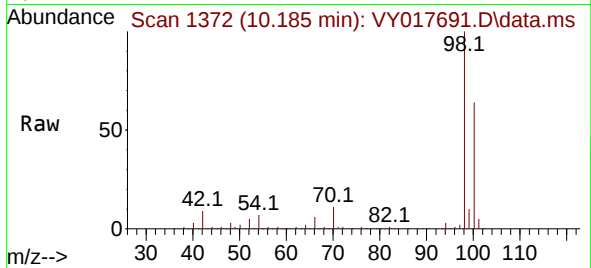

#62
4-Bromofluorobenzene
Concen: 39.359 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13

Tgt Ion: 95 Resp: 64482
Ion Ratio Lower Upper
95 100
174 94.2 0.0 175.6
176 91.3 0.0 171.4


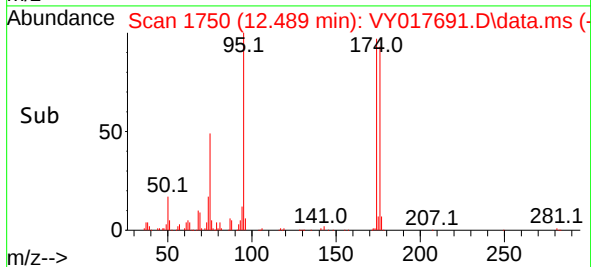
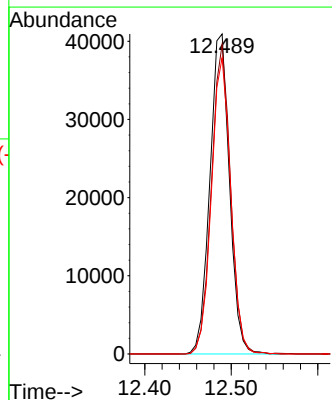
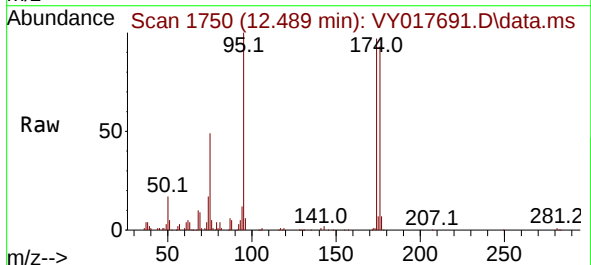


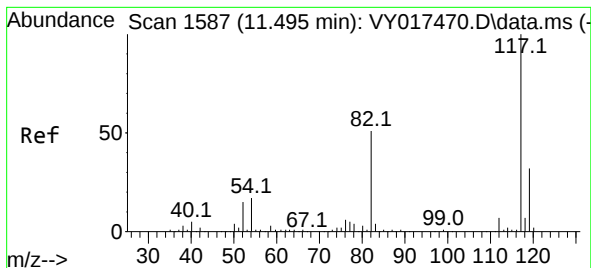

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13

Instrument :
MSVOA_Y
ClientSampleId :
GRAB-1

Tgt Ion:117 Resp: 190022
Ion Ratio Lower Upper
117 100
82 52.1 42.4 63.6
119 32.3 25.9 38.9

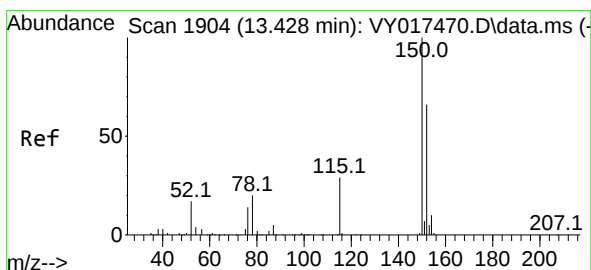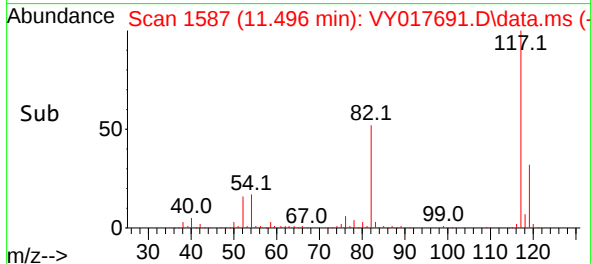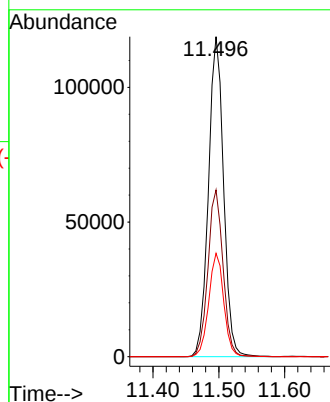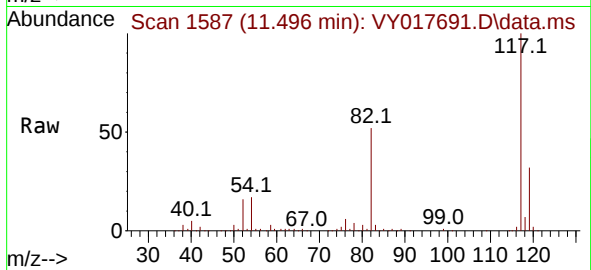

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY017691.D
Acq: 18 Mar 2024 16:13

Tgt Ion:152 Resp: 68273
Ion Ratio Lower Upper
152 100
115 55.2 28.2 84.7
150 155.7 0.0 345.6

