

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031925\
 Data File : VY021565.D
 Acq On : 19 Mar 2025 12:40
 Operator : SY/MD
 Sample : Q1592-01
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OILY-DEBRIS-COMP

Quant Time: Mar 20 01:29:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 05 12:42:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	253134	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	466194	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	406514	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.352	152	146155	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	146236	54.658	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	109.320%
35) Dibromofluoromethane	7.634	113	157160	51.286	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.580%
50) Toluene-d8	10.109	98	564936	48.690	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.380%
62) 4-Bromofluorobenzene	12.407	95	162892	41.273	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	82.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY031925\
Data File : VY021565.D
Acq On : 19 Mar 2025 12:40
Operator : SY/MD
Sample : Q1592-01
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OILY-DEBRIS-COMP

Quant Time: Mar 20 01:29:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Quant Title : SW846 8260
QLast Update : Wed Mar 05 12:42:45 2025
Response via : Initial Calibration




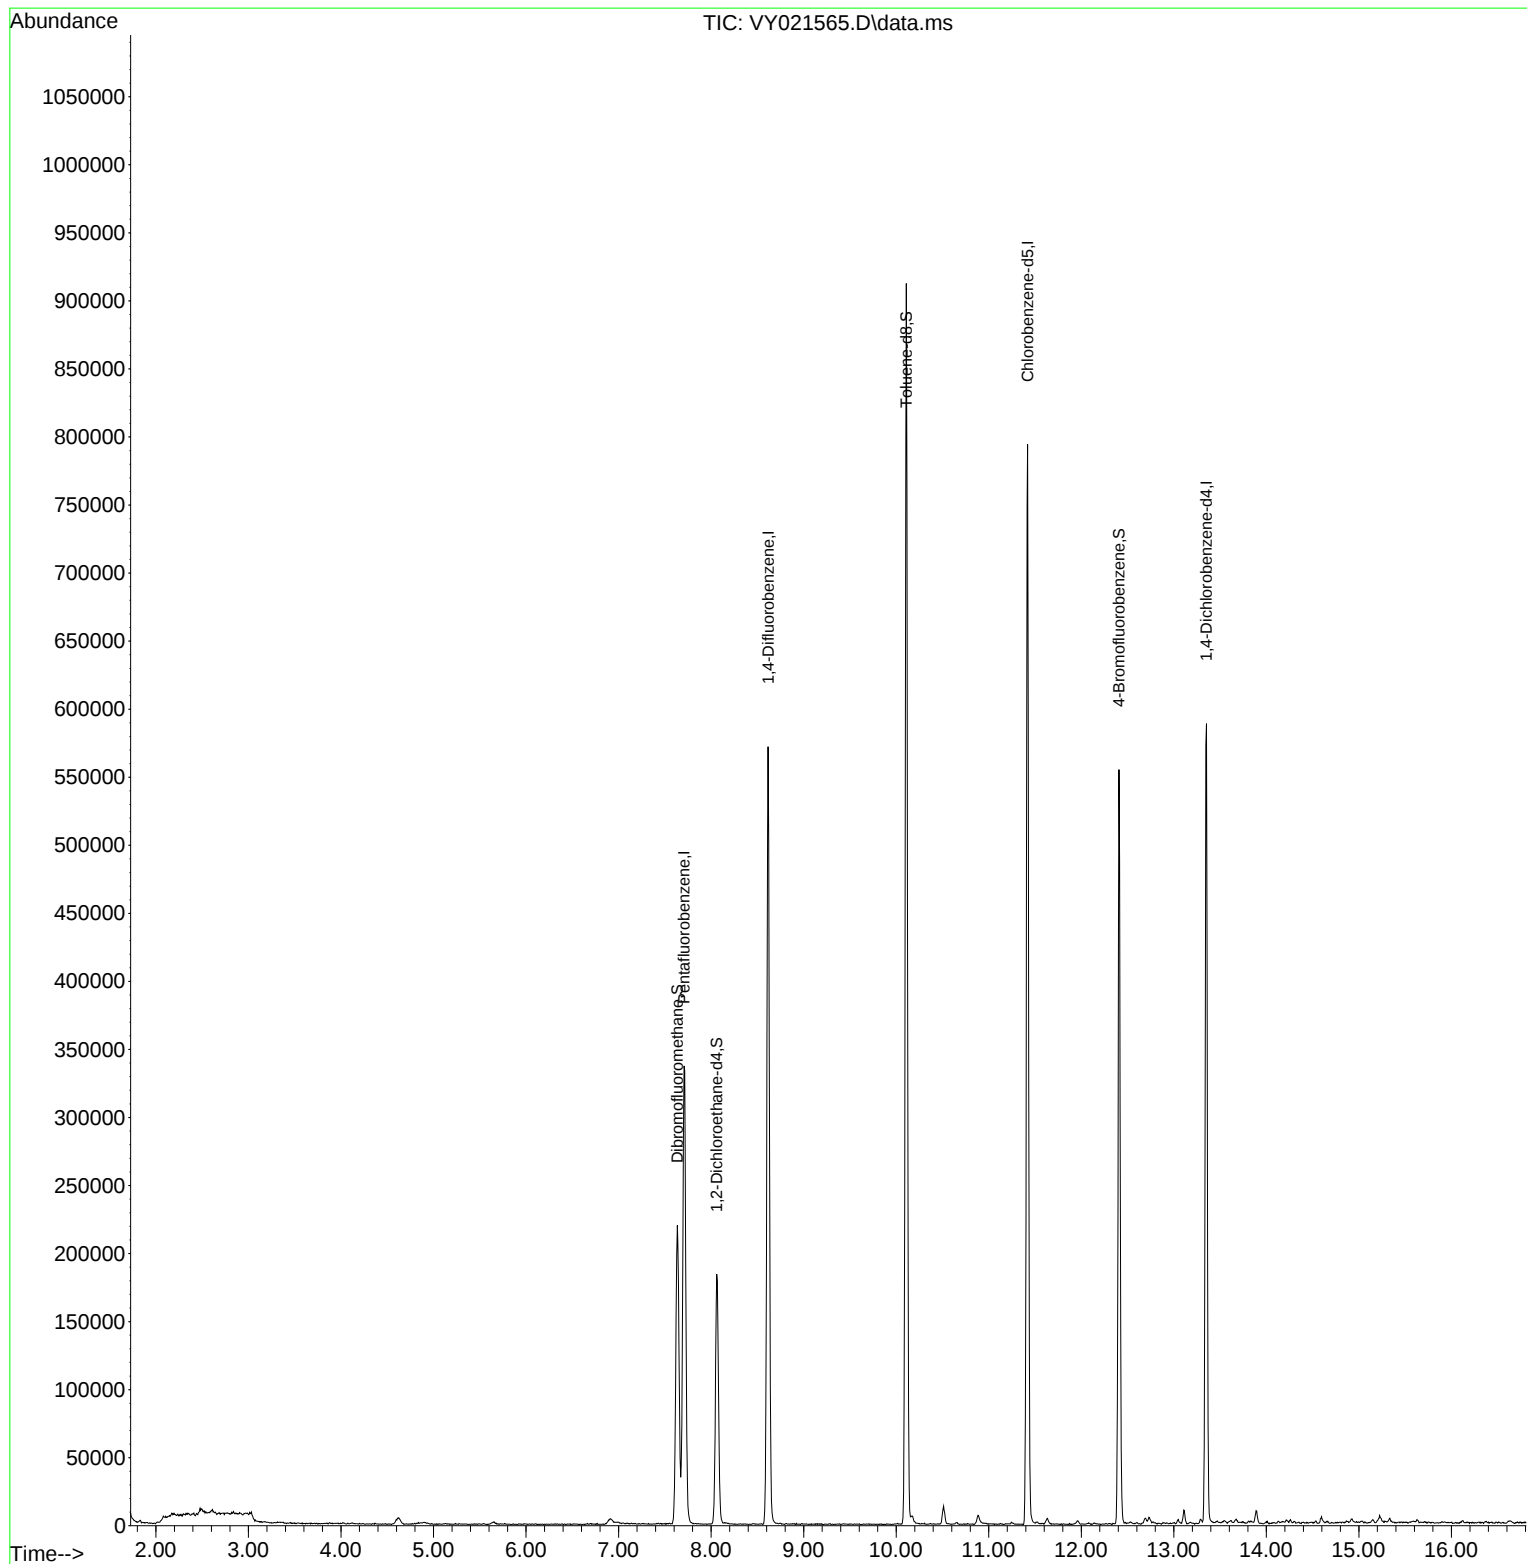


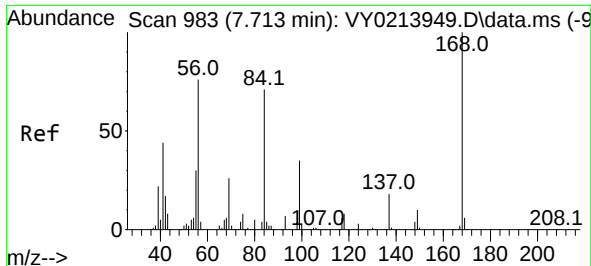

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40




Instrument :
MSVOA_Y
ClientSampleId :
OILY-DEBRIS-COMP


Tgt Ion:168 Resp: 253134
Ion Ratio Lower Upper
168 100
99 57.1 46.0 69.0

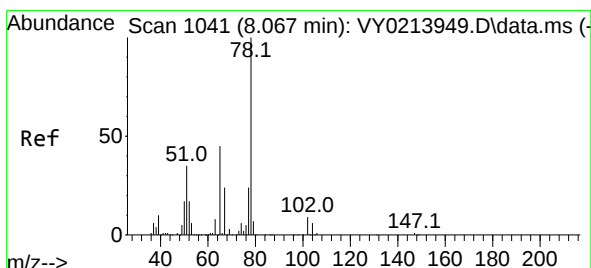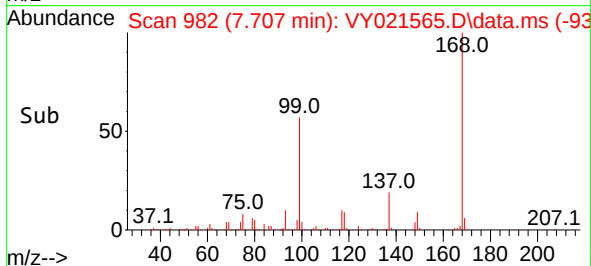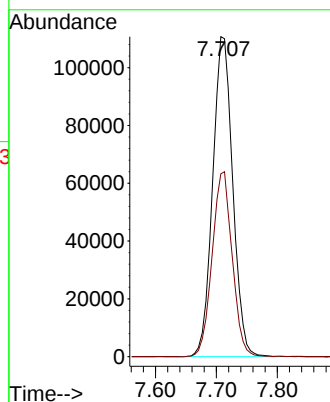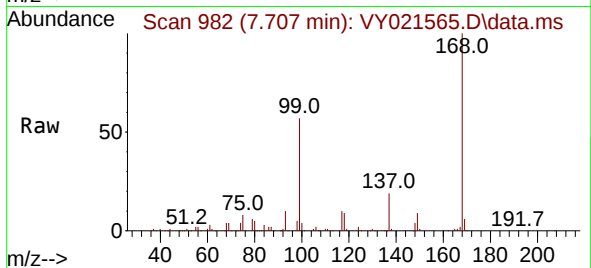

#33
1,2-Dichloroethane-d4
Concen: 54.658 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40

Tgt Ion: 65 Resp: 146236
Ion Ratio Lower Upper
65 100
67 52.6 0.0 102.8


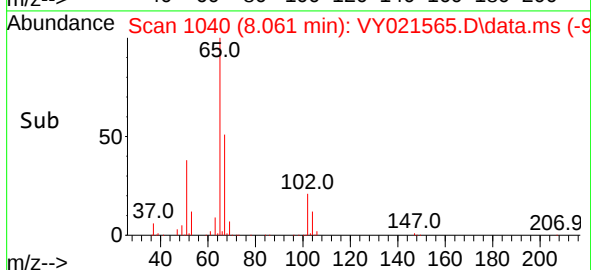
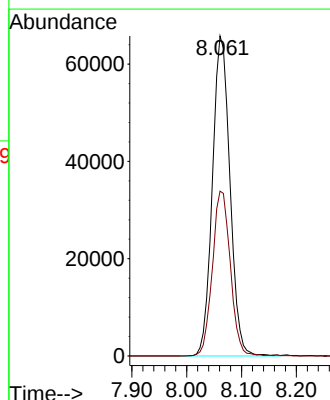
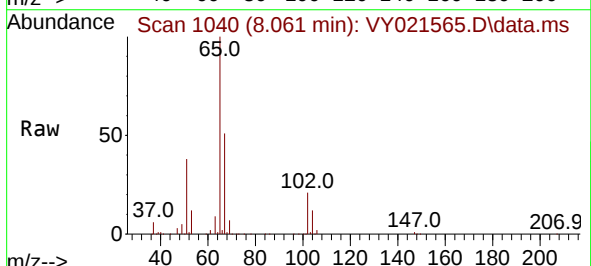


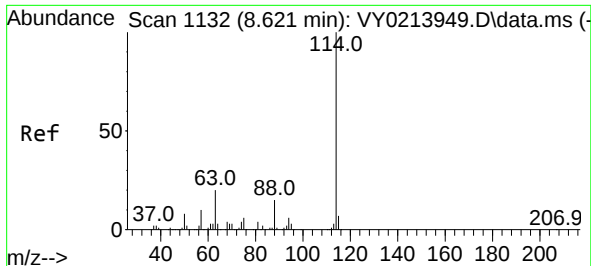

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1132
Delta R.T. -0.006 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40




Instrument :
MSVOA_Y
ClientSampleId :
OILY-DEBRIS-COMP


Tgt Ion:114 Resp: 466194
Ion Ratio Lower Upper
114 100
63 21.1 0.0 40.8
88 15.8 0.0 30.8

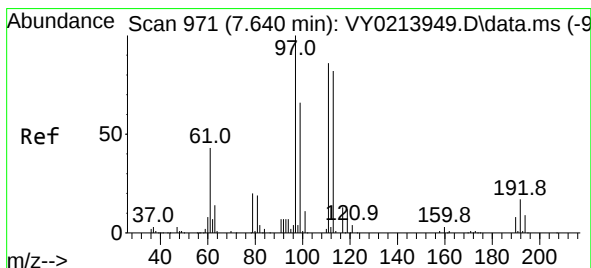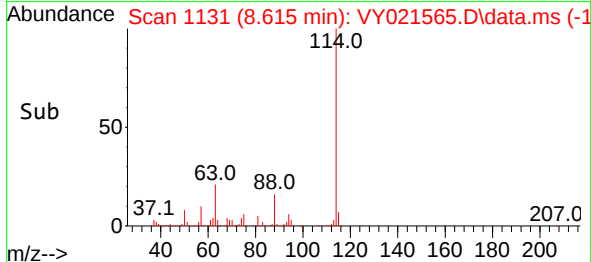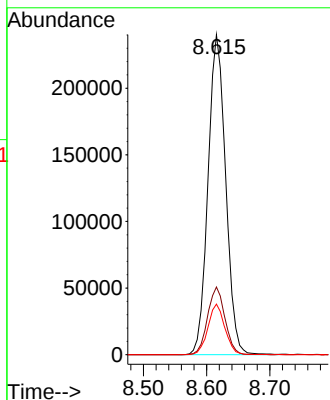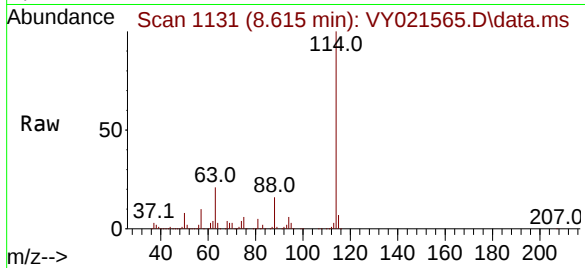

#35
Dibromofluoromethane
Concen: 51.286 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.006 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40

Tgt Ion:113 Resp: 157160
Ion Ratio Lower Upper
113 100
111 102.1 82.0 123.0
192 18.9 15.9 23.9


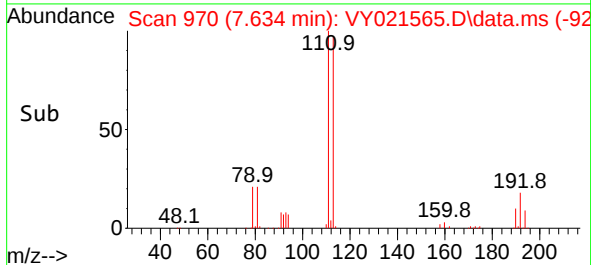
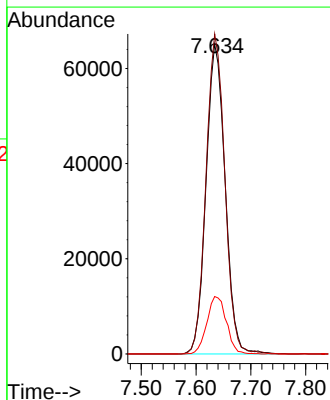
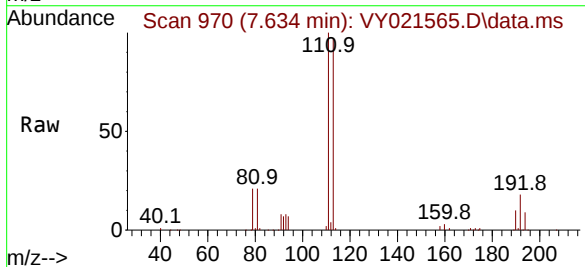


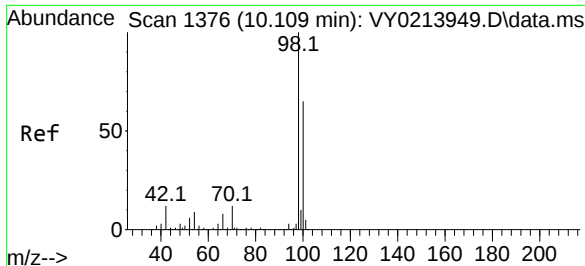

#50
Toluene-d8
Concen: 48.690 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40




Instrument :
MSVOA_Y
ClientSampleId :
OILY-DEBRIS-COMP


Tgt Ion: 98 Resp: 564936
Ion Ratio Lower Upper
98 100
100 64.6 52.1 78.1

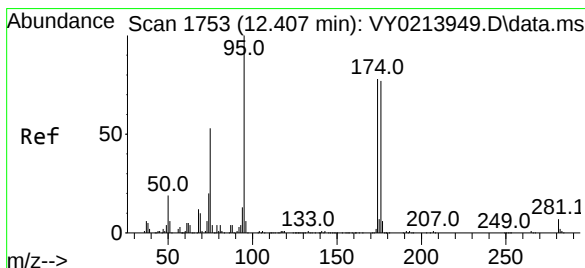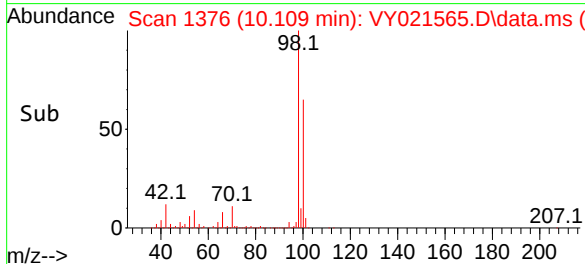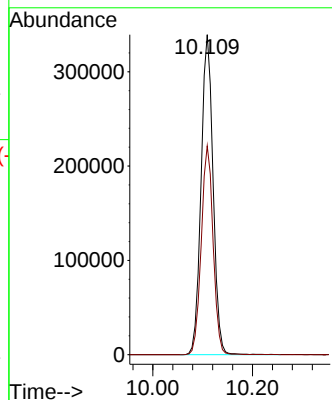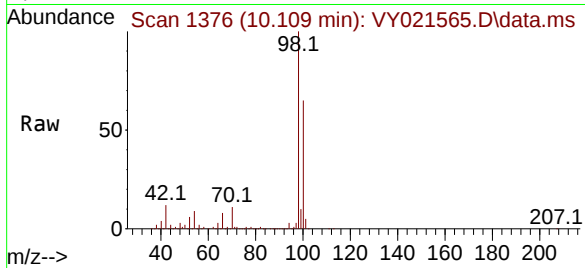

#62
4-Bromofluorobenzene
Concen: 41.273 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40

Tgt Ion: 95 Resp: 162892
Ion Ratio Lower Upper
95 100
174 82.1 0.0 165.0
176 79.4 0.0 160.0


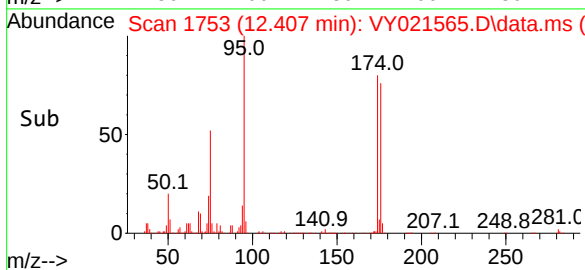
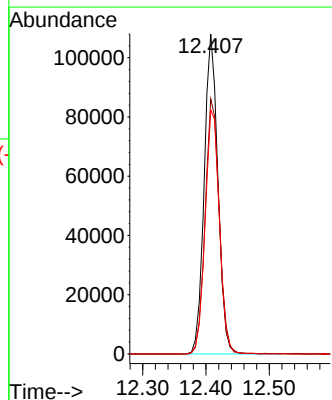
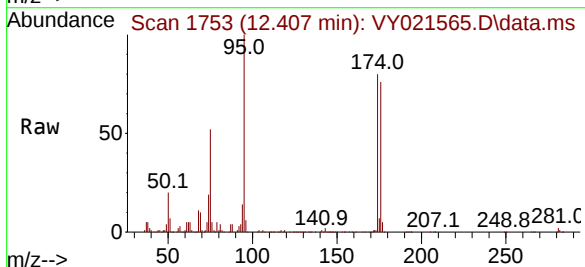


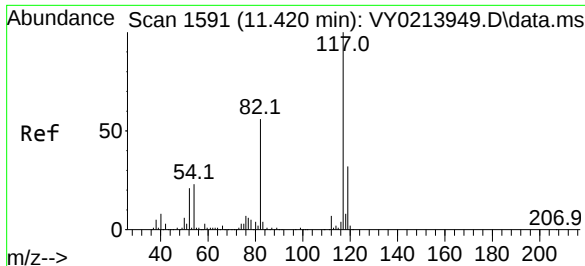

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40

Instrument :
MSVOA_Y
ClientSampleId :
OILY-DEBRIS-COMP

Tgt Ion:117 Resp: 406514
Ion Ratio Lower Upper
117 100
82 55.2 44.6 67.0
119 32.1 25.4 38.0

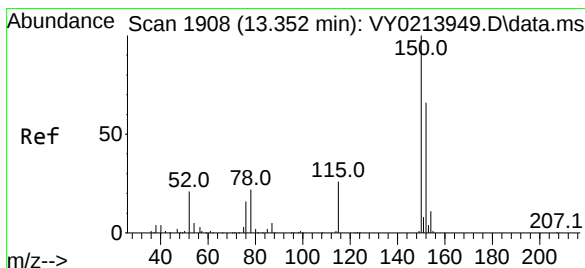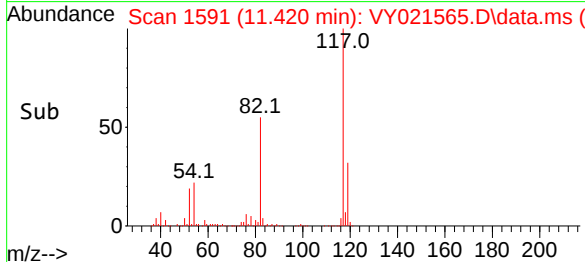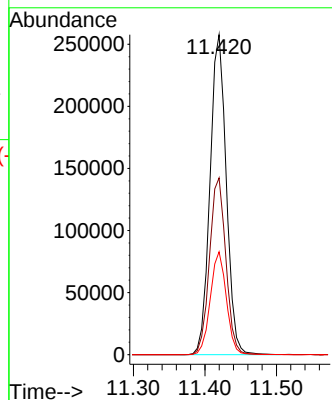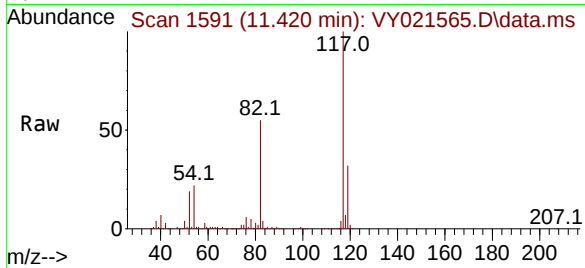

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.352 min Scan# 1908
Delta R.T. 0.000 min
Lab File: VY021565.D
Acq: 19 Mar 2025 12:40

Tgt Ion:152 Resp: 146155
Ion Ratio Lower Upper
152 100
115 58.5 29.0 87.0
150 154.8 0.0 347.2

