
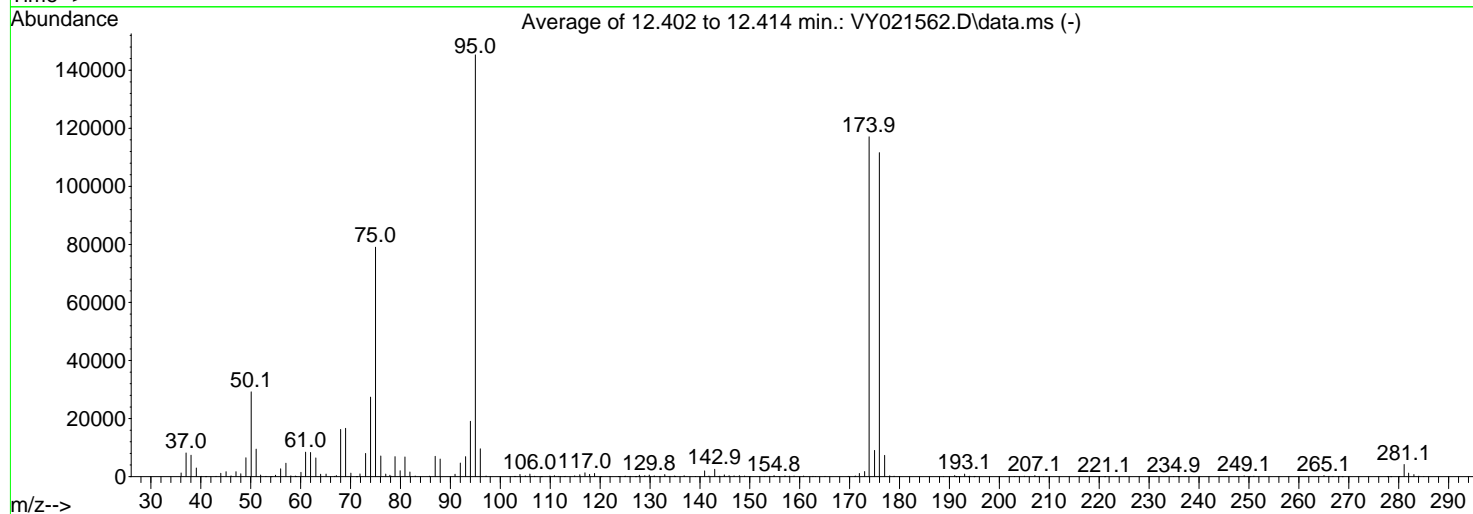


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY031925\  
 Data File : VY021562.D  
 Acq On : 19 Mar 2025 09:14  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y030425S.M  
 Title : SW846 8260  
 Last Update : Wed Mar 05 12:42:45 2025

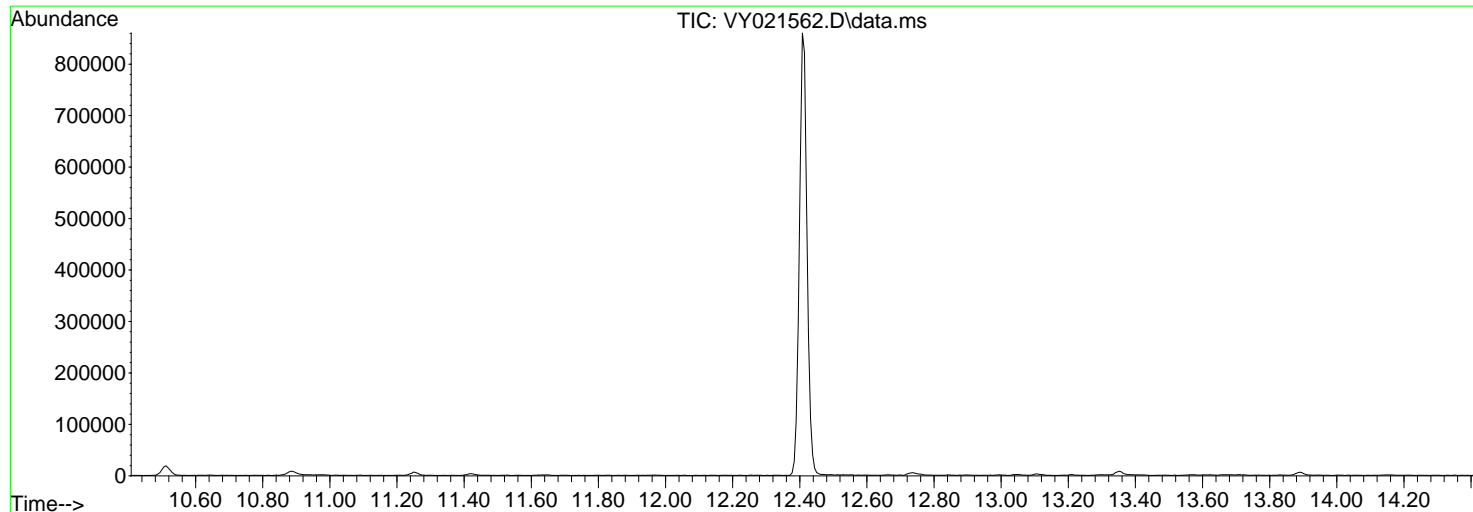

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	29219	PASS
75	95	30	60	54.4	79037	PASS
95	95	100	100	100.0	145309	PASS
96	95	5	9	6.6	9586	PASS
173	174	0.00	2	1.5	1786	PASS
174	95	50	100	80.6	117053	PASS
175	174	5	9	7.7	9036	PASS
176	174	95	101	95.4	111645	PASS
177	176	5	9	6.6	7337	PASS