


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv032020\
Data File : VY002030.D
Acq On : 20 Mar 2020 09:21
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y030420S.M
Title : SW846 8260
Last Update : Thu Mar 05 04:05:33 2020

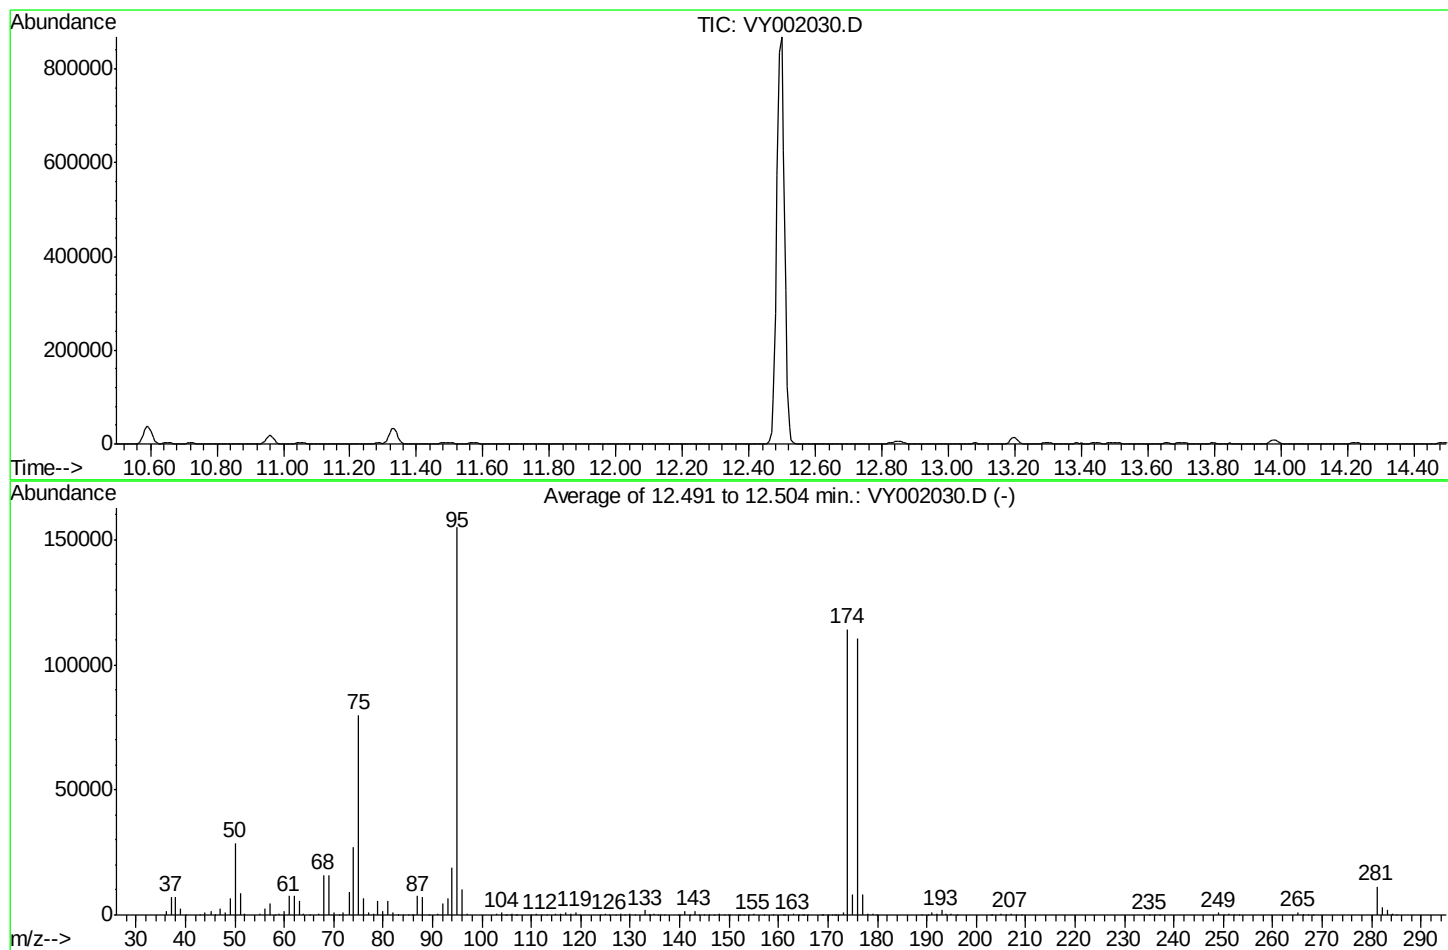

AutoFind: Scans 1764, 1765, 1766; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	28917	PASS
75	95	30	60	51.6	79970	PASS
95	95	100	100	100.0	154922	PASS
96	95	5	9	6.6	10207	PASS
173	174	0.00	2	0.9	1005	PASS
174	95	50	100	73.7	114133	PASS
175	174	5	9	7.3	8357	PASS
176	174	95	101	96.6	110282	PASS
177	176	5	9	7.2	7952	PASS