
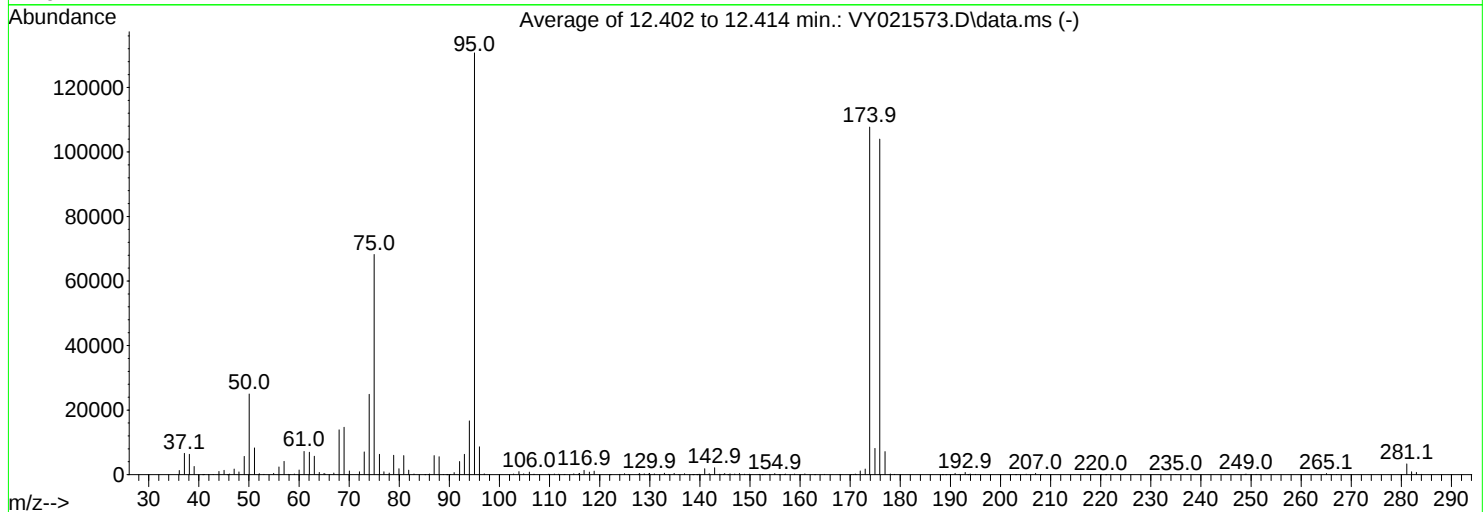


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032025\
Data File : VY021573.D
Acq On : 20 Mar 2025 10:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Title : SW846 8260
Last Update : Wed Mar 05 12:42:45 2025

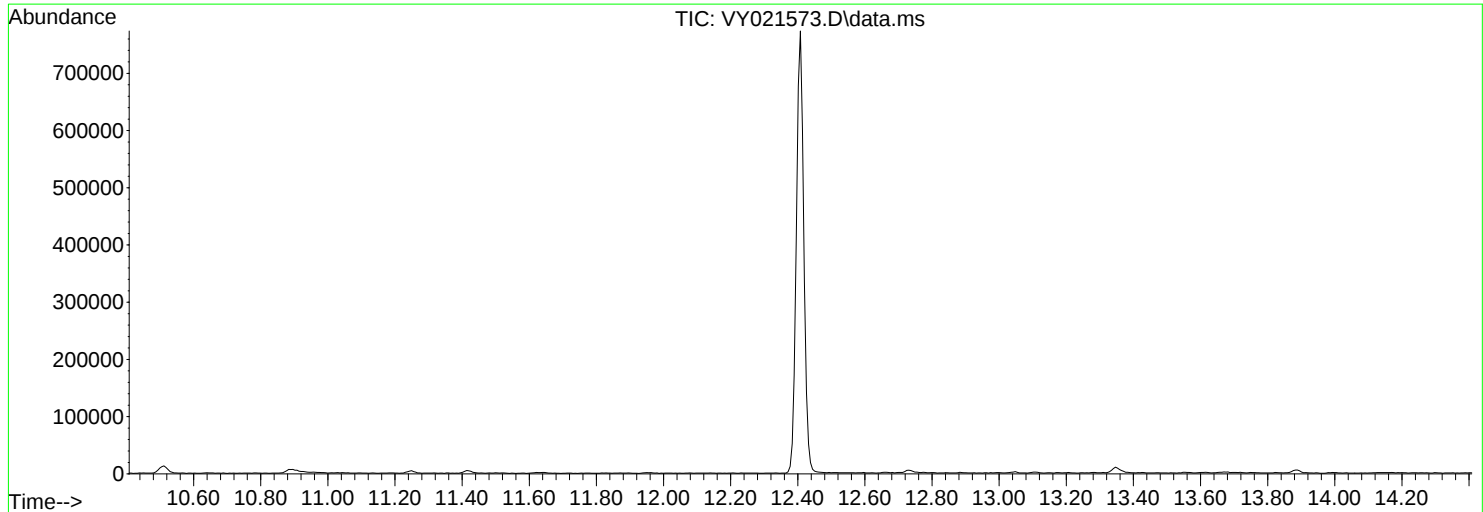

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	25013	PASS
75	95	30	60	52.2	68227	PASS
95	95	100	100	100.0	130731	PASS
96	95	5	9	6.6	8620	PASS
173	174	0.00	2	1.6	1743	PASS
174	95	50	100	82.4	107715	PASS
175	174	5	9	7.6	8141	PASS
176	174	95	101	96.6	104005	PASS
177	176	5	9	6.9	7127	PASS