

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032122\
 Data File : VY007984.D
 Acq On : 22 Mar 2022 04:14
 Operator : SY/MD
 Sample : N2057-03
 Misc : 7.90g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 UST-7-NORTH-SIDEWALL

Quant Time: Mar 22 06:56:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 13:55:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	62282	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	109143	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	83946	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	28880	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	31824	44.814	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	89.620%		
35) Dibromofluoromethane	7.722	113	31983	41.726	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	83.460%		
50) Toluene-d8	10.179	98	129352	56.679	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery =	113.360%		
62) 4-Bromofluorobenzene	12.477	95	38910	35.370	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery =	70.740%		
Target Compounds					Qvalue	
3) Chloromethane	2.113	50	423	Below Cal		93
4) Vinyl Chloride	2.253	62	272	Below Cal	#	43
5) Bromomethane	2.668	94	379	Below Cal	#	29
11) Tert butyl alcohol	4.966	59	267	3.227 ug/l	#	77
16) Acetone	3.948	43	4749	25.209 ug/l		91
17) Carbon Disulfide	4.204	76	2581	Below Cal	#	91
18) Methyl Acetate	4.479	43	105	Below Cal	#	56
20) Methylene Chloride	4.710	84	1469	Below Cal	#	79
25) 2-Butanone	6.996	43	1669	5.531 ug/l	#	71
29) Tetrahydrofuran	7.344	42	202	1.045 ug/l	#	38
31) Cyclohexane	7.795	56	2620	Below Cal	#	48
36) 1,1-Dichloropropene	7.783	75	5784	5.088 ug/l	#	48
38) Carbon Tetrachloride	7.795	117	6965	5.733 ug/l	#	15
39) Methylcyclohexane	9.191	83	6660	2.225 ug/l	#	82
44) Trichloroethene	8.941	130	1560	1.698 ug/l		74
55) 1,1,2-Trichloroethane	10.618	97	3544	4.847 ug/l	#	20
56) Ethyl methacrylate	10.520	69	2155	2.053 ug/l	#	1
59) 2-Hexanone	10.801	43	6638	13.174 ug/l	#	33
60) Dibromochloromethane	10.715	129	45575	52.048 ug/l	#	11
64) Tetrachloroethene	10.721	164	49514	75.798 ug/l		96
74) N-amyl acetate	12.124	43	22429	29.906 ug/l	#	61
75) 1,1,2,2-Tetrachloroethane	12.550	83	3324	6.075 ug/l	#	26
76) 1,2,3-Trichloropropane	12.483	75	22821	55.440 ug/l	#	100
81) trans-1,4-Dichloro-2-b...	12.483	75	22821	116.446 ug/l	#	12
84) 1,2,4-Trimethylbenzene	12.971	105	2192	1.070 ug/l		84
85) sec-Butylbenzene	13.251	105	3305	1.179 ug/l		81
89) n-Butylbenzene	13.696	91	2554	1.169 ug/l	#	81
90) Hexachloroethane	13.971	117	1142	2.514 ug/l	#	6
92) 1,2-Dibromo-3-Chloropr...	14.385	75	95	1.009 ug/l	#	22
96) 1,2,3-Trichlorobenzene	15.446	180	637	1.120 ug/l	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032122\
Data File : VY007984.D
Acq On : 22 Mar 2022 04:14
Operator : SY/MD
Sample : N2057-03
Misc : 7.90g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Quant Time: Mar 22 06:56:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 13:55:34 2022
Response via : Initial Calibration




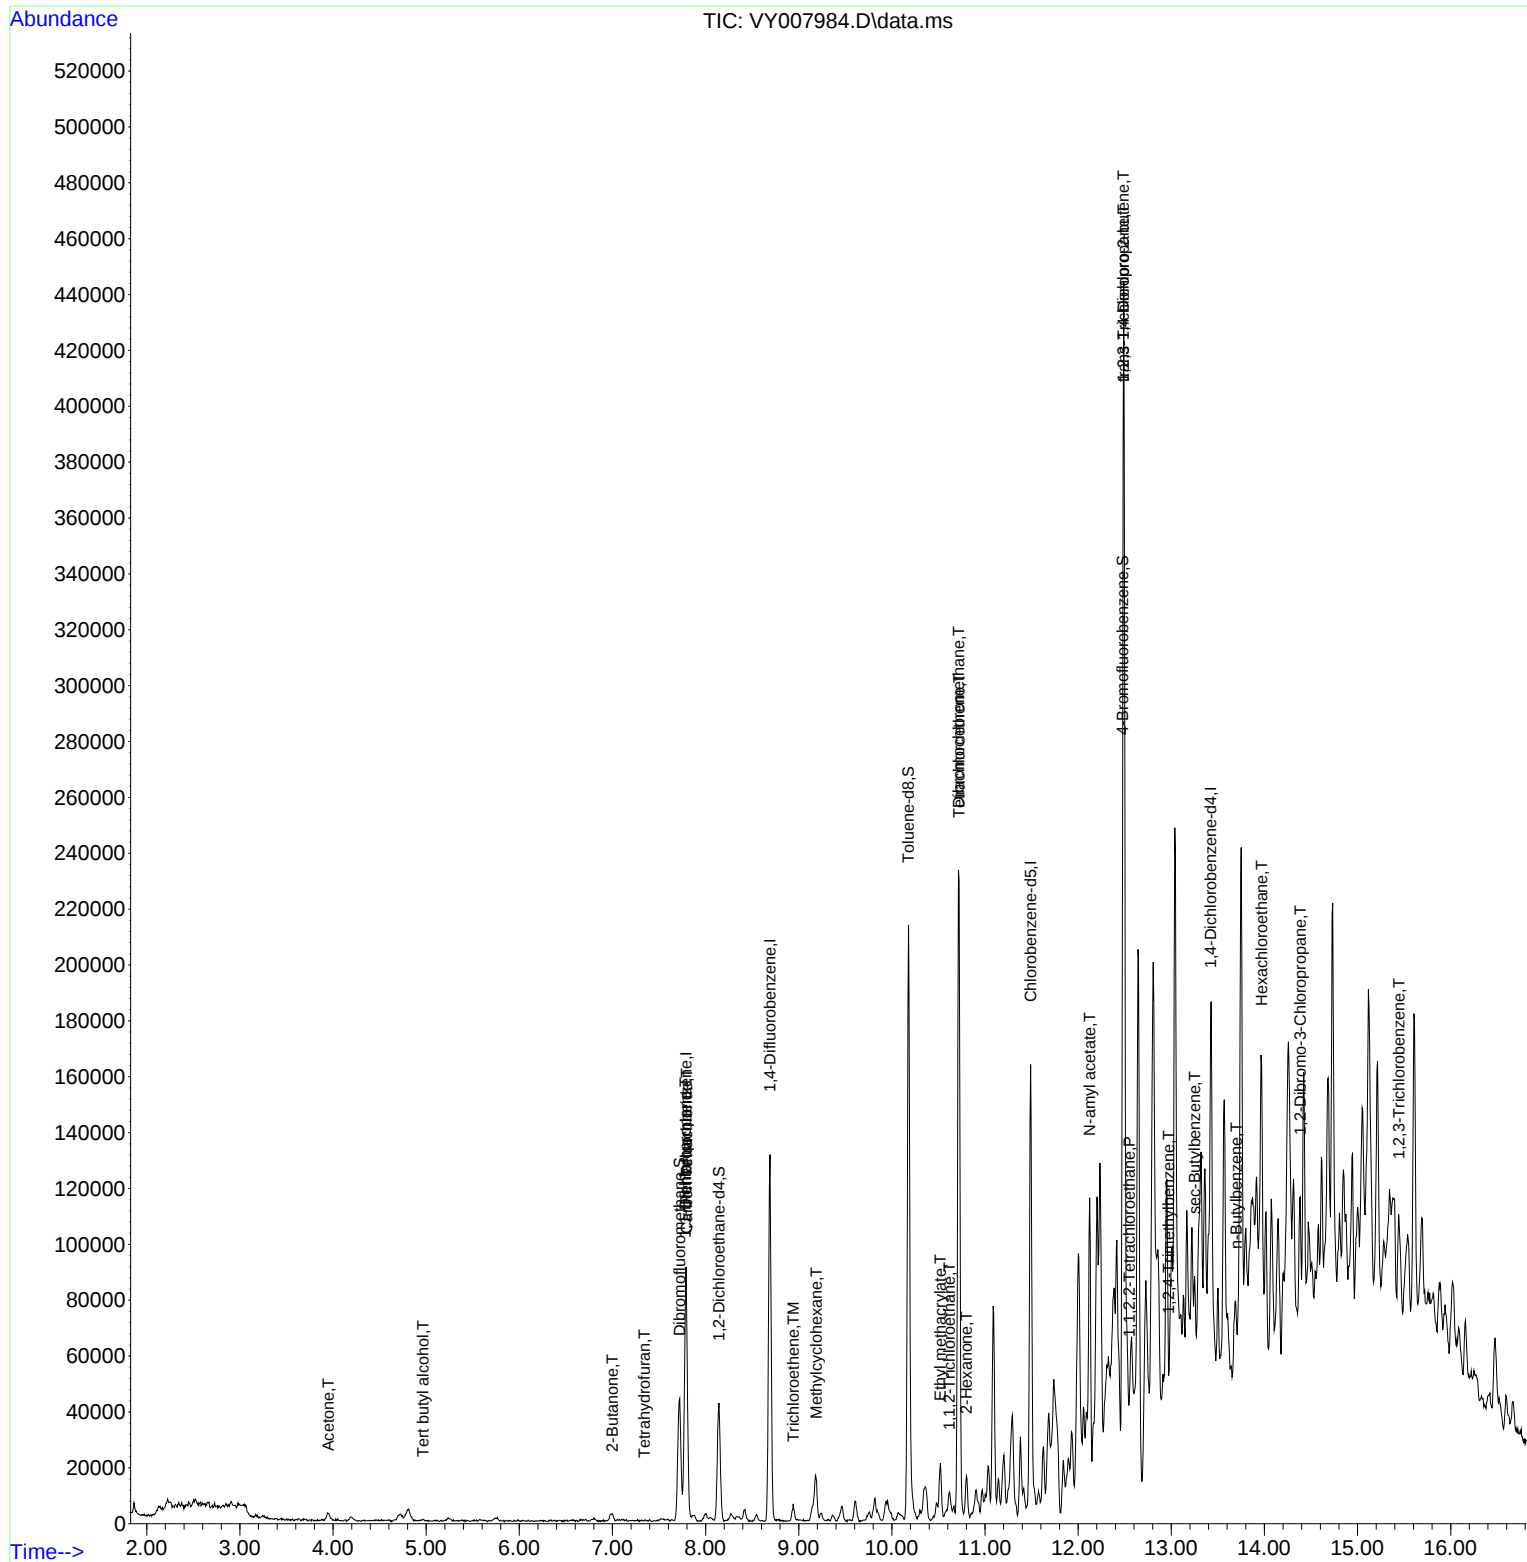




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion:168 Resp: 62282
Ion Ratio Lower Upper
168 100
99 62.9 46.9 70.3

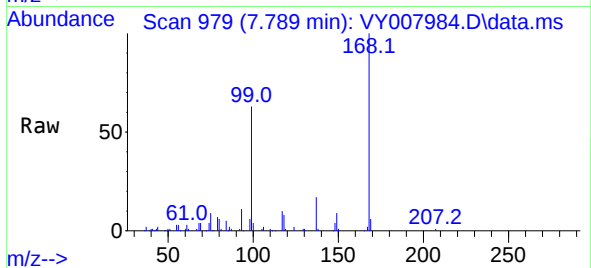

#3
Chloromethane
Concen: Below Cal
RT: 2.113 min Scan# 48
Delta R.T. -0.000 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 50 Resp: 423
Ion Ratio Lower Upper
50 100
52 34.9 24.6 37.0


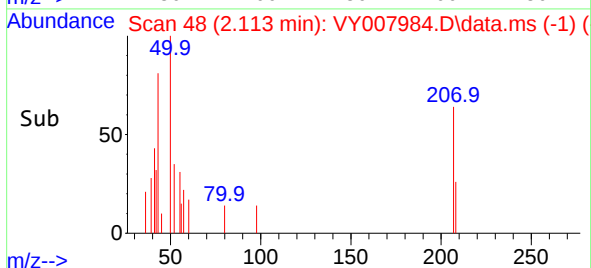
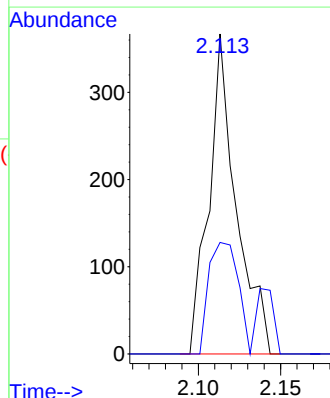



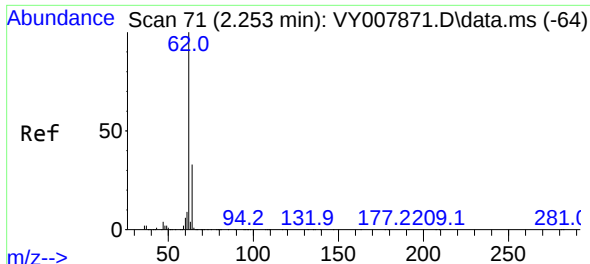

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 2.253 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: VY007984.D
 Acq: 22 Mar 2022 04:14




Instrument :
 MSVOA_Y
 ClientSampleId :
 UST-7-NORTH-SIDEWALL


Tgt Ion: 62 Resp: 272
 Ion Ratio Lower Upper
 62 100
 64 0.0 25.0 37.6#

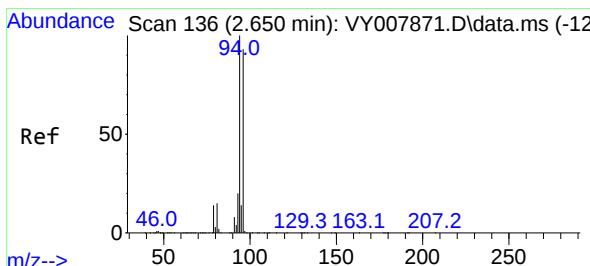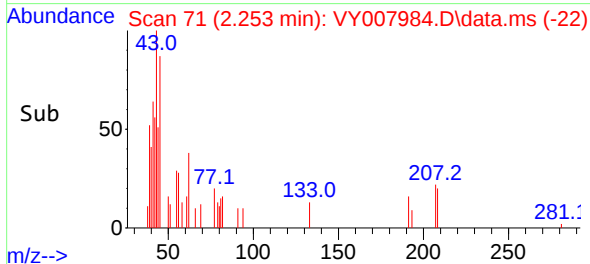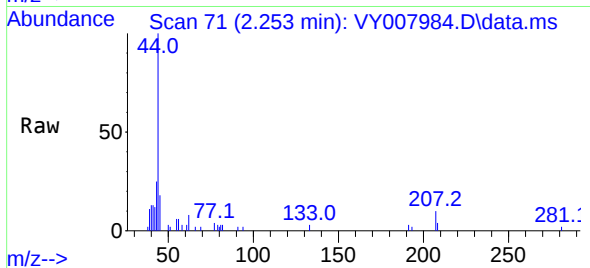

#5
 Bromomethane
 Concen: Below Cal
 RT: 2.668 min Scan# 139
 Delta R.T. 0.018 min
 Lab File: VY007984.D
 Acq: 22 Mar 2022 04:14

Tgt Ion: 94 Resp: 379
 Ion Ratio Lower Upper
 94 100
 96 24.6 73.5 110.3#


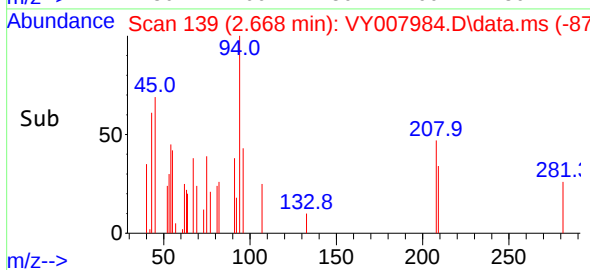

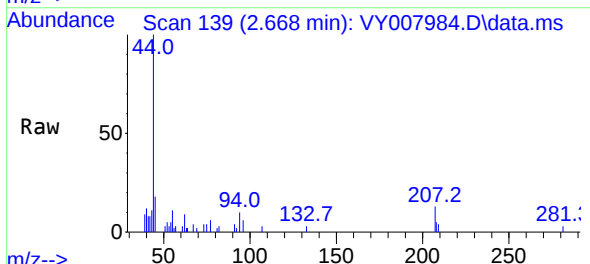


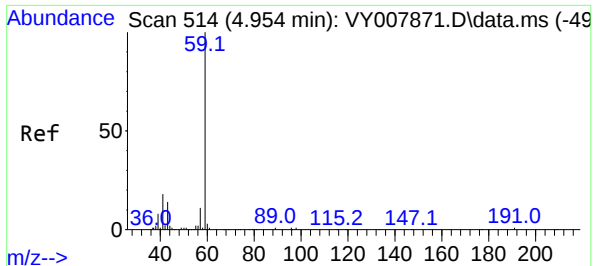

#11
Tert butyl alcohol
Concen: 3.227 ug/l
RT: 4.966 min Scan# 514
Delta R.T. 0.012 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion: 59 Resp: 267
Ion Ratio Lower Upper
59 100
57 0.0 6.4 9.6#

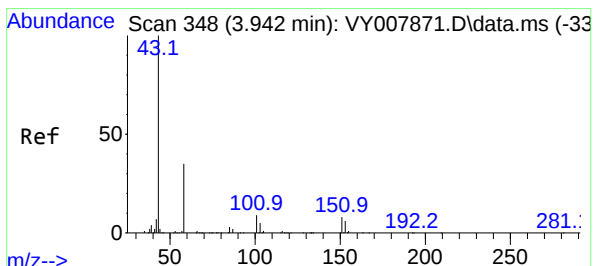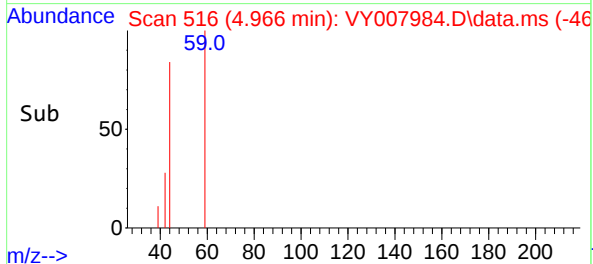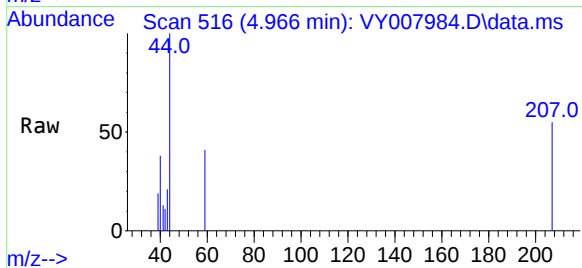

#16
Acetone
Concen: 25.209 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 43 Resp: 4749
Ion Ratio Lower Upper
43 100
58 23.0 22.0 33.0


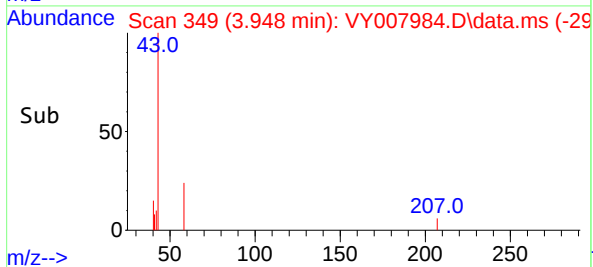

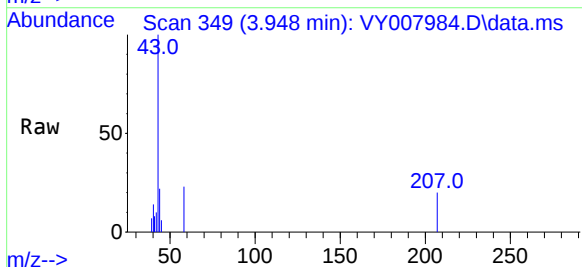




#17
Carbon Disulfide
Concen: Below Cal
RT: 4.204 min Scan# 391
Delta R.T. 0.012 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion: 76 Resp: 2581
Ion Ratio Lower Upper
76 100
78 5.8 7.4 11.0#

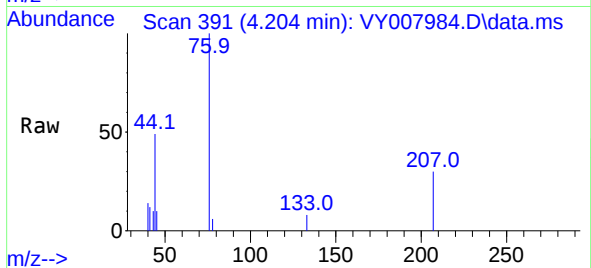

#18
Methyl Acetate
Concen: Below Cal
RT: 4.479 min Scan# 436
Delta R.T. 0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 43 Resp: 105
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

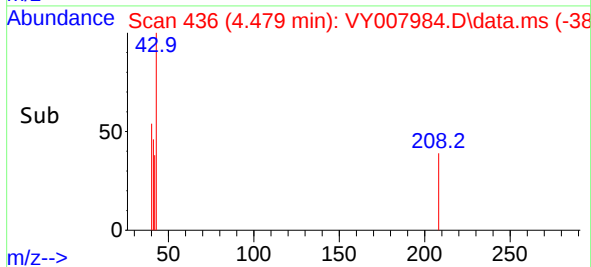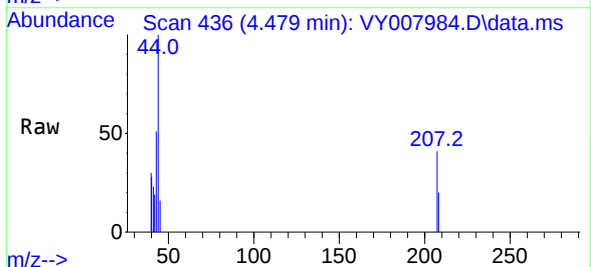




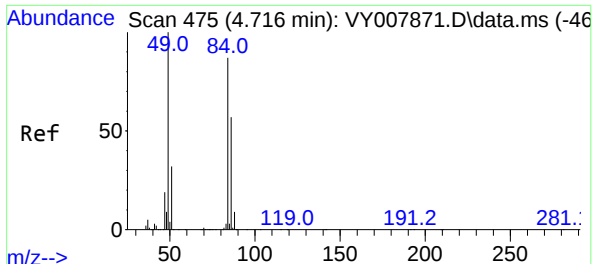


#20
Methylene Chloride
Concen: Below Cal
RT: 4.710 min Scan# 41
Delta R.T. -0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Tgt Ion: 84 Resp: 1469




Ion	Ratio	Lower	Upper
84	100		
49	100.8	114.4	171.6#
51	39.8	35.3	52.9
86	66.1	53.7	80.5

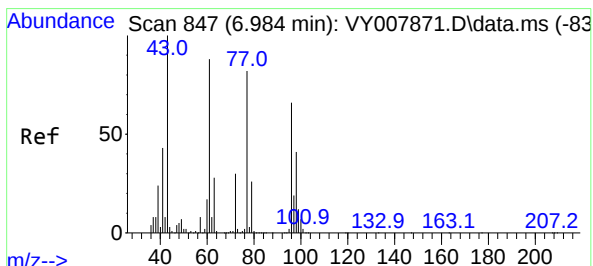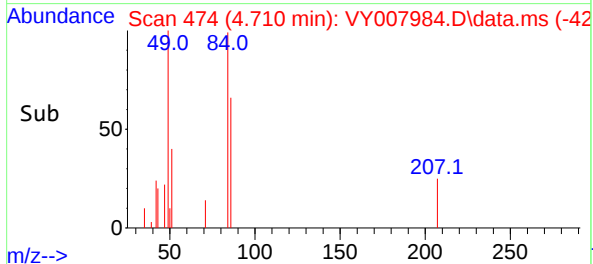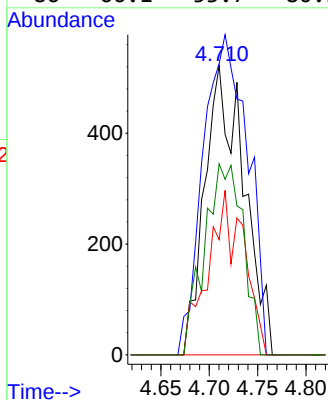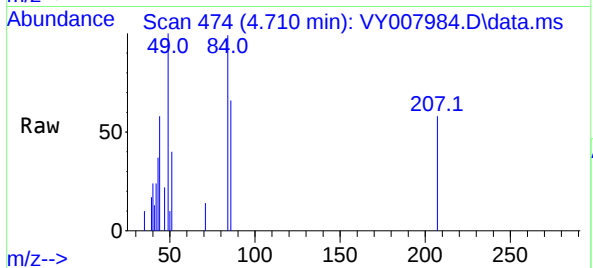


#25
2-Butanone
Concen: 5.531 ug/l
RT: 6.996 min Scan# 849
Delta R.T. 0.012 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 43 Resp: 1669

Ion	Ratio	Lower	Upper
43	100		
72	35.8	17.7	26.5#

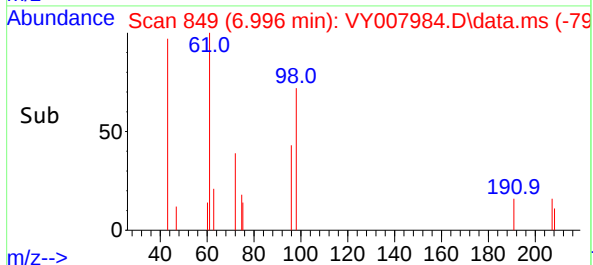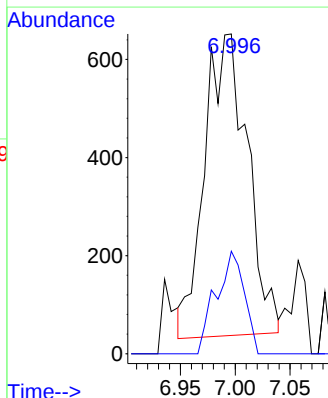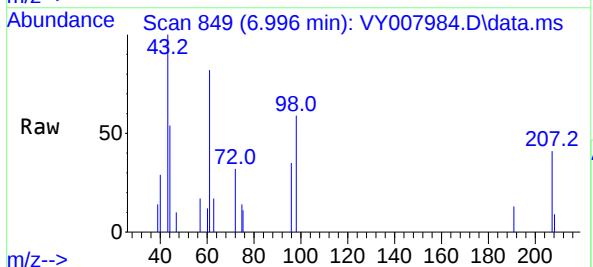



#29

Tetrahydrofuran

Concen: 1.045 ug/l

RT: 7.344 min Scan# 90

Delta R.T. -0.000 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14

Instrument :

MSVOA_Y

ClientSampleId :

UST-7-NORTH-SIDEWALL





Tgt Ion: 42 Resp: 202

Ion Ratio Lower Upper

42 100

72 0.0 30.3 45.5#

71 0.0 29.0 43.4#

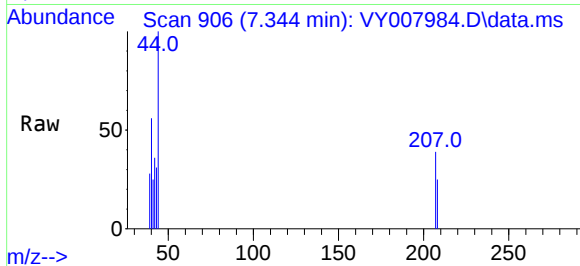

#31

Cyclohexane

Concen: Below Cal

RT: 7.795 min Scan# 980

Delta R.T. 0.012 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14




Tgt Ion: 56 Resp: 2620


Ion Ratio Lower Upper

56 100

69 82.6 26.7 40.1#

84 118.3 67.2 100.8#

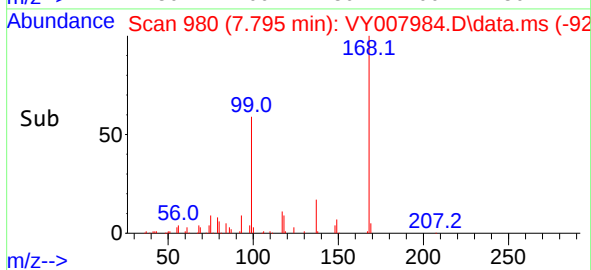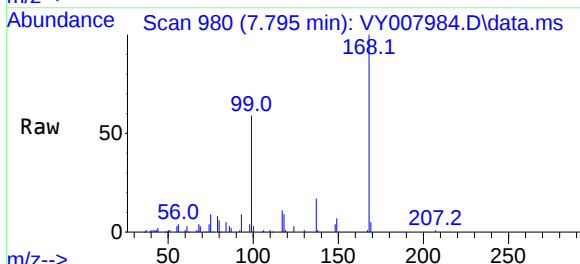

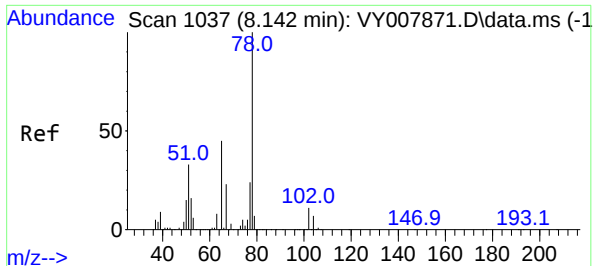

#33

1,2-Dichloroethane-d4

Concen: 44.814 ug/l

RT: 8.143 min Scan# 1037

Delta R.T. 0.006 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14

Instrument :

MSVOA_Y

ClientSampleId :





UST-7-NORTH-SIDEWALL

Tgt Ion: 65 Resp: 31824

Ion Ratio Lower Upper

65 100

67 55.8 0.0 99.4

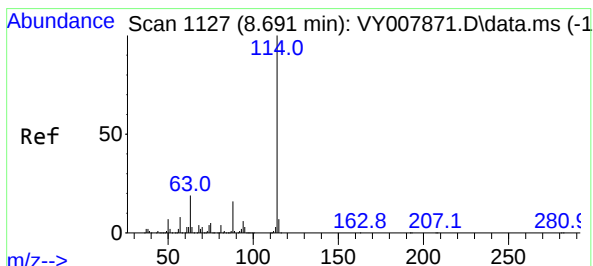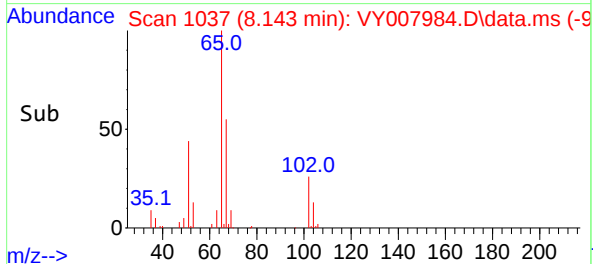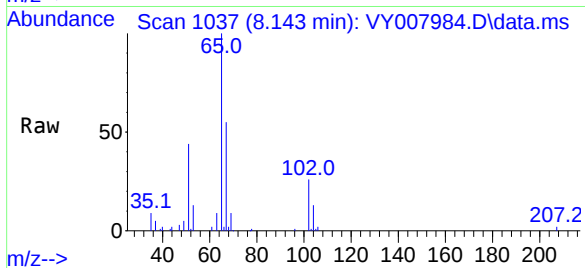

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14




Tgt Ion: 114 Resp: 109143


Ion Ratio Lower Upper

114 100

63 20.4 0.0 43.2

88 15.4 0.0 31.8


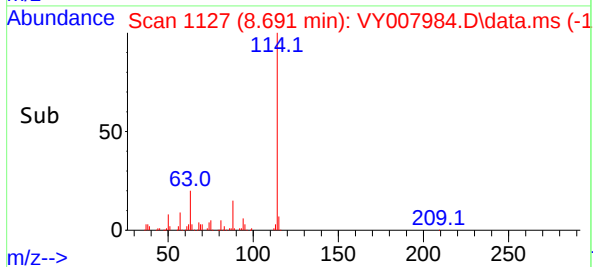

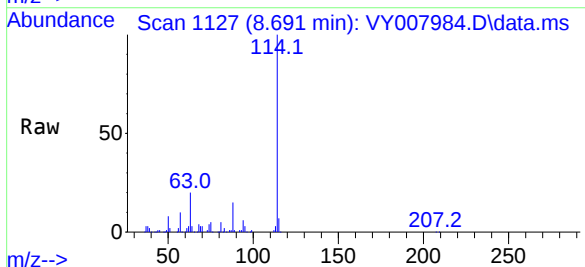




#35
Dibromofluoromethane
Concen: 41.726 ug/l
RT: 7.722 min Scan# 90
Delta R.T. 0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion:113 Resp: 31983
Ion Ratio Lower Upper
113 100
111 102.0 82.6 124.0
192 16.6 17.6 26.4#

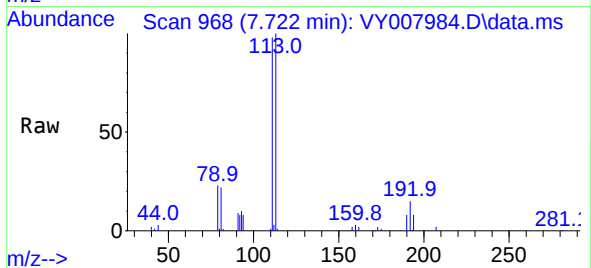

#36
1,1-Dichloropropene
Concen: 5.088 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.134 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 75 Resp: 5784
Ion Ratio Lower Upper
75 100
110 6.3 17.1 51.2#
77 0.0 24.4 36.6#


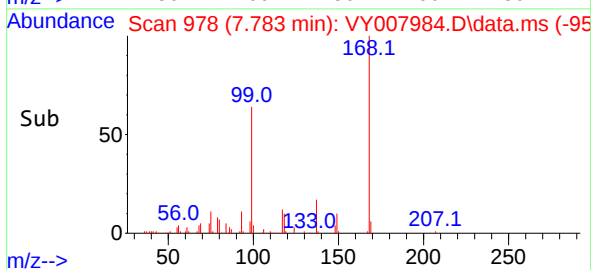






#38
Carbon Tetrachloride
Concen: 5.733 ug/l
RT: 7.795 min Scan# 91
Delta R.T. -0.104 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion:117 Resp: 6965
Ion Ratio Lower Upper
117 100
119 4.5 77.9 116.9#
121 0.0 24.8 37.2#



#39
Methylcyclohexane
Concen: 2.225 ug/l
RT: 9.191 min Scan# 1209
Delta R.T. 0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 83 Resp: 6660
Ion Ratio Lower Upper
83 100
55 64.4 66.5 99.7#
98 38.5 37.9 56.9

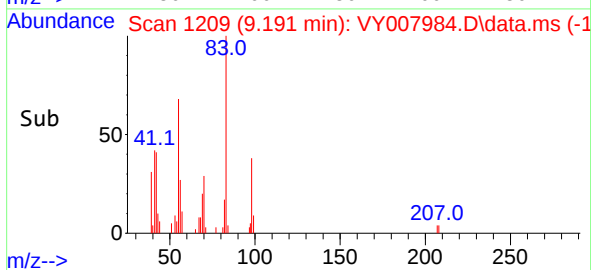

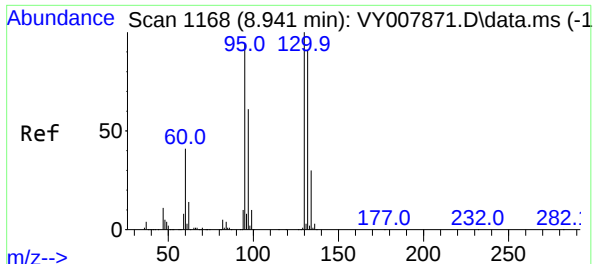

#44

Trichloroethene

Concen: 1.698 ug/l

RT: 8.941 min Scan# 1168

Delta R.T. -0.000 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14

Instrument :

MSVOA_Y

ClientSampleId :





UST-7-NORTH-SIDEWALL

Tgt Ion:130 Resp: 1560

Ion Ratio Lower Upper

130 100

95 119.6 0.0 188.2

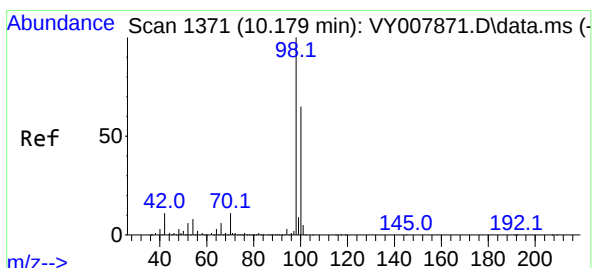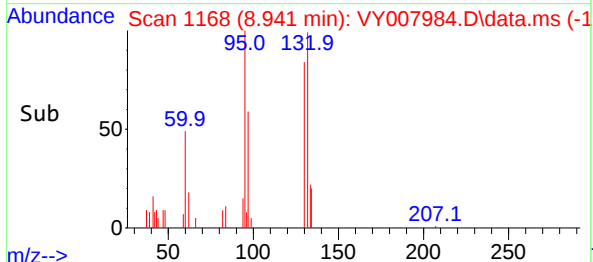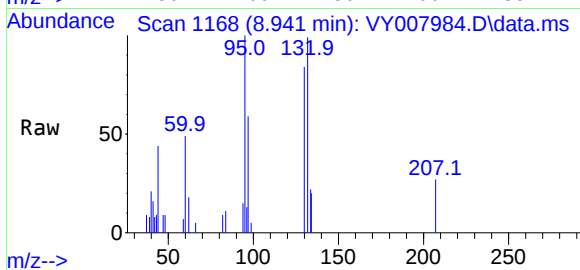

#50

Toluene-d8

Concen: 56.679 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY007984.D




Acq: 22 Mar 2022 04:14


Tgt Ion: 98 Resp: 129352

Ion Ratio Lower Upper

98 100

100 63.5 50.2 75.2

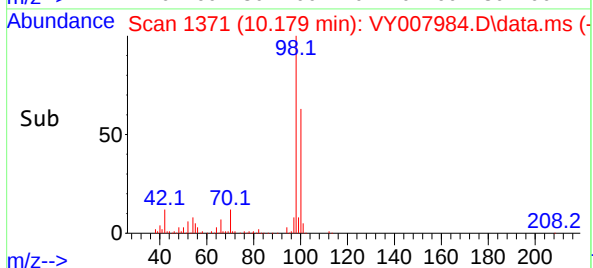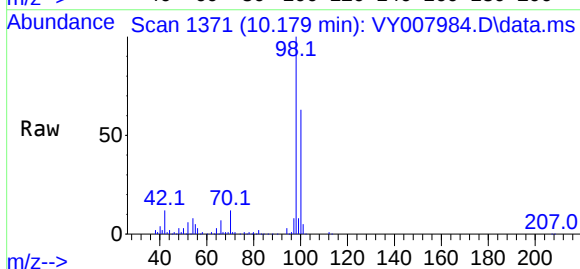







#55
1,1,2-Trichloroethane
Concen: 4.847 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.024 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Tgt Ion: 97 Resp: 3544




Ion	Ratio	Lower	Upper
97	100		
83	7.7	69.8	104.8#
85	4.7	44.3	66.5#
99	0.0	49.8	74.6#

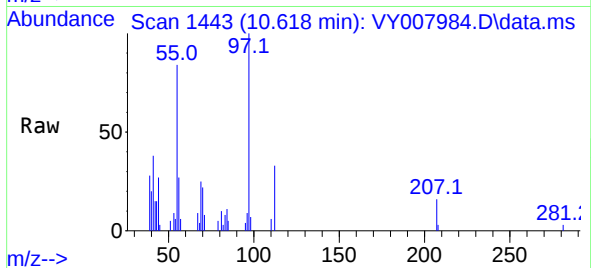


#56
Ethyl methacrylate
Concen: 2.053 ug/l
RT: 10.520 min Scan# 1427
Delta R.T. 0.012 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 69 Resp: 2155

Ion	Ratio	Lower	Upper
69	100		
41	203.2	63.4	95.0#
39	83.1	35.8	53.8#


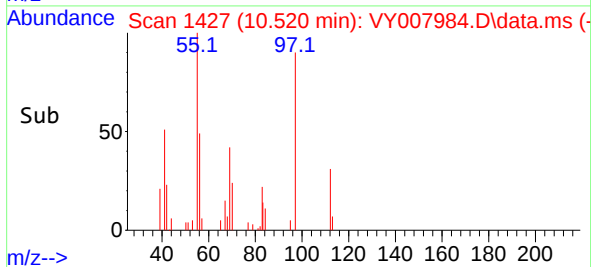

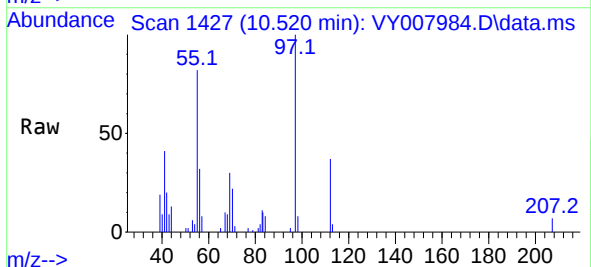




#59
2-Hexanone
Concen: 13.174 ug/l
RT: 10.801 min Scan# 1473
Delta R.T. -0.031 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion: 43 Resp: 6638
Ion Ratio Lower Upper
43 100
58 3.2 24.4 73.4#



#60
Dibromochloromethane
Concen: 52.048 ug/l
RT: 10.715 min Scan# 1459
Delta R.T. -0.268 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion:129 Resp: 45575
Ion Ratio Lower Upper
129 100
127 0.2 38.7 116.1#


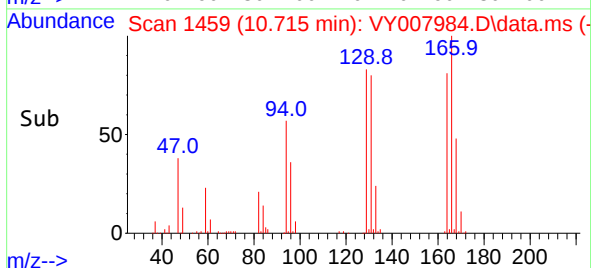
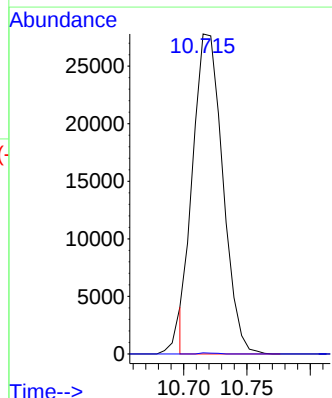





#62
4-Bromofluorobenzene
Concen: 35.370 ug/l
RT: 12.477 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion: 95 Resp: 38910
Ion Ratio Lower Upper
95 100
174 65.5 0.0 177.0
176 65.1 0.0 175.8

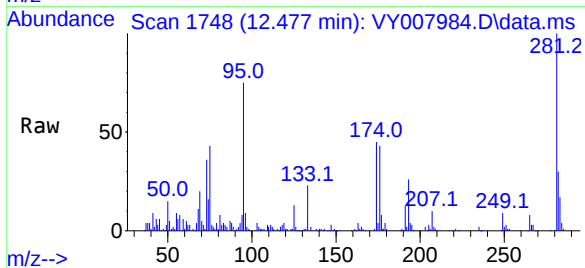

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 117 Resp: 83946
Ion Ratio Lower Upper
117 100
82 55.0 43.0 64.4
119 30.5 25.4 38.0

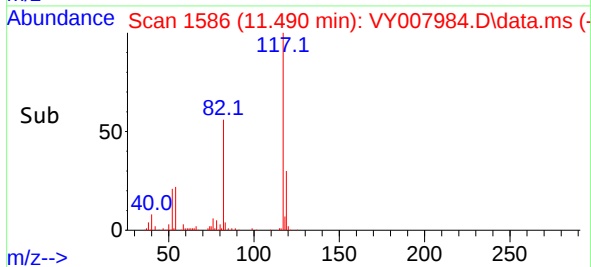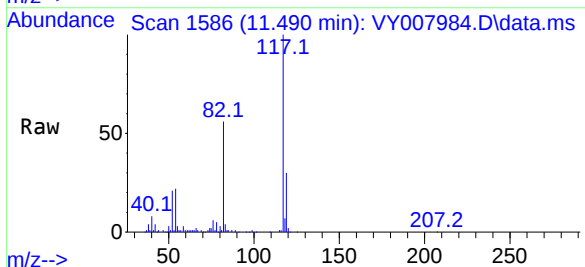







#64
Tetrachloroethene
Concen: 75.798 ug/l
RT: 10.721 min Scan# 1460
Delta R.T. -0.000 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Tgt Ion:164 Resp: 49514




Ion	Ratio	Lower	Upper
164	100		
166	120.7	100.4	150.6
129	96.2	71.4	107.0
131	87.3	70.8	106.2

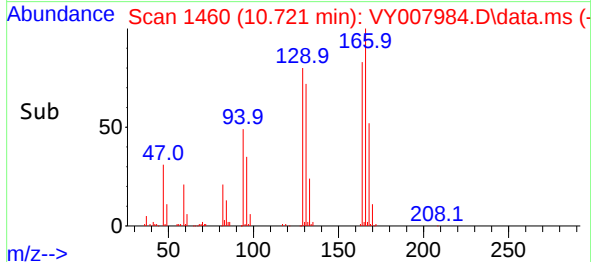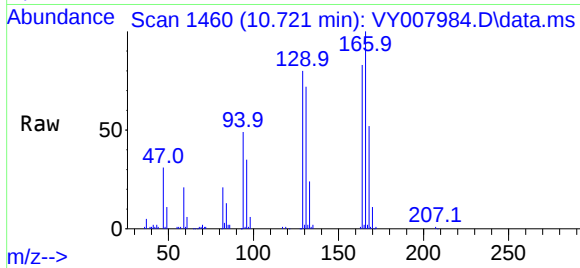


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion:152 Resp: 28880

Ion	Ratio	Lower	Upper
152	100		
115	61.0	28.2	84.7
150	151.3	0.0	347.6

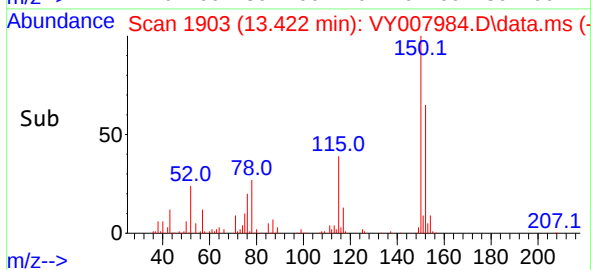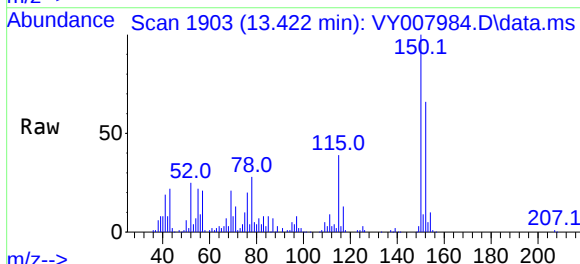







#74
N-amy1 acetate
Concen: 29.906 ug/l
RT: 12.124 min Scan# 1
Delta R.T. -0.018 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Tgt Ion: 43 Resp: 22429




Ion	Ratio	Lower	Upper
43	100		
70	8.0	28.7	43.1#
55	12.0	17.3	25.9#
61	0.0	17.0	25.6#

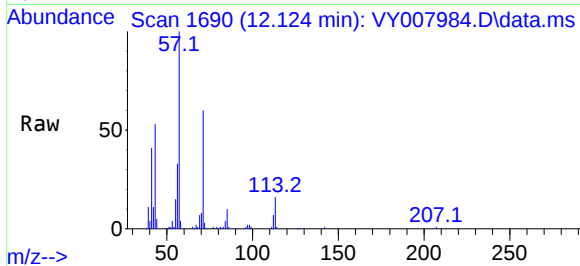


#75
1,1,2,2-Tetrachloroethane
Concen: 6.075 ug/l
RT: 12.550 min Scan# 1760
Delta R.T. -0.031 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 83 Resp: 3324

Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.6	16.8#
85	0.0	32.3	96.8#


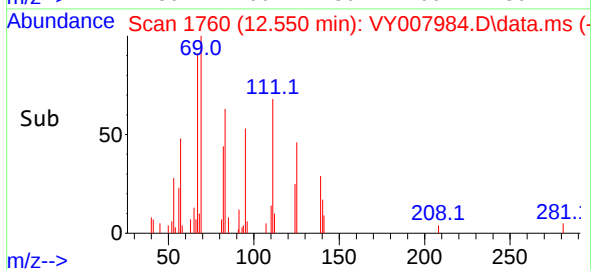

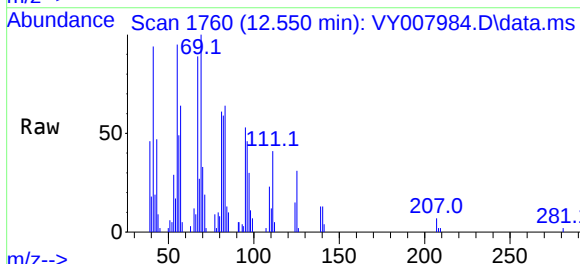




#76
1,2,3-Trichloropropane
Concen: 55.440 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion: 75 Resp: 22821
Ion Ratio Lower Upper
75 100
77 4.4 0.0 0.0#

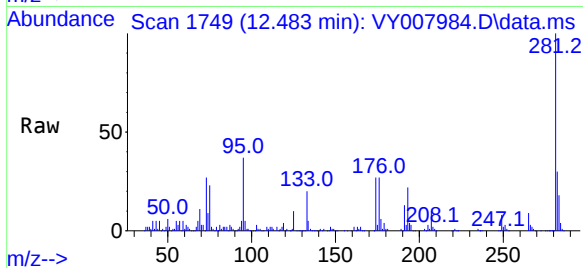

#81
trans-1,4-Dichloro-2-butene
Concen: 116.446 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.104 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 75 Resp: 22821
Ion Ratio Lower Upper
75 100
53 2.7 85.3 127.9#
89 5.7 37.0 55.4#


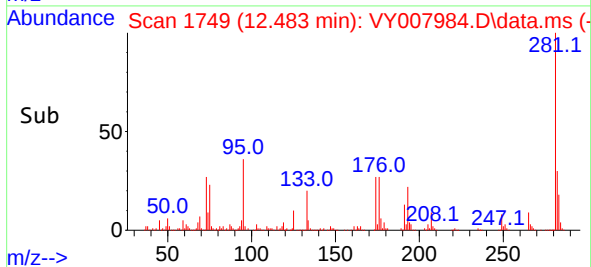

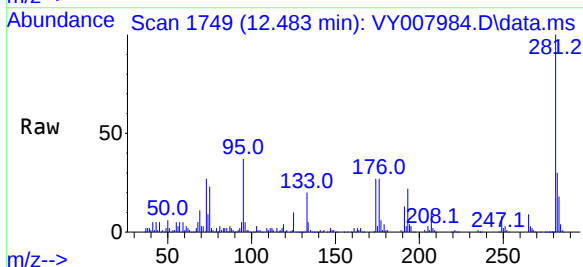




#84
1,2,4-Trimethylbenzene
Concen: 1.070 ug/l
RT: 12.971 min Scan# 1829
Delta R.T. -0.152 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14




Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL


Tgt Ion:105 Resp: 2192
Ion Ratio Lower Upper
105 100
120 34.5 22.3 66.9

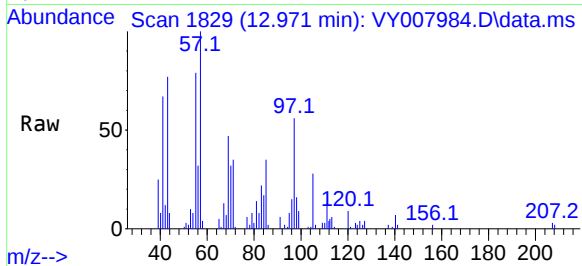

#85
sec-Butylbenzene
Concen: 1.179 ug/l
RT: 13.251 min Scan# 1875
Delta R.T. -0.000 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion:105 Resp: 3305
Ion Ratio Lower Upper
105 100
134 29.2 10.2 30.4

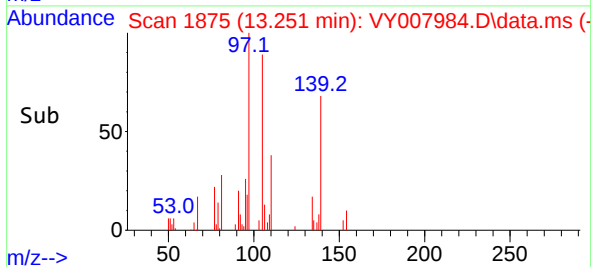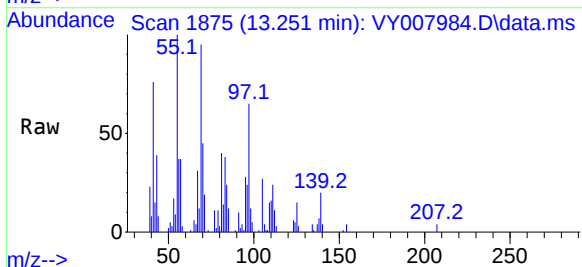



#89

n-Butylbenzene

Concen: 1.169 ug/l

RT: 13.696 min Scan# 1948

Delta R.T. -0.000 min

Lab File: VY007984.D

Acq: 22 Mar 2022 04:14

Instrument :

MSVOA_Y

ClientSampleId :

UST-7-NORTH-SIDEWALL





Tgt Ion: 91 Resp: 2554

Ion Ratio Lower Upper

91 100

92 49.9 26.3 78.9

134 0.0 13.0 38.9#

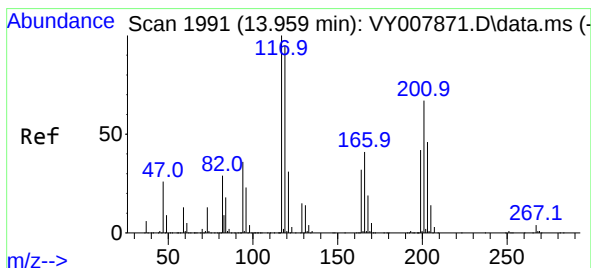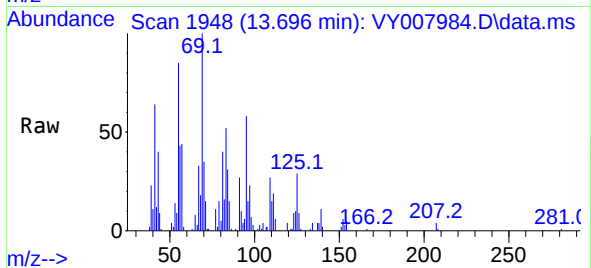

#90

Hexachloroethane

Concen: 2.514 ug/l

RT: 13.971 min Scan# 1993

Delta R.T. 0.006 min

Lab File: VY007984.D




Acq: 22 Mar 2022 04:14


Tgt Ion: 117 Resp: 1142

Ion Ratio Lower Upper

117 100

201 0.0 43.0 128.8#


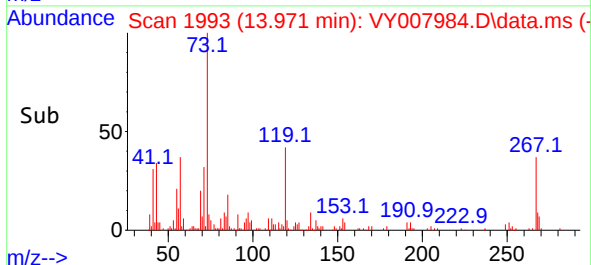

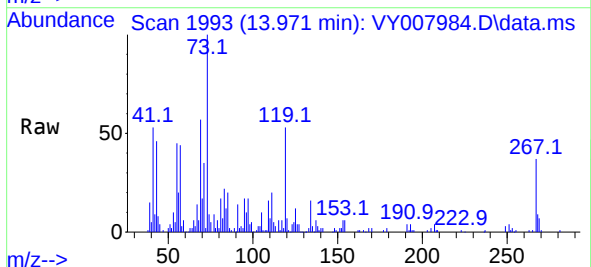




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.009 ug/l
RT: 14.385 min Scan# 2056
Delta R.T. 0.030 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Instrument :
MSVOA_Y
ClientSampleId :
UST-7-NORTH-SIDEWALL

Tgt Ion: 75 Resp: 95
Ion Ratio Lower Upper
75 100
155 31.6 38.0 113.9#
157 0.0 47.8 143.3#

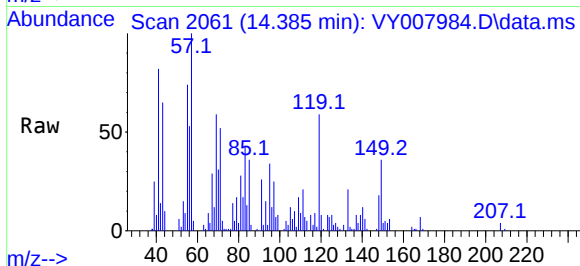

#96
1,2,3-Trichlorobenzene
Concen: 1.120 ug/l
RT: 15.446 min Scan# 2235
Delta R.T. 0.018 min
Lab File: VY007984.D
Acq: 22 Mar 2022 04:14

Tgt Ion: 180 Resp: 637
Ion Ratio Lower Upper
180 100
182 0.0 47.3 141.9#
145 845.1 15.3 45.9#

