

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032122\
 Data File : VY007965.D
 Acq On : 21 Mar 2022 19:19
 Operator : SY/MD
 Sample : N2001-01
 Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 D-14A

Quant Time: Mar 22 03:41:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 13:55:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	243173	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	466819	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	432634	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	182977	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	165285	59.613	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	119.220%
35) Dibromofluoromethane	7.716	113	146899	44.808	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	89.620%
50) Toluene-d8	10.179	98	579154	59.633	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	119.260%
62) 4-Bromofluorobenzene	12.483	95	202080	42.948	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	85.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032122\
Data File : VY007965.D
Acq On : 21 Mar 2022 19:19
Operator : SY/MD
Sample : N2001-01
Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
D-14A

Quant Time: Mar 22 03:41:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y031722S.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 13:55:34 2022
Response via : Initial Calibration




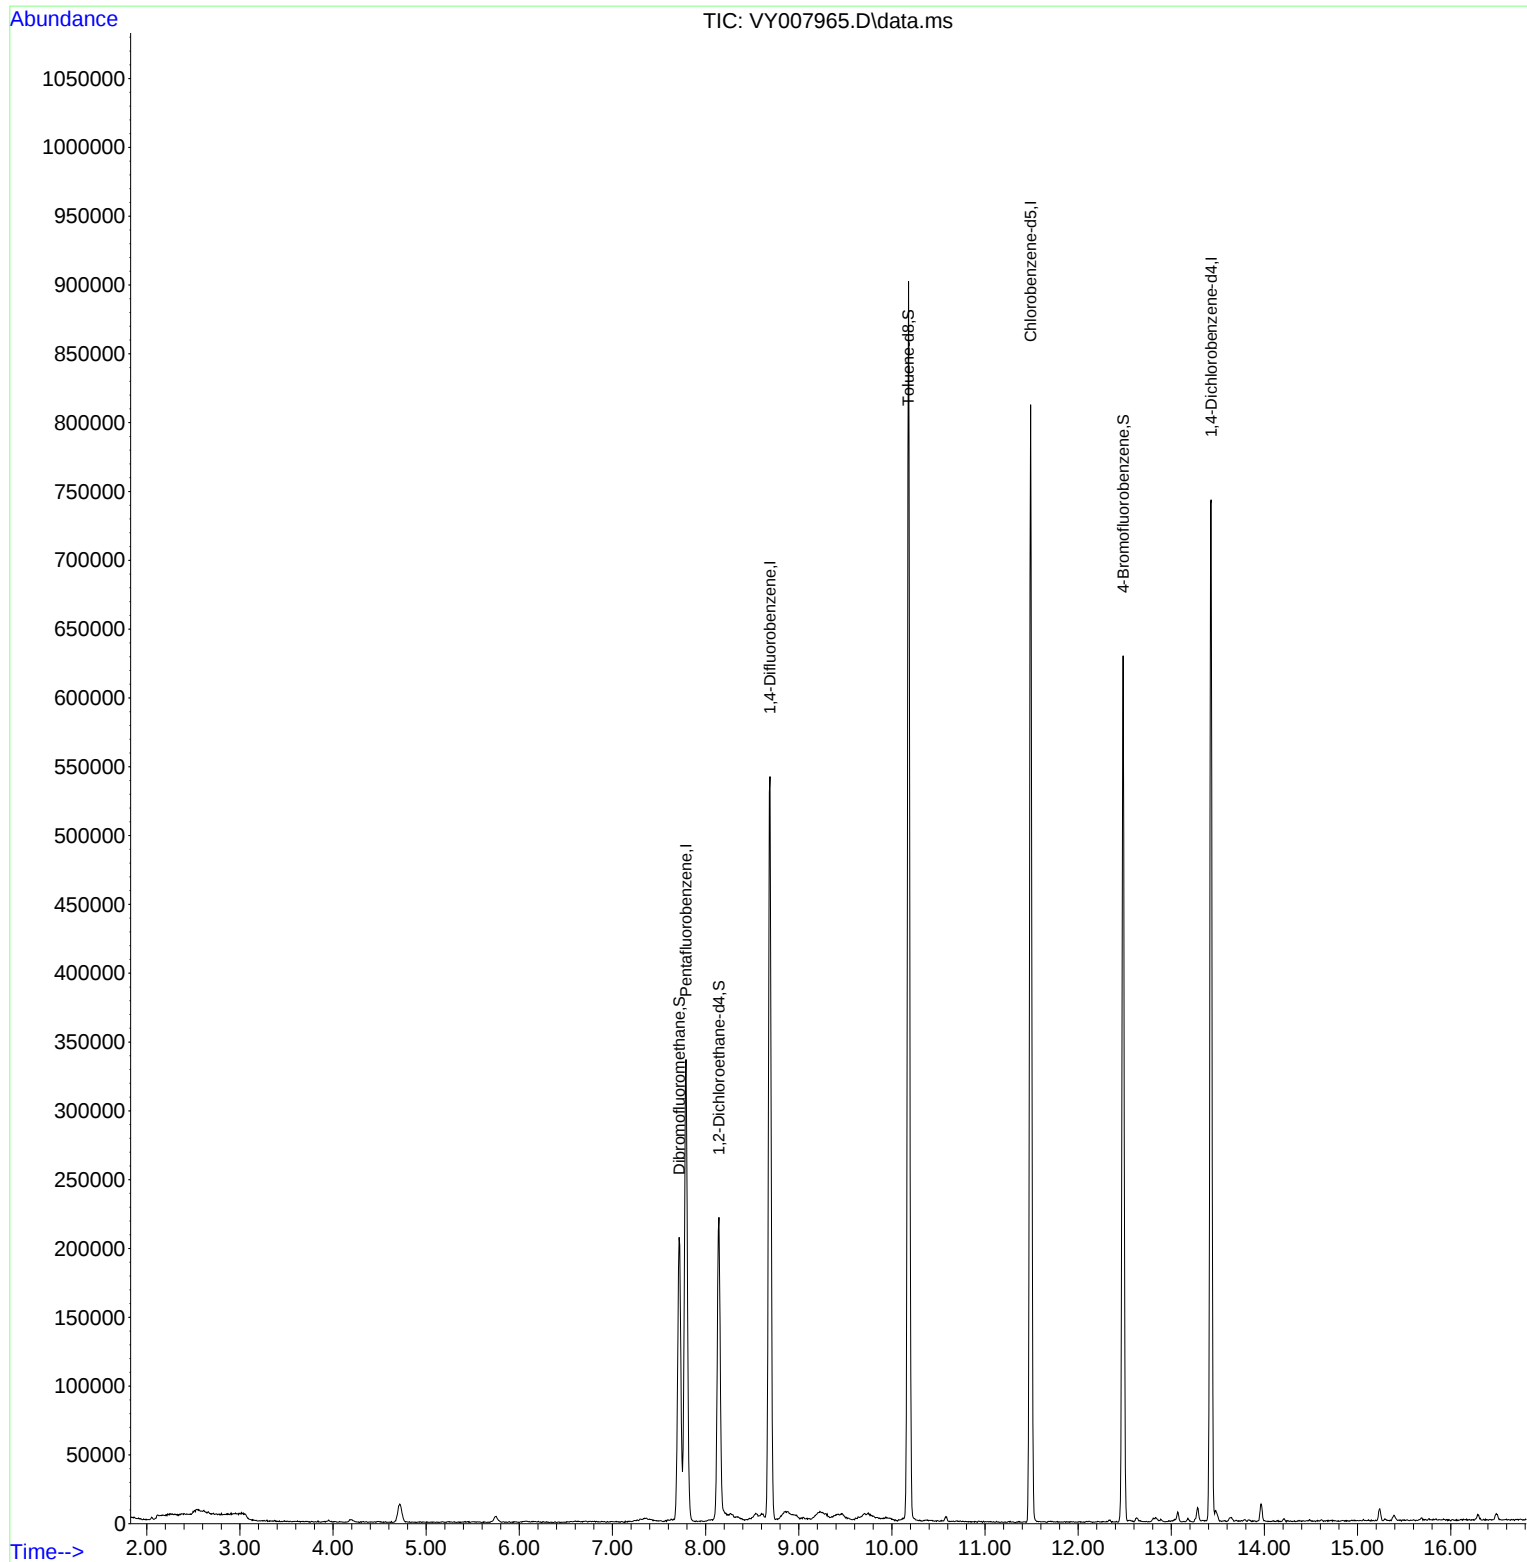


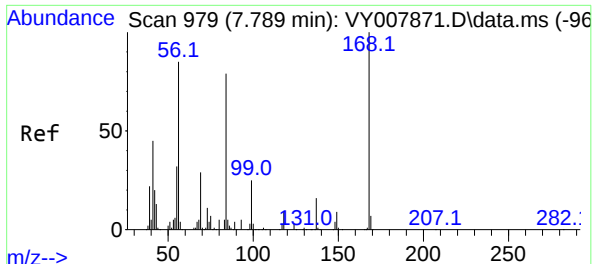

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19




Instrument :
MSVOA_Y
ClientSampleId :
D-14A


Tgt Ion:168 Resp: 243173
Ion Ratio Lower Upper
168 100
99 62.5 46.9 70.3

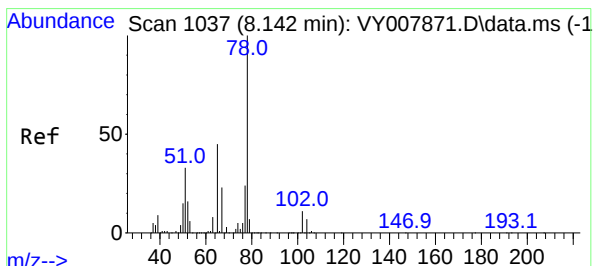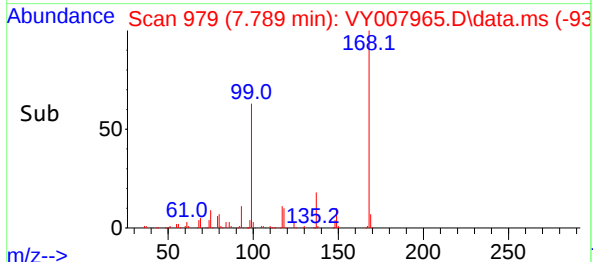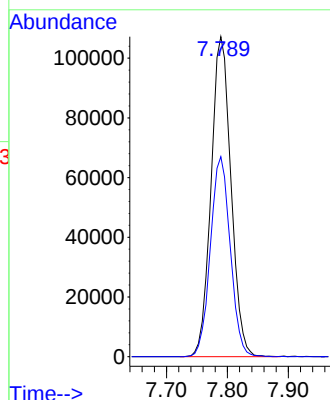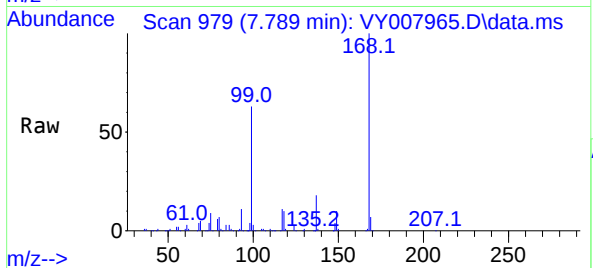

#33
1,2-Dichloroethane-d4
Concen: 59.613 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19

Tgt Ion: 65 Resp: 165285
Ion Ratio Lower Upper
65 100
67 53.2 0.0 99.4


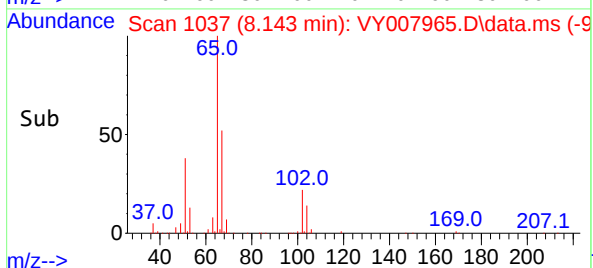
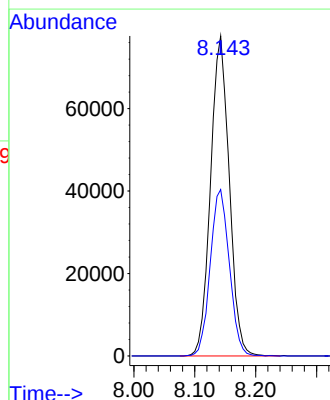
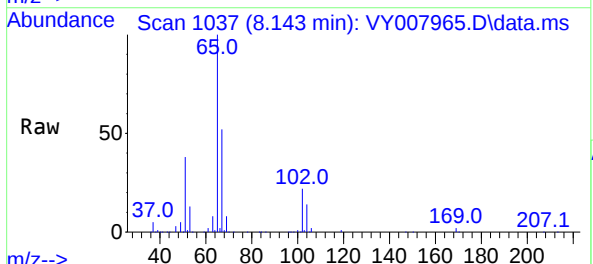


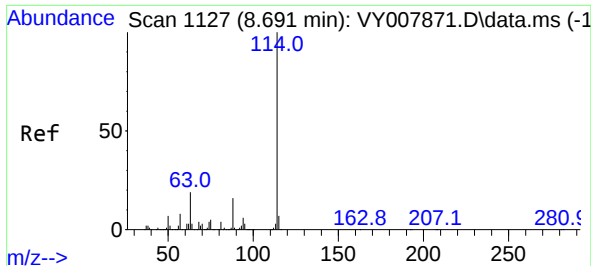

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19




Instrument :
MSVOA_Y
ClientSampleId :
D-14A


Tgt Ion:114 Resp: 466819
Ion Ratio Lower Upper
114 100
63 20.1 0.0 43.2
88 16.2 0.0 31.8

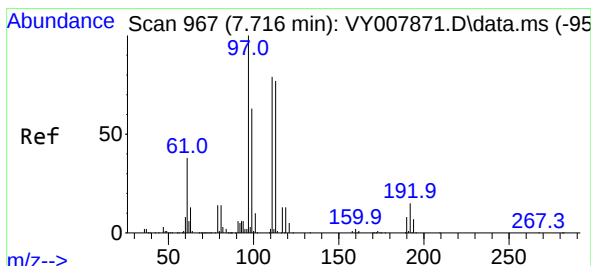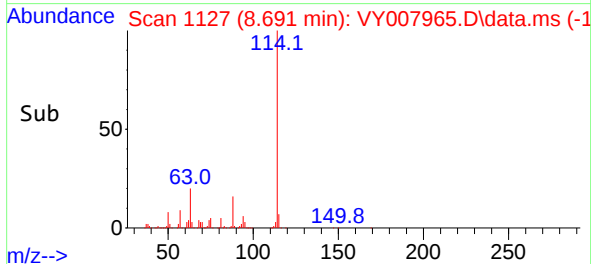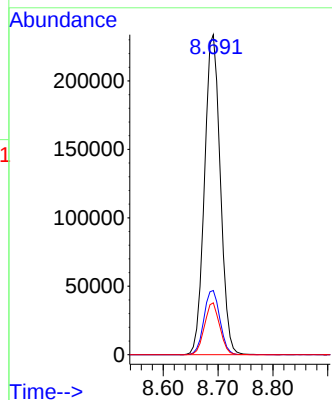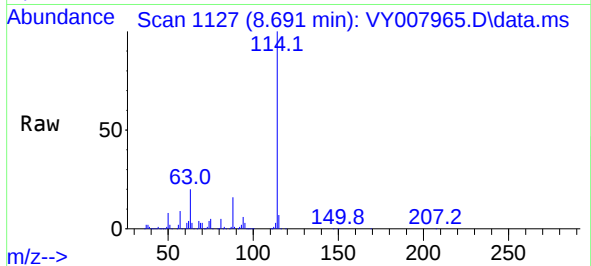

#35
Dibromofluoromethane
Concen: 44.808 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19

Tgt Ion:113 Resp: 146899
Ion Ratio Lower Upper
113 100
111 102.0 82.6 124.0
192 16.5 17.6 26.4#


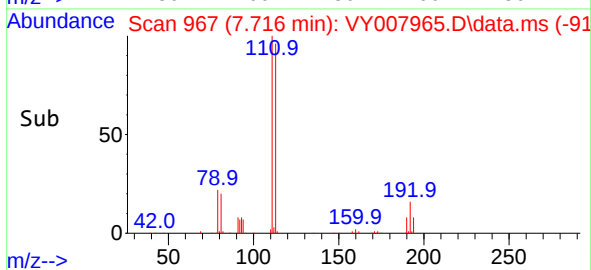
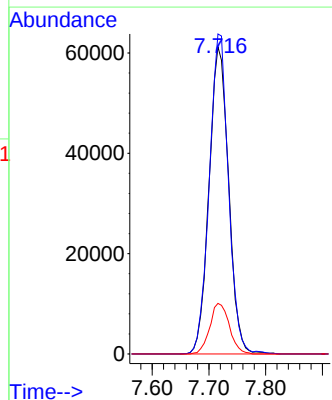
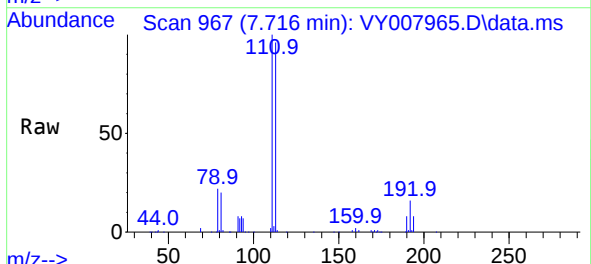


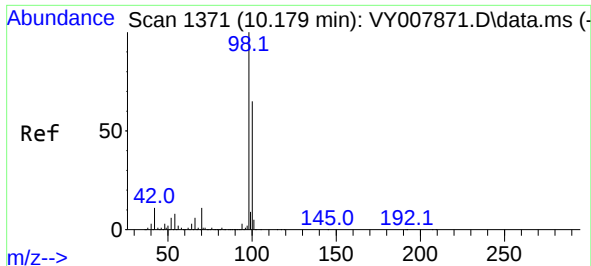

#50
Toluene-d8
Concen: 59.633 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19




Instrument :
MSVOA_Y
ClientSampleId :
D-14A


Tgt Ion: 98 Resp: 579154
Ion Ratio Lower Upper
98 100
100 65.1 50.2 75.2

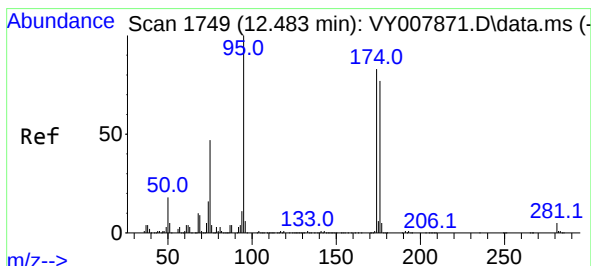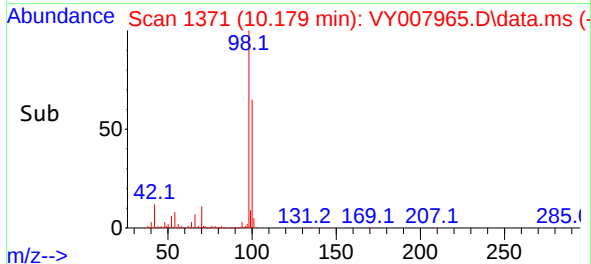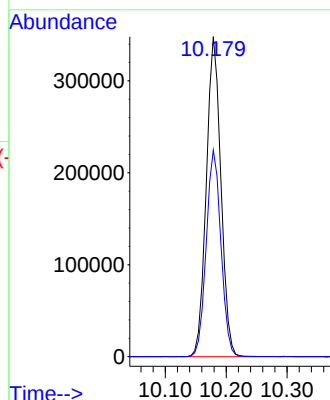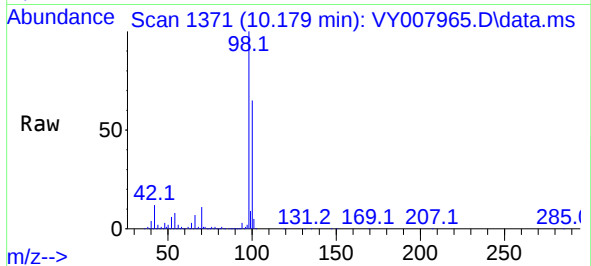

#62
4-Bromofluorobenzene
Concen: 42.948 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19

Tgt Ion: 95 Resp: 202080
Ion Ratio Lower Upper
95 100
174 71.3 0.0 177.0
176 68.9 0.0 175.8


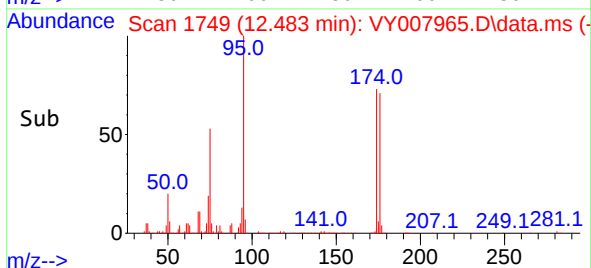
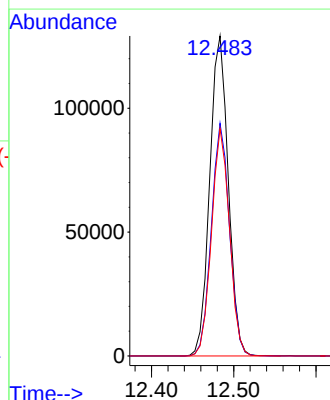
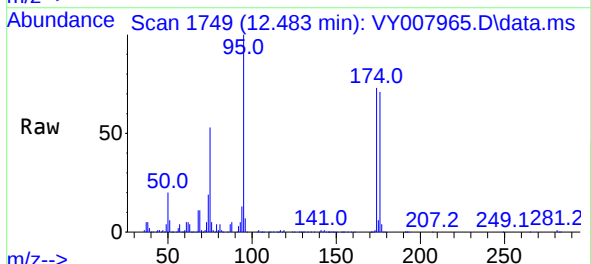


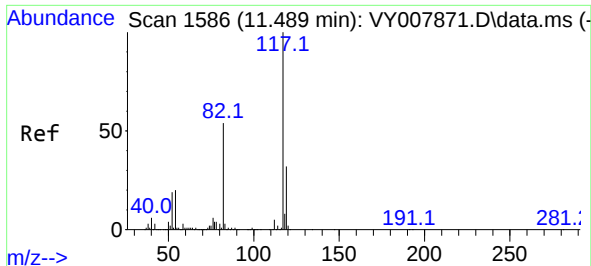

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19

Instrument :
MSVOA_Y
ClientSampleId :
D-14A

Tgt Ion:117 Resp: 432634
Ion Ratio Lower Upper
117 100
82 58.0 43.0 64.4
119 32.4 25.4 38.0

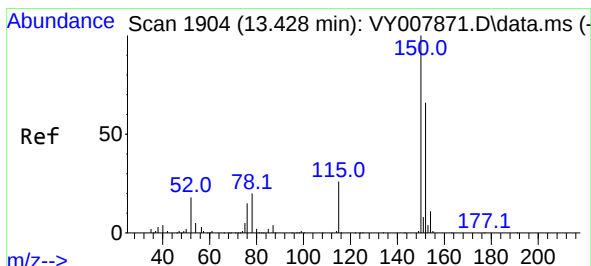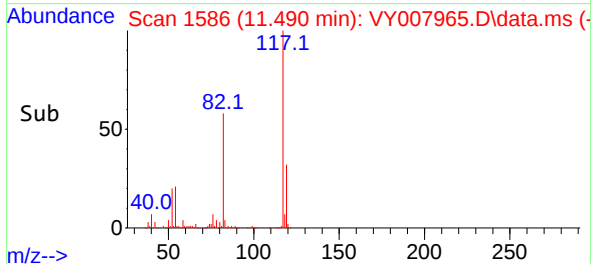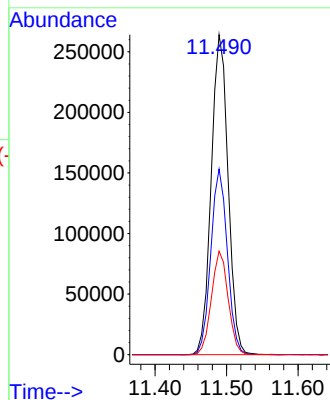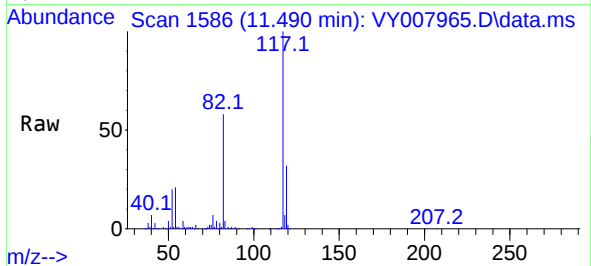

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY007965.D
Acq: 21 Mar 2022 19:19

Tgt Ion:152 Resp: 182977
Ion Ratio Lower Upper
152 100
115 62.5 28.2 84.7
150 159.3 0.0 347.6

