

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032825\
 Data File : VY021705.D
 Acq On : 28 Mar 2025 20:19
 Operator : SY/MD
 Sample : Q1664-21
 Misc : 5.14g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P001-BBDGA-008-01

Quant Time: Mar 28 23:49:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.713	168	212653	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	414302	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	380711	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	149200	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	129845	56.356	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	=	112.720%	
35) Dibromofluoromethane	7.634	113	138793	51.644	ug/l	0.00
Spiked Amount	50.000	Range 54 - 147	Recovery	=	103.280%	
50) Toluene-d8	10.109	98	512383	50.115	ug/l	0.00
Spiked Amount	50.000	Range 58 - 134	Recovery	=	100.240%	
62) 4-Bromofluorobenzene	12.408	95	156217	45.172	ug/l	0.00
Spiked Amount	50.000	Range 30 - 143	Recovery	=	90.340%	
Target Compounds						
20) Methylene Chloride	4.622	84	25093	7.595	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032825\
Data File : VY021705.D
Acq On : 28 Mar 2025 20:19
Operator : SY/MD
Sample : Q1664-21
Misc : 5.14g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P001-BBDGA-008-01

Quant Time: Mar 28 23:49:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




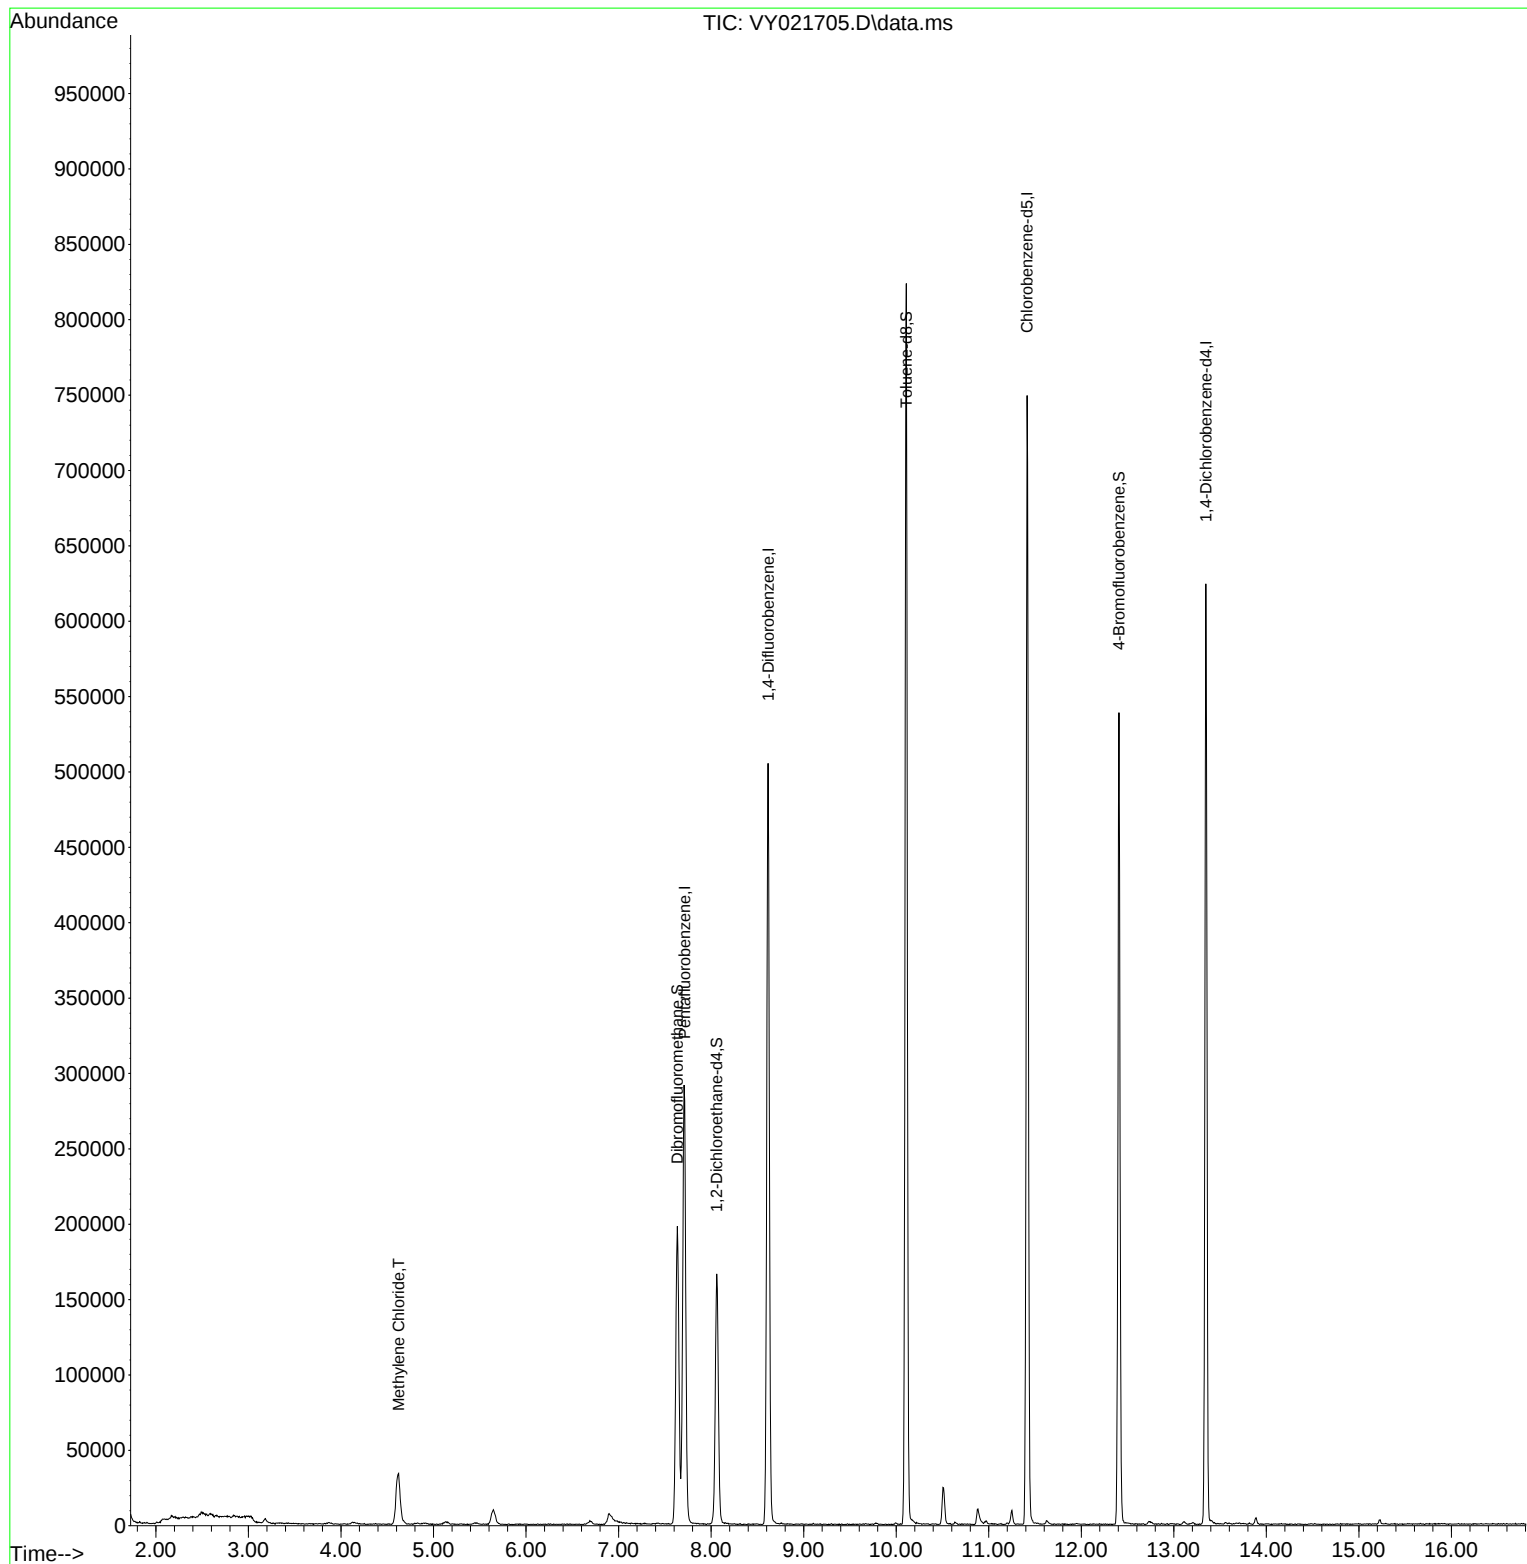


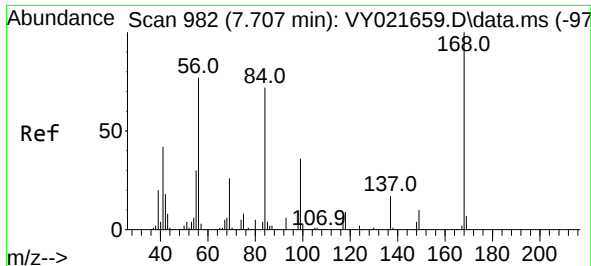

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19




Instrument :
MSVOA_Y
ClientSampleId :
P001-BBDGA-008-01


Tgt Ion:168 Resp: 212653
Ion Ratio Lower Upper
168 100
99 58.5 46.7 70.1

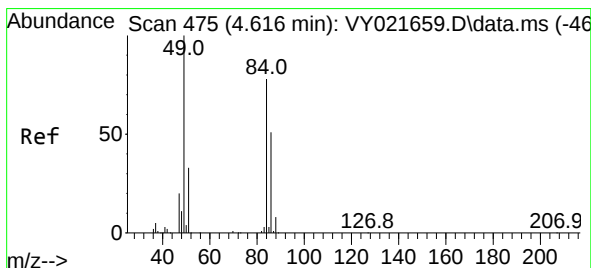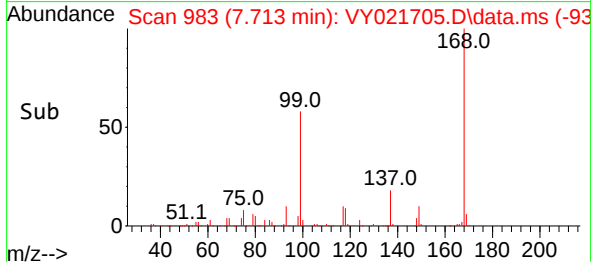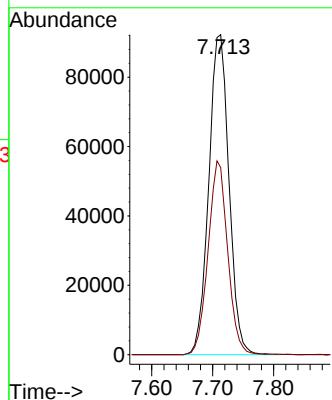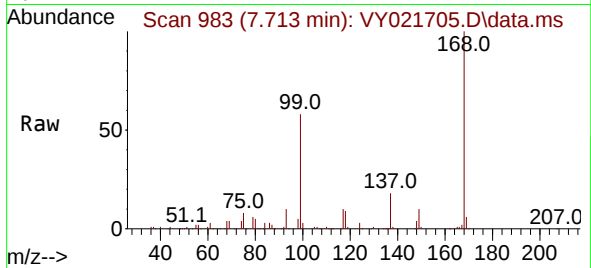

#20
Methylene Chloride
Concen: 7.595 ug/l
RT: 4.622 min Scan# 476
Delta R.T. 0.006 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19

Tgt Ion: 84 Resp: 25093
Ion Ratio Lower Upper
84 100
49 117.9 102.8 154.2
51 37.4 33.5 50.3
86 60.3 52.0 78.0

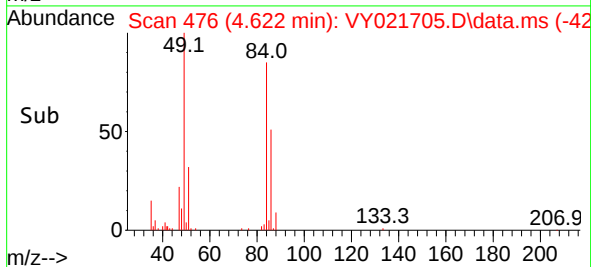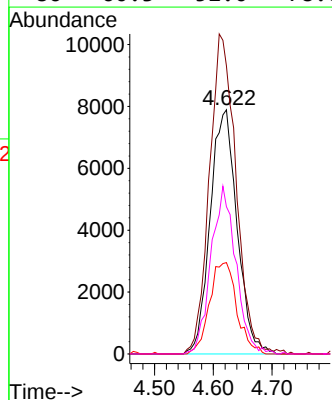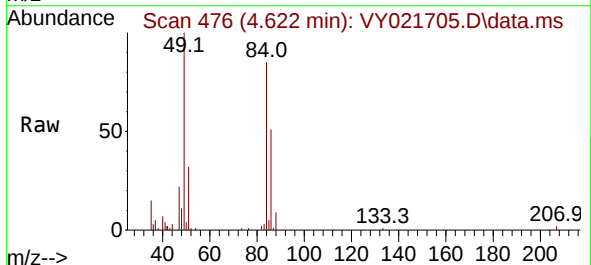

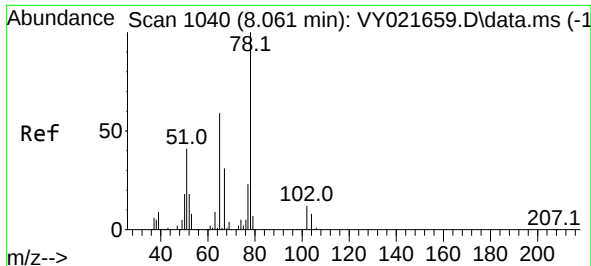

#33

1,2-Dichloroethane-d4

Concen: 56.356 ug/l

RT: 8.061 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VY021705.D

Acq: 28 Mar 2025 20:19

Instrument :

MSVOA_Y

ClientSampleId :





P001-BBDGA-008-01

Tgt Ion: 65 Resp: 129845

Ion Ratio Lower Upper

65 100

67 52.2 0.0 104.6

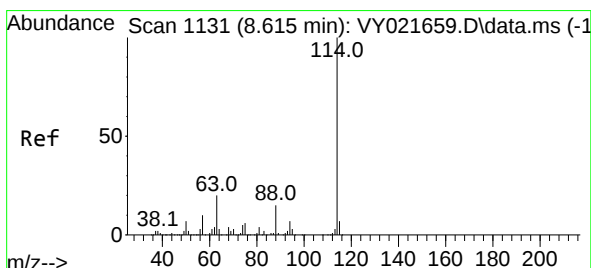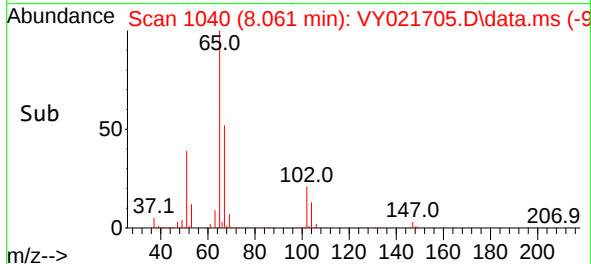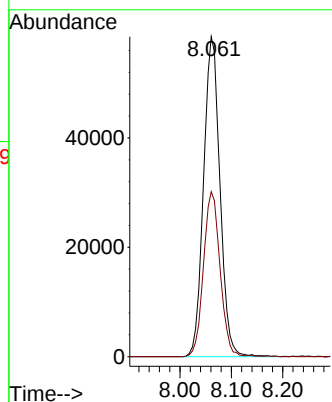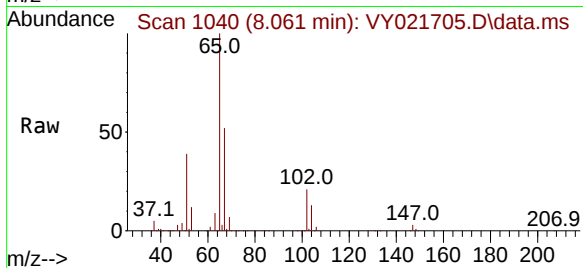

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY021705.D

Acq: 28 Mar 2025 20:19




Tgt Ion: 114 Resp: 414302


Ion Ratio Lower Upper

114 100

63 21.0 0.0 40.2

88 16.1 0.0 29.8


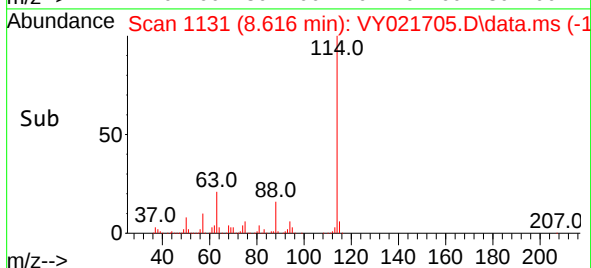
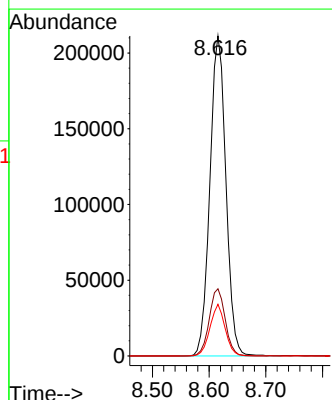
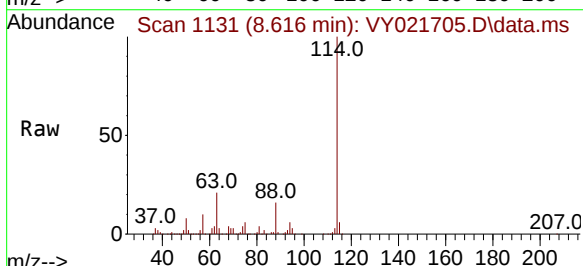


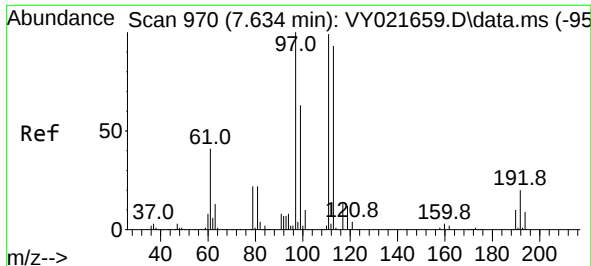

#35
Dibromofluoromethane
Concen: 51.644 ug/l
RT: 7.634 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19




Instrument :
MSVOA_Y
ClientSampleId :
P001-BBDGA-008-01


Tgt Ion:113 Resp: 138793
Ion Ratio Lower Upper
113 100
111 102.5 82.6 123.8
192 19.3 16.2 24.4

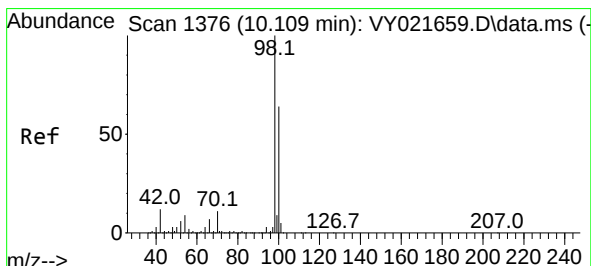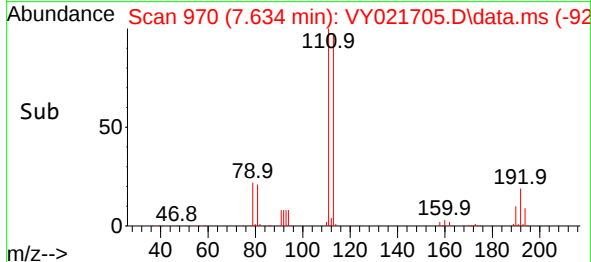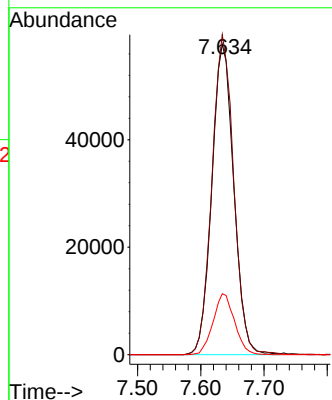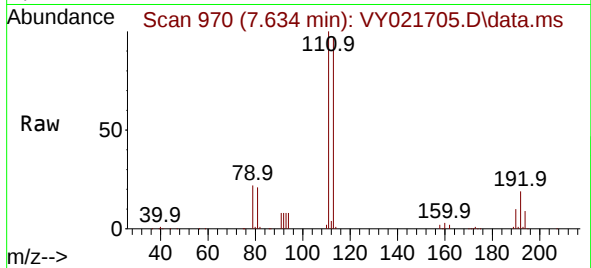

#50
Toluene-d8
Concen: 50.115 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19

Tgt Ion: 98 Resp: 512383
Ion Ratio Lower Upper
98 100
100 64.0 52.1 78.1


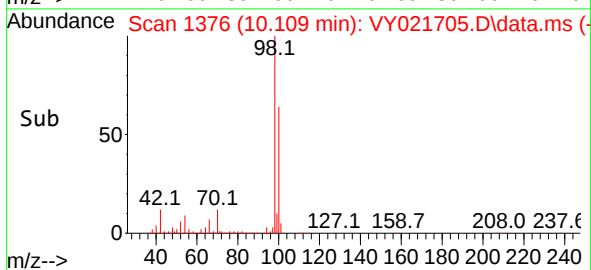
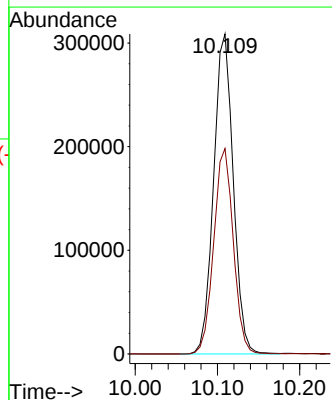
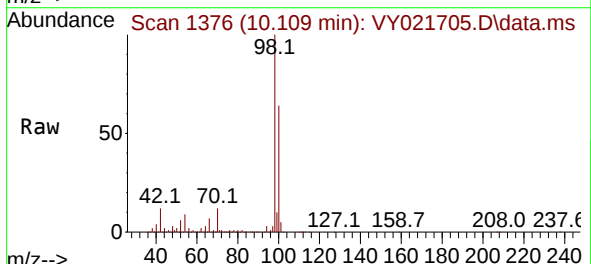


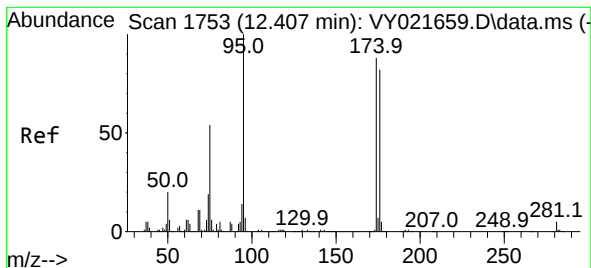

#62
4-Bromofluorobenzene
Concen: 45.172 ug/l
RT: 12.408 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19




Instrument :
MSVOA_Y
ClientSampleId :
P001-BBDGA-008-01


Tgt Ion: 95 Resp: 156217
Ion Ratio Lower Upper
95 100
174 82.5 0.0 170.8
176 79.4 0.0 162.0

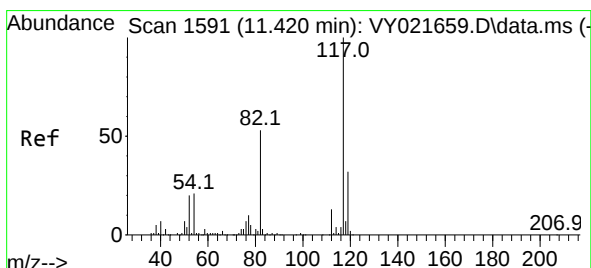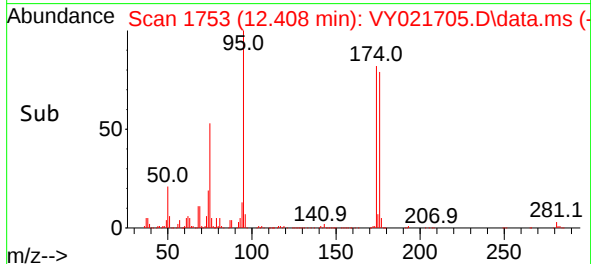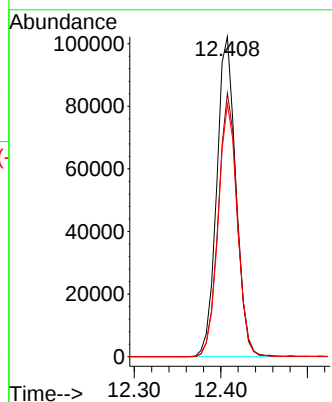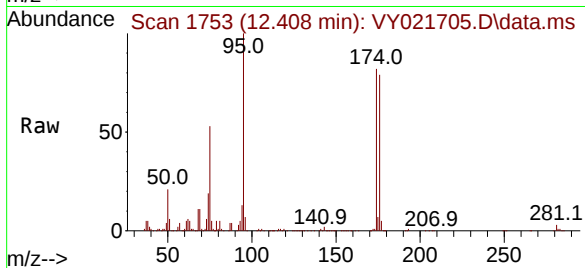

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.006 min
Lab File: VY021705.D
Acq: 28 Mar 2025 20:19


Tgt Ion: 117 Resp: 380711
Ion Ratio Lower Upper
117 100
82 55.5 42.8 64.2
119 32.2 25.7 38.5

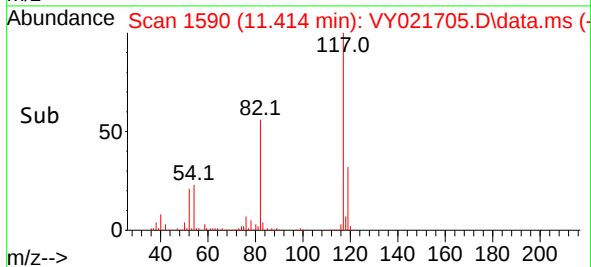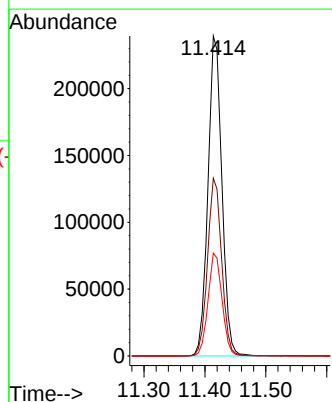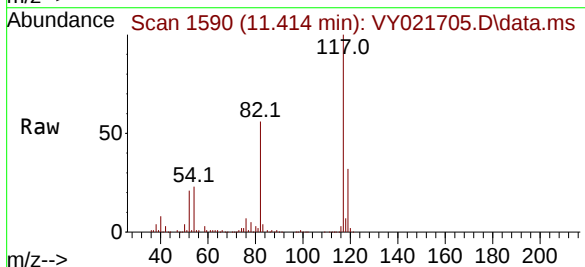

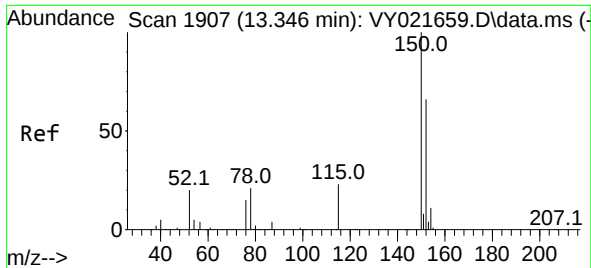

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. 0.000 min
 Lab File: VY021705.D
 Acq: 28 Mar 2025 20:19

Instrument :
 MSVOA_Y
 ClientSampleId :
 P001-BBDGA-008-01

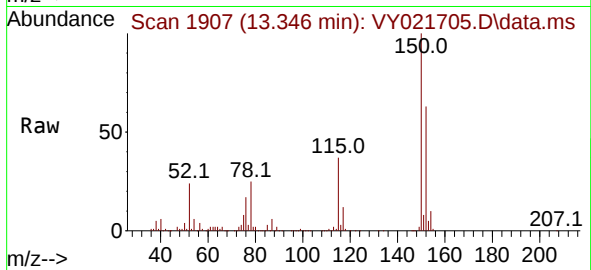

Tgt Ion:	152	Resp:	149200
Ion Ratio	Lower	Upper	
152	100		
115	59.4	28.8	86.5
150	158.3	0.0	348.4

