
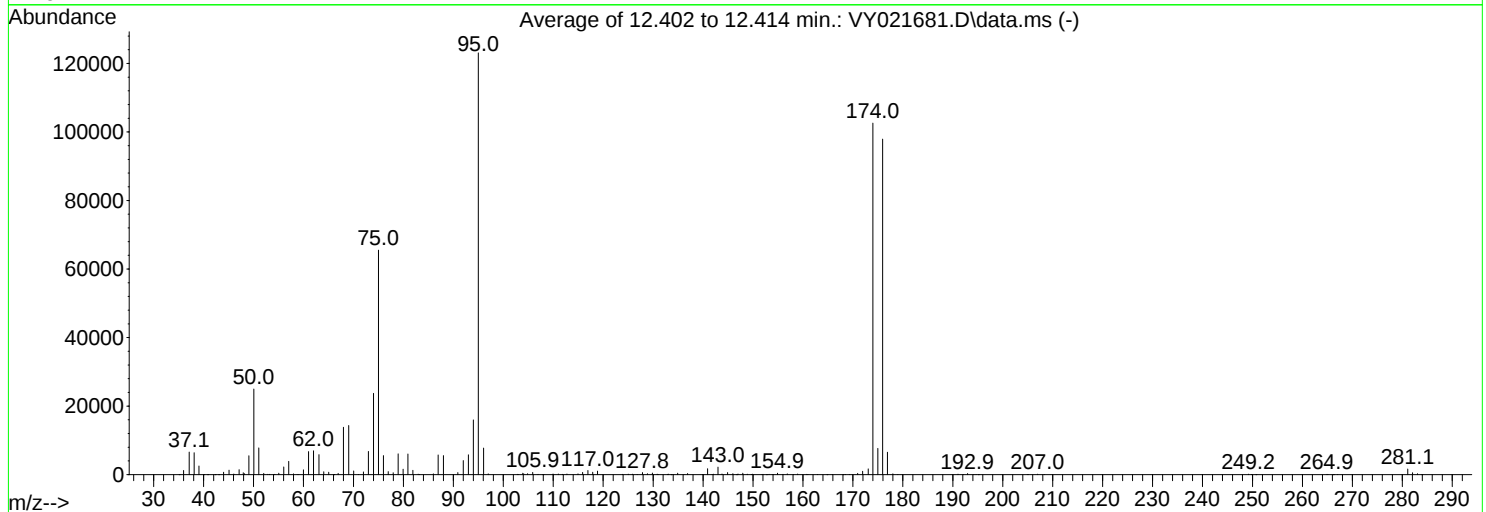


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032825\
Data File : VY021681.D
Acq On : 28 Mar 2025 10:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

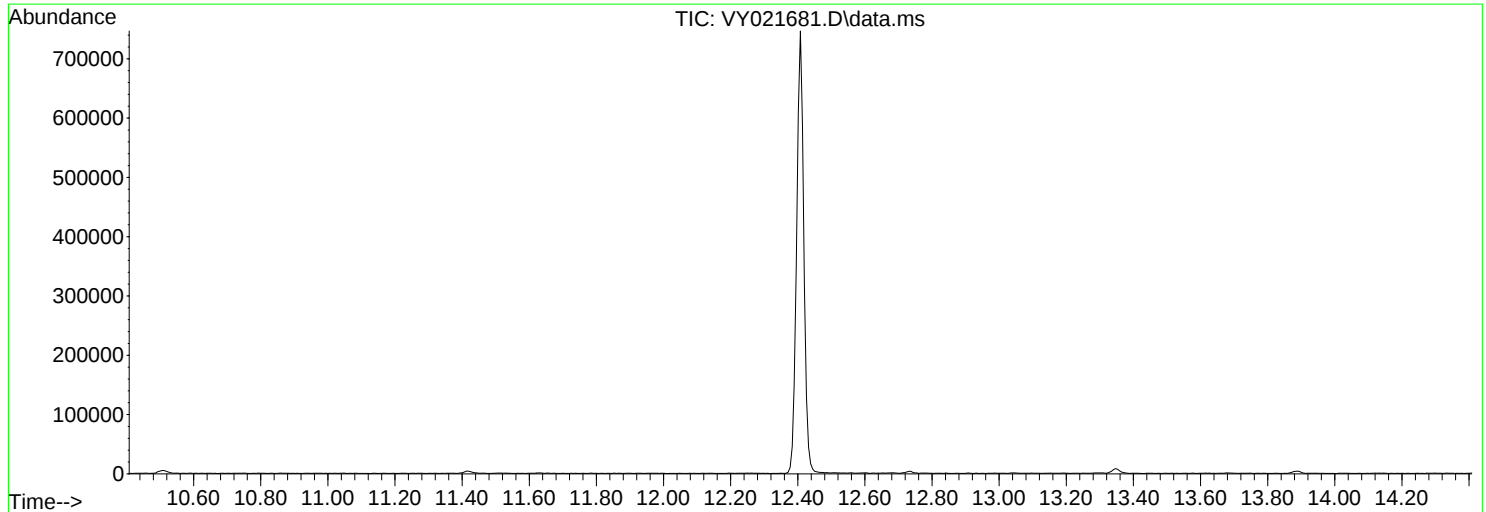

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	24984	PASS
75	95	30	60	53.2	65507	PASS
95	95	100	100	100.0	123093	PASS
96	95	5	9	6.3	7747	PASS
173	174	0.00	2	1.6	1660	PASS
174	95	50	100	83.3	102576	PASS
175	174	5	9	7.5	7678	PASS
176	174	95	101	95.5	97923	PASS
177	176	5	9	6.7	6544	PASS