

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032922\
 Data File : VY008098.D
 Acq On : 29 Mar 2022 19:33
 Operator : SY/MD
 Sample : N2106-01
 Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Mar 30 04:02:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	127905	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	229314	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	203212	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	62944	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	71764	55.923	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 111.840%			
35) Dibromofluoromethane	7.722	113	71054	49.421	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 98.840%			
50) Toluene-d8	10.179	98	274227	50.626	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 101.260%			
62) 4-Bromofluorobenzene	12.483	95	82242	43.036	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 86.080%			
Target Compounds						Qvalue
11) Tert butyl alcohol	4.954	59	166541	1250.837	ug/l #	94
13) Acrolein	3.747	56	148	1.366	ug/l #	14
14) Allyl chloride	4.412	41	11565	6.477	ug/l #	38
15) Acrylonitrile	5.161	53	6006	16.476	ug/l	94
16) Acetone	3.948	43	214406	730.966	ug/l #	88
18) Methyl Acetate	4.491	43	988	Below Cal	#	72
20) Methylene Chloride	4.722	84	5750	Below Cal	#	72
25) 2-Butanone	6.984	43	80116	179.485	ug/l #	75
29) Tetrahydrofuran	7.350	42	890	3.067	ug/l #	89
31) Cyclohexane	7.783	56	4130	1.722	ug/l #	45
36) 1,1-Dichloropropene	7.789	75	9885	4.377	ug/l #	51
37) Ethyl Acetate	6.984	43	80116	75.938	ug/l #	72
38) Carbon Tetrachloride	7.795	117	12586	5.114	ug/l #	16
40) Benzene	8.161	78	16645	2.577	ug/l	95
41) Methacrylonitrile	7.326	41	759	1.433	ug/l #	37
43) Isopropyl Acetate	8.246	43	2419	1.168	ug/l #	56
48) Methyl methacrylate	9.264	41	2016	2.198	ug/l #	44
51) 4-Methyl-2-Pentanone	10.069	43	6025	5.768	ug/l #	77
52) Toluene	10.246	92	71986	16.991	ug/l	95
59) 2-Hexanone	10.831	43	10172	13.916	ug/l	88
67) Ethyl Benzene	11.593	91	31571	3.931	ug/l	94
68) m/p-Xylenes	11.697	106	51563	16.147	ug/l	92
69) o-Xylene	12.032	106	17439	5.704	ug/l	96
74) N-amyl acetate	12.105	43	5918	5.182	ug/l #	55
76) 1,2,3-Trichloropropane	12.483	75	41741	54.400	ug/l #	100
78) n-propylbenzene	12.672	91	11429	1.865	ug/l	98
79) 2-Chlorotoluene	12.739	91	3870	1.138	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.819	105	10415	2.447	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.483	75	41741	121.376	ug/l #	7
84) 1,2,4-Trimethylbenzene	13.123	105	46719	11.272	ug/l	98
85) sec-Butylbenzene	13.123	105	46719	8.347	ug/l #	56
95) Naphthalene	15.239	128	7578	2.751	ug/l #	84
96) 1,2,3-Trichlorobenzene	15.391	180	1632	1.514	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_Y
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032922\
Data File : VY008098.D
Acq On : 29 Mar 2022 19:33
Operator : SY/MD
Sample : N2106-01
Misc : 5.06g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Mar 30 04:02:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration

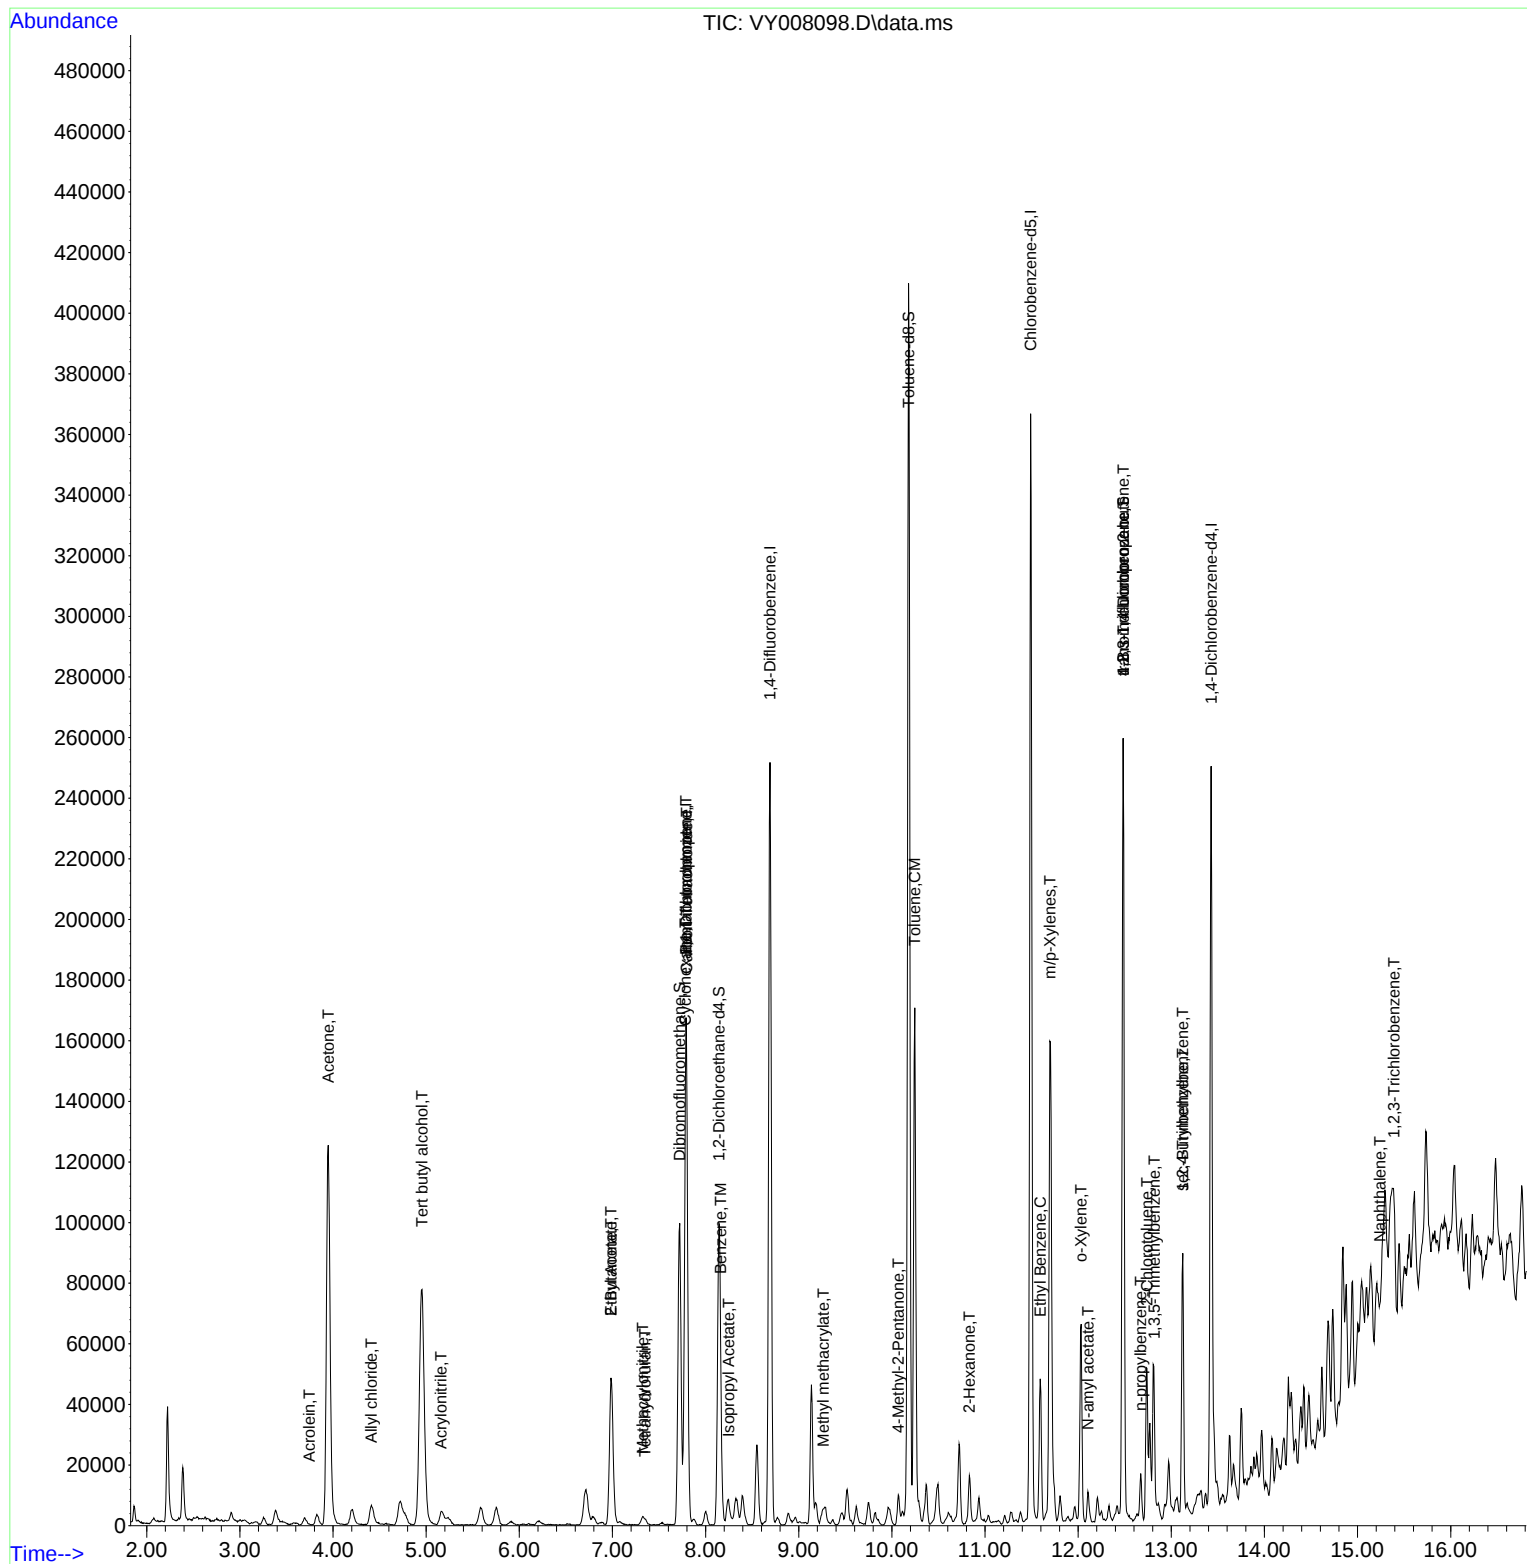






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :



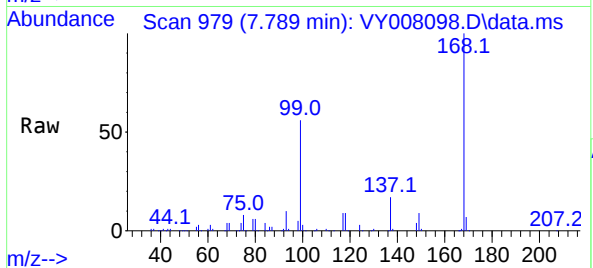



Tgt Ion:168 Resp: 127905
Ion Ratio Lower Upper
168 100
99 56.4 46.9 70.3

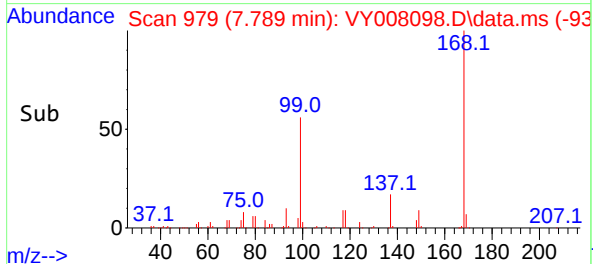

#11
Tert butyl alcohol
Concen: 1250.837 ug/l
RT: 4.954 min Scan# 514
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Tgt Ion: 59 Resp: 166541
Ion Ratio Lower Upper
59 100
57 10.1 6.4 9.6#

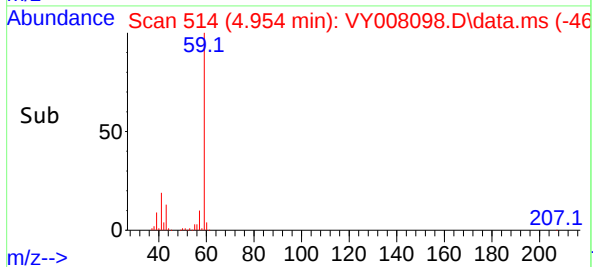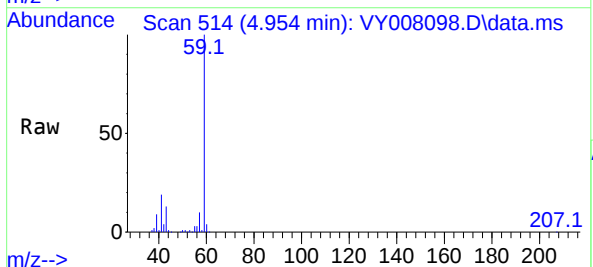






#13
Acrolein
Concen: 1.366 ug/l
RT: 3.747 min Scan# 312
Delta R.T. 0.024 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Instrument :
MSVOA_Y
ClientSampleId :





Tgt Ion: 56 Resp: 148
Ion Ratio Lower Upper
56 100
55 0.0 57.6 86.4#




#14
Allyl chloride
Concen: 6.477 ug/l
RT: 4.412 min Scan# 425
Delta R.T. -0.067 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Tgt Ion: 41 Resp: 11565
Ion Ratio Lower Upper
41 100
39 19.5 58.8 88.2#
76 0.0 25.1 37.7#

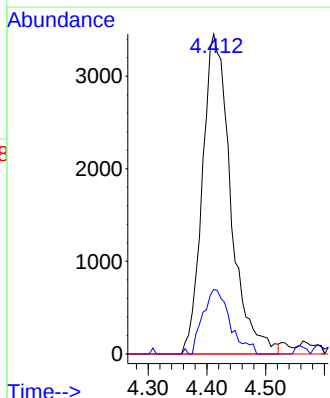






#15
Acrylonitrile
Concen: 16.476 ug/l
RT: 5.161 min Scan# 54
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Instrument :
MSVOA_Y
ClientSampleId :

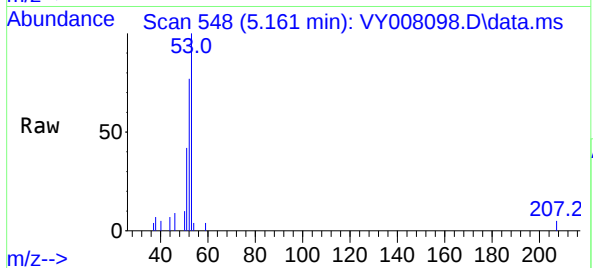



Tgt Ion: 53 Resp: 6006
Ion Ratio Lower Upper
53 100
52 77.5 67.0 100.4
51 34.4 29.8 44.6

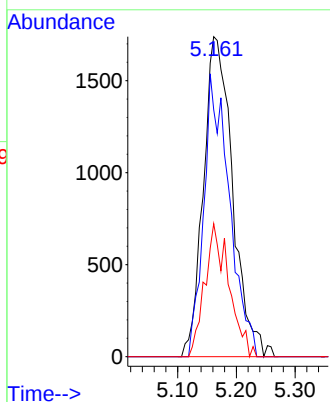


#16
Acetone
Concen: 730.966 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33



Tgt Ion: 43 Resp: 214406
Ion Ratio Lower Upper
43 100
58 34.0 22.0 33.0#

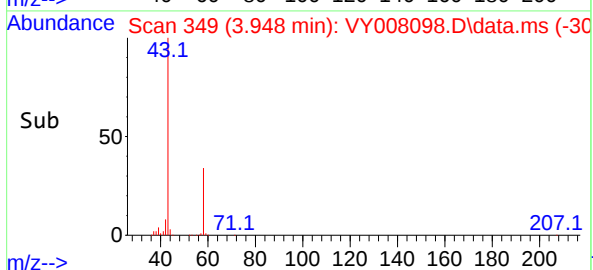



#18

Methyl Acetate

Concen: Below Cal

RT: 4.491 min Scan# 41

Delta R.T. 0.019 min

Lab File: VY008098.D

Acq: 29 Mar 2022 19:33

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 43 Resp: 988

Ion Ratio Lower Upper

43 100

74 7.8 16.6 24.8#



#25

2-Butanone

Concen: 179.485 ug/l

RT: 6.984 min Scan# 847

Delta R.T. 0.006 min

Lab File: VY008098.D




Acq: 29 Mar 2022 19:33


Tgt Ion: 43 Resp: 80116

Ion Ratio Lower Upper

43 100


72 34.0 17.7 26.5#

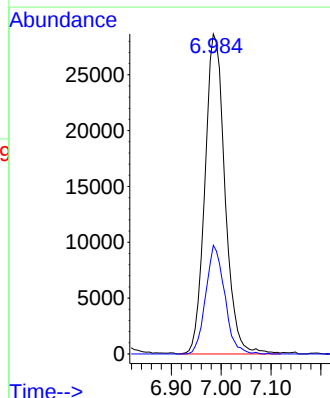



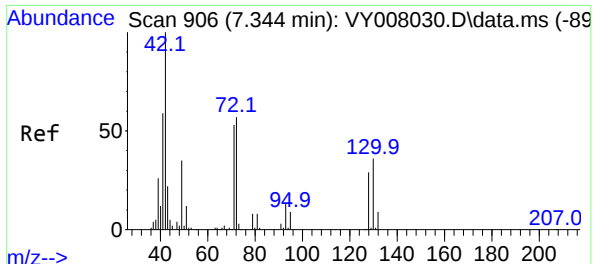


#29
Tetrahydrofuran
Concen: 3.067 ug/l
RT: 7.350 min Scan# 906
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :



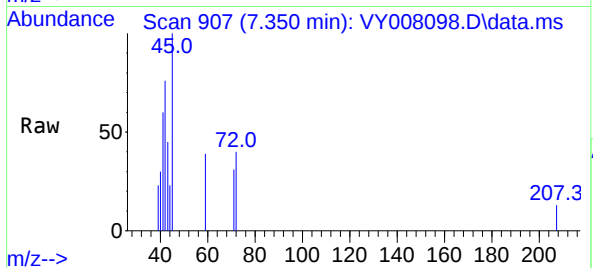



Tgt Ion: 42 Resp: 890
Ion Ratio Lower Upper
42 100
72 50.0 30.3 45.5#
71 35.5 29.0 43.4

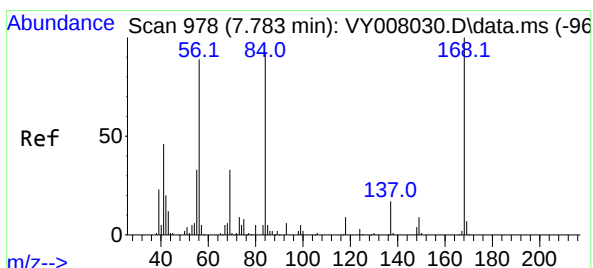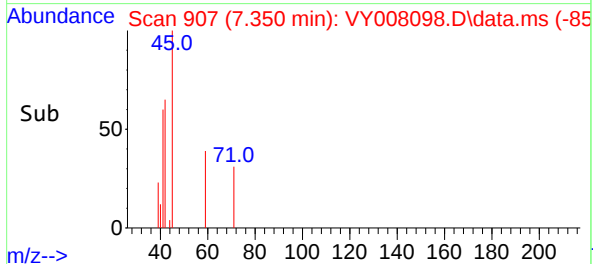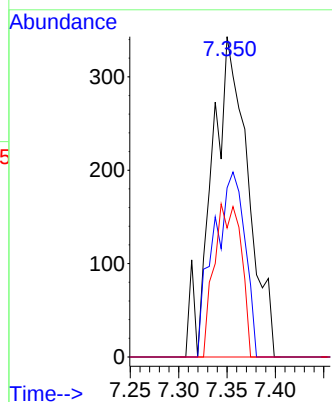

#31
Cyclohexane
Concen: 1.722 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 56 Resp: 4130
Ion Ratio Lower Upper
56 100
69 101.4 26.7 40.1#
84 111.1 67.2 100.8#

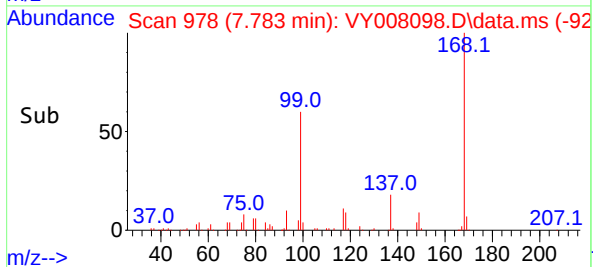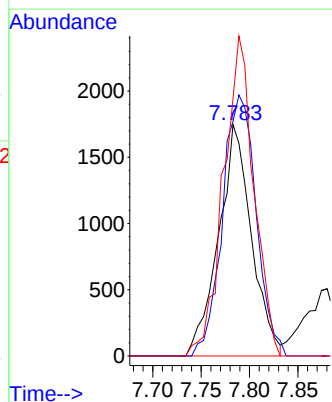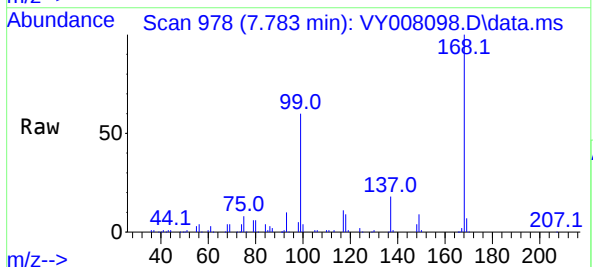



#33

1,2-Dichloroethane-d4

Concen: 55.923 ug/l

RT: 8.143 min Scan# 1037

Delta R.T. 0.007 min

Lab File: VY008098.D

Acq: 29 Mar 2022 19:33

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 65 Resp: 71764

Ion Ratio Lower Upper

65 100

67 52.9 0.0 99.4

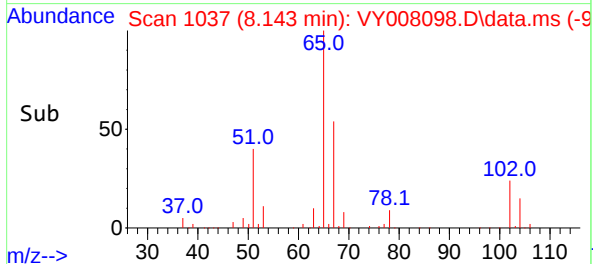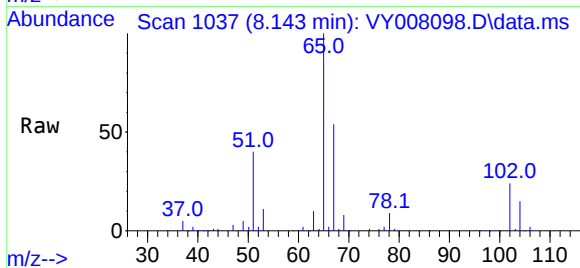

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY008098.D

Acq: 29 Mar 2022 19:33




Tgt Ion: 114 Resp: 229314


Ion Ratio Lower Upper

114 100

63 17.4 0.0 43.2


88 14.1 0.0 31.8

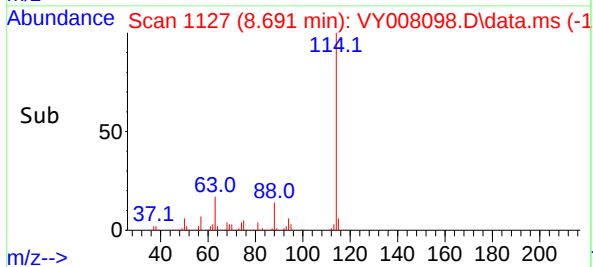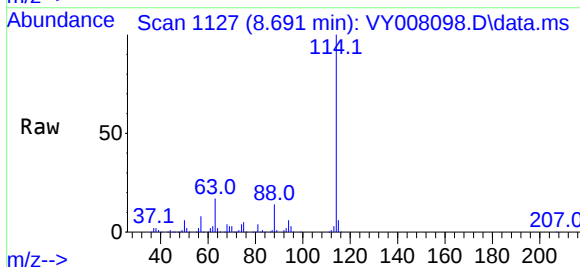






#35
Dibromofluoromethane
Concen: 49.421 ug/l
RT: 7.722 min Scan# 910
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :



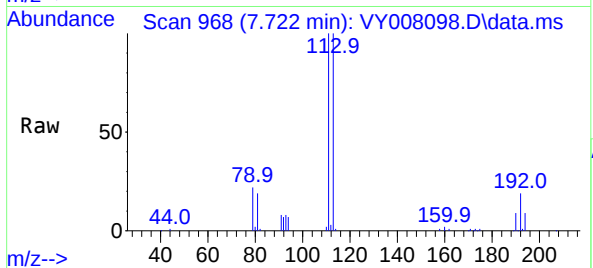



Tgt Ion:113 Resp: 71054
Ion Ratio Lower Upper
113 100
111 103.7 82.6 124.0
192 18.2 17.6 26.4

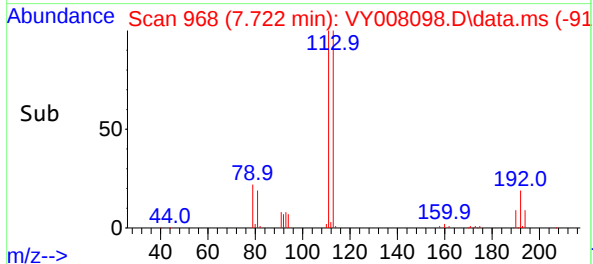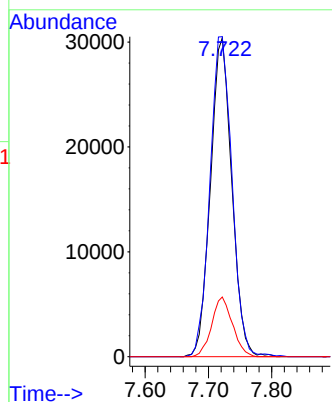

#36
1,1-Dichloropropene
Concen: 4.377 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.128 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Tgt Ion: 75 Resp: 9885
Ion Ratio Lower Upper
75 100
110 9.2 17.1 51.2#
77 0.0 24.4 36.6#

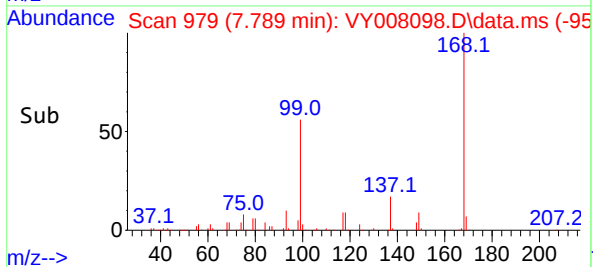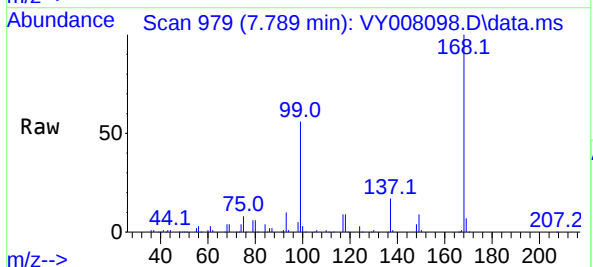






#37
Ethyl Acetate
Concen: 75.938 ug/l
RT: 6.984 min Scan# 84
Delta R.T. -0.085 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 43 Resp: 80116
Ion Ratio Lower Upper
43 100
61 0.0 9.7 14.5#
70 0.0 7.1 10.7#

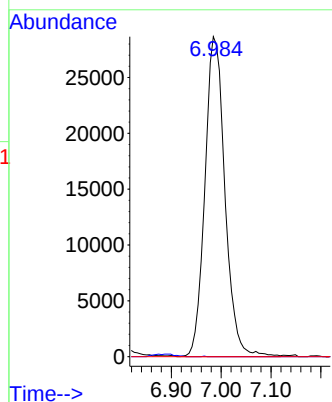

#38
Carbon Tetrachloride
Concen: 5.114 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.104 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 117 Resp: 12586
Ion Ratio Lower Upper
117 100
119 5.6 77.9 116.9#
121 0.0 24.8 37.2#


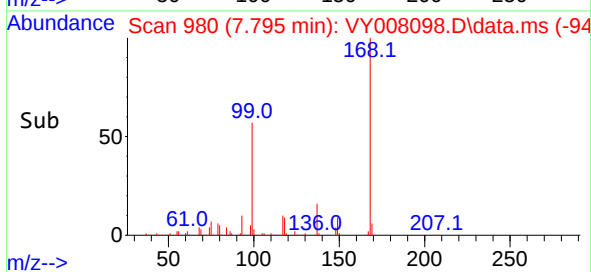
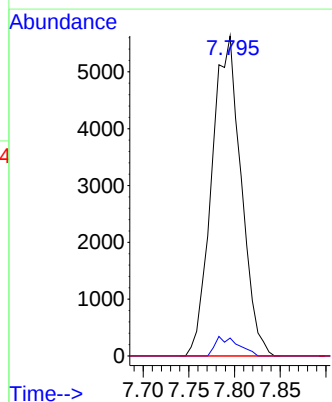





#40
Benzene
Concen: 2.577 ug/l
RT: 8.161 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 78 Resp: 16645
Ion Ratio Lower Upper
78 100
77 23.2 20.4 30.6

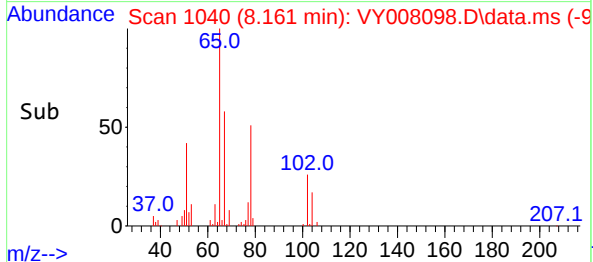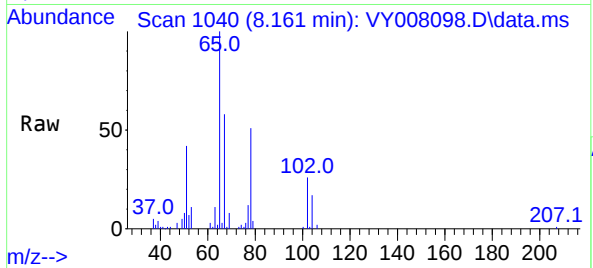

#41
Methacrylonitrile
Concen: 1.433 ug/l
RT: 7.326 min Scan# 903
Delta R.T. 0.019 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Tgt Ion: 41 Resp: 759
Ion Ratio Lower Upper
41 100
39 48.0 92.9 139.3#
67 0.0 0.0 0.0
52 0.0 0.0 0.0

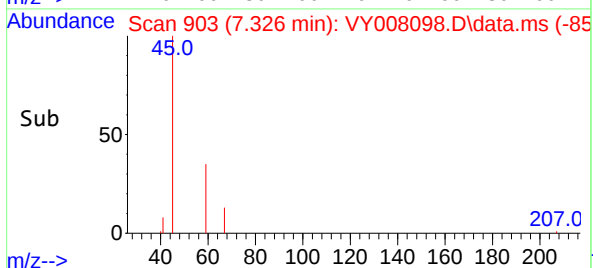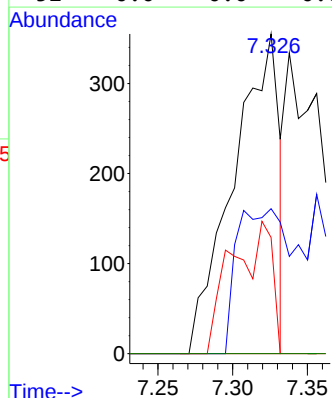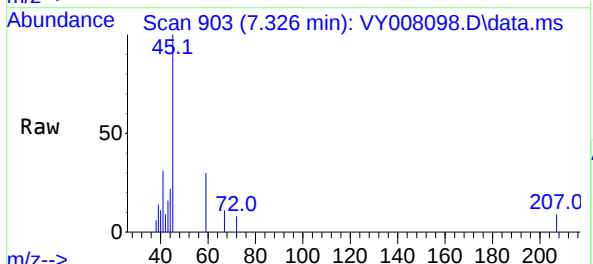






#43
Isopropyl Acetate
Concen: 1.168 ug/l
RT: 8.246 min Scan# 1054
Delta R.T. -0.025 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 43 Resp: 2419
Ion Ratio Lower Upper
43 100
61 0.0 20.2 30.2#
87 0.0 8.9 13.3#



#48
Methyl methacrylate
Concen: 2.198 ug/l
RT: 9.264 min Scan# 1221
Delta R.T. -0.025 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 41 Resp: 2016
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 44.9 47.4 71.0#


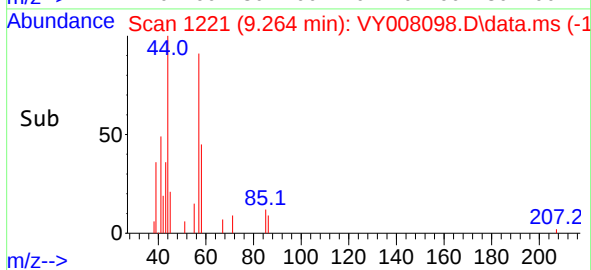






#50
Toluene-d8
Concen: 50.626 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 274227
Ion Ratio Lower Upper
98 100
100 65.5 50.2 75.2

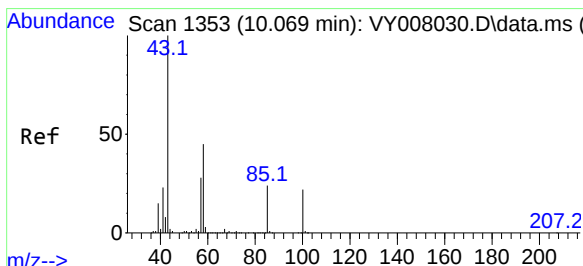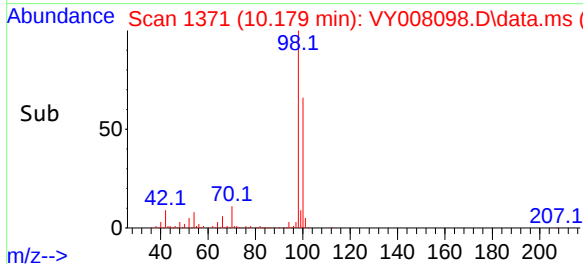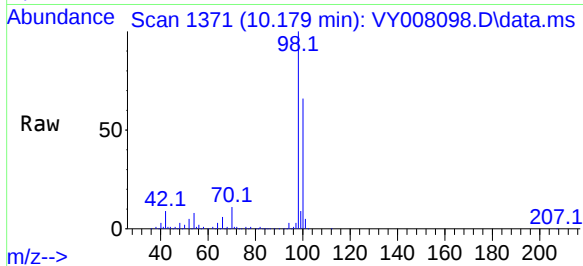

#51
4-Methyl-2-Pentanone
Concen: 5.768 ug/l
RT: 10.069 min Scan# 1353
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 43 Resp: 6025
Ion Ratio Lower Upper
43 100
58 48.3 28.1 42.1#


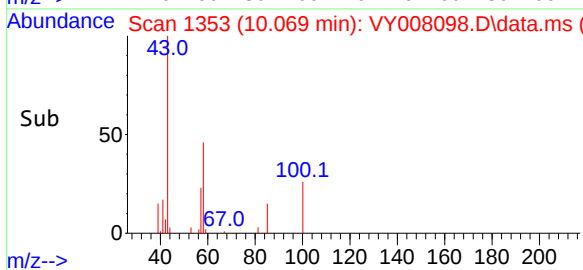

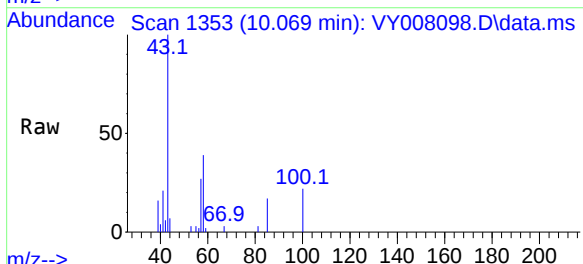




#52
Toluene
Concen: 16.991 ug/l
RT: 10.246 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 92 Resp: 71986
Ion Ratio Lower Upper
92 100
91 171.6 142.6 213.8

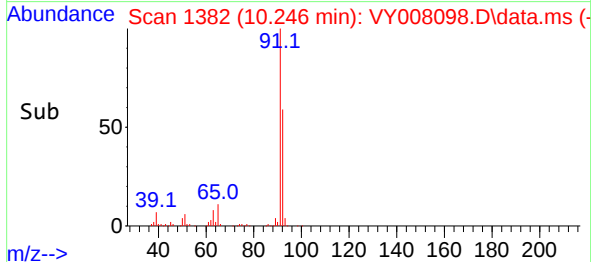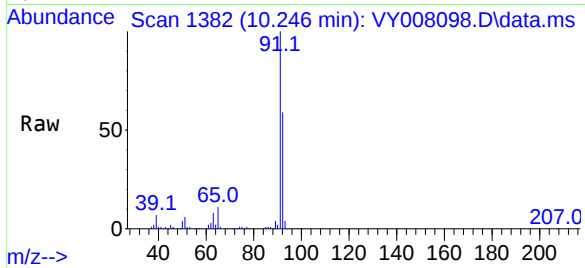

#59
2-Hexanone
Concen: 13.916 ug/l
RT: 10.831 min Scan# 1478
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 43 Resp: 10172
Ion Ratio Lower Upper
43 100
58 57.1 24.4 73.4


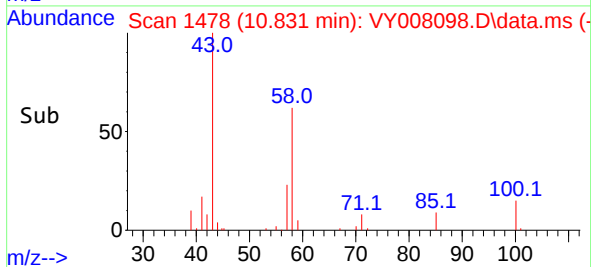

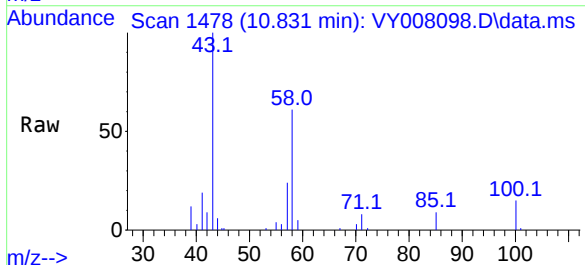




#62
4-Bromofluorobenzene
Concen: 43.036 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 95 Resp: 82242
Ion Ratio Lower Upper
95 100
174 79.0 0.0 177.0
176 75.9 0.0 175.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. 0.001 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 117 Resp: 203212
Ion Ratio Lower Upper
117 100
82 53.2 43.0 64.4
119 31.8 25.4 38.0

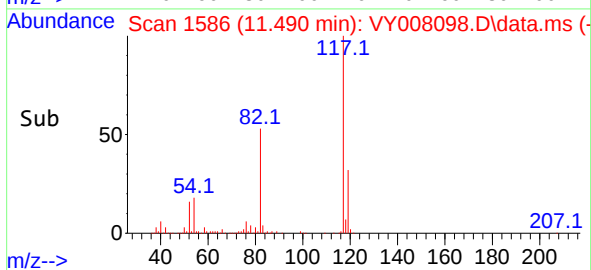



#67

Ethyl Benzene

Concen: 3.931 ug/l

RT: 11.593 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY008098.D

Acq: 29 Mar 2022 19:33

Instrument :

MSVOA_Y


ClientSampleId :

Tgt Ion: 91 Resp: 31571




Ion Ratio Lower Upper

91 100

106 33.9 24.5 36.7



Abundance

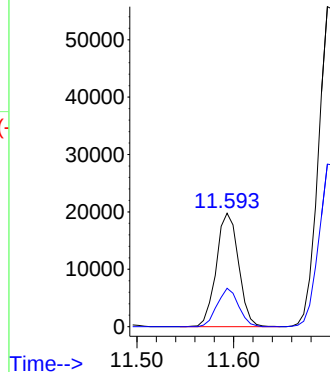

#68

m/p-Xylenes

Concen: 16.147 ug/l

RT: 11.697 min Scan# 1620

Delta R.T. -0.006 min

Lab File: VY008098.D


Acq: 29 Mar 2022 19:33

Tgt Ion:106 Resp: 51563



Ion Ratio Lower Upper


106 100

91 195.8 166.6 249.8



Abundance




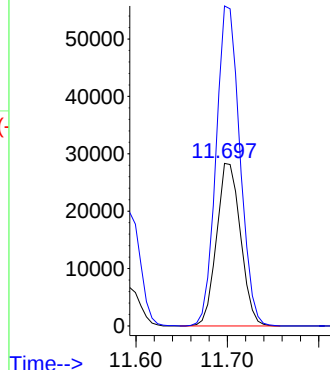




#69
o-Xylene
Concen: 5.704 ug/l
RT: 12.032 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:106 Resp: 17439
Ion Ratio Lower Upper
106 100
91 213.8 110.3 331.0

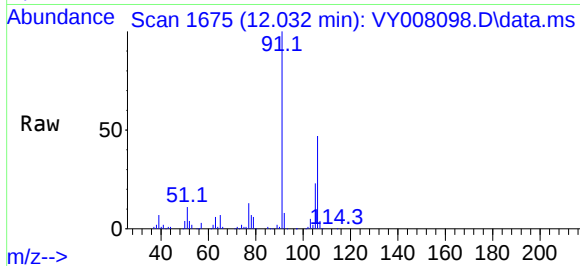

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Tgt Ion:152 Resp: 62944
Ion Ratio Lower Upper
152 100
115 60.0 28.2 84.7
150 156.4 0.0 347.6

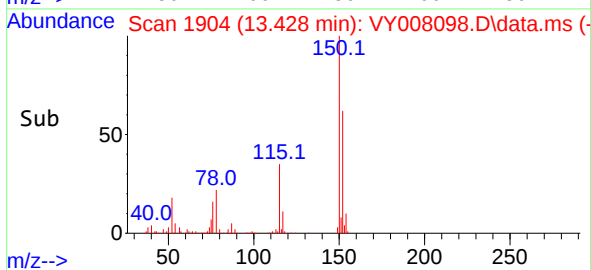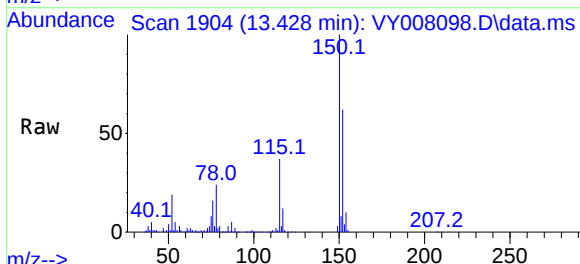






#74
N-amy1 acetate
Concen: 5.182 ug/l
RT: 12.105 min Scan# 1
Delta R.T. -0.037 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Instrument :
MSVOA_Y
ClientSampleId :



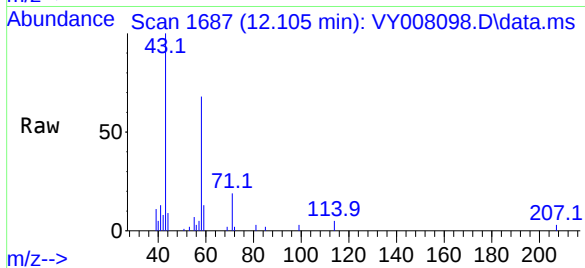



Tgt Ion: 43 Resp: 5918
Ion Ratio Lower Upper
43 100
70 0.0 28.7 43.1#
55 13.0 17.3 25.9#
61 0.0 17.0 25.6#

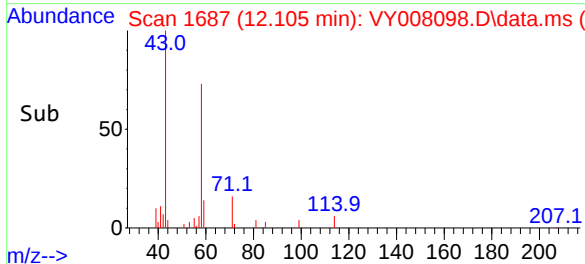

#76
1,2,3-Trichloropropane
Concen: 54.400 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.146 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 75 Resp: 41741
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#


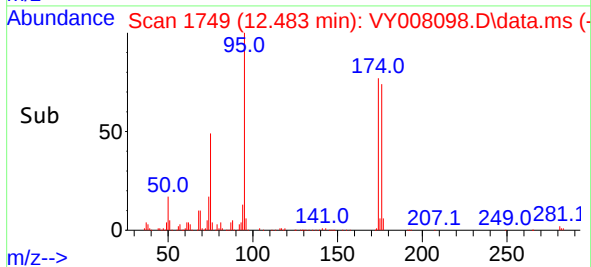

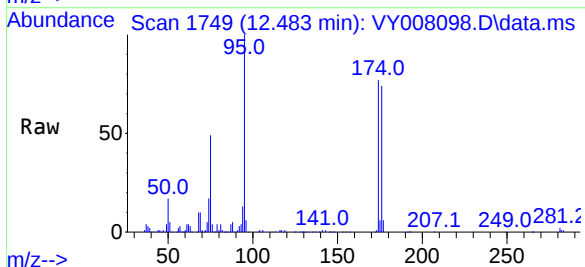




#78
n-propylbenzene
Concen: 1.865 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 11429
Ion Ratio Lower Upper
91 100
120 23.6 11.3 33.9



#79
2-Chlorotoluene
Concen: 1.138 ug/l
RT: 12.739 min Scan# 1791
Delta R.T. -0.019 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 91 Resp: 3870
Ion Ratio Lower Upper
91 100
126 0.0 16.9 50.6#









#80
1,3,5-Trimethylbenzene
Concen: 2.447 ug/l
RT: 12.819 min Scan# 1749
Delta R.T. 0.007 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 10415
Ion Ratio Lower Upper
105 100
120 48.7 24.4 73.4

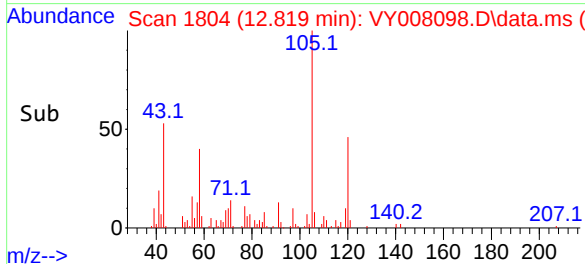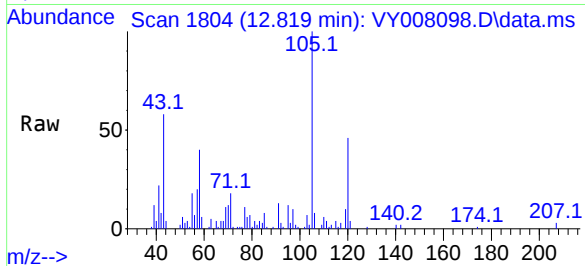

#81
trans-1,4-Dichloro-2-butene
Concen: 121.376 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.103 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33

Tgt Ion: 75 Resp: 41741
Ion Ratio Lower Upper
75 100
53 0.2 85.3 127.9#
89 0.2 37.0 55.4#


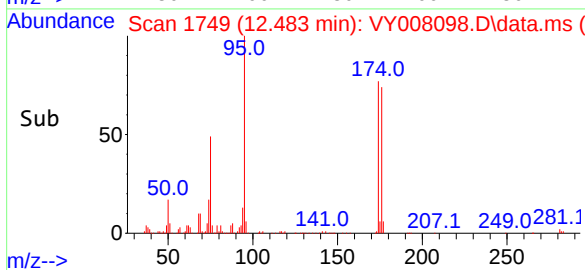

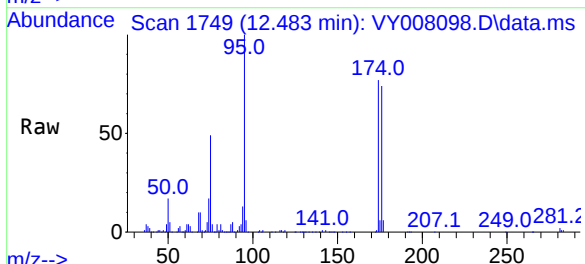




#84
1,2,4-Trimethylbenzene
Concen: 11.272 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.006 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 46719
Ion Ratio Lower Upper
105 100
120 45.6 22.3 66.9

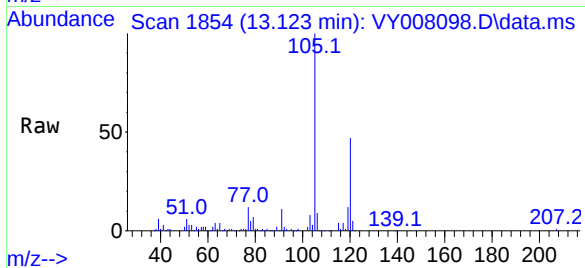

#85
sec-Butylbenzene
Concen: 8.347 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. -0.128 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Tgt Ion:105 Resp: 46719
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#

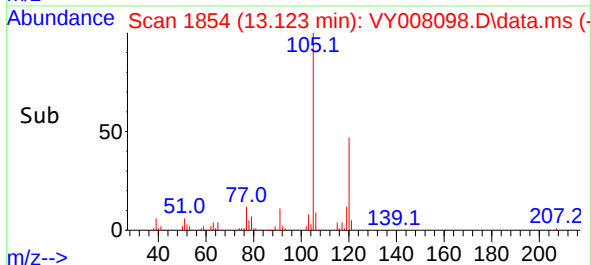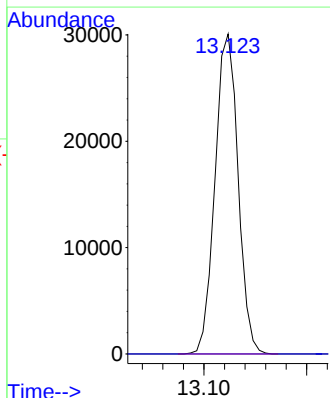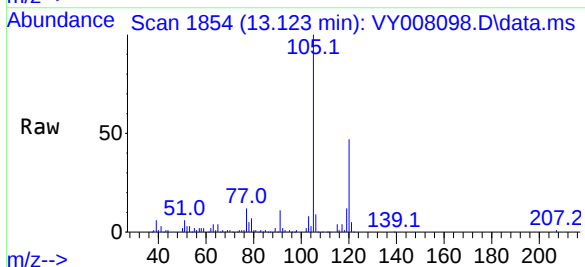






#95
Naphthalene
Concen: 2.751 ug/l
RT: 15.239 min Scan# 21
Delta R.T. -0.000 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33


Instrument :
MSVOA_Y
ClientSampleId :



Tgt Ion:128 Resp: 7578
Ion Ratio Lower Upper
128 100
127 19.4 11.0 16.4#
129 17.4 8.4 12.6#

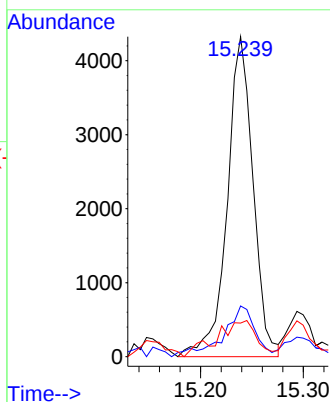

#96
1,2,3-Trichlorobenzene
Concen: 1.514 ug/l
RT: 15.391 min Scan# 2226
Delta R.T. -0.031 min
Lab File: VY008098.D
Acq: 29 Mar 2022 19:33



Tgt Ion:180 Resp: 1632
Ion Ratio Lower Upper
180 100
182 17.7 47.3 141.9#
145 91.7 15.3 45.9#

