

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032922\
 Data File : VY008094.D
 Acq On : 29 Mar 2022 17:59
 Operator : SY/MD
 Sample : N2108-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 R206

Quant Time: Mar 30 04:01:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	93243	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	165287	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	152842	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	65796	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	51631	55.190	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.380%
35) Dibromofluoromethane	7.722	113	51404	49.603	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.200%
50) Toluene-d8	10.179	98	199392	51.070	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.140%
62) 4-Bromofluorobenzene	12.483	95	67016	48.652	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	97.300%
Target Compounds						
					Qvalue	
16) Acetone	3.948	43	4189	19.590	ug/l	90
91) 1,2-Dichlorobenzene	13.739	146	11326	5.208	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY032922\
Data File : VY008094.D
Acq On : 29 Mar 2022 17:59
Operator : SY/MD
Sample : N2108-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
R206

Quant Time: Mar 30 04:01:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




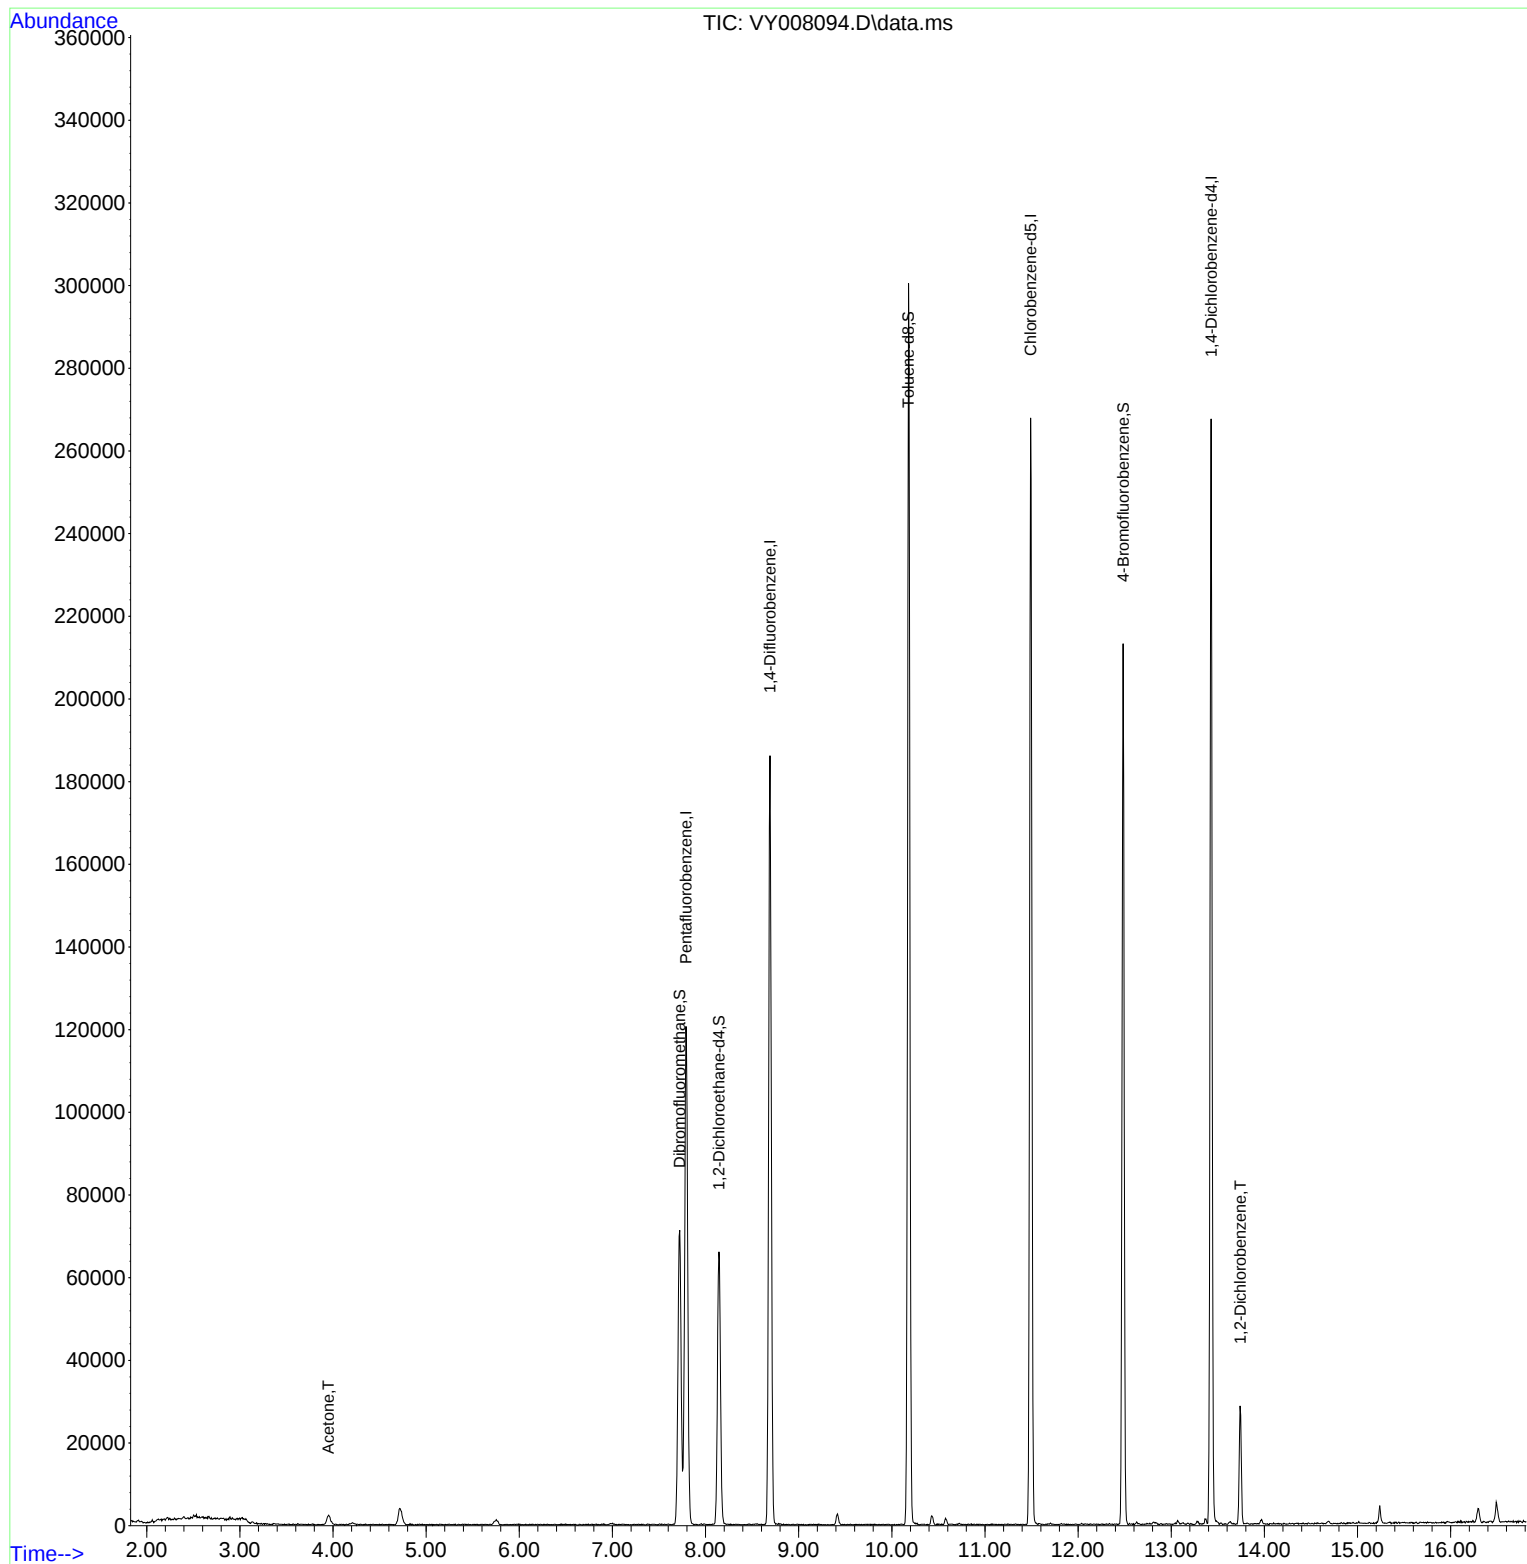


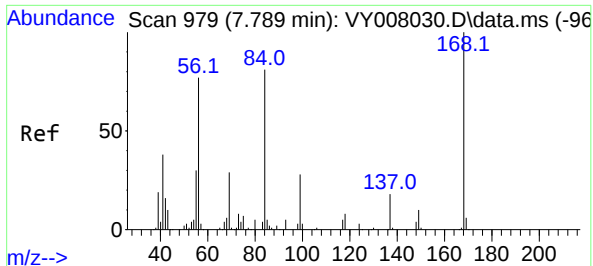

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59




Instrument :
MSVOA_Y
ClientSampleId :
R206


Tgt Ion:168 Resp: 93243
Ion Ratio Lower Upper
168 100
99 60.0 46.9 70.3

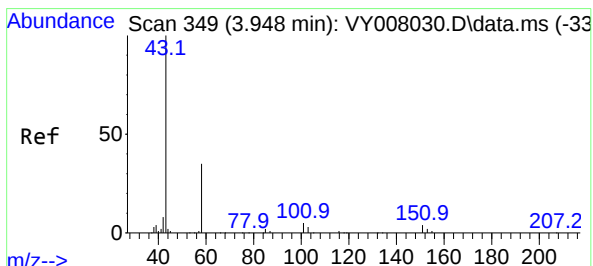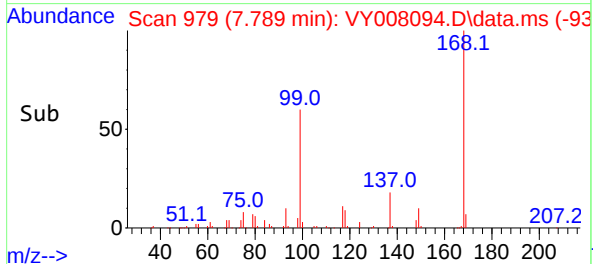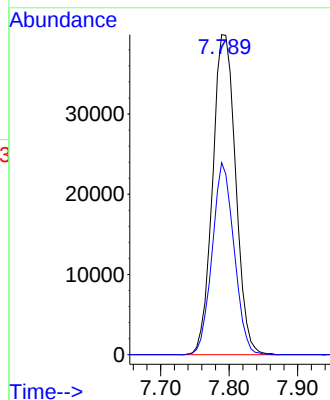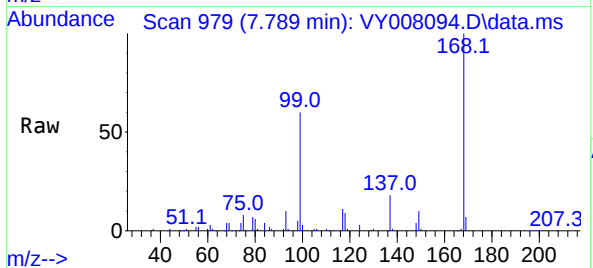

#16
Acetone
Concen: 19.590 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59

Tgt Ion: 43 Resp: 4189
Ion Ratio Lower Upper
43 100
58 33.0 22.0 33.0

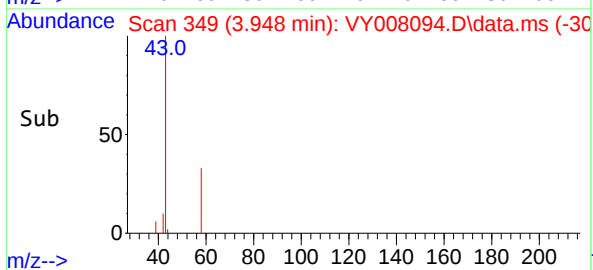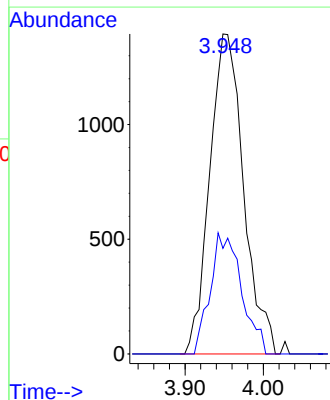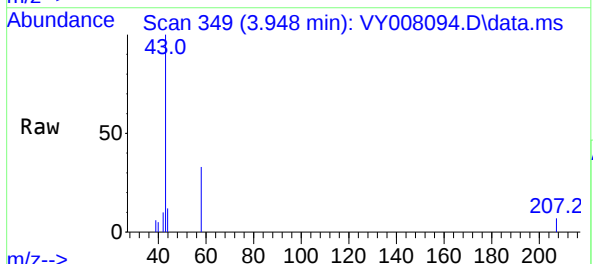

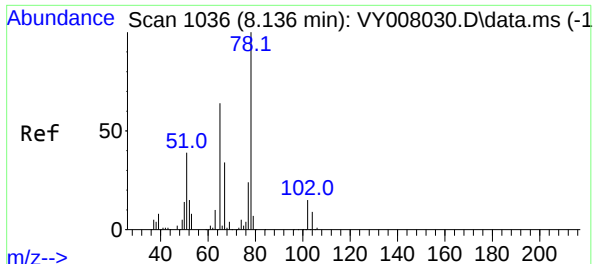

#33

1,2-Dichloroethane-d4

Concen: 55.190 ug/l

RT: 8.143 min Scan# 110

Delta R.T. 0.007 min

Lab File: VY008094.D

Acq: 29 Mar 2022 17:59

Instrument :

MSVOA_Y

ClientSampleId :





R206

Tgt Ion: 65 Resp: 51631

Ion Ratio Lower Upper

65 100

67 53.5 0.0 99.4

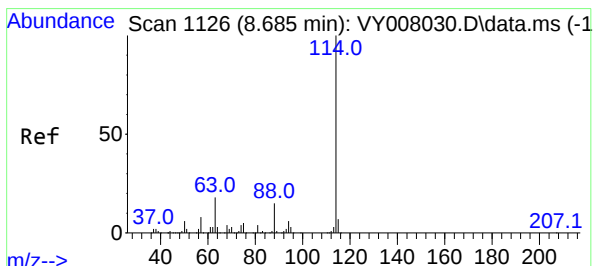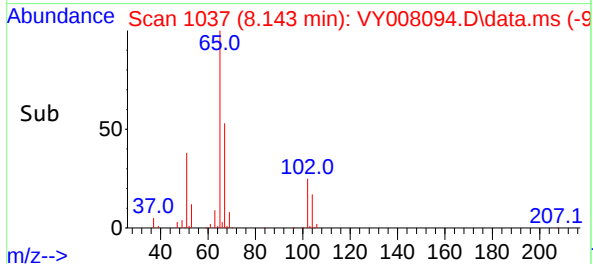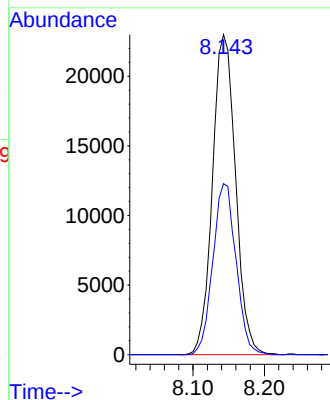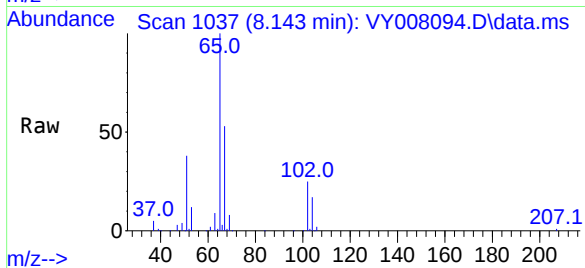

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY008094.D

Acq: 29 Mar 2022 17:59




Tgt Ion: 114 Resp: 165287


Ion Ratio Lower Upper

114 100

63 18.8 0.0 43.2

88 14.8 0.0 31.8


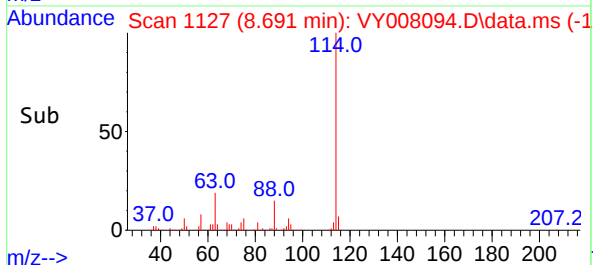
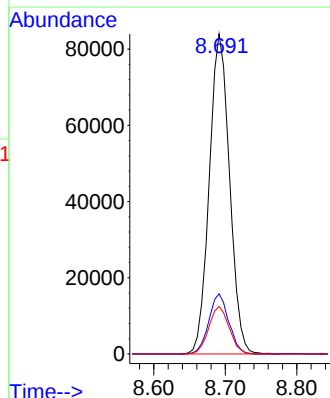
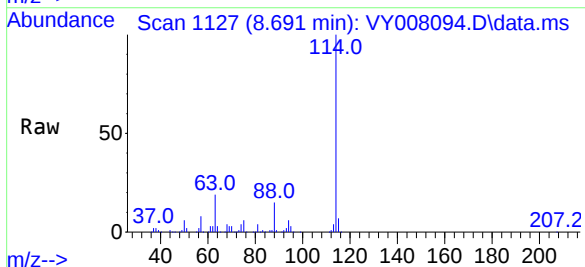


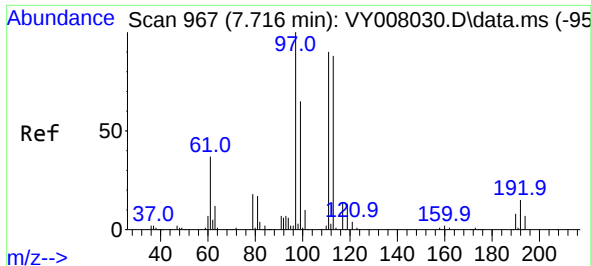

#35
Dibromofluoromethane
Concen: 49.603 ug/l
RT: 7.722 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59




Instrument :
MSVOA_Y
ClientSampleId :
R206


Tgt Ion:113 Resp: 51404
Ion Ratio Lower Upper
113 100
111 103.5 82.6 124.0
192 17.6 17.6 26.4#

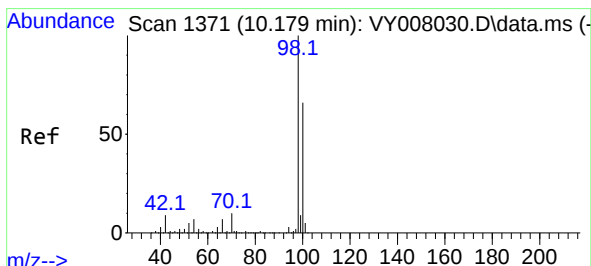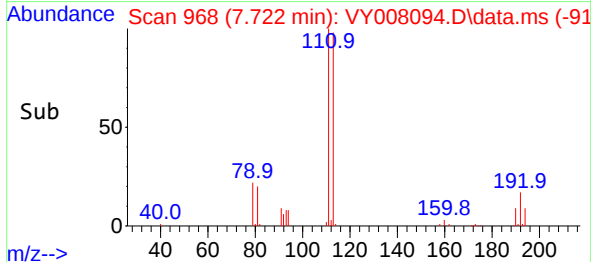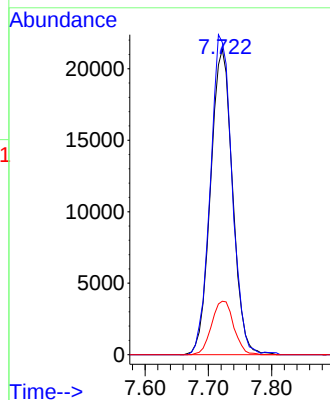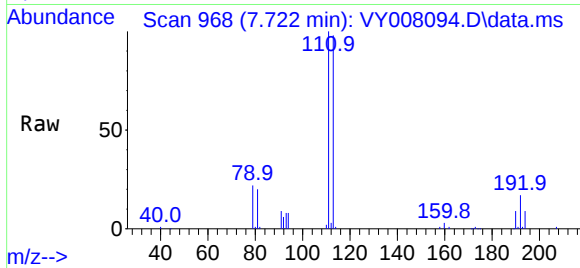

#50
Toluene-d8
Concen: 51.070 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59

Tgt Ion: 98 Resp: 199392
Ion Ratio Lower Upper
98 100
100 66.1 50.2 75.2


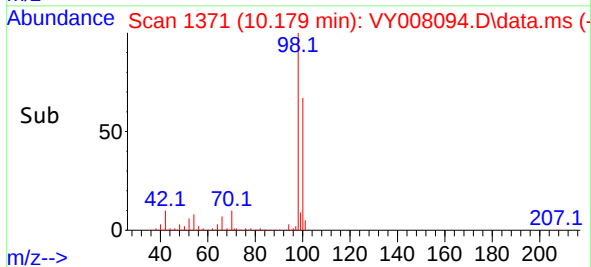
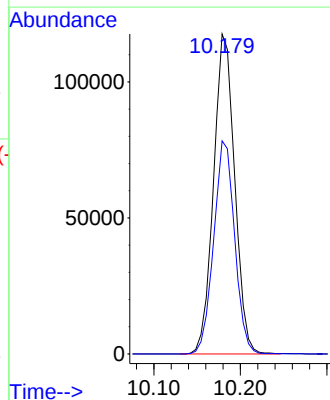
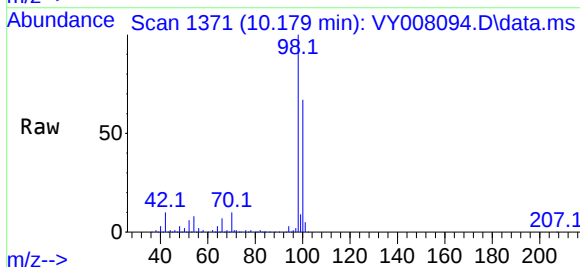


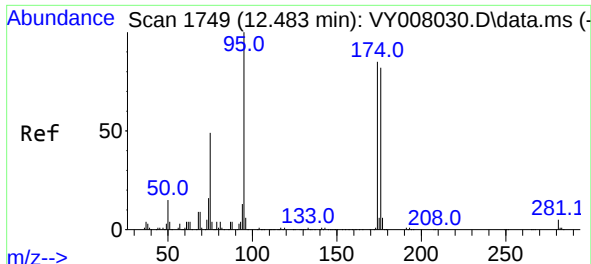

#62
4-Bromofluorobenzene
Concen: 48.652 ug/l
RT: 12.483 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59




Instrument :
MSVOA_Y
ClientSampleId :
R206


Tgt Ion: 95 Resp: 67016
Ion Ratio Lower Upper
95 100
174 80.0 0.0 177.0
176 77.4 0.0 175.8

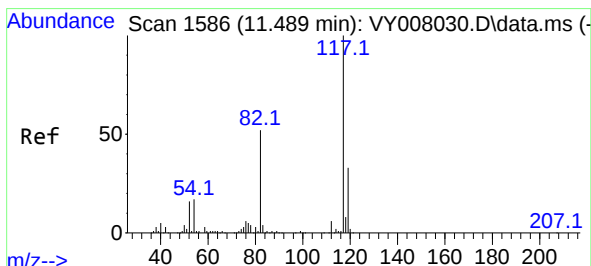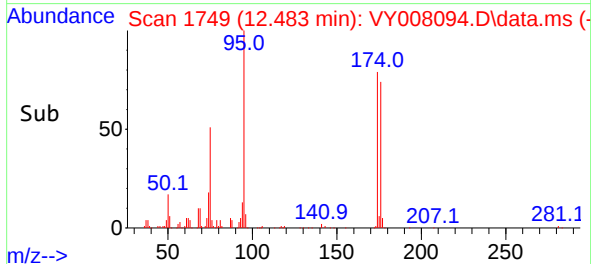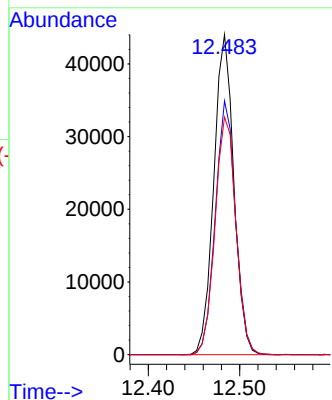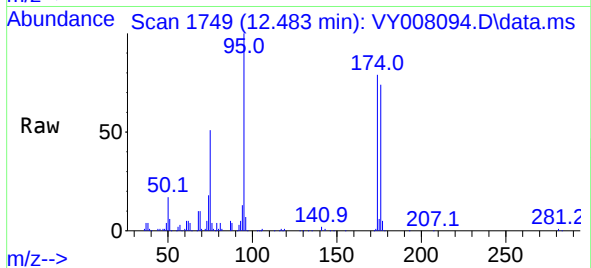

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. 0.001 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59

Tgt Ion: 117 Resp: 152842
Ion Ratio Lower Upper
117 100
82 55.4 43.0 64.4
119 33.1 25.4 38.0


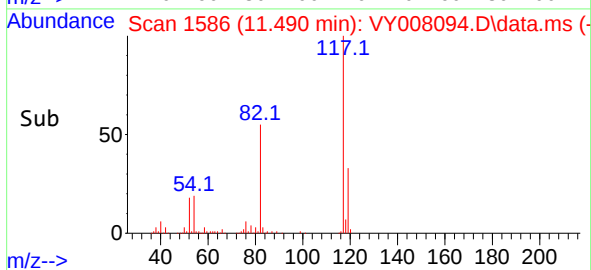
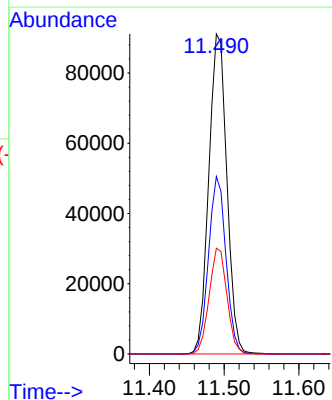
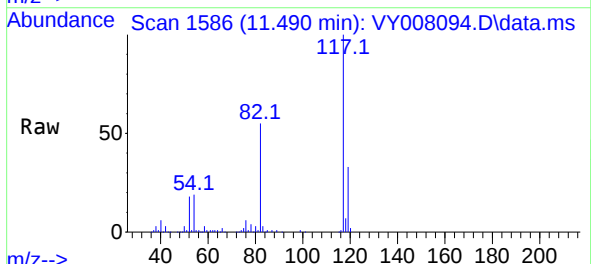


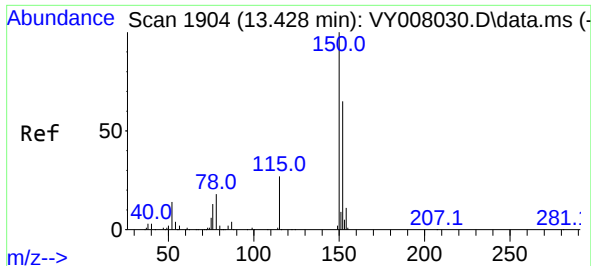

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59

Instrument :
MSVOA_Y
ClientSampleId :
R206

Tgt Ion:152 Resp: 65796
Ion Ratio Lower Upper
152 100
115 60.3 28.2 84.7
150 160.8 0.0 347.6

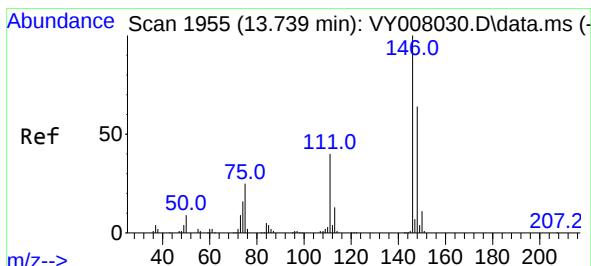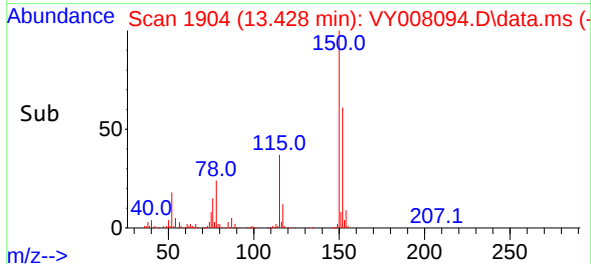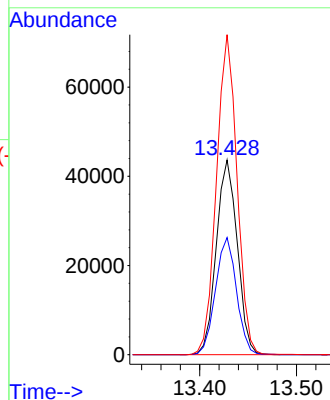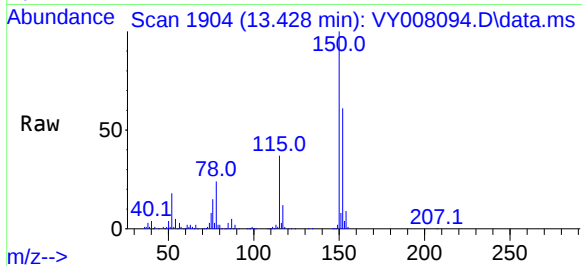

#91
1,2-Dichlorobenzene
Concen: 5.208 ug/l
RT: 13.739 min Scan# 1955
Delta R.T. 0.000 min
Lab File: VY008094.D
Acq: 29 Mar 2022 17:59

Tgt Ion:146 Resp: 11326
Ion Ratio Lower Upper
146 100
111 42.6 20.3 60.9
148 66.1 32.3 96.9

