
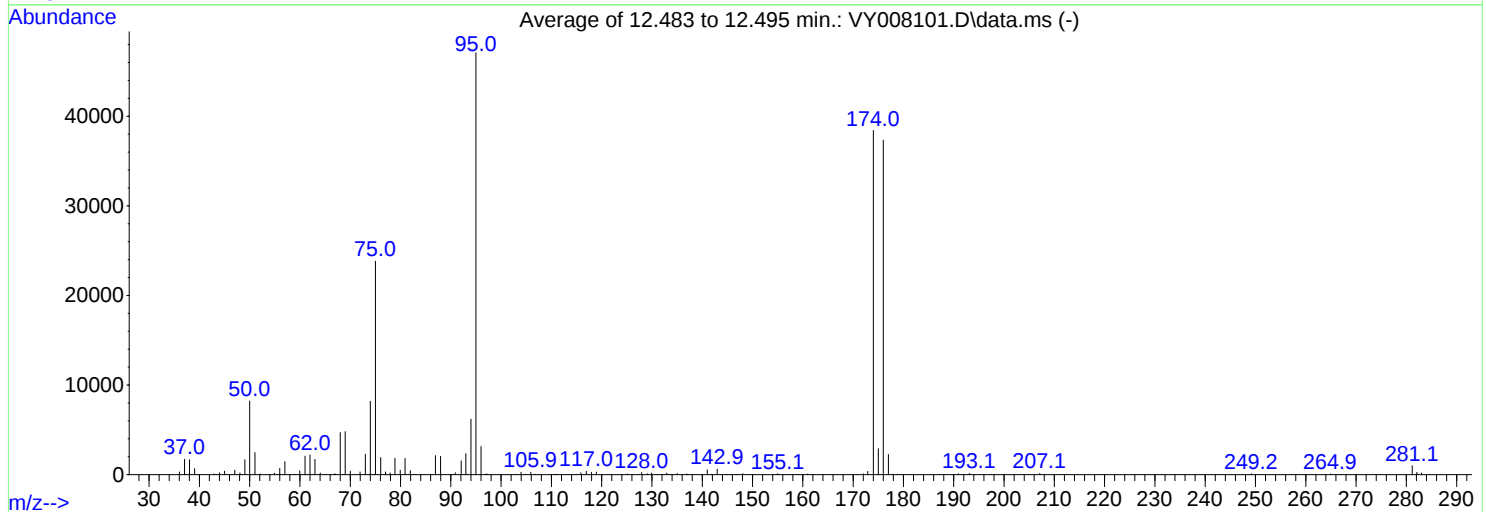


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY033022\
 Data File : VY008101.D
 Acq On : 30 Mar 2022 08:50
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Title : SW846 8260
 Last Update : Sat Mar 26 03:24:51 2022

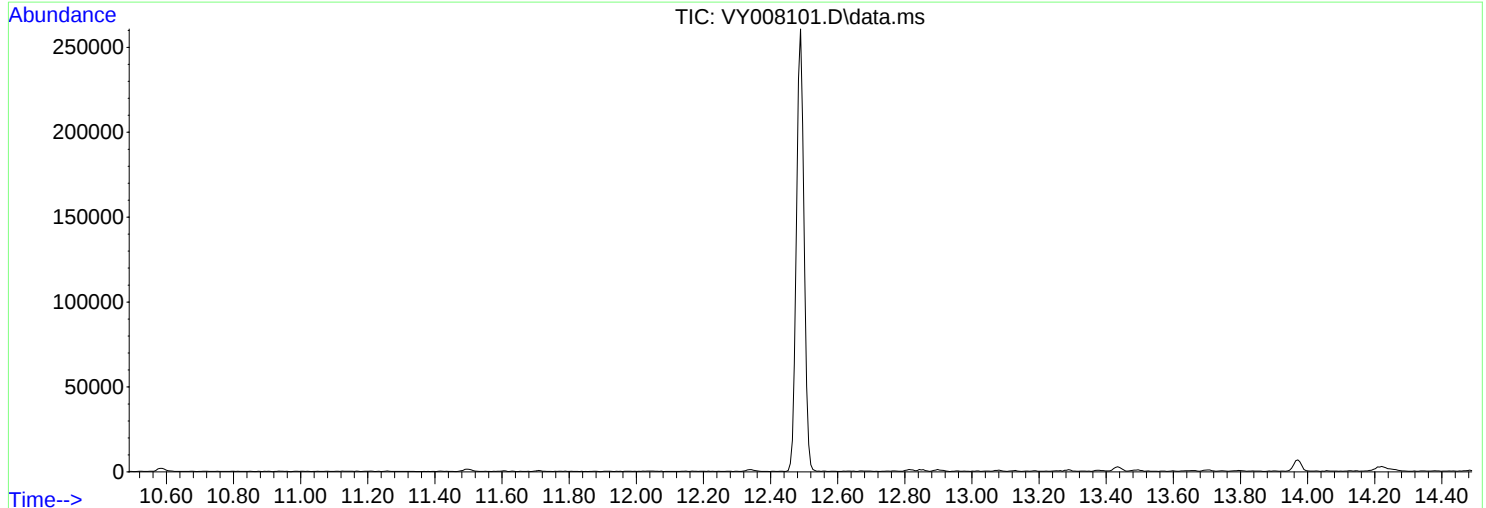

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	8208	PASS
75	95	30	60	50.6	23821	PASS
95	95	100	100	100.0	47067	PASS
96	95	5	9	6.7	3138	PASS
173	174	0.00	2	0.9	360	PASS
174	95	50	100	81.6	38403	PASS
175	174	5	9	7.5	2884	PASS
176	174	95	101	97.2	37333	PASS
177	176	5	9	6.0	2258	PASS