
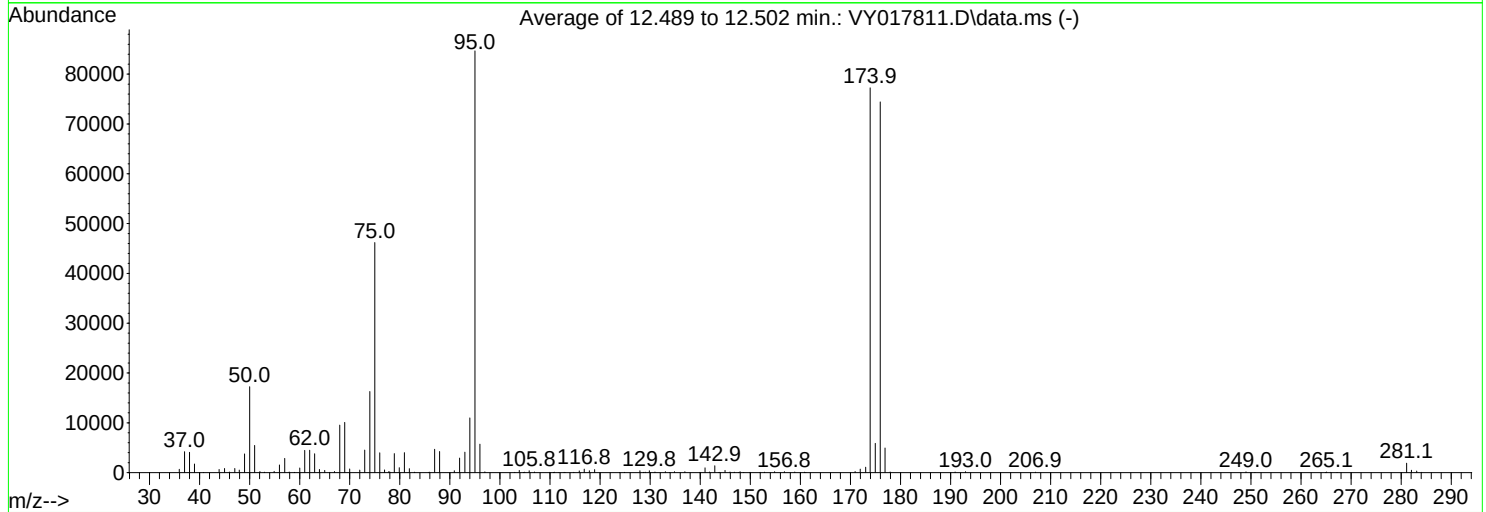


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040224\
Data File : VY017811.D
Acq On : 02 Apr 2024 08:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032924S.M
Title : SW846 8260
Last Update : Sat Mar 30 05:58:13 2024

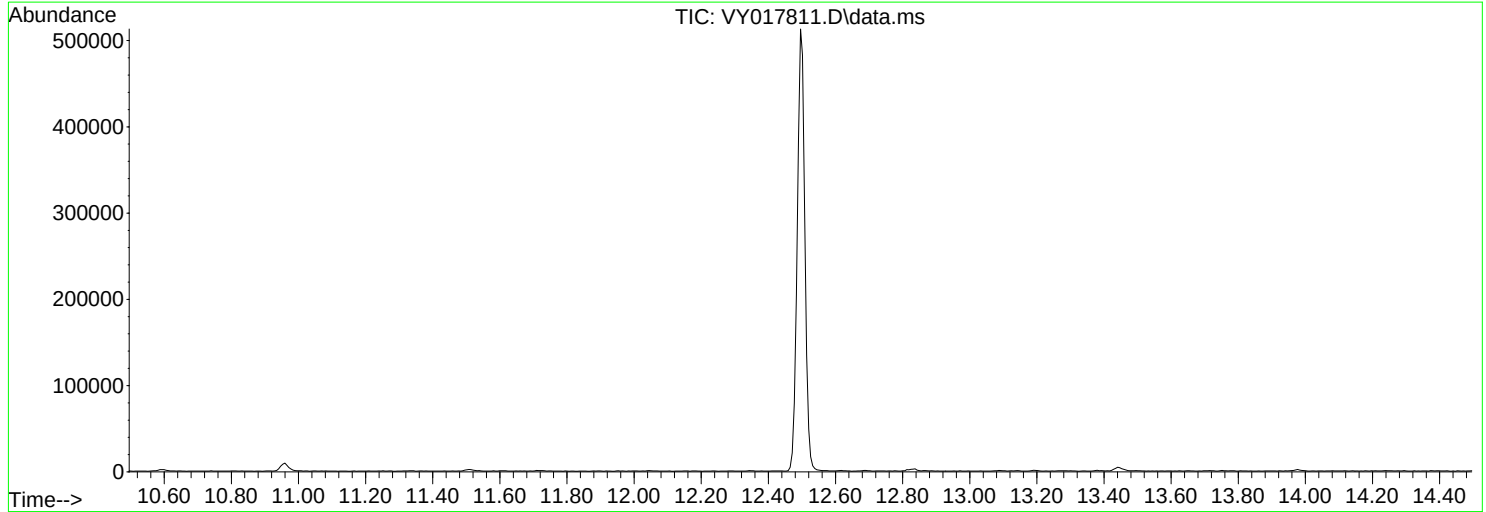

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	17267	PASS
75	95	30	60	54.6	46195	PASS
95	95	100	100	100.0	84677	PASS
96	95	5	9	6.8	5731	PASS
173	174	0.00	2	1.4	1108	PASS
174	95	50	100	91.2	77267	PASS
175	174	5	9	7.6	5867	PASS
176	174	95	101	96.3	74429	PASS
177	176	5	9	6.7	4959	PASS