

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040225\
 Data File : VY021752.D
 Acq On : 02 Apr 2025 12:11
 Operator : SY/MD
 Sample : Q1687-01
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 72-12016

Quant Time: Apr 02 14:04:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	93538	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	157036	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	136588	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	45953	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	50588	49.916	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.840%
35) Dibromofluoromethane	7.634	113	56077	55.049	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.100%
50) Toluene-d8	10.109	98	186709	48.179	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.360%
62) 4-Bromofluorobenzene	12.408	95	49857	38.035	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	76.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040225\
Data File : VY021752.D
Acq On : 02 Apr 2025 12:11
Operator : SY/MD
Sample : Q1687-01
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
72-12016

Quant Time: Apr 02 14:04:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




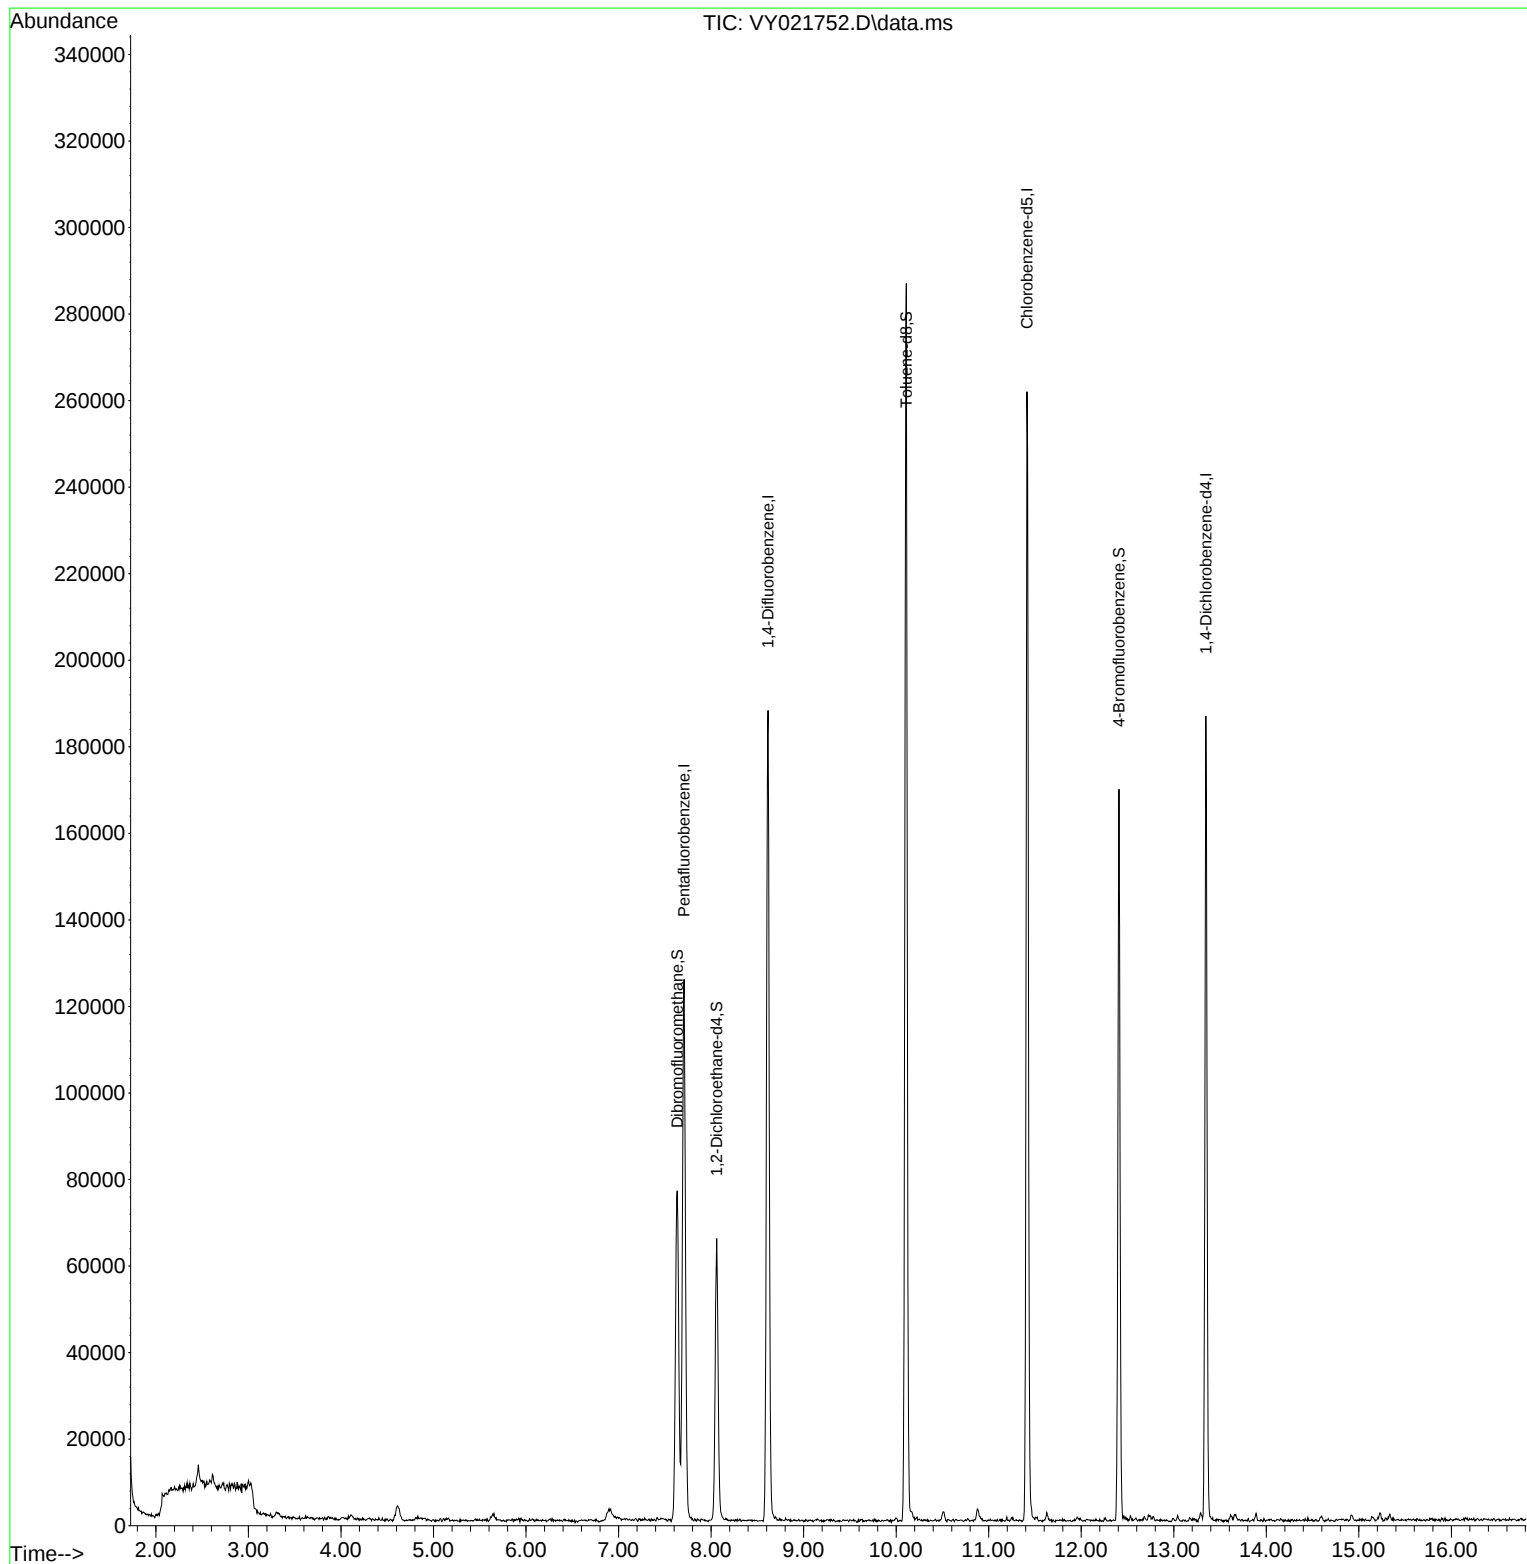


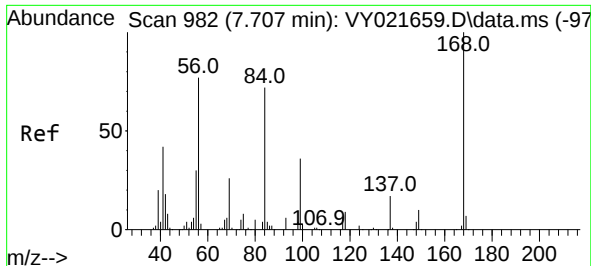

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11




Instrument :
MSVOA_Y
ClientSampleId :
72-12016


Tgt Ion:168 Resp: 93538
Ion Ratio Lower Upper
168 100
99 56.4 46.7 70.1

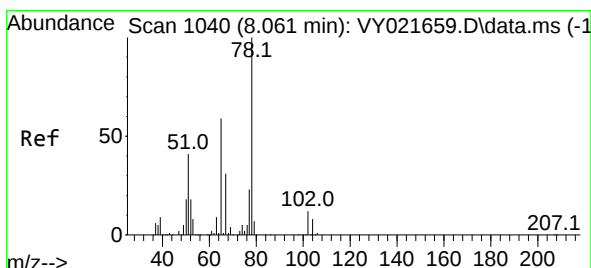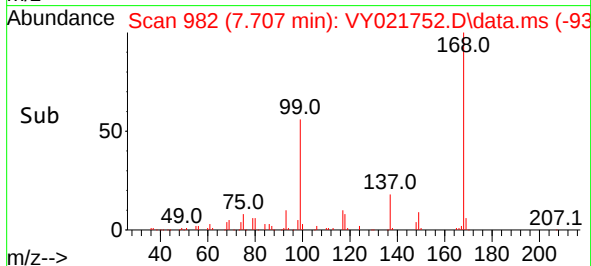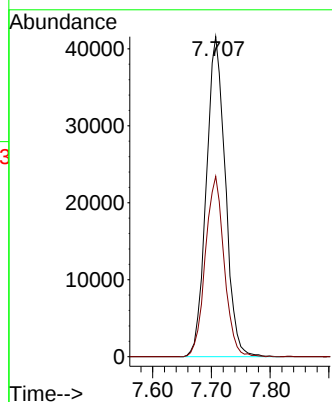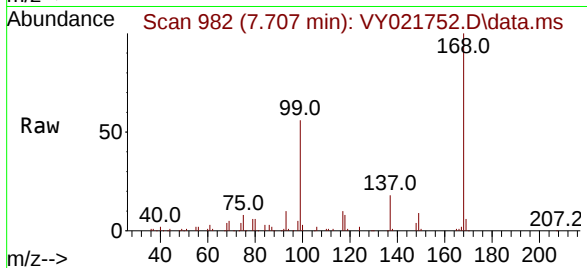

#33
1,2-Dichloroethane-d4
Concen: 49.916 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11

Tgt Ion: 65 Resp: 50588
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.6


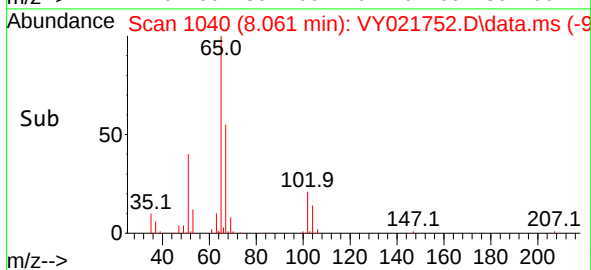
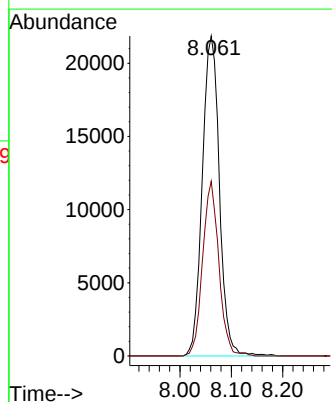
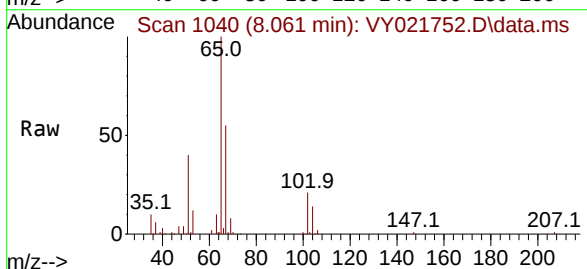


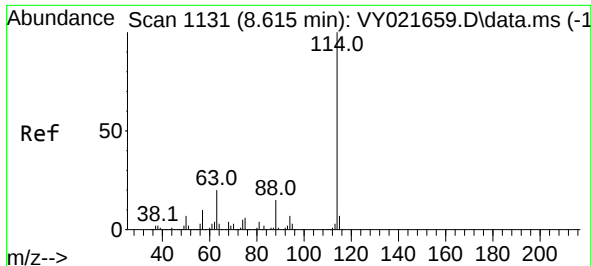

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11




Instrument :
MSVOA_Y
ClientSampleId :
72-12016


Tgt Ion:114 Resp: 157036
Ion Ratio Lower Upper
114 100
63 19.2 0.0 40.2
88 15.3 0.0 29.8

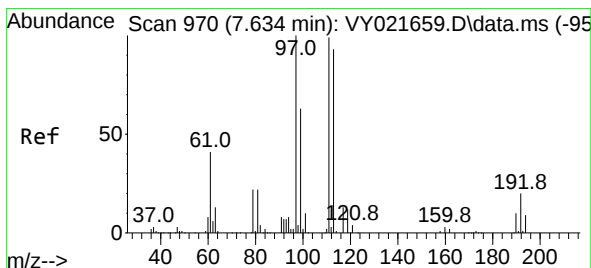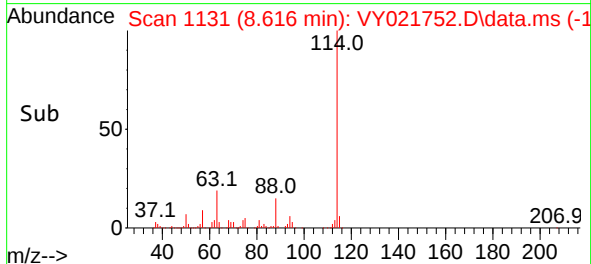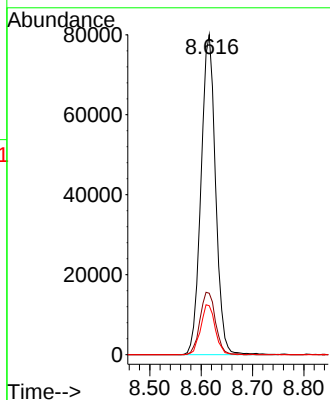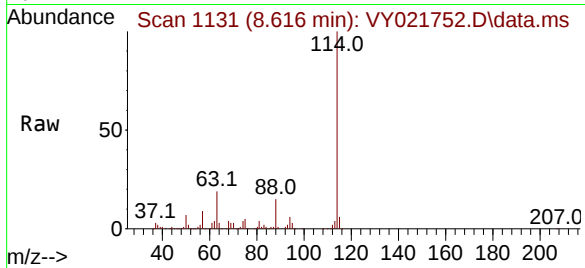

#35
Dibromofluoromethane
Concen: 55.049 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11

Tgt Ion:113 Resp: 56077
Ion Ratio Lower Upper
113 100
111 100.5 82.6 123.8
192 18.6 16.2 24.4

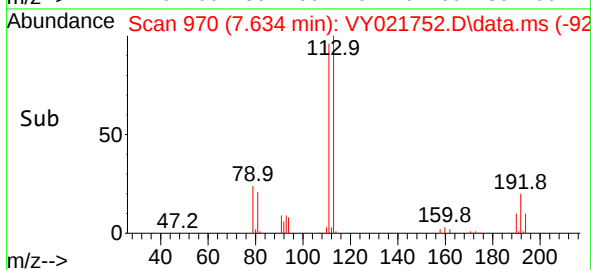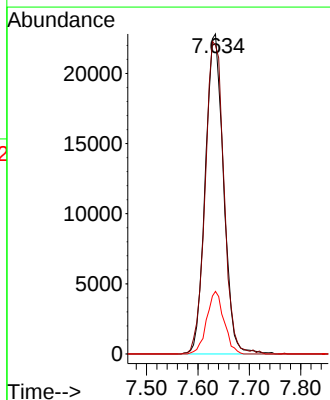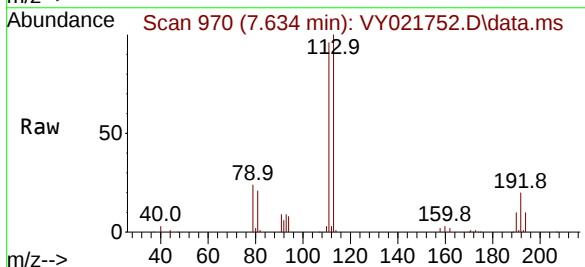

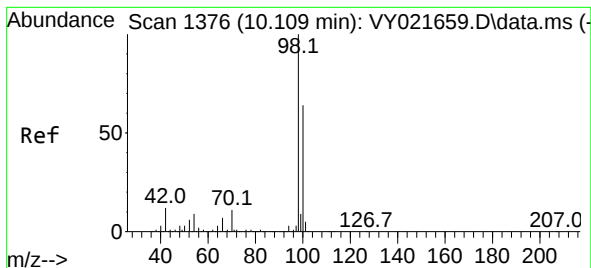

#50

Toluene-d8

Concen: 48.179 ug/l

RT: 10.109 min Scan# 1376

Delta R.T. 0.000 min

Lab File: VY021752.D

Acq: 02 Apr 2025 12:11

Instrument :

MSVOA_Y

ClientSampleId :





72-12016

Tgt Ion: 98 Resp: 186709

Ion Ratio Lower Upper

98 100

100 64.4 52.1 78.1

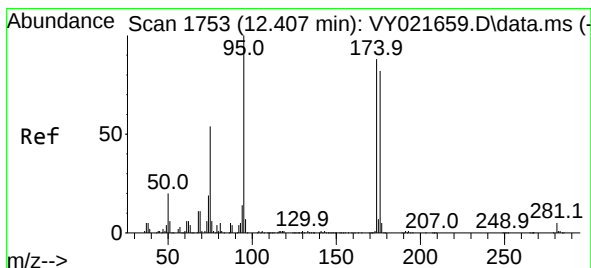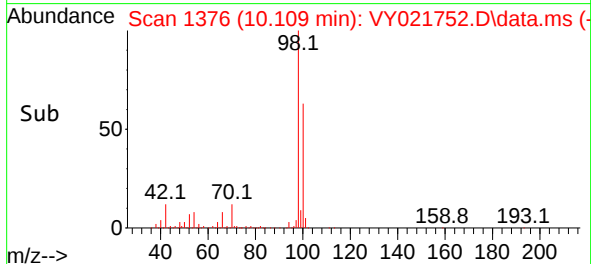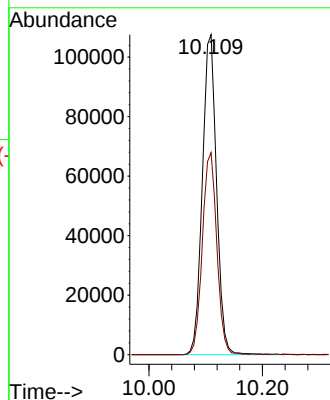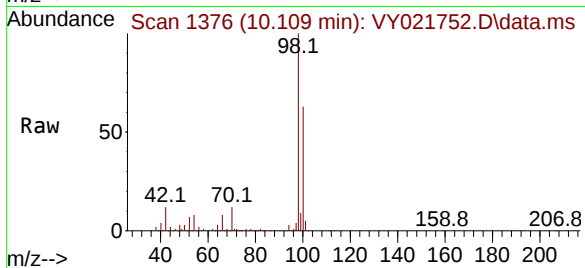

#62

4-Bromofluorobenzene

Concen: 38.035 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.000 min

Lab File: VY021752.D

Acq: 02 Apr 2025 12:11




Tgt Ion: 95 Resp: 49857


Ion Ratio Lower Upper

95 100

174 84.6 0.0 170.8

176 80.0 0.0 162.0


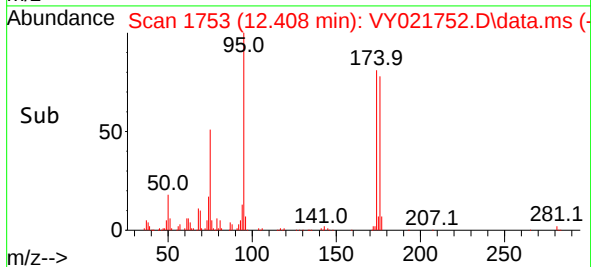
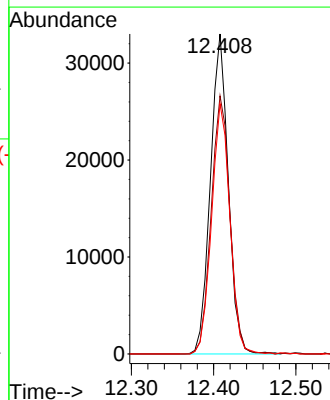
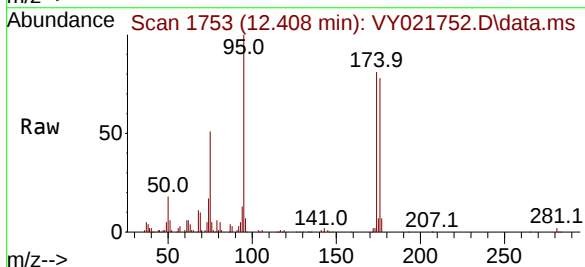


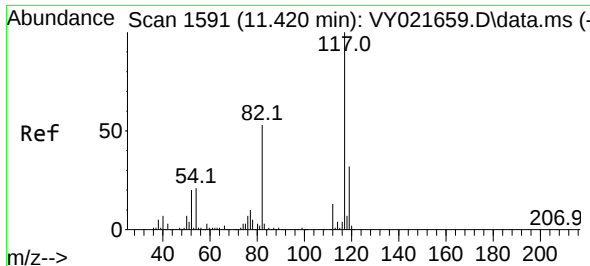

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11

Instrument :
MSVOA_Y
ClientSampleId :
72-12016

Tgt Ion:117 Resp: 136588
Ion Ratio Lower Upper
117 100
82 56.6 42.8 64.2
119 32.4 25.7 38.5

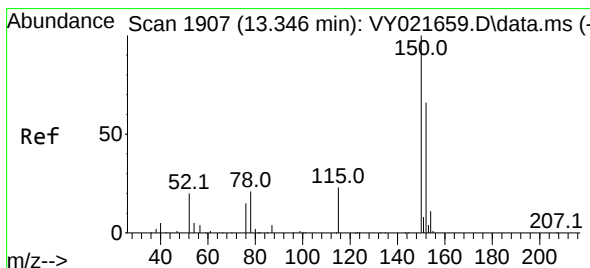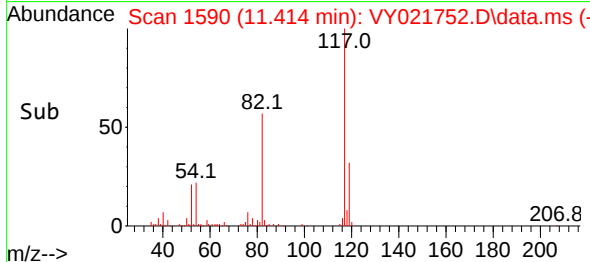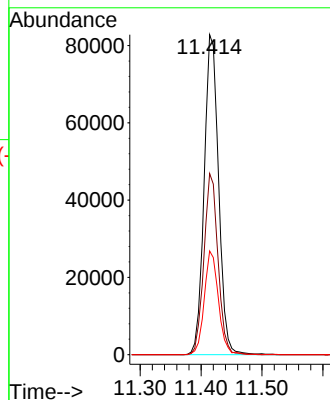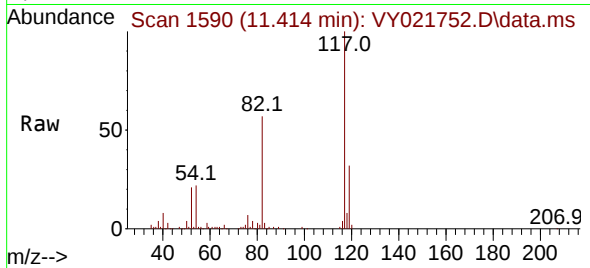

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY021752.D
Acq: 02 Apr 2025 12:11

Tgt Ion:152 Resp: 45953
Ion Ratio Lower Upper
152 100
115 59.2 28.8 86.5
150 156.9 0.0 348.4

