

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040225\
 Data File : VY021758.D
 Acq On : 02 Apr 2025 14:31
 Operator : SY/MD
 Sample : Q1693-03
 Misc : 5.31g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WCS-TP-3-VOC

Quant Time: Apr 03 03:36:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	214137	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	424062	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	411281	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	172509	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	144887	62.448	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.900%
35) Dibromofluoromethane	7.628	113	146908	53.405	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.820%
50) Toluene-d8	10.103	98	527896	50.444	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.880%
62) 4-Bromofluorobenzene	12.402	95	176232	49.787	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	99.580%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040225\
Data File : VY021758.D
Acq On : 02 Apr 2025 14:31
Operator : SY/MD
Sample : Q1693-03
Misc : 5.31g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WCS-TP-3-VOC

Quant Time: Apr 03 03:36:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




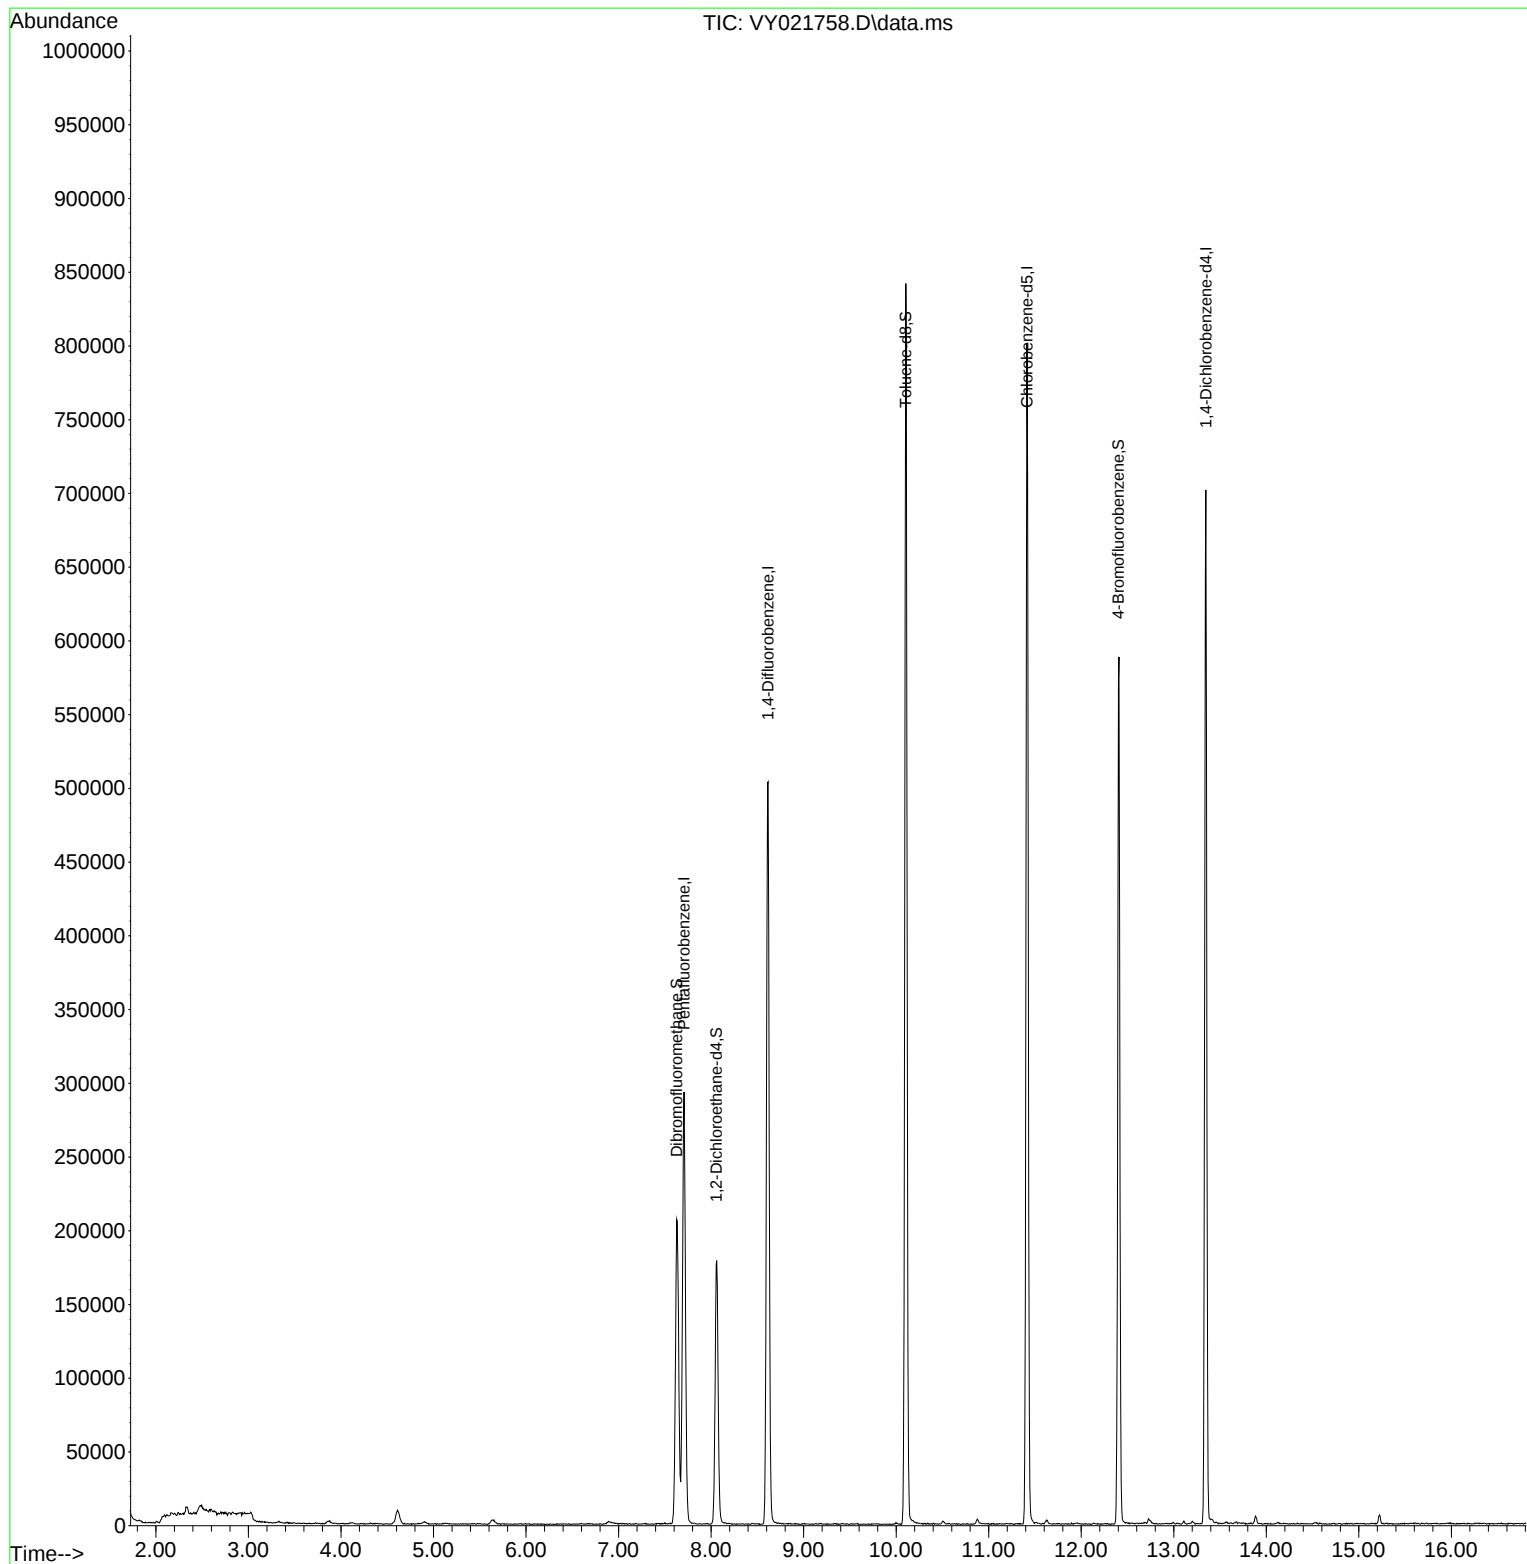




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31




Instrument :
MSVOA_Y
ClientSampleId :
WCS-TP-3-VOC


Tgt Ion:168 Resp: 214137
Ion Ratio Lower Upper
168 100
99 55.7 46.7 70.1

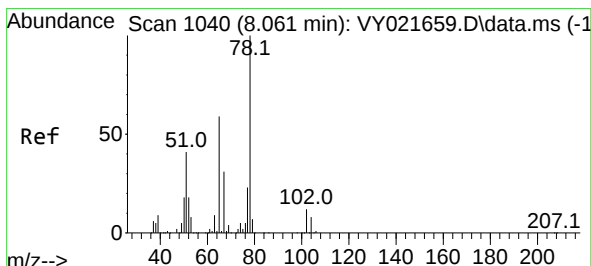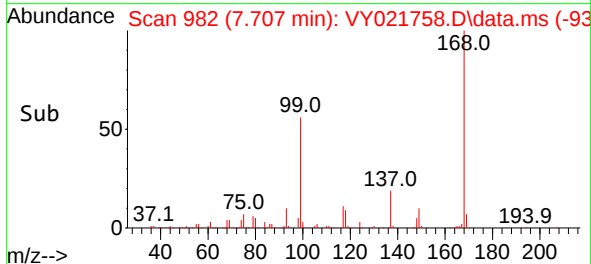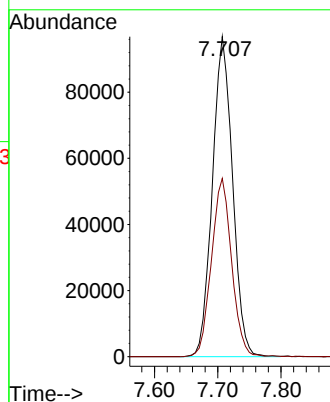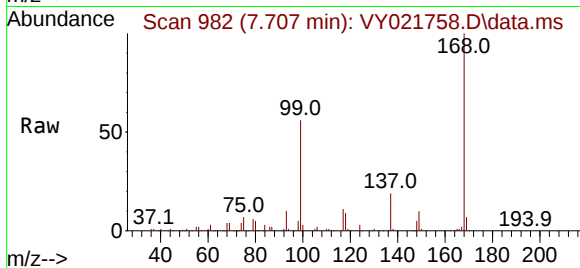

#33
1,2-Dichloroethane-d4
Concen: 62.448 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. -0.006 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31

Tgt Ion: 65 Resp: 144887
Ion Ratio Lower Upper
65 100
67 51.0 0.0 104.6


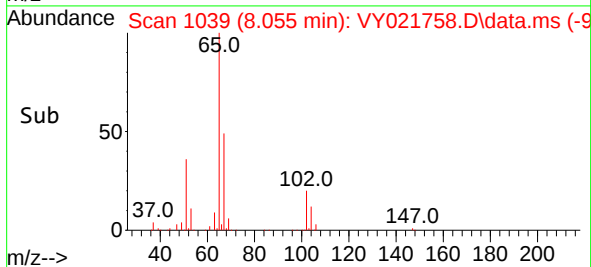
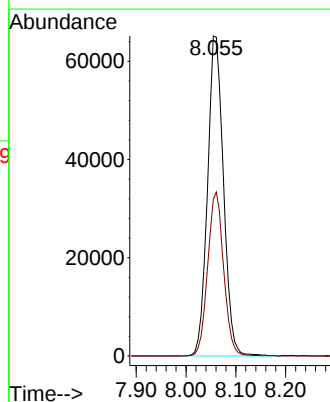
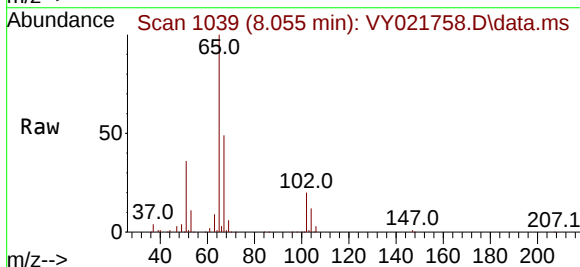


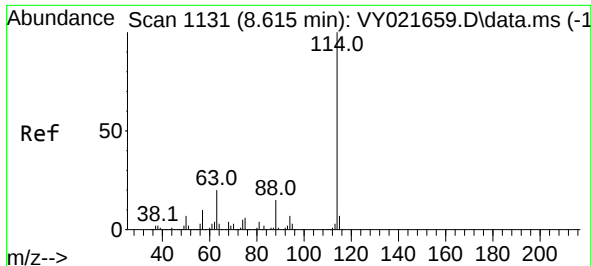

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31




Instrument :
MSVOA_Y
ClientSampleId :
WCS-TP-3-VOC


Tgt Ion:114 Resp: 424062
Ion Ratio Lower Upper
114 100
63 21.1 0.0 40.2
88 15.8 0.0 29.8

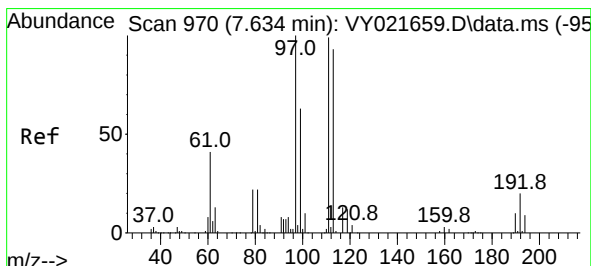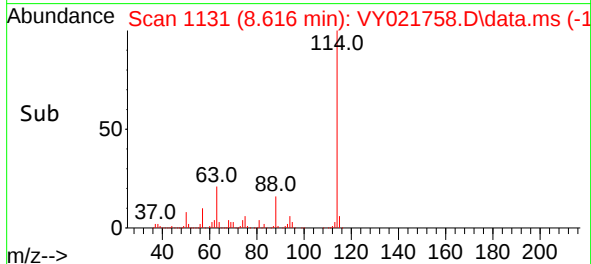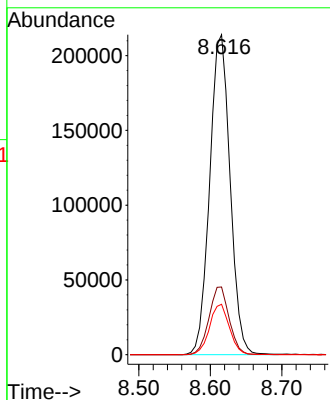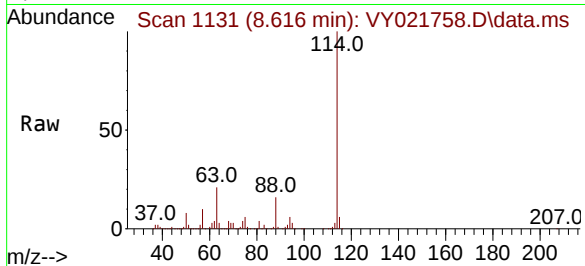

#35
Dibromofluoromethane
Concen: 53.405 ug/l
RT: 7.628 min Scan# 969
Delta R.T. -0.006 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31

Tgt Ion:113 Resp: 146908
Ion Ratio Lower Upper
113 100
111 101.5 82.6 123.8
192 19.6 16.2 24.4


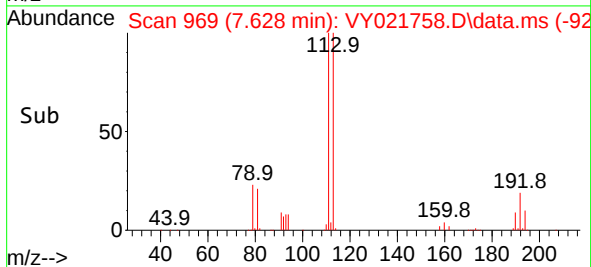
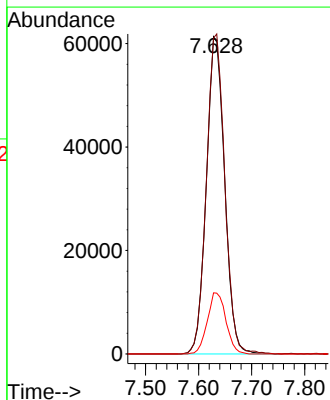
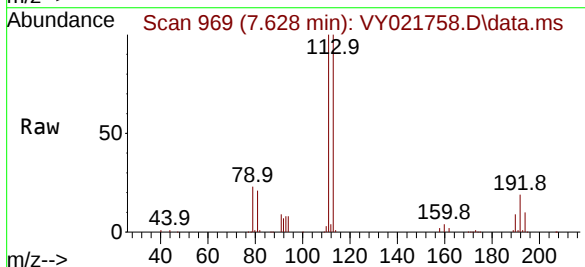


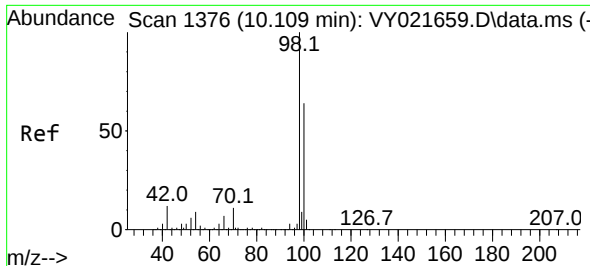

#50
Toluene-d8
Concen: 50.444 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31




Instrument :
MSVOA_Y
ClientSampleId :
WCS-TP-3-VOC


Tgt Ion: 98 Resp: 527896
Ion Ratio Lower Upper
98 100
100 64.5 52.1 78.1

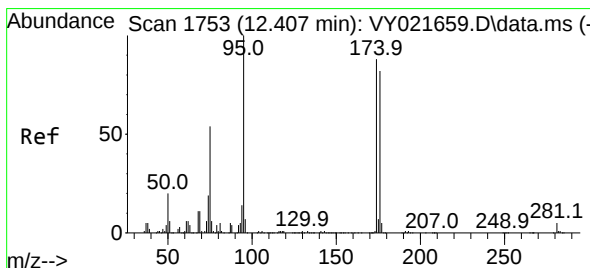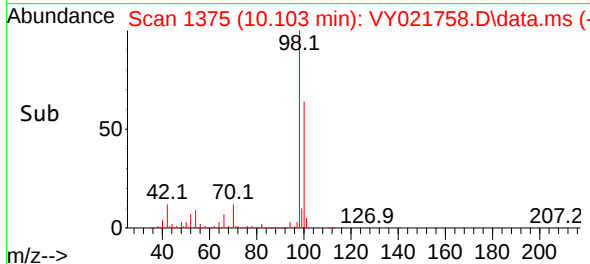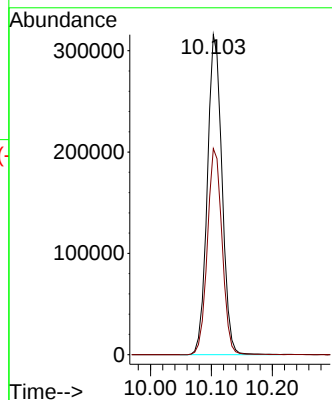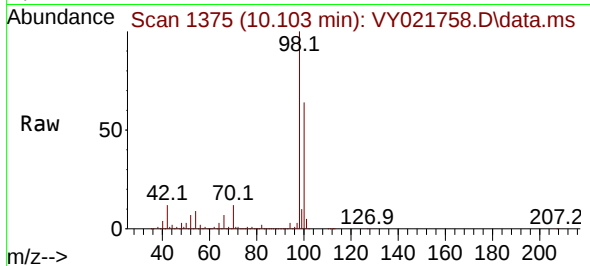

#62
4-Bromofluorobenzene
Concen: 49.787 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY021758.D
Acq: 02 Apr 2025 14:31

Tgt Ion: 95 Resp: 176232
Ion Ratio Lower Upper
95 100
174 82.8 0.0 170.8
176 79.2 0.0 162.0

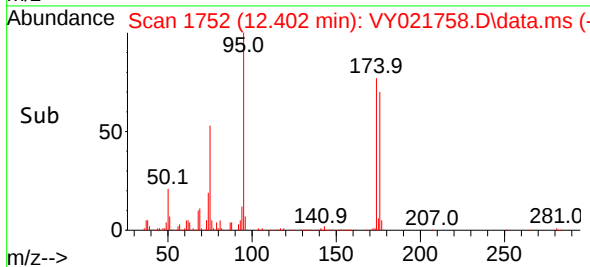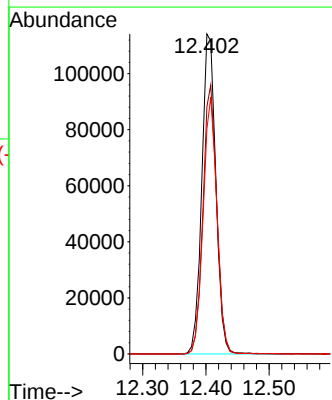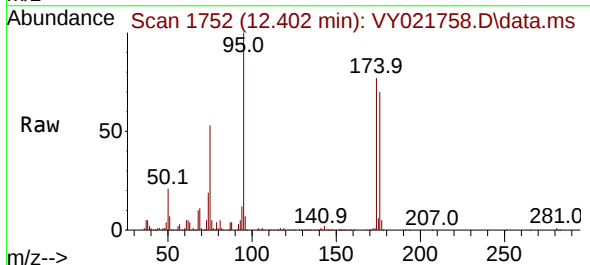

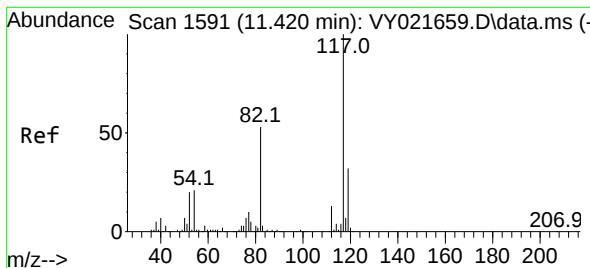

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY021758.D

Acq: 02 Apr 2025 14:31

Instrument :

MSVOA_Y

ClientSampleId :

WCS-TP-3-VOC





Tgt Ion:117 Resp: 411281

Ion Ratio Lower Upper

117 100

82 57.4 42.8 64.2

119 32.4 25.7 38.5

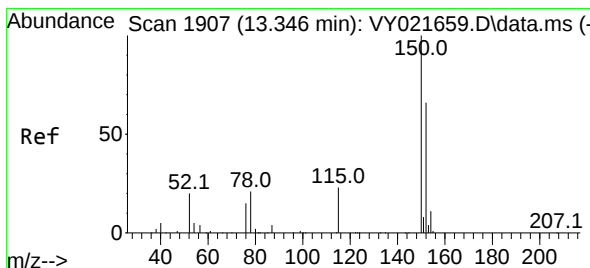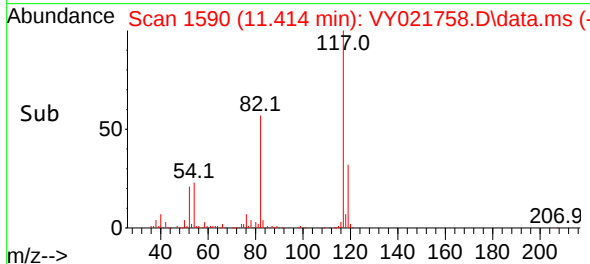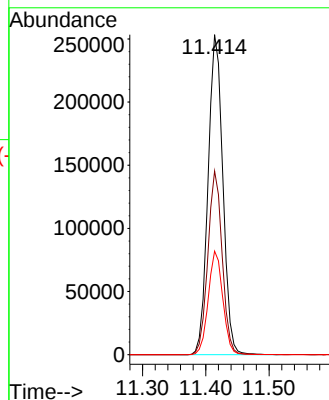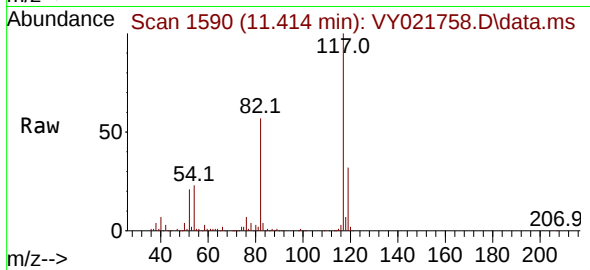

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY021758.D

Acq: 02 Apr 2025 14:31

Tgt Ion:152 Resp: 172509

Ion Ratio Lower Upper

152 100

115 58.1 28.8 86.5

150 158.0 0.0 348.4

