
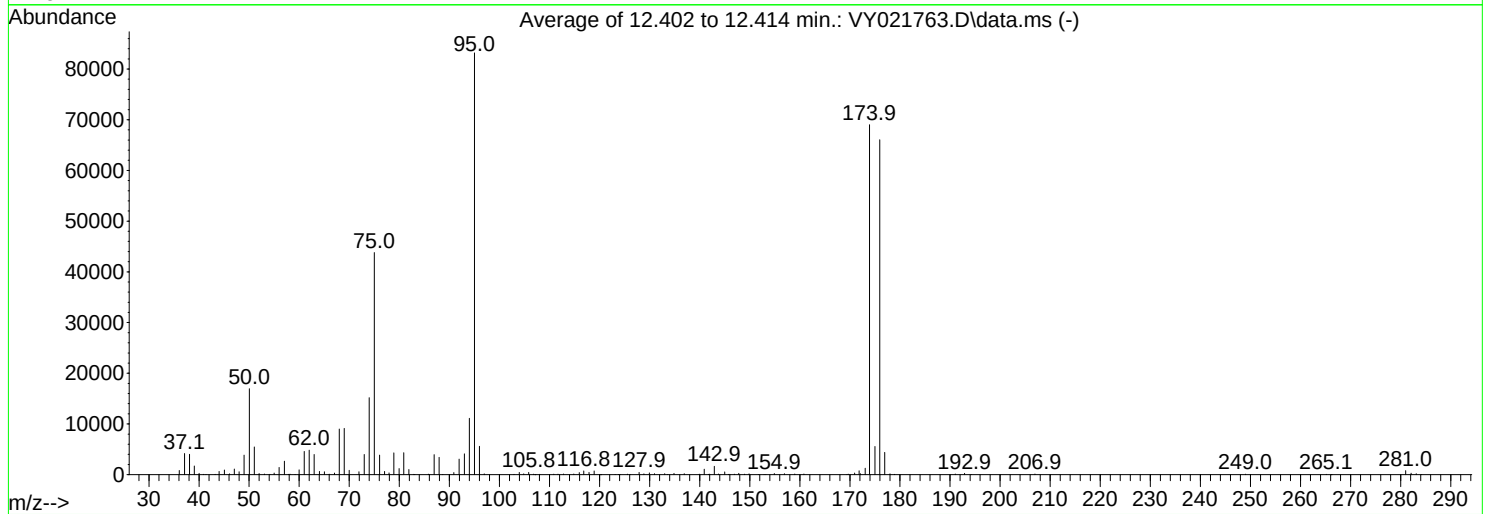


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040325\
Data File : VY021763.D
Acq On : 03 Apr 2025 10:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Title : SW846 8260
Last Update : Fri Mar 28 02:30:29 2025

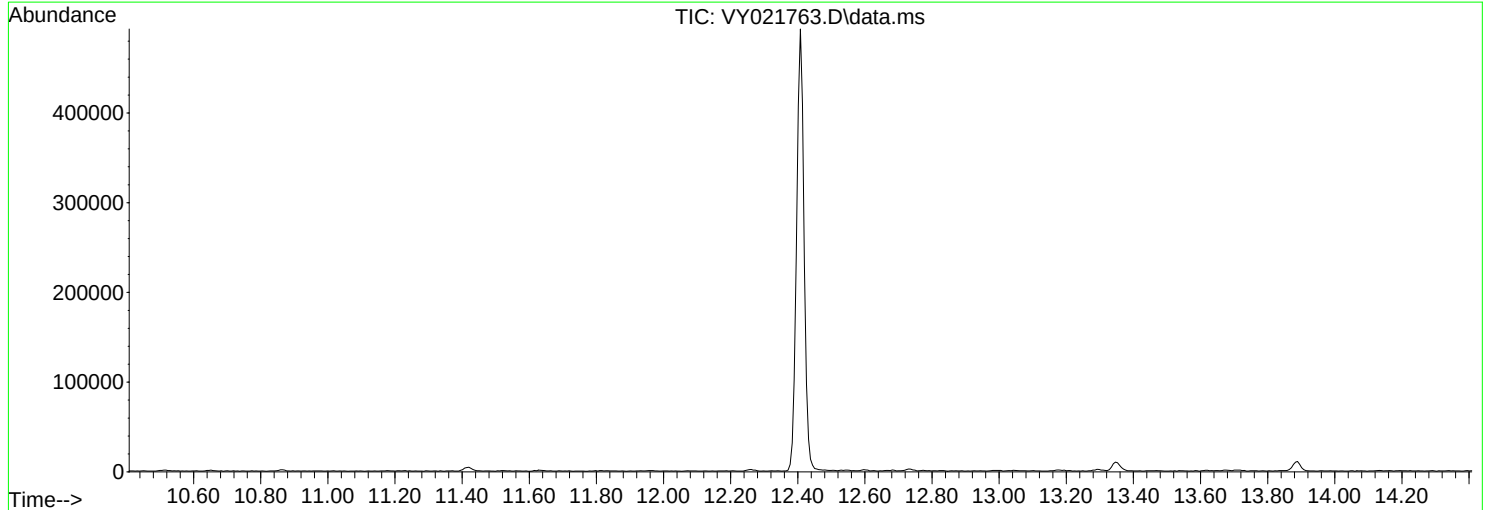

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	16938	PASS
75	95	30	60	52.7	43819	PASS
95	95	100	100	100.0	83192	PASS
96	95	5	9	6.7	5582	PASS
173	174	0.00	2	1.8	1273	PASS
174	95	50	100	83.0	69027	PASS
175	174	5	9	8.1	5565	PASS
176	174	95	101	95.7	66037	PASS
177	176	5	9	6.6	4384	PASS