

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040422\
 Data File : VY008189.D
 Acq On : 04 Apr 2022 18:36
 Operator : SY/MD
 Sample : N2237-06
 Misc : 4.64g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 A01015

Quant Time: Apr 05 04:43:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	49295	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	58033	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	19734	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	1684	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	4632	9.366	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	18.740%#
35) Dibromofluoromethane	7.716	113	10689	29.377	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	58.760%
50) Toluene-d8	10.179	98	54931	40.072	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	80.140%
62) 4-Bromofluorobenzene	12.483	95	3810	7.878	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	15.760%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040422\
Data File : VY008189.D
Acq On : 04 Apr 2022 18:36
Operator : SY/MD
Sample : N2237-06
Misc : 4.64g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
A01015

Quant Time: Apr 05 04:43:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




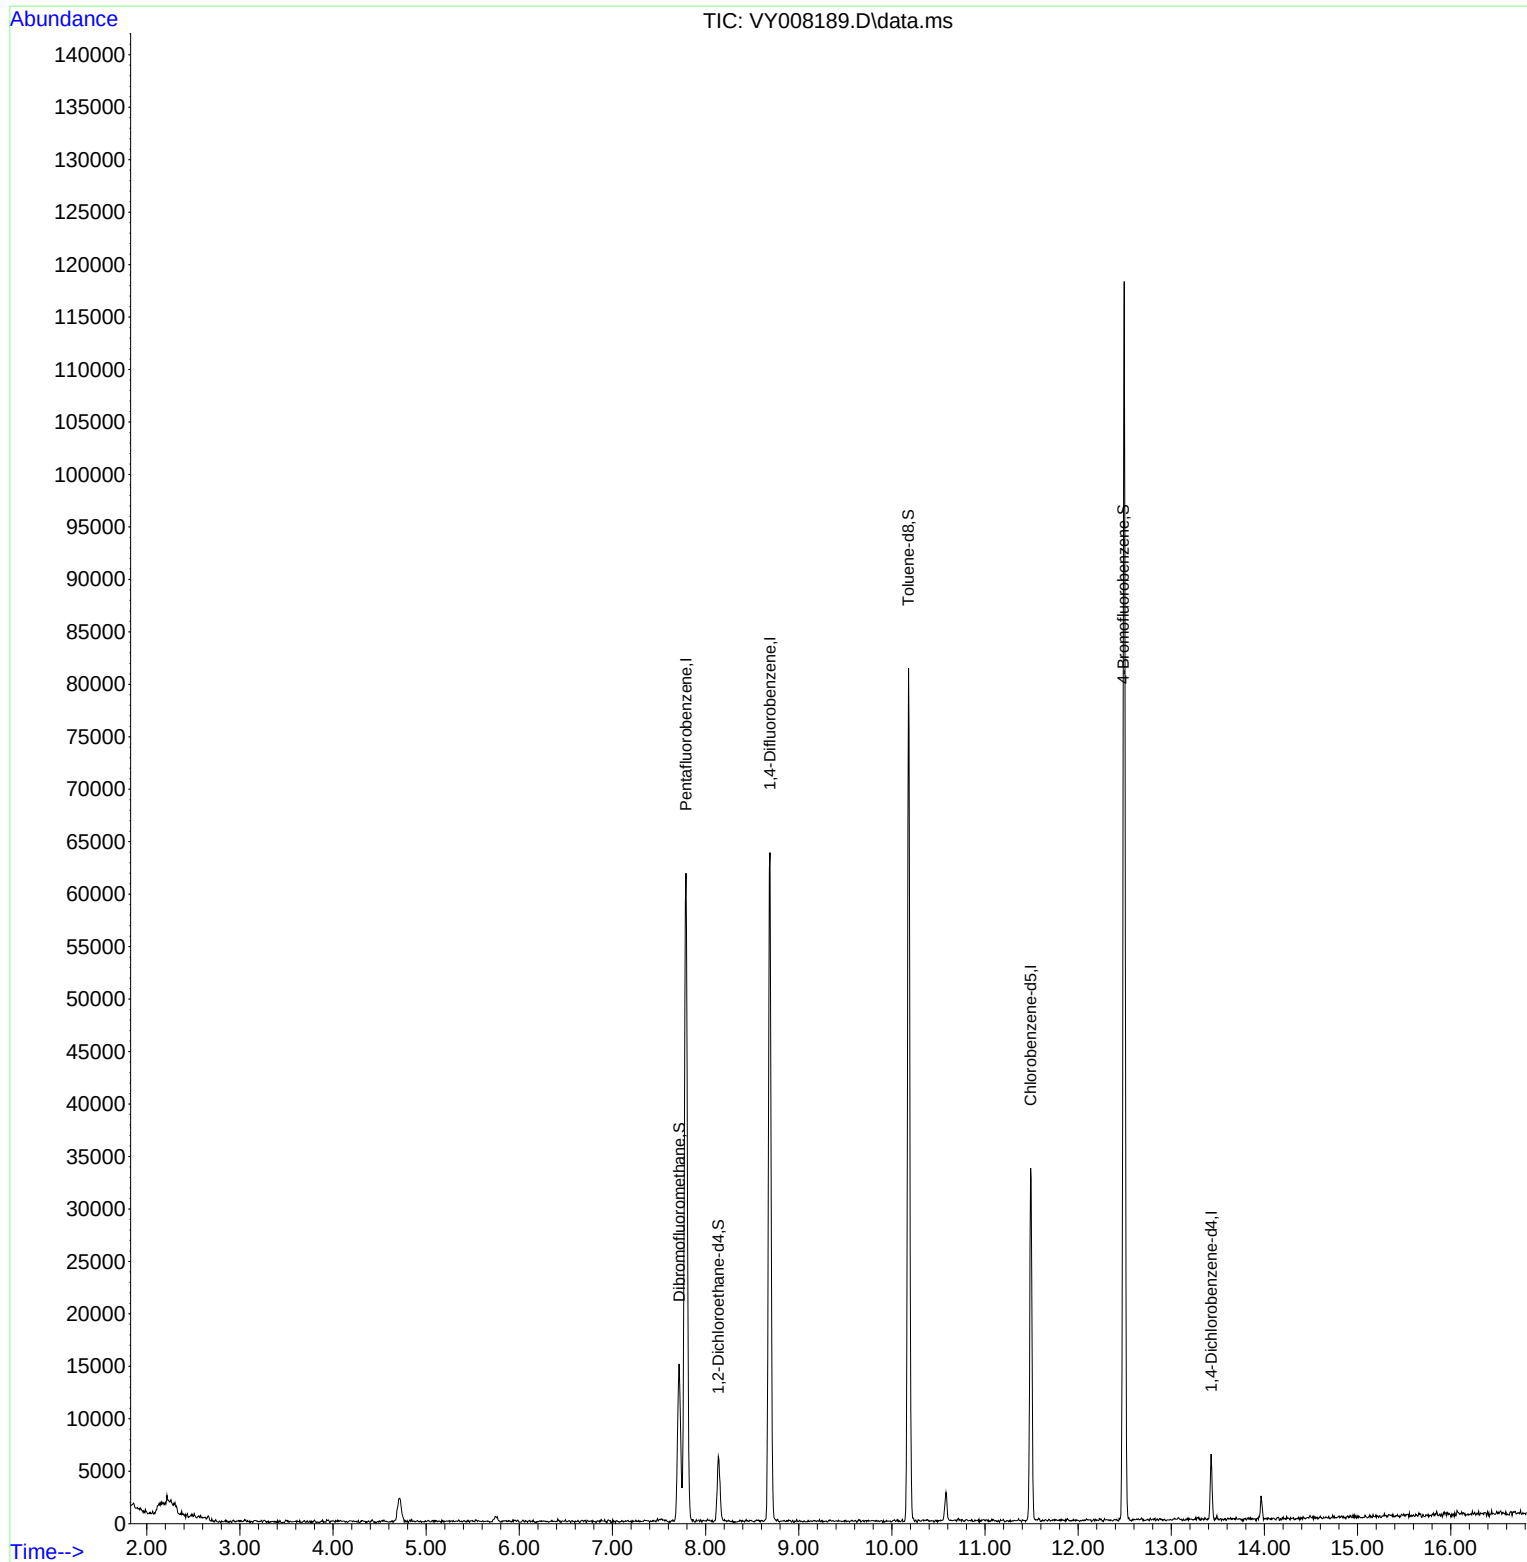


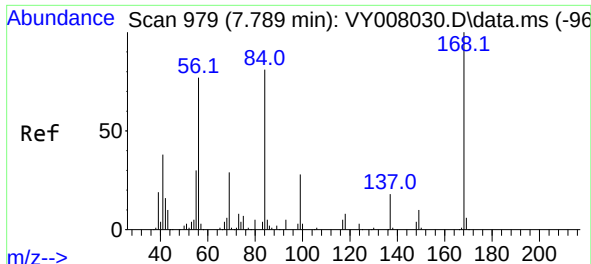

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36




Instrument :
MSVOA_Y
ClientSampleId :
A01015


Tgt Ion:168 Resp: 49295
Ion Ratio Lower Upper
168 100
99 58.8 46.9 70.3

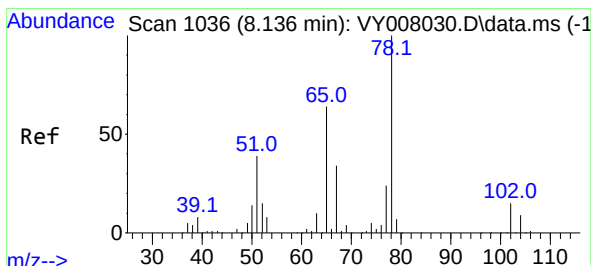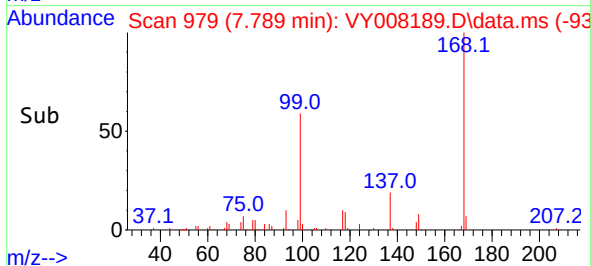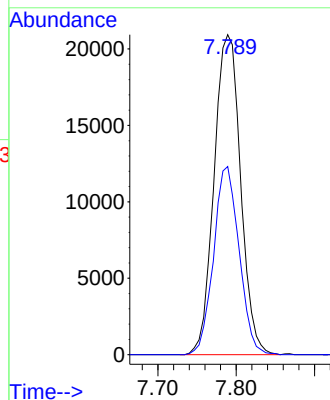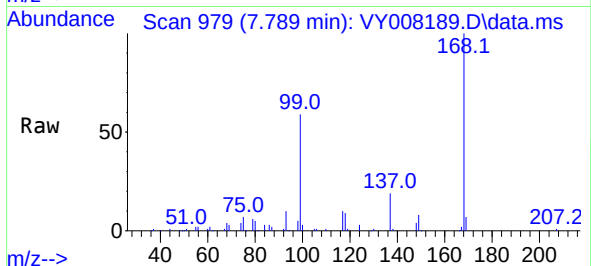

#33
1,2-Dichloroethane-d4
Concen: 9.366 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36

Tgt Ion: 65 Resp: 4632
Ion Ratio Lower Upper
65 100
67 58.9 0.0 99.4

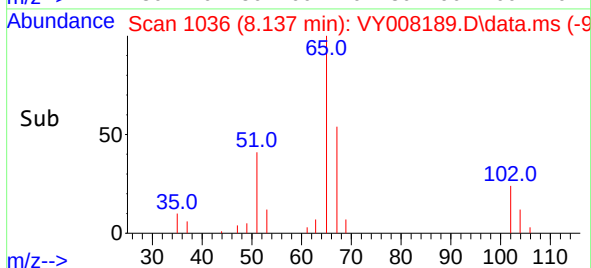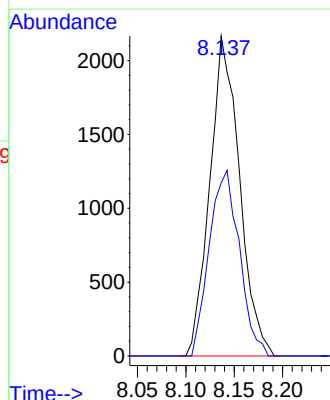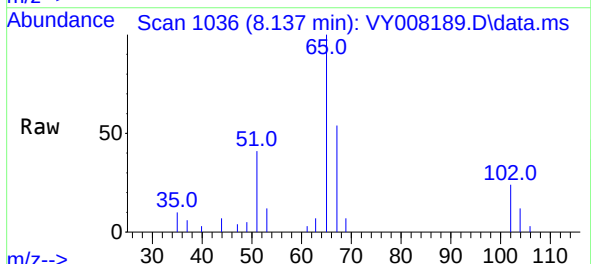

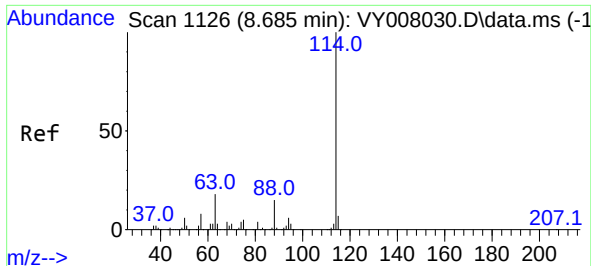

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY008189.D

Acq: 04 Apr 2022 18:36

Instrument :

MSVOA_Y

ClientSampleId :

A01015





Tgt Ion:114 Resp: 58033

Ion Ratio Lower Upper

114 100

63 18.6 0.0 43.2

88 14.3 0.0 31.8

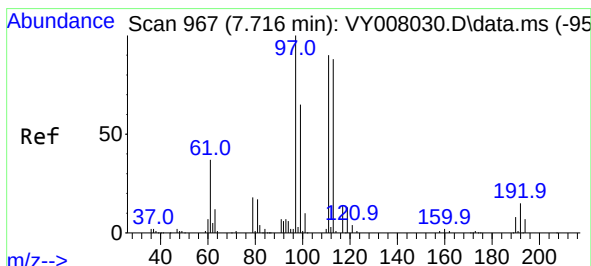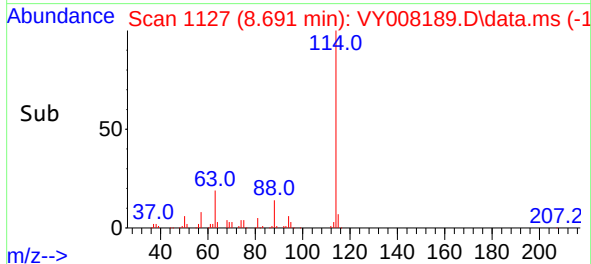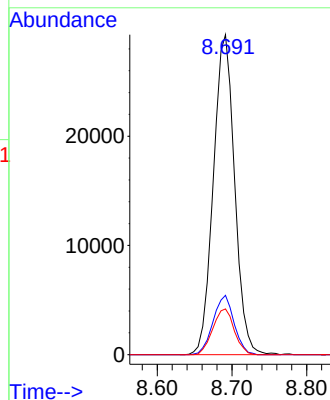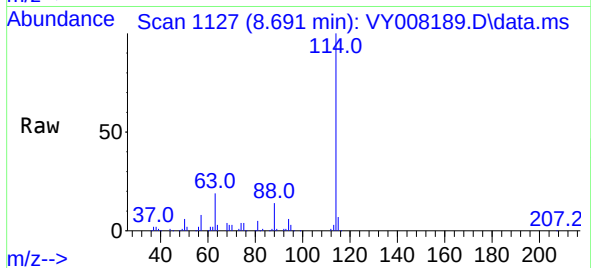

#35

Dibromofluoromethane

Concen: 29.377 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008189.D

Acq: 04 Apr 2022 18:36




Tgt Ion:113 Resp: 10689


Ion Ratio Lower Upper

113 100

111 102.2 82.6 124.0

192 17.7 17.6 26.4


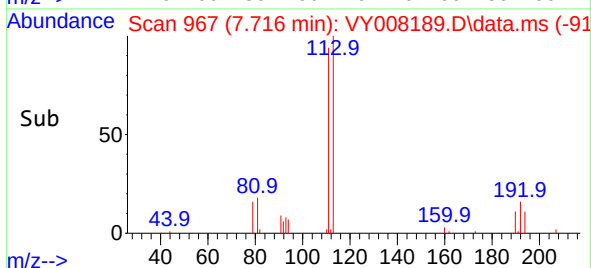
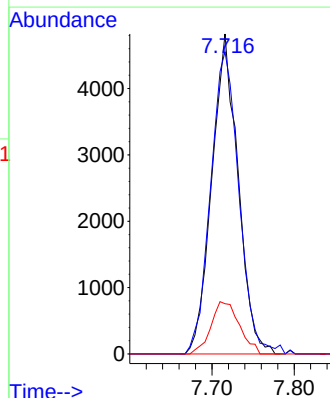
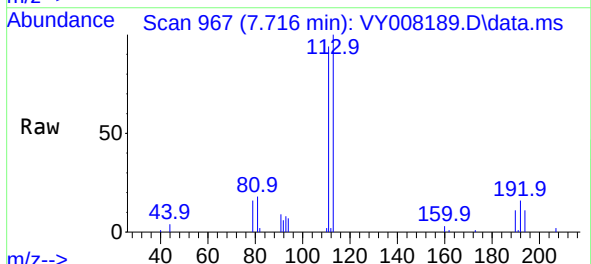


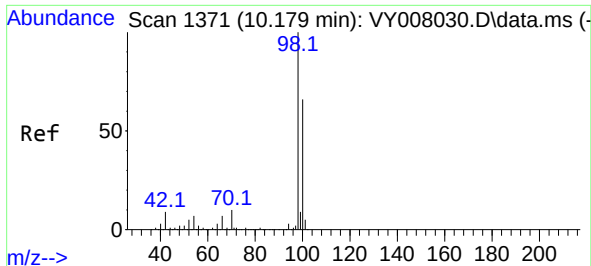

#50
Toluene-d8
Concen: 40.072 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36




Instrument :
MSVOA_Y
ClientSampleId :
A01015


Tgt Ion: 98 Resp: 54931
Ion Ratio Lower Upper
98 100
100 65.4 50.2 75.2

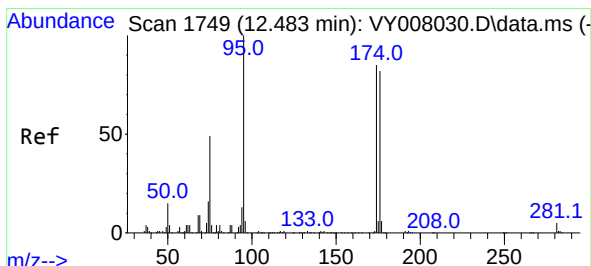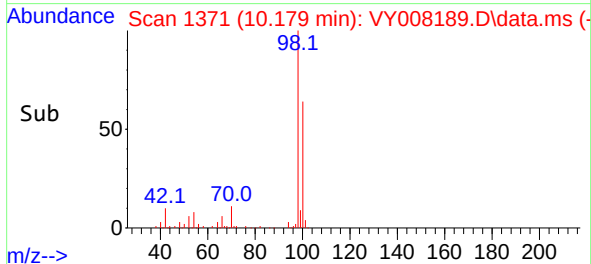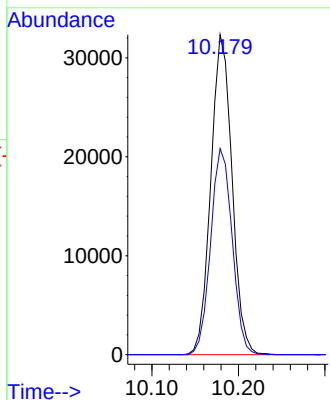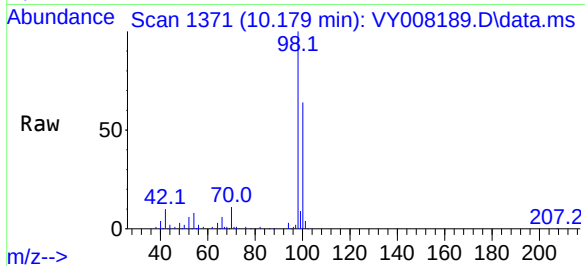

#62
4-Bromofluorobenzene
Concen: 7.878 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36

Tgt Ion: 95 Resp: 3810
Ion Ratio Lower Upper
95 100
174 88.1 0.0 177.0
176 95.2 0.0 175.8


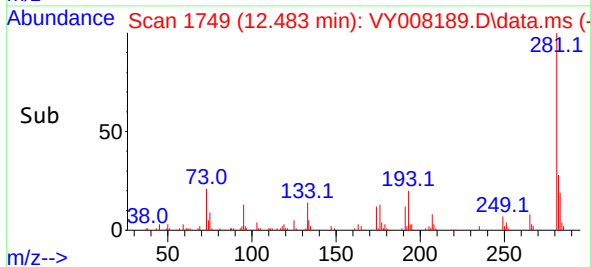
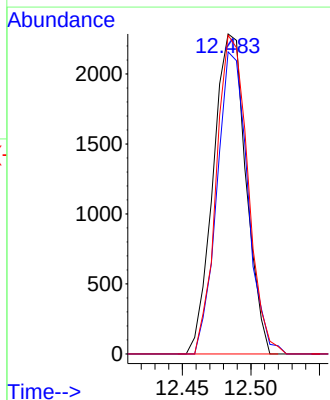
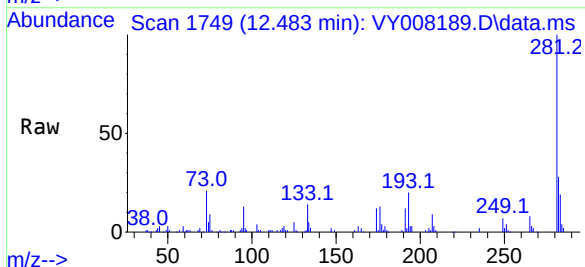


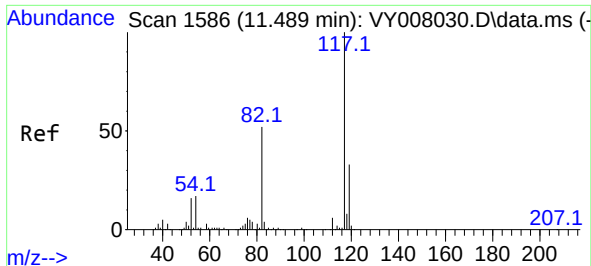

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11734
Delta R.T. 0.001 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36

Instrument :
MSVOA_Y
ClientSampleId :
A01015

Tgt Ion:	117	Resp:	19734
Ion	Ratio	Lower	Upper
117	100		
82	54.7	43.0	64.4
119	31.0	25.4	38.0

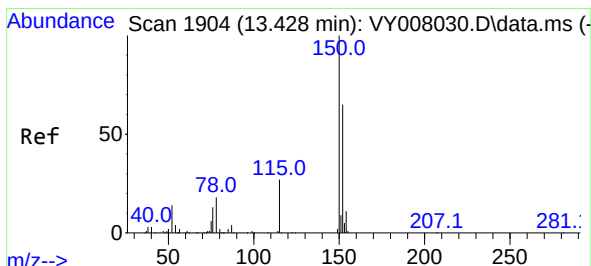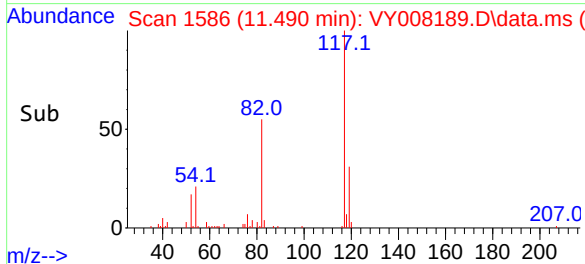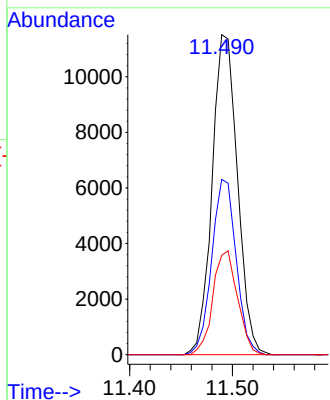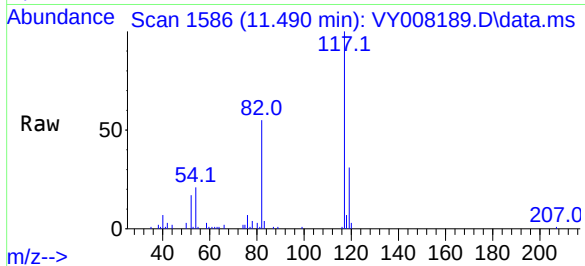

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008189.D
Acq: 04 Apr 2022 18:36

Tgt Ion:	152	Resp:	1684
Ion	Ratio	Lower	Upper
152	100		
115	61.8	28.2	84.7
150	168.1	0.0	347.6

