

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040522\
 Data File : VY008215.D
 Acq On : 05 Apr 2022 17:24
 Operator : SY/MD
 Sample : N2257-01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1

Quant Time: Apr 06 03:58:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	110793	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	205258	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	194141	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	85133	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	63246	56.897	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.800%
35) Dibromofluoromethane	7.716	113	63512	49.352	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.700%
50) Toluene-d8	10.179	98	250472	51.660	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.320%
62) 4-Bromofluorobenzene	12.483	95	82594	48.285	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040522\
Data File : VY008215.D
Acq On : 05 Apr 2022 17:24
Operator : SY/MD
Sample : N2257-01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Quant Time: Apr 06 03:58:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration




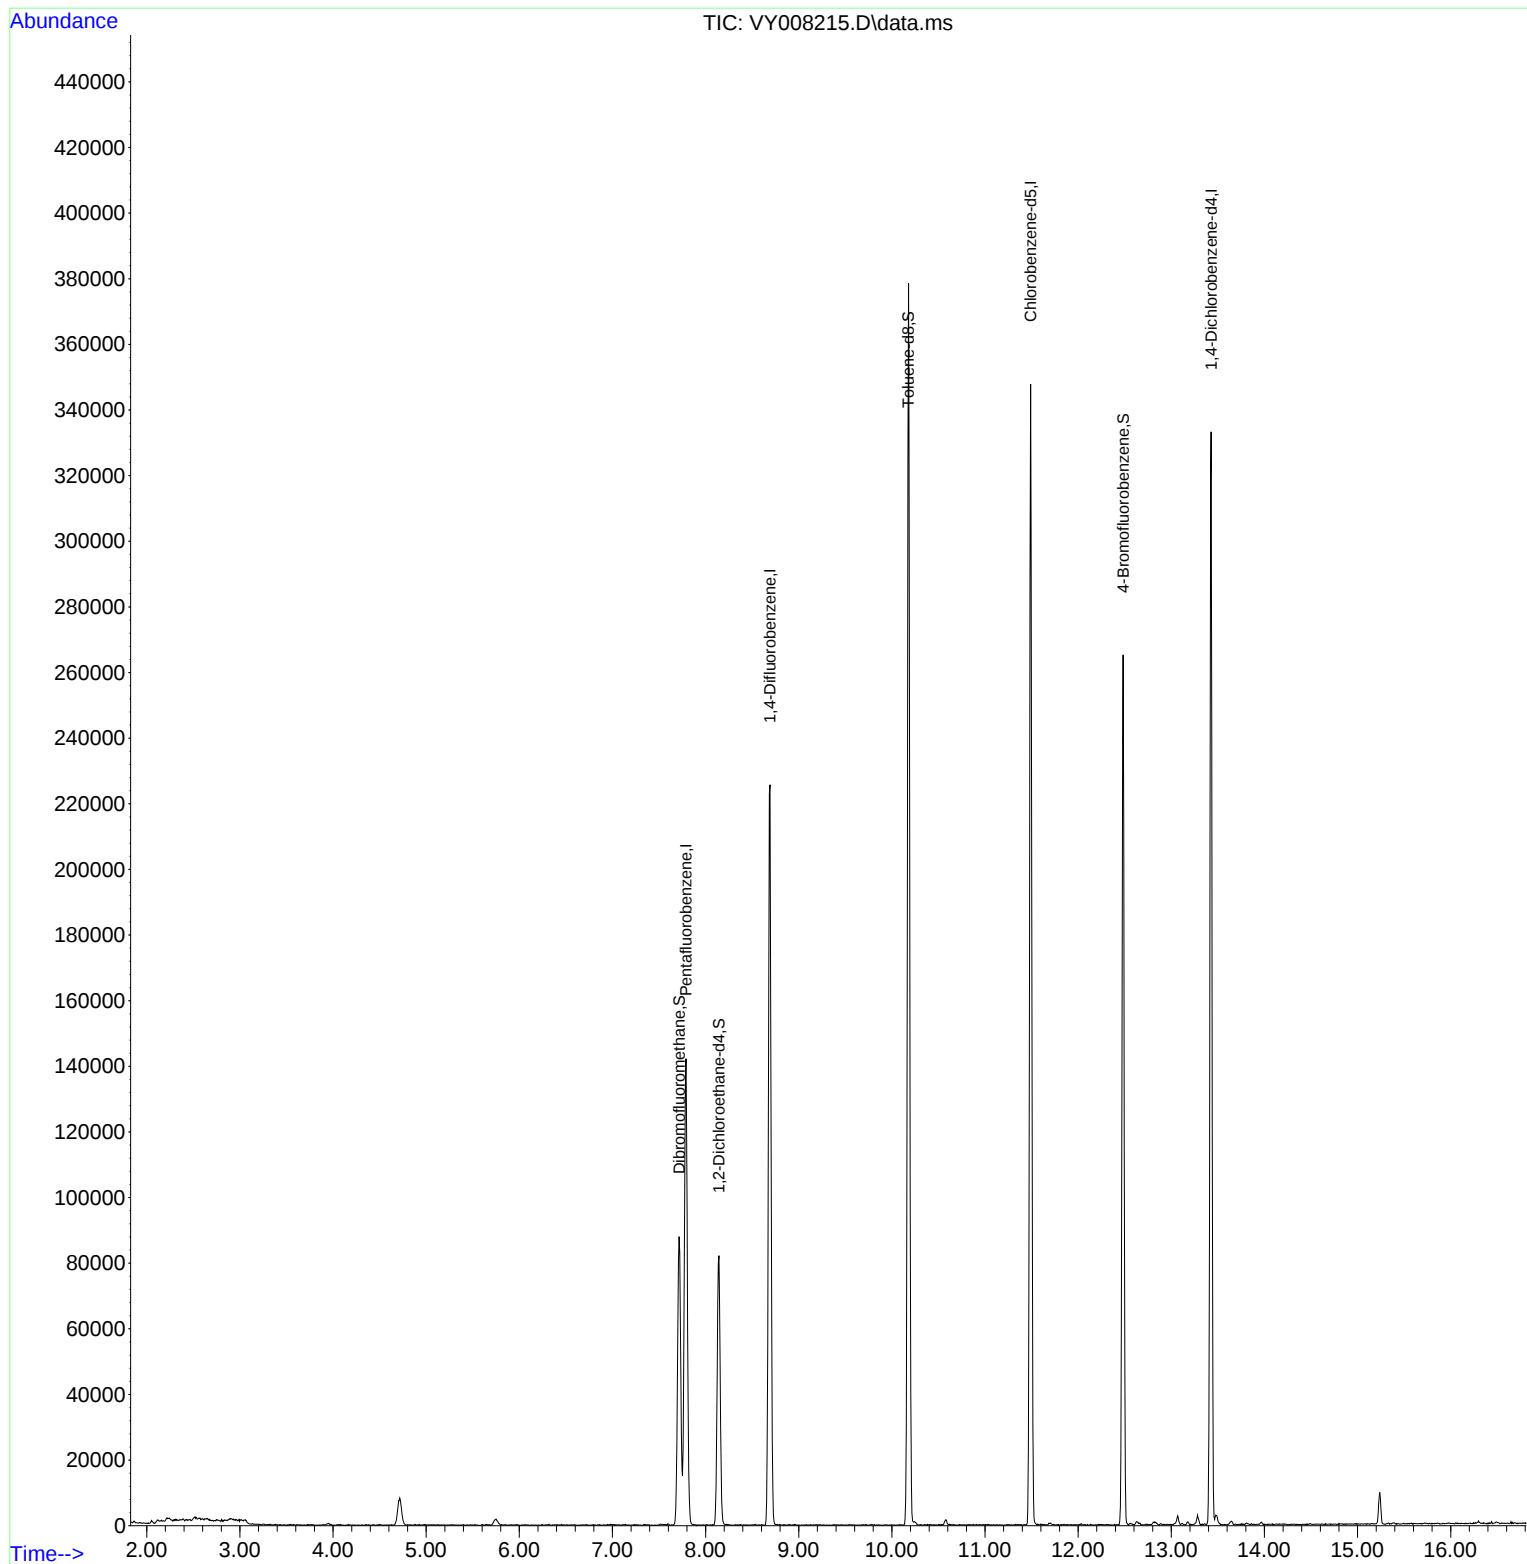


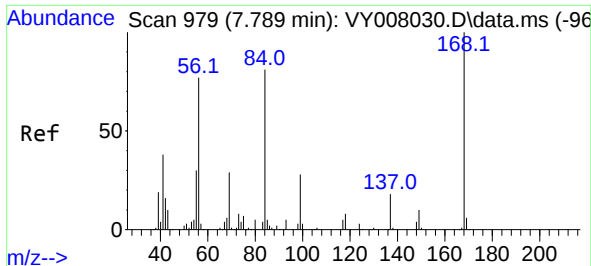

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 110793
Ion Ratio Lower Upper
168 100
99 53.0 46.9 70.3

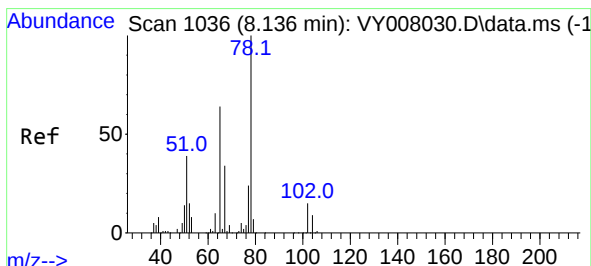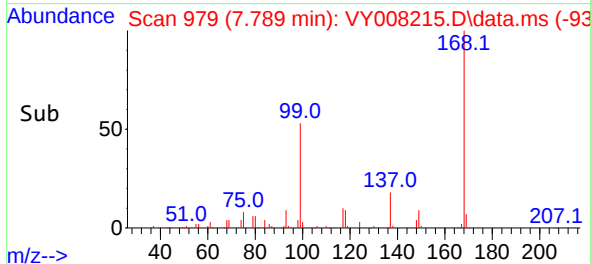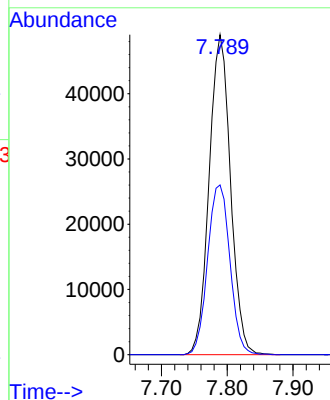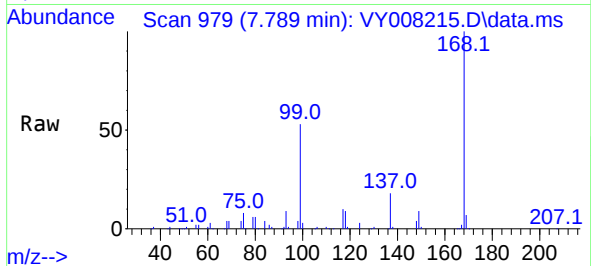

#33
1,2-Dichloroethane-d4
Concen: 56.897 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24

Tgt Ion: 65 Resp: 63246
Ion Ratio Lower Upper
65 100
67 54.5 0.0 99.4

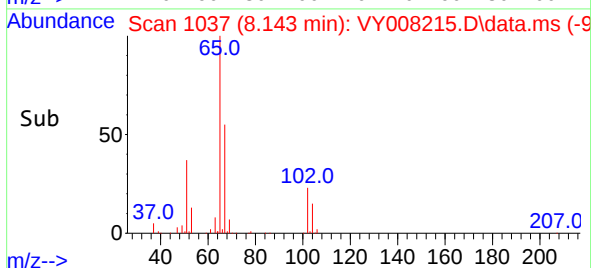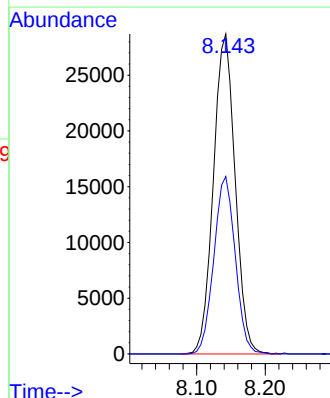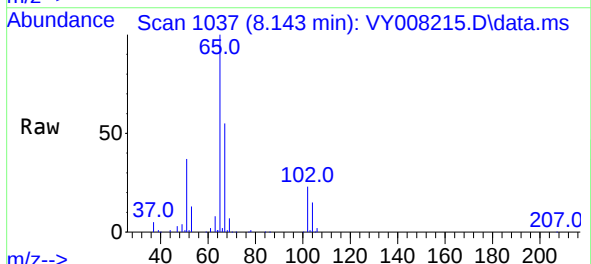

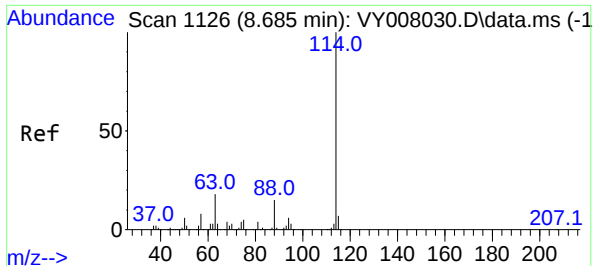

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY008215.D

Acq: 05 Apr 2022 17:24

Instrument :

MSVOA_Y

ClientSampleId :

TP-1





Tgt Ion:114 Resp: 205258

Ion Ratio Lower Upper

114 100

63 17.1 0.0 43.2

88 13.9 0.0 31.8

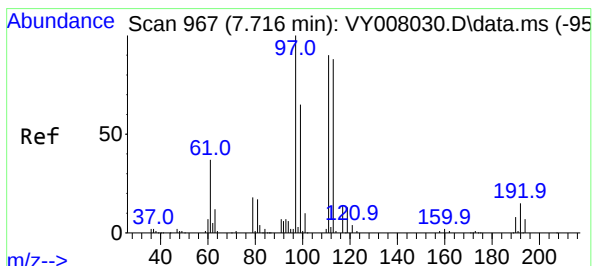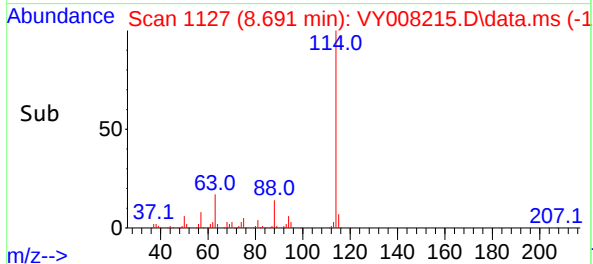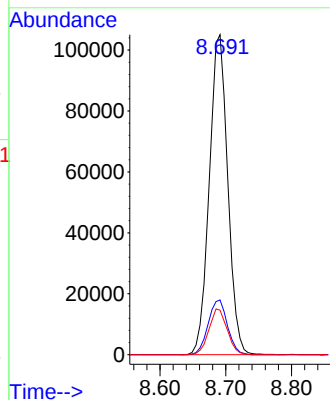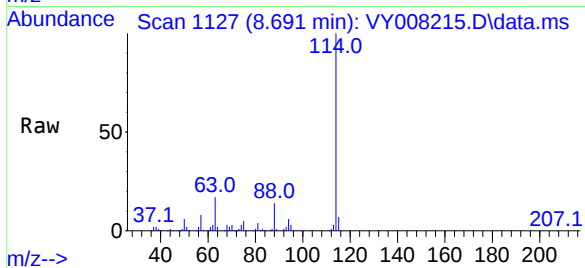

#35

Dibromofluoromethane

Concen: 49.352 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008215.D

Acq: 05 Apr 2022 17:24




Tgt Ion:113 Resp: 63512


Ion Ratio Lower Upper

113 100

111 103.1 82.6 124.0

192 18.9 17.6 26.4

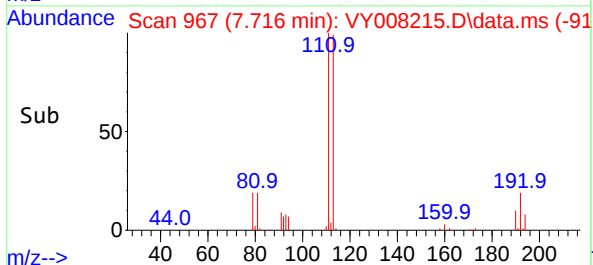
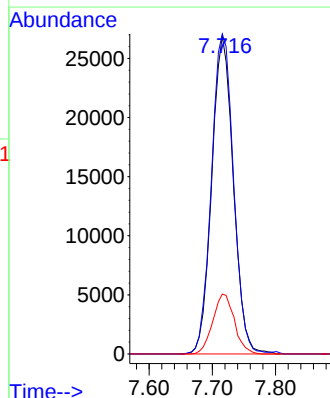
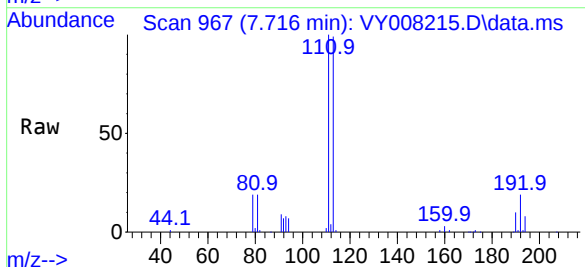


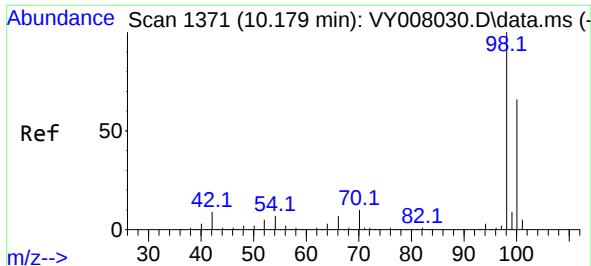

#50
Toluene-d8
Concen: 51.660 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion: 98 Resp: 250472
Ion Ratio Lower Upper
98 100
100 65.0 50.2 75.2

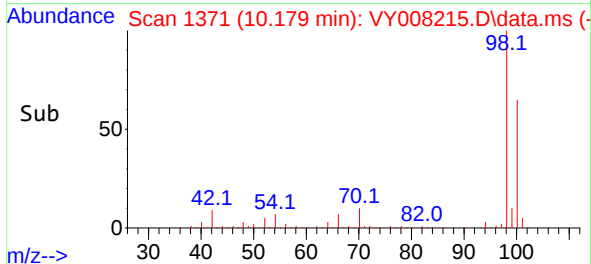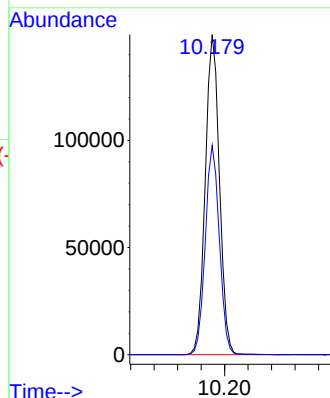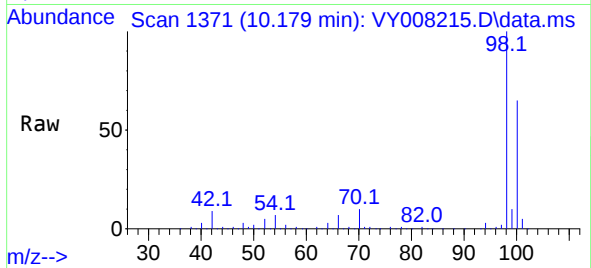

#62
4-Bromofluorobenzene
Concen: 48.285 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24

Tgt Ion: 95 Resp: 82594
Ion Ratio Lower Upper
95 100
174 81.9 0.0 177.0
176 79.8 0.0 175.8


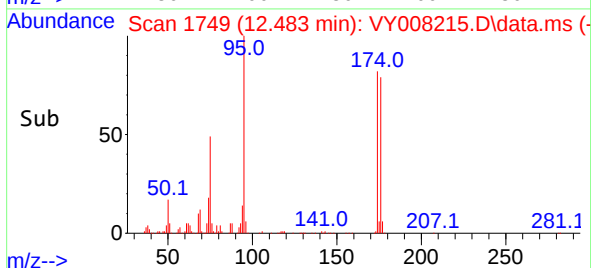
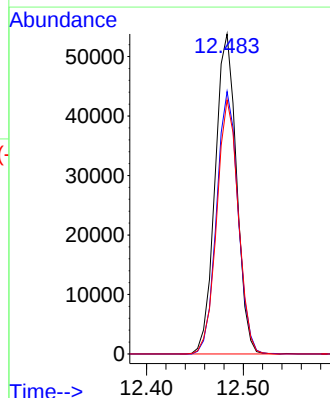
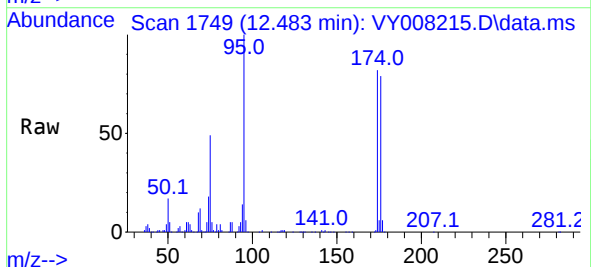


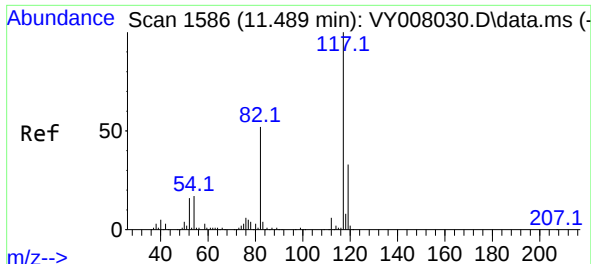

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Tgt Ion:117 Resp: 194141
Ion Ratio Lower Upper
117 100
82 52.2 43.0 64.4
119 32.6 25.4 38.0

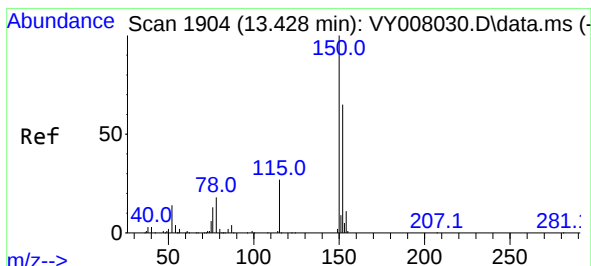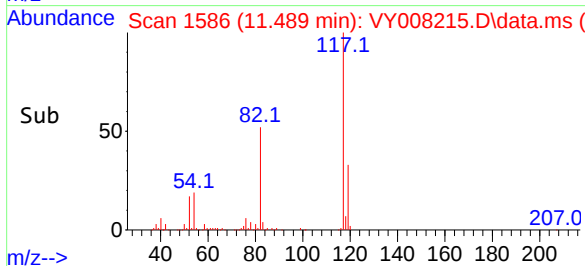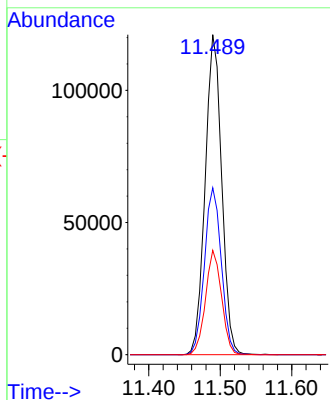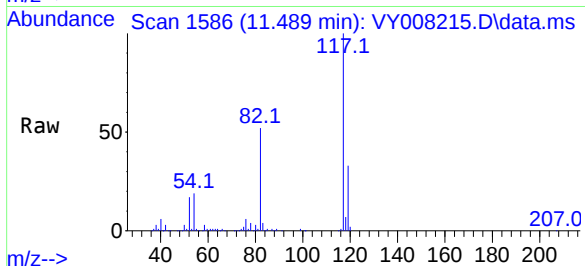

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008215.D
Acq: 05 Apr 2022 17:24

Tgt Ion:152 Resp: 85133
Ion Ratio Lower Upper
152 100
115 57.4 28.2 84.7
150 156.9 0.0 347.6

