

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040722\
 Data File : VY008247.D
 Acq On : 07 Apr 2022 15:24
 Operator : KP/MD
 Sample : N2272-01
 Misc : 3.80g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1

Quant Time: Apr 08 02:35:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 26 03:24:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	116129	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	207285	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	201275	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	90421	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	65152	55.919	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.840%
35) Dibromofluoromethane	7.716	113	65625	50.496	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.000%
50) Toluene-d8	10.179	98	257597	52.610	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.220%
62) 4-Bromofluorobenzene	12.483	95	84721	49.044	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	98.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040722\
Data File : VY008247.D
Acq On : 07 Apr 2022 15:24
Operator : KP/MD
Sample : N2272-01
Misc : 3.80g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Quant Time: Apr 08 02:35:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032522S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 26 03:24:51 2022
Response via : Initial Calibration

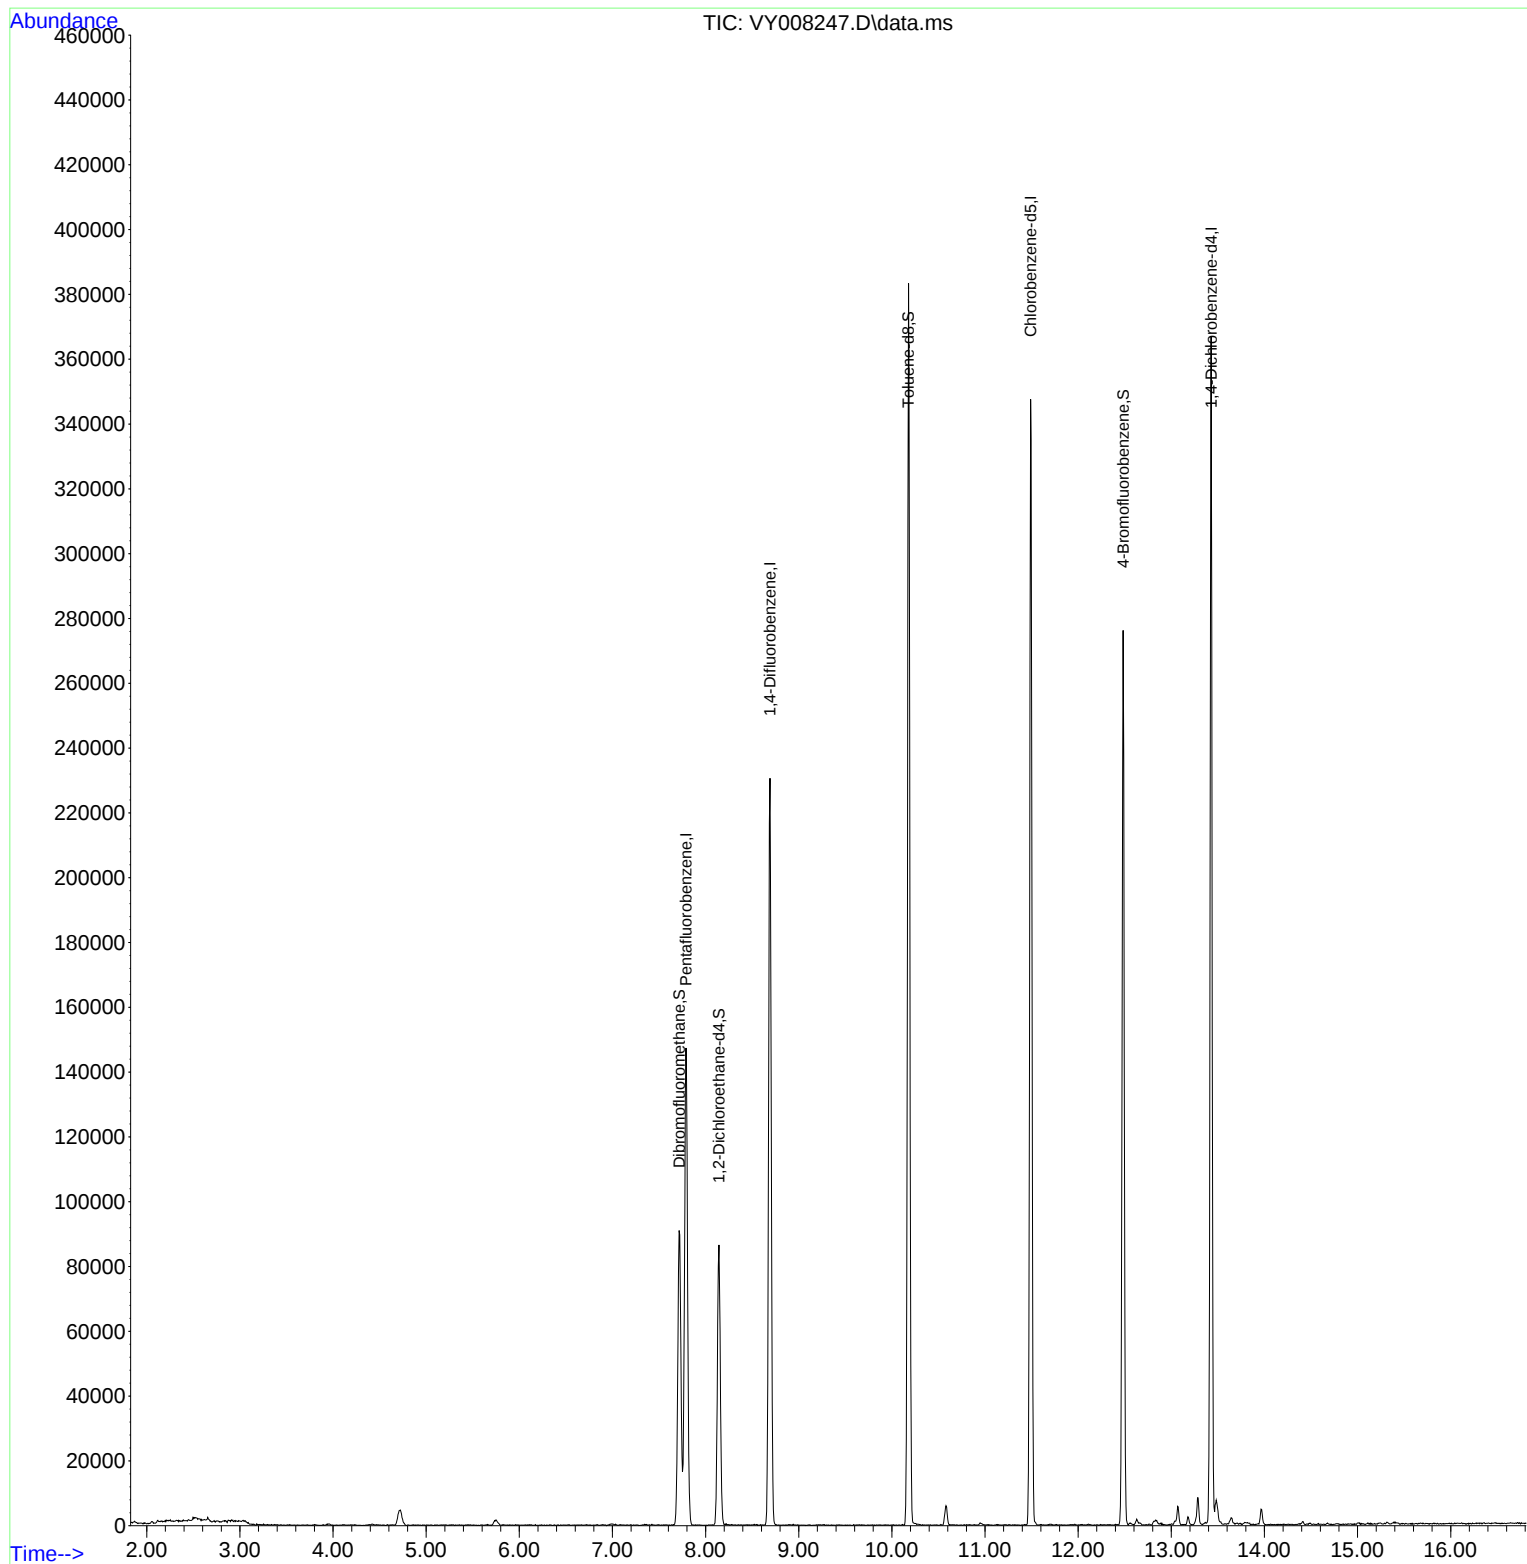



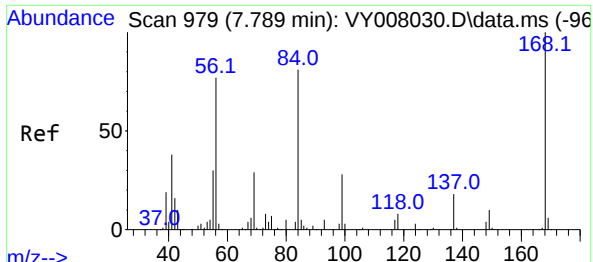


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24


Instrument :
MSVOA_Y
ClientSampleId :
TP-1

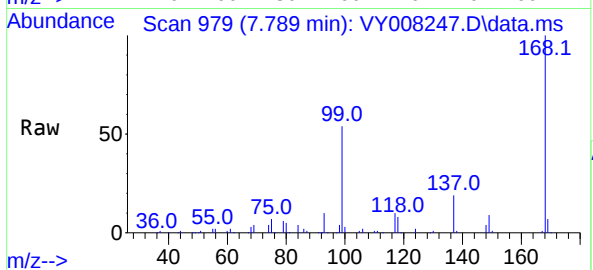



Tgt Ion:168 Resp: 116129
Ion Ratio Lower Upper
168 100
99 53.6 46.9 70.3

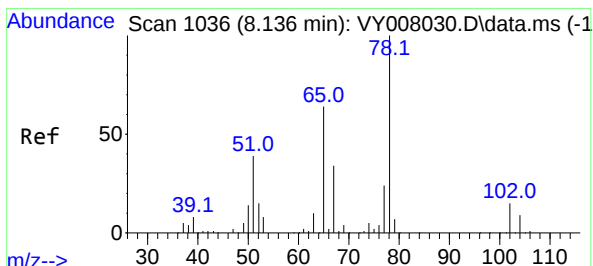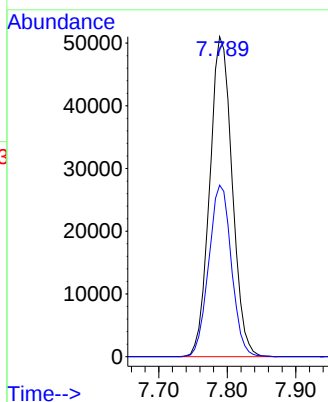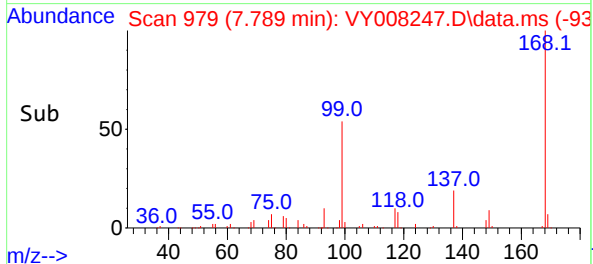

#33
1,2-Dichloroethane-d4
Concen: 55.919 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24

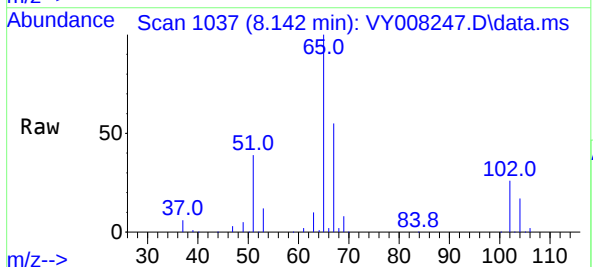

Tgt Ion: 65 Resp: 65152
Ion Ratio Lower Upper
65 100
67 54.5 0.0 99.4

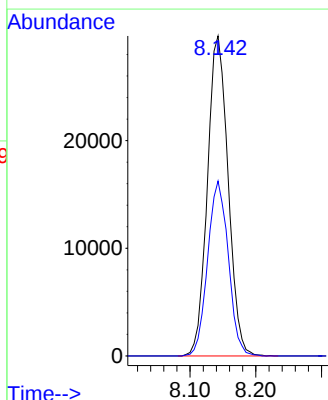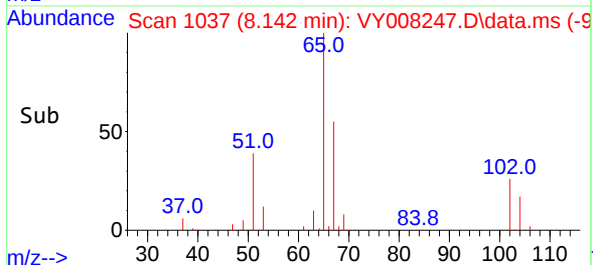



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY008247.D

Acq: 07 Apr 2022 15:24

Instrument :

MSVOA_Y

ClientSampleId :

TP-1




Tgt Ion:114 Resp: 207285

Ion Ratio Lower Upper

114 100

63 17.6 0.0 43.2

88 15.1 0.0 31.8

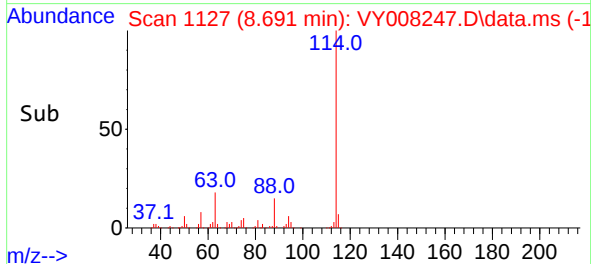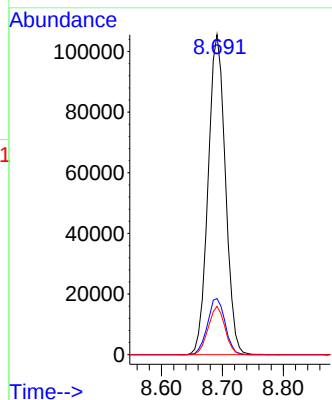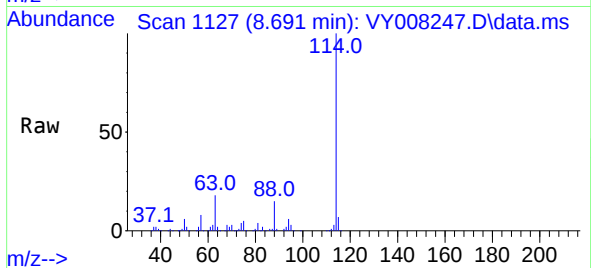

#35

Dibromofluoromethane

Concen: 50.496 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY008247.D

Acq: 07 Apr 2022 15:24




Tgt Ion:113 Resp: 65625


Ion Ratio Lower Upper

113 100

111 102.4 82.6 124.0

192 18.2 17.6 26.4


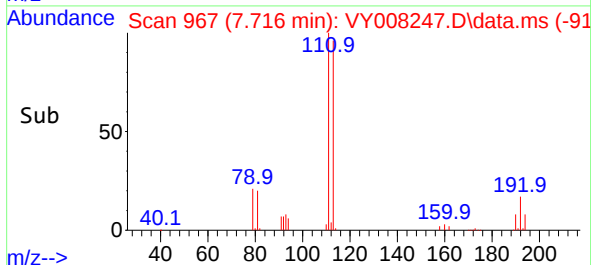
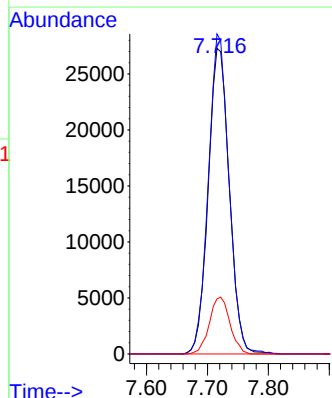
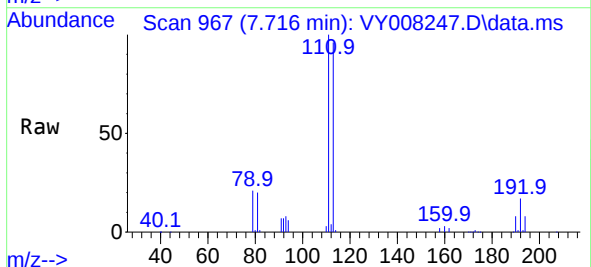


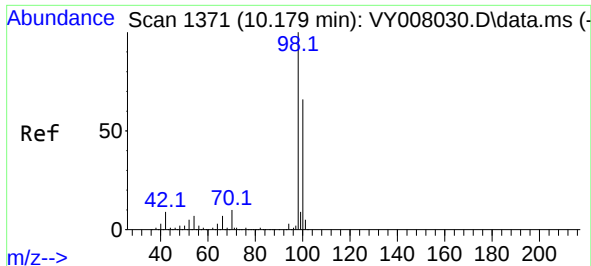

#50
Toluene-d8
Concen: 52.610 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Tgt Ion: 98 Resp: 257597
Ion Ratio Lower Upper
98 100
100 65.6 50.2 75.2

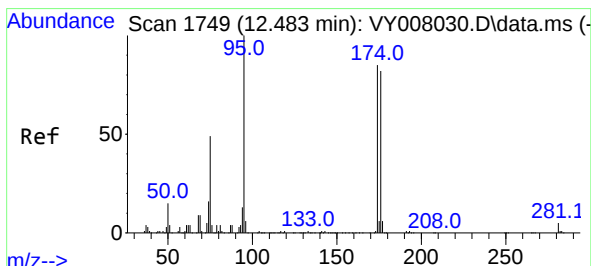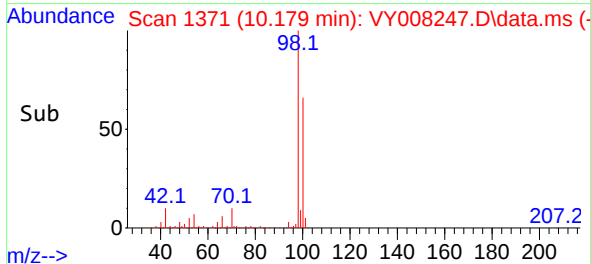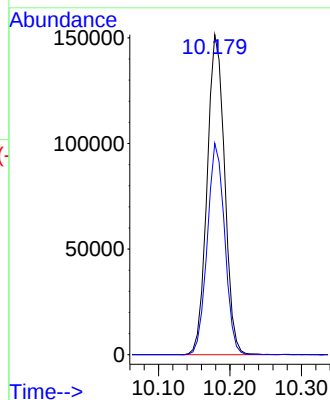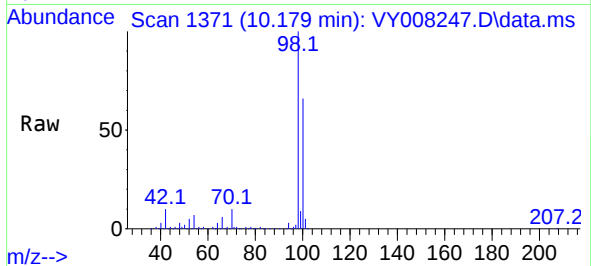

#62
4-Bromofluorobenzene
Concen: 49.044 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24

Tgt Ion: 95 Resp: 84721
Ion Ratio Lower Upper
95 100
174 84.3 0.0 177.0
176 80.6 0.0 175.8


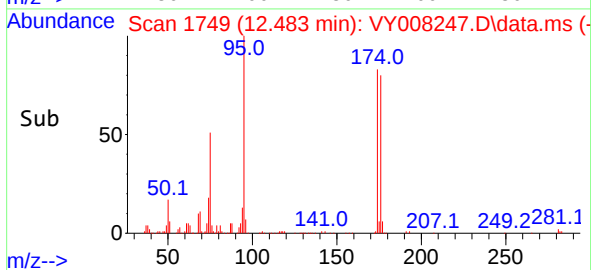
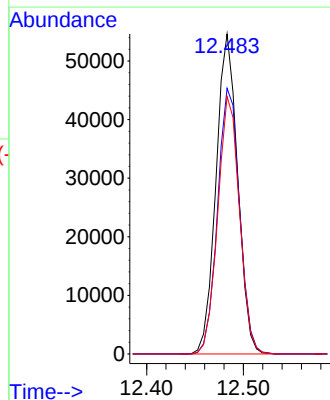
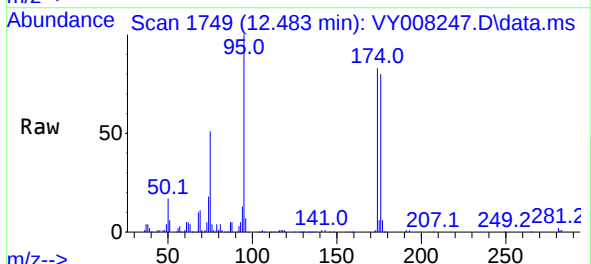




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Tgt Ion:117 Resp: 201275
Ion Ratio Lower Upper
117 100
82 52.6 43.0 64.4
119 32.2 25.4 38.0

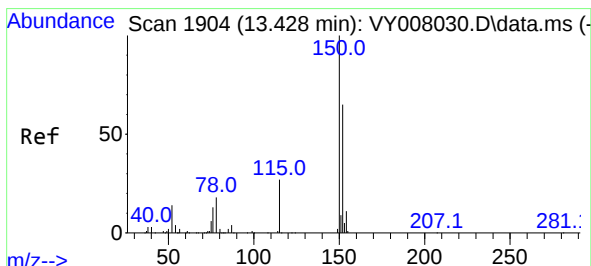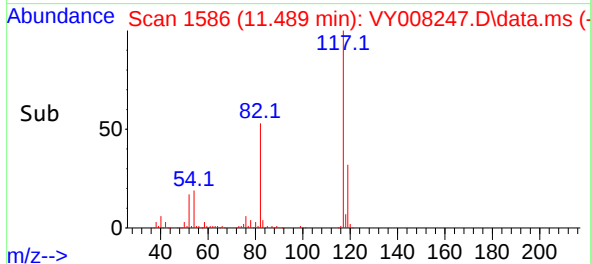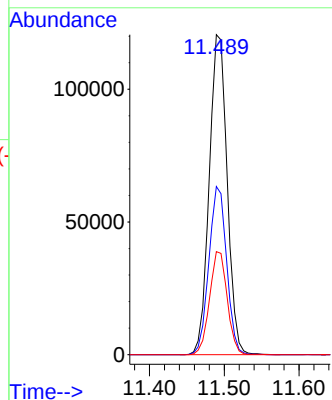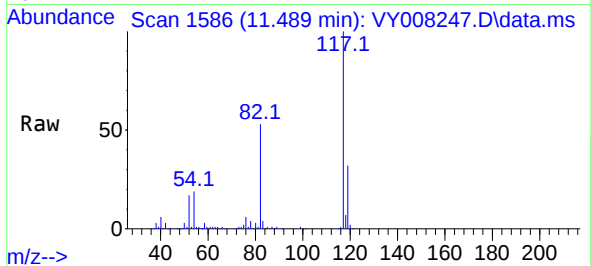

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008247.D
Acq: 07 Apr 2022 15:24

Tgt Ion:152 Resp: 90421
Ion Ratio Lower Upper
152 100
115 57.7 28.2 84.7
150 154.9 0.0 347.6

