

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040725\
 Data File : VY021803.D
 Acq On : 07 Apr 2025 17:06
 Operator : SY/MD
 Sample : Q1738-01
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OK-02-040425

Quant Time: Apr 08 03:35:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 28 02:30:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	76356	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	113098	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	88388	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	29892	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	35541	42.961	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.920%
35) Dibromofluoromethane	7.634	113	32460	44.245	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	88.480%
50) Toluene-d8	10.109	98	132280	47.395	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.780%
62) 4-Bromofluorobenzene	12.408	95	33178	35.144	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	70.280%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY040725\
Data File : VY021803.D
Acq On : 07 Apr 2025 17:06
Operator : SY/MD
Sample : Q1738-01
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OK-02-040425

Quant Time: Apr 08 03:35:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y032725S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 28 02:30:29 2025
Response via : Initial Calibration




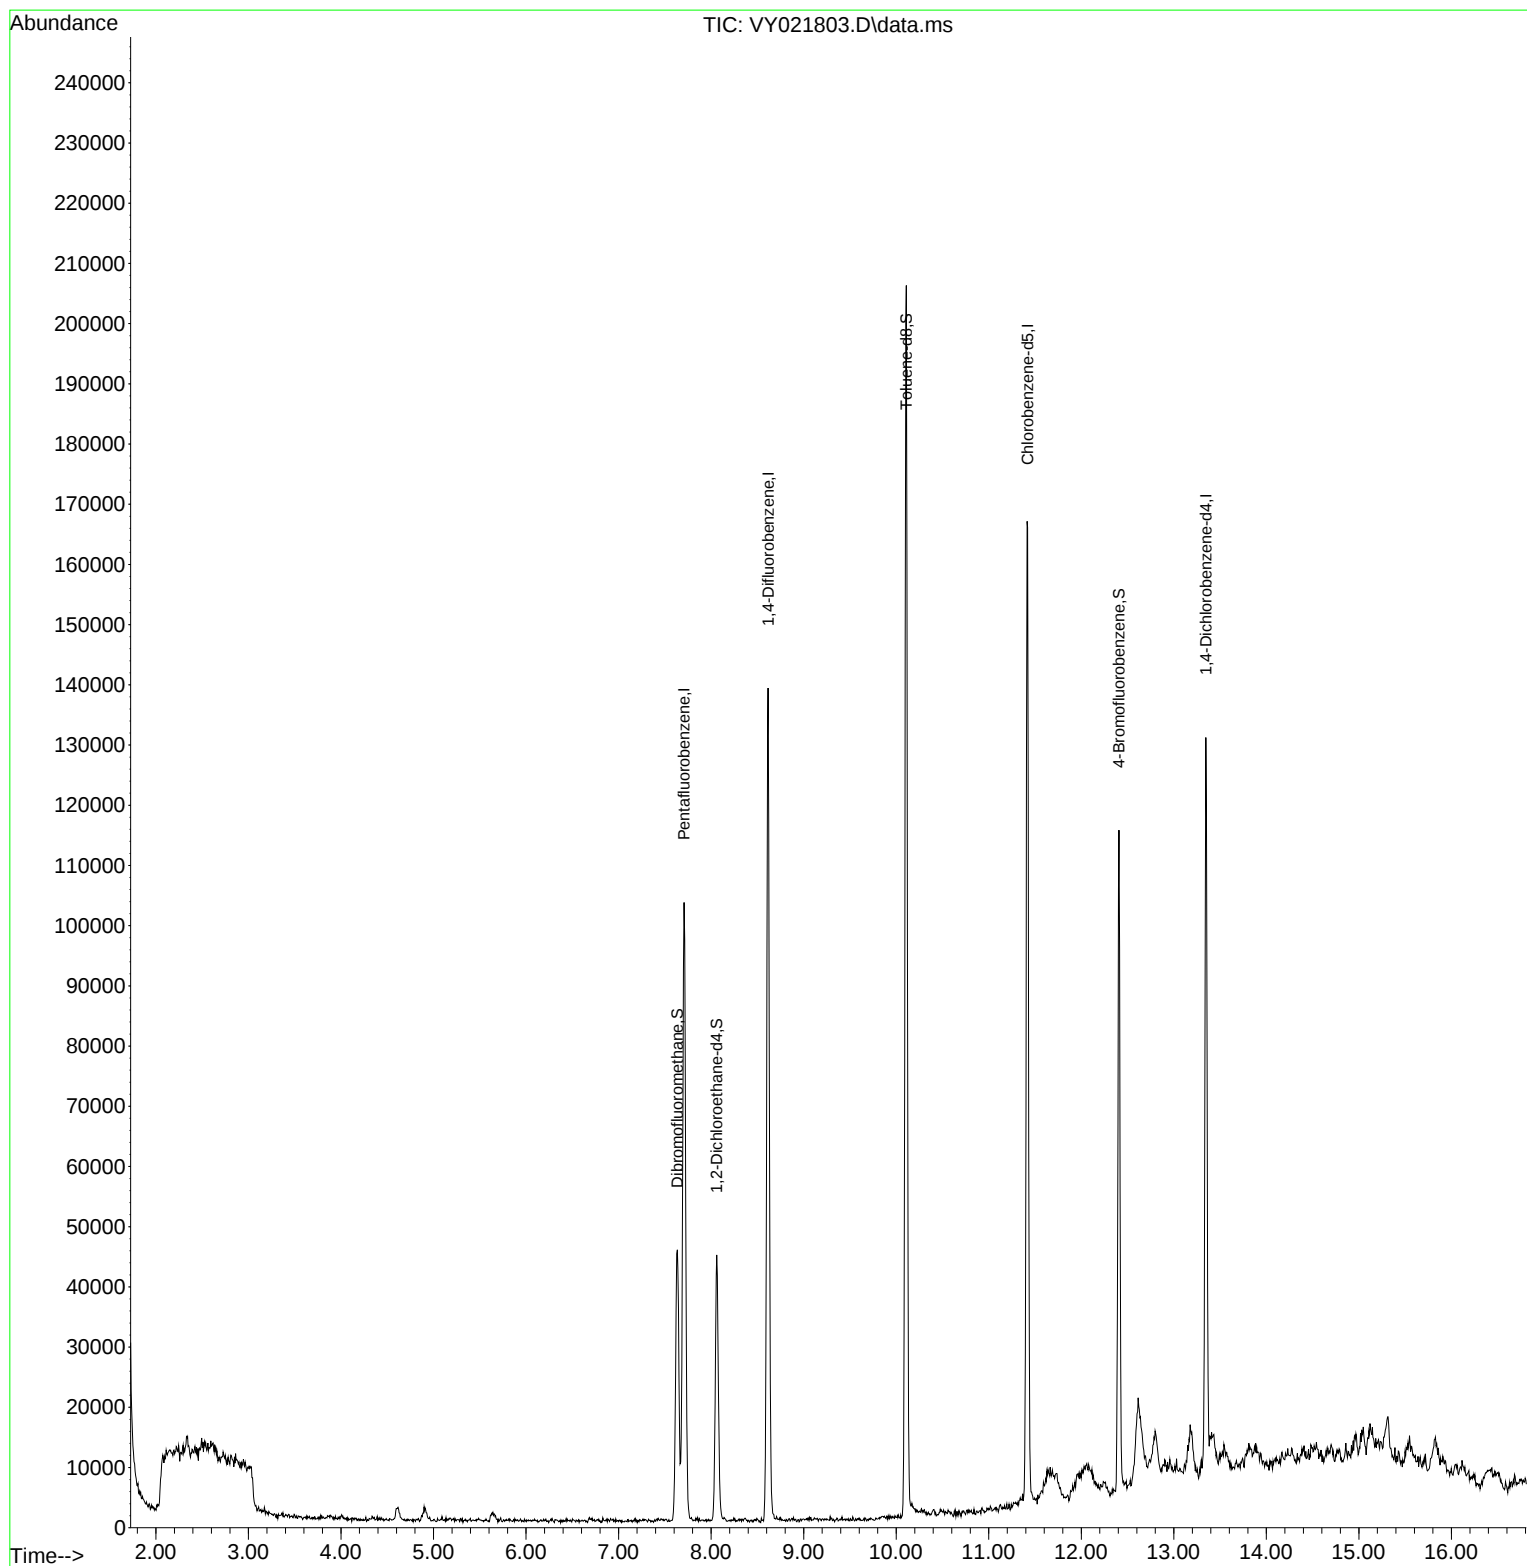


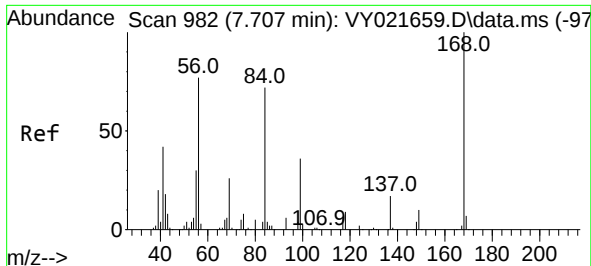

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06




Instrument :
MSVOA_Y
ClientSampleId :
OK-02-040425


Tgt Ion:168 Resp: 76356
Ion Ratio Lower Upper
168 100
99 54.4 46.7 70.1

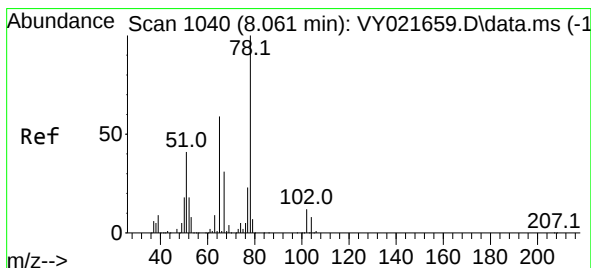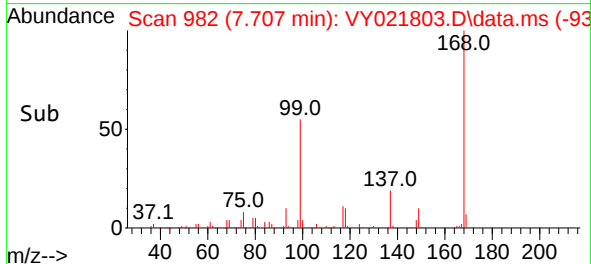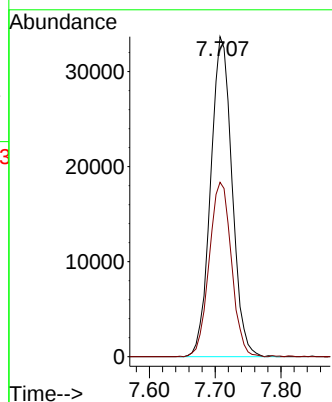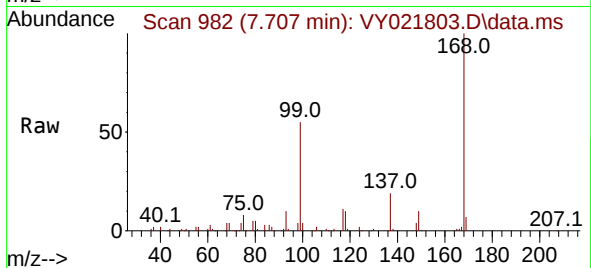

#33
1,2-Dichloroethane-d4
Concen: 42.961 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06

Tgt Ion: 65 Resp: 35541
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.6


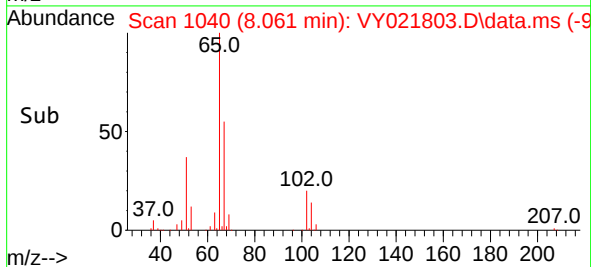
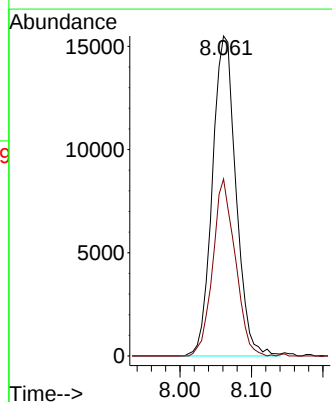
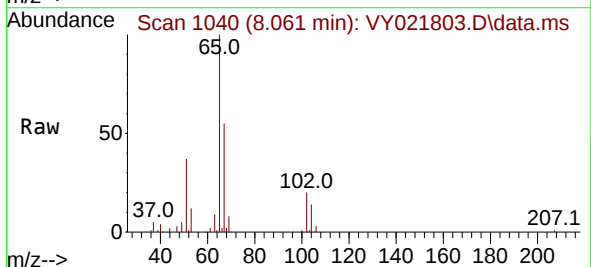


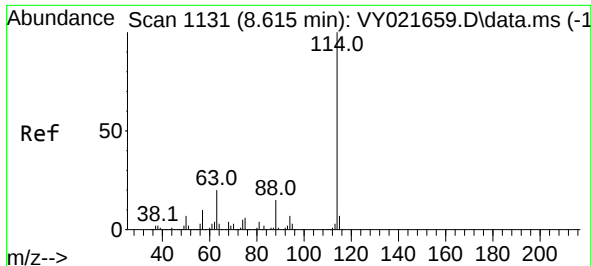

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06




Instrument :
MSVOA_Y
ClientSampleId :
OK-02-040425


Tgt Ion:114 Resp: 113098
Ion Ratio Lower Upper
114 100
63 20.4 0.0 40.2
88 14.1 0.0 29.8

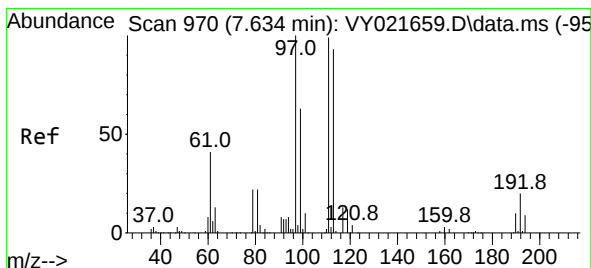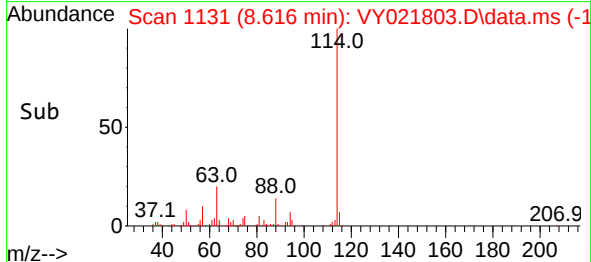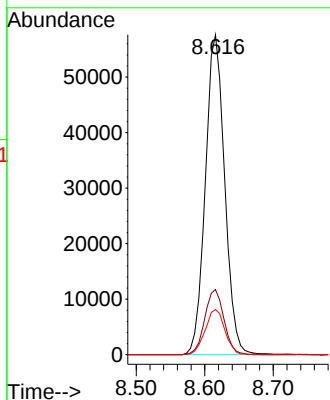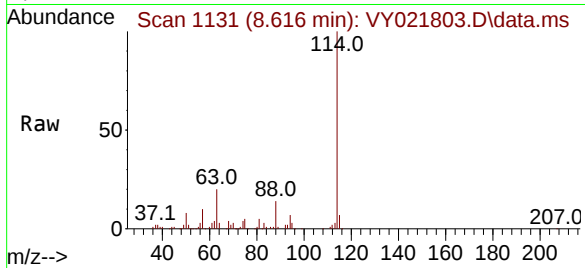

#35
Dibromofluoromethane
Concen: 44.245 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06

Tgt Ion:113 Resp: 32460
Ion Ratio Lower Upper
113 100
111 104.6 82.6 123.8
192 19.9 16.2 24.4


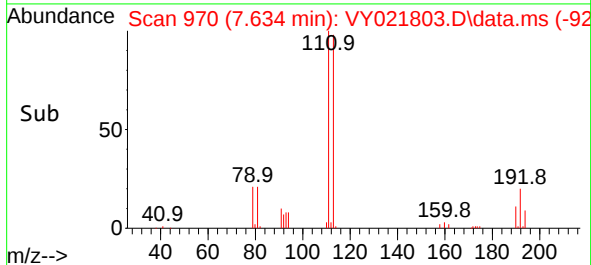
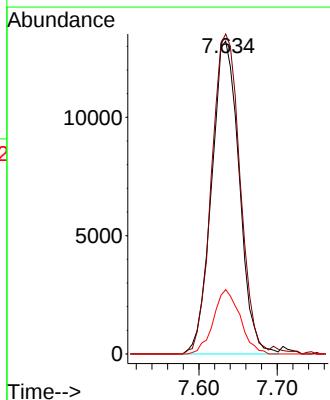
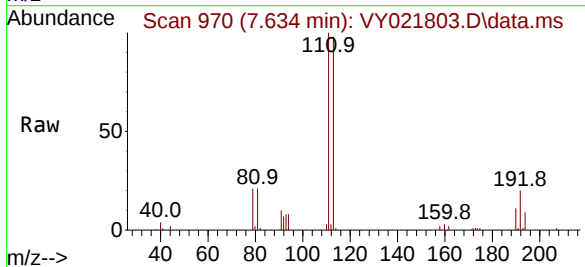


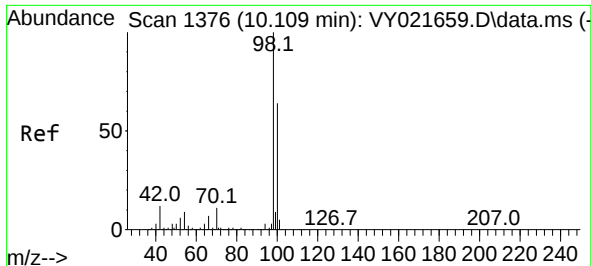

#50
Toluene-d8
Concen: 47.395 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06




Instrument :
MSVOA_Y
ClientSampleId :
OK-02-040425


Tgt Ion: 98 Resp: 132280
Ion Ratio Lower Upper
98 100
100 64.8 52.1 78.1

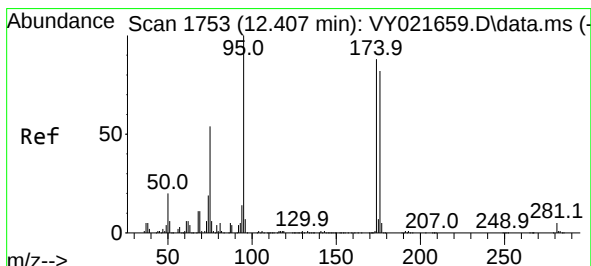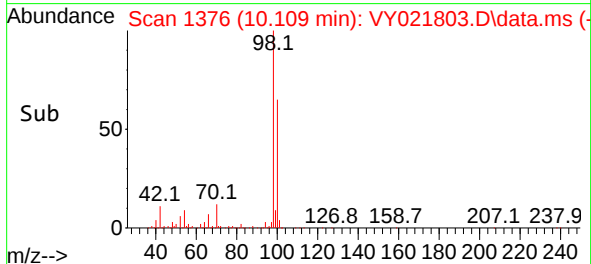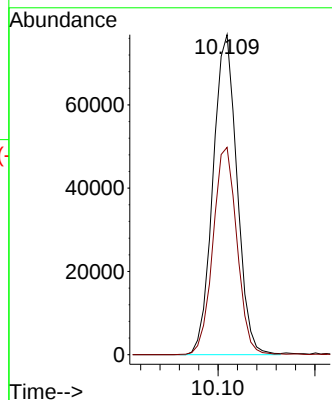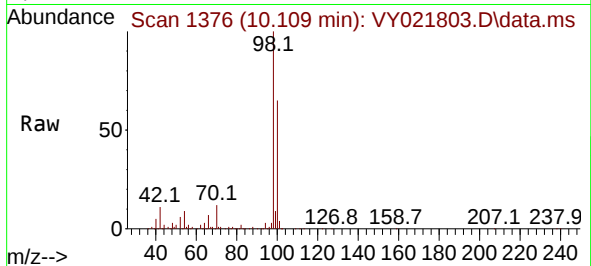

#62
4-Bromofluorobenzene
Concen: 35.144 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06

Tgt Ion: 95 Resp: 33178
Ion Ratio Lower Upper
95 100
174 85.5 0.0 170.8
176 82.5 0.0 162.0


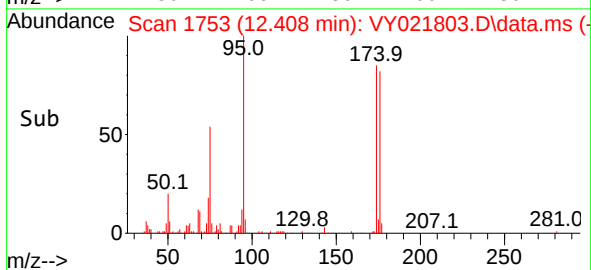
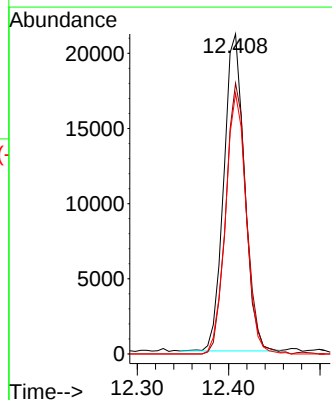
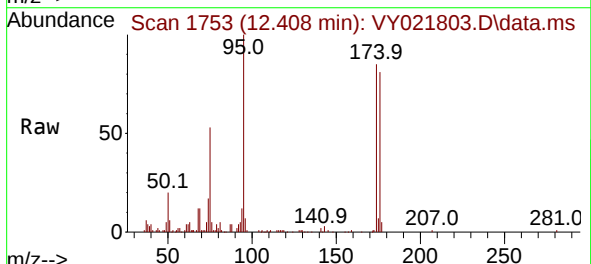


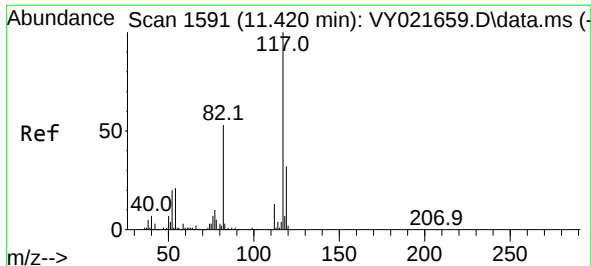

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06

Instrument :
MSVOA_Y
ClientSampleId :
OK-02-040425

Tgt Ion:117 Resp: 88388
Ion Ratio Lower Upper
117 100
82 54.5 42.8 64.2
119 31.6 25.7 38.5

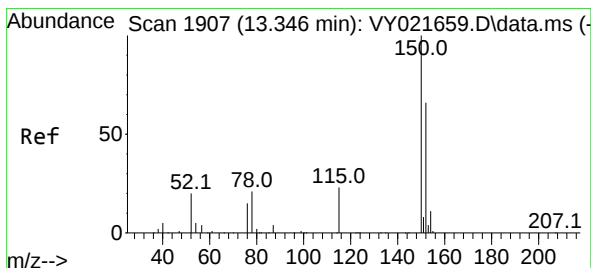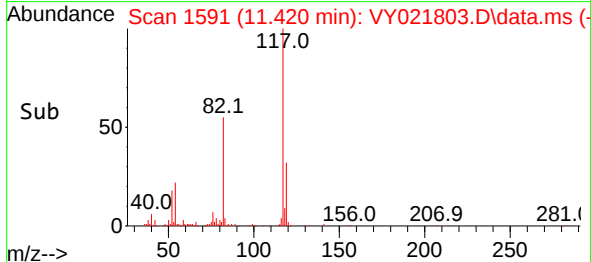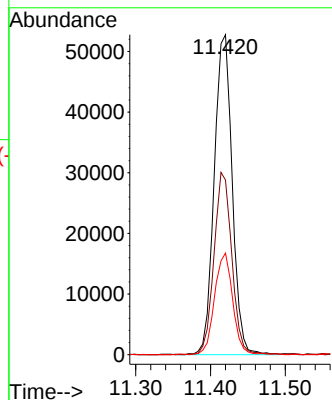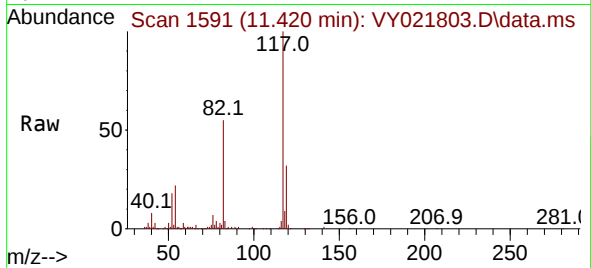

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY021803.D
Acq: 07 Apr 2025 17:06

Tgt Ion:152 Resp: 29892
Ion Ratio Lower Upper
152 100
115 57.4 28.8 86.5
150 160.1 0.0 348.4

