


Chloromethane

Response Ratio

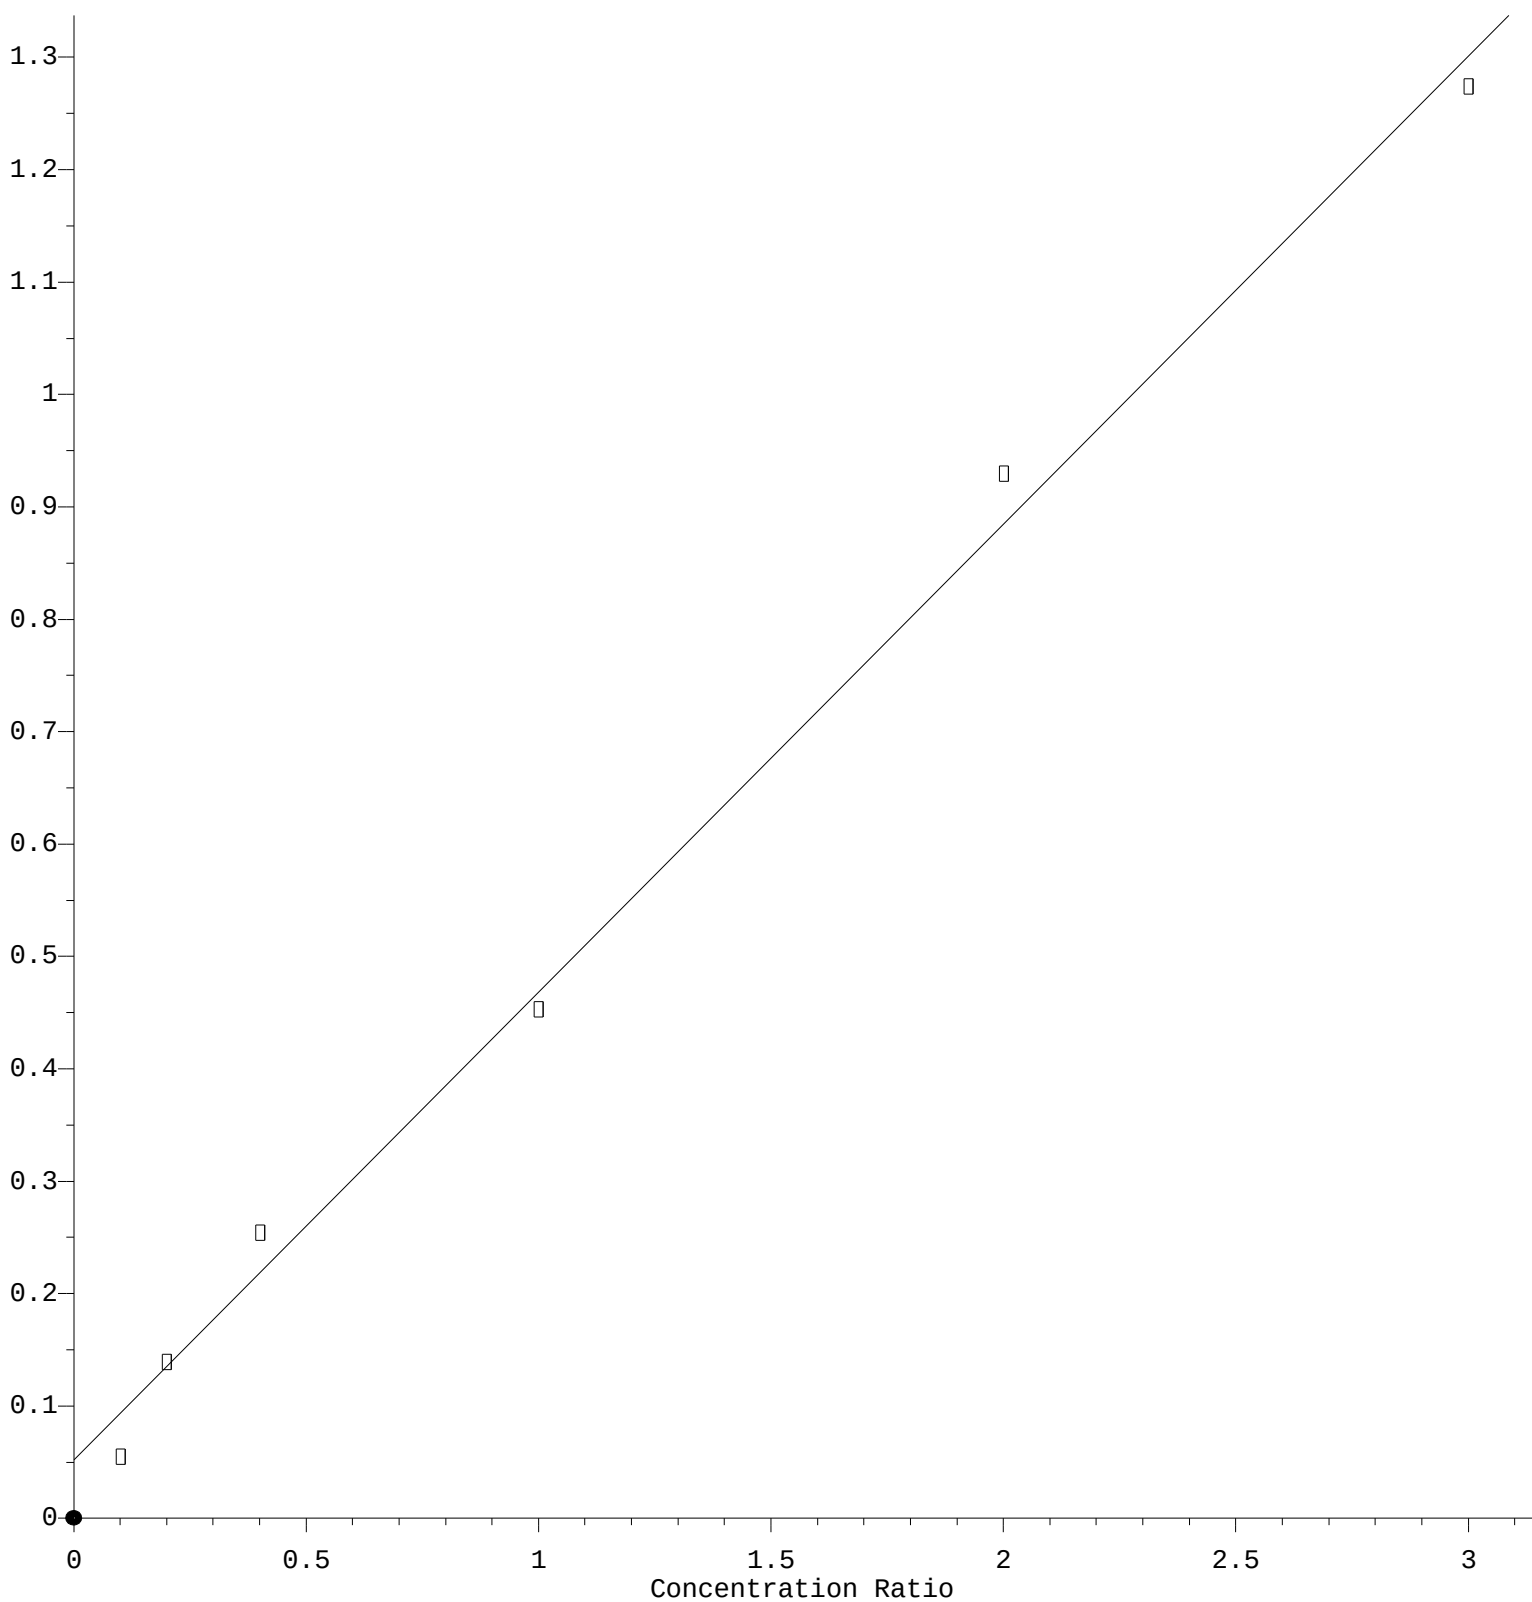

$$\text{Response} = 4.164\text{e-}001 * \text{Amt} + 5.235\text{e-}002$$


Coef of Det (r^2) = 0.995075 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M

Calibration Table Last Updated: Fri Apr 08 16:02:50 2022

Methyl Iodide

Response Ratio

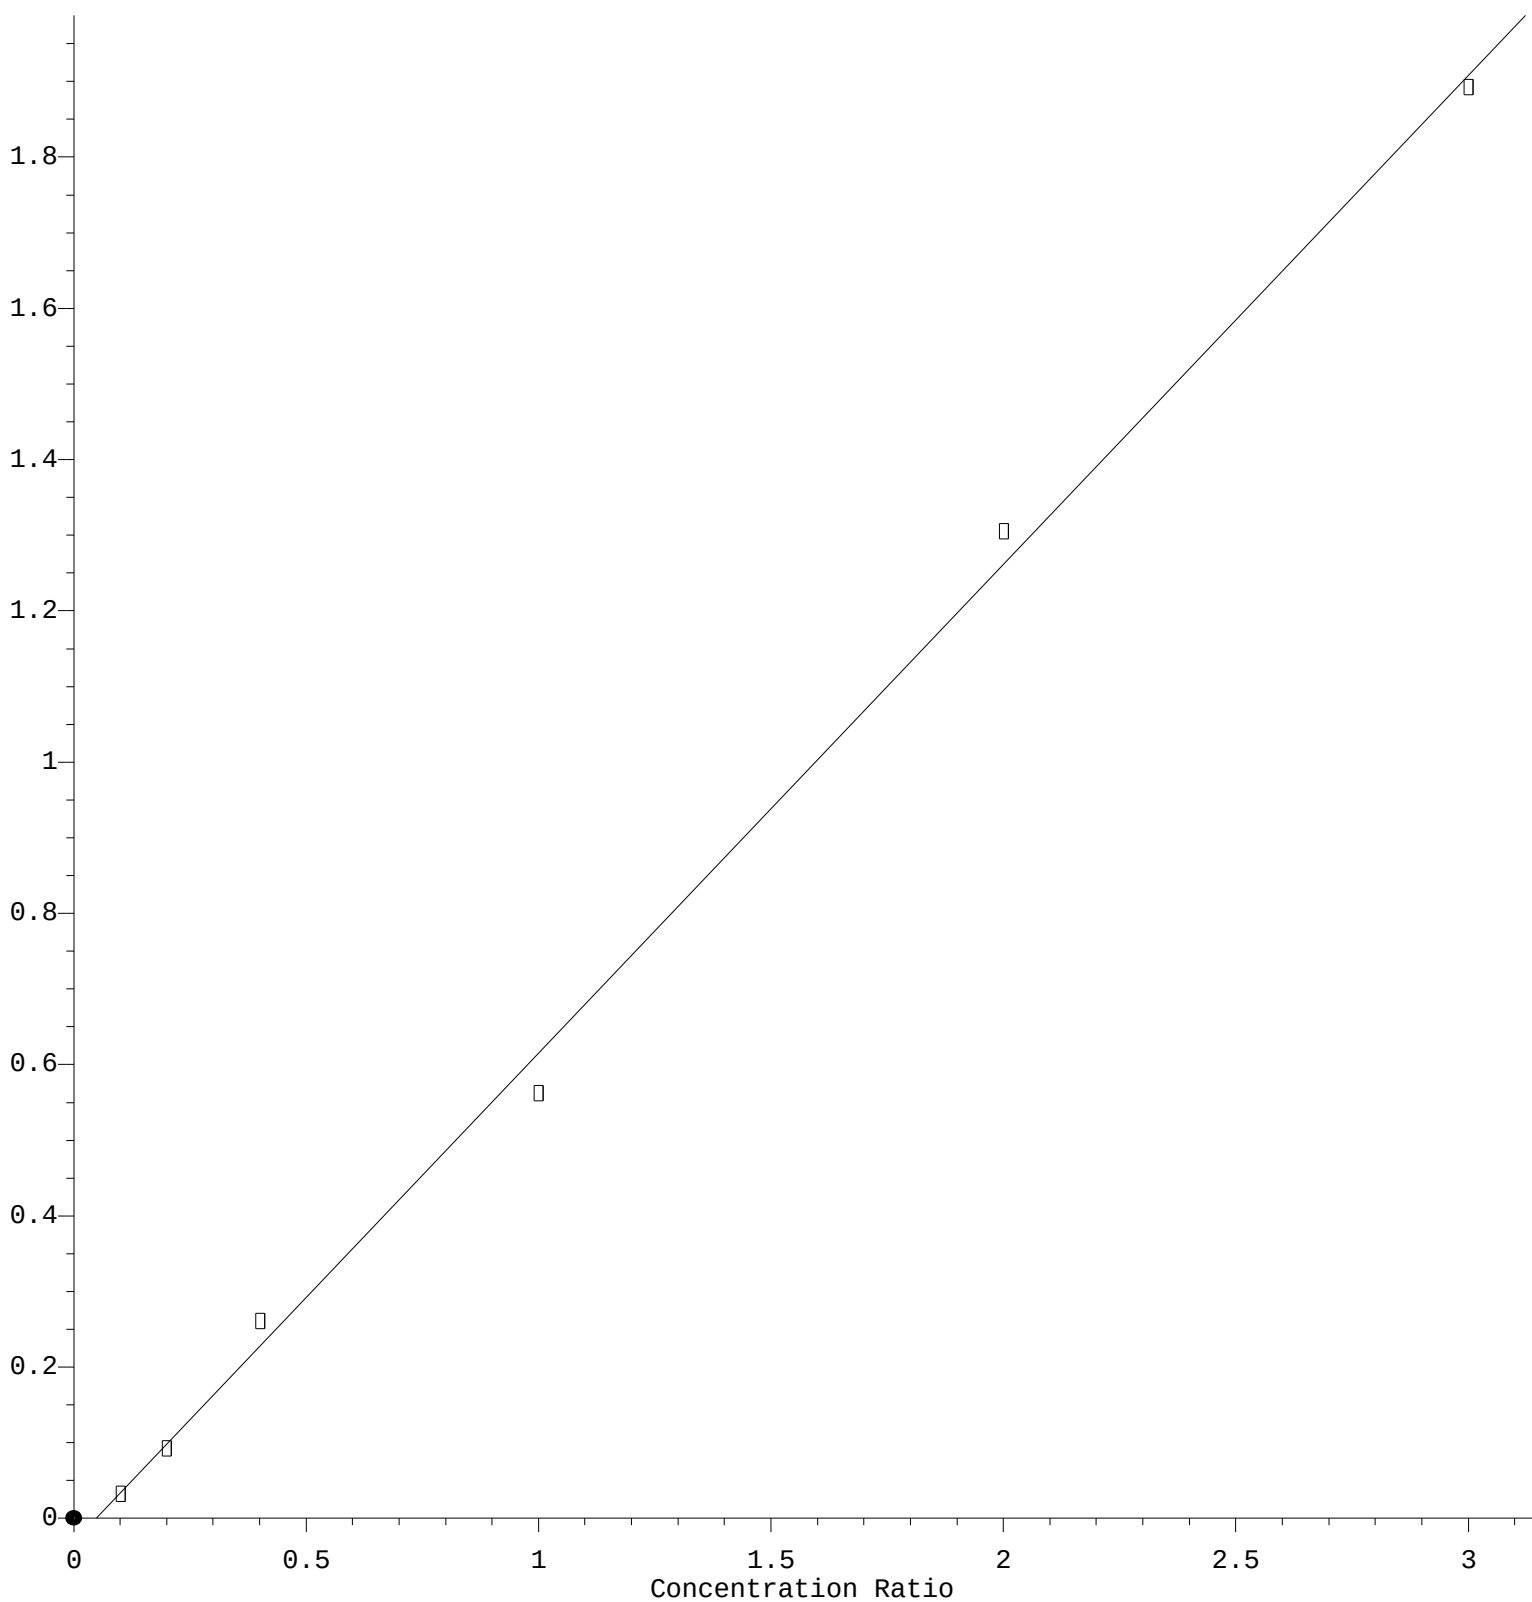

$$\text{Response} = 6.462\text{e-}001 * \text{Amt} - 3.091\text{e-}002$$


Coef of Det (r^2) = 0.997818 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M

Calibration Table Last Updated: Fri Apr 08 16:02:50 2022

Bromomethane

Response Ratio

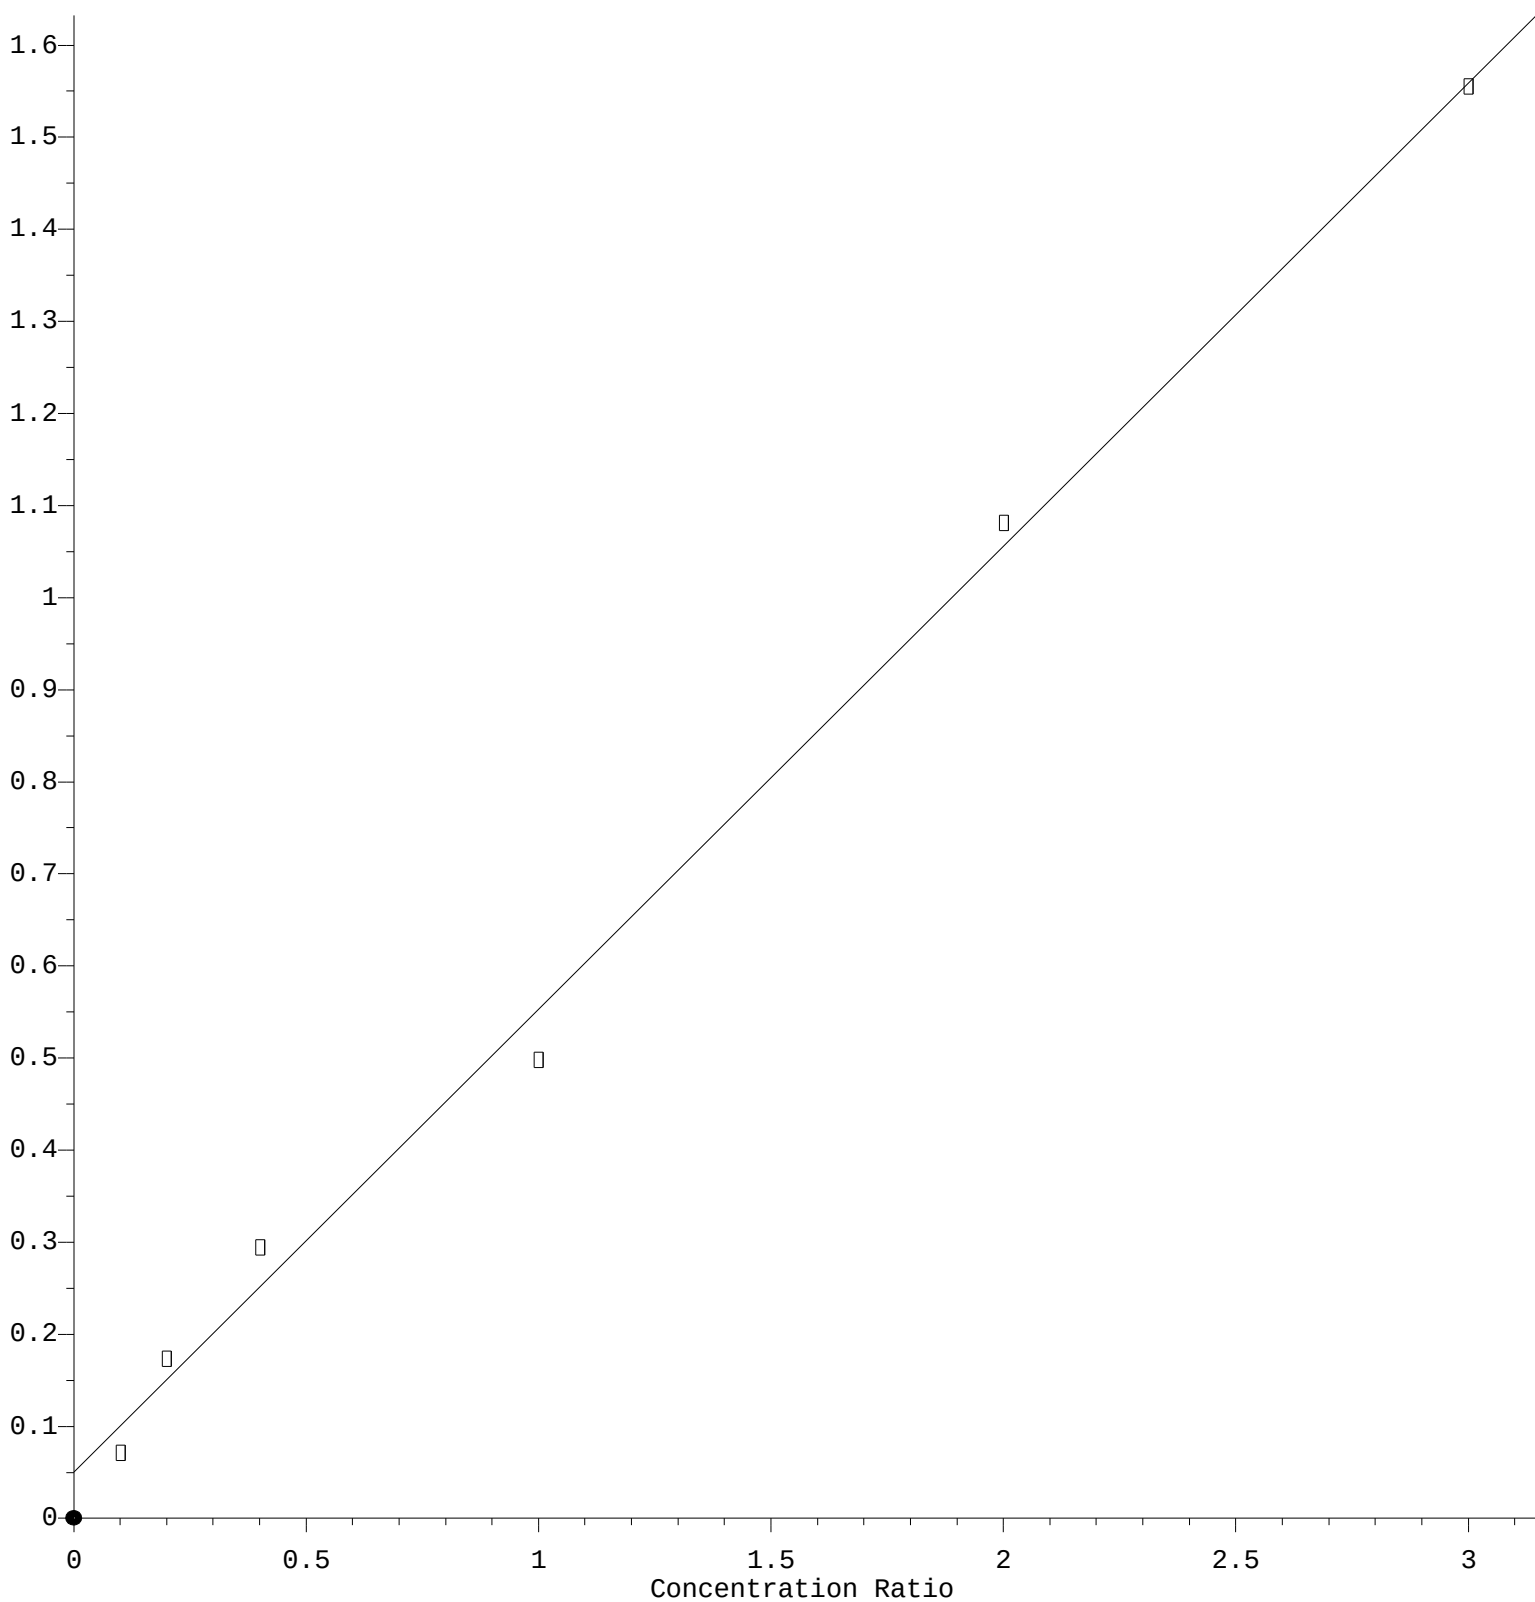


$$\text{Response} = 5.029\text{e-}001 * \text{Amt} + 5.032\text{e-}002$$

Coef of Det (r^2) = 0.995933 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M

Calibration Table Last Updated: Fri Apr 08 16:02:50 2022


Methyl Acetate

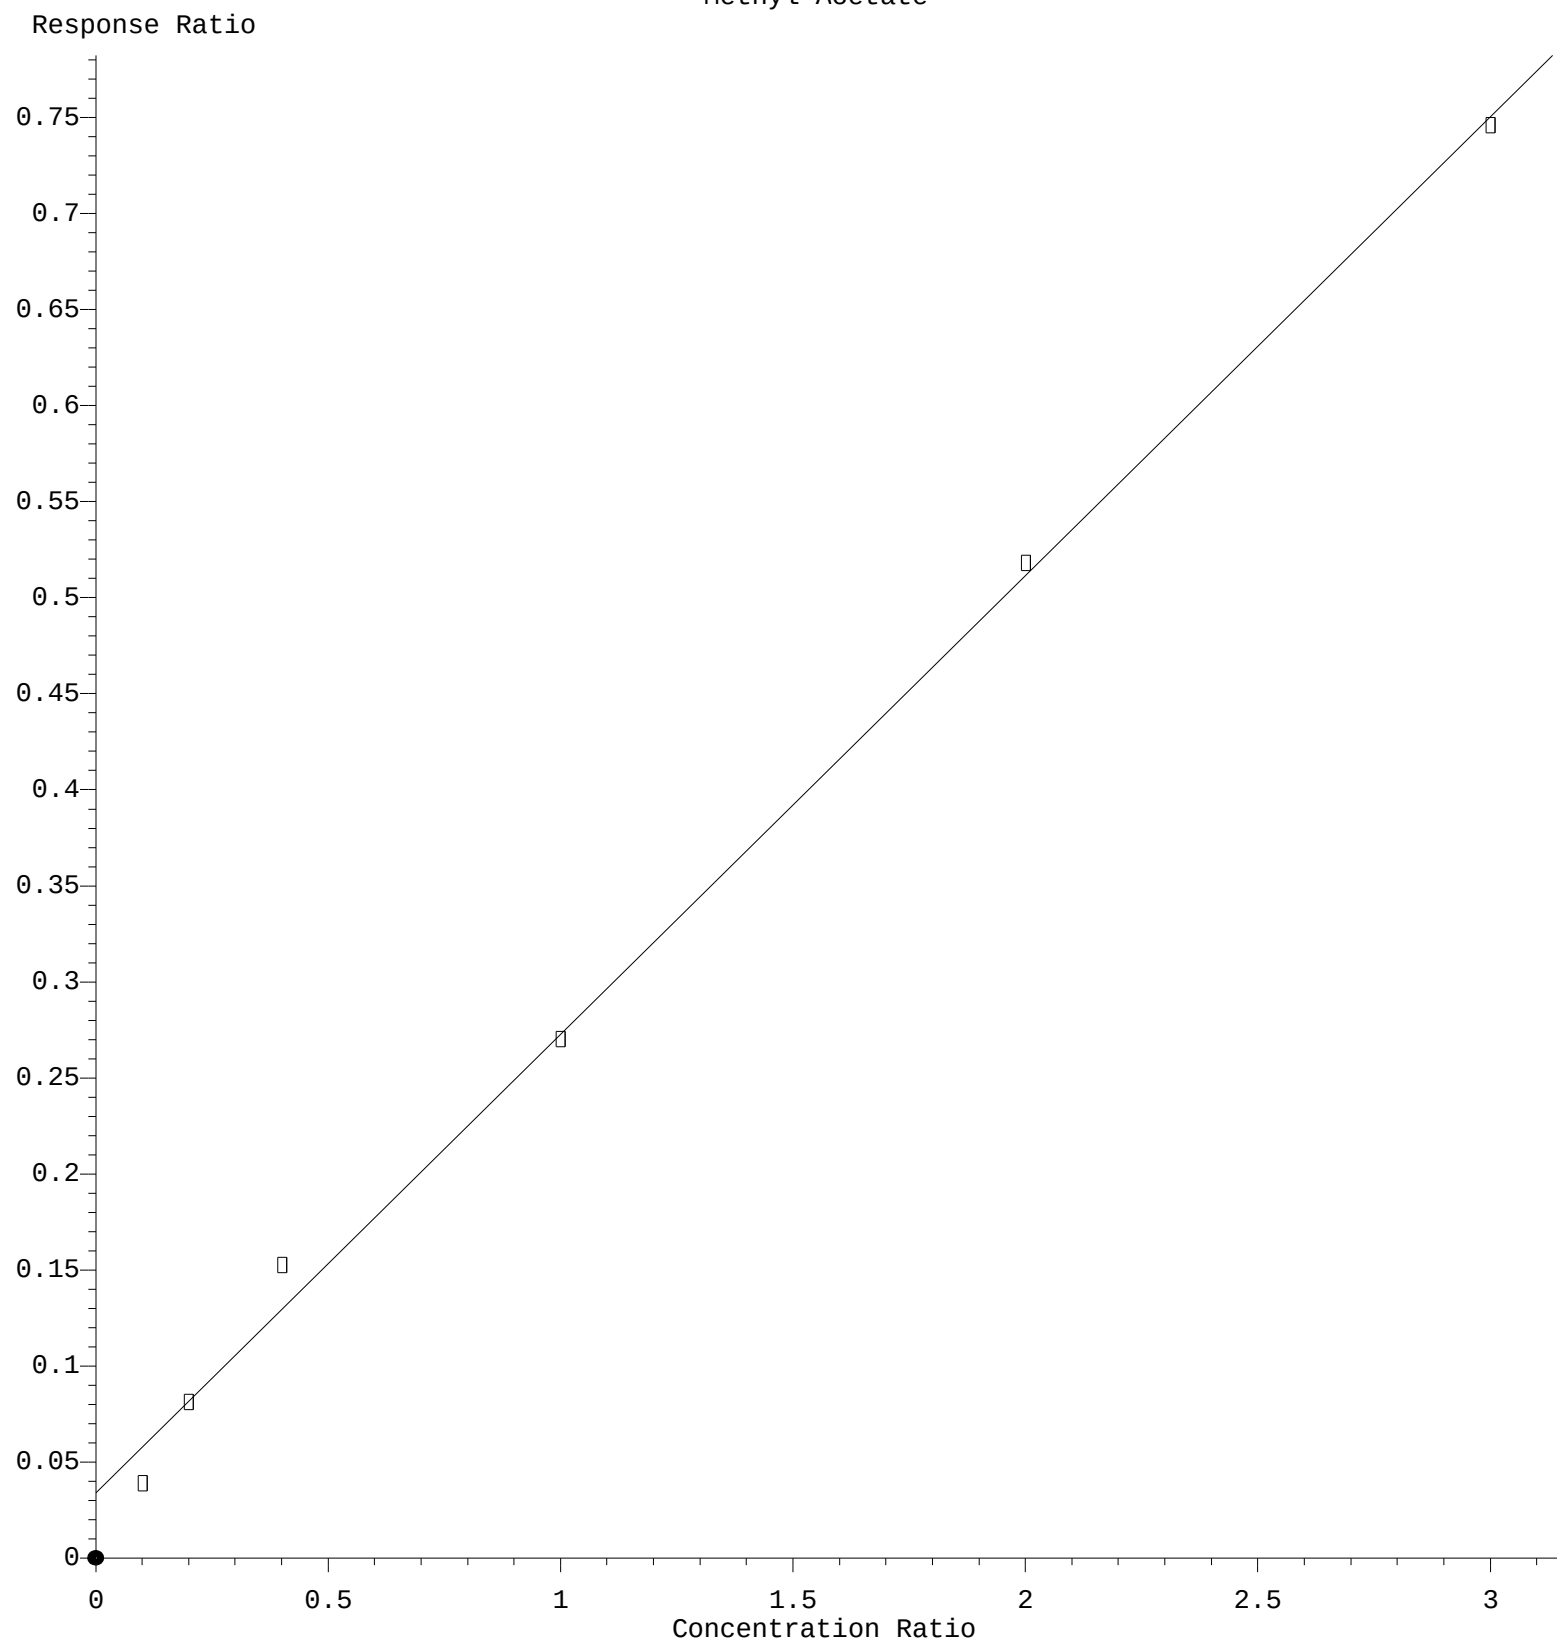

Response = 2.388e-001 * Amt + 3.440e-002
 Coef of Det (r^2) = 0.997502 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Calibration Table Last Updated: Fri Apr 08 16:02:50 2022

Methylene Chloride

Response Ratio

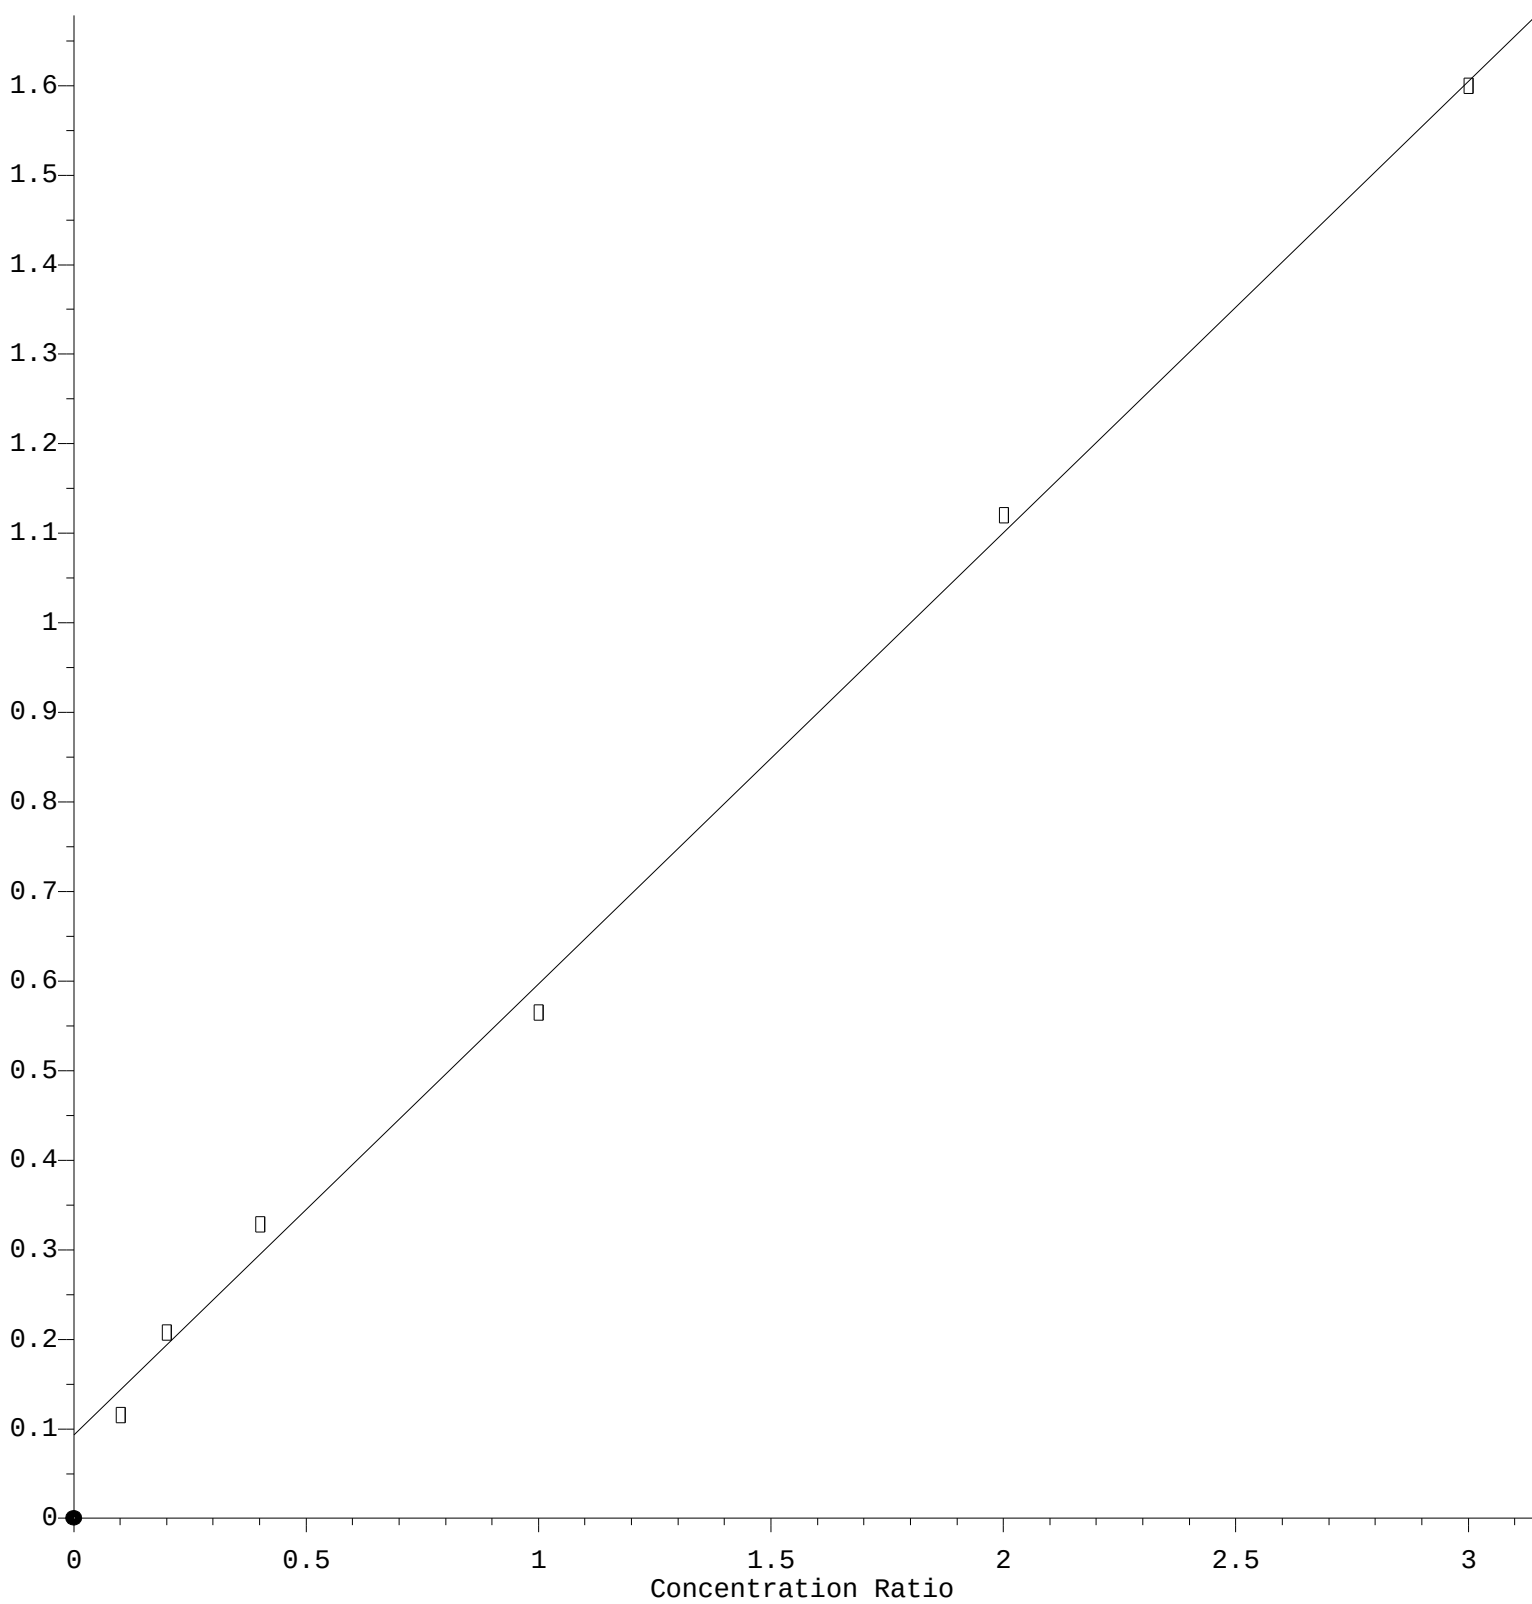

$$\text{Response} = 5.042\text{e-}001 * \text{Amt} + 9.260\text{e-}002$$

Coef of Det (r^2) = 0.997910 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M

Calibration Table Last Updated: Fri Apr 08 16:02:50 2022