

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041122\
 Data File : VY008272.D
 Acq On : 11 Apr 2022 14:56
 Operator : KP/MD
 Sample : N2340-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Apr 12 06:58:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 08 16:02:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	20839	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	31727	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	29787	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	14402	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	8846	45.191	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 90.380%			
35) Dibromofluoromethane	7.716	113	9484	51.755	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 103.500%			
50) Toluene-d8	10.179	98	34961	55.755	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 111.520%			
62) 4-Bromofluorobenzene	12.483	95	13025	55.227	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 110.460%			
Target Compounds						Qvalue
3) Chloromethane	2.113	50	116	Below Cal	#	44
5) Bromomethane	2.668	94	226	Below Cal	#	58
10) Methyl Iodide	4.113	142	145	2.930	ug/l #	35
16) Acetone	3.960	43	410	8.708	ug/l	91
18) Methyl Acetate	4.204	43	44	Below Cal	#	56
20) Methylene Chloride	4.716	84	502	Below Cal	#	52
31) Cyclohexane	7.777	56	678	1.915	ug/l #	30
36) 1,1-Dichloropropene	7.789	75	1258	4.299	ug/l #	44
38) Carbon Tetrachloride	7.789	117	1796	5.705	ug/l #	11
39) Methylcyclohexane	9.179	83	1744	4.632	ug/l #	74
55) 1,1,2-Trichloroethane	10.618	97	654	3.254	ug/l #	15
56) Ethyl methacrylate	10.514	69	255	1.035	ug/l #	1
59) 2-Hexanone	10.795	43	1385	13.920	ug/l #	28
73) Isopropylbenzene	12.331	105	7978	7.451	ug/l	96
74) N-amyl acetate	12.124	43	1737	7.472	ug/l #	77
76) 1,2,3-Trichloropropane	12.483	75	6398	40.168	ug/l #	100
77) Bromobenzene	12.410	156	7459	28.427	ug/l #	1
78) n-propylbenzene	12.672	91	16220	12.837	ug/l	95
79) 2-Chlorotoluene	12.672	91	16220	22.874	ug/l #	43
80) 1,3,5-Trimethylbenzene	12.977	105	1519	1.730	ug/l	71
81) trans-1,4-Dichloro-2-b...	12.483	75	6398	89.874	ug/l #	8
82) 4-Chlorotoluene	12.672	91	16212	22.248	ug/l #	43
84) 1,2,4-Trimethylbenzene	13.123	105	2439	2.807	ug/l	97
85) sec-Butylbenzene	13.258	105	12609	10.798	ug/l	83
89) n-Butylbenzene	13.703	91	13453	15.280	ug/l #	83
90) Hexachloroethane	13.977	117	3755	20.617	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.379	75	91	2.807	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.007	180	574	2.099	ug/l #	1
95) Naphthalene	15.239	128	2882	4.920	ug/l #	28
96) 1,2,3-Trichlorobenzene	15.440	180	636	2.658	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041122\
Data File : VY008272.D
Acq On : 11 Apr 2022 14:56
Operator : KP/MD
Sample : N2340-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Apr 12 06:58:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
Quant Title : SW846 8260
QLast Update : Fri Apr 08 16:02:50 2022
Response via : Initial Calibration




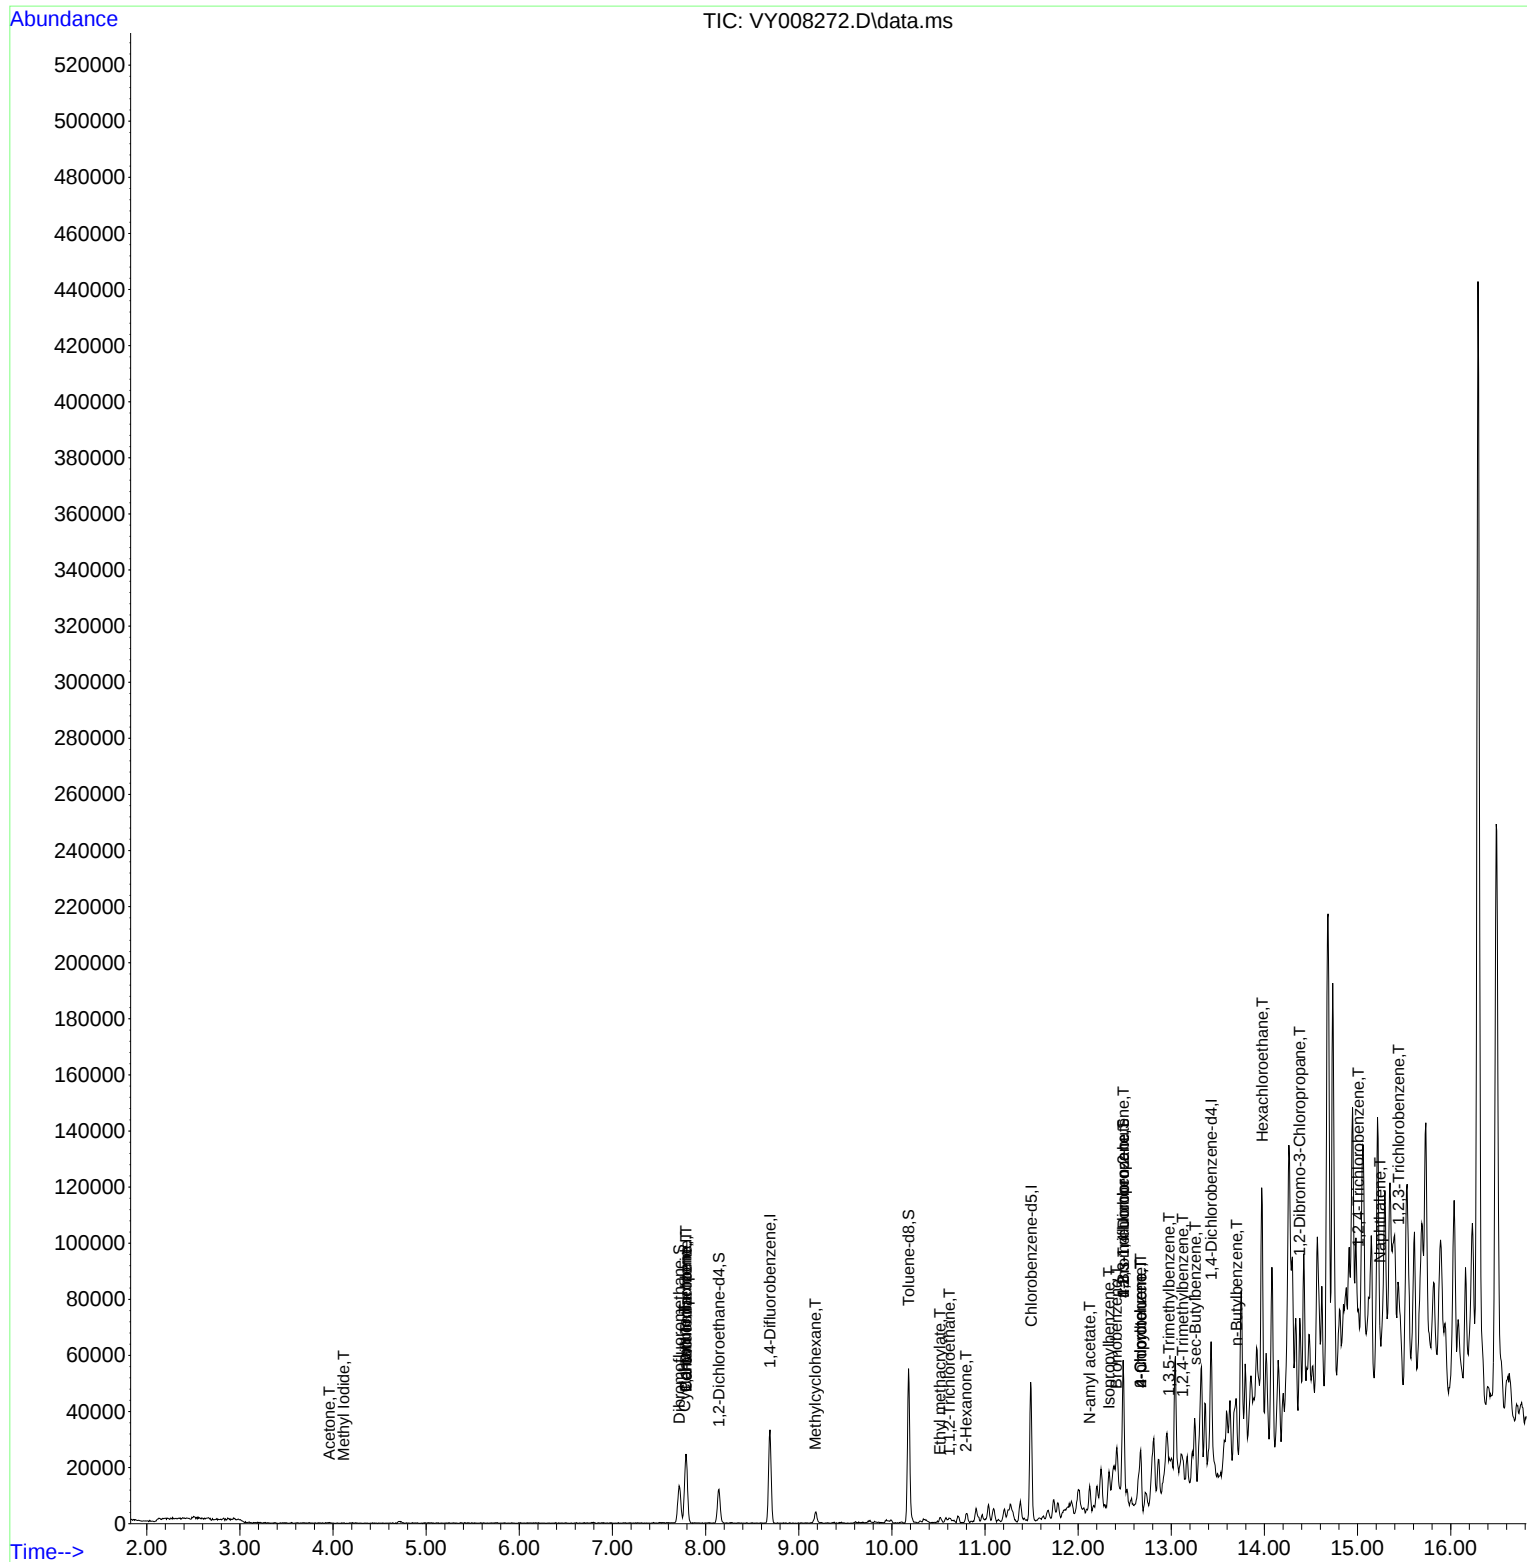




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 20839
Ion Ratio Lower Upper
168 100
99 49.8 46.9 70.3

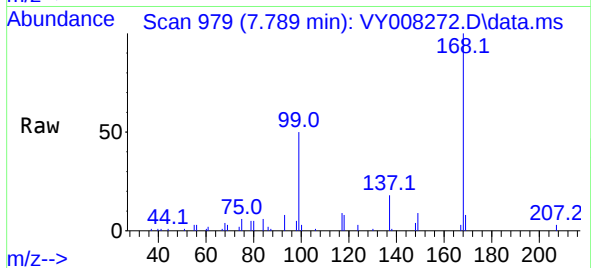

#3
Chloromethane
Concen: Below Cal
RT: 2.113 min Scan# 48
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 50 Resp: 116
Ion Ratio Lower Upper
50 100
52 0.0 24.6 37.0#


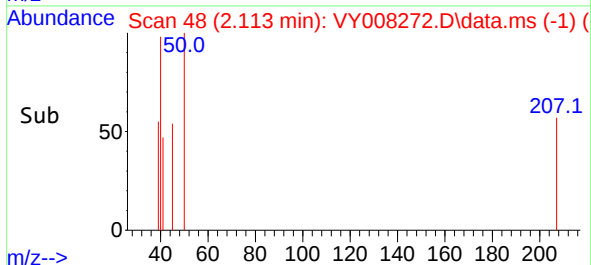

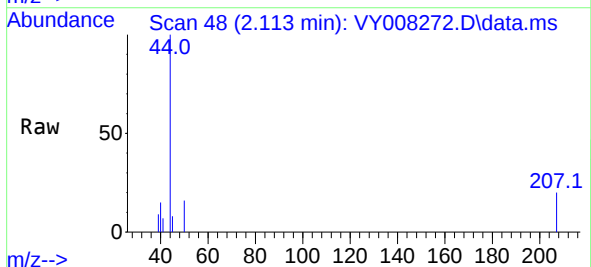




#5
Bromomethane
Concen: Below Cal
RT: 2.668 min Scan# 11
Delta R.T. 0.019 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 94 Resp: 226
Ion Ratio Lower Upper
94 100
96 51.6 73.5 110.3#



#10
Methyl Iodide
Concen: 2.930 ug/l
RT: 4.113 min Scan# 376
Delta R.T. 0.025 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion:142 Resp: 145
Ion Ratio Lower Upper
142 100
127 0.0 41.5 62.3#
141 0.0 11.9 17.9#

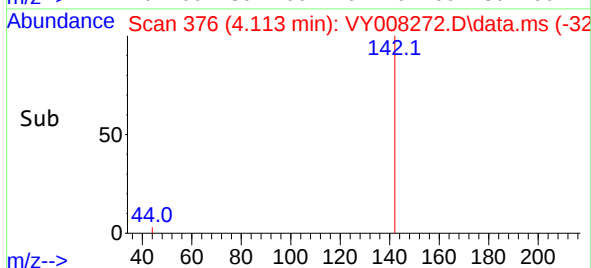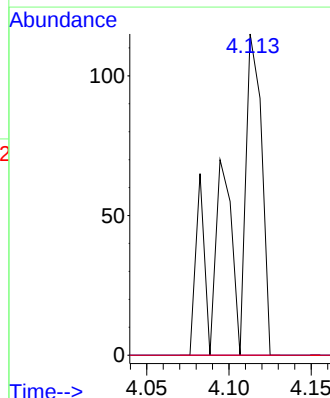



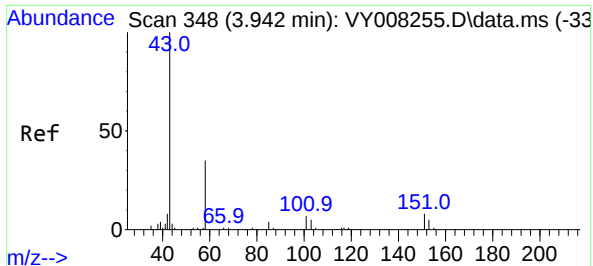


#16
Acetone
Concen: 8.708 ug/l
RT: 3.960 min Scan# 31
Delta R.T. 0.018 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :



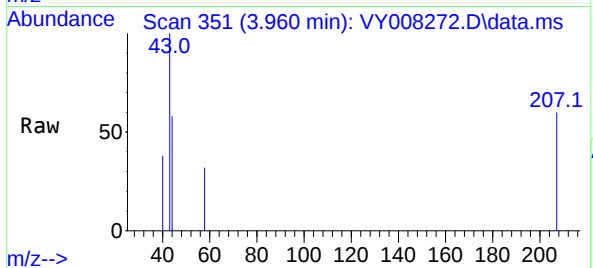



Tgt Ion: 43 Resp: 410
Ion Ratio Lower Upper
43 100
58 32.3 22.0 33.0

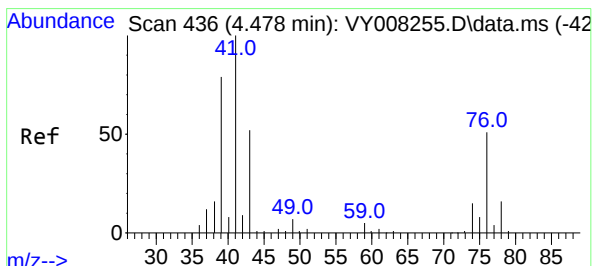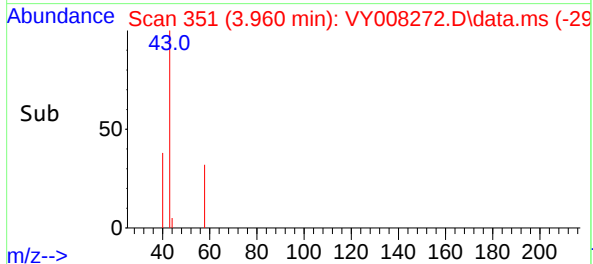

#18
Methyl Acetate
Concen: Below Cal
RT: 4.204 min Scan# 391
Delta R.T. -0.274 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion: 43 Resp: 44
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

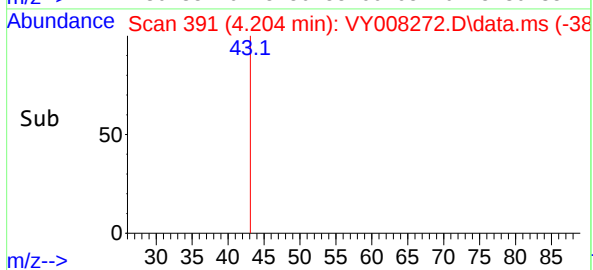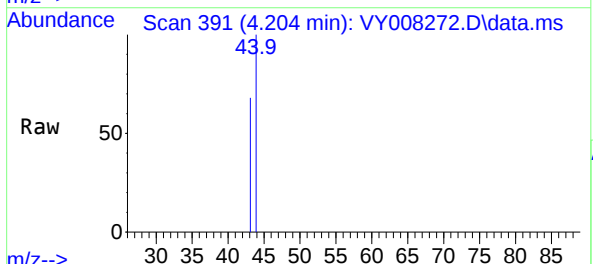

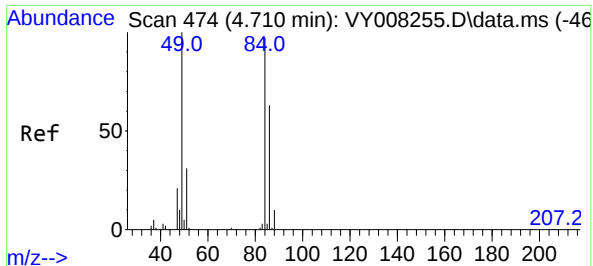




#20
Methylene Chloride
Concen: Below Cal
RT: 4.716 min Scan# 41
Delta R.T. 0.006 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :

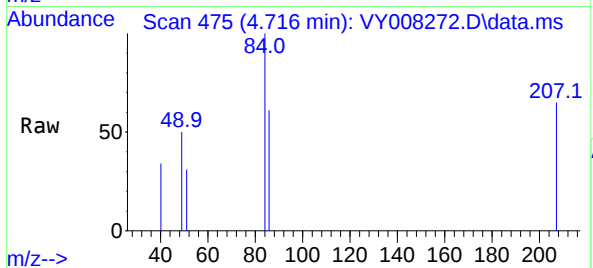

Tgt Ion: 84 Resp: 502




Ion	Ratio	Lower	Upper
84	100		
49	49.8	114.4	171.6#
51	31.3	35.3	52.9#
86	61.3	53.7	80.5

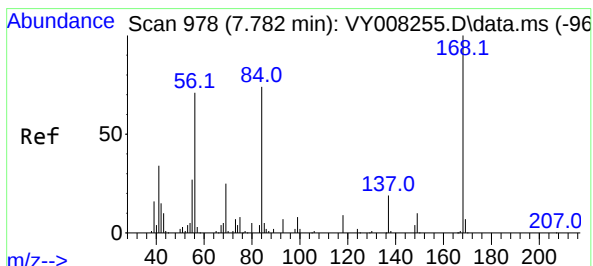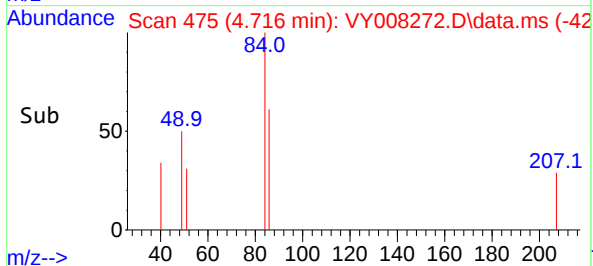


#31
Cyclohexane
Concen: 1.915 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.005 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 56 Resp: 678

Ion	Ratio	Lower	Upper
56	100		
69	64.5	26.7	40.1#
84	153.3	67.2	100.8#

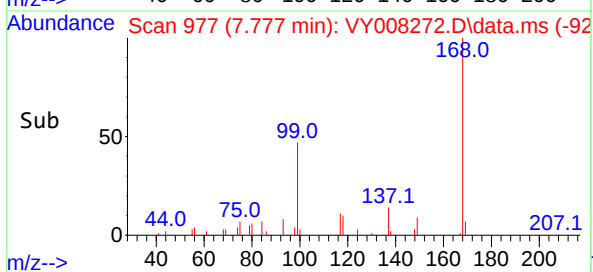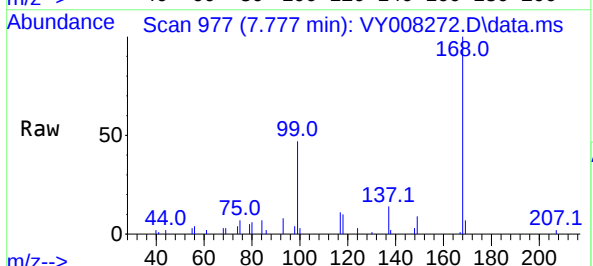

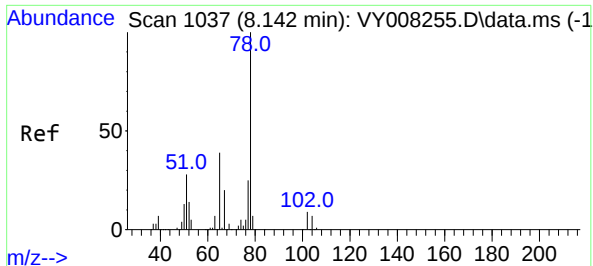

#33

1,2-Dichloroethane-d4

Concen: 45.191 ug/l

RT: 8.143 min Scan# 1037

Delta R.T. 0.001 min

Lab File: VY008272.D

Acq: 11 Apr 2022 14:56

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 65 Resp: 8846

Ion Ratio Lower Upper

65 100

67 54.6 0.0 99.4

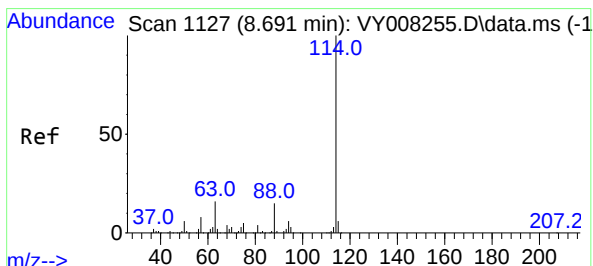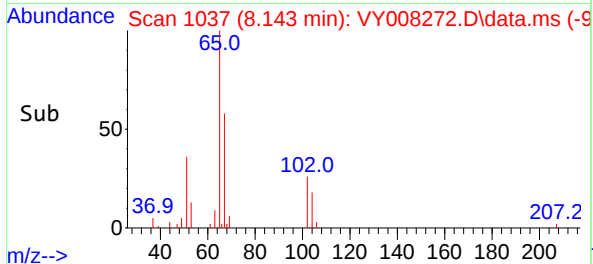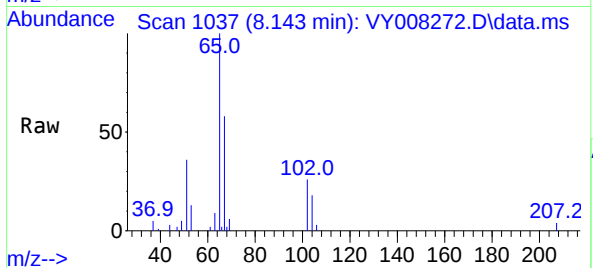

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY008272.D

Acq: 11 Apr 2022 14:56




Tgt Ion: 114 Resp: 31727


Ion Ratio Lower Upper

114 100

63 14.7 0.0 43.2


88 13.9 0.0 31.8

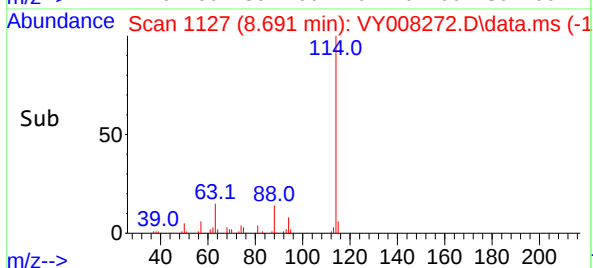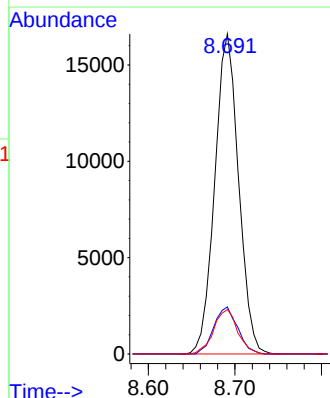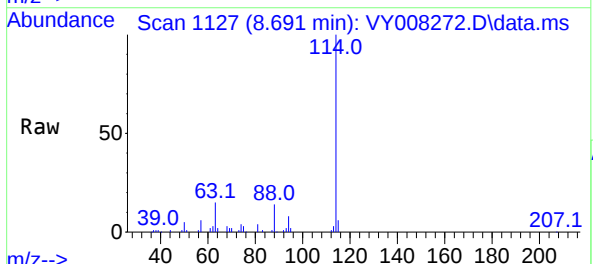






#35
Dibromofluoromethane
Concen: 51.755 ug/l
RT: 7.716 min Scan# 910
Delta R.T. 0.001 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :



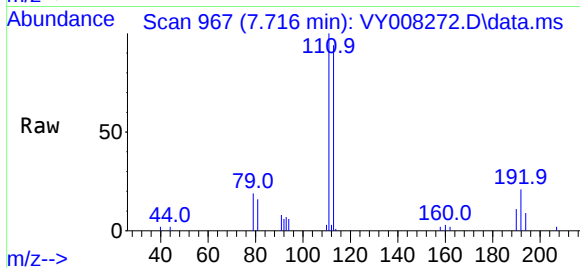



Tgt Ion:113 Resp: 9484
Ion Ratio Lower Upper
113 100
111 102.6 82.6 124.0
192 22.7 17.6 26.4

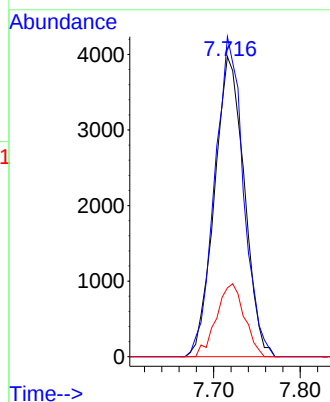

#36
1,1-Dichloropropene
Concen: 4.299 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.128 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion: 75 Resp: 1258
Ion Ratio Lower Upper
75 100
110 1.4 17.1 51.2#
77 0.0 24.4 36.6#

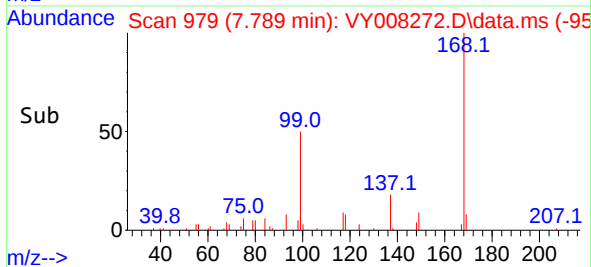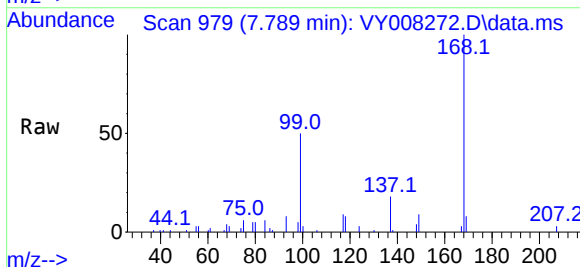






#38
Carbon Tetrachloride
Concen: 5.705 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.109 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :



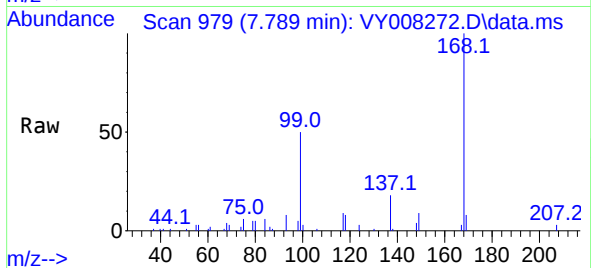



Tgt Ion:117 Resp: 1796
Ion Ratio Lower Upper
117 100
119 0.0 77.9 116.9#
121 0.0 24.8 37.2#

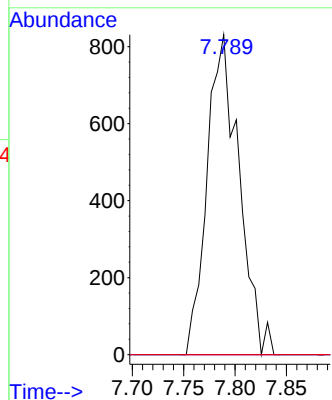

#39
Methylcyclohexane
Concen: 4.632 ug/l
RT: 9.179 min Scan# 1207
Delta R.T. -0.006 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 83 Resp: 1744
Ion Ratio Lower Upper
83 100
55 63.3 66.5 99.7#
98 68.6 37.9 56.9#


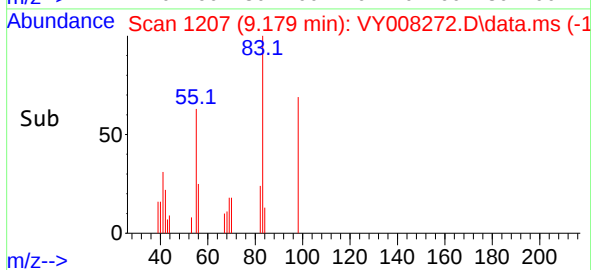
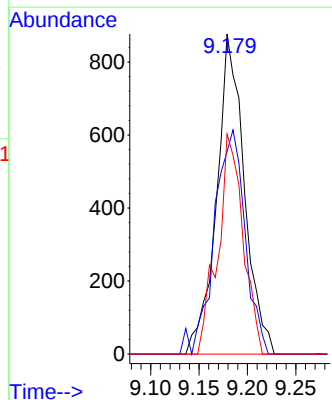





#50
Toluene-d8
Concen: 55.755 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 34961
Ion Ratio Lower Upper
98 100
100 66.8 50.2 75.2

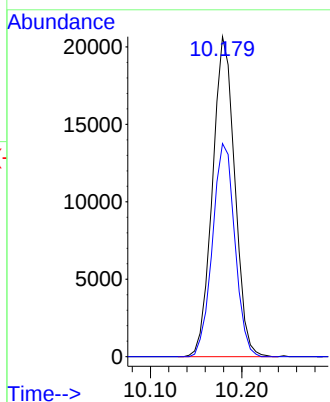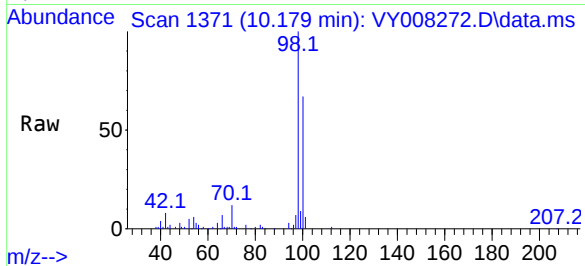

#55
1,1,2-Trichloroethane
Concen: 3.254 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.030 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 97 Resp: 654
Ion Ratio Lower Upper
97 100
83 0.0 69.8 104.8#
85 0.0 44.3 66.5#
99 0.0 49.8 74.6#


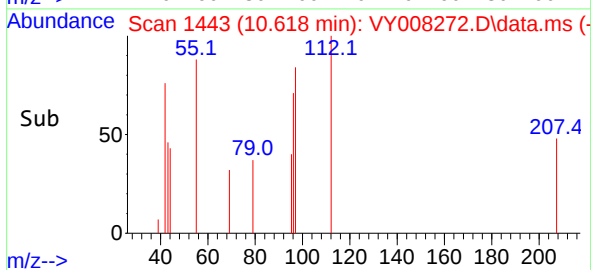
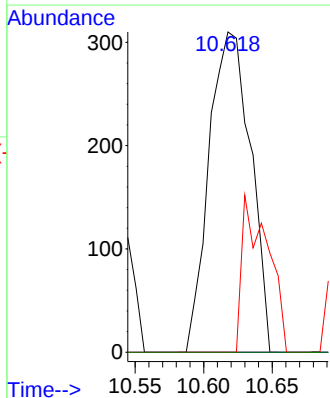





#56
Ethyl methacrylate
Concen: 1.035 ug/l
RT: 10.514 min Scan# 1426
Delta R.T. 0.006 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 69 Resp: 255
Ion Ratio Lower Upper
69 100
41 208.6 63.4 95.0#
39 25.1 35.8 53.8#

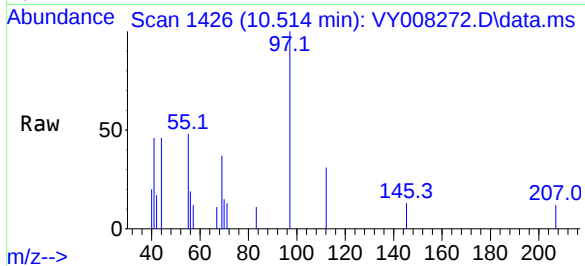

#59
2-Hexanone
Concen: 13.920 ug/l
RT: 10.795 min Scan# 1472
Delta R.T. -0.036 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 43 Resp: 1385
Ion Ratio Lower Upper
43 100
58 0.0 24.4 73.4#


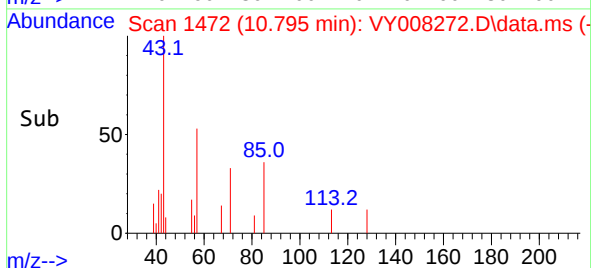
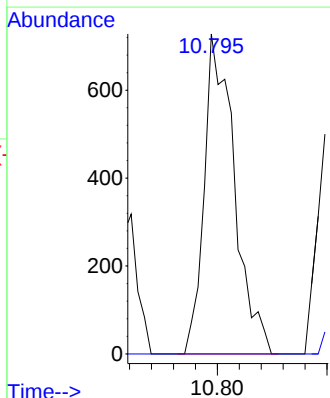





#62
4-Bromofluorobenzene
Concen: 55.227 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 95 Resp: 13025
Ion Ratio Lower Upper
95 100
174 96.4 0.0 177.0
176 92.5 0.0 175.8

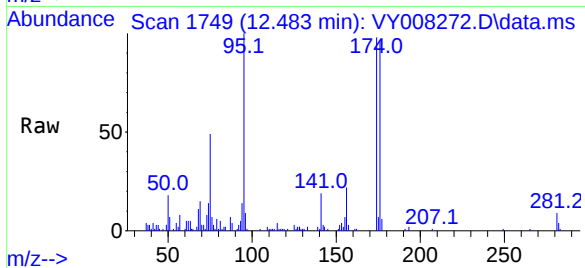

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.007 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion: 117 Resp: 29787
Ion Ratio Lower Upper
117 100
82 45.4 43.0 64.4
119 31.0 25.4 38.0

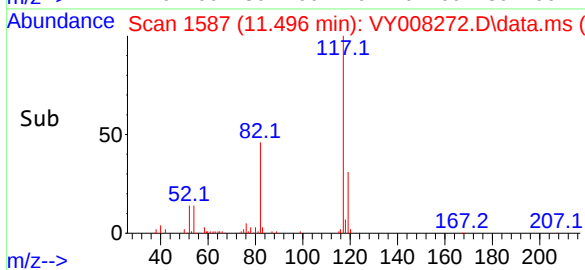






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :



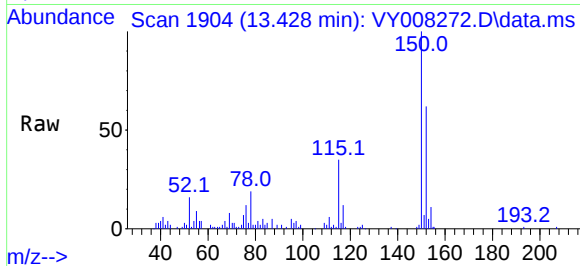



Tgt Ion:152 Resp: 14402
Ion Ratio Lower Upper
152 100
115 54.4 28.2 84.7
150 157.0 0.0 347.6

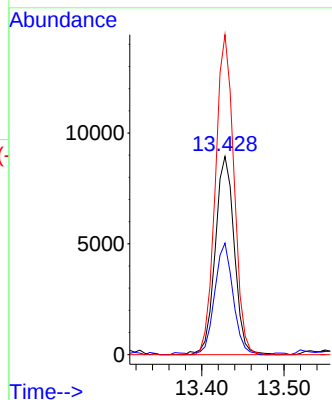

#73
Isopropylbenzene
Concen: 7.451 ug/l
RT: 12.331 min Scan# 1724
Delta R.T. 0.001 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion:105 Resp: 7978
Ion Ratio Lower Upper
105 100
120 28.8 13.4 40.2

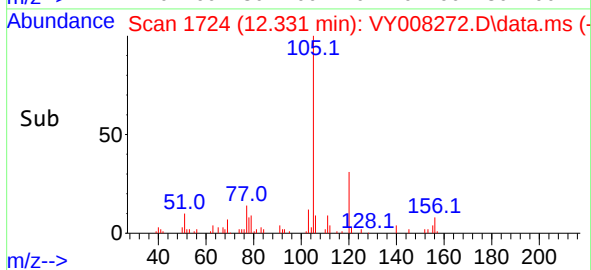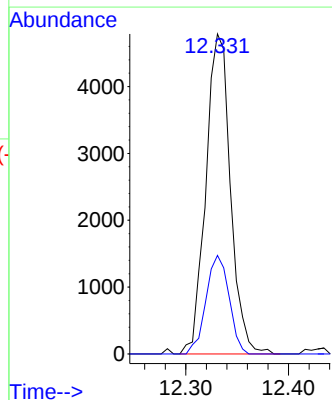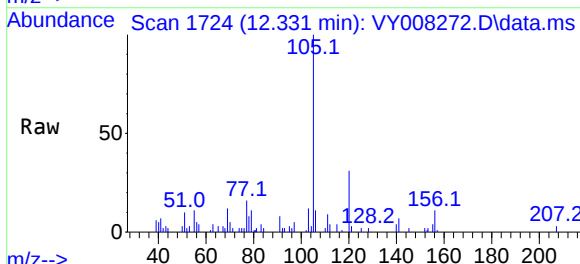






#74
N-amy1 acetate
Concen: 7.472 ug/l
RT: 12.124 min Scan# 1737
Delta R.T. -0.024 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :



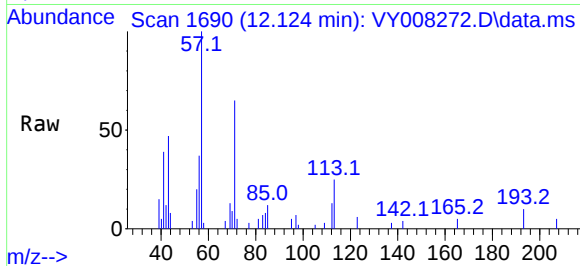



Tgt Ion:	43	Resp:	1737
Ion	Ratio	Lower	Upper
43	100		
70	44.6	28.7	43.1#
55	29.2	17.3	25.9#
61	0.0	17.0	25.6#

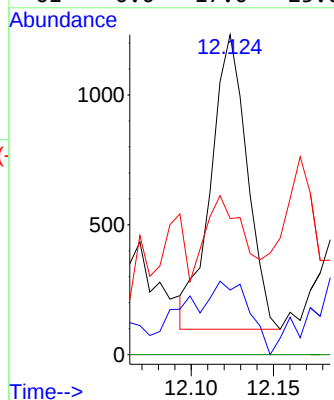

#76
1,2,3-Trichloropropane
Concen: 40.168 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion:	75	Resp:	6398
Ion	Ratio	Lower	Upper
75	100		
77	0.0	0.0	0.0

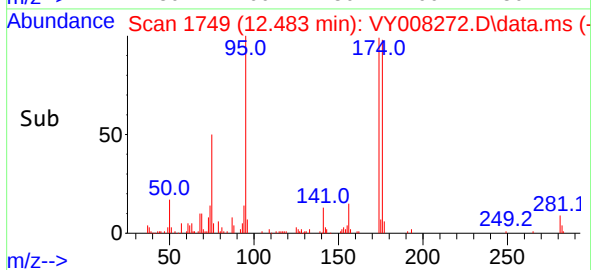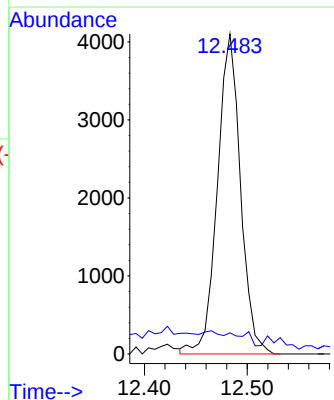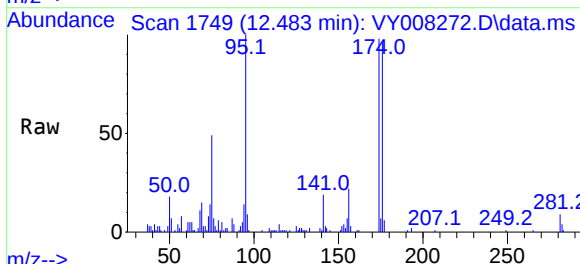






#77
Bromobenzene
Concen: 28.427 ug/l
RT: 12.410 min Scan# 1737
Delta R.T. -0.201 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:156 Resp: 7459
Ion Ratio Lower Upper
156 100
77 0.0 95.5 286.4#
158 0.0 48.0 144.0#

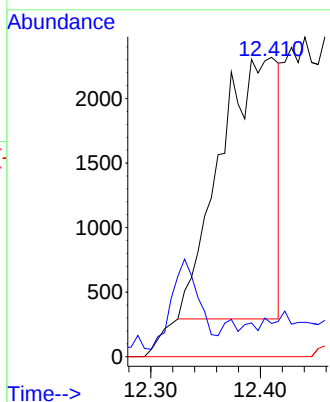

#78
n-propylbenzene
Concen: 12.837 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 91 Resp: 16220
Ion Ratio Lower Upper
91 100
120 24.9 11.3 33.9


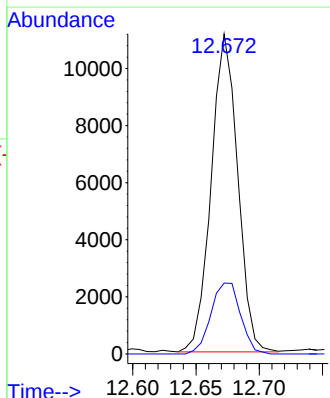
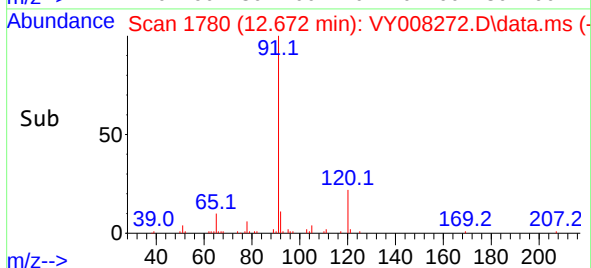





#79
2-Chlorotoluene
Concen: 22.874 ug/l
RT: 12.672 min Scan# 11
Delta R.T. -0.085 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91 Resp: 16220
Ion Ratio Lower Upper
91 100
126 1.4 16.9 50.6#

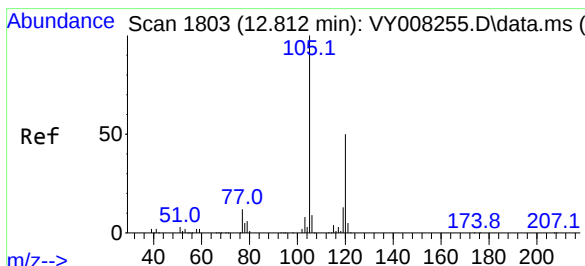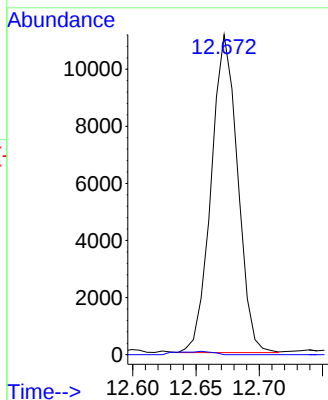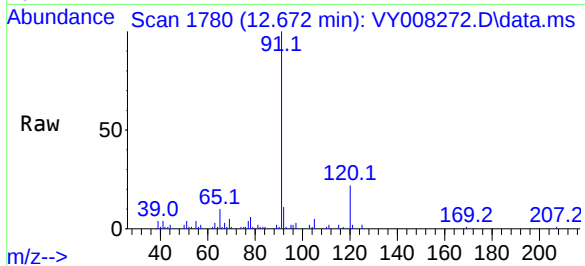

#80
1,3,5-Trimethylbenzene
Concen: 1.730 ug/l
RT: 12.977 min Scan# 1830
Delta R.T. 0.165 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 105 Resp: 1519
Ion Ratio Lower Upper
105 100
120 28.9 24.4 73.4


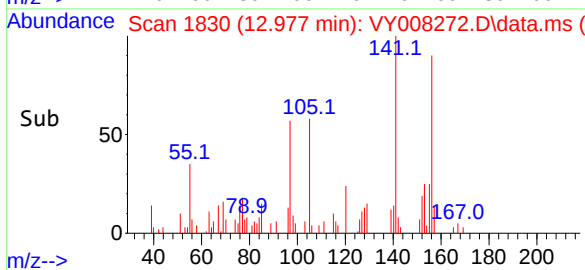
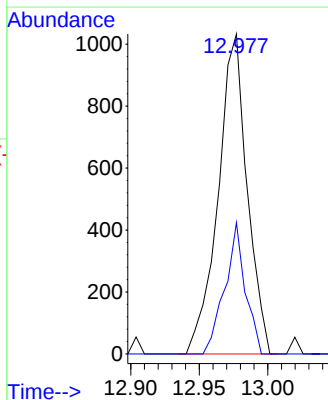





#81
trans-1,4-Dichloro-2-butene
Concen: 89.874 ug/l
RT: 12.483 min Scan# 1732
Delta R.T. 0.104 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 6398
Ion Ratio Lower Upper
75 100
53 1.6 85.3 127.9#
89 0.0 37.0 55.4#

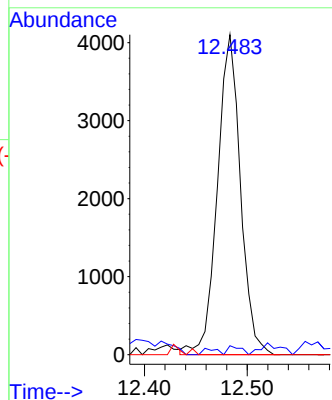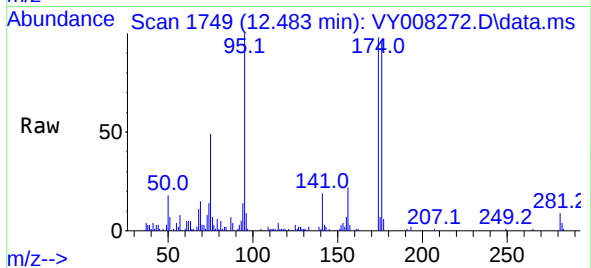

#82
4-Chlorotoluene
Concen: 22.248 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. -0.183 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion: 91 Resp: 16212
Ion Ratio Lower Upper
91 100
126 1.4 17.0 51.0#


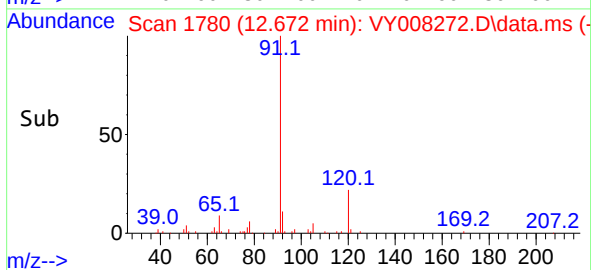
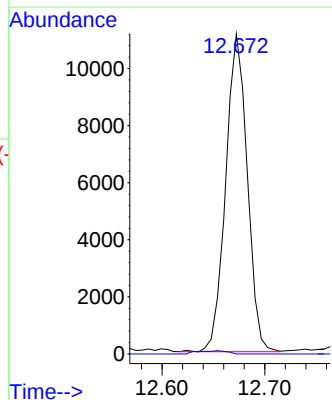





#84
1,2,4-Trimethylbenzene
Concen: 2.807 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 2439
Ion Ratio Lower Upper
105 100
120 42.4 22.3 66.9

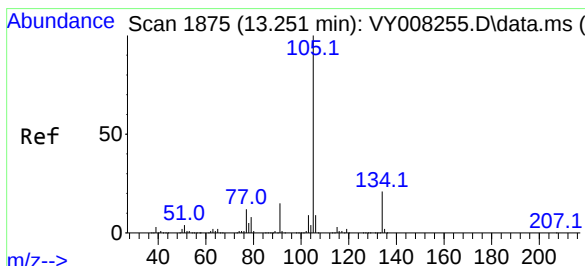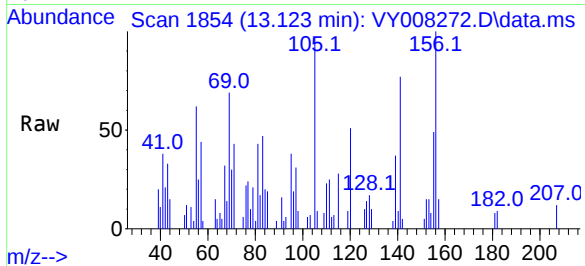

#85
sec-Butylbenzene
Concen: 10.798 ug/l
RT: 13.258 min Scan# 1876
Delta R.T. 0.007 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion:105 Resp: 12609
Ion Ratio Lower Upper
105 100
134 28.1 10.2 30.4

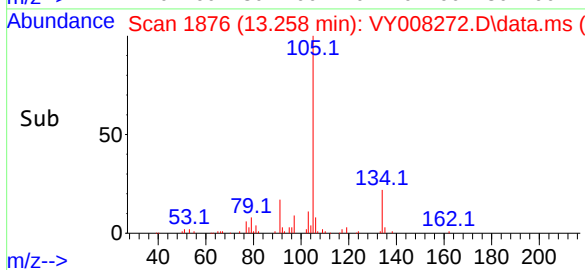



#89

n-Butylbenzene

Concen: 15.280 ug/l

RT: 13.703 min Scan# 1949

Delta R.T. 0.007 min

Lab File: VY008272.D





Acq: 11 Apr 2022 14:56

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:	91	Resp:	13453
Ion	Ratio	Lower	Upper
91	100		
92	49.4	26.3	78.9
134	47.1	13.0	38.9#

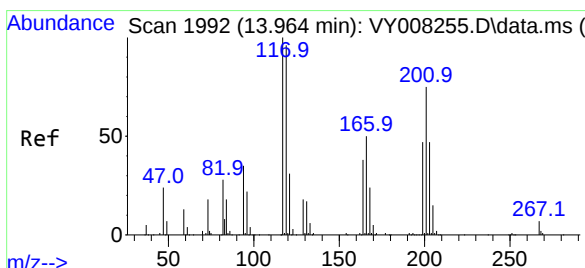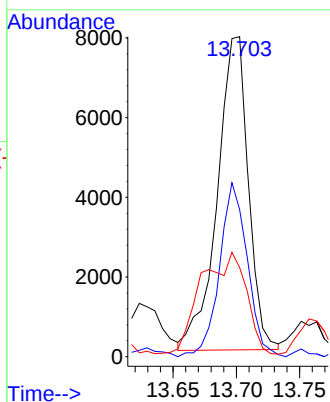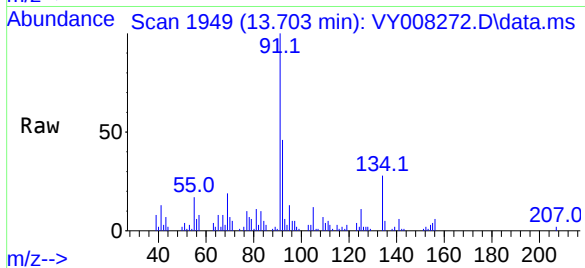

#90

Hexachloroethane

Concen: 20.617 ug/l




RT: 13.977 min Scan# 1994


Delta R.T. 0.013 min

Lab File: VY008272.D

Acq: 11 Apr 2022 14:56

Tgt Ion:	117	Resp:	3755
Ion	Ratio	Lower	Upper
117	100		
201	0.0	43.0	128.8#


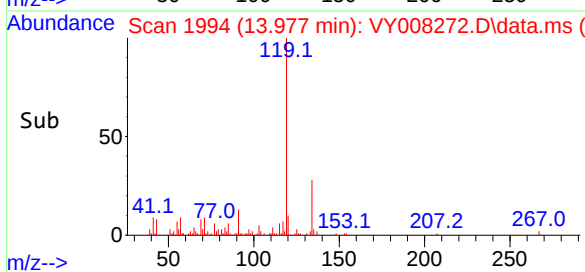
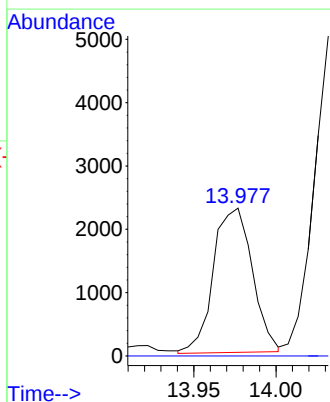
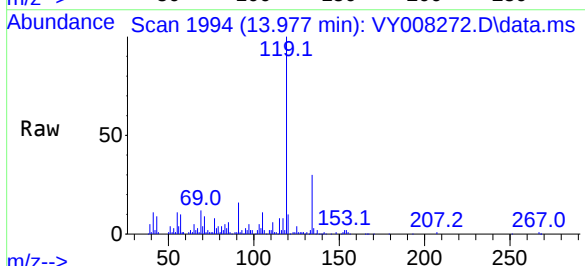




#92
1,2-Dibromo-3-Chloropropane
Concen: 2.807 ug/l
RT: 14.379 min Scan# 2057
Delta R.T. 0.018 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 91
Ion Ratio Lower Upper
75 100
155 0.0 38.0 113.9#
157 0.0 47.8 143.3#

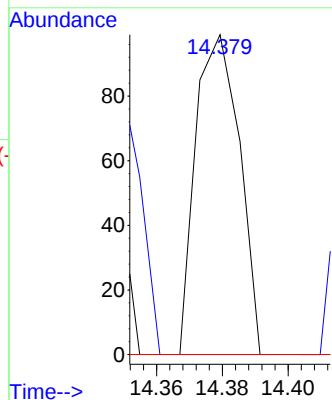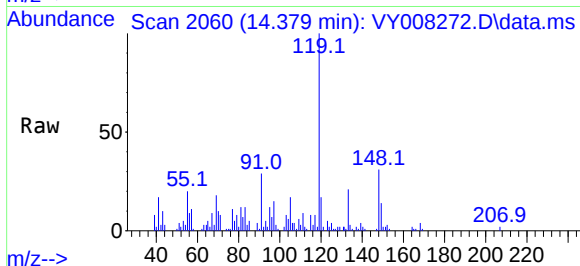

#93
1,2,4-Trichlorobenzene
Concen: 2.099 ug/l
RT: 15.007 min Scan# 2163
Delta R.T. 0.000 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56


Tgt Ion:180 Resp: 574
Ion Ratio Lower Upper
180 100
182 84.0 47.3 141.9
145 1880.8 14.6 43.8#

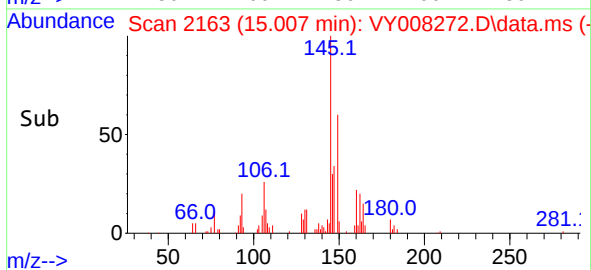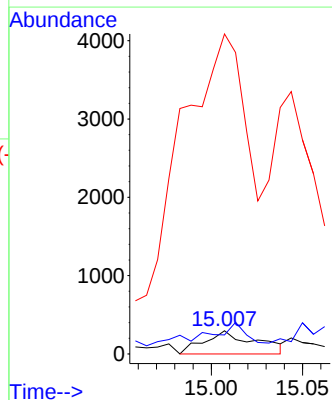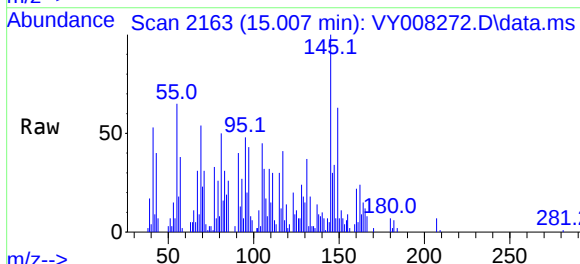






#95
Naphthalene
Concen: 4.920 ug/l
RT: 15.239 min Scan# 21
Delta R.T. 0.001 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Instrument :
MSVOA_Y
ClientSampleId :

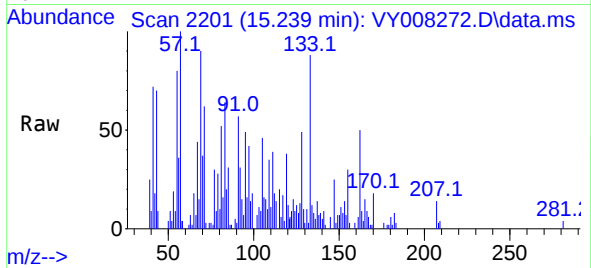

Tgt Ion:128 Resp: 2882
Ion Ratio Lower Upper
128 100
127 56.1 11.0 16.4#
129 0.0 8.4 12.6#

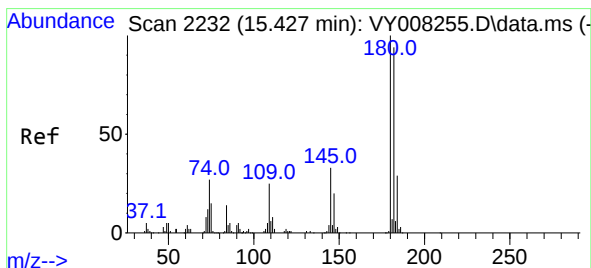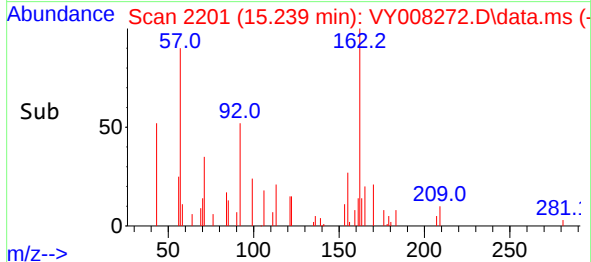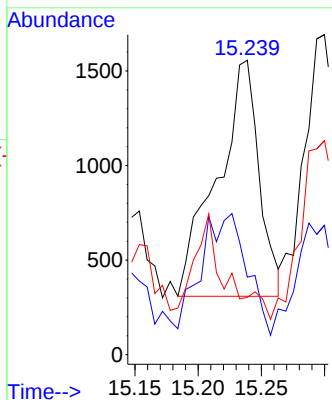

#96
1,2,3-Trichlorobenzene
Concen: 2.658 ug/l
RT: 15.440 min Scan# 2234
Delta R.T. 0.013 min
Lab File: VY008272.D
Acq: 11 Apr 2022 14:56

Tgt Ion:180 Resp: 636
Ion Ratio Lower Upper
180 100
182 0.0 47.3 141.9#
145 1445.4 15.3 45.9#

