
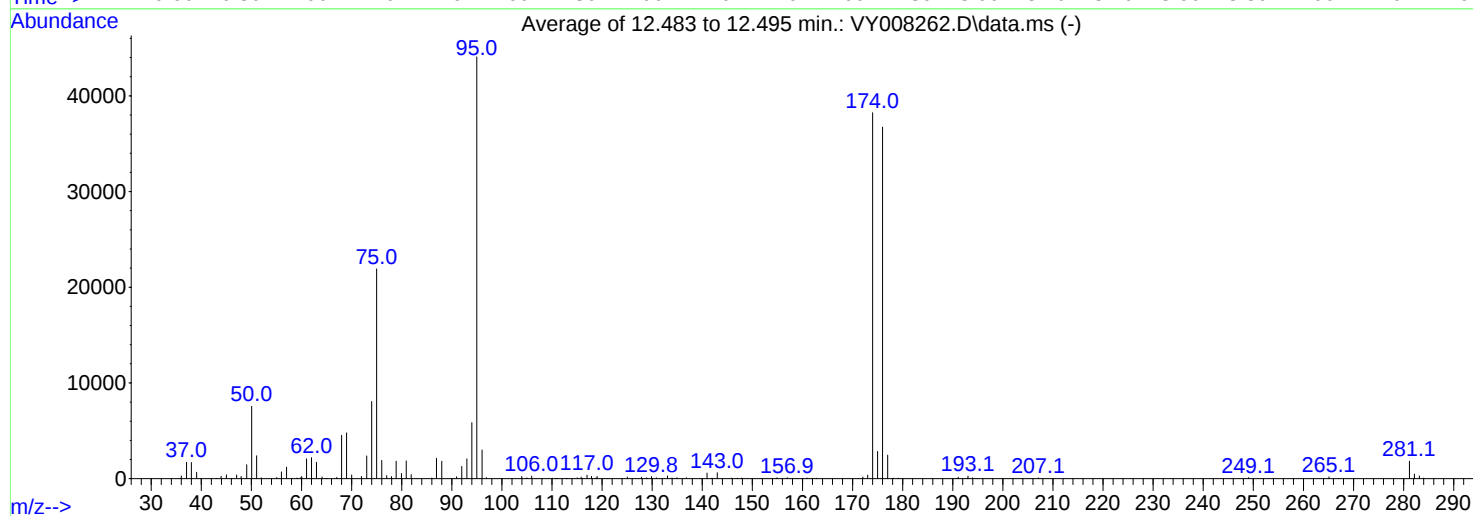


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041122\
 Data File : VY008262.D
 Acq On : 11 Apr 2022 08:59
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y040822S.M
 Title : SW846 8260
 Last Update : Fri Apr 08 16:02:50 2022

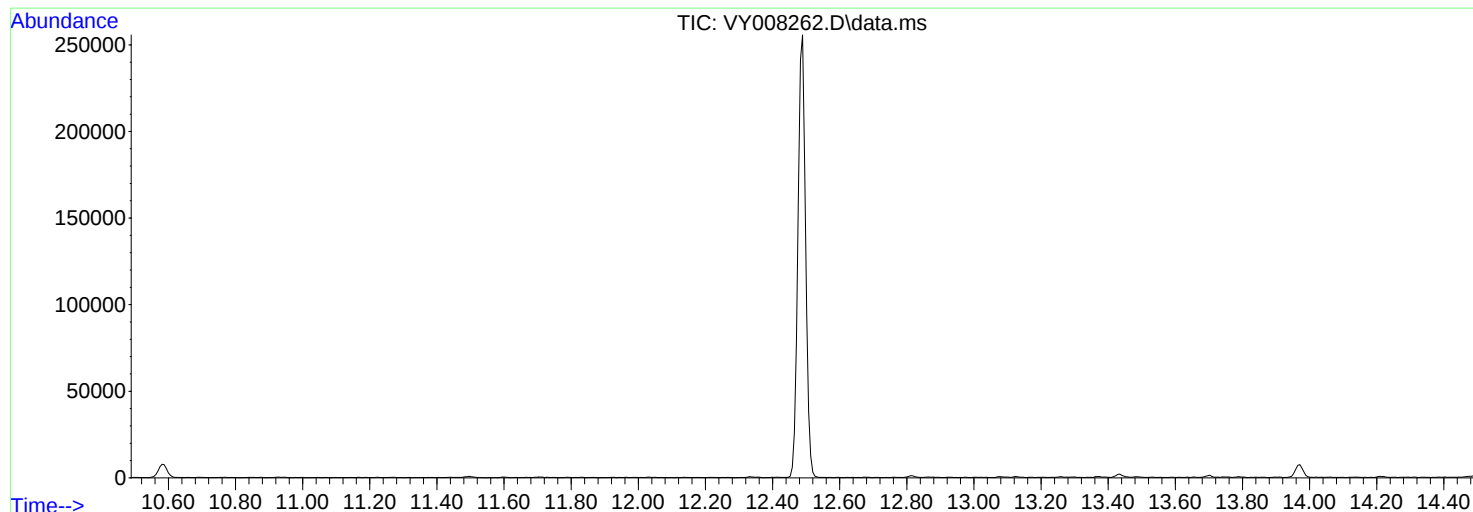

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7563	PASS
75	95	30	60	49.7	21922	PASS
95	95	100	100	100.0	44077	PASS
96	95	5	9	6.8	2992	PASS
173	174	0.00	2	1.0	367	PASS
174	95	50	100	86.8	38240	PASS
175	174	5	9	7.5	2851	PASS
176	174	95	101	96.0	36728	PASS
177	176	5	9	6.7	2461	PASS